

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS103019\
 Data File : PS007520.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Oct 2019 19:15
 Operator : SM\AJ
 Sample : K5540-19
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 31 00:46:49 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 14 13:54:23 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.431	5.157	251.0E6	121.6E6	183.362	172.930
Target Compounds							
1) T	Dalapon	1.992	1.700	82788869	255.0E6	49.477	280.223 #
2) T	3,5-DICHL...	0.000	4.492	0	49982851	N.D.	58.090
5) T	DICAMBA	5.525	5.292	50661967	17121065	10.311	6.580 #
7) T	MCPA	5.900	5.527	27017041	23894195	5.238	8.219 #
9) T	2,4-D	6.483	6.062	38864289	9779362	31.537	12.258 #
10) T	Pentachlo...	0.000	6.449	0	7402056	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	6.752	0	5492139	N.D.	1.444
13) T	2,4-DB	8.015	7.711	-21070728	16219129	N.D.	34.605
14) T	DINOSEB	0.000	7.948	0	61756590	N.D.	21.998
15) T	Picloram	0.000	8.926	0	28780591	N.D.	4.687
16) T	DCPA	0.000	8.812	0	17215668	N.D.	3.433



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS103019\
Data File : PS007520.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Oct 2019 19:15
Operator : SM\AJ
Sample : K5540-19
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 31 00:46:49 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
Quant Title : 8080.M
QLast Update : Mon Oct 14 13:54:23 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

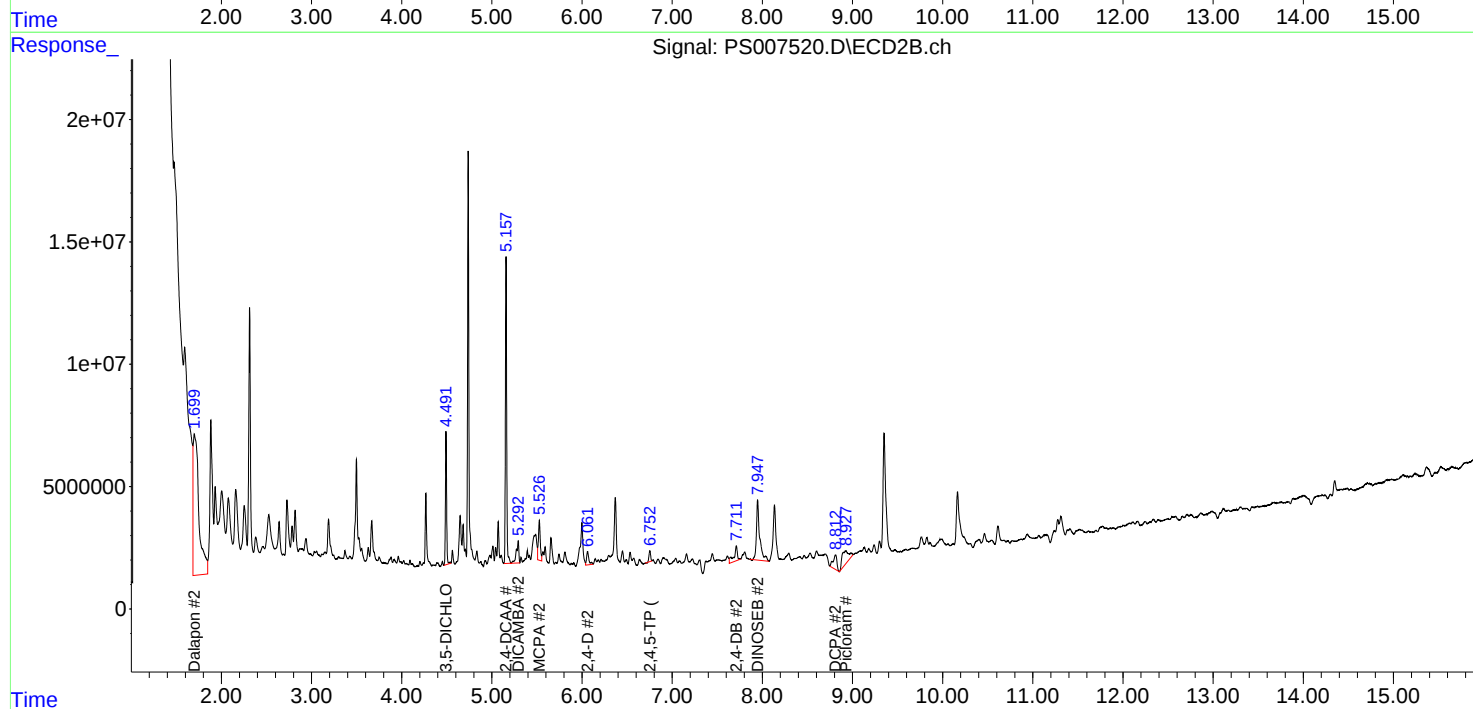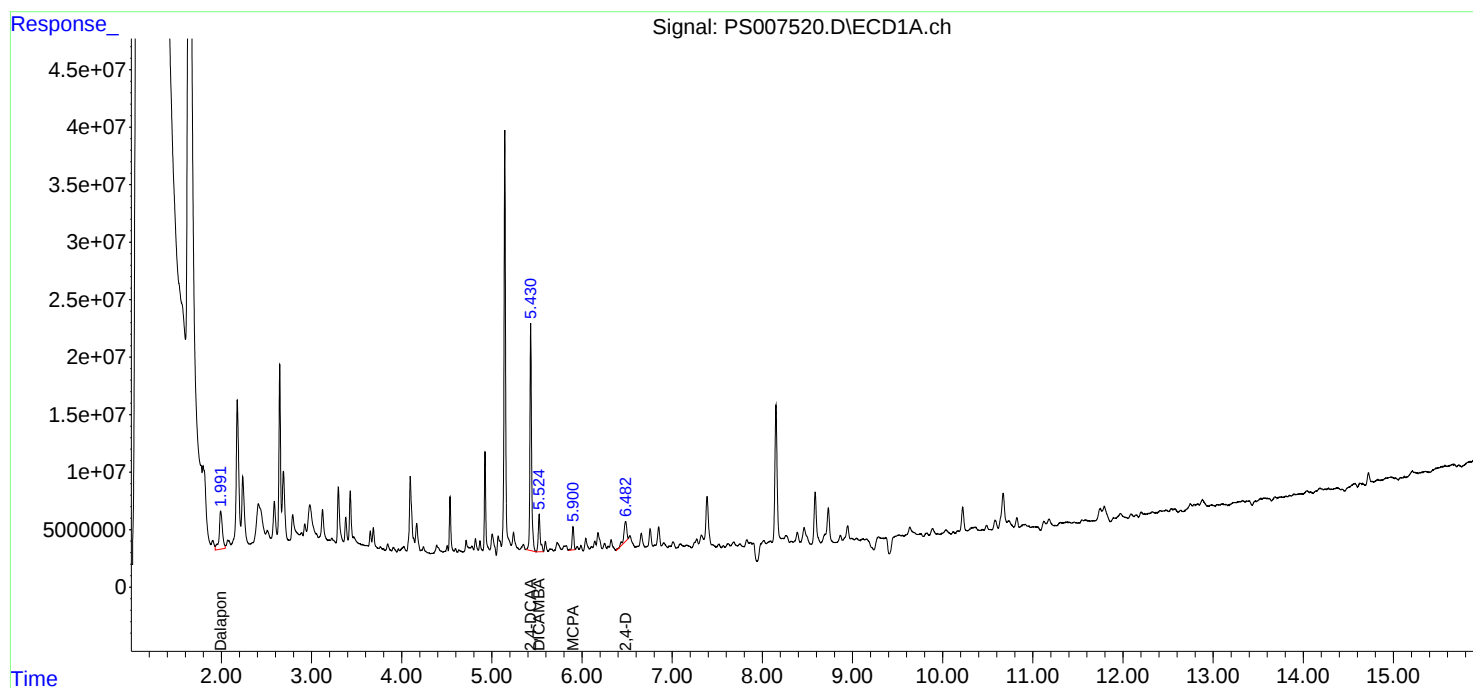


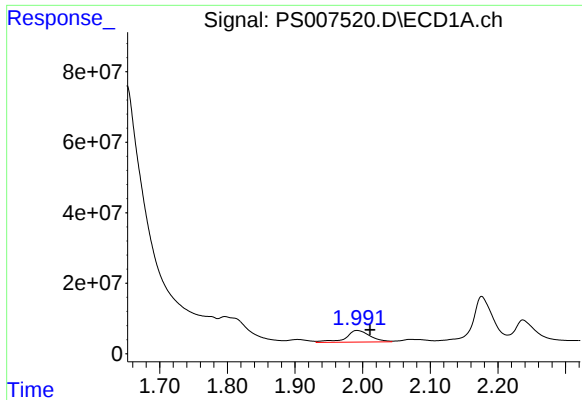

#1 Dalapon


R.T.: 1.992 min
Delta R.T.: -0.019 min
Response: 82788869
Conc: 49.48 ng/ml

Instrument :
ECD_S
ClientSampleId :

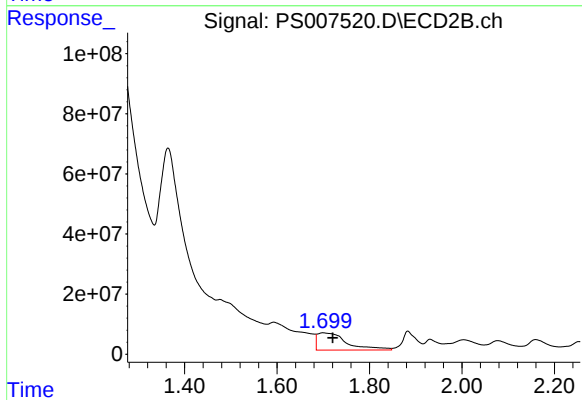


#1 Dalapon

R.T.: 1.700 min
Delta R.T.: -0.021 min
Response: 255003723
Conc: 280.22 ng/ml

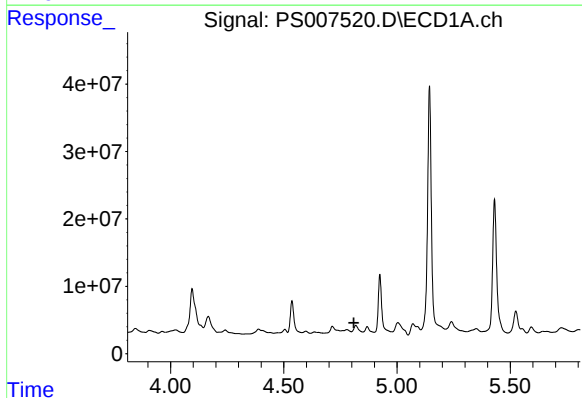


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.810 min
Response: 0
Conc: N.D.

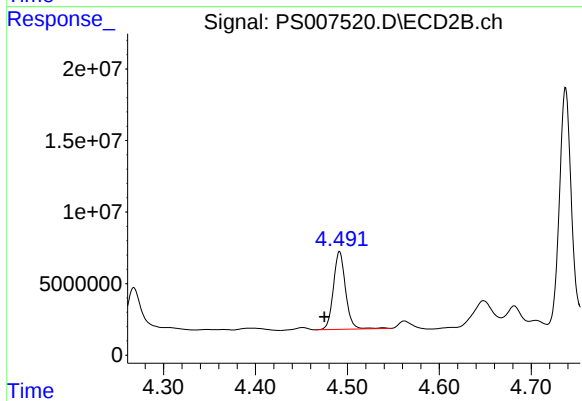

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.492 min
Delta R.T.: 0.017 min
Response: 49982851
Conc: 58.09 ng/ml

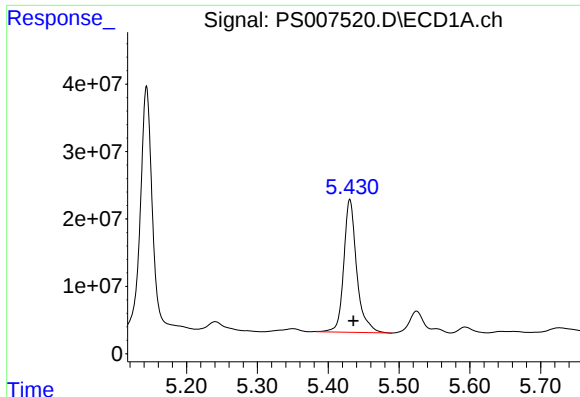

#4 2,4-DCAA


R.T.: 5.431 min
Delta R.T.: -0.005 min
Response: 250961872
Conc: 183.36 ng/ml

Instrument :
ECD_S
ClientSampleId :

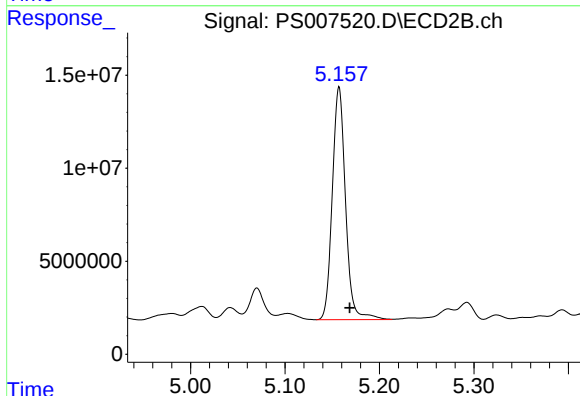


#4 2,4-DCAA

R.T.: 5.157 min
Delta R.T.: -0.011 min
Response: 121622716
Conc: 172.93 ng/ml

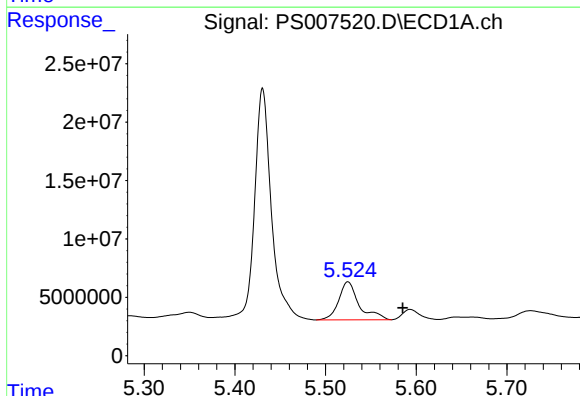


#5 DICAMBA

R.T.: 5.525 min
Delta R.T.: -0.060 min
Response: 50661967
Conc: 10.31 ng/ml

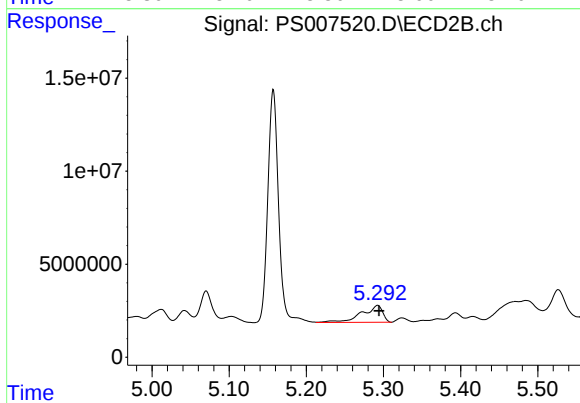

#5 DICAMBA


R.T.: 5.292 min
Delta R.T.: -0.002 min
Response: 17121065
Conc: 6.58 ng/ml

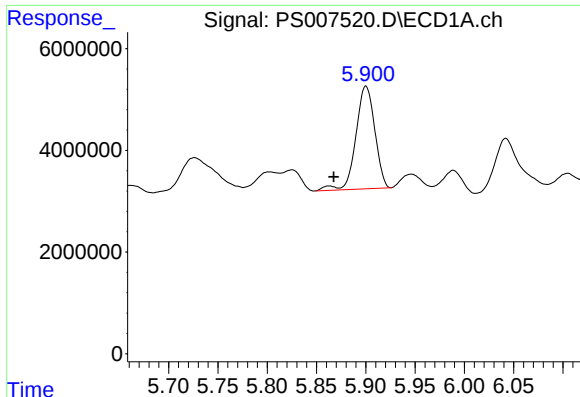

#7 MCPA


R.T.: 5.900 min
Delta R.T.: 0.033 min
Response: 27017041
Conc: 5.24 ug/ml

Instrument :
ECD_S
ClientSampleId :

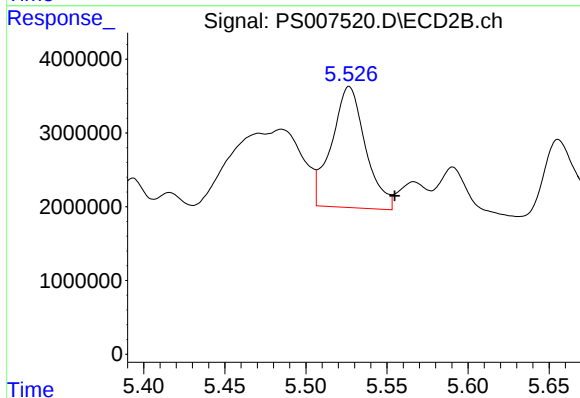


#7 MCPA

R.T.: 5.527 min
Delta R.T.: -0.028 min
Response: 23894195
Conc: 8.22 ug/ml

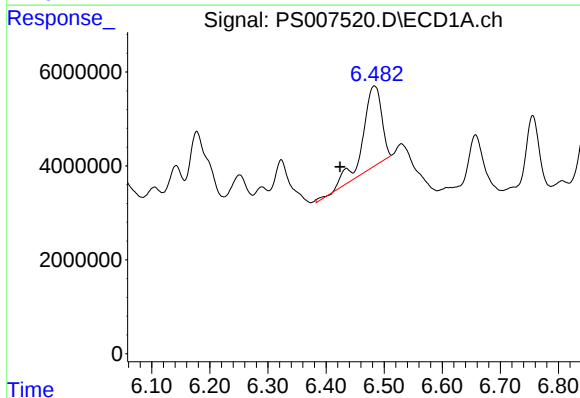


#9 2,4-D

R.T.: 6.483 min
Delta R.T.: 0.059 min
Response: 38864289
Conc: 31.54 ng/ml

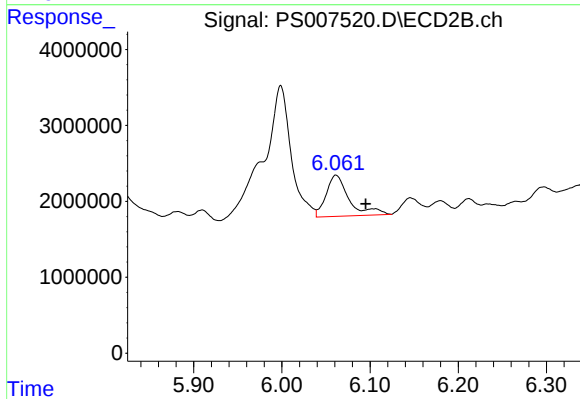

#9 2,4-D


R.T.: 6.062 min
Delta R.T.: -0.034 min
Response: 9779362
Conc: 12.26 ng/ml

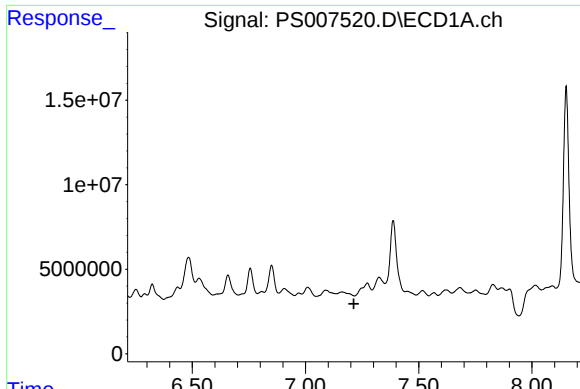

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.214 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

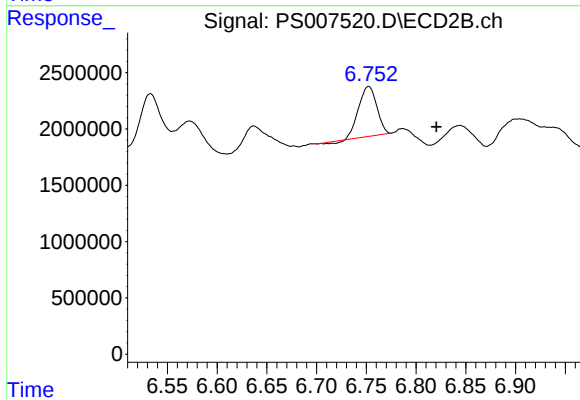


#11 2,4,5-TP (SILVEX)

R.T.: 6.752 min
Delta R.T.: -0.068 min
Response: 5492139
Conc: 1.44 ng/ml

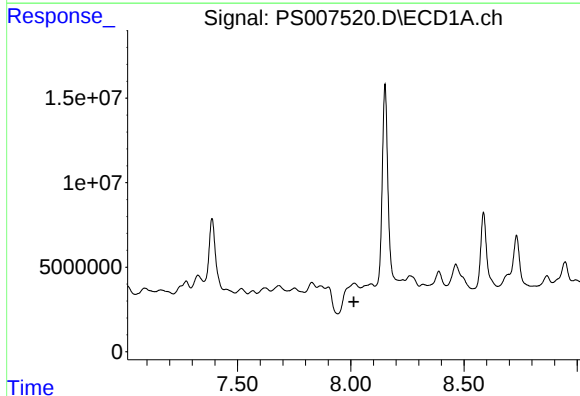


#13 2,4-DB

R.T.: 8.015 min
Delta R.T.: 0.002 min
Response: -21070728
Conc: N.D.

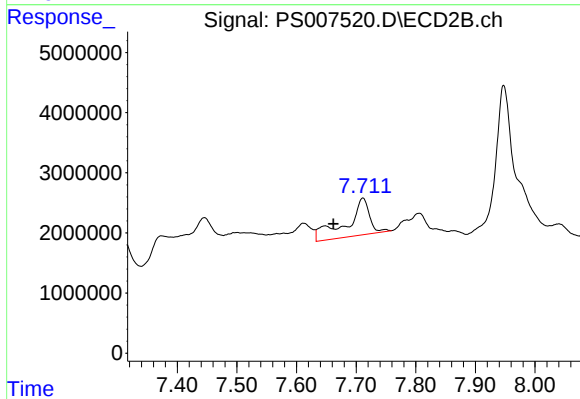

#13 2,4-DB


R.T.: 7.711 min
Delta R.T.: 0.049 min
Response: 16219129
Conc: 34.60 ng/ml

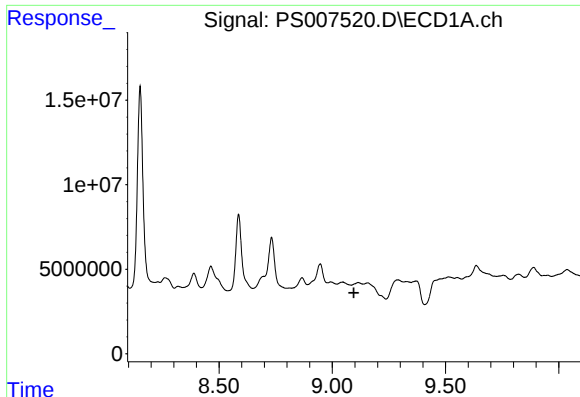

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 9.095 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

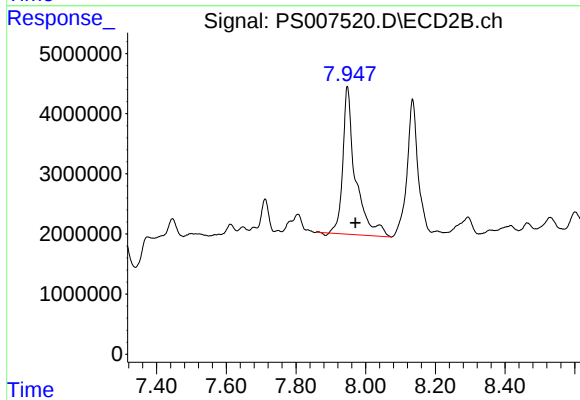


#14 DINOSEB

R.T.: 7.948 min
Delta R.T.: -0.023 min
Response: 61756590
Conc: 22.00 ng/ml

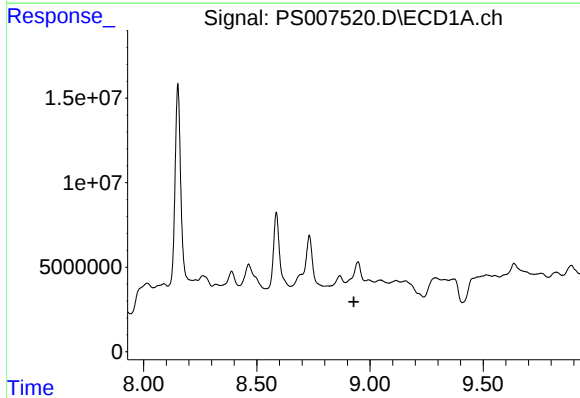


#15 Picloram

R.T.: 0.000 min
Exp R.T.: 8.929 min
Response: 0
Conc: N.D.

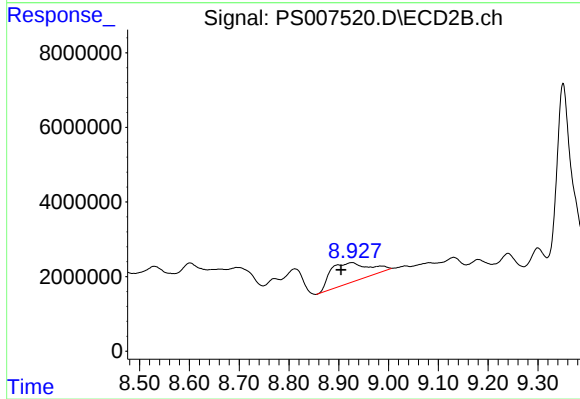

#15 Picloram


R.T.: 8.926 min
Delta R.T.: 0.022 min
Response: 28780591
Conc: 4.69 ng/ml

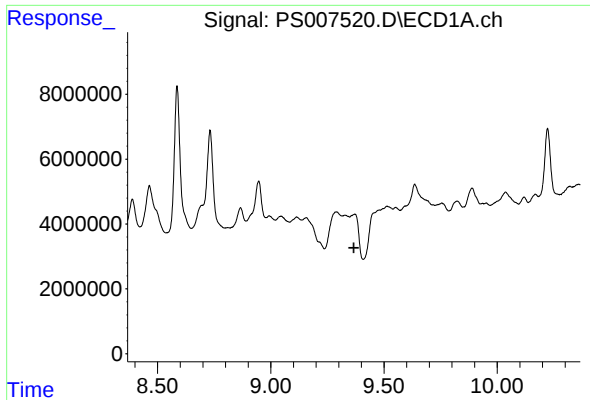

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 9.367 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

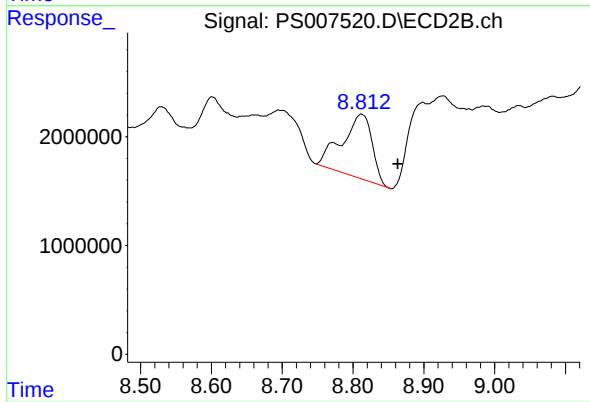

#16 DCPA

R.T.: 8.812 min
Delta R.T.: -0.051 min
Response: 17215668
Conc: 3.43 ng/ml