

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS103020\
 Data File : PS013059.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Oct 2020 18:33
 Operator : DD\AJ
 Sample : PB132740TB
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 31 06:03:25 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102020.M
 Quant Title : 8080.M
 QLast Update : Wed Oct 21 02:27:47 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.211	6.914	330.6E6	172.9E6	369.306	430.957
Target Compounds							
1) T	Dalapon	2.992	2.590	69381920	129.3E6	68.251	245.967 #
2) T	3,5-DICHL...	0.000	6.045	0	3330240	N.D.	5.285
3) T	4-Nitroph...	6.980	0.000	3896644	0	9.317	N.D. #
5) T	DICAMBA	7.387	7.047	13526773	6264225	3.799	3.681
6) T	MCPD	0.000	7.123	0	2067783	N.D.	1.553
7) T	MCPA	7.714	0.000	68834753	0	17.977	N.D. #
8) T	DICHLORPROP	0.000	7.745	0	13058794	N.D.	28.428
9) T	2,4-D	8.388	0.000	72273533	0	70.046	N.D. #
10) T	Pentachlo...	8.684	0.000	11109327	0	<MDL	N.D. #
11) T	2,4,5-TP ...	0.000	8.741	0	49833000	N.D.	21.021
12) T	2,4,5-T	9.398	0.000	100.3E6	0	19.154	N.D. #
15) T	Picloram	0.000	11.032	0	2361001	N.D.	<MDL
16) T	DCPA	0.000	10.932	0	12514	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS103020\
Data File : PS013059.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Oct 2020 18:33
Operator : DD\AJ
Sample : PB132740TB
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 31 06:03:25 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102020.M
Quant Title : 8080.M
QLast Update : Wed Oct 21 02:27:47 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

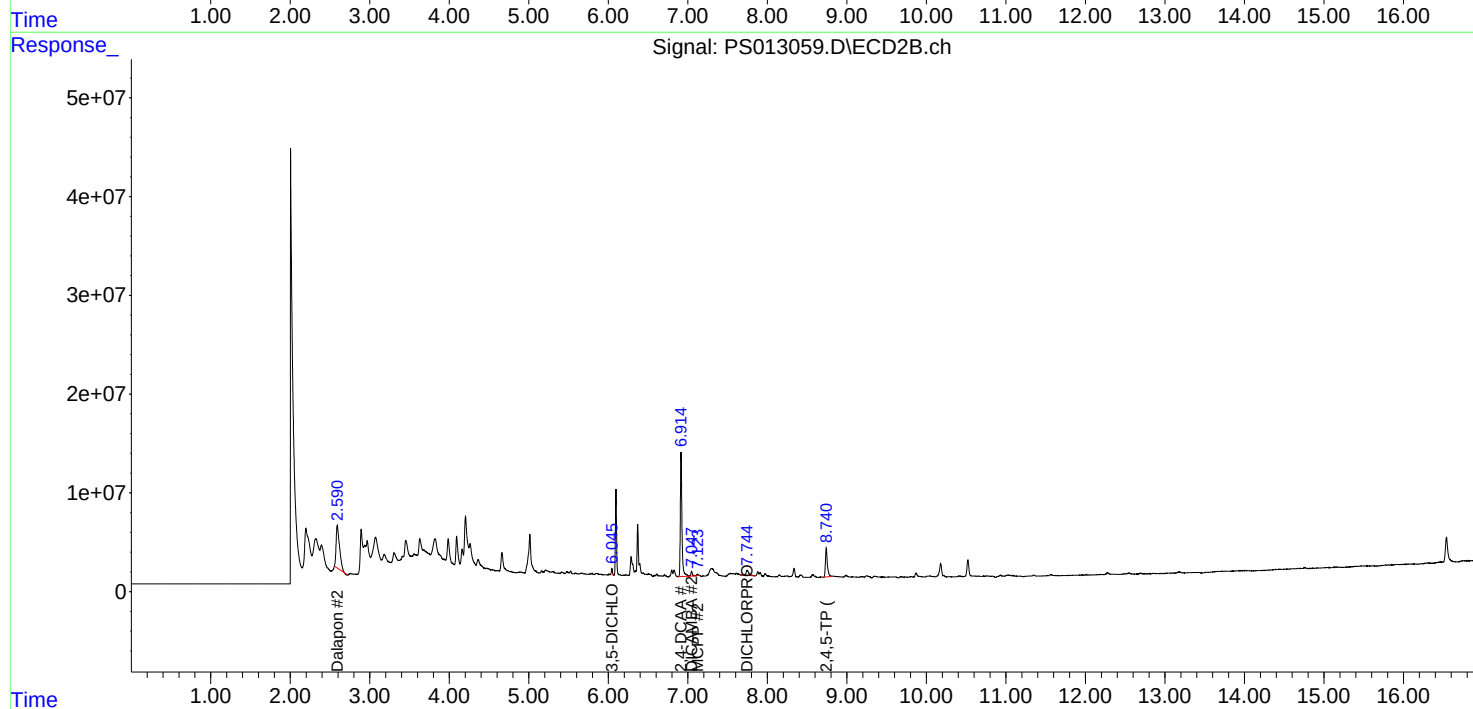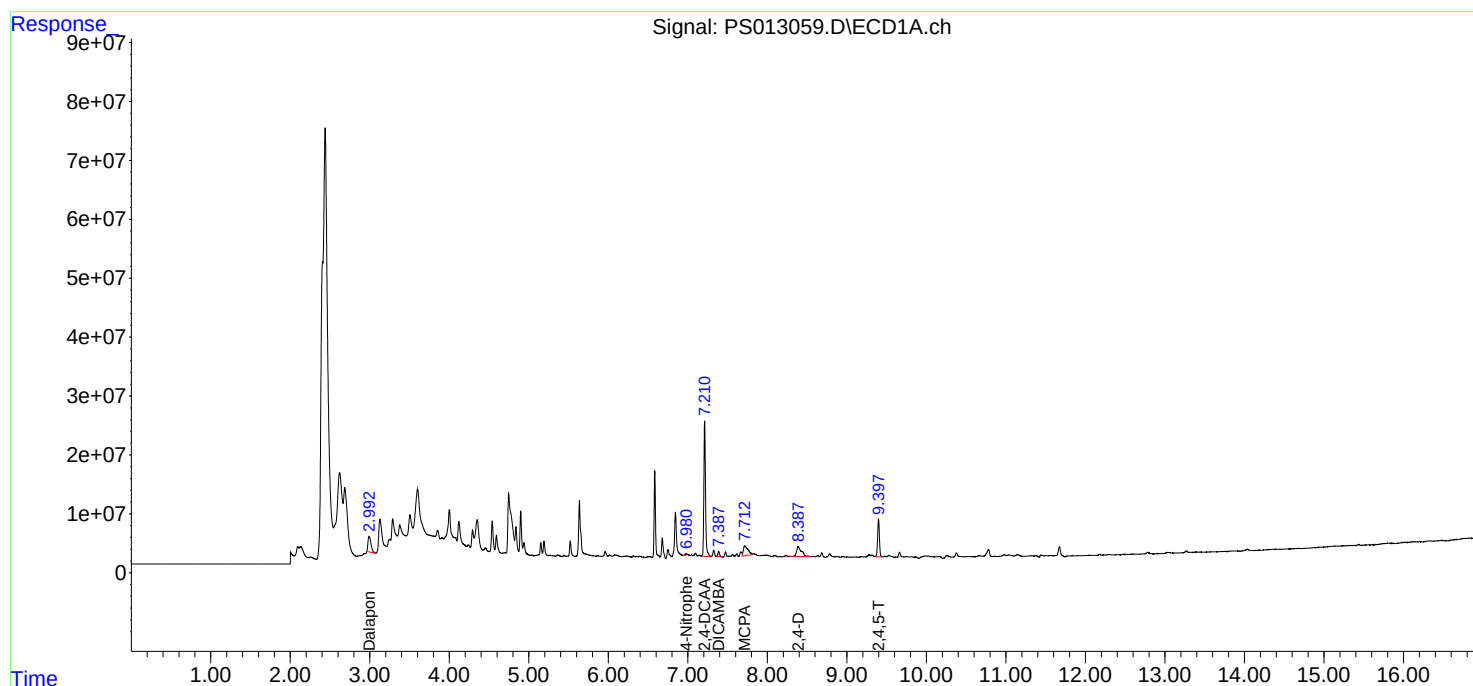


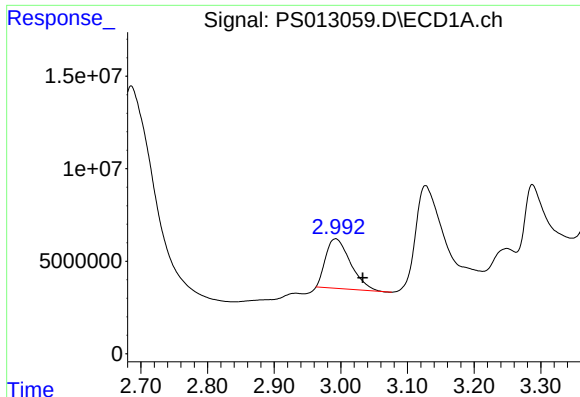

#1 Dalapon


R.T.: 2.992 min
Delta R.T.: -0.041 min
Response: 69381920
Conc: 68.25 ng/ml

Instrument :
ECD_S
ClientSampleId :

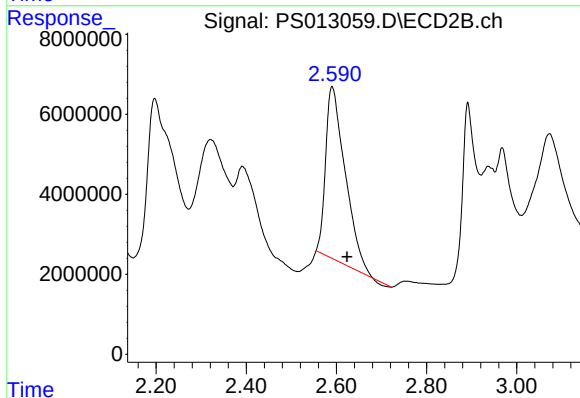


#1 Dalapon

R.T.: 2.590 min
Delta R.T.: -0.033 min
Response: 129348356
Conc: 245.97 ng/ml

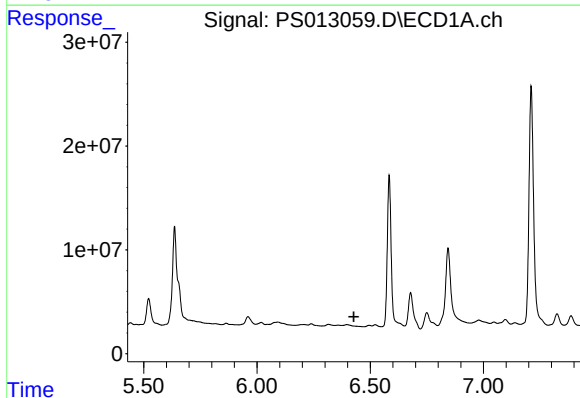


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.428 min
Response: 0
Conc: N.D.

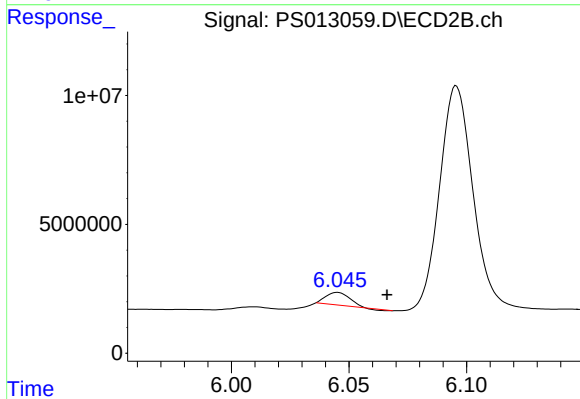

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.045 min
Delta R.T.: -0.021 min
Response: 3330240
Conc: 5.29 ng/ml

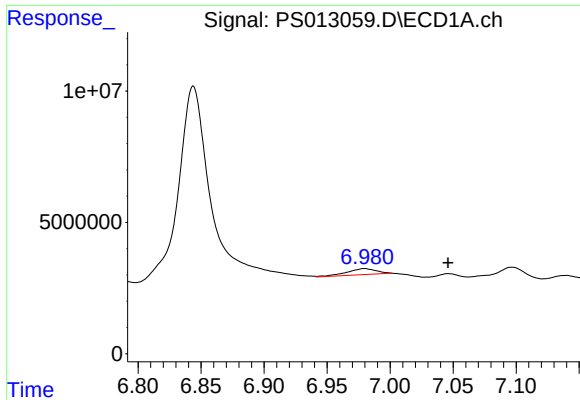

#3 4-Nitrophenol


R.T.: 6.980 min
Delta R.T.: -0.066 min
Response: 3896644
Conc: 9.32 ng/ml

Instrument :
ECD_S
ClientSampleId :

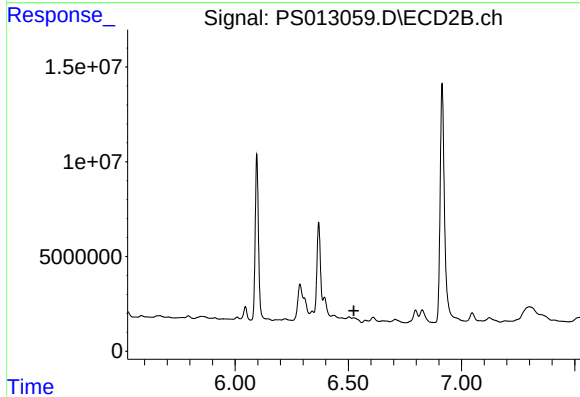


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.525 min
Response: 0
Conc: N.D.

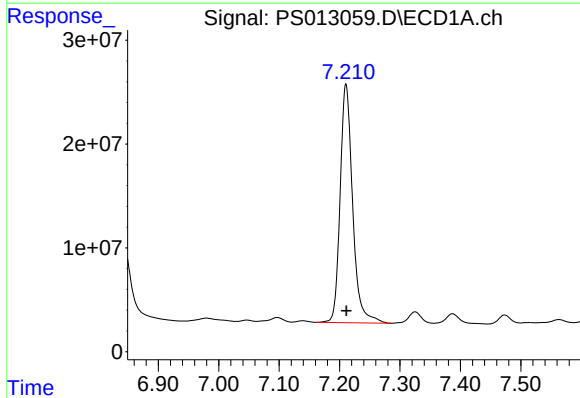


#4 2,4-DCAA

R.T.: 7.211 min
Delta R.T.: 0.000 min
Response: 330554206
Conc: 369.31 ng/ml

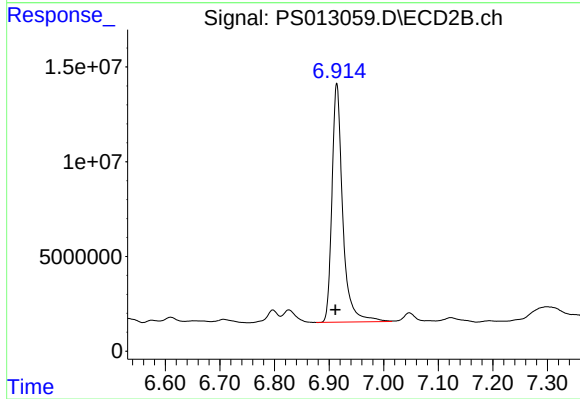

#4 2,4-DCAA


R.T.: 6.914 min
Delta R.T.: 0.002 min
Response: 172922320
Conc: 430.96 ng/ml

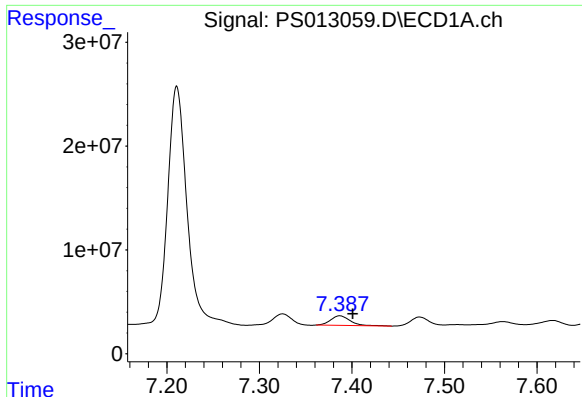

#5 DICAMBA


R.T.: 7.387 min
Delta R.T.: -0.014 min
Response: 13526773
Conc: 3.80 ng/ml

Instrument :
ECD_S
ClientSampleId :

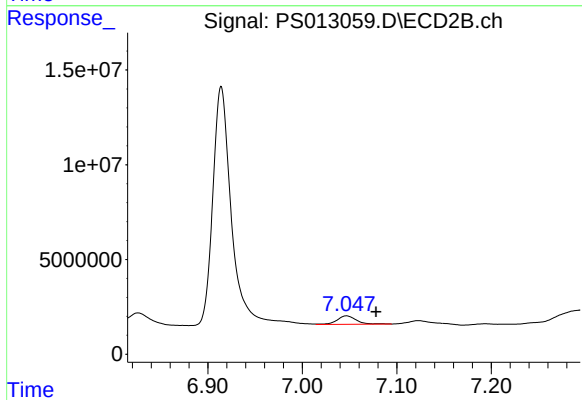


#5 DICAMBA

R.T.: 7.047 min
Delta R.T.: -0.031 min
Response: 6264225
Conc: 3.68 ng/ml

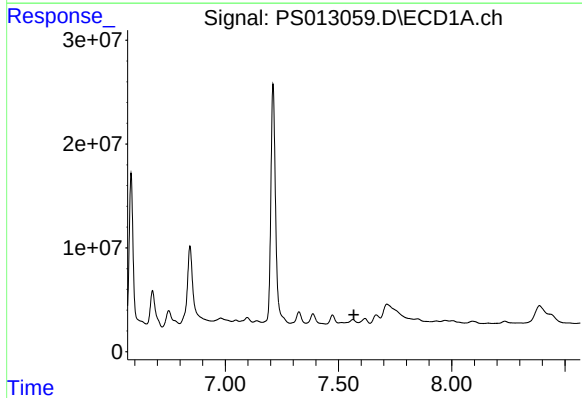


#6 MCP

R.T.: 0.000 min
Exp R.T. : 7.568 min
Response: 0
Conc: N.D.

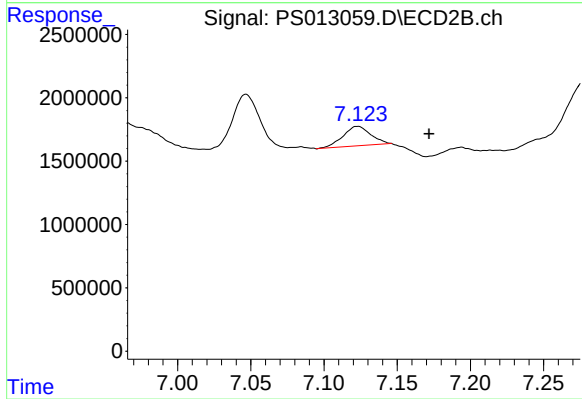

#6 MCP


R.T.: 7.123 min
Delta R.T.: -0.049 min
Response: 2067783
Conc: 1.55 ug/ml

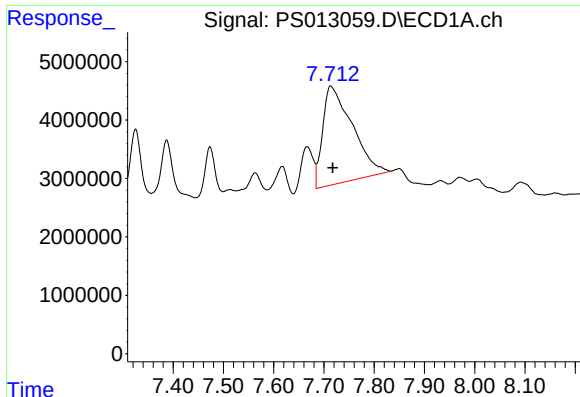

#7 MCPA


R.T.: 7.714 min
Delta R.T.: -0.003 min
Response: 68834753
Conc: 17.98 ug/ml

Instrument :
ECD_S
ClientSampleId :

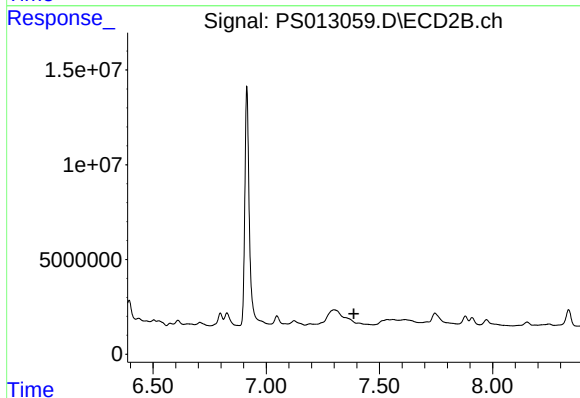


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.387 min
Response: 0
Conc: N.D.

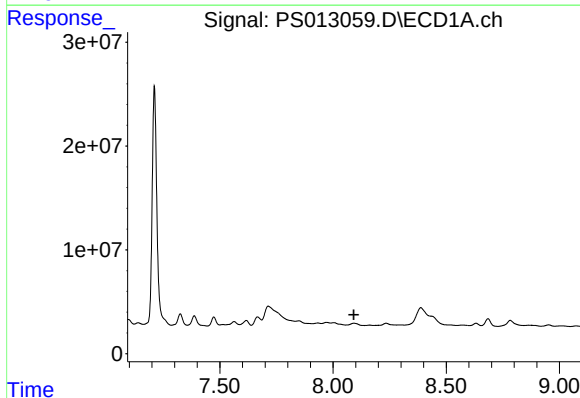


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.092 min
Response: 0
Conc: N.D.

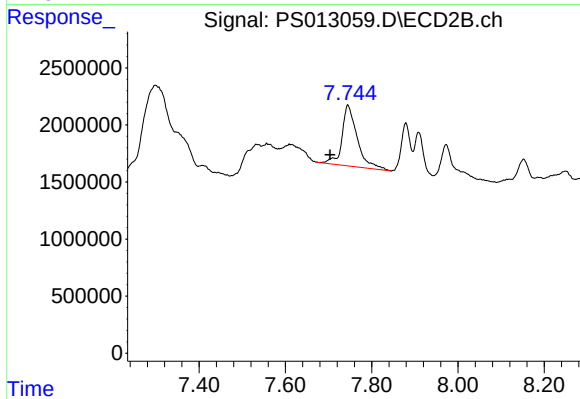

#8 DICHLORPROP


R.T.: 7.745 min
Delta R.T.: 0.041 min
Response: 13058794
Conc: 28.43 ng/ml

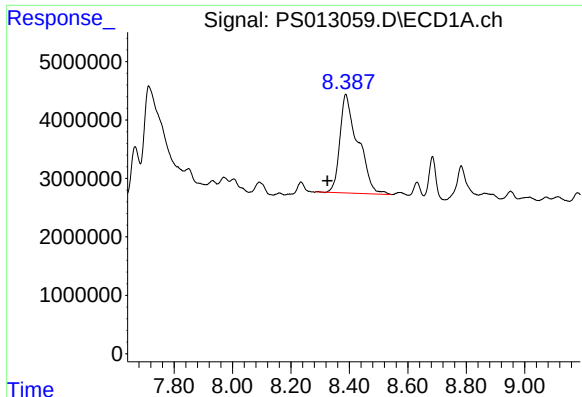

#9 2,4-D


R.T.: 8.388 min
Delta R.T.: 0.063 min
Response: 72273533
Conc: 70.05 ng/ml

Instrument :
ECD_S
ClientSampleId :

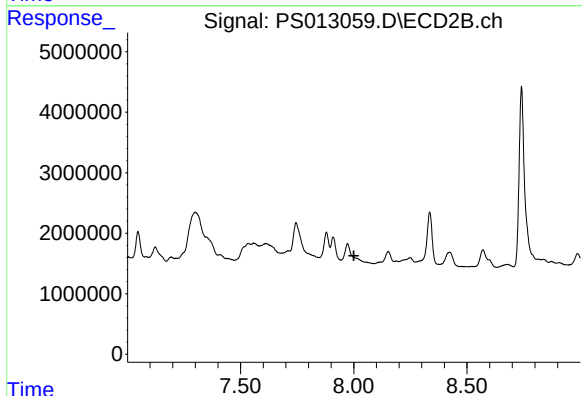


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 8.001 min
Response: 0
Conc: N.D.

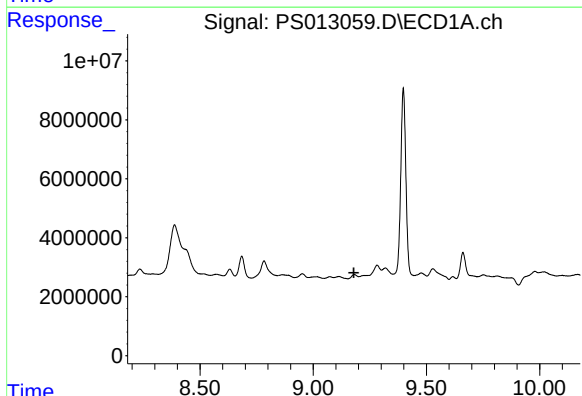


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 9.180 min
Response: 0
Conc: N.D.

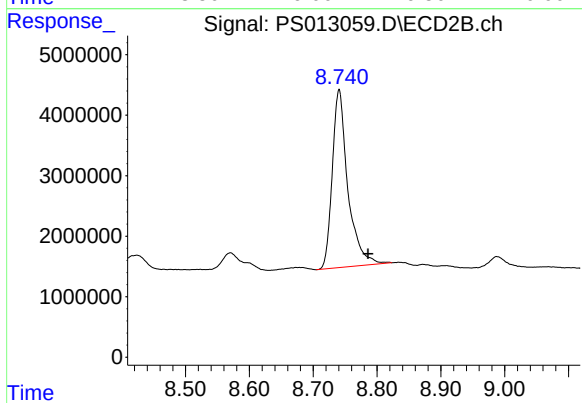

#11 2,4,5-TP (SILVEX)


R.T.: 8.741 min
Delta R.T.: -0.045 min
Response: 49833000
Conc: 21.02 ng/ml

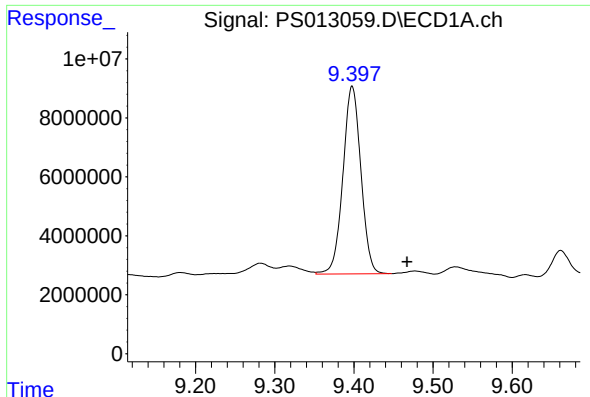

#12 2,4,5-T

R.T.: 9.398 min
Delta R.T.: -0.069 min
Response: 100300449
Conc: 19.15 ng/ml

Instrument :
ECD_S
ClientSampleId :

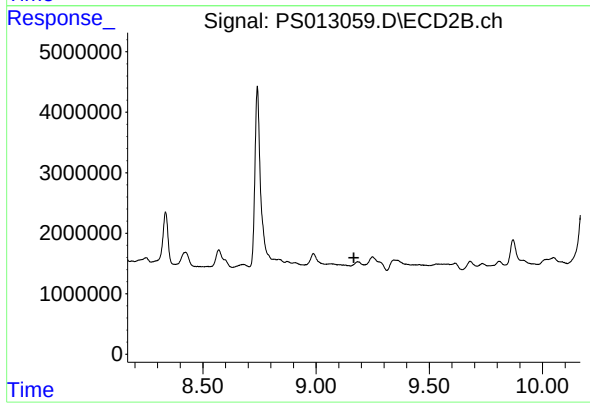

#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.167 min
Response: 0
Conc: N.D.