

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS103020\
 Data File : PS013067.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Oct 2020 21:38
 Operator : DD\AJ
 Sample : L4549-01
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 BUS-WASH-RECLAMATION-PIT

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 31 06:06:19 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102020.M
 Quant Title : 8080.M
 QLast Update : Wed Oct 21 02:27:47 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.210	6.913	398.6E6	206.2E6	445.278	513.998
Target Compounds							
1) T	Dalapon	2.988	2.589	70421519	141.6E6	69.273	269.179 #
2) T	3,5-DICHL...	0.000	6.095	0	85105729	N.D.	135.067
3) T	4-Nitroph...	7.093	0.000	7142214	0	17.078	N.D. #
5) T	DICAMBA	7.386	7.046	7527092	7501390	2.114	4.408 #
6) T	MCPD	7.618	0.000	6732846	0	2.528	N.D. #
7) T	MCPA	7.701	0.000	76119556	0	19.879	N.D. #
8) T	DICHLORPROP	0.000	7.735	0	17011730	N.D.	37.033
9) T	2,4-D	8.388	0.000	68244578	0	66.141	N.D. #
10) T	Pentachlo...	8.684	0.000	9873502	0	<MDL	N.D. #
11) T	2,4,5-TP ...	0.000	8.792	0	6001627	N.D.	2.532
12) T	2,4,5-T	9.531	0.000	12667999	0	2.419	N.D. #
14) T	DINOSEB	0.000	10.049	0	14021906	N.D.	8.338
15) T	Picloram	10.972	0.000	29307523	0	4.630	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS103020\
Data File : PS013067.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Oct 2020 21:38
Operator : DD\AJ
Sample : L4549-01
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
BUS-WASH-RECLAMATION-PIT

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 31 06:06:19 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102020.M
Quant Title : 8080.M
QLast Update : Wed Oct 21 02:27:47 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

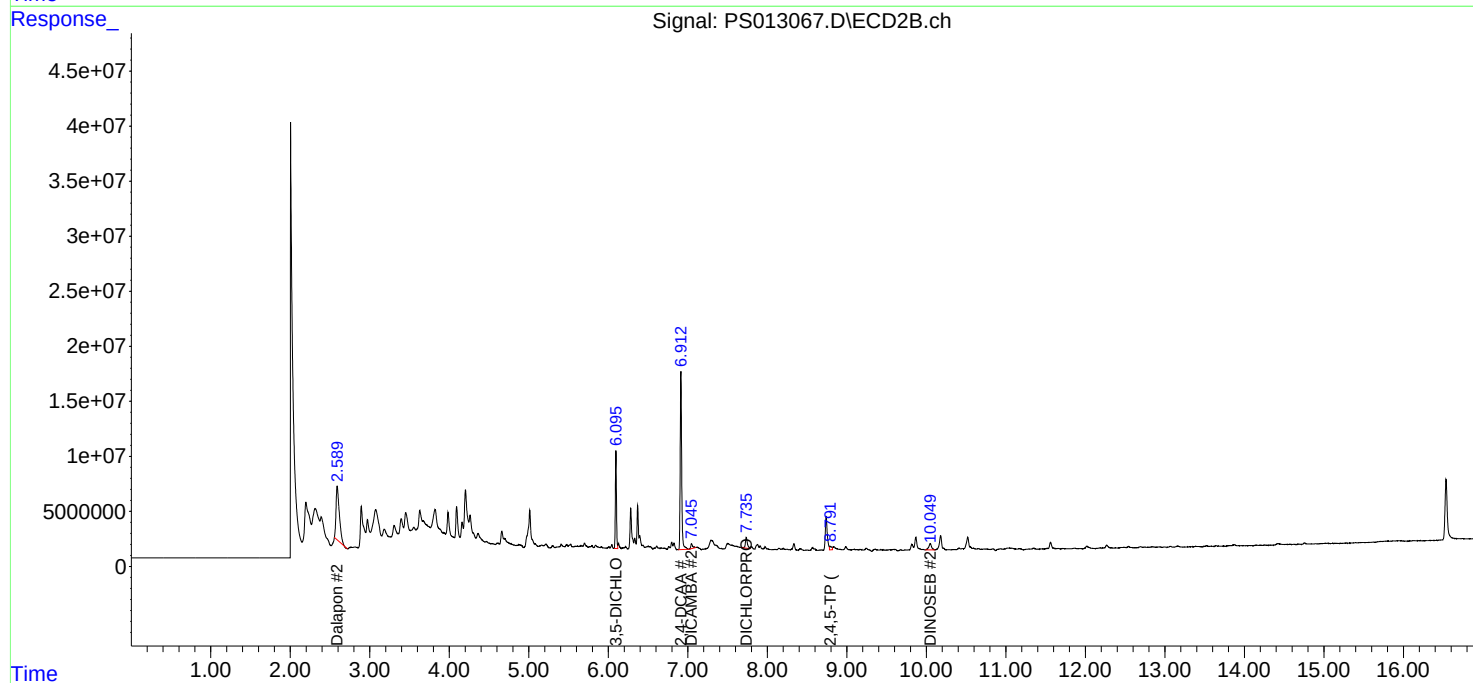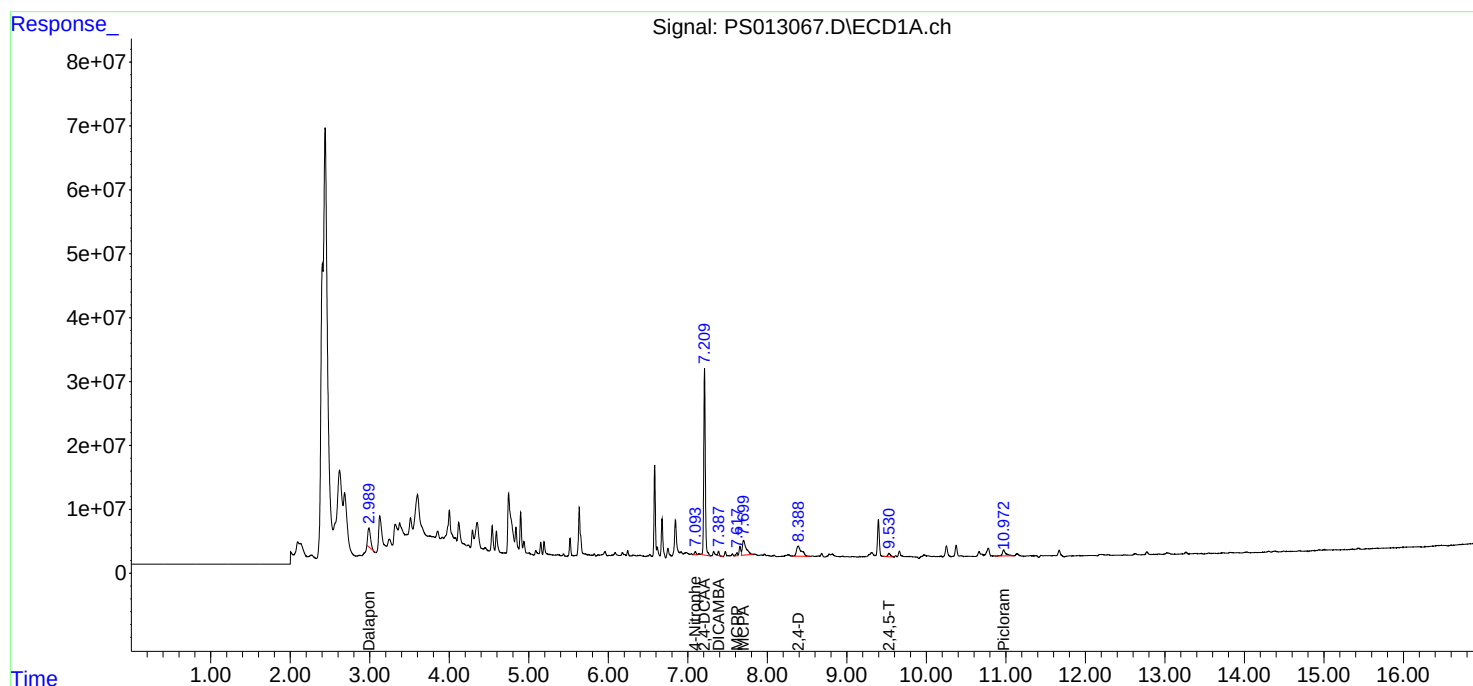


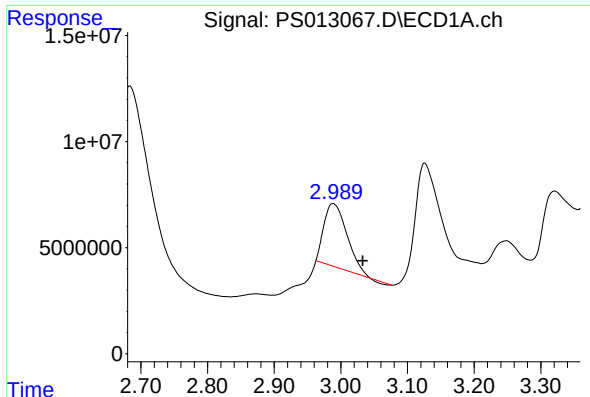

#1 Dalapon


R.T.: 2.988 min
Delta R.T.: -0.045 min
Response: 70421519
Conc: 69.27 ng/ml

Instrument :
ECD_S
ClientSampleId :
BUS-WASH-RECLAMATION-PIT

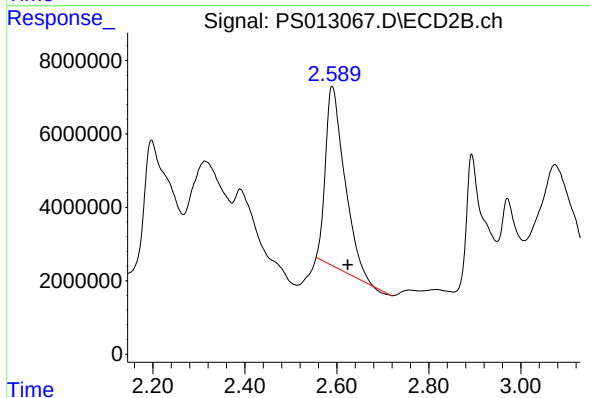


#1 Dalapon

R.T.: 2.589 min
Delta R.T.: -0.034 min
Response: 141554796
Conc: 269.18 ng/ml

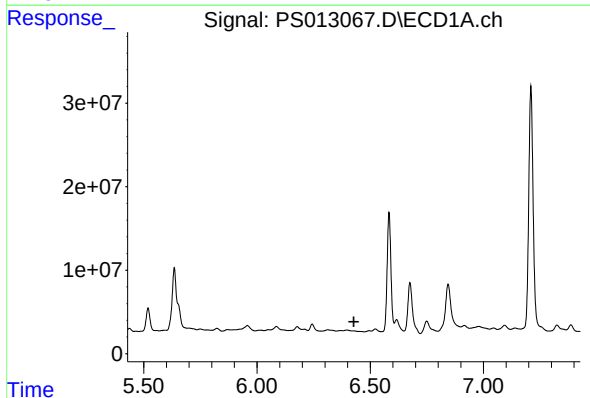


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.428 min
Response: 0
Conc: N.D.

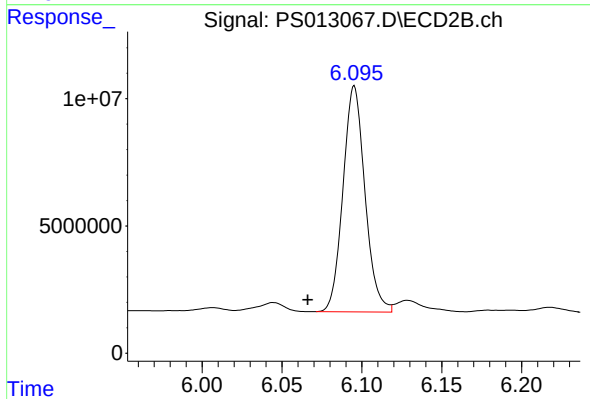

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.095 min
Delta R.T.: 0.029 min
Response: 85105729
Conc: 135.07 ng/ml

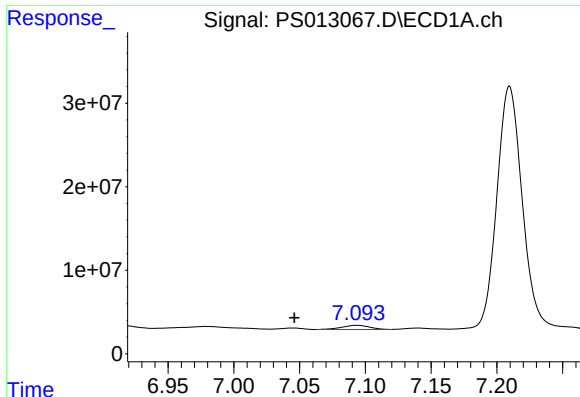

#3 4-Nitrophenol


R.T.: 7.093 min
Delta R.T.: 0.047 min
Response: 7142214
Conc: 17.08 ng/ml

Instrument :
ECD_S
ClientSampleId :
BUS-WASH-RECLAMATION-PIT

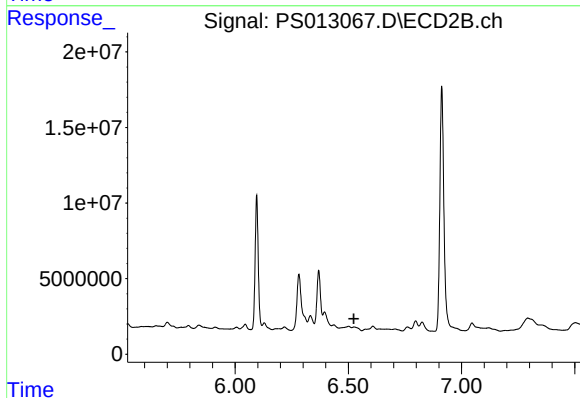


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.525 min
Response: 0
Conc: N.D.

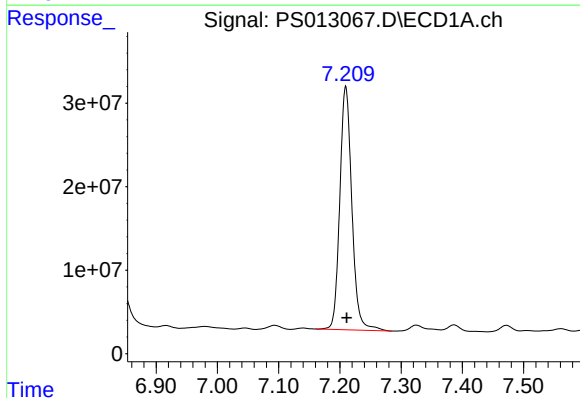


#4 2,4-DCAA

R.T.: 7.210 min
Delta R.T.: -0.002 min
Response: 398554690
Conc: 445.28 ng/ml

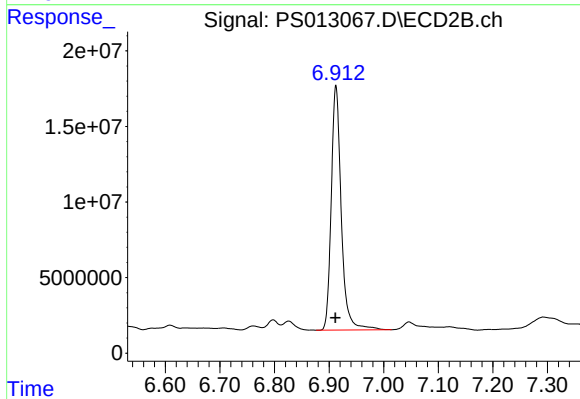

#4 2,4-DCAA


R.T.: 6.913 min
Delta R.T.: 0.000 min
Response: 206242379
Conc: 514.00 ng/ml

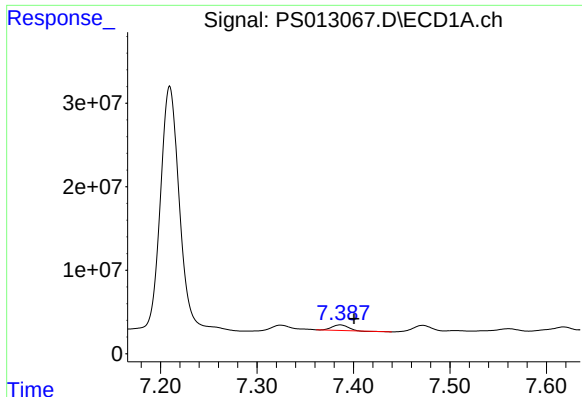

#5 DICAMBA


R.T.: 7.386 min
Delta R.T.: -0.015 min
Response: 7527092
Conc: 2.11 ng/ml

Instrument :
ECD_S
ClientSampleId :
BUS-WASH-RECLAMATION-PIT

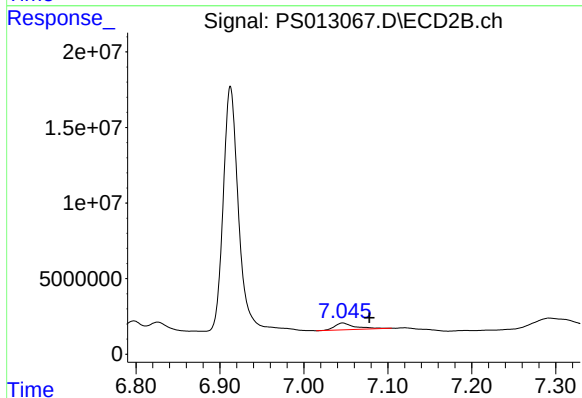


#5 DICAMBA

R.T.: 7.046 min
Delta R.T.: -0.032 min
Response: 7501390
Conc: 4.41 ng/ml

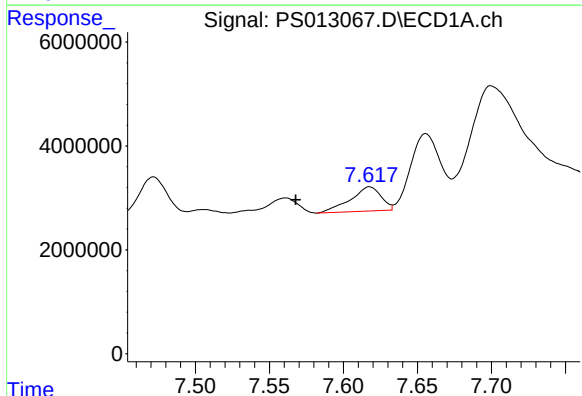


#6 MCP

R.T.: 7.618 min
Delta R.T.: 0.050 min
Response: 6732846
Conc: 2.53 ug/ml

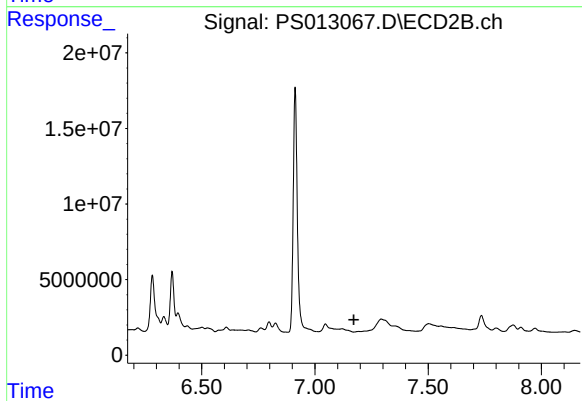

#6 MCP


R.T.: 0.000 min
Exp R.T.: 7.172 min
Response: 0
Conc: N.D.

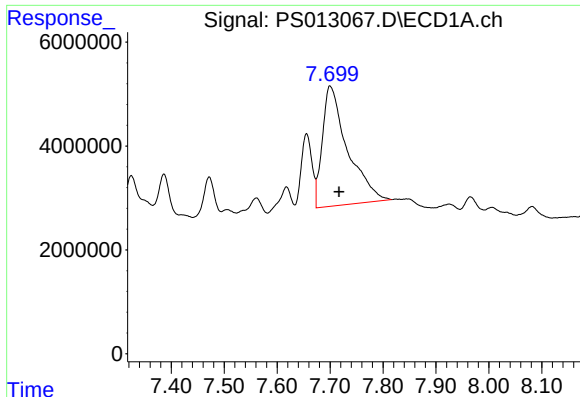

#7 MCPA


R.T.: 7.701 min
Delta R.T.: -0.017 min
Response: 76119556
Conc: 19.88 ug/ml

Instrument :
ECD_S
ClientSampleId :
BUS-WASH-RECLAMATION-PIT

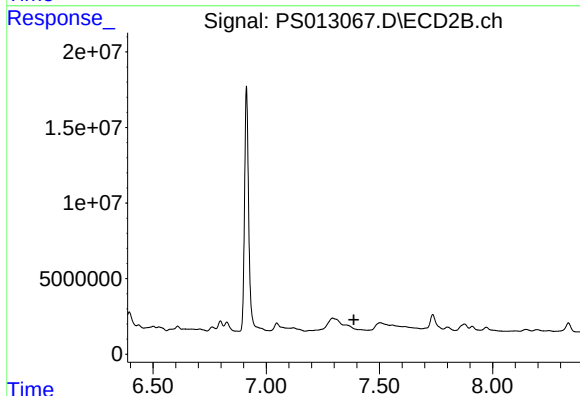


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.387 min
Response: 0
Conc: N.D.

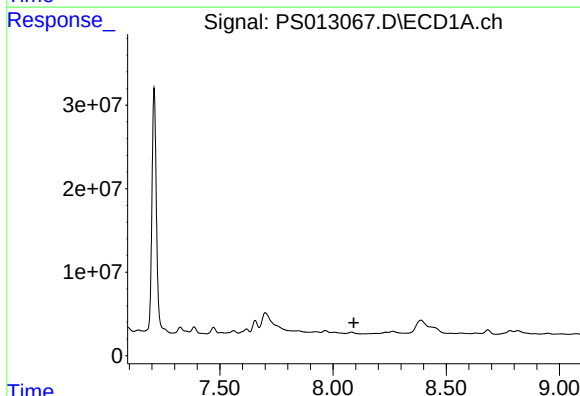


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.092 min
Response: 0
Conc: N.D.

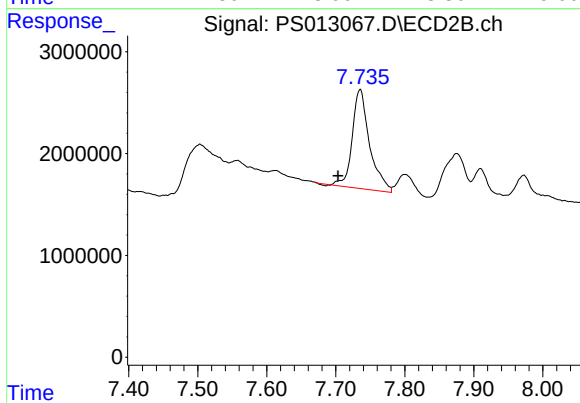

#8 DICHLORPROP


R.T.: 7.735 min
Delta R.T.: 0.032 min
Response: 17011730
Conc: 37.03 ng/ml

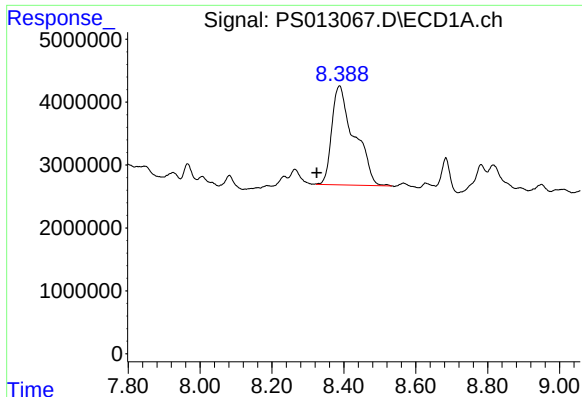

#9 2,4-D


R.T.: 8.388 min
Delta R.T.: 0.063 min
Response: 68244578
Conc: 66.14 ng/ml

Instrument :
ECD_S
ClientSampleId :
BUS-WASH-RECLAMATION-PIT

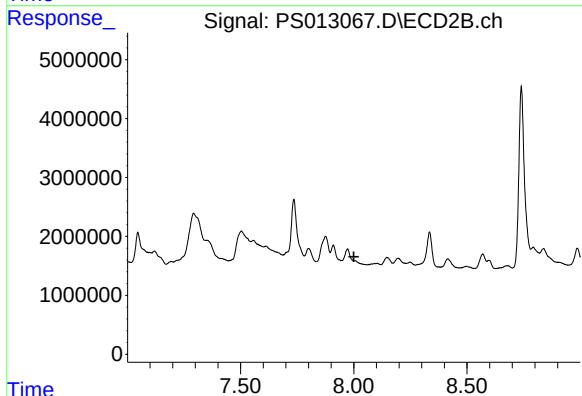


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 8.001 min
Response: 0
Conc: N.D.

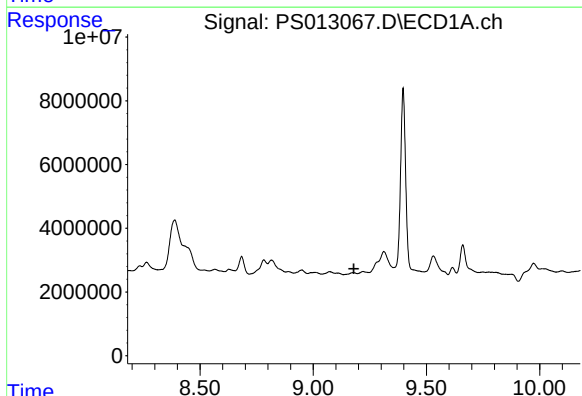


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 9.180 min
Response: 0
Conc: N.D.

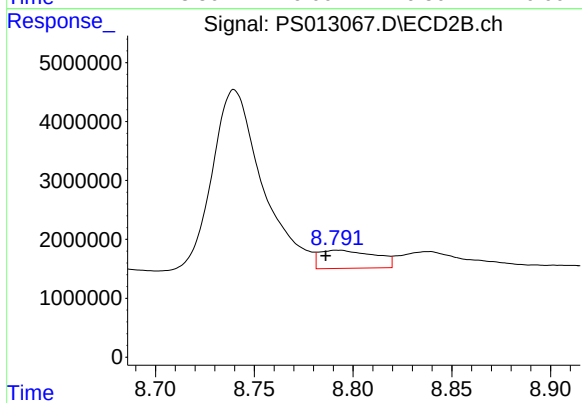

#11 2,4,5-TP (SILVEX)


R.T.: 8.792 min
Delta R.T.: 0.006 min
Response: 6001627
Conc: 2.53 ng/ml

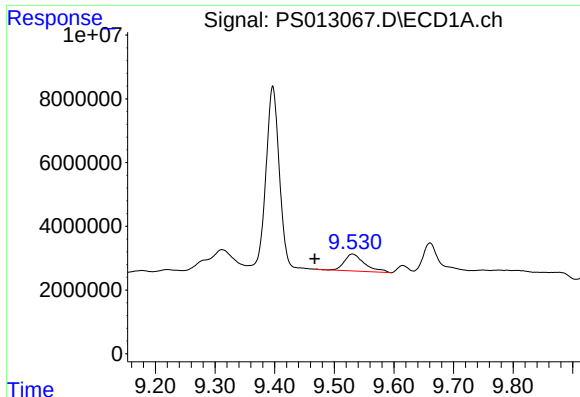

#12 2,4,5-T


R.T.: 9.531 min
Delta R.T.: 0.063 min
Response: 12667999
Conc: 2.42 ng/ml

Instrument :
ECD_S
ClientSampleId :
BUS-WASH-RECLAMATION-PIT

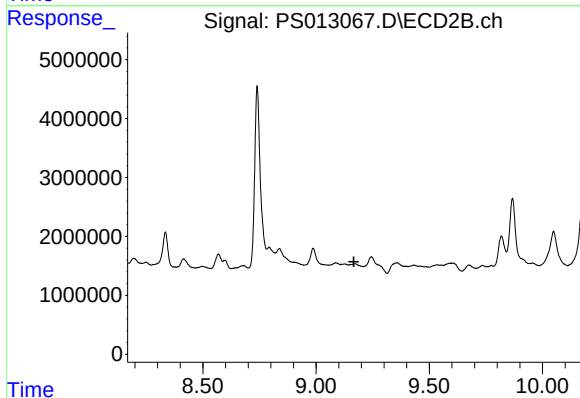


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.167 min
Response: 0
Conc: N.D.

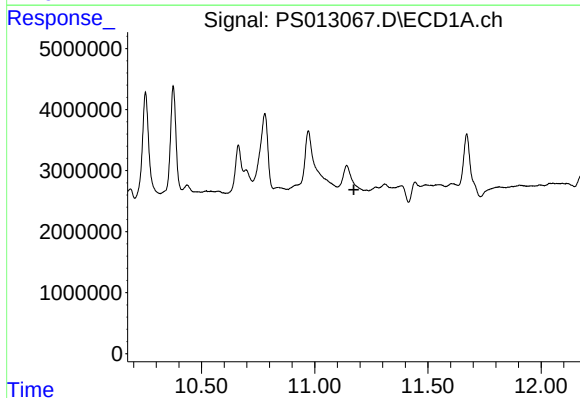


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 11.173 min
Response: 0
Conc: N.D.

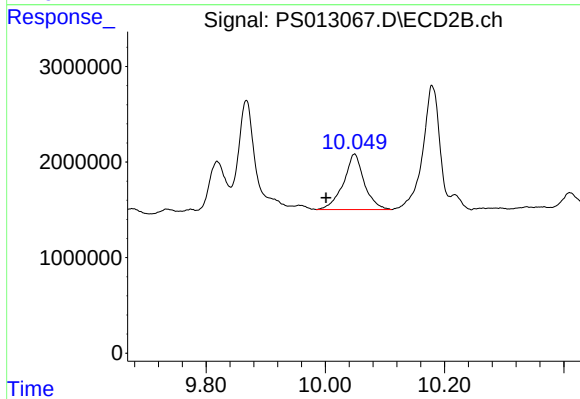

#14 DINOSEB


R.T.: 10.049 min
Delta R.T.: 0.048 min
Response: 14021906
Conc: 8.34 ng/ml

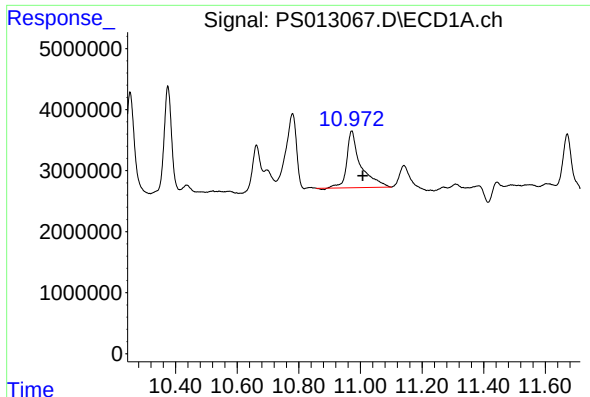

#15 Picloram

R.T.: 10.972 min
Delta R.T.: -0.036 min
Response: 29307523
Conc: 4.63 ng/ml

Instrument :
ECD_S
ClientSampleId :
BUS-WASH-RECLAMATION-PIT

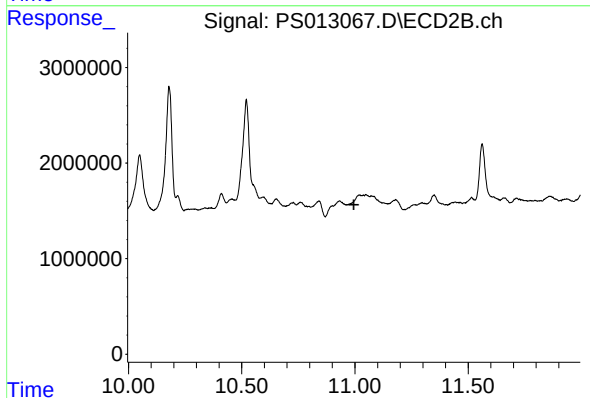

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 10.995 min
Response: 0
Conc: N.D.