

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS103118\
 Data File : PS002223.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Oct 2018 10:20
 Operator : EI\SJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 01 02:24:06 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102618.M
 Quant Title : 8080.M
 QLast Update : Sat Oct 27 01:34:10 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.409	10.909	5422735	104372	17.232	0.291 #
Target Compounds							
1) T	Dalapon	0.000	2.436	0 45065233		N.D.	99.811 #
2) T	3,5-DICHL...	0.000	9.078	0 214080		N.D.	0.483 #
3) T	4-Nitroph...	0.000	10.056	0 335236		N.D.	1.880 #
5) T	DICAMBA	0.000	11.186	0 124721		N.D.	0.100 #
6) T	MCP	0.000	11.445	0 1540084		N.D.	1.790 #
7) T	MCPA	0.000	11.815	0 459728		N.D.	0.340 #
10) T	Pentachlo...	0.000	13.335	0 107404		N.D.	0.023 #
11) T	2,4,5-TP ...	0.000	13.949	0 191477		N.D.	0.105 #
12) T	2,4,5-T	0.000	14.517	0 13487779		N.D.	9.007 #
14) T	DINOSEB	0.000	15.590	0 392701		N.D.	0.310 #
15) T	Picloram	16.921	16.774	16174467	1101685	6.781	0.487 #
16) T	DCPA	0.000	16.827	0 20465958		N.D.	8.643 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS103118\
Data File : PS002223.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Oct 2018 10:20
Operator : EI\SJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 01 02:24:06 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102618.M
Quant Title : 8080.M
QLast Update : Sat Oct 27 01:34:10 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

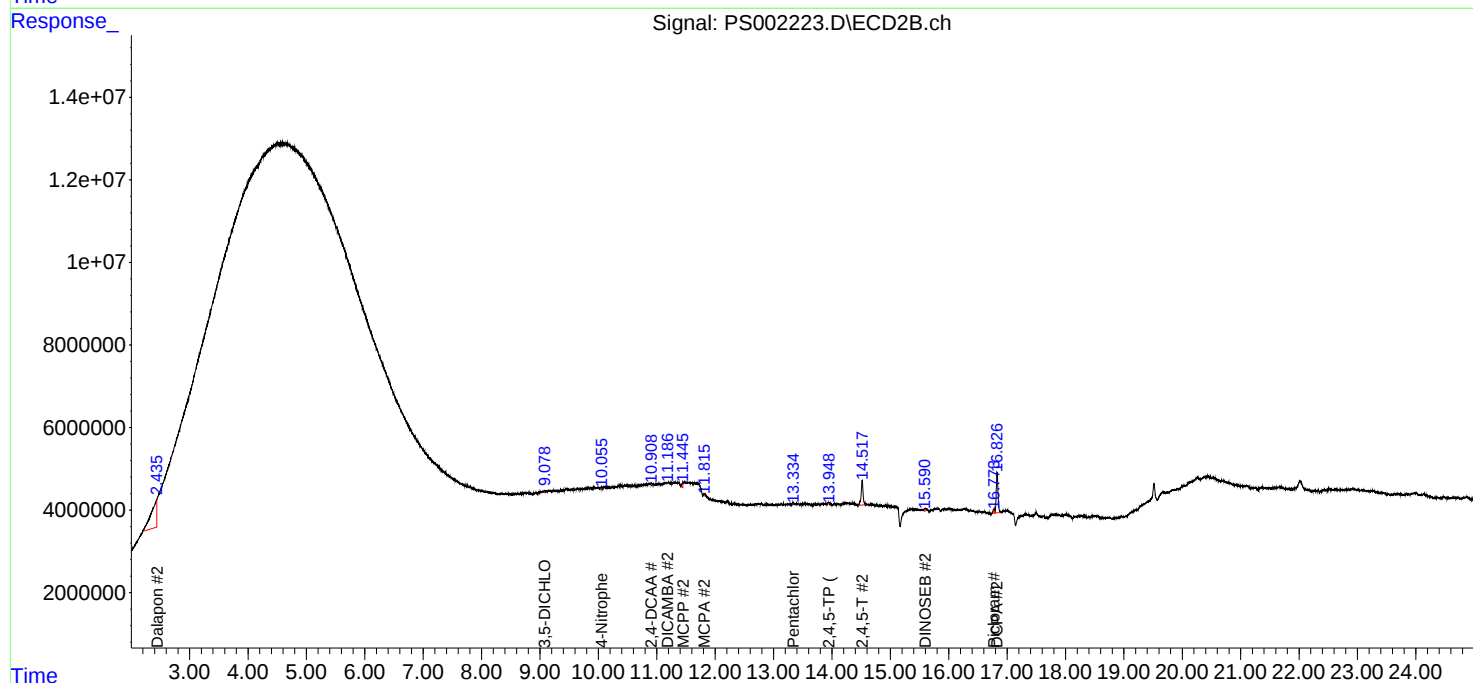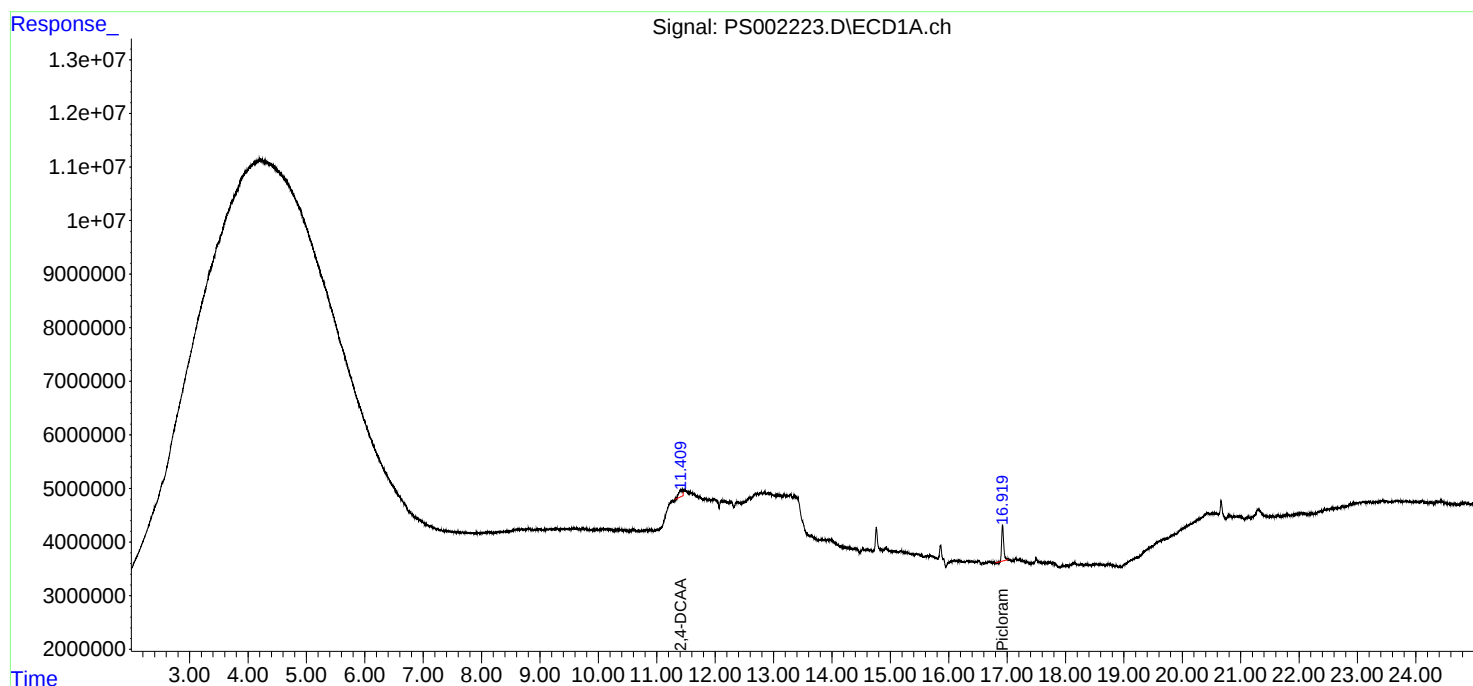


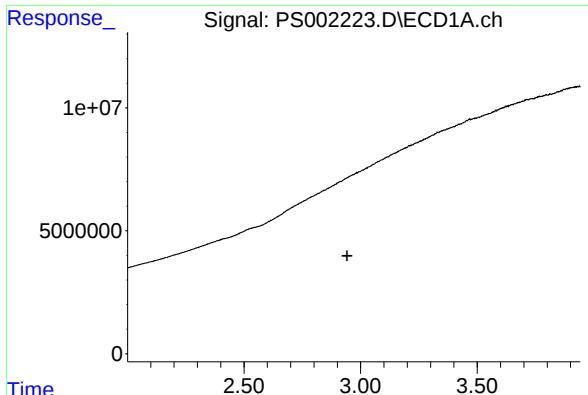

#1 Dalapon


R.T.: 0.000 min
Exp R.T. : 2.942 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

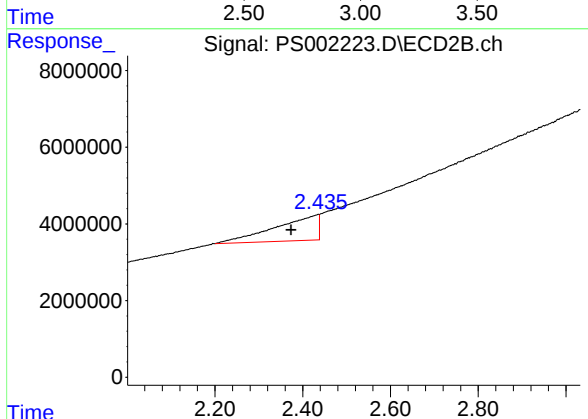


#1 Dalapon

R.T.: 2.436 min
Delta R.T.: 0.063 min
Response: 45065233
Conc: 99.81 ng/ml

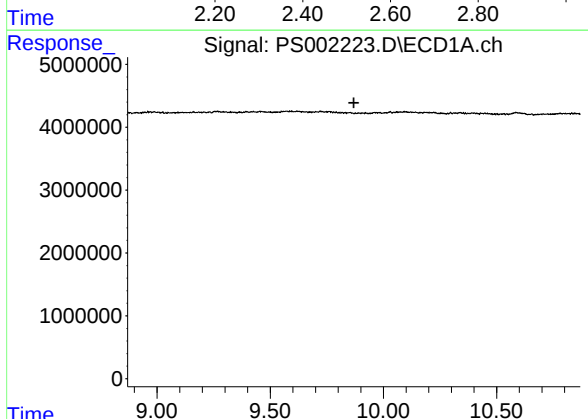


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.870 min
Response: 0
Conc: N.D.

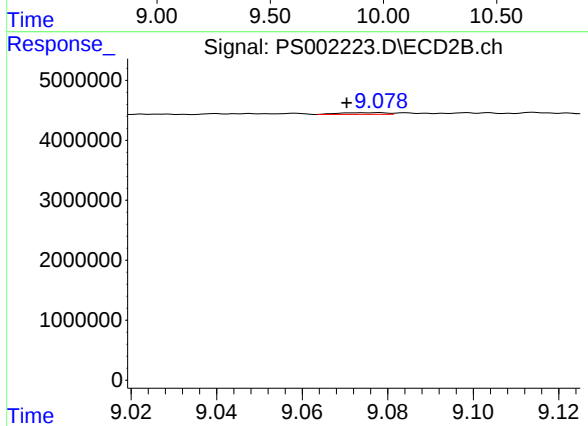

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.078 min
Delta R.T.: 0.008 min
Response: 214080
Conc: 0.48 ng/ml

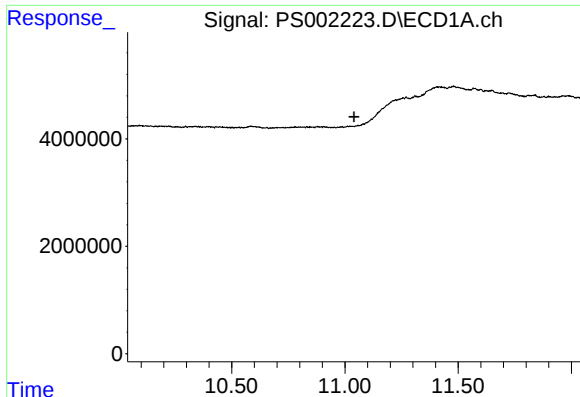

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 11.040 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

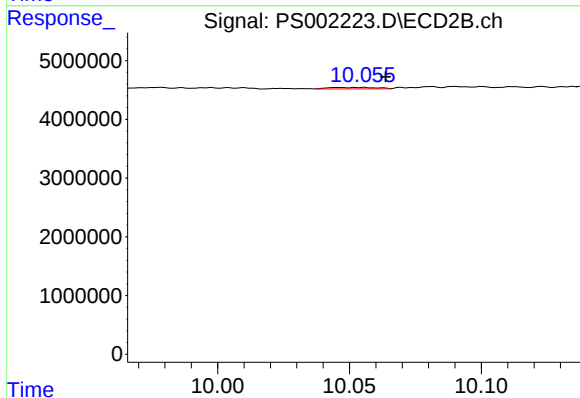


#3 4-Nitrophenol

R.T.: 10.056 min
Delta R.T.: -0.008 min
Response: 335236
Conc: 1.88 ng/ml

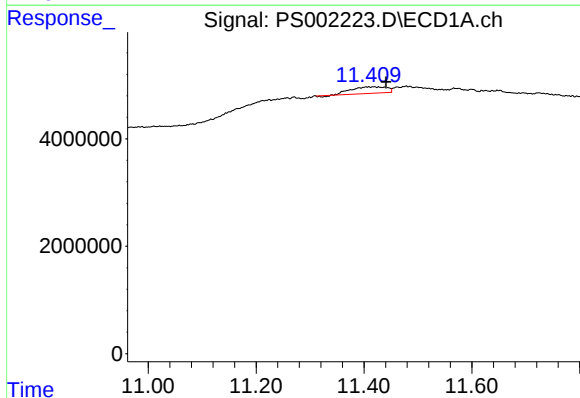


#4 2,4-DCAA

R.T.: 11.409 min
Delta R.T.: -0.032 min
Response: 5422735
Conc: 17.23 ng/ml

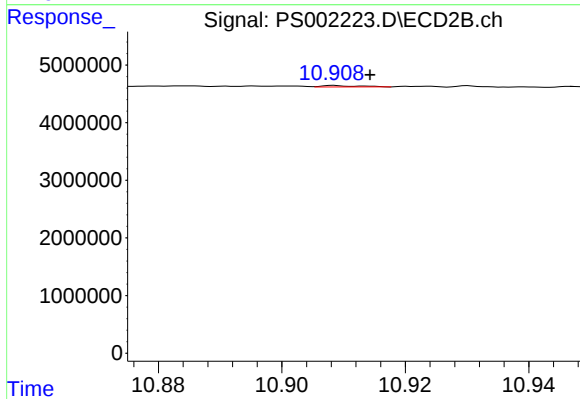

#4 2,4-DCAA


R.T.: 10.909 min
Delta R.T.: -0.006 min
Response: 104372
Conc: 0.29 ng/ml

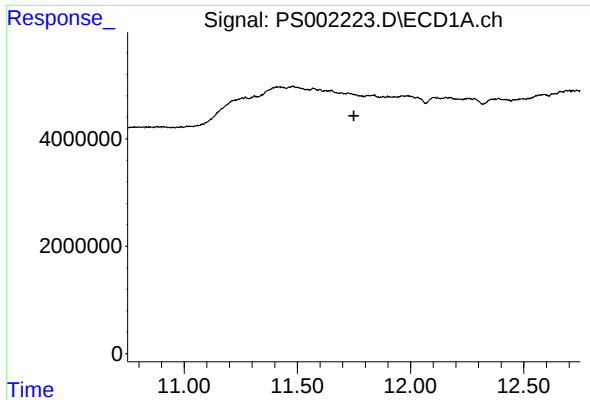

#5 DICAMBA


R.T.: 0.000 min
Exp R.T. : 11.750 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

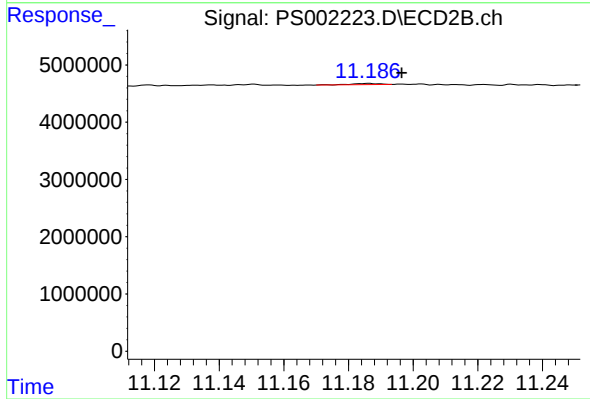


#5 DICAMBA

R.T.: 11.186 min
Delta R.T.: -0.010 min
Response: 124721
Conc: 0.10 ng/ml

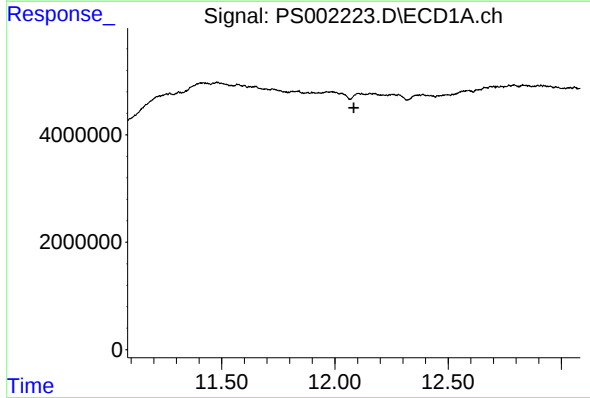


#6 MCP

R.T.: 0.000 min
Exp R.T. : 12.084 min
Response: 0
Conc: N.D.

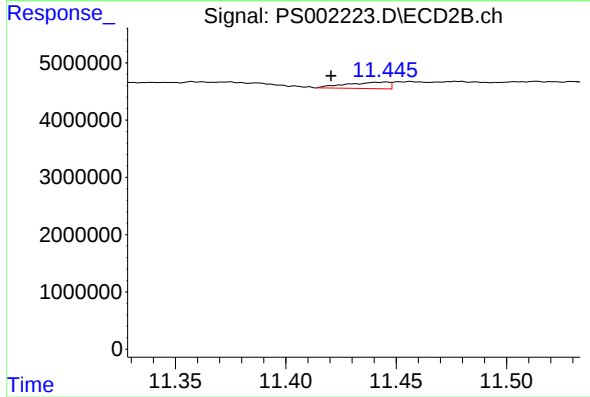

#6 MCP


R.T.: 11.445 min
Delta R.T.: 0.025 min
Response: 1540084
Conc: 1.79 ug/ml

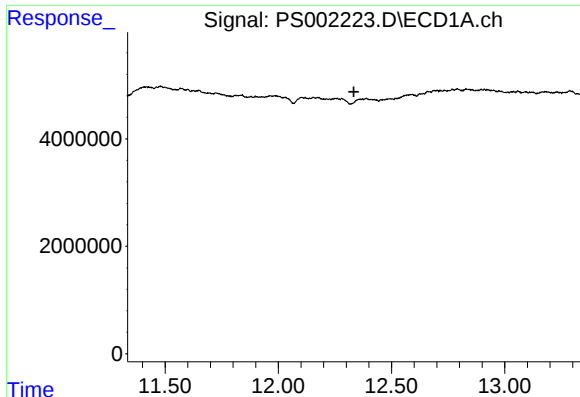

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 12.333 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

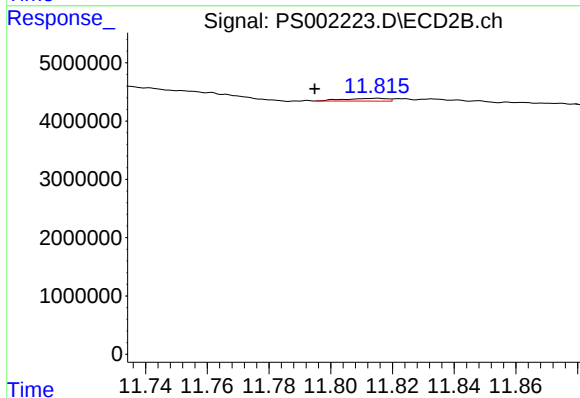


#7 MCPA

R.T.: 11.815 min
Delta R.T.: 0.020 min
Response: 459728
Conc: 0.34 ug/ml

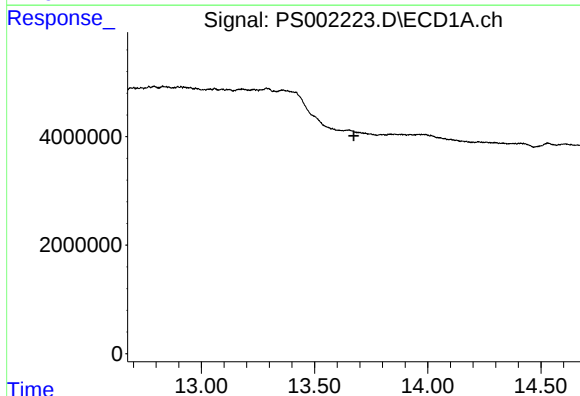


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 13.674 min
Response: 0
Conc: N.D.

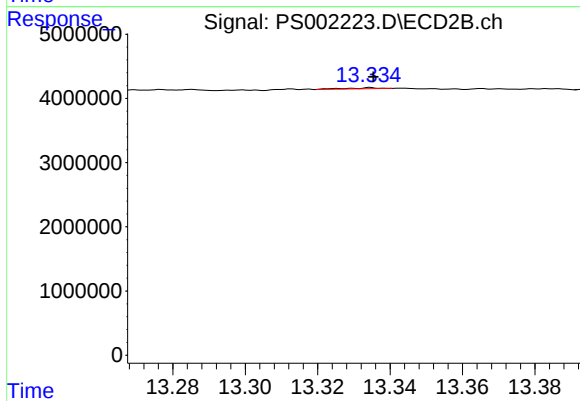

#10 Pentachlorophenol


R.T.: 13.335 min
Delta R.T.: 0.000 min
Response: 107404
Conc: 0.02 ng/ml

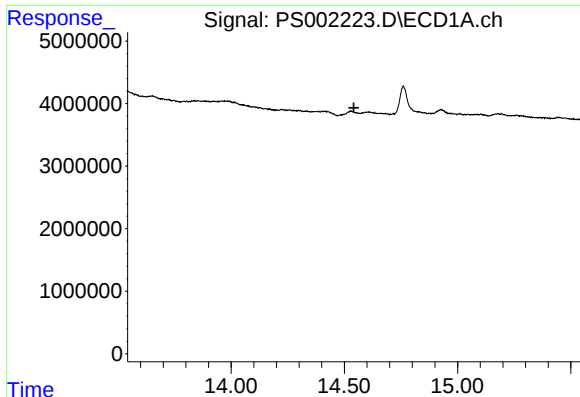

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 14.542 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

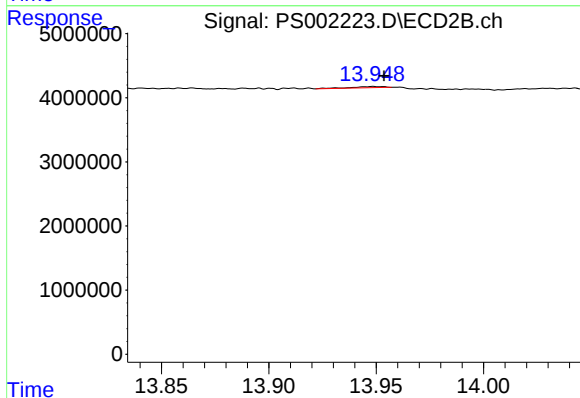


#11 2,4,5-TP (SILVEX)

R.T.: 13.949 min
Delta R.T.: -0.005 min
Response: 191477
Conc: 0.10 ng/ml

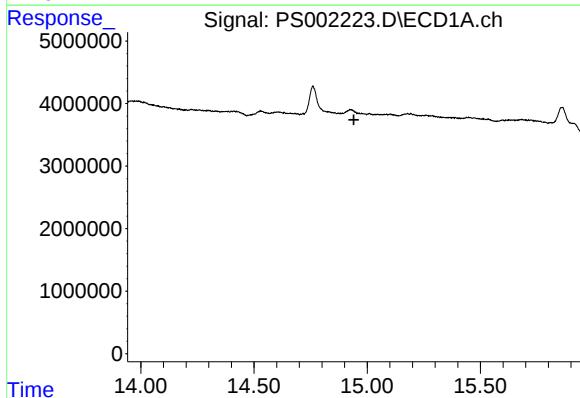


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 14.941 min
Response: 0
Conc: N.D.

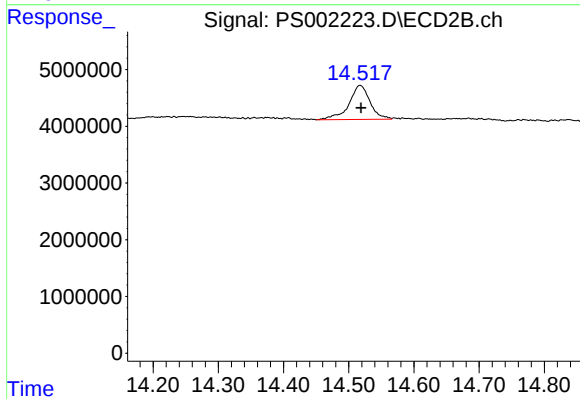

#12 2,4,5-T


R.T.: 14.517 min
Delta R.T.: -0.002 min
Response: 13487779
Conc: 9.01 ng/ml

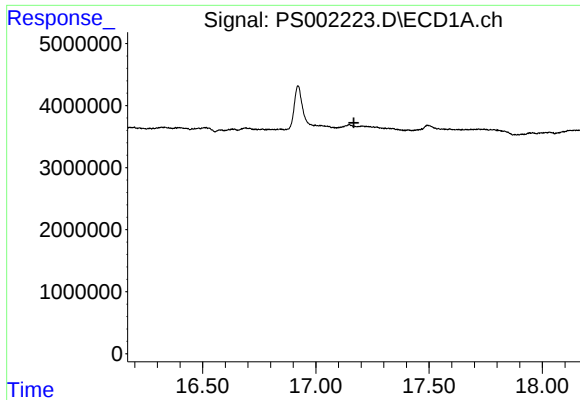

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 17.168 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

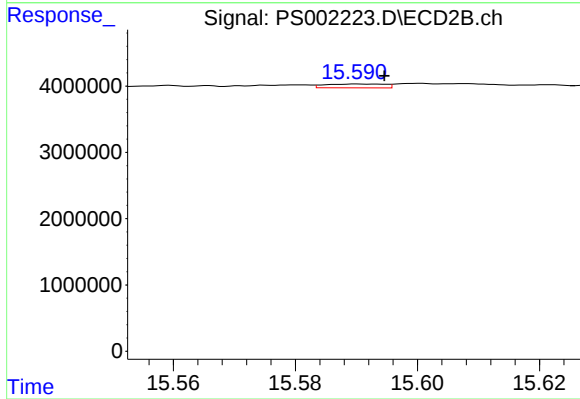


#14 DINOSEB

R.T.: 15.590 min
Delta R.T.: -0.004 min
Response: 392701
Conc: 0.31 ng/ml

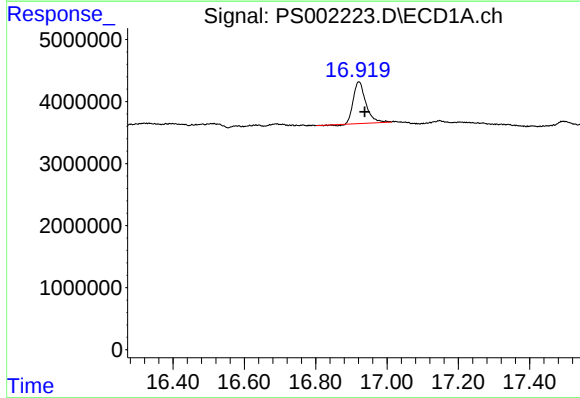


#15 Picloram

R.T.: 16.921 min
Delta R.T.: -0.016 min
Response: 16174467
Conc: 6.78 ng/ml

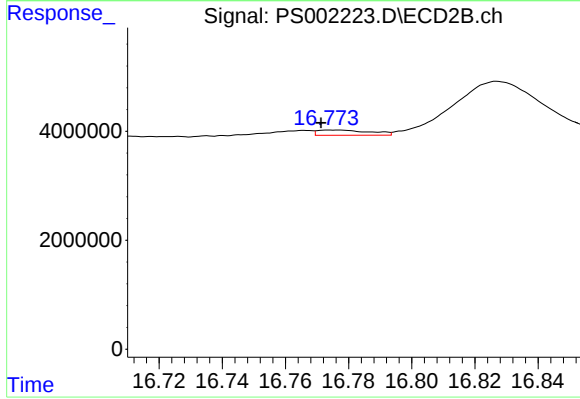

#15 Picloram


R.T.: 16.774 min
Delta R.T.: 0.002 min
Response: 1101685
Conc: 0.49 ng/ml

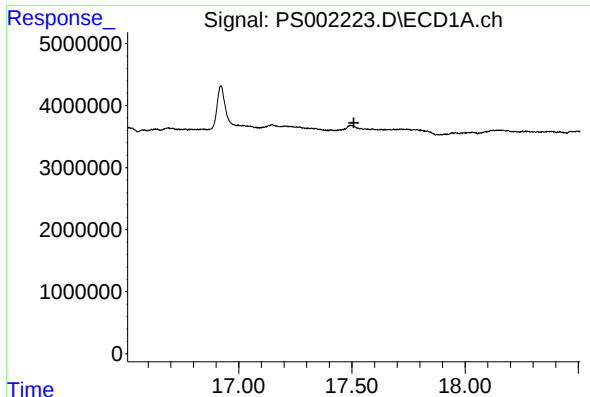

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.509 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

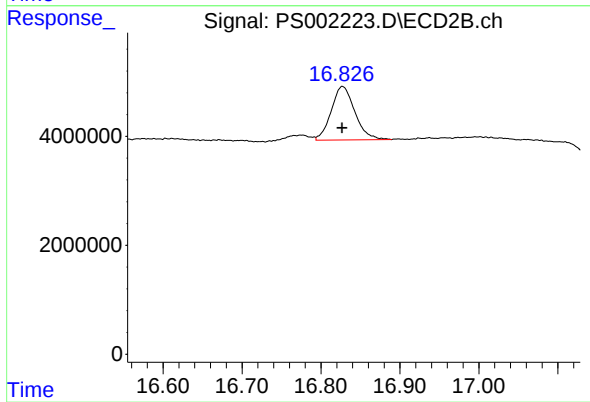

#16 DCPA

R.T.: 16.827 min
Delta R.T.: 0.000 min
Response: 20465958
Conc: 8.64 ng/ml