

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS103119\
 Data File : PS007526.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Oct 2019 08:54
 Operator : SM\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 31 14:38:31 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 14 13:54:23 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.452	5.176	564.8E6	287.7E6	412.679	409.035
Target Compounds							
7) T	MCPA	0.000	5.491	0	38945315	N.D.	13.396
12) T	2,4,5-T	0.000	7.232	0	37810469	N.D.	10.792
15) T	Picloram	8.963	8.916	320.1E6	191.6E6	29.004	31.208
16) T	DCPA	0.000	8.916	0	191.6E6	N.D.	38.213



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS103119\
Data File : PS007526.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Oct 2019 08:54
Operator : SM\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 31 14:38:31 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
Quant Title : 8080.M
QLast Update : Mon Oct 14 13:54:23 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

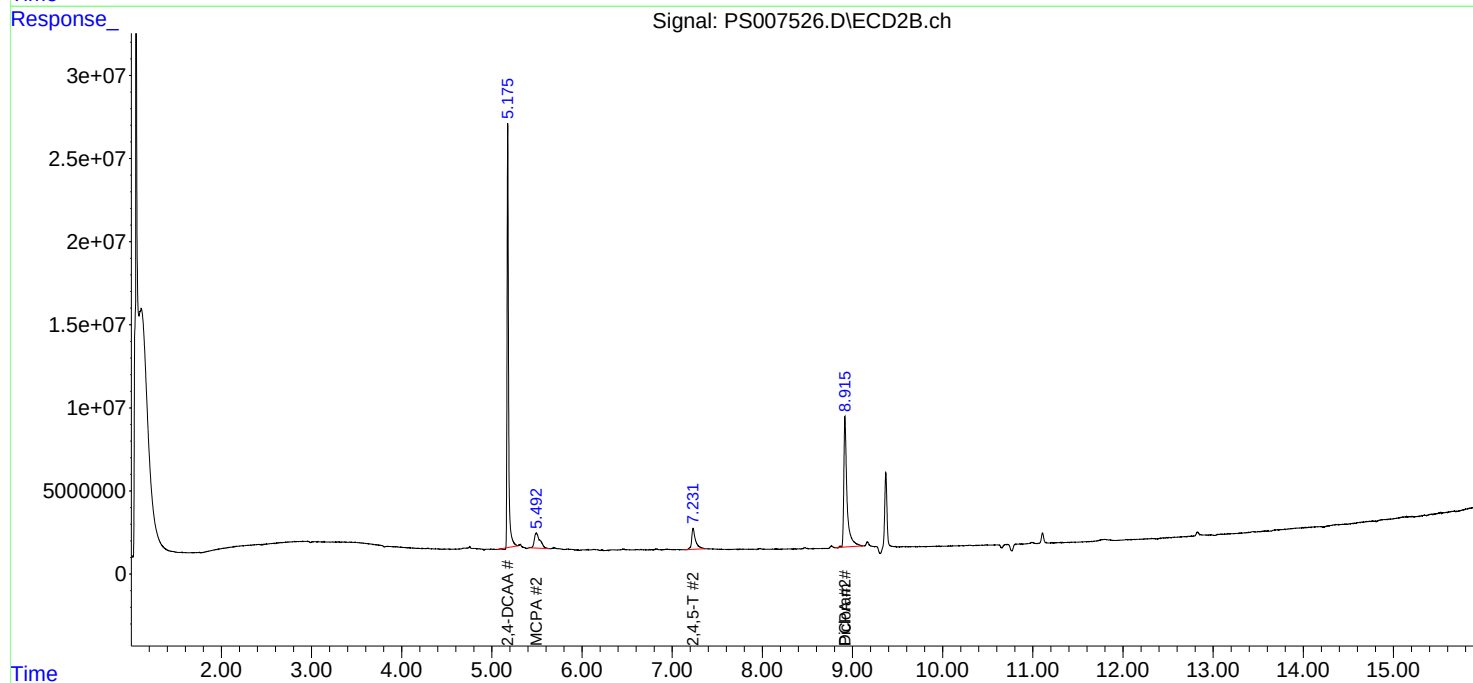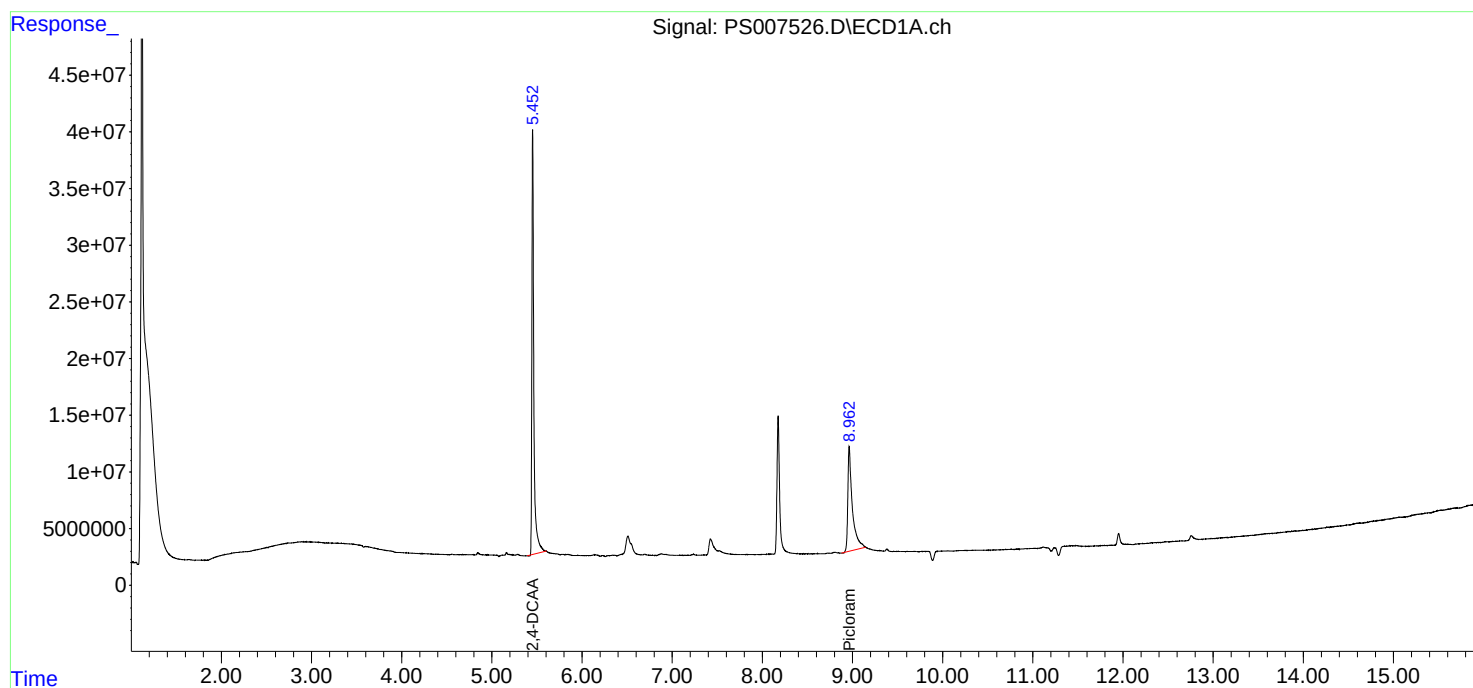


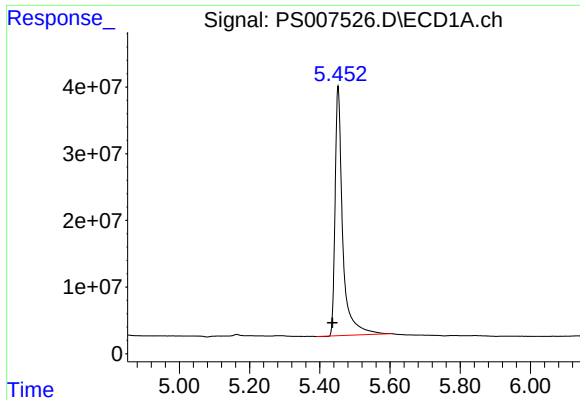

#4 2,4-DCAA


R.T.: 5.452 min
Delta R.T.: 0.017 min
Response: 564820911
Conc: 412.68 ng/ml

Instrument :
ECD_S
ClientSampleId :

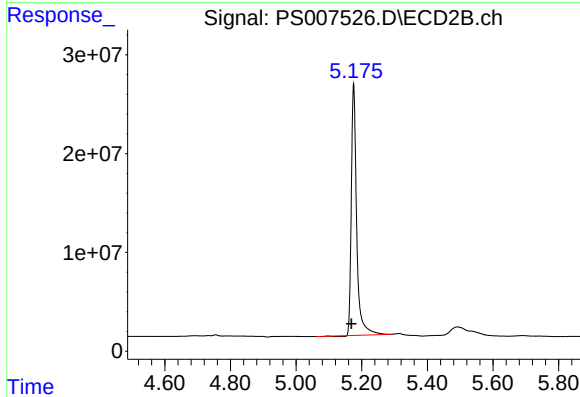


#4 2,4-DCAA

R.T.: 5.176 min
Delta R.T.: 0.007 min
Response: 287676776
Conc: 409.03 ng/ml

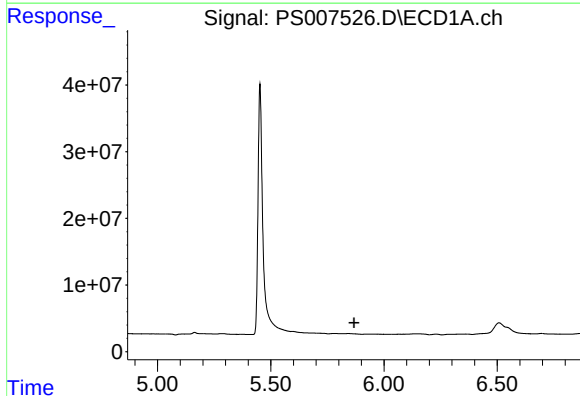


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 5.867 min
Response: 0
Conc: N.D.

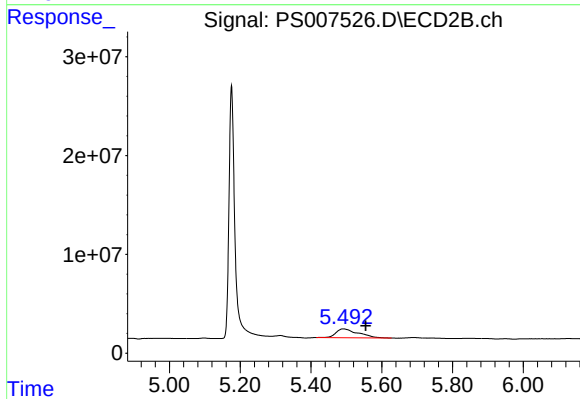

#7 MCPA


R.T.: 5.491 min
Delta R.T.: -0.063 min
Response: 38945315
Conc: 13.40 ug/ml

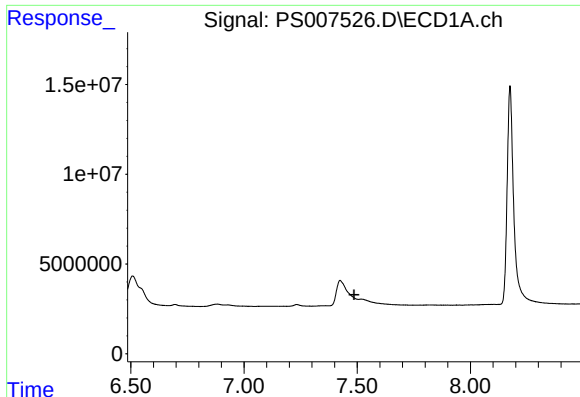

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 7.486 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

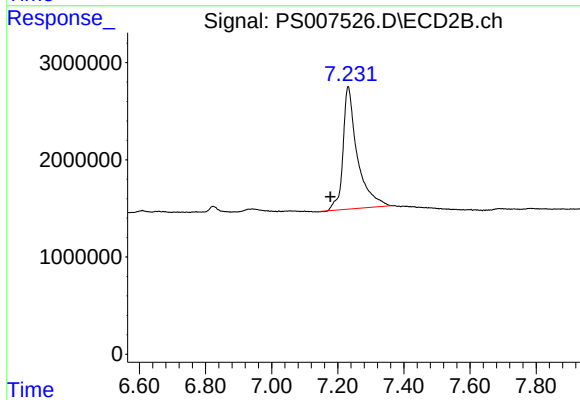


#12 2,4,5-T

R.T.: 7.232 min
Delta R.T.: 0.053 min
Response: 37810469
Conc: 10.79 ng/ml

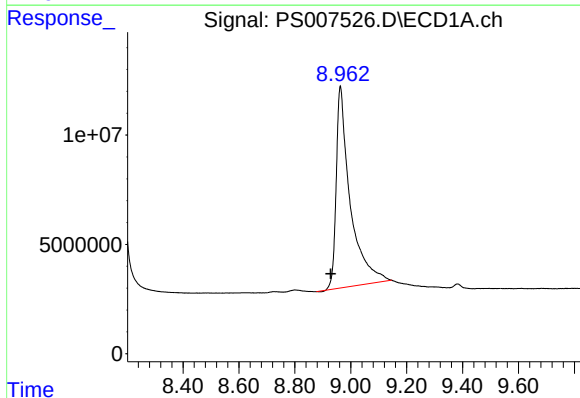


#15 Picloram

R.T.: 8.963 min
Delta R.T.: 0.034 min
Response: 320124949
Conc: 29.00 ng/ml

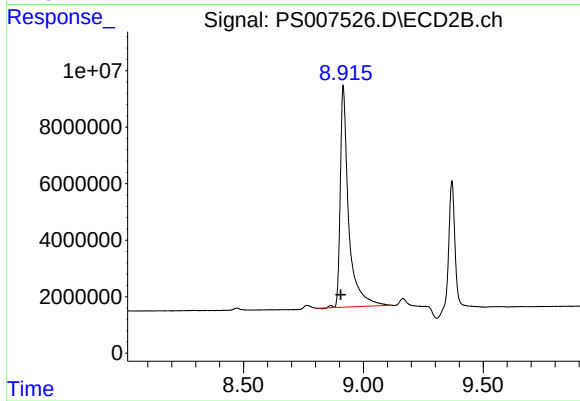

#15 Picloram


R.T.: 8.916 min
Delta R.T.: 0.011 min
Response: 191623828
Conc: 31.21 ng/ml

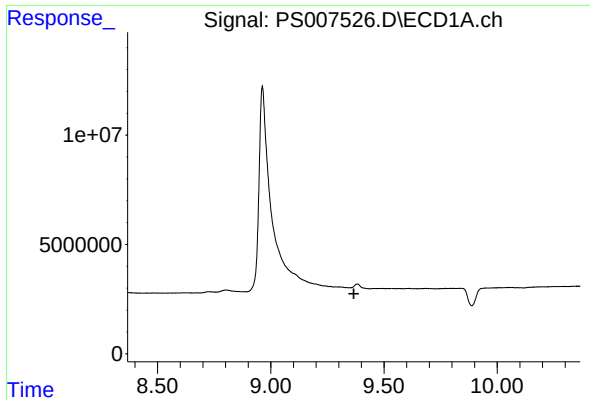

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 9.367 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

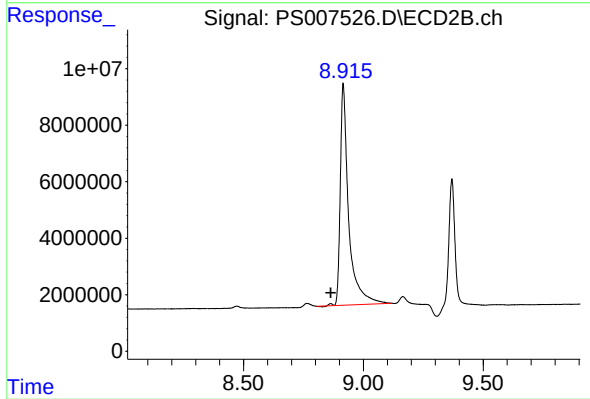

#16 DCPA

R.T.: 8.916 min
Delta R.T.: 0.052 min
Response: 191623828
Conc: 38.21 ng/ml