

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS103119\
 Data File : PS007531.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Oct 2019 12:14
 Operator : SM\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 31 14:39:40 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 14 13:54:23 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.467	5.187	585.9E6	297.4E6	428.045	422.823
Target Compounds							
3) T	4-Nitroph...	0.000	4.826	0 75005856		N.D.	189.939
15) T	Picloram	0.000	8.933	0 13807028		N.D.	2.249
16) T	DCPA	0.000	8.933	0 13807028		N.D.	2.753



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS103119\
Data File : PS007531.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Oct 2019 12:14
Operator : SM\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 31 14:39:40 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
Quant Title : 8080.M
QLast Update : Mon Oct 14 13:54:23 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

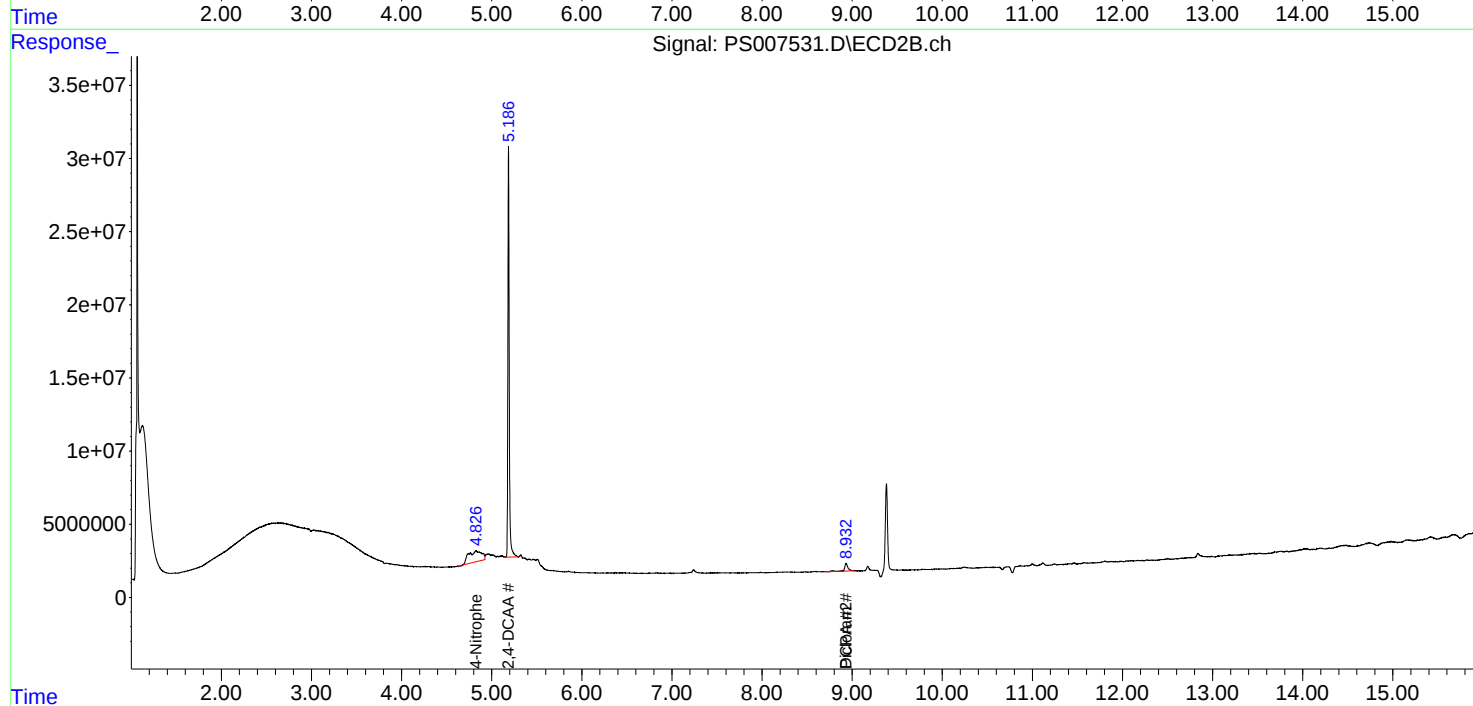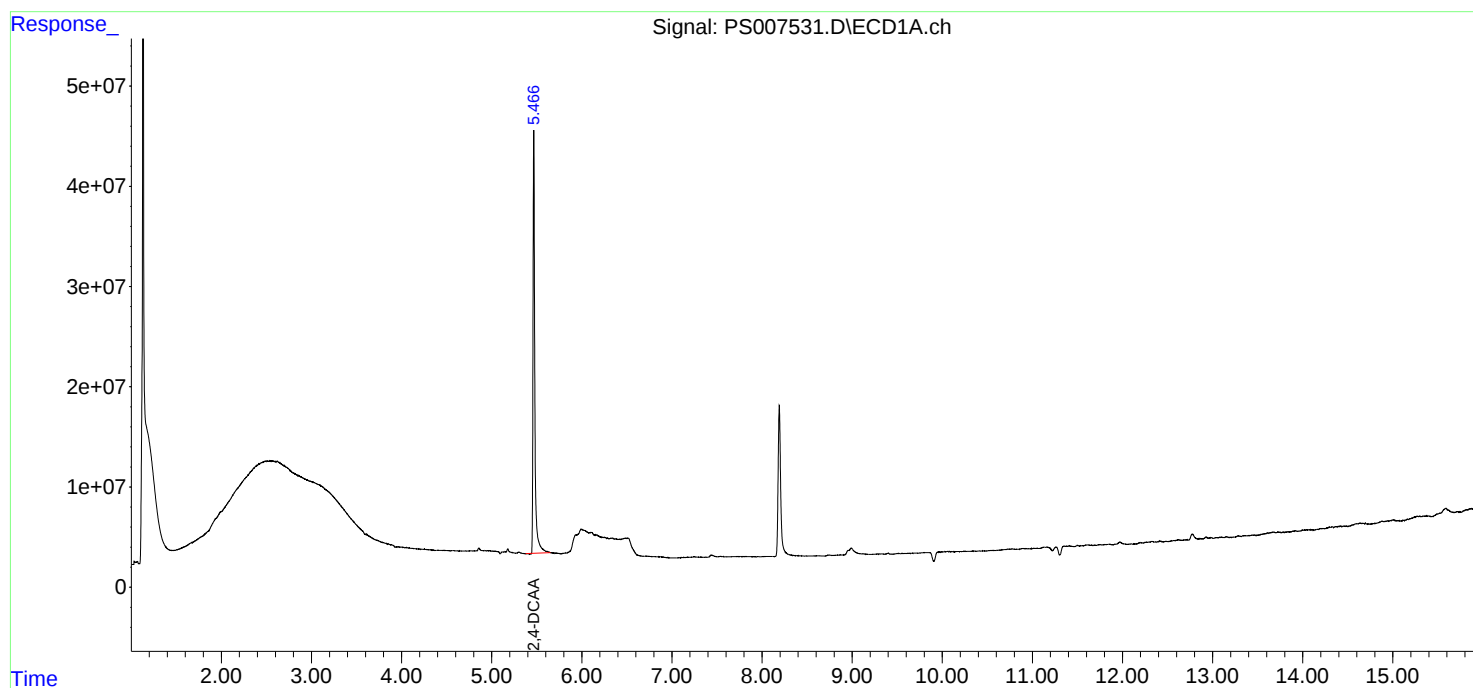


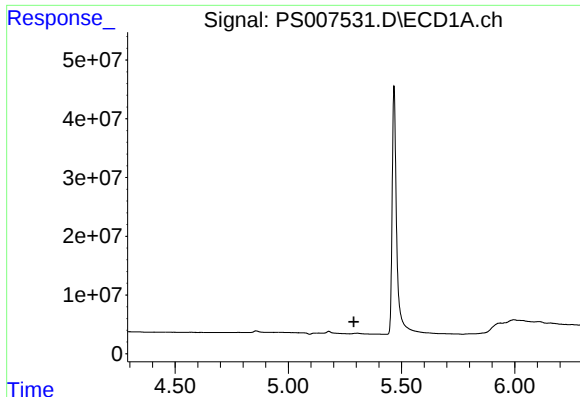

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 5.290 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

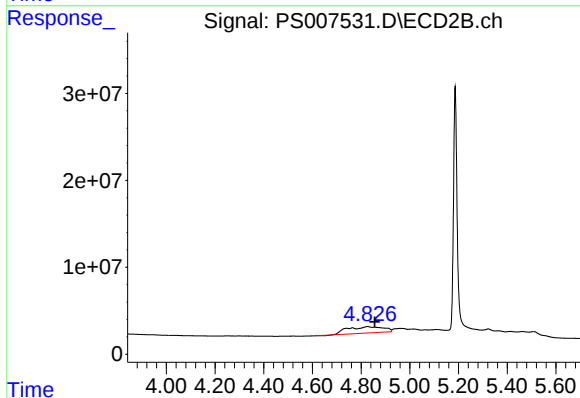


#3 4-Nitrophenol

R.T.: 4.826 min
Delta R.T.: -0.030 min
Response: 75005856
Conc: 189.94 ng/ml

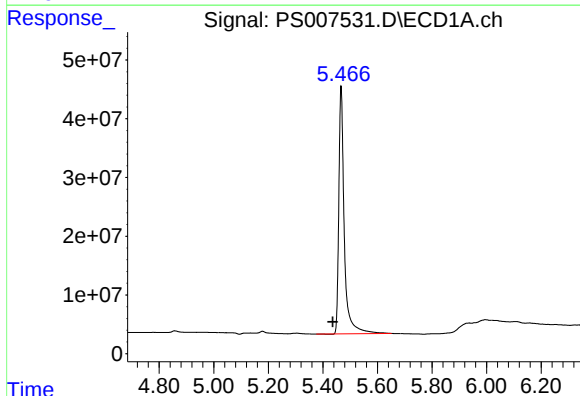


#4 2,4-DCAA

R.T.: 5.467 min
Delta R.T.: 0.032 min
Response: 585851933
Conc: 428.05 ng/ml

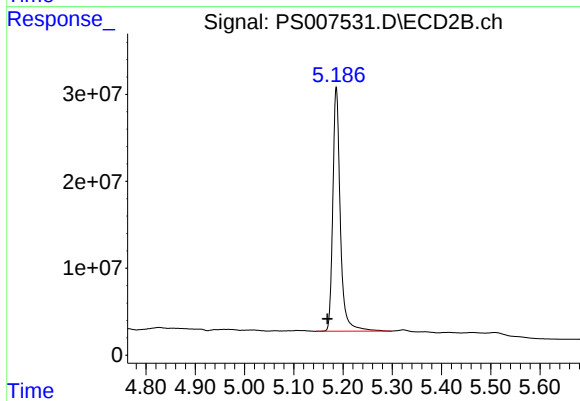

#4 2,4-DCAA


R.T.: 5.187 min
Delta R.T.: 0.018 min
Response: 297373940
Conc: 422.82 ng/ml

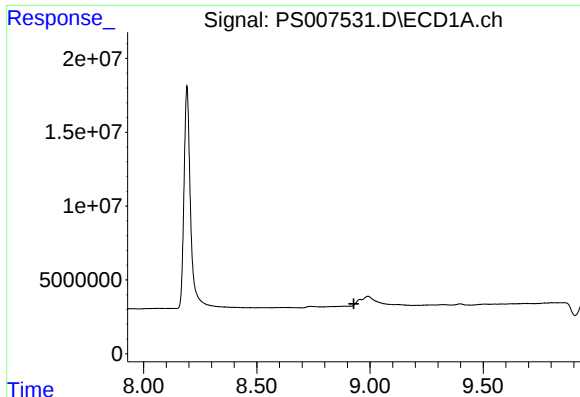

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 8.929 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

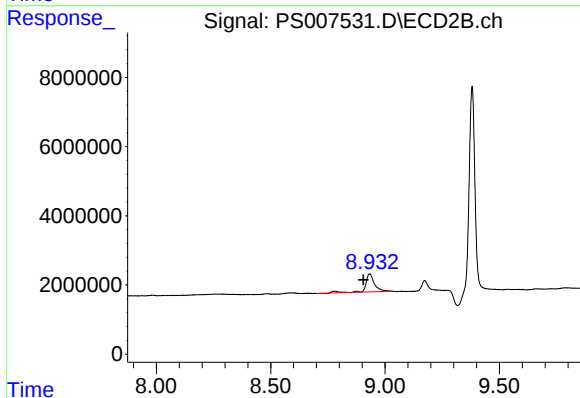


#15 Picloram

R.T.: 8.933 min
Delta R.T.: 0.028 min
Response: 13807028
Conc: 2.25 ng/ml

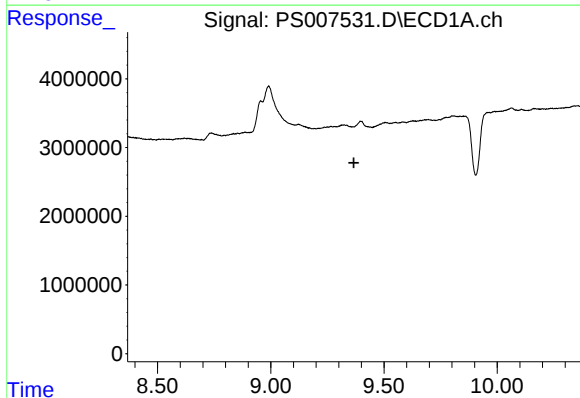

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 9.367 min
Response: 0
Conc: N.D.

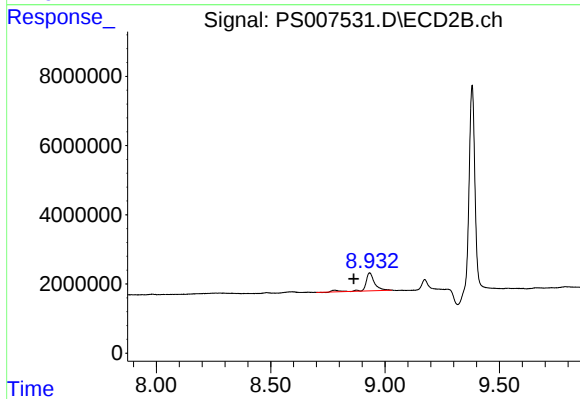

#16 DCPA

R.T.: 8.933 min
Delta R.T.: 0.069 min
Response: 13807028
Conc: 2.75 ng/ml