

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS103119\
 Data File : PS007533.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Oct 2019 18:11
 Operator : SM\AJ
 Sample : PB124384BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 01 03:20:52 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 14 13:54:23 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.453	5.172	788.2E6	416.5E6	575.865	592.207
Target Compounds							
1) T	Dalapon	2.012	1.716	217.5E6	119.8E6	129.964	131.650
2) T	3,5-DICHL...	0.000	4.506	0	57853682	N.D.	67.238
3) T	4-Nitroph...	5.263	0.000	28719672	0	47.828	N.D. #
5) T	DICAMBA	5.548	0.000	58162381	0	11.837	N.D. #
7) T	MCPA	5.925	5.542	23773041	13257325	4.609	4.560
9) T	2,4-D	0.000	6.076	0	9382331	N.D.	11.760
10) T	Pentachlo...	0.000	6.460	0	11286989	N.D.	1.174
11) T	2,4,5-TP ...	0.000	6.768	0	6090343	N.D.	1.601
12) T	2,4,5-T	0.000	7.220	0	27594353	N.D.	7.876
14) T	DINOSEB	0.000	7.964	0	23184110	N.D.	8.258
15) T	Picloram	8.965	8.912	174.1E6	110.0E6	15.772	17.919
16) T	DCPA	0.000	8.912	0	110.0E6	N.D.	21.940



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS103119\
Data File : PS007533.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Oct 2019 18:11
Operator : SM\AJ
Sample : PB124384BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 01 03:20:52 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
Quant Title : 8080.M
QLast Update : Mon Oct 14 13:54:23 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

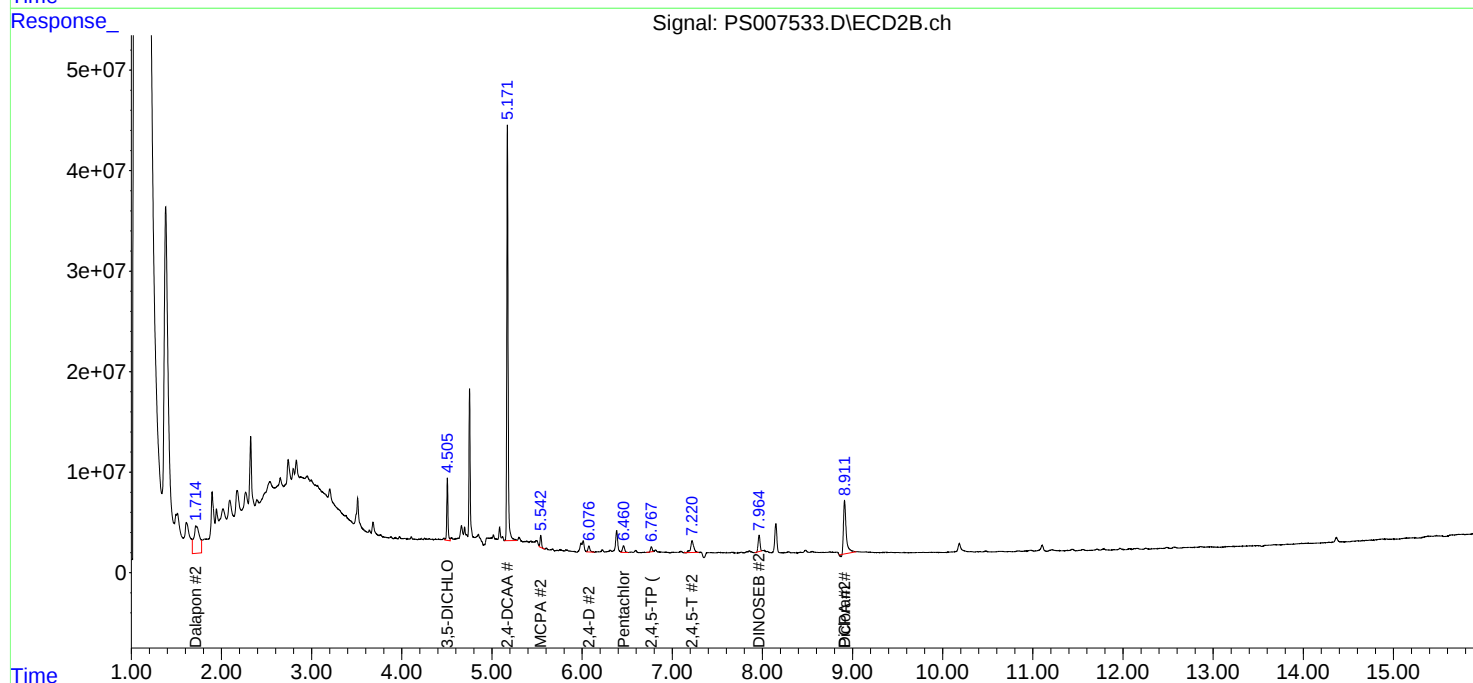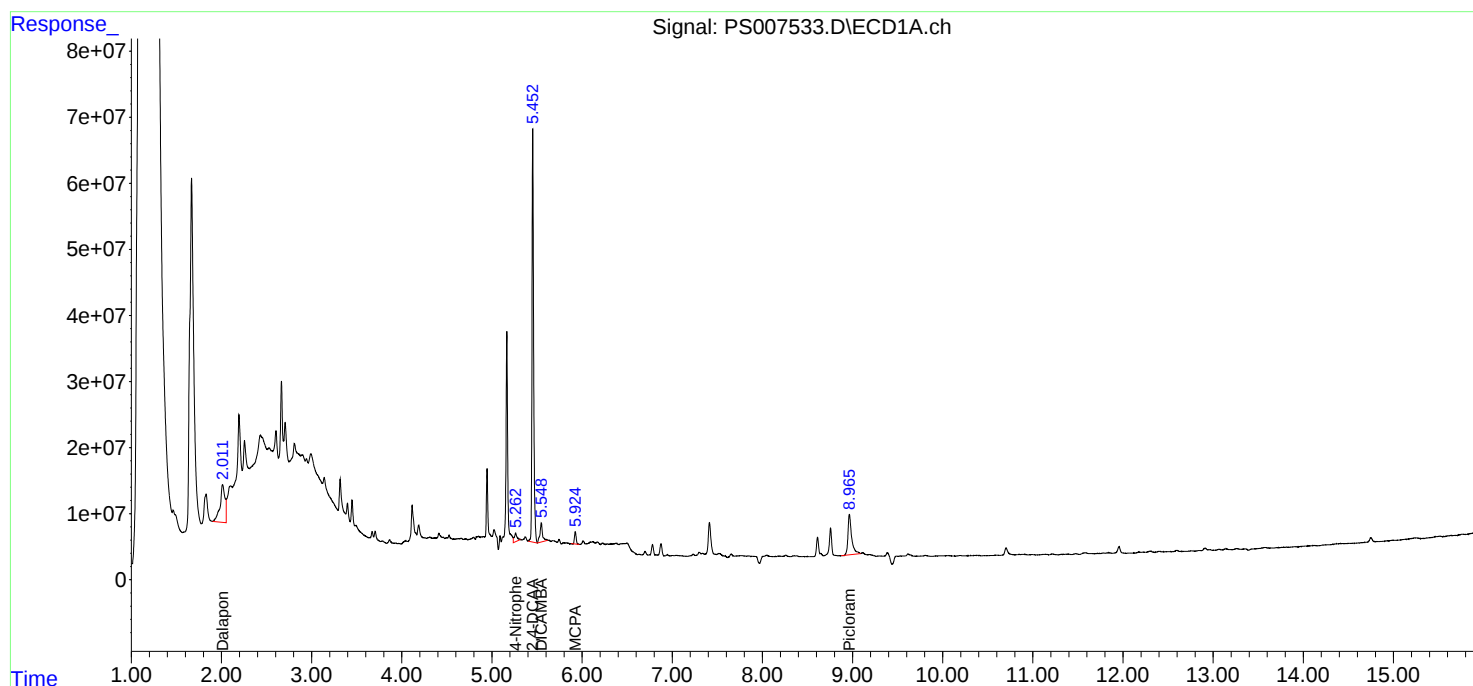


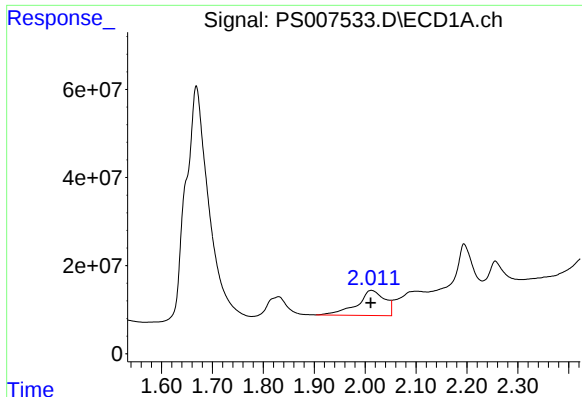

#1 Dalapon


R.T.: 2.012 min
Delta R.T.: 0.001 min
Response: 217466638
Conc: 129.96 ng/ml

Instrument :
ECD_S
ClientSampleId :

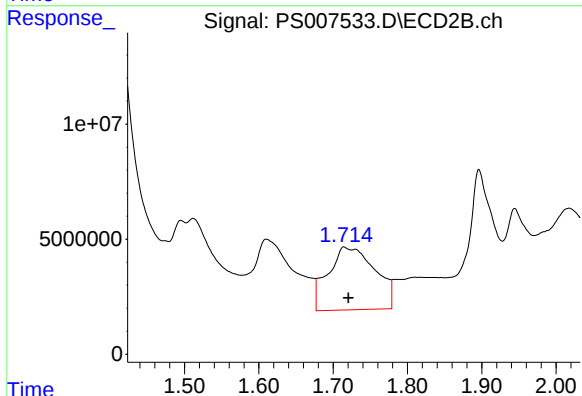


#1 Dalapon

R.T.: 1.716 min
Delta R.T.: -0.005 min
Response: 119802149
Conc: 131.65 ng/ml

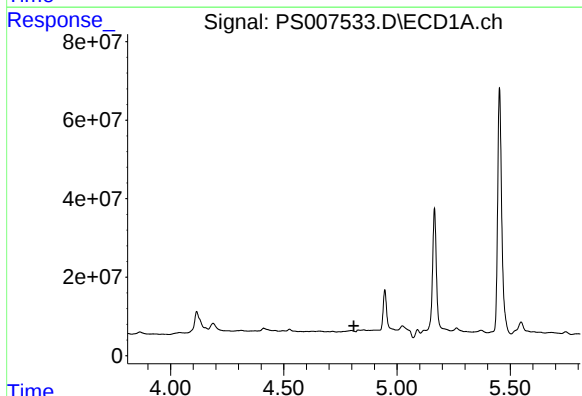


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.810 min
Response: 0
Conc: N.D.

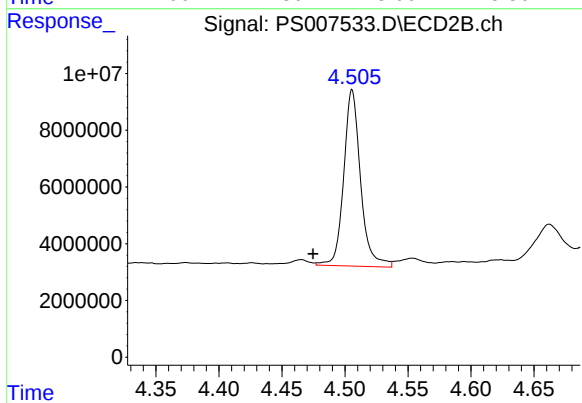

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.506 min
Delta R.T.: 0.031 min
Response: 57853682
Conc: 67.24 ng/ml

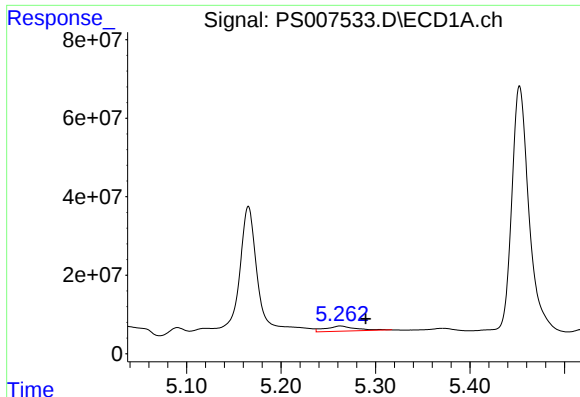

#3 4-Nitrophenol


R.T.: 5.263 min
Delta R.T.: -0.027 min
Response: 28719672
Conc: 47.83 ng/ml

Instrument :
ECD_S
ClientSampleId :

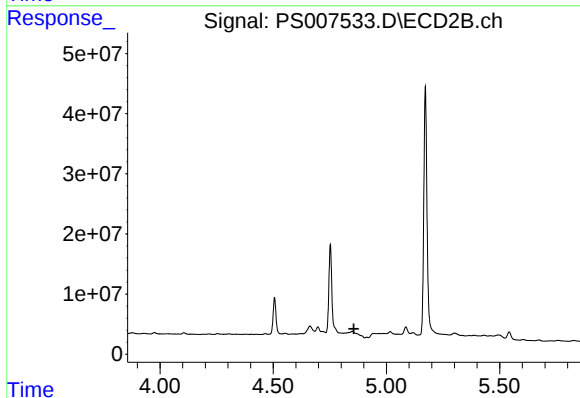


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 4.856 min
Response: 0
Conc: N.D.

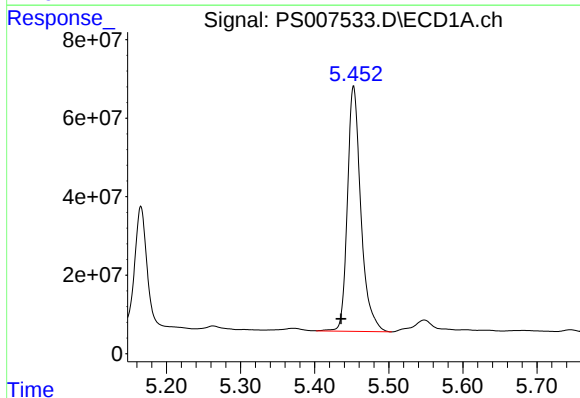


#4 2,4-DCAA

R.T.: 5.453 min
Delta R.T.: 0.017 min
Response: 788169014
Conc: 575.87 ng/ml

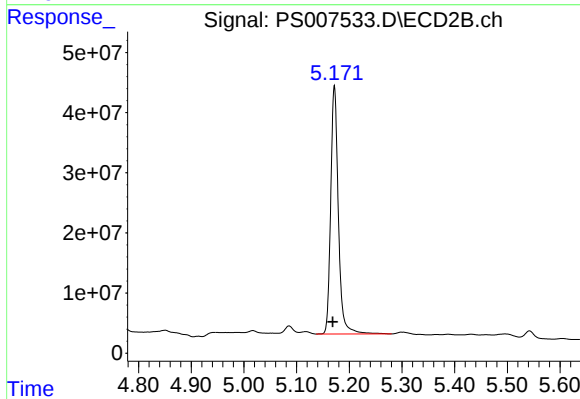

#4 2,4-DCAA


R.T.: 5.172 min
Delta R.T.: 0.003 min
Response: 416502934
Conc: 592.21 ng/ml

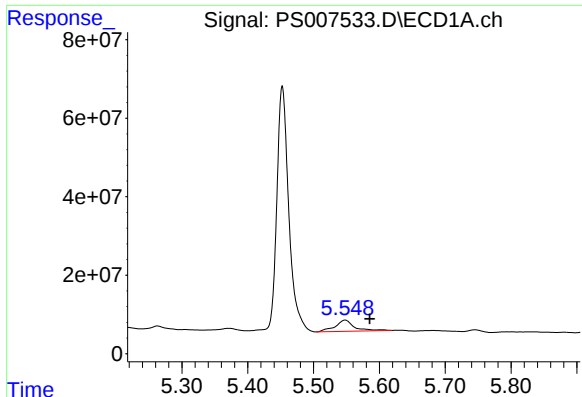

#5 DICAMBA


R.T.: 5.548 min
Delta R.T.: -0.037 min
Response: 58162381
Conc: 11.84 ng/ml

Instrument :
ECD_S
ClientSampleId :

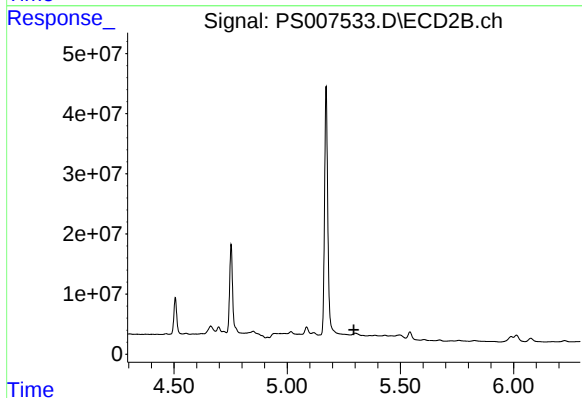


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 5.294 min
Response: 0
Conc: N.D.

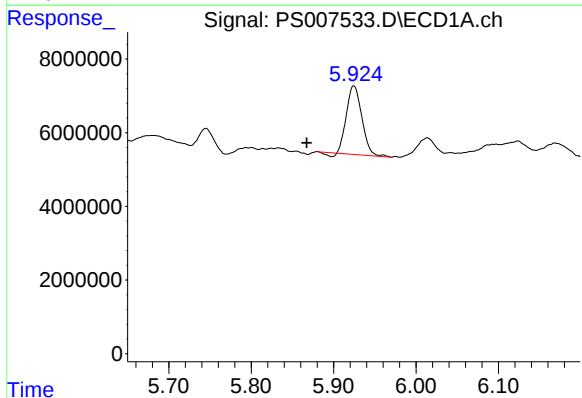


#7 MCPA

R.T.: 5.925 min
Delta R.T.: 0.057 min
Response: 23773041
Conc: 4.61 ug/ml

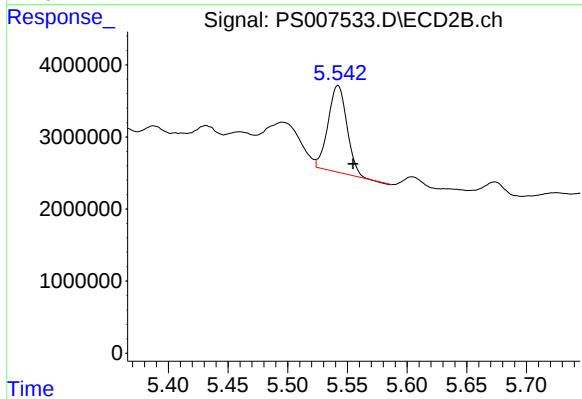

#7 MCPA


R.T.: 5.542 min
Delta R.T.: -0.013 min
Response: 13257325
Conc: 4.56 ug/ml

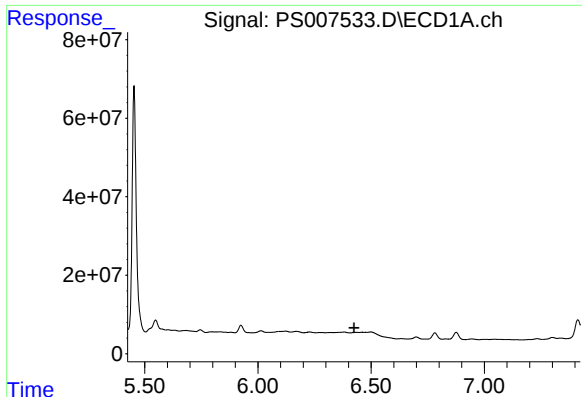

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.424 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

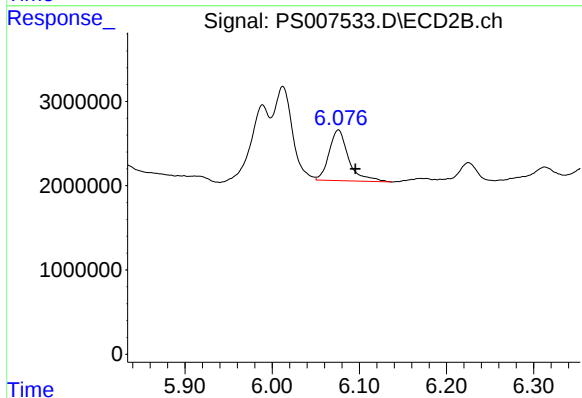


#9 2,4-D

R.T.: 6.076 min
Delta R.T.: -0.019 min
Response: 9382331
Conc: 11.76 ng/ml

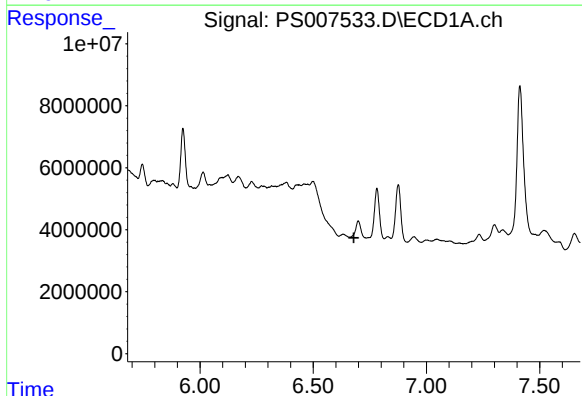


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T.: 6.680 min
Response: 0
Conc: N.D.

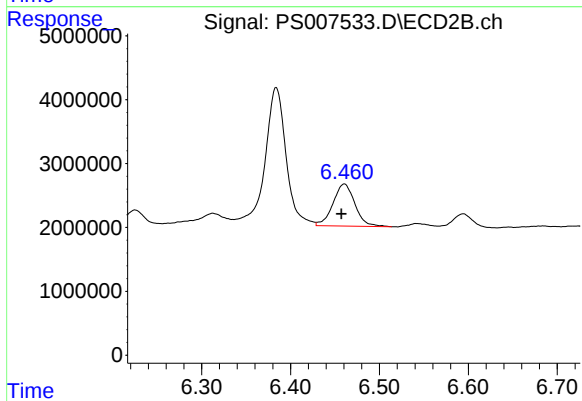

#10 Pentachlorophenol


R.T.: 6.460 min
Delta R.T.: 0.003 min
Response: 11286989
Conc: 1.17 ng/ml

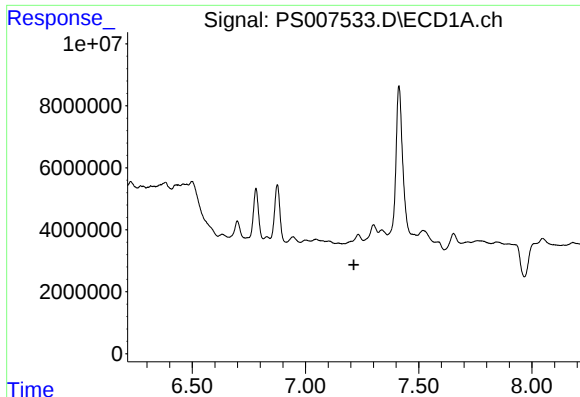

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.214 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

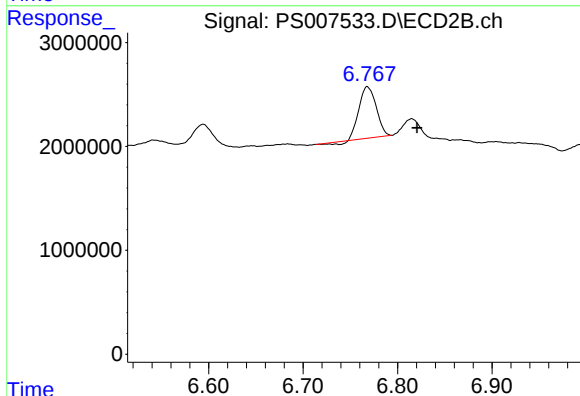


#11 2,4,5-TP (SILVEX)

R.T.: 6.768 min
Delta R.T.: -0.052 min
Response: 6090343
Conc: 1.60 ng/ml

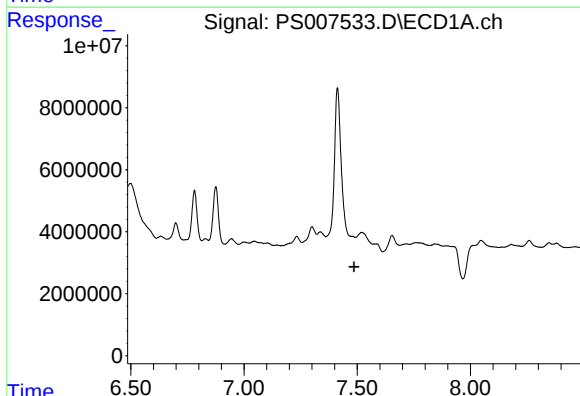


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 7.486 min
Response: 0
Conc: N.D.

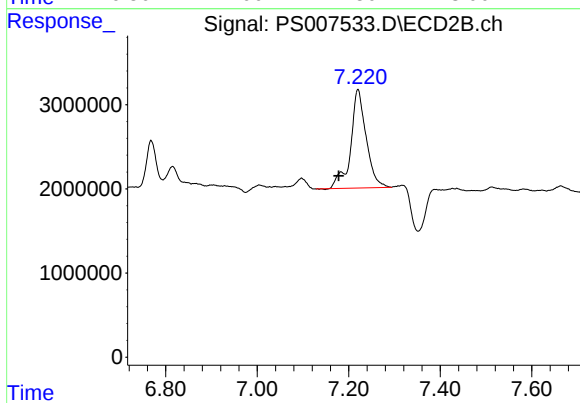

#12 2,4,5-T


R.T.: 7.220 min
Delta R.T.: 0.042 min
Response: 27594353
Conc: 7.88 ng/ml

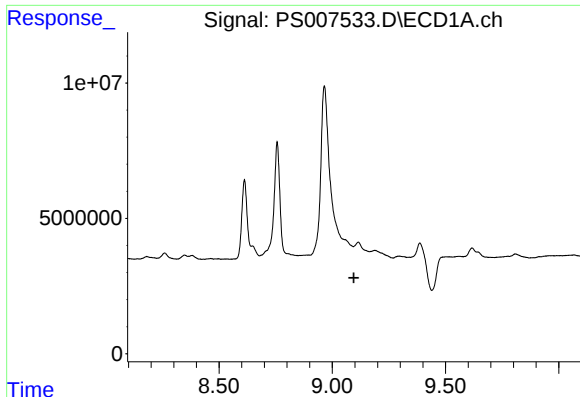

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 9.095 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

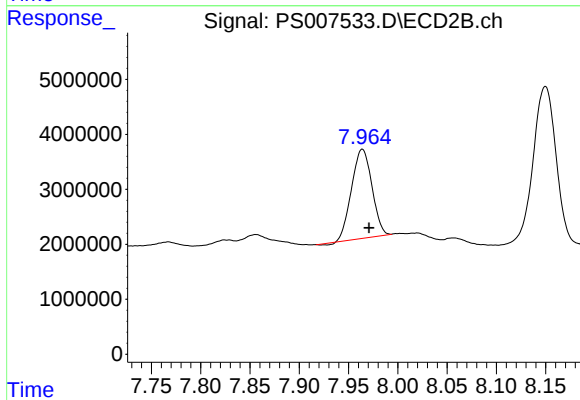


#14 DINOSEB

R.T.: 7.964 min
Delta R.T.: -0.007 min
Response: 23184110
Conc: 8.26 ng/ml

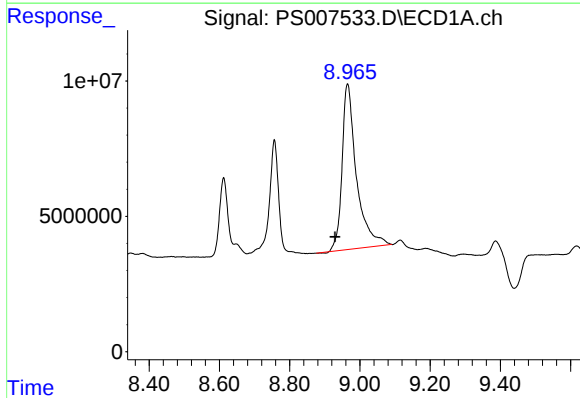


#15 Picloram

R.T.: 8.965 min
Delta R.T.: 0.036 min
Response: 174080071
Conc: 15.77 ng/ml

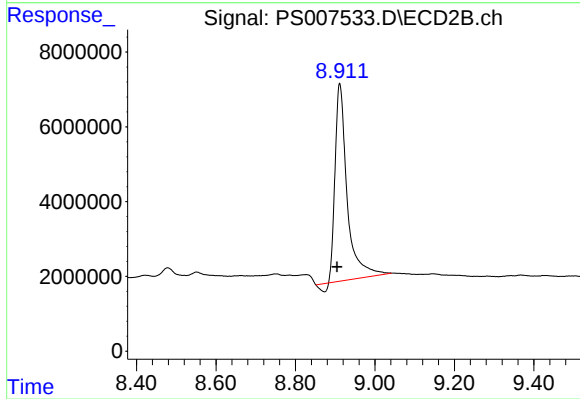

#15 Picloram


R.T.: 8.912 min
Delta R.T.: 0.007 min
Response: 110023742
Conc: 17.92 ng/ml

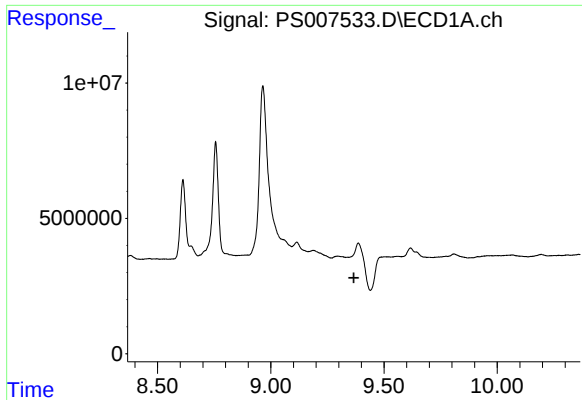

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 9.367 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

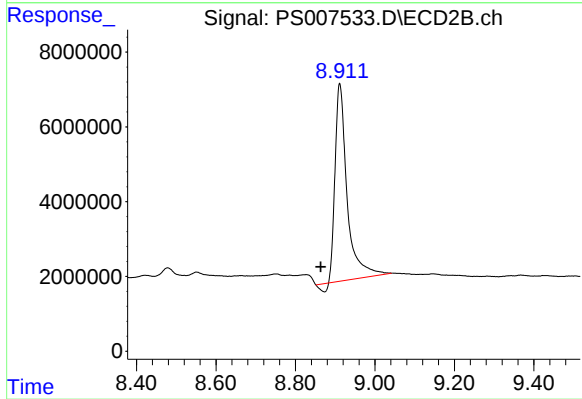

#16 DCPA

R.T.: 8.912 min
Delta R.T.: 0.048 min
Response: 110023742
Conc: 21.94 ng/ml