

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS103119\
 Data File : PS007544.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Oct 2019 22:14
 Operator : SM\AJ
 Sample : K5541-15
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 01 03:24:49 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 14 13:54:23 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	0.000	5.169	0	10688278	N.D.	15.197
Target Compounds							
1) T	Dalapon	2.005	0.000	62518370	0	37.363	N.D. #
2) T	3,5-DICHL...	0.000	4.503	0	98675935	N.D.	114.682
3) T	4-Nitroph...	0.000	4.846	0	14885425	N.D.	37.695
5) T	DICAMBA	5.539	5.303	95705073	5602683	19.478	2.153 #
7) T	MCPA	5.914	5.539	35120783	29823946	6.809	10.259 #
9) T	2,4-D	0.000	6.072	0	15241015	N.D.	19.104
10) T	Pentachlo...	0.000	6.456	0	9200736	N.D.	<MDL
13) T	2,4-DB	0.000	7.654	0	4787474	N.D.	10.214
15) T	Picloram	0.000	8.948	0	30397542	N.D.	4.951



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS103119\
Data File : PS007544.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Oct 2019 22:14
Operator : SM\AJ
Sample : K5541-15
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 01 03:24:49 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
Quant Title : 8080.M
QLast Update : Mon Oct 14 13:54:23 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

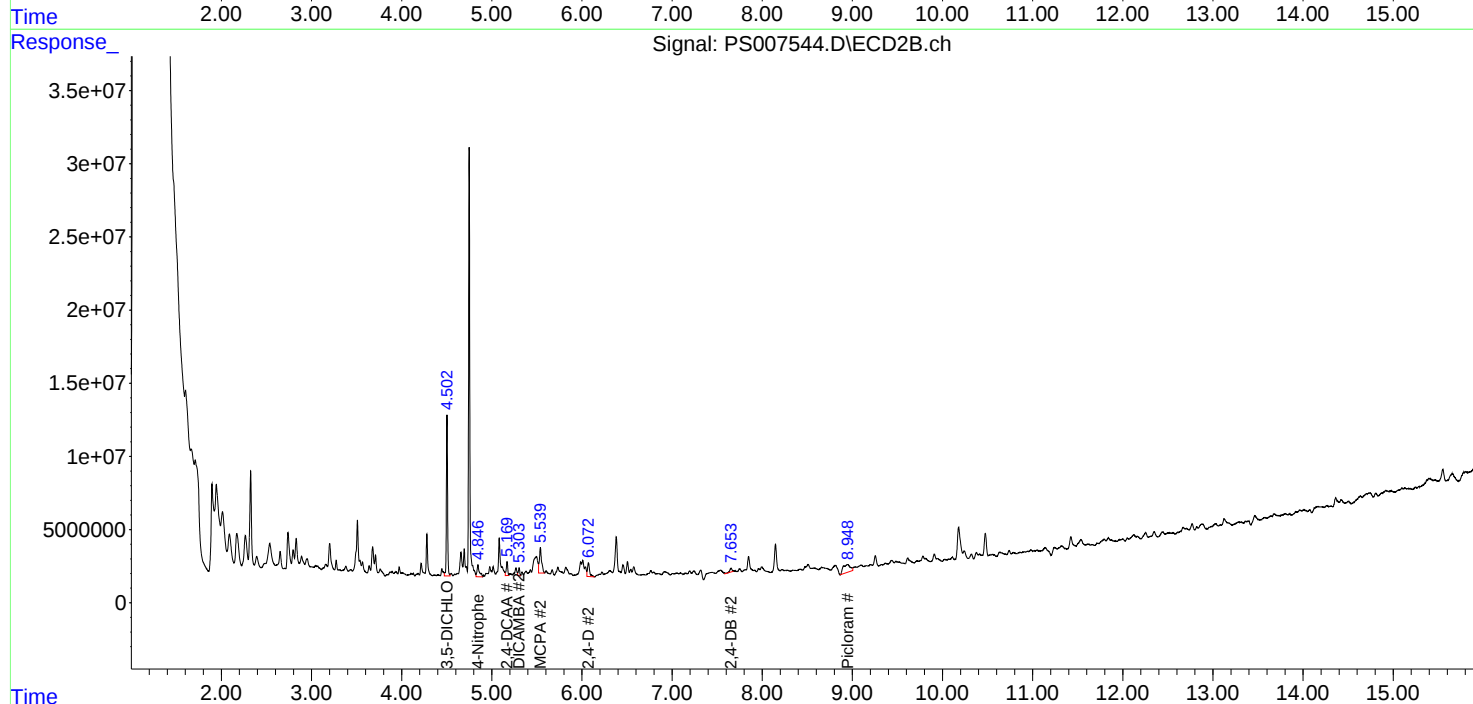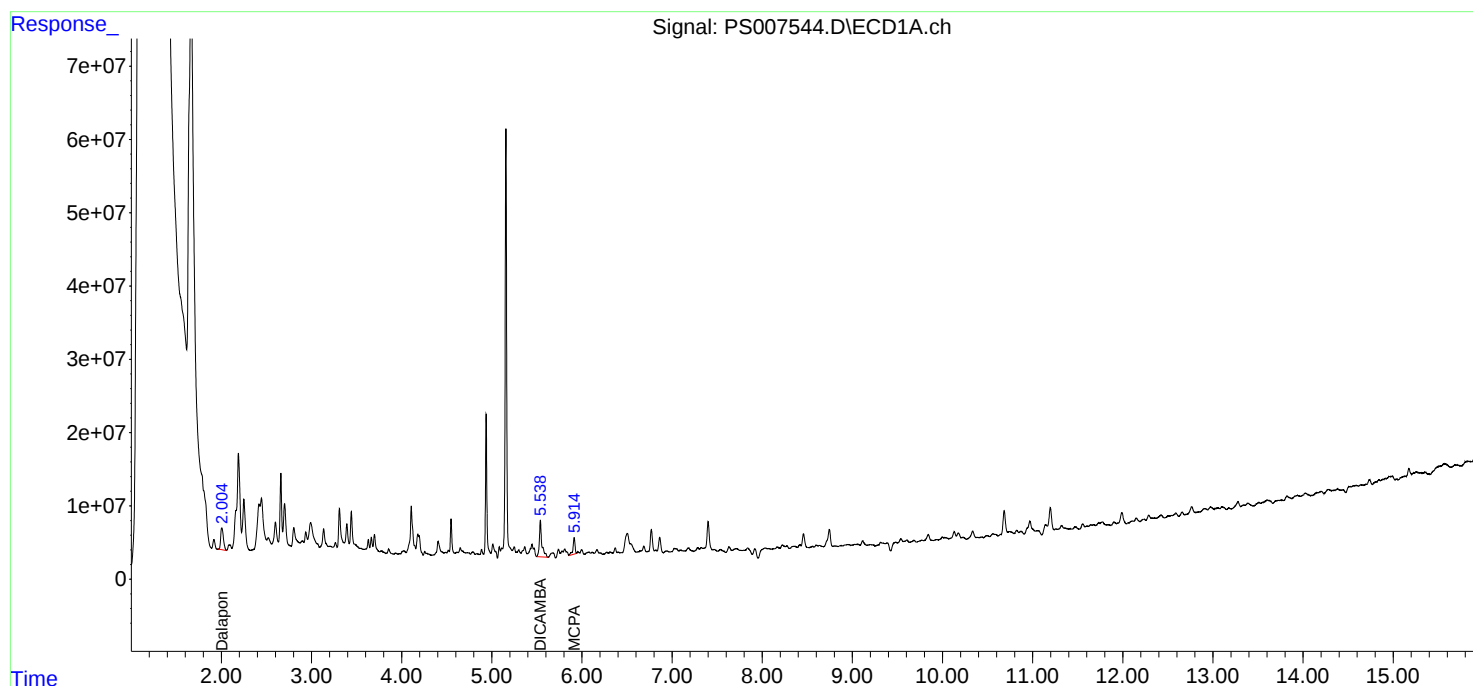


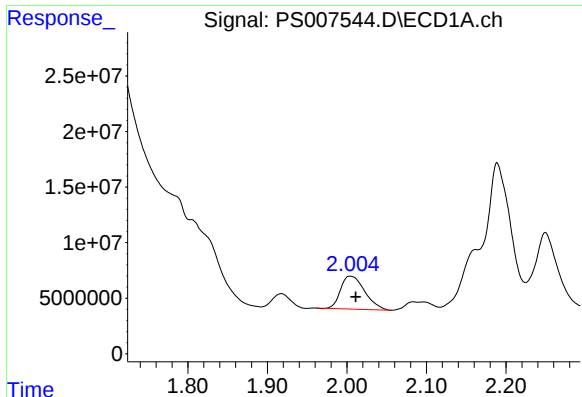

#1 Dalapon


R.T.: 2.005 min
Delta R.T.: -0.006 min
Response: 62518370
Conc: 37.36 ng/ml

Instrument :
ECD_S
ClientSampleId :

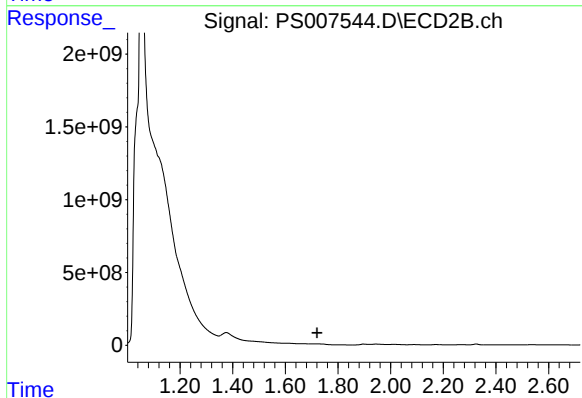


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 1.721 min
Response: 0
Conc: N.D.

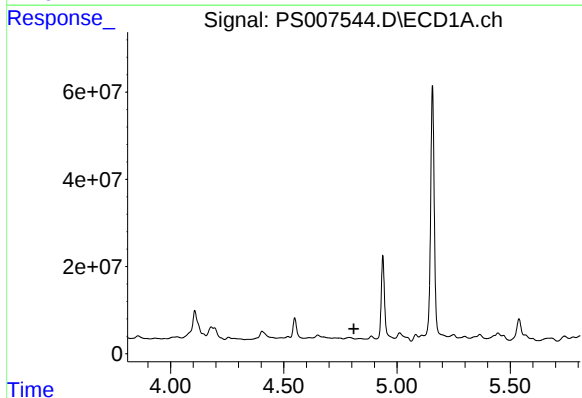


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.810 min
Response: 0
Conc: N.D.

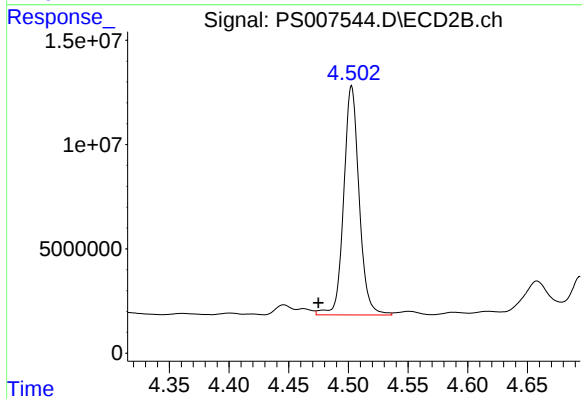

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.503 min
Delta R.T.: 0.028 min
Response: 98675935
Conc: 114.68 ng/ml

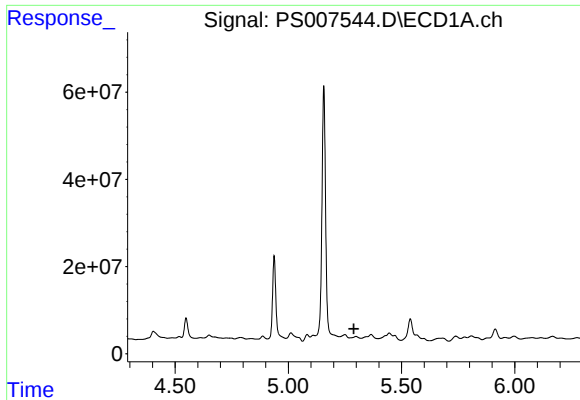

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 5.290 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

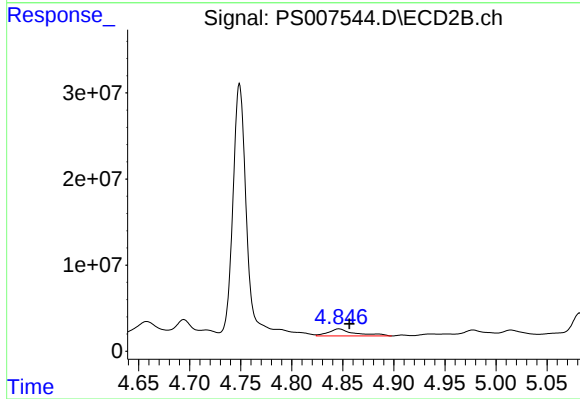


#3 4-Nitrophenol

R.T.: 4.846 min
Delta R.T.: -0.010 min
Response: 14885425
Conc: 37.69 ng/ml

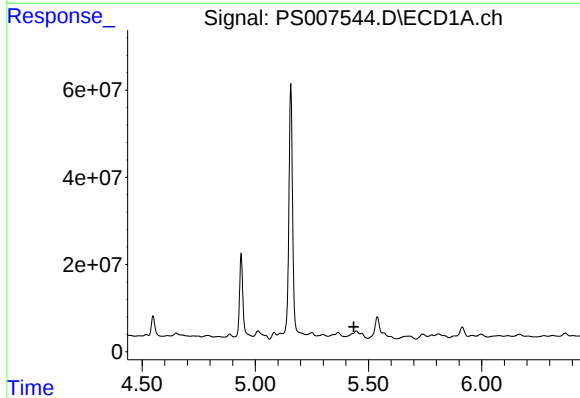


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 5.436 min
Response: 0
Conc: N.D.

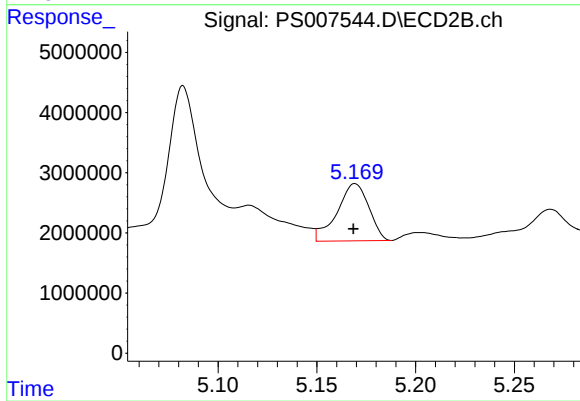

#4 2,4-DCAA


R.T.: 5.169 min
Delta R.T.: 0.000 min
Response: 10688278
Conc: 15.20 ng/ml

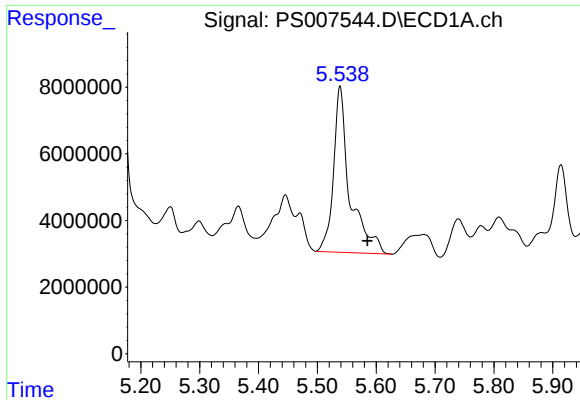

#5 DICAMBA


R.T.: 5.539 min
Delta R.T.: -0.047 min
Response: 95705073
Conc: 19.48 ng/ml

Instrument :
ECD_S
ClientSampleId :

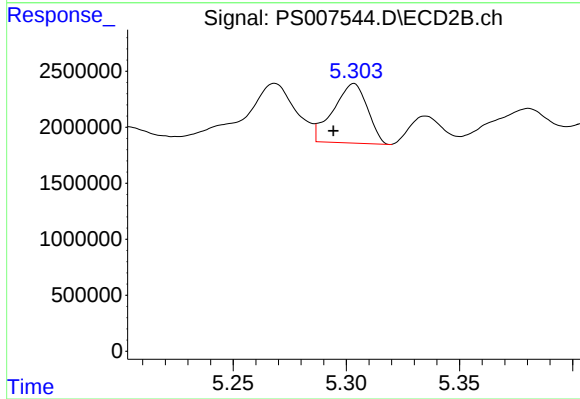


#5 DICAMBA

R.T.: 5.303 min
Delta R.T.: 0.009 min
Response: 5602683
Conc: 2.15 ng/ml

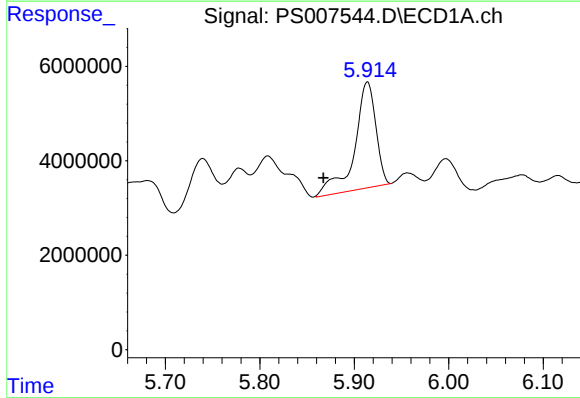


#7 MCPA

R.T.: 5.914 min
Delta R.T.: 0.046 min
Response: 35120783
Conc: 6.81 ug/ml

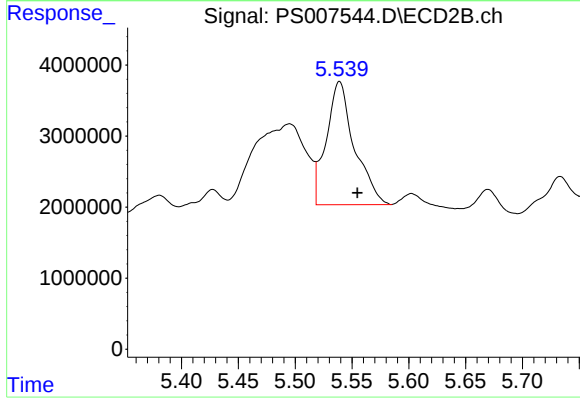

#7 MCPA


R.T.: 5.539 min
Delta R.T.: -0.016 min
Response: 29823946
Conc: 10.26 ug/ml

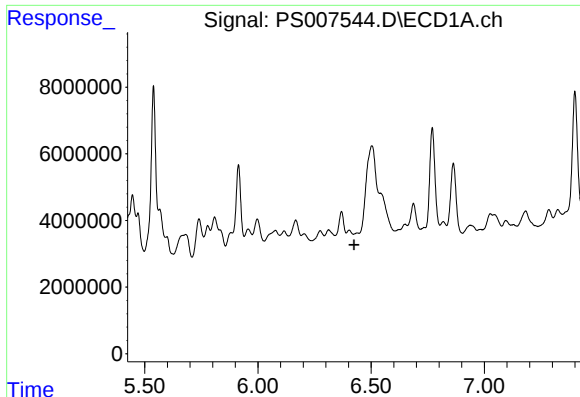

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.424 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

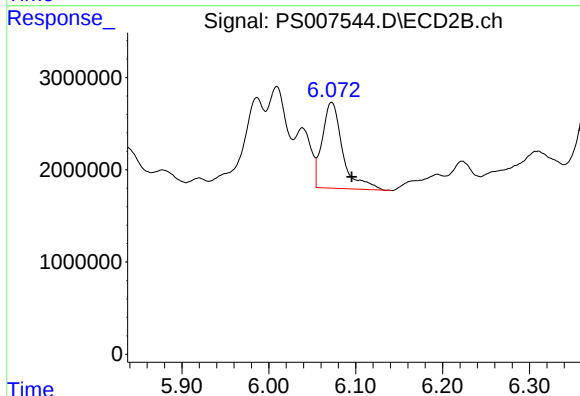


#9 2,4-D

R.T.: 6.072 min
Delta R.T.: -0.023 min
Response: 15241015
Conc: 19.10 ng/ml

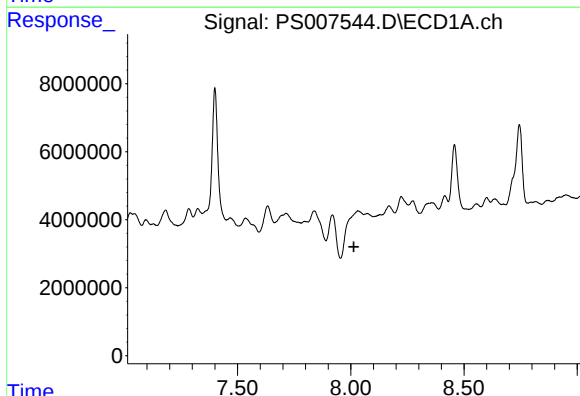


#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 8.014 min
Response: 0
Conc: N.D.

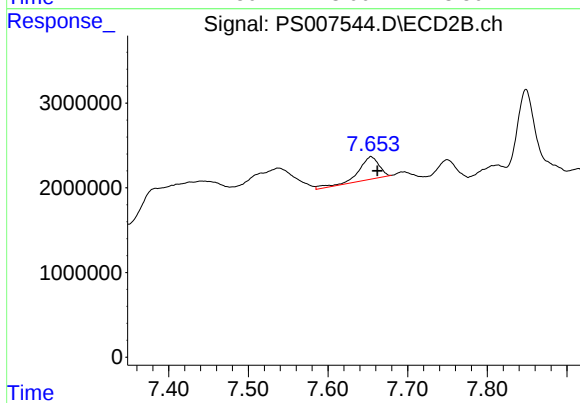

#13 2,4-DB


R.T.: 7.654 min
Delta R.T.: -0.008 min
Response: 4787474
Conc: 10.21 ng/ml

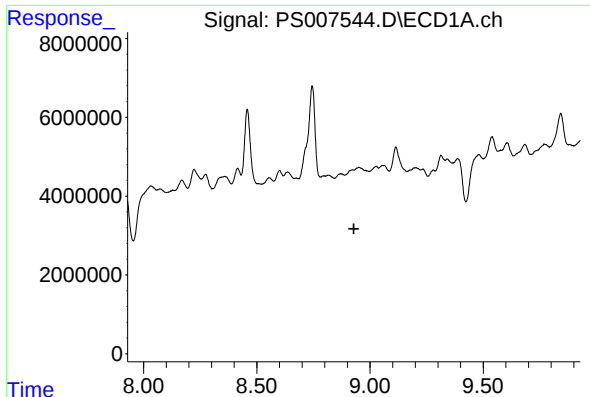

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 8.929 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

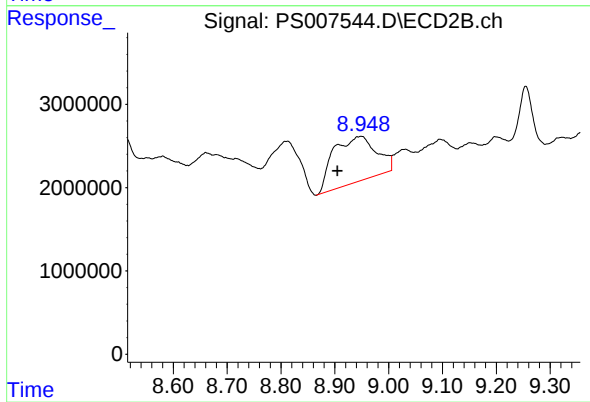

#15 Picloram

R.T.: 8.948 min
Delta R.T.: 0.043 min
Response: 30397542
Conc: 4.95 ng/ml