

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS103119\
 Data File : PS007545.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Oct 2019 22:36
 Operator : SM\AJ
 Sample : K5541-17
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 01 03:25:08 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 14 13:54:23 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	0.000	5.177	0	8553064	N.D.	12.161
Target Compounds							
1) T	Dalapon	2.014	0.000	95643931	0	57.160	N.D. #
2) T	3,5-DICHL...	0.000	4.511	0	73747718	N.D.	85.710
3) T	4-Nitroph...	0.000	4.854	0	14682251	N.D.	37.180
5) T	DICAMBA	5.547	5.278	91589672	3814389	18.641	1.466 #
7) T	MCPA	5.923	5.547	37930522	31130861	7.354	10.708 #
8) T	DICHLORPROP	0.000	5.830	0	9105600	N.D.	13.982
9) T	2,4-D	0.000	6.080	0	16954488	N.D.	21.252
10) T	Pentachlo...	0.000	6.466	0	7347649	N.D.	<MDL
13) T	2,4-DB	0.000	7.662	0	19923601	N.D.	42.509
15) T	Picloram	0.000	8.956	0	28990575	N.D.	4.721
16) T	DCPA	0.000	8.816	0	20780085	N.D.	4.144



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS103119\
Data File : PS007545.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Oct 2019 22:36
Operator : SM\AJ
Sample : K5541-17
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 01 03:25:08 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
Quant Title : 8080.M
QLast Update : Mon Oct 14 13:54:23 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

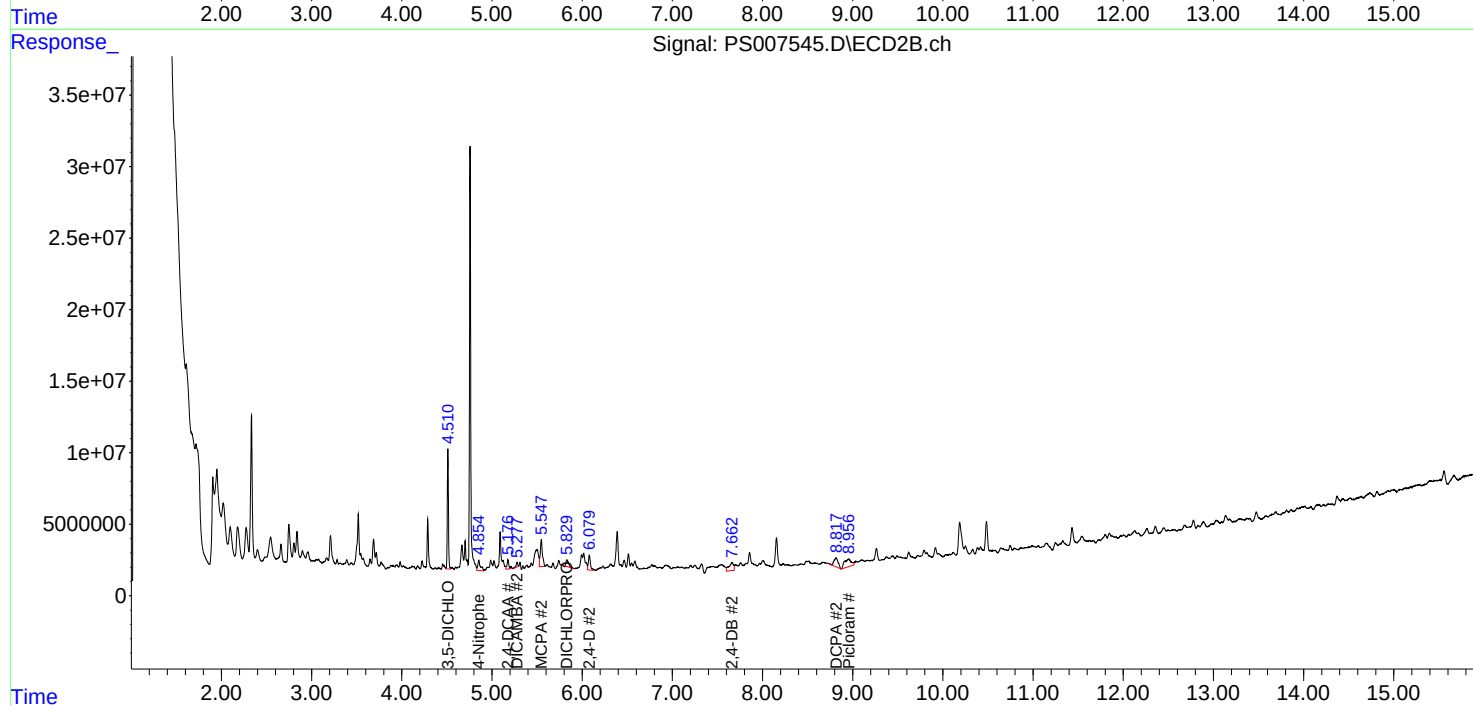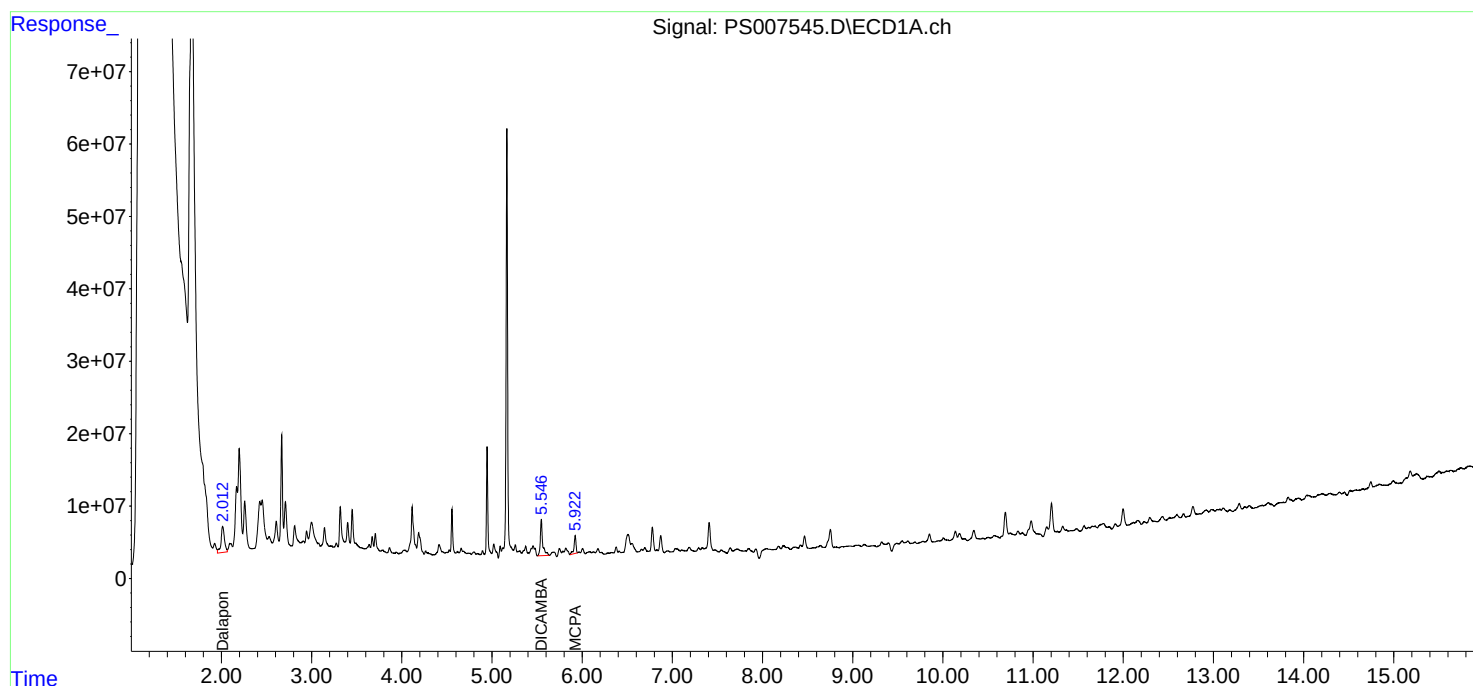


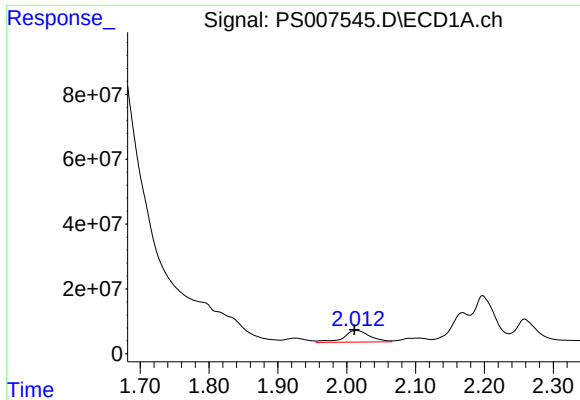

#1 Dalapon


R.T.: 2.014 min
Delta R.T.: 0.003 min
Response: 95643931
Conc: 57.16 ng/ml

Instrument :
ECD_S
ClientSampleId :

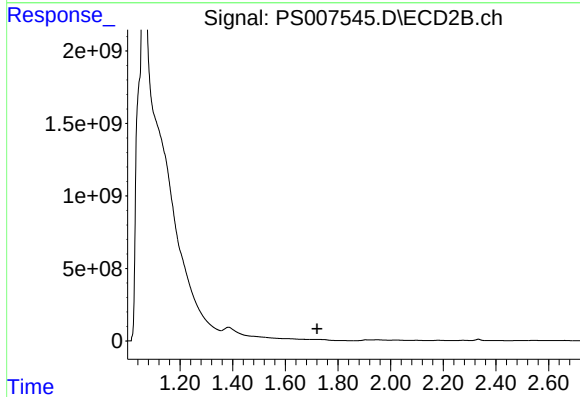


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 1.721 min
Response: 0
Conc: N.D.

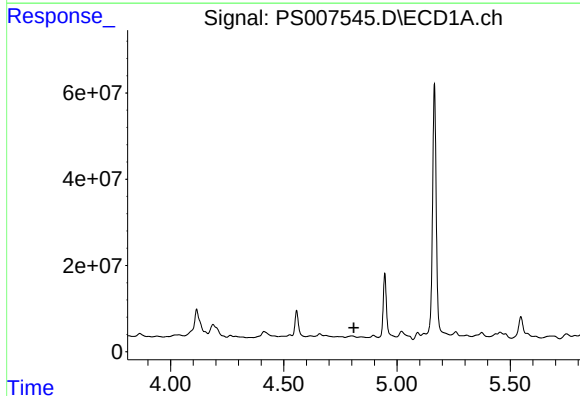


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.810 min
Response: 0
Conc: N.D.

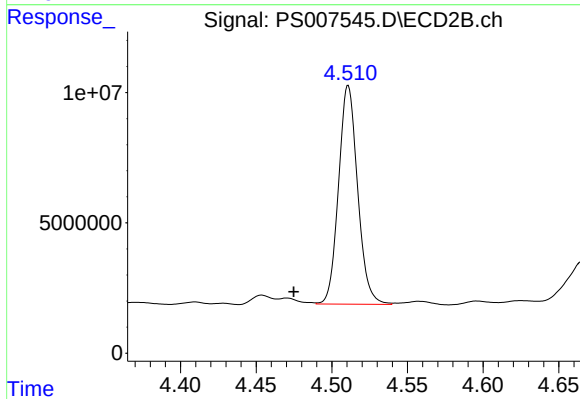

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.511 min
Delta R.T.: 0.036 min
Response: 73747718
Conc: 85.71 ng/ml

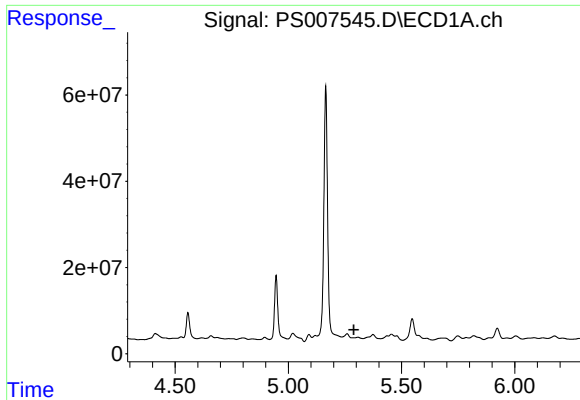

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 5.290 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

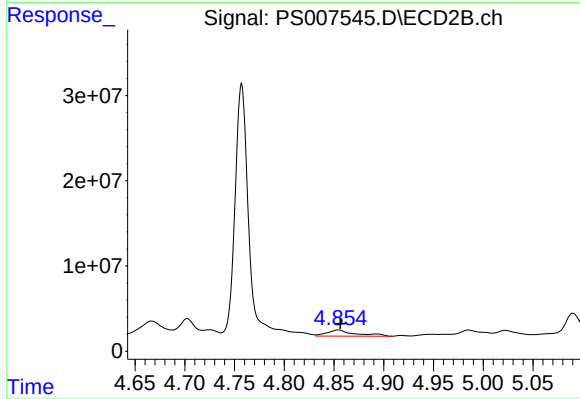


#3 4-Nitrophenol

R.T.: 4.854 min
Delta R.T.: -0.002 min
Response: 14682251
Conc: 37.18 ng/ml

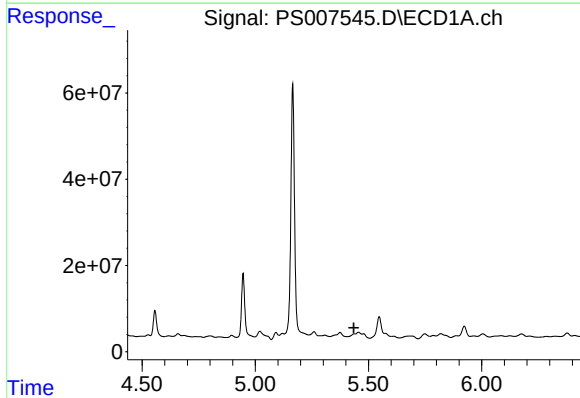


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 5.436 min
Response: 0
Conc: N.D.

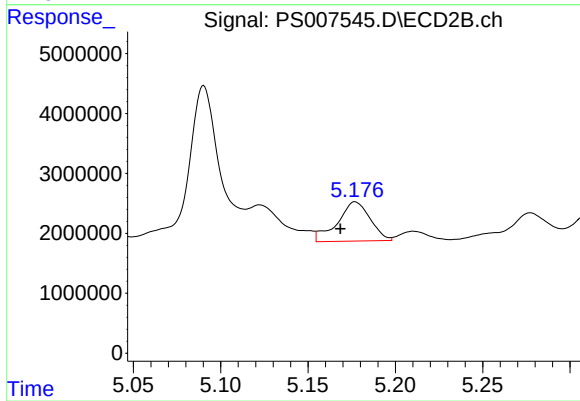

#4 2,4-DCAA


R.T.: 5.177 min
Delta R.T.: 0.009 min
Response: 8553064
Conc: 12.16 ng/ml

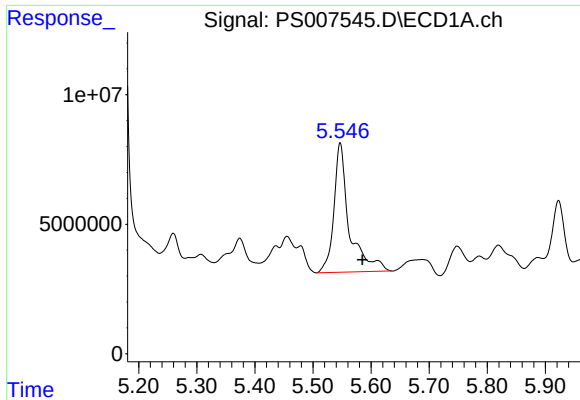

#5 DICAMBA


R.T.: 5.547 min
Delta R.T.: -0.038 min
Response: 91589672
Conc: 18.64 ng/ml

Instrument :
ECD_S
ClientSampleId :

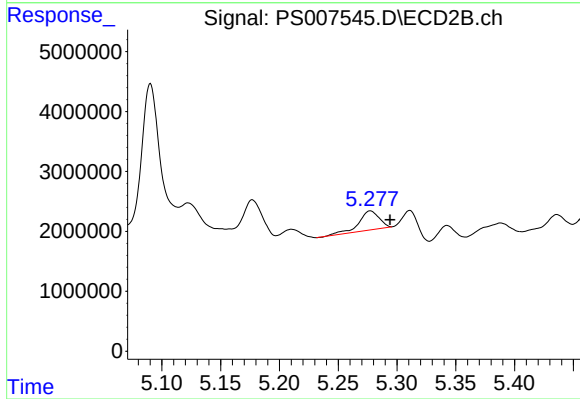


#5 DICAMBA

R.T.: 5.278 min
Delta R.T.: -0.017 min
Response: 3814389
Conc: 1.47 ng/ml

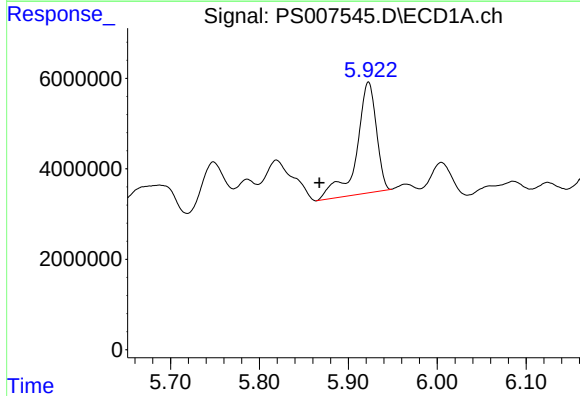


#7 MCPA

R.T.: 5.923 min
Delta R.T.: 0.055 min
Response: 37930522
Conc: 7.35 ug/ml

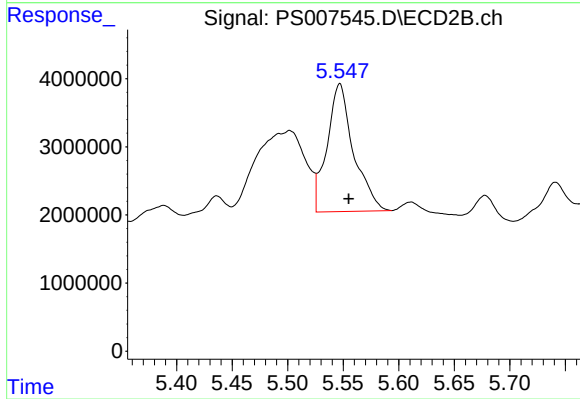

#7 MCPA


R.T.: 5.547 min
Delta R.T.: -0.008 min
Response: 31130861
Conc: 10.71 ug/ml

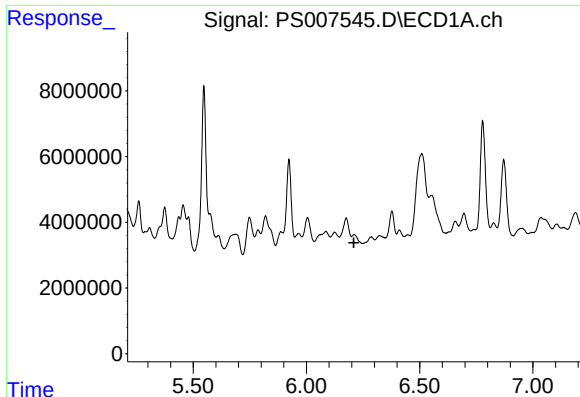

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 6.209 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

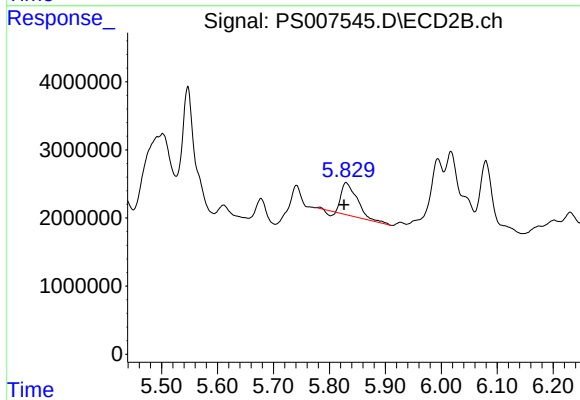


#8 DICHLORPROP

R.T.: 5.830 min
Delta R.T.: 0.004 min
Response: 9105600
Conc: 13.98 ng/ml

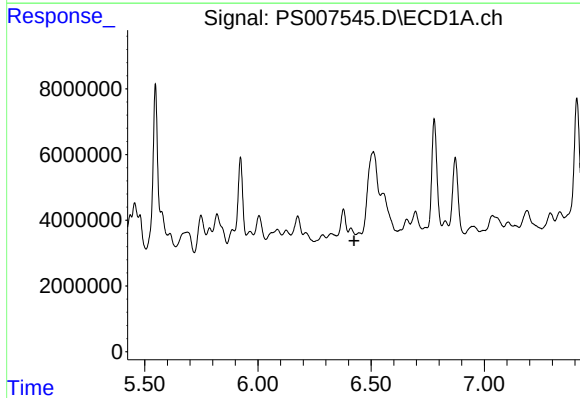


#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 6.424 min
Response: 0
Conc: N.D.

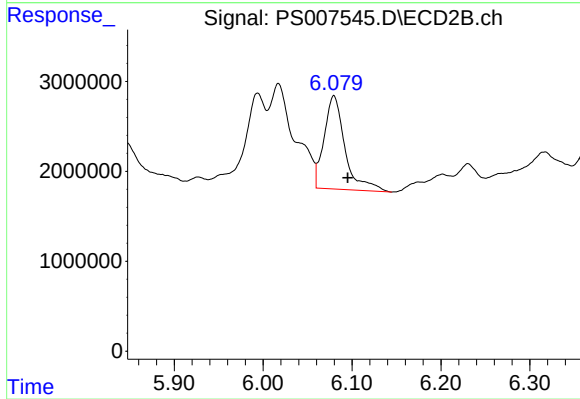

#9 2,4-D


R.T.: 6.080 min
Delta R.T.: -0.016 min
Response: 16954488
Conc: 21.25 ng/ml

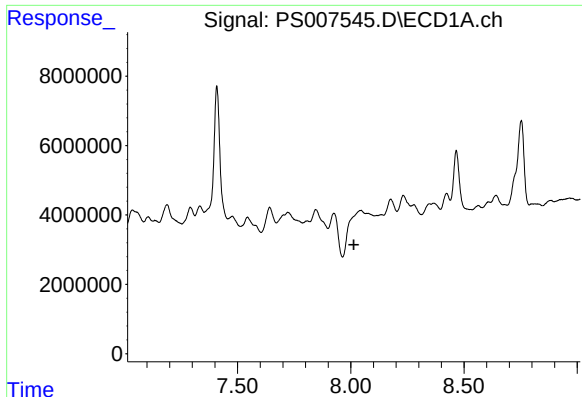

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 8.014 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

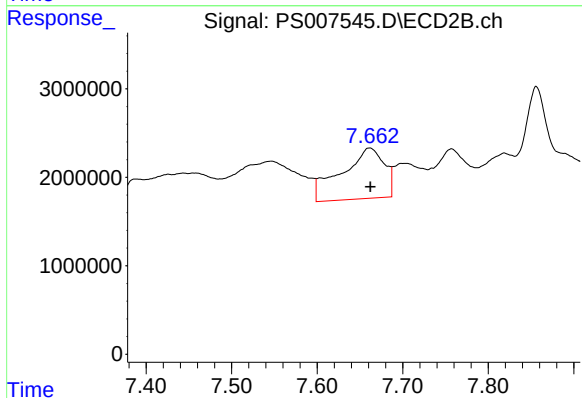


#13 2,4-DB

R.T.: 7.662 min
Delta R.T.: 0.000 min
Response: 19923601
Conc: 42.51 ng/ml

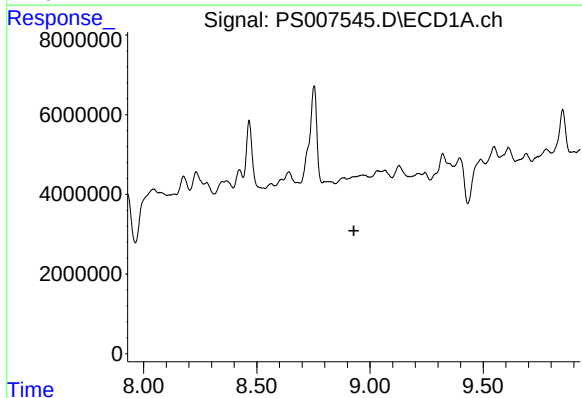


#15 Picloram

R.T.: 0.000 min
Exp R.T.: 8.929 min
Response: 0
Conc: N.D.

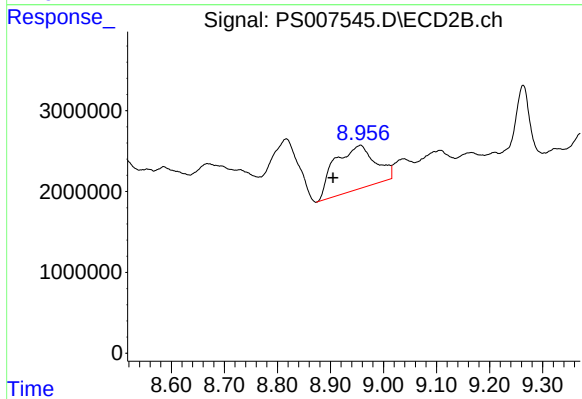

#15 Picloram


R.T.: 8.956 min
Delta R.T.: 0.051 min
Response: 28990575
Conc: 4.72 ng/ml

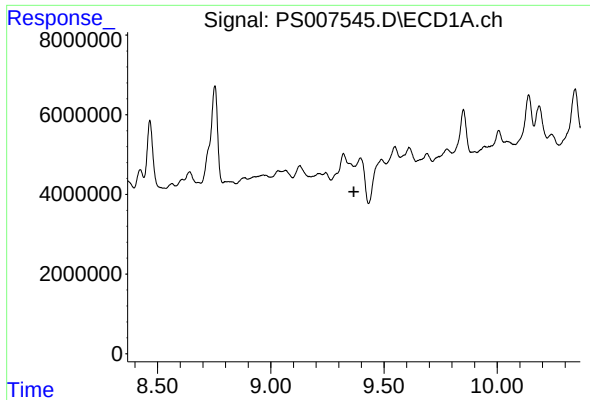

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 9.367 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

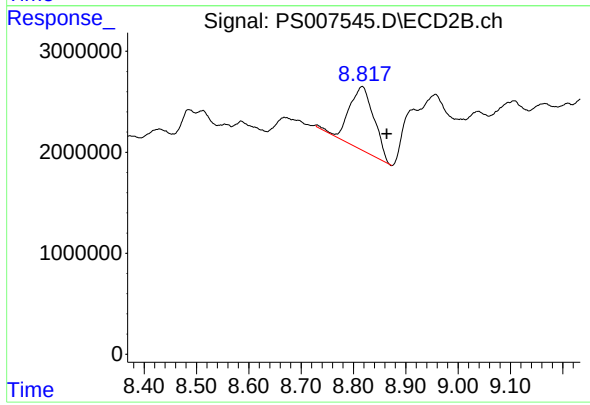

#16 DCPA

R.T.: 8.816 min
Delta R.T.: -0.047 min
Response: 20780085
Conc: 4.14 ng/ml