

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS103122\
 Data File : PS020945.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Oct 2022 09:46
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 31 14:14:08 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102822.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 31 10:07:57 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.351f	0.000	593570	0	<MDL	N.D. #
Target Compounds							
1) T	Dalapon	2.539	0.000	1304574	0	<MDL	N.D. #
2) T	3,5-DICHL...	5.744	0.000	376107	0	<MDL	N.D. #
3) T	4-Nitroph...	6.242	0.000	1292259	0	<MDL	N.D. #
5) T	DICAMBA	6.503f	0.000	2770997	0	<MDL	N.D. #
6) T	MCP	6.740	0.000	2373983	0	<MDL	N.D. #
8) T	DICHLORPROP	7.177	7.661	-22784	749943	N.D.	<MDL
10) T	Pentachlo...	7.575	0.000	448858	0	<MDL	N.D. #
11) T	2,4,5-TP ...	8.119	8.681f	2429224	2525312	<MDL	<MDL #
12) T	2,4,5-T	8.391	9.152f	3716405	3838845	<MDL	<MDL #
13) T	2,4-DB	8.868	0.000	1087434	0	<MDL	N.D. #
14) T	DINOSEB	9.942	0.000	452116	0	<MDL	N.D. #
15) T	Picloram	9.777	10.914	31201946	18815240	1.477	1.483
16) T	DCPA	10.237	10.914	2056874	18815240	<MDL	1.762 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS103122\
Data File : PS020945.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Oct 2022 09:46
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 31 14:14:08 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102822.M
Quant Title : 8080.M
QLast Update : Mon Oct 31 10:07:57 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

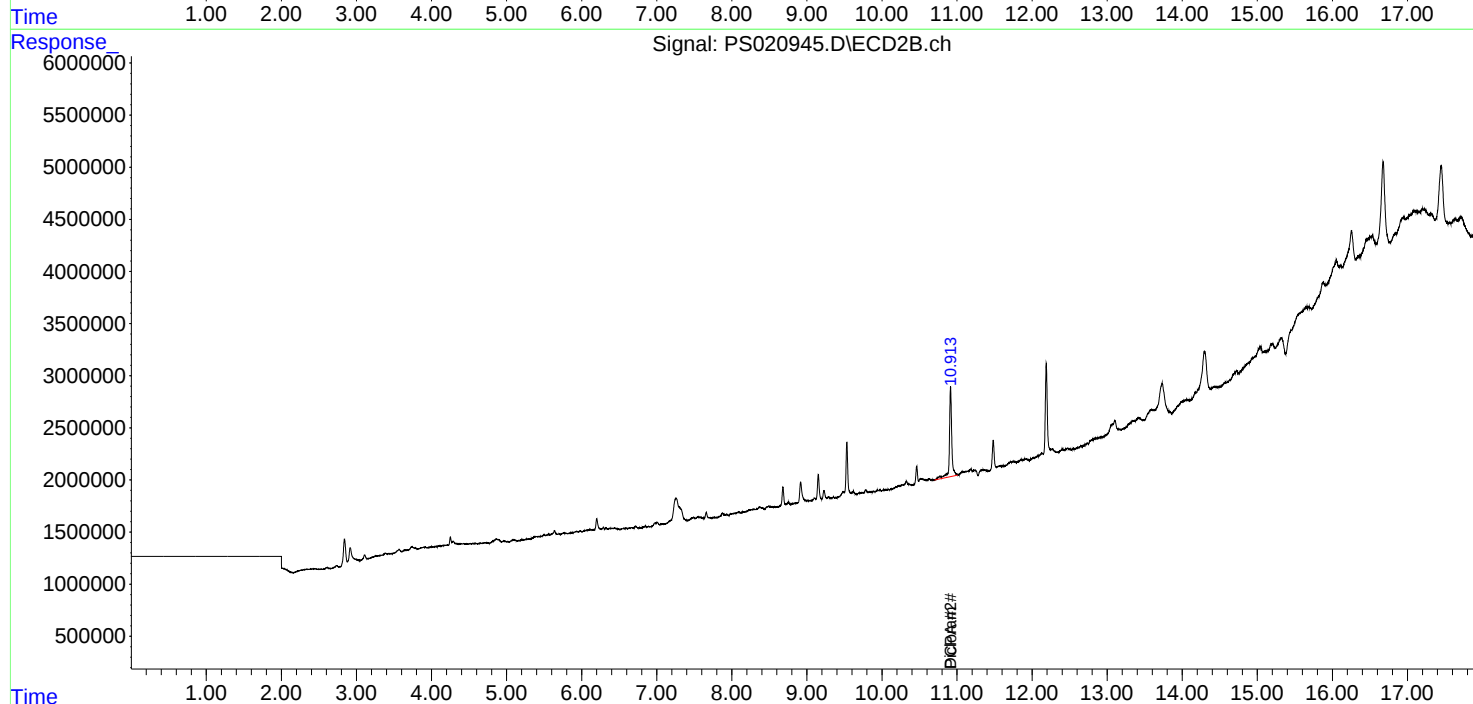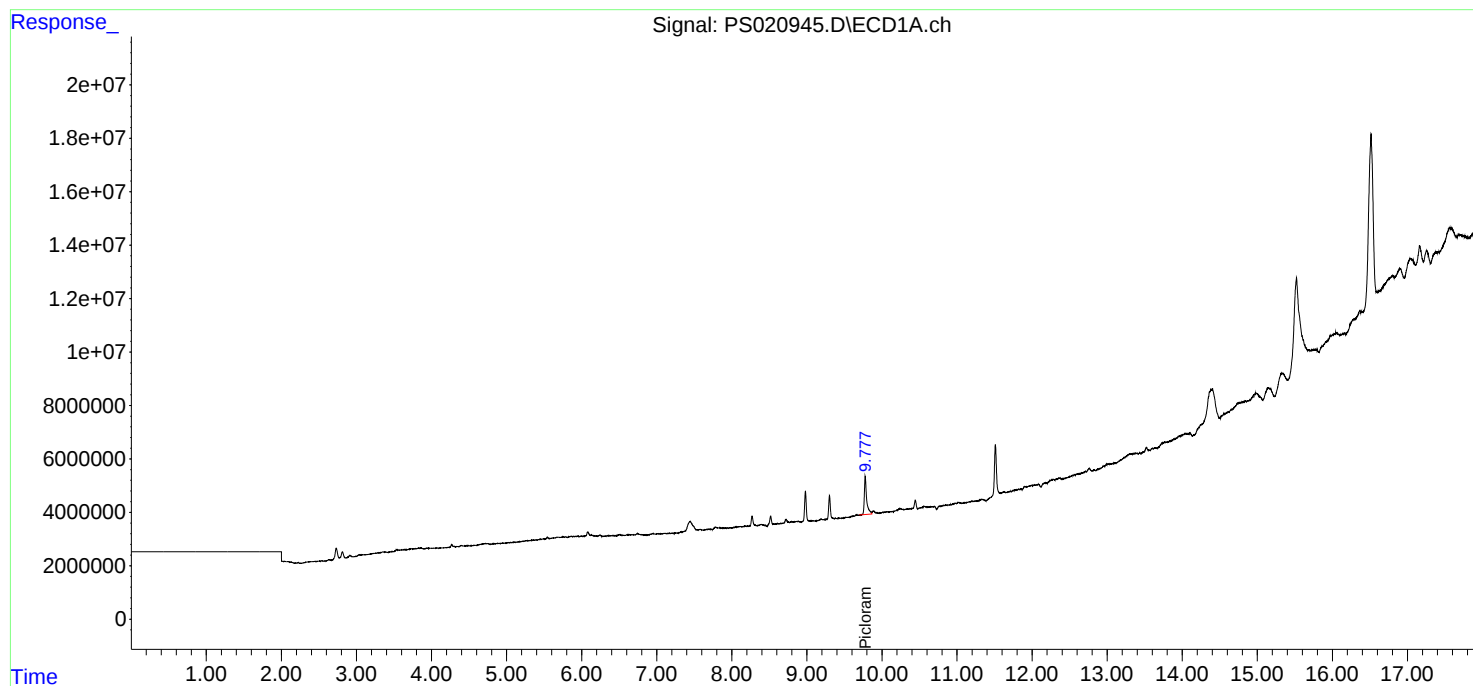


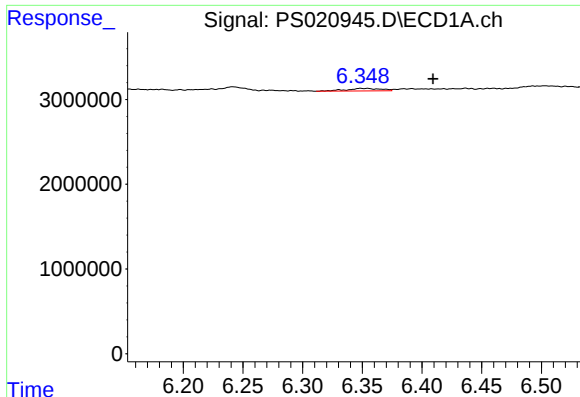

#4 2,4-DCAA


R.T.: 6.351 min
Delta R.T.: -0.058 min
Response: 593570
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

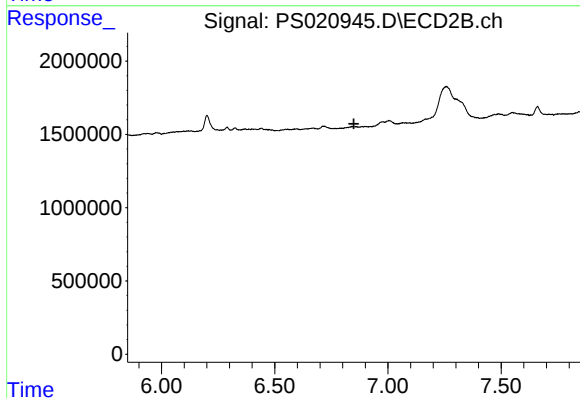


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 6.850 min
Response: 0
Conc: N.D.

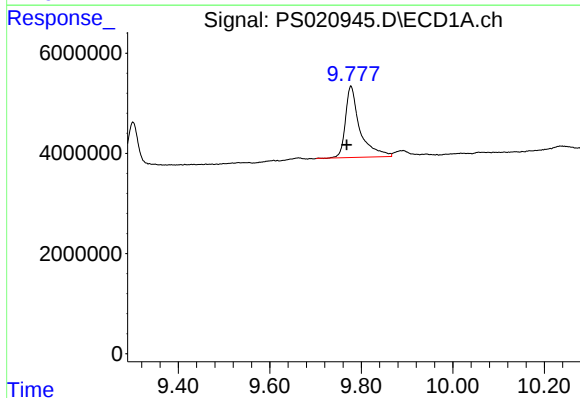


#15 Picloram

R.T.: 9.777 min
Delta R.T.: 0.009 min
Response: 31201946
Conc: 1.48 ng/ml

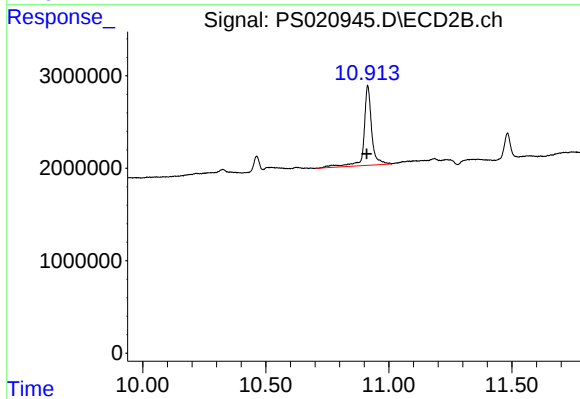

#15 Picloram


R.T.: 10.914 min
Delta R.T.: 0.003 min
Response: 18815240
Conc: 1.48 ng/ml

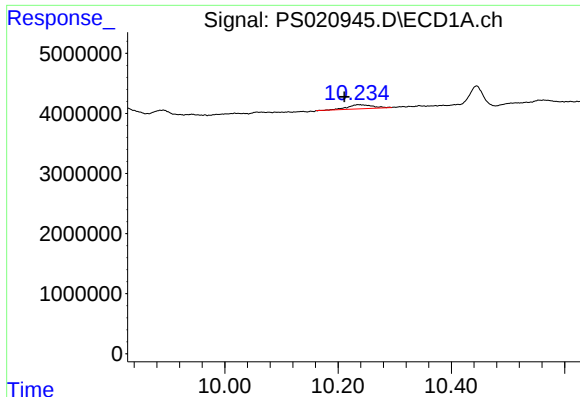

#16 DCPA

R.T.: 10.237 min
Delta R.T.: 0.025 min
Response: 2056874
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

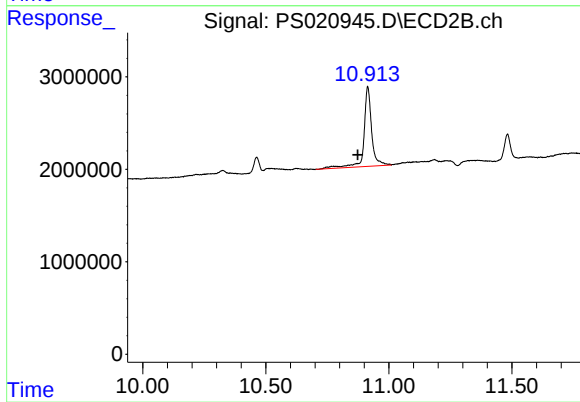

#16 DCPA

R.T.: 10.914 min
Delta R.T.: 0.040 min
Response: 18815240
Conc: 1.76 ng/ml