

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS103124\
 Data File : PS028121.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Oct 2024 18:29
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 01 02:23:26 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS103124.M
 Quant Title : 8080.M
 QLast Update : Thu Oct 31 13:10:03 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.063	7.615	1589.0E6	547.4E6	507.885	547.899
Target Compounds							
1) T	Dalapon	2.516	0.000	22950350	0	5.589	N.D. #
2) T	3,5-DICHL...	6.236	0.000	4486802	0	<MDL	N.D. #
3) T	4-Nitroph...	6.860	0.000	14077855	0	5.985	N.D. #
6) T	MCP	0.000	7.897	0	1499838	N.D.	<MDL
7) T	MCPA	0.000	8.141	0	12072161	N.D.	2.665
8) T	DICHLORPROP	7.949f	8.554f	790903	3748740	<MDL	3.428 #
9) T	2,4-D	8.153	0.000	33765024	0	8.314	N.D. #
10) T	Pentachlo...	8.397f	0.000	3683169	0	<MDL	N.D. #
11) T	2,4,5-TP ...	8.982	0.000	9291753	0	<MDL	N.D. #
13) T	2,4-DB	9.826	0.000	4032151	0	1.186	N.D. #
15) T	Picloram	10.831	12.179f	32570832	6735100	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS103124\
Data File : PS028121.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Oct 2024 18:29
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 01 02:23:26 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS103124.M
Quant Title : 8080.M
QLast Update : Thu Oct 31 13:10:03 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

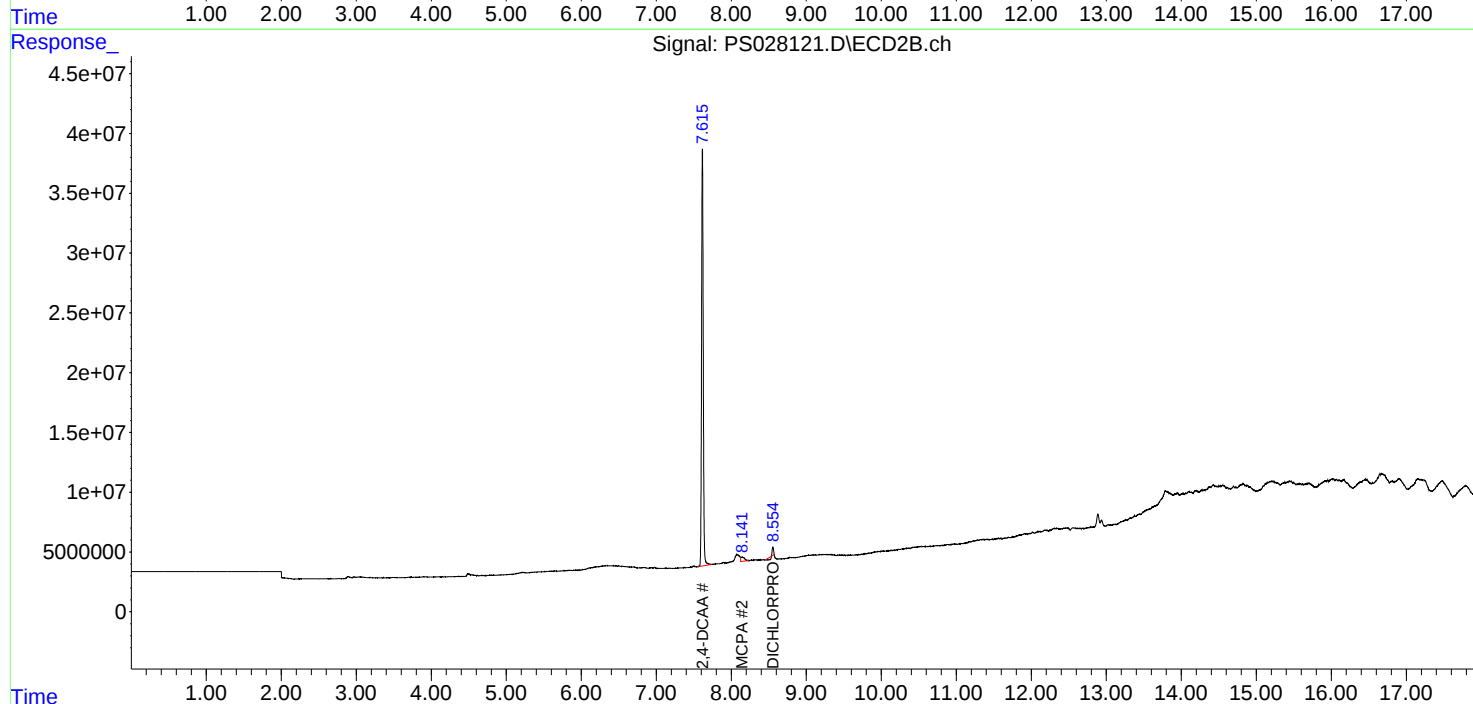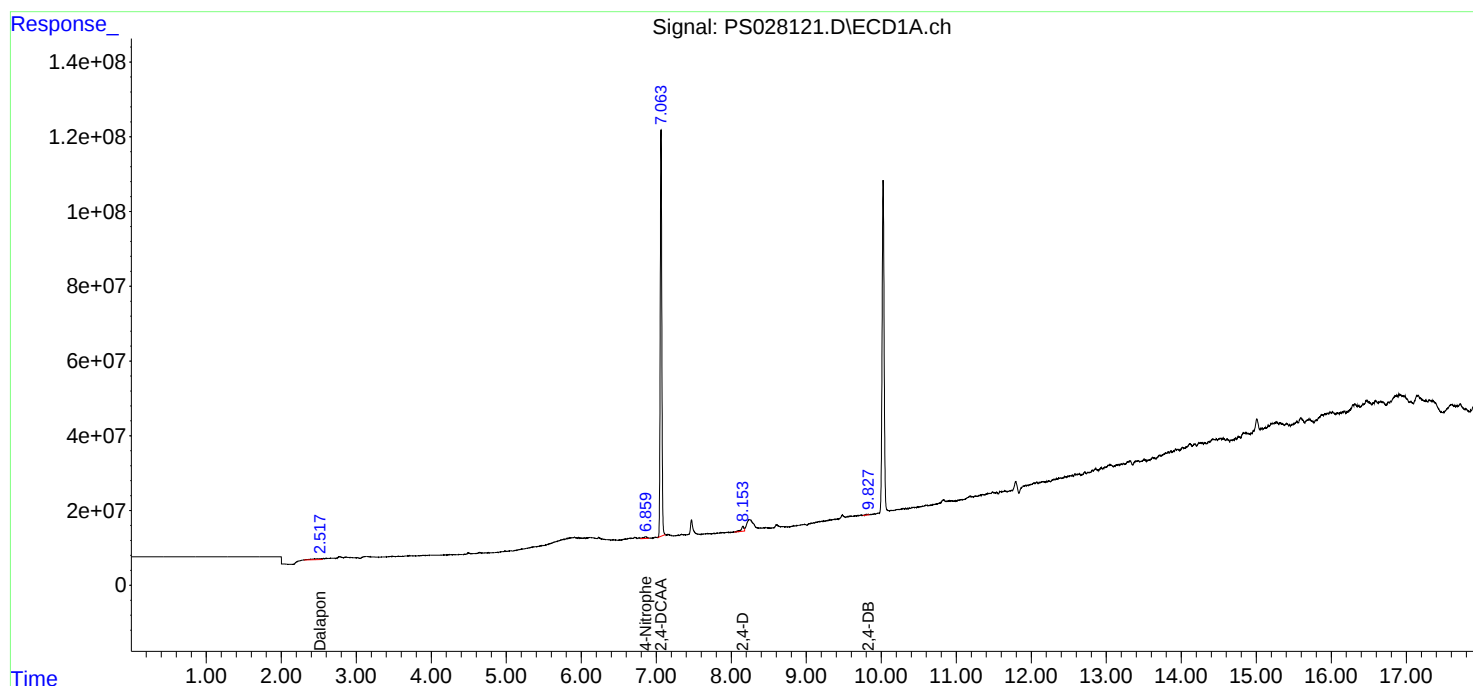


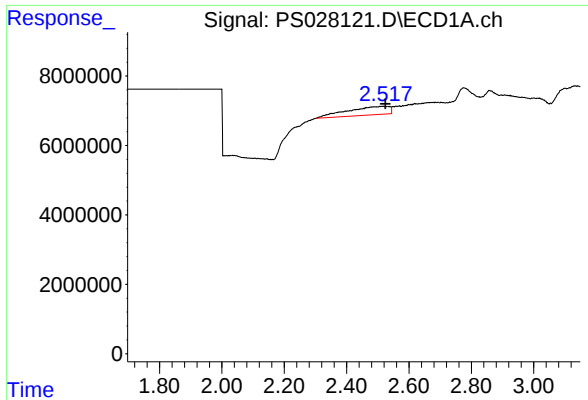

#1 Dalapon


R.T.: 2.516 min
Delta R.T.: -0.008 min
Response: 22950350
Conc: 5.59 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

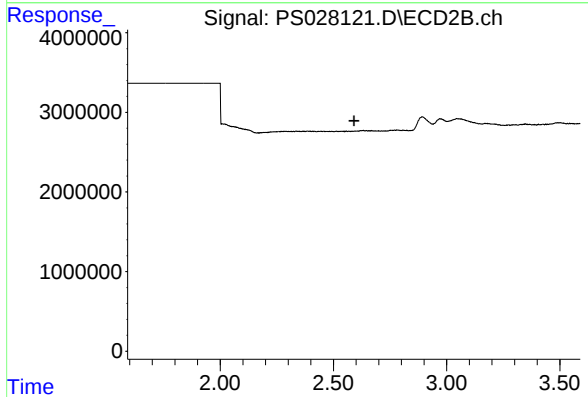


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.591 min
Response: 0
Conc: N.D.

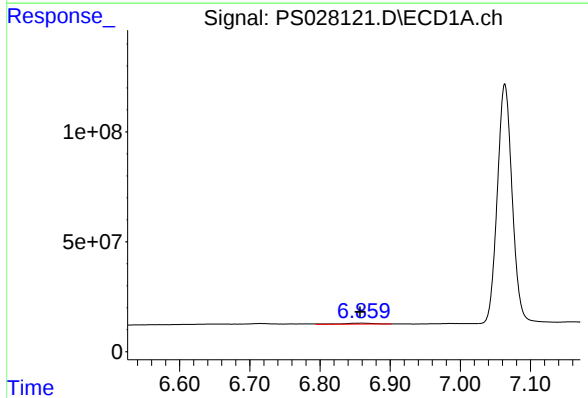


#3 4-Nitrophenol

R.T.: 6.860 min
Delta R.T.: 0.003 min
Response: 14077855
Conc: 5.99 ng/ml

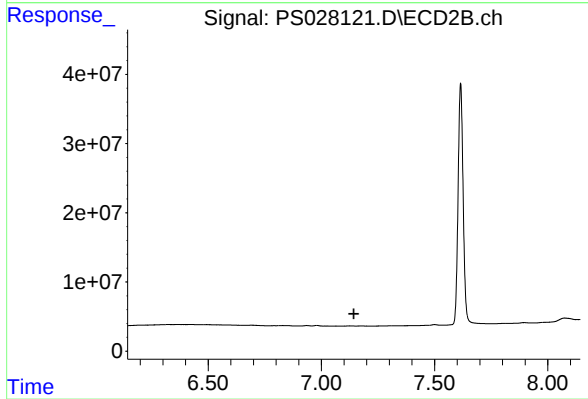

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 7.144 min
Response: 0
Conc: N.D.

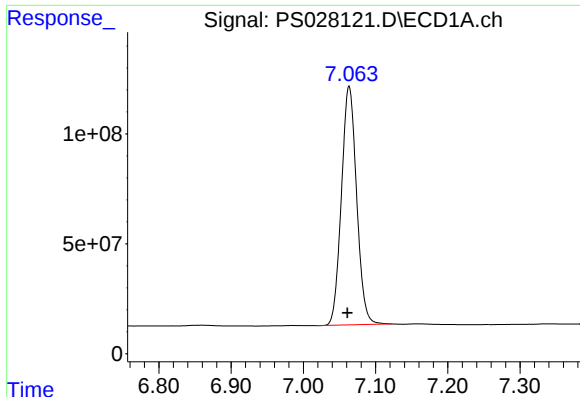

#4 2,4-DCAA


R.T.: 7.063 min
Delta R.T.: 0.002 min
Response: 1589042646
Conc: 507.88 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

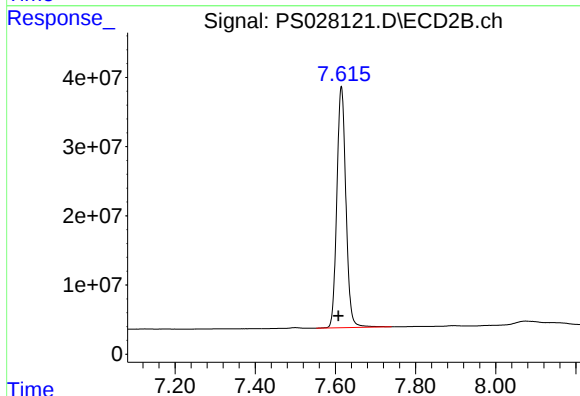


#4 2,4-DCAA

R.T.: 7.615 min
Delta R.T.: 0.008 min
Response: 547430131
Conc: 547.90 ng/ml

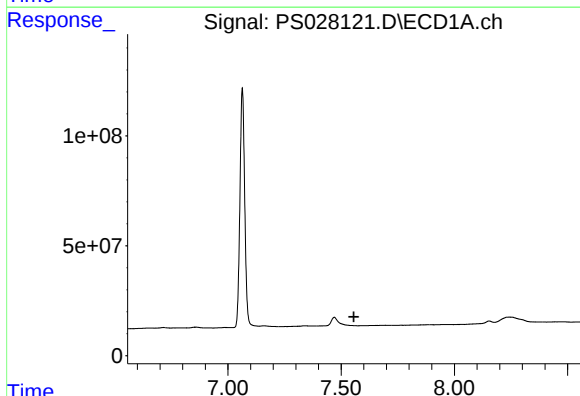


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.556 min
Response: 0
Conc: N.D.

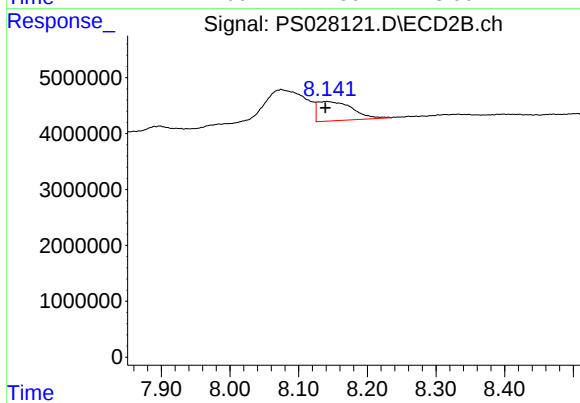

#7 MCPA


R.T.: 8.141 min
Delta R.T.: 0.002 min
Response: 12072161
Conc: 2.66 ug/ml

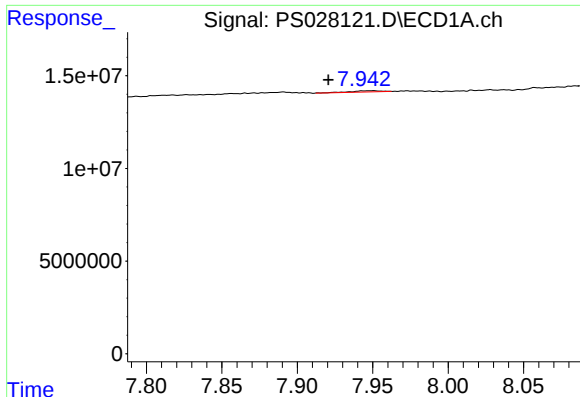

#8 DICHLORPROP


R.T.: 7.949 min
Delta R.T.: 0.028 min
Response: 790903
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

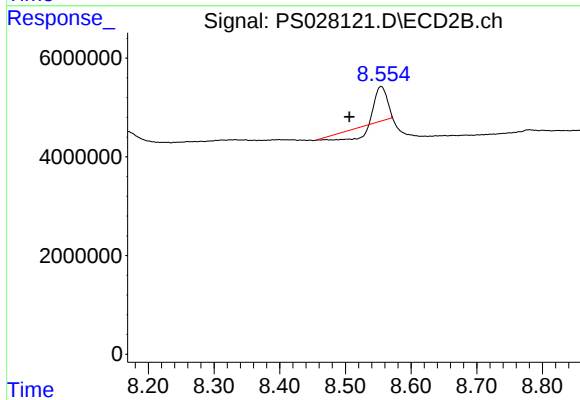


#8 DICHLORPROP

R.T.: 8.554 min
Delta R.T.: 0.048 min
Response: 3748740
Conc: 3.43 ng/ml

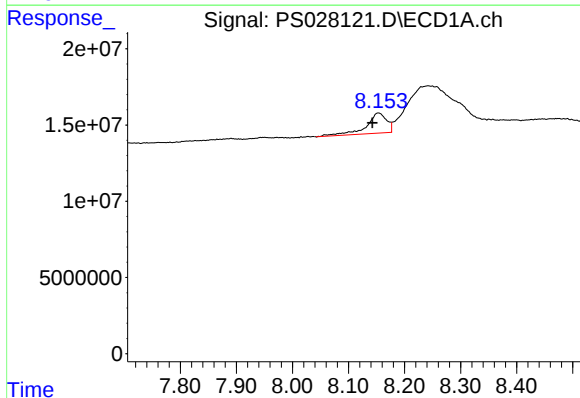


#9 2,4-D

R.T.: 8.153 min
Delta R.T.: 0.011 min
Response: 33765024
Conc: 8.31 ng/ml

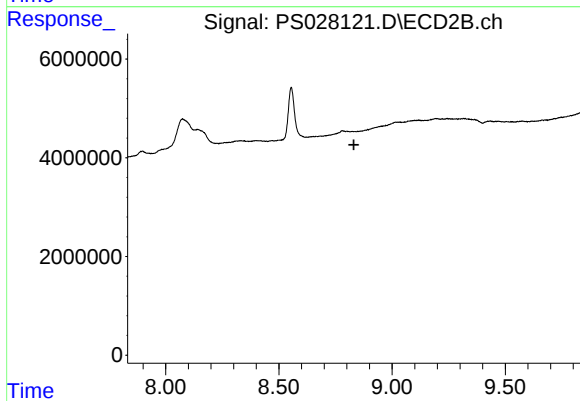

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.831 min
Response: 0
Conc: N.D.

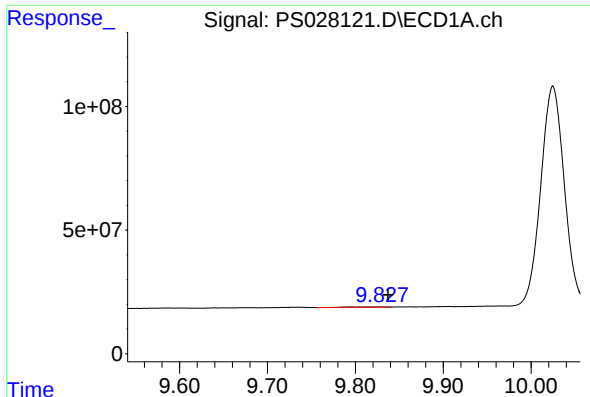

#13 2,4-DB

R.T.: 9.826 min
Delta R.T.: -0.011 min
Response: 4032151
Conc: 1.19 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

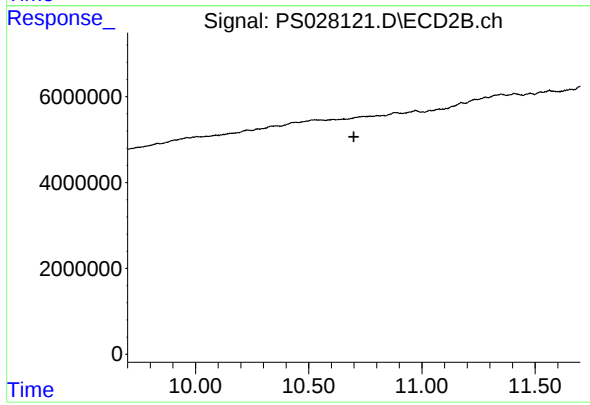

#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 10.700 min
Response: 0
Conc: N.D.