

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS103124\
 Data File : PS028133.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Oct 2024 23:42
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 01 02:28:00 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS103124.M
 Quant Title : 8080.M
 QLast Update : Thu Oct 31 13:10:03 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.063	7.609	1643.8E6	537.4E6	525.383	537.827
Target Compounds							
2) T	3,5-DICHL...	6.237	0.000	9171763	0	1.980	N.D. #
3) T	4-Nitroph...	6.856	0.000	14430425	0	6.135	N.D. #
8) T	DICHLORPROP	7.951f	8.549f	-475042	5087509	N.D.	4.652
9) T	2,4-D	8.154	0.000	36612074	0	9.015	N.D. #
10) T	Pentachlo...	8.439	0.000	4005584	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.041f	0.000	8586873	0	<MDL	N.D. #
12) T	2,4,5-T	9.307f	0.000	1446440	0	<MDL	N.D. #
13) T	2,4-DB	9.850	0.000	3265871	0	<MDL	N.D. #
14) T	DINOSEB	11.006	0.000	3444811	0	<MDL	N.D. #
15) T	Picloram	10.825	0.000	54532722	0	1.580	N.D. #
16) T	DCPA	11.313	0.000	1945374	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS103124\
Data File : PS028133.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Oct 2024 23:42
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 01 02:28:00 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS103124.M
Quant Title : 8080.M
QLast Update : Thu Oct 31 13:10:03 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

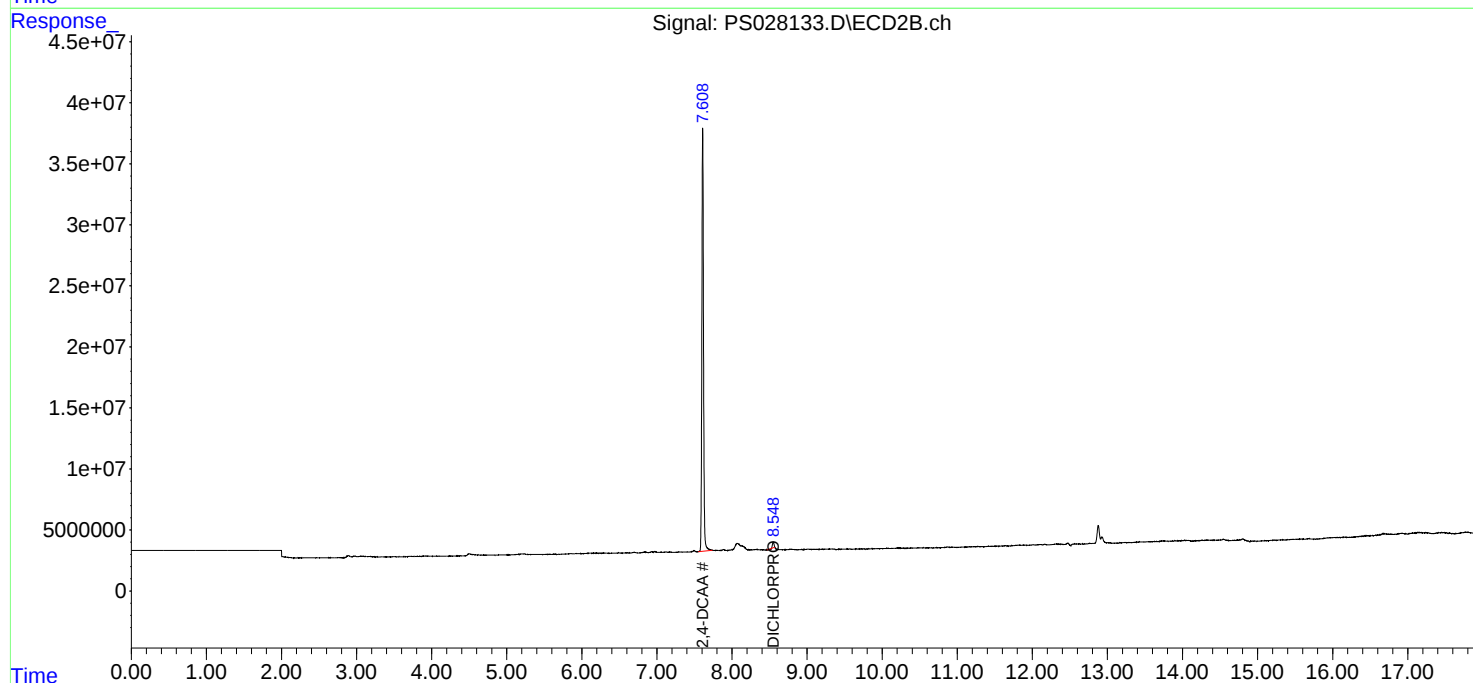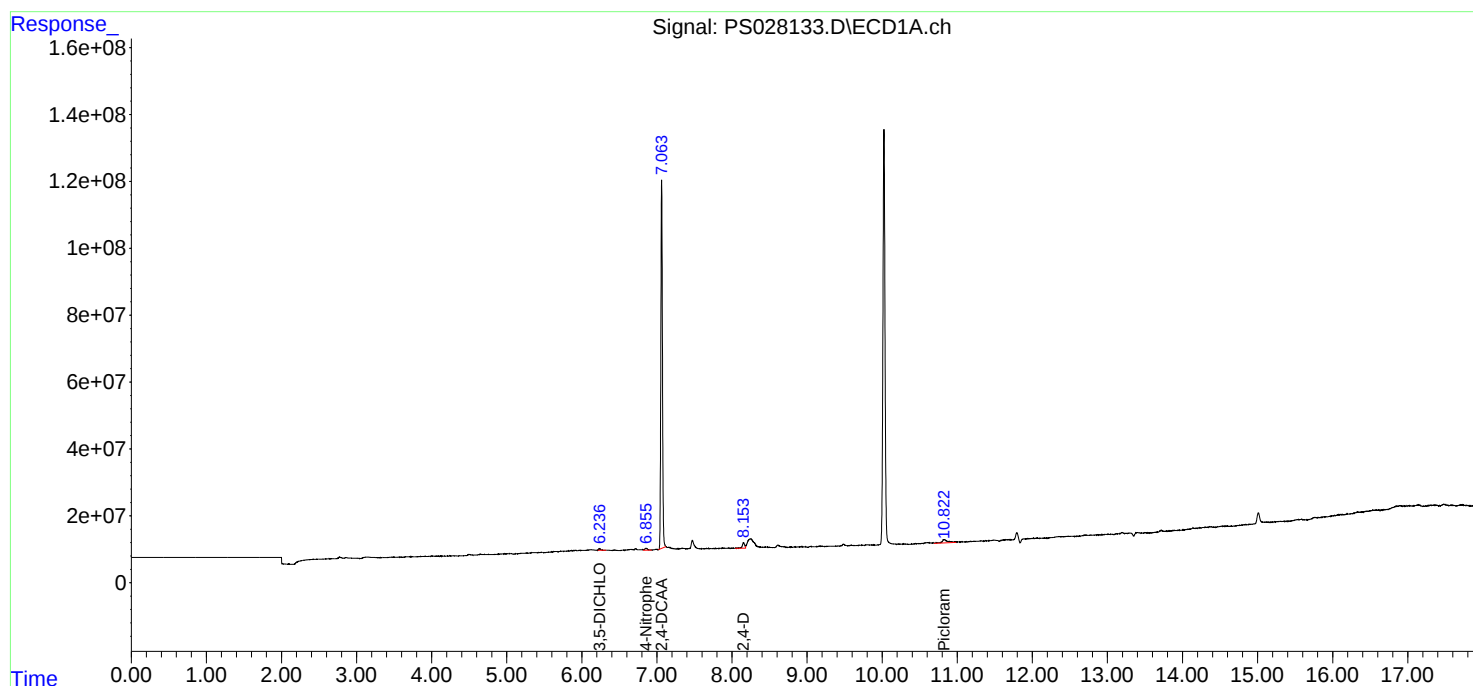


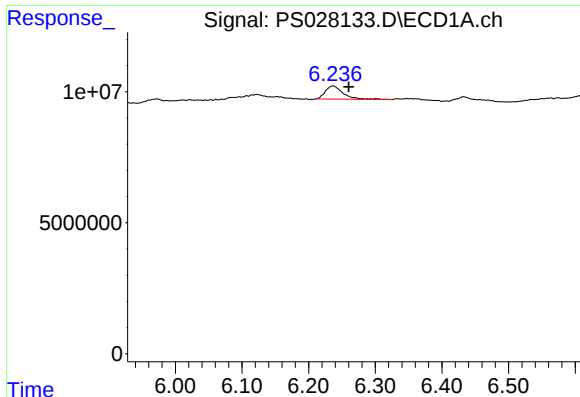

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.237 min
Delta R.T.: -0.023 min
Response: 9171763
Conc: 1.98 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

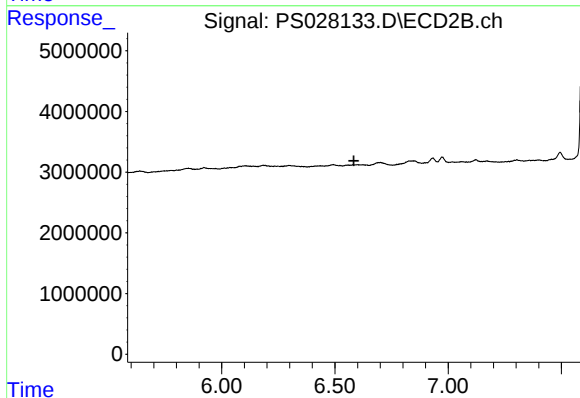


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.584 min
Response: 0
Conc: N.D.

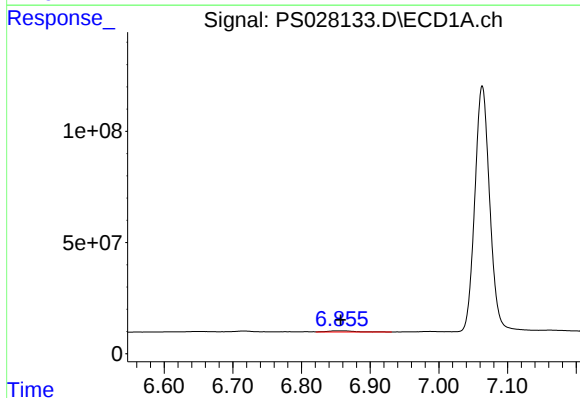


#3 4-Nitrophenol

R.T.: 6.856 min
Delta R.T.: -0.001 min
Response: 14430425
Conc: 6.14 ng/ml

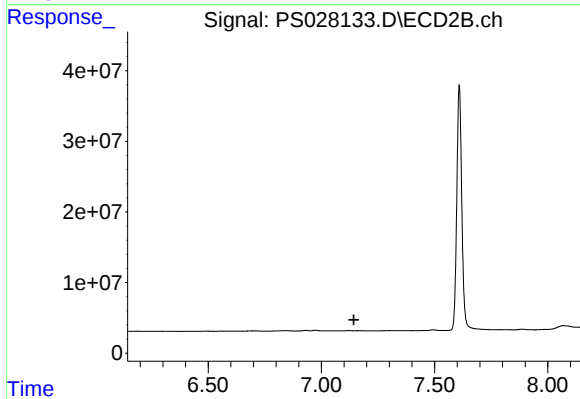

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 7.144 min
Response: 0
Conc: N.D.

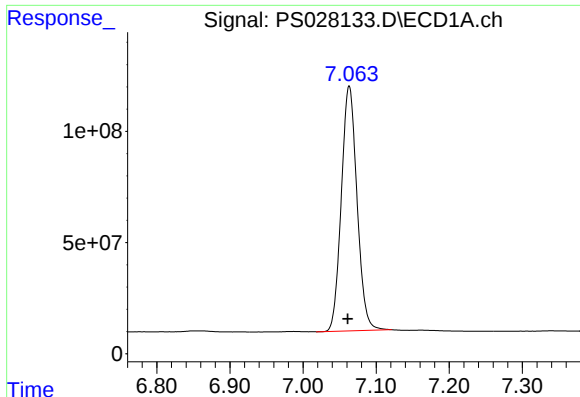

#4 2,4-DCAA


R.T.: 7.063 min
Delta R.T.: 0.002 min
Response: 1643790200
Conc: 525.38 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

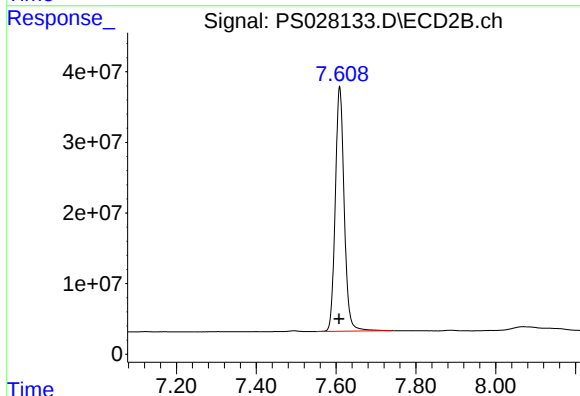


#4 2,4-DCAA

R.T.: 7.609 min
Delta R.T.: 0.002 min
Response: 537366995
Conc: 537.83 ng/ml

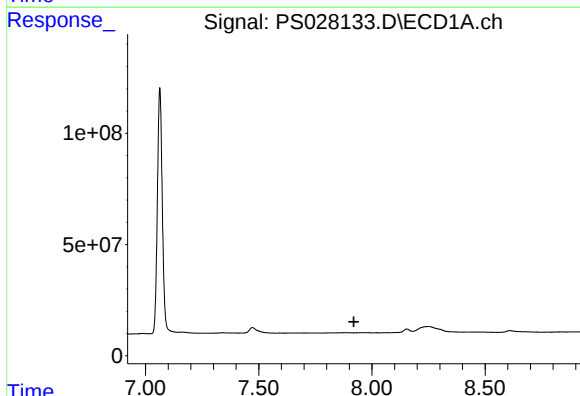


#8 DICHLORPROP

R.T.: 7.951 min
Delta R.T.: 0.030 min
Response: -475042
Conc: N.D.

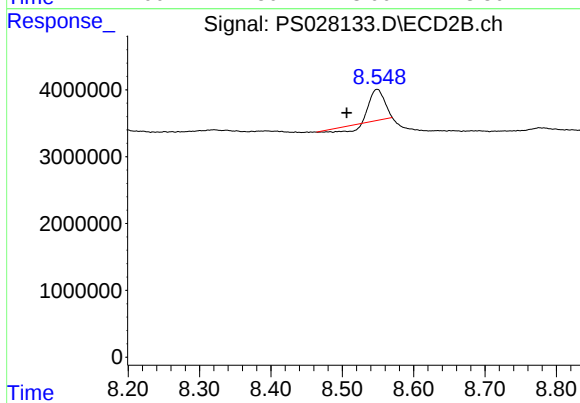

#8 DICHLORPROP


R.T.: 8.549 min
Delta R.T.: 0.043 min
Response: 5087509
Conc: 4.65 ng/ml

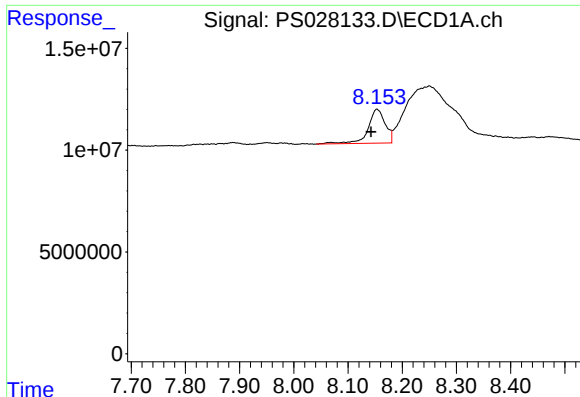

#9 2,4-D


R.T.: 8.154 min
Delta R.T.: 0.011 min
Response: 36612074
Conc: 9.01 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

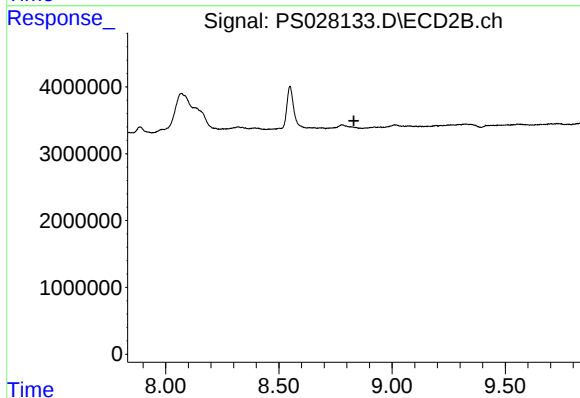


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 8.831 min
Response: 0
Conc: N.D.

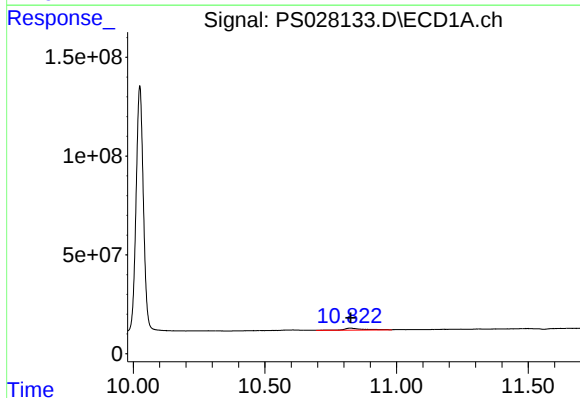

#15 Picloram

R.T.: 10.825 min
Delta R.T.: -0.001 min
Response: 54532722
Conc: 1.58 ng/ml

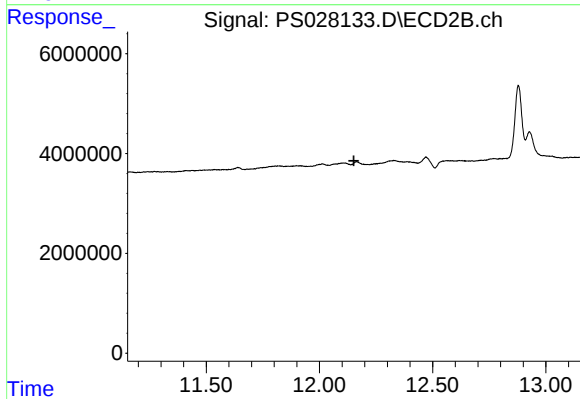

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 12.152 min
Response: 0
Conc: N.D.