

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS103124\
 Data File : PS028145.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Nov 2024 04:54
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 01 05:36:49 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS103124.M
 Quant Title : 8080.M
 QLast Update : Thu Oct 31 13:10:03 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.064	7.612	1656.6E6	552.7E6	529.482	553.133
Target Compounds							
2) T	3,5-DICHL...	6.238	0.000	11366263	0	2.454	N.D. #
3) T	4-Nitroph...	6.862	0.000	13189421	0	5.607	N.D. #
7) T	MCPA	0.000	8.131	0	8465171	N.D.	1.869
8) T	DICHLORPROP	7.890f	8.553f	411161	1617247	<MDL	1.479 #
9) T	2,4-D	8.155	0.000	34356406	0	8.459	N.D. #
10) T	Pentachlo...	8.445	0.000	2697177	0	<MDL	N.D. #
11) T	2,4,5-TP ...	8.983	0.000	3685345	0	<MDL	N.D. #
12) T	2,4,5-T	9.320f	0.000	2287941	0	<MDL	N.D. #
13) T	2,4-DB	9.846	0.000	1300084	0	<MDL	N.D. #
15) T	Picloram	10.823	0.000	94055171	0	2.726	N.D. #
16) T	DCPA	11.319	0.000	1833181	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS103124\
Data File : PS028145.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Nov 2024 04:54
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 01 05:36:49 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS103124.M
Quant Title : 8080.M
QLast Update : Thu Oct 31 13:10:03 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

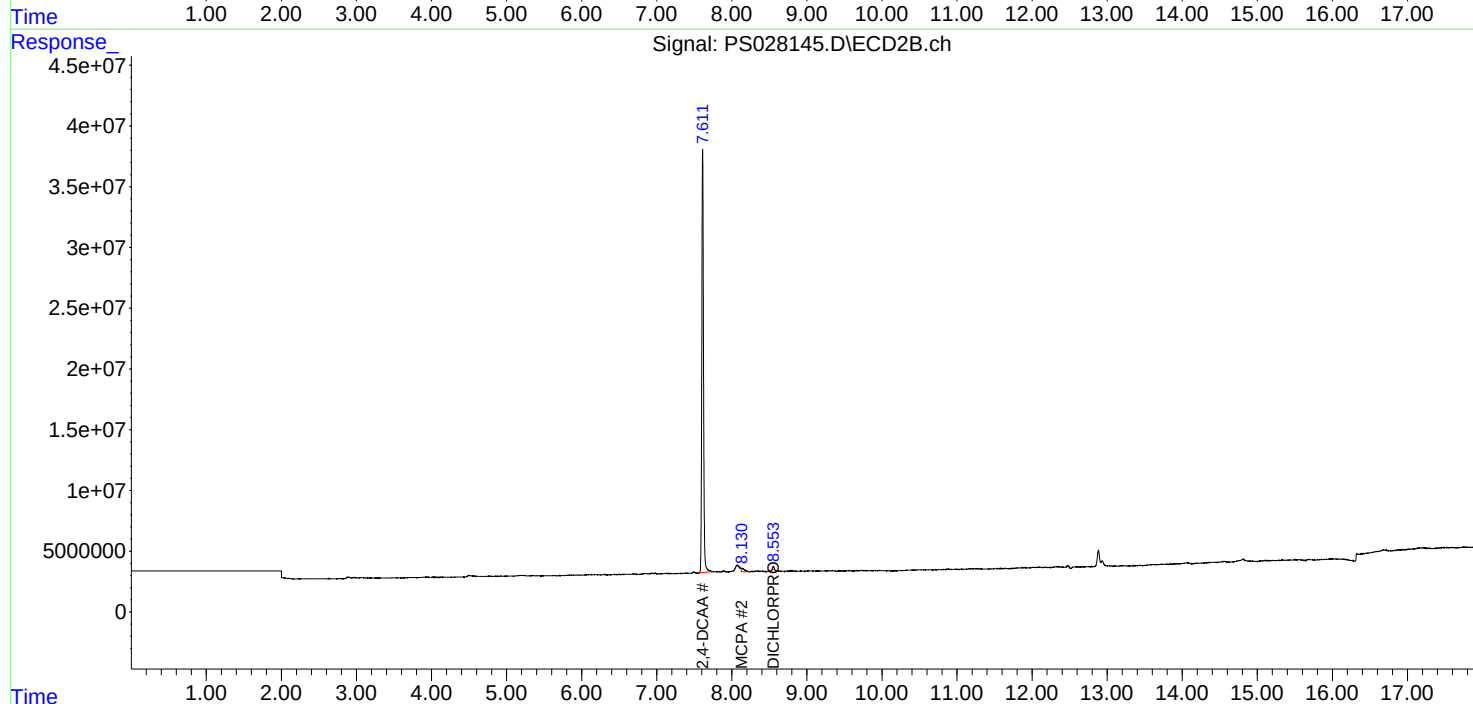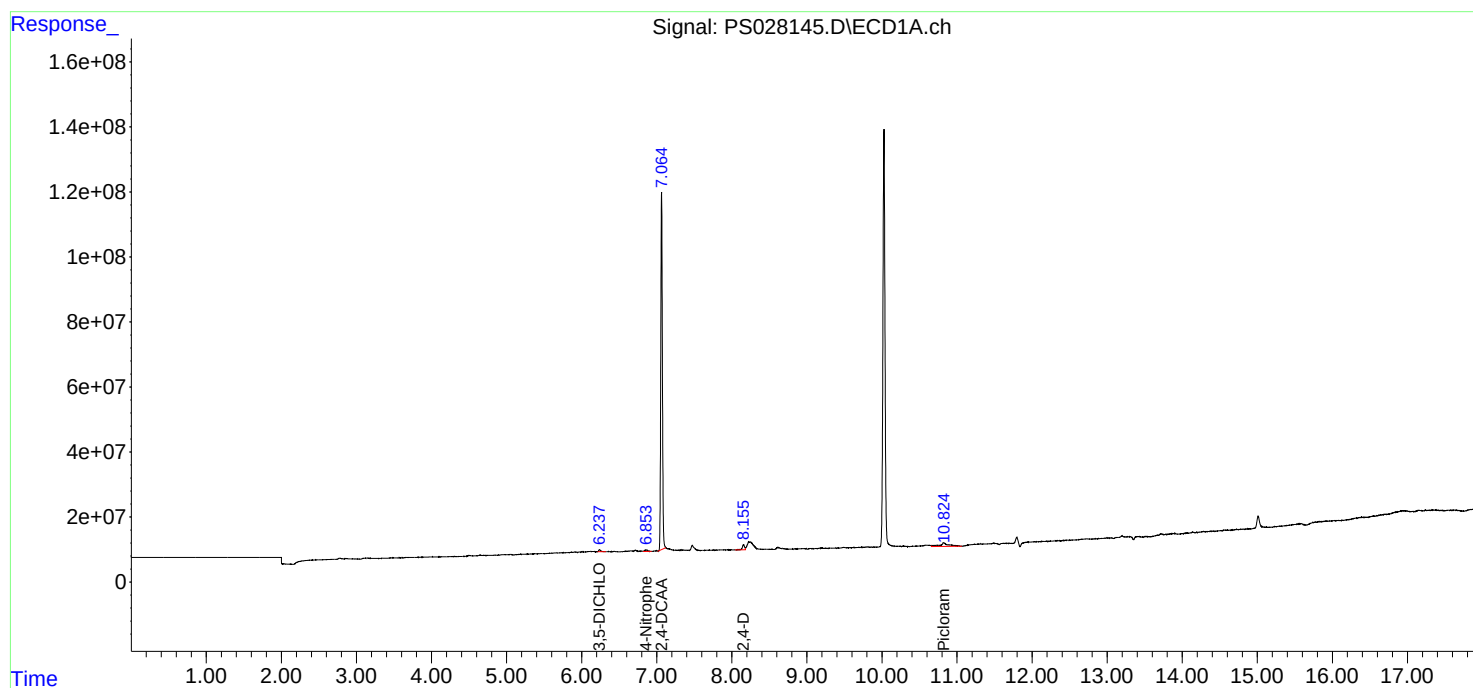


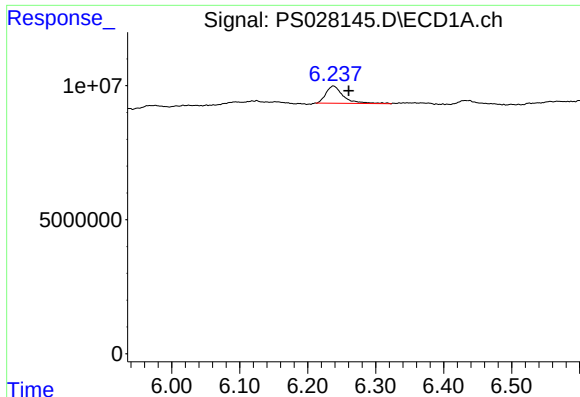

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.238 min
Delta R.T.: -0.022 min
Response: 11366263
Conc: 2.45 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

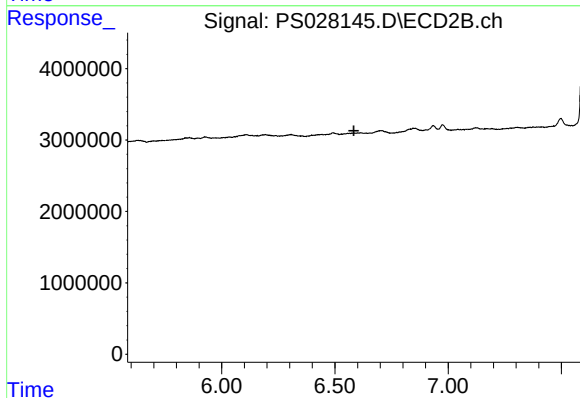


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.584 min
Response: 0
Conc: N.D.

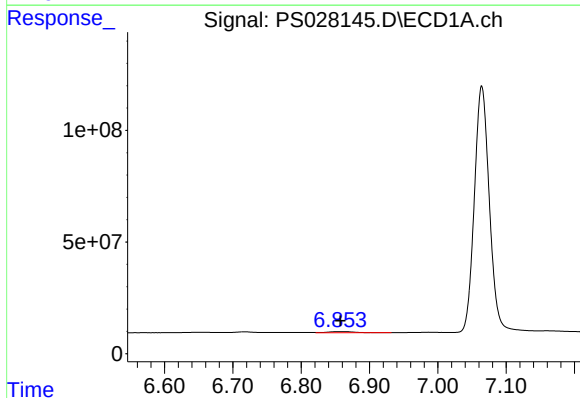


#3 4-Nitrophenol

R.T.: 6.862 min
Delta R.T.: 0.005 min
Response: 13189421
Conc: 5.61 ng/ml

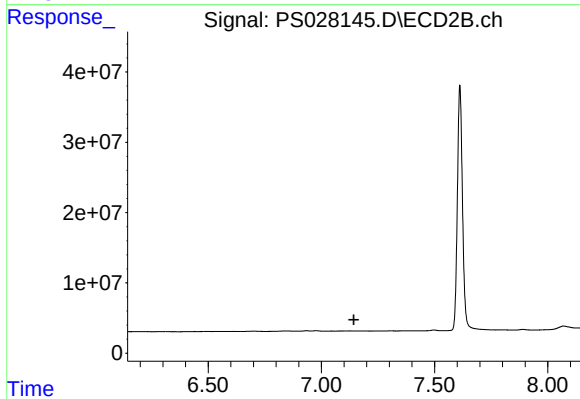

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 7.144 min
Response: 0
Conc: N.D.

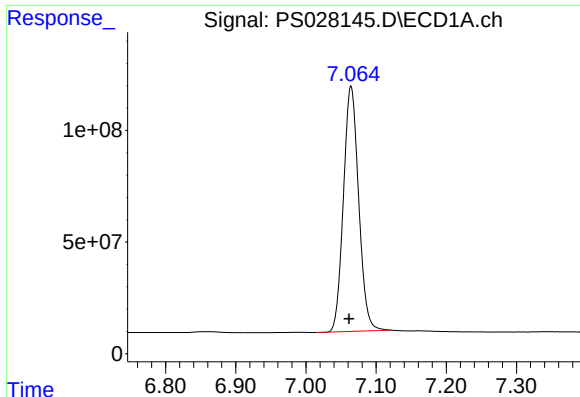

#4 2,4-DCAA


R.T.: 7.064 min
Delta R.T.: 0.003 min
Response: 1656616126
Conc: 529.48 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

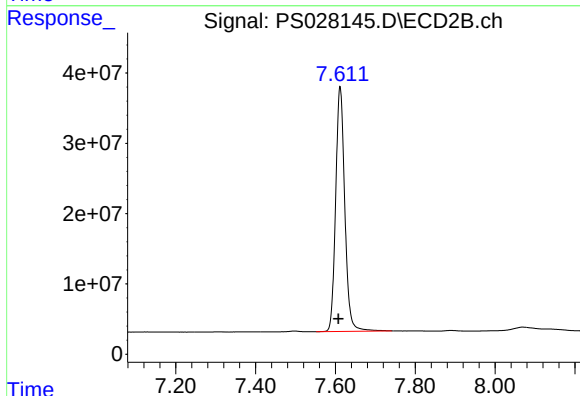


#4 2,4-DCAA

R.T.: 7.612 min
Delta R.T.: 0.004 min
Response: 552660035
Conc: 553.13 ng/ml

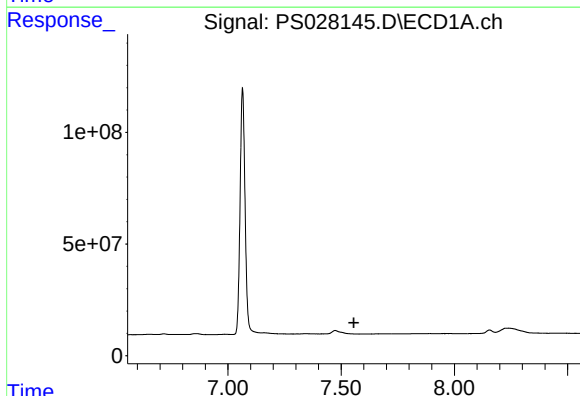


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.556 min
Response: 0
Conc: N.D.

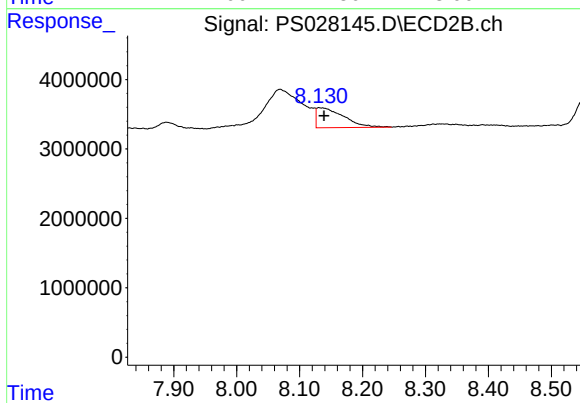

#7 MCPA


R.T.: 8.131 min
Delta R.T.: -0.008 min
Response: 8465171
Conc: 1.87 ug/ml

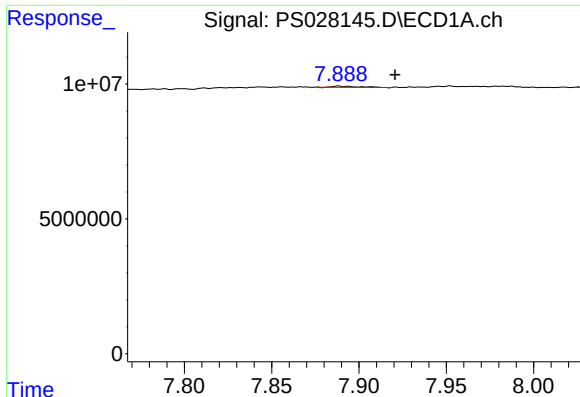

#8 DICHLORPROP


R.T.: 7.890 min
Delta R.T.: -0.031 min
Response: 411161
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

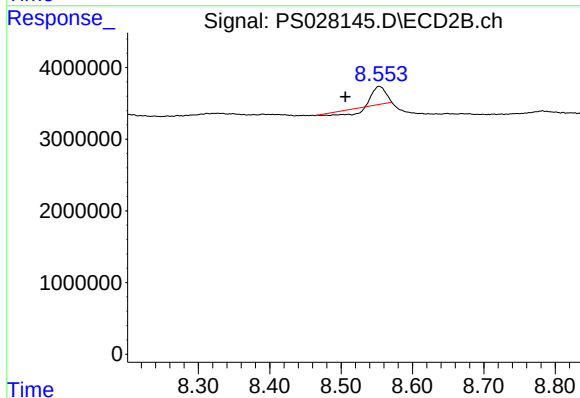


#8 DICHLORPROP

R.T.: 8.553 min
Delta R.T.: 0.047 min
Response: 1617247
Conc: 1.48 ng/ml

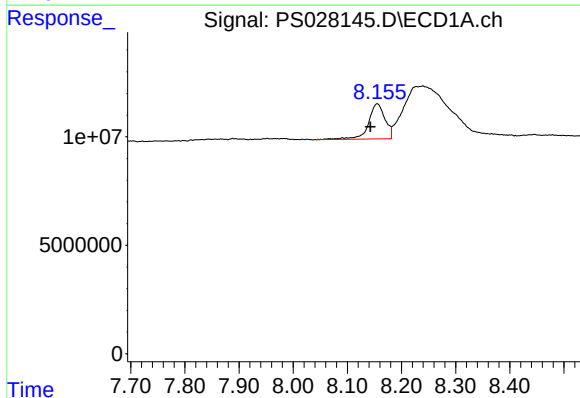


#9 2,4-D

R.T.: 8.155 min
Delta R.T.: 0.012 min
Response: 34356406
Conc: 8.46 ng/ml

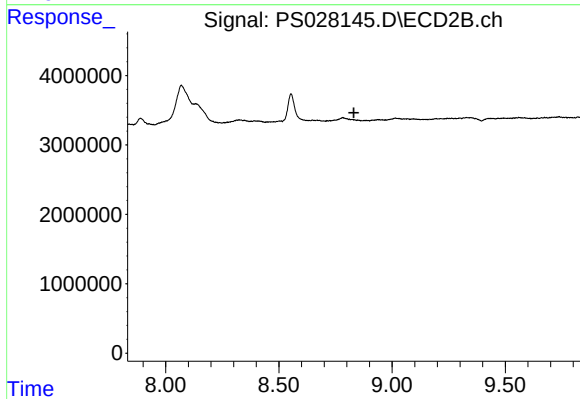

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.831 min
Response: 0
Conc: N.D.

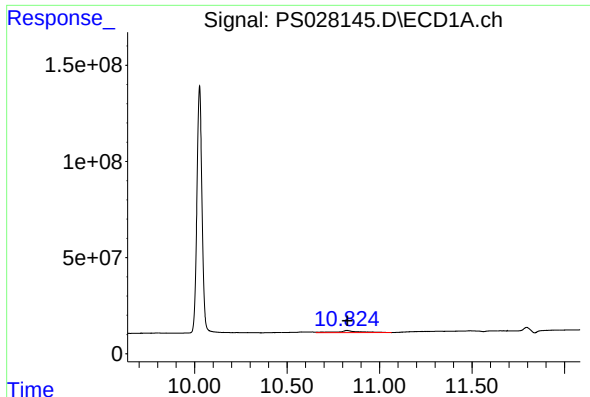

#15 Picloram

R.T.: 10.823 min
Delta R.T.: -0.003 min
Response: 94055171
Conc: 2.73 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

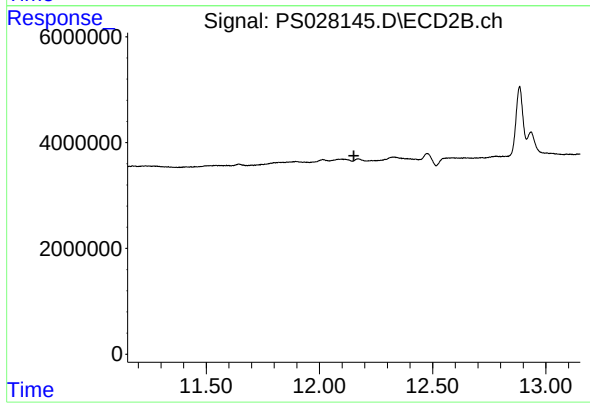

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 12.152 min
Response: 0
Conc: N.D.