

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS103124\
 Data File : PS028157.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Nov 2024 10:07
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 04 02:28:13 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS103124.M
 Quant Title : 8080.M
 QLast Update : Thu Oct 31 13:10:03 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.064	7.605	1666.1E6	527.1E6	532.528	527.508
Target Compounds							
2) T	3,5-DICHL...	6.236	0.000	9145315	0	1.974	N.D. #
3) T	4-Nitroph...	6.857	0.000	16603674	0	7.059	N.D. #
8) T	DICHLORPROP	7.946f	8.546f	-283715	5935220	N.D.	5.427
9) T	2,4-D	8.155	0.000	35195731	0	8.666	N.D. #
10) T	Pentachlo...	8.447	0.000	4213920	0	<MDL	N.D. #
11) T	2,4,5-TP ...	8.986	0.000	3175126	0	<MDL	N.D. #
12) T	2,4,5-T	9.297	0.000	2253017	0	<MDL	N.D. #
13) T	2,4-DB	9.857	0.000	776293	0	<MDL	N.D. #
14) T	DINOSEB	11.016	0.000	1857533	0	<MDL	N.D. #
15) T	Picloram	10.827	0.000	36575118	0	1.060	N.D. #
16) T	DCPA	11.312	0.000	2241399	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS103124\
Data File : PS028157.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Nov 2024 10:07
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 04 02:28:13 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS103124.M
Quant Title : 8080.M
QLast Update : Thu Oct 31 13:10:03 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

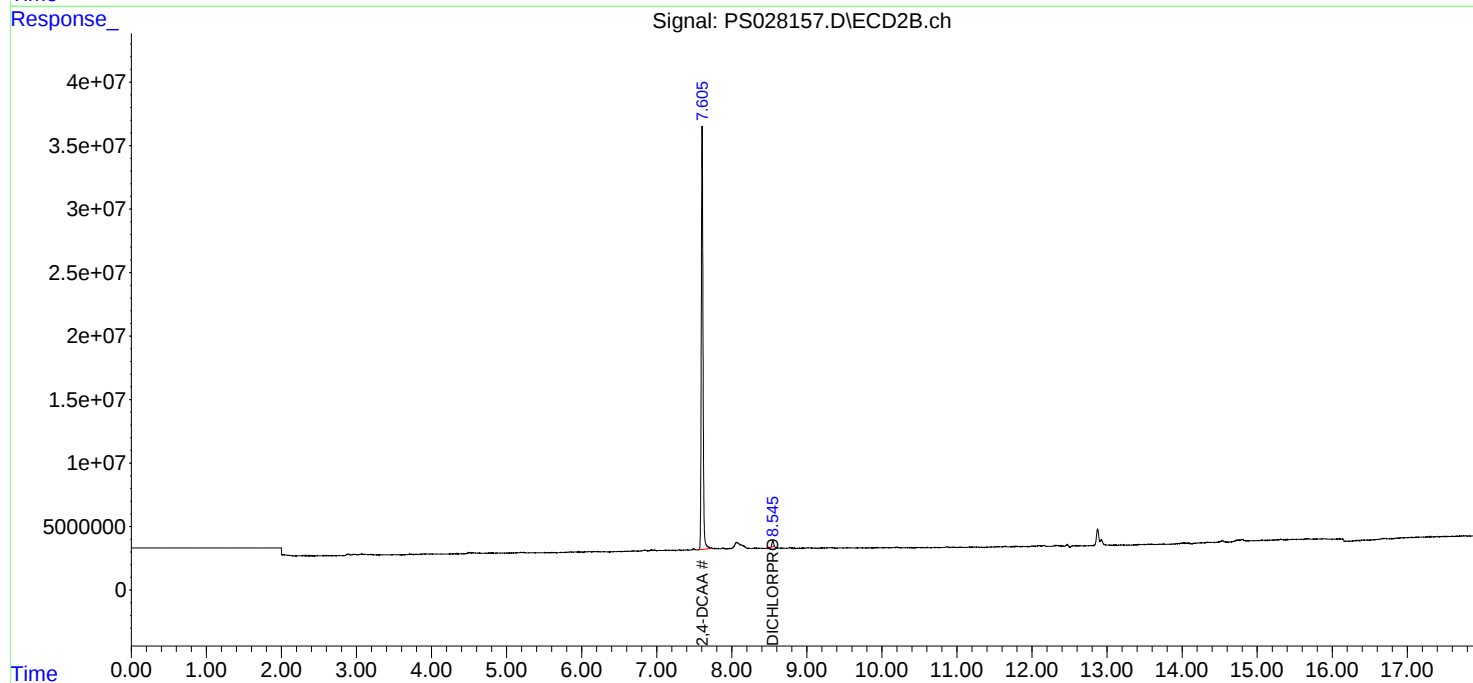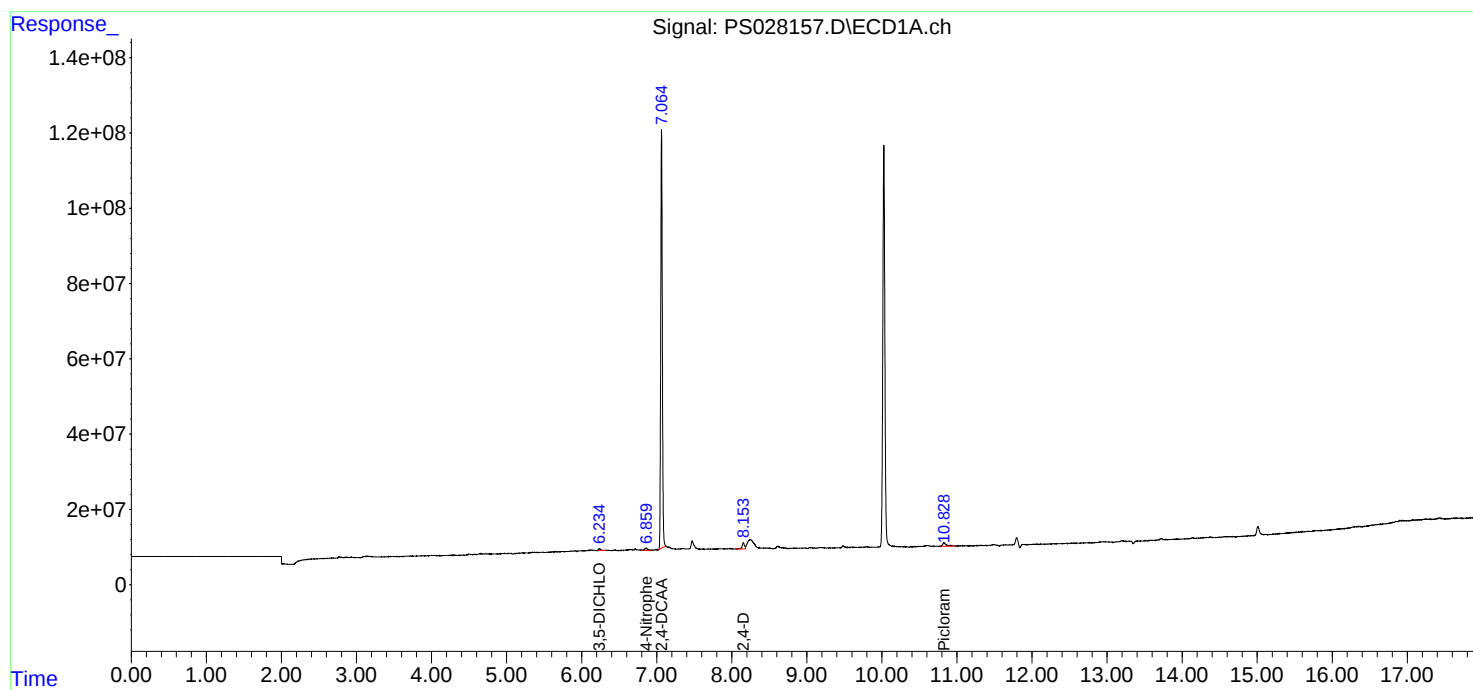


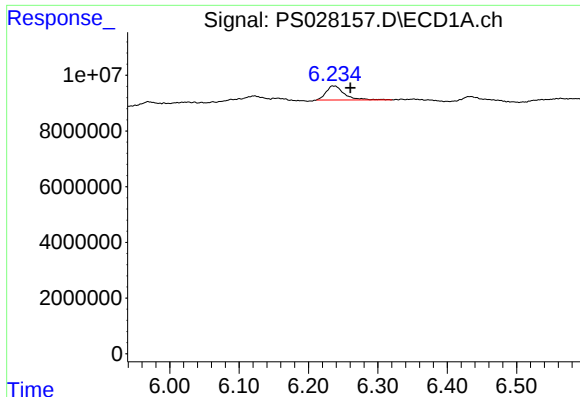

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.236 min
Delta R.T.: -0.024 min
Response: 9145315
Conc: 1.97 ng/ml

Instrument :
ECD_S
ClientSampleId :

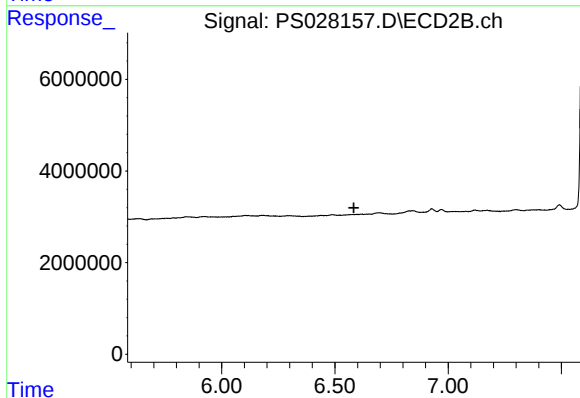


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.584 min
Response: 0
Conc: N.D.

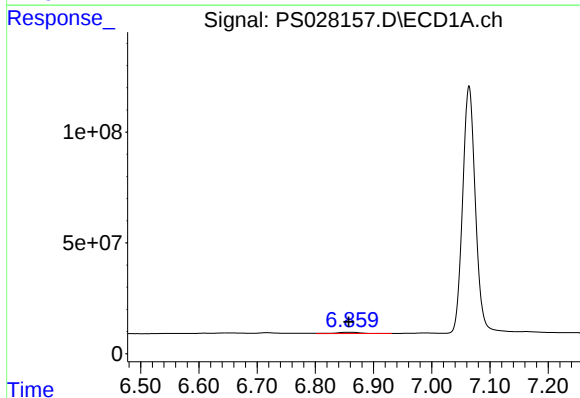


#3 4-Nitrophenol

R.T.: 6.857 min
Delta R.T.: 0.000 min
Response: 16603674
Conc: 7.06 ng/ml

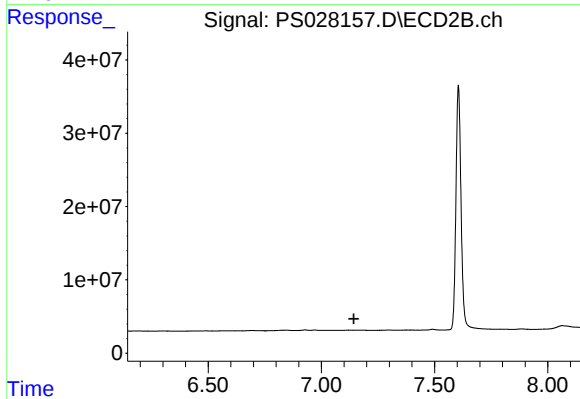

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 7.144 min
Response: 0
Conc: N.D.

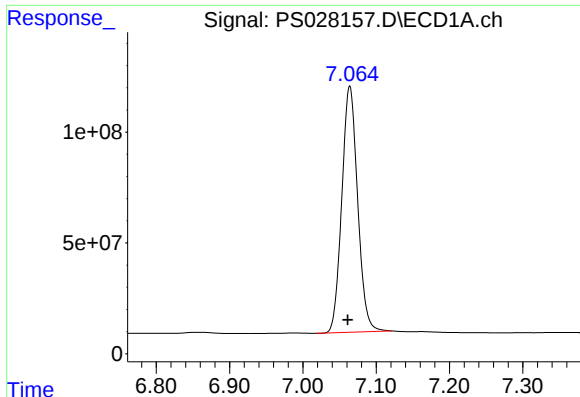

#4 2,4-DCAA


R.T.: 7.064 min
Delta R.T.: 0.003 min
Response: 1666144625
Conc: 532.53 ng/ml

Instrument :
ECD_S
ClientSampleId :

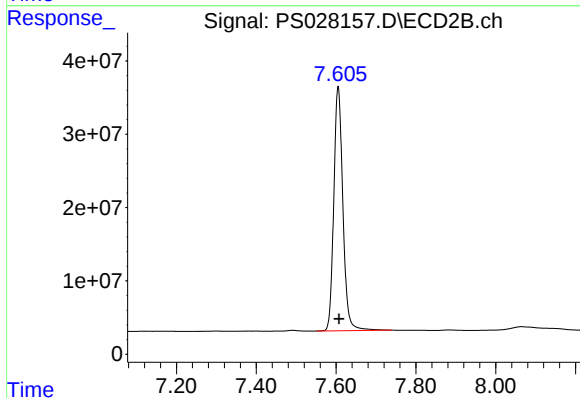


#4 2,4-DCAA

R.T.: 7.605 min
Delta R.T.: -0.002 min
Response: 527056840
Conc: 527.51 ng/ml

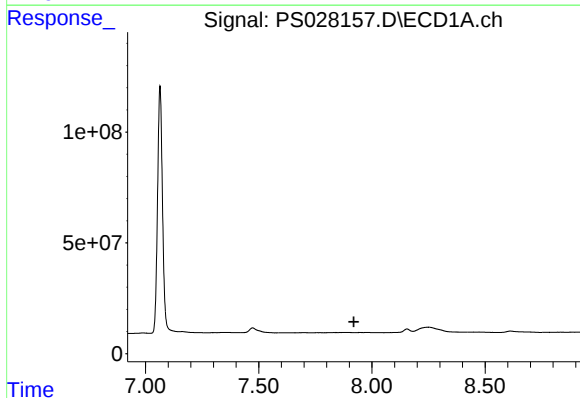


#8 DICHLORPROP

R.T.: 7.946 min
Delta R.T.: 0.025 min
Response: -283715
Conc: N.D.

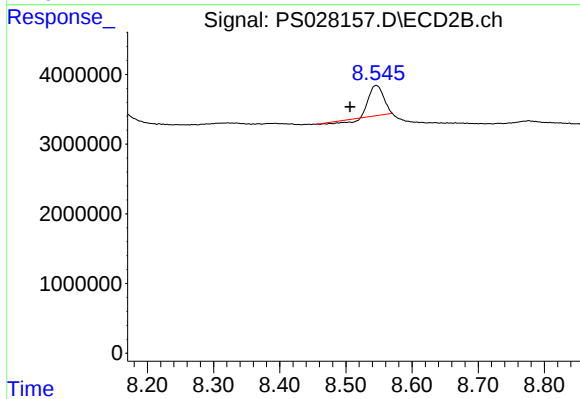

#8 DICHLORPROP


R.T.: 8.546 min
Delta R.T.: 0.039 min
Response: 5935220
Conc: 5.43 ng/ml

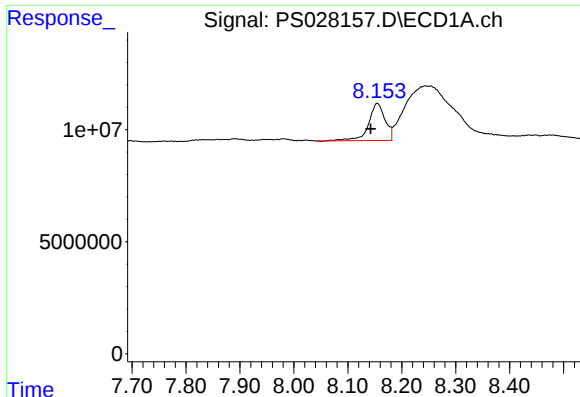

#9 2,4-D


R.T.: 8.155 min
Delta R.T.: 0.012 min
Response: 35195731
Conc: 8.67 ng/ml

Instrument :
ECD_S
ClientSampleId :

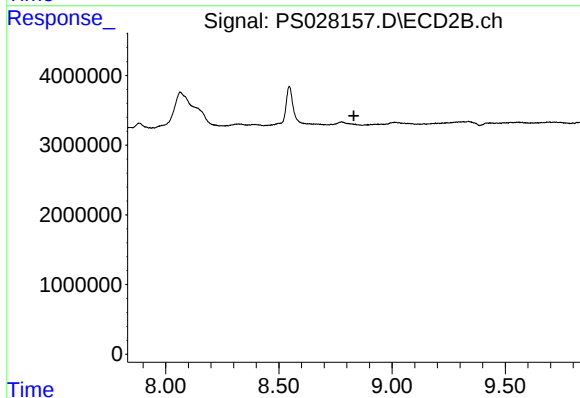


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 8.831 min
Response: 0
Conc: N.D.

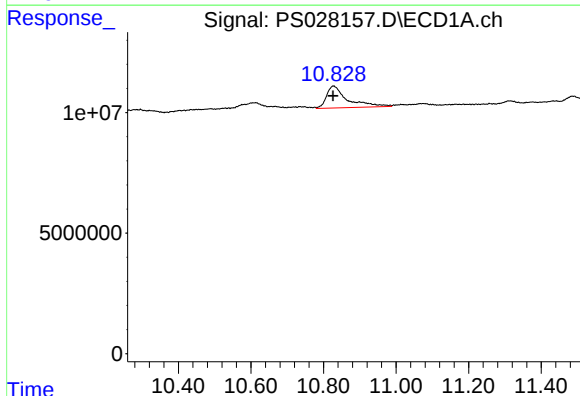

#15 Picloram

R.T.: 10.827 min
Delta R.T.: 0.002 min
Response: 36575118
Conc: 1.06 ng/ml

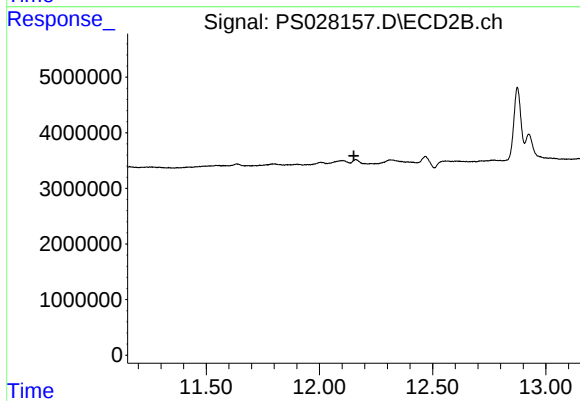

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 12.152 min
Response: 0
Conc: N.D.