

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110118\
 Data File : PS002229.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Nov 2018 10:19
 Operator : EI\SJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 02 03:45:49 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102618.M
 Quant Title : 8080.M
 QLast Update : Sat Oct 27 01:34:10 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	0.000	10.912	0	333718	N.D.	0.929 #
Target Compounds							
2) T	3,5-DICHL...	0.000	9.073	0	114587	N.D.	0.258 #
3) T	4-Nitroph...	11.026	10.062	3190959	446169	19.127	2.502 #
5) T	DICAMBA	0.000	11.192	0	121962	N.D.	0.098 #
6) T	MCP	12.117	11.427	2613728	798624	2.646	0.928 #
7) T	MCPA	12.360	11.815	2468475	496551	1.644	0.367 #
8) T	DICHLORPROP	0.000	12.339	0	240700	N.D.	0.750 #
9) T	2,4-D	0.000	12.774	0	46509	N.D.	0.109 #
10) T	Pentachlo...	0.000	13.335	0	128989	N.D.	0.027 #
11) T	2,4,5-TP ...	0.000	13.952	0	446713	N.D.	0.244 #
12) T	2,4,5-T	0.000	14.515	0	14394952	N.D.	9.613 #
13) T	2,4-DB	0.000	15.146	0	117183	N.D.	0.529 #
14) T	DINOSEB	0.000	15.589	0	43717	N.D.	0.035 #
15) T	Picloram	16.918	16.825	37859081	35987396	15.872	15.908
16) T	DCPA	0.000	16.825	0	35987396	N.D.	15.198 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110118\
Data File : PS002229.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Nov 2018 10:19
Operator : EI\SJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 02 03:45:49 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102618.M
Quant Title : 8080.M
QLast Update : Sat Oct 27 01:34:10 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

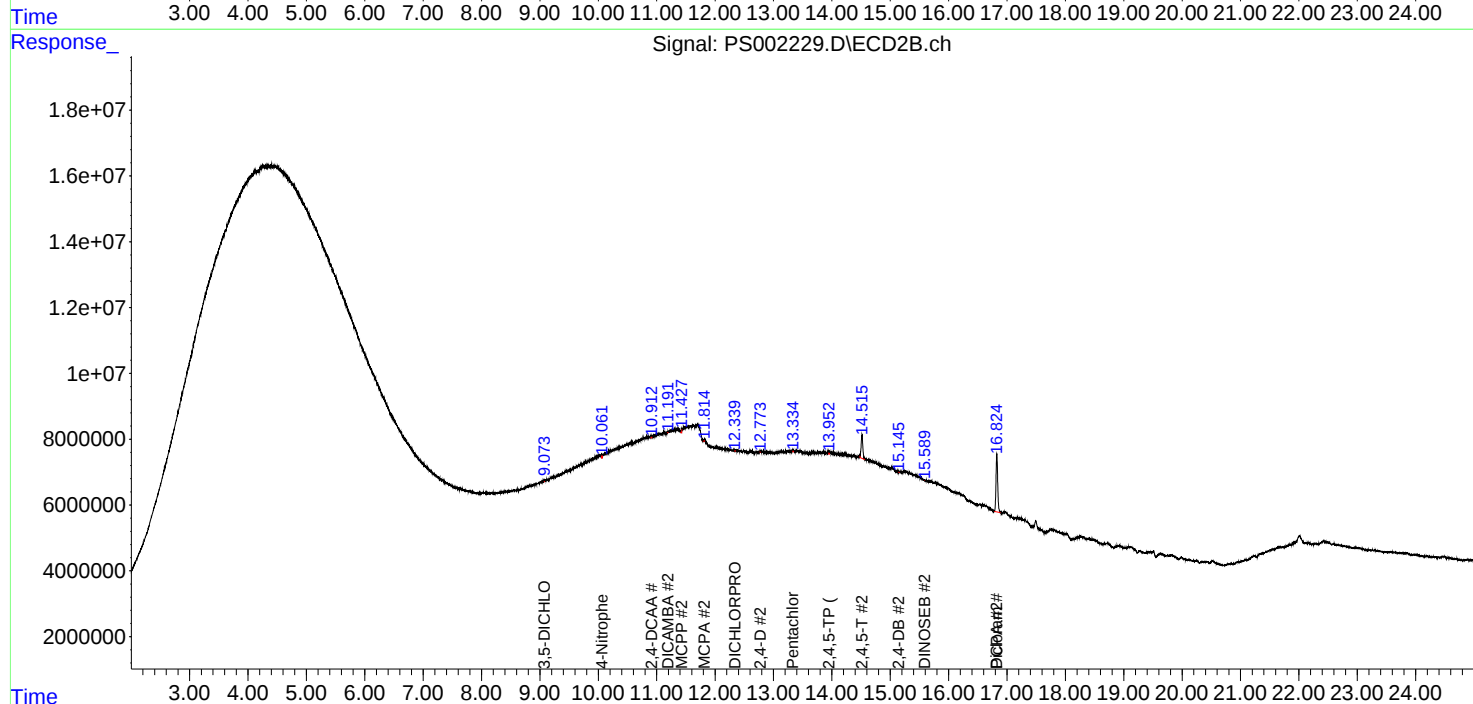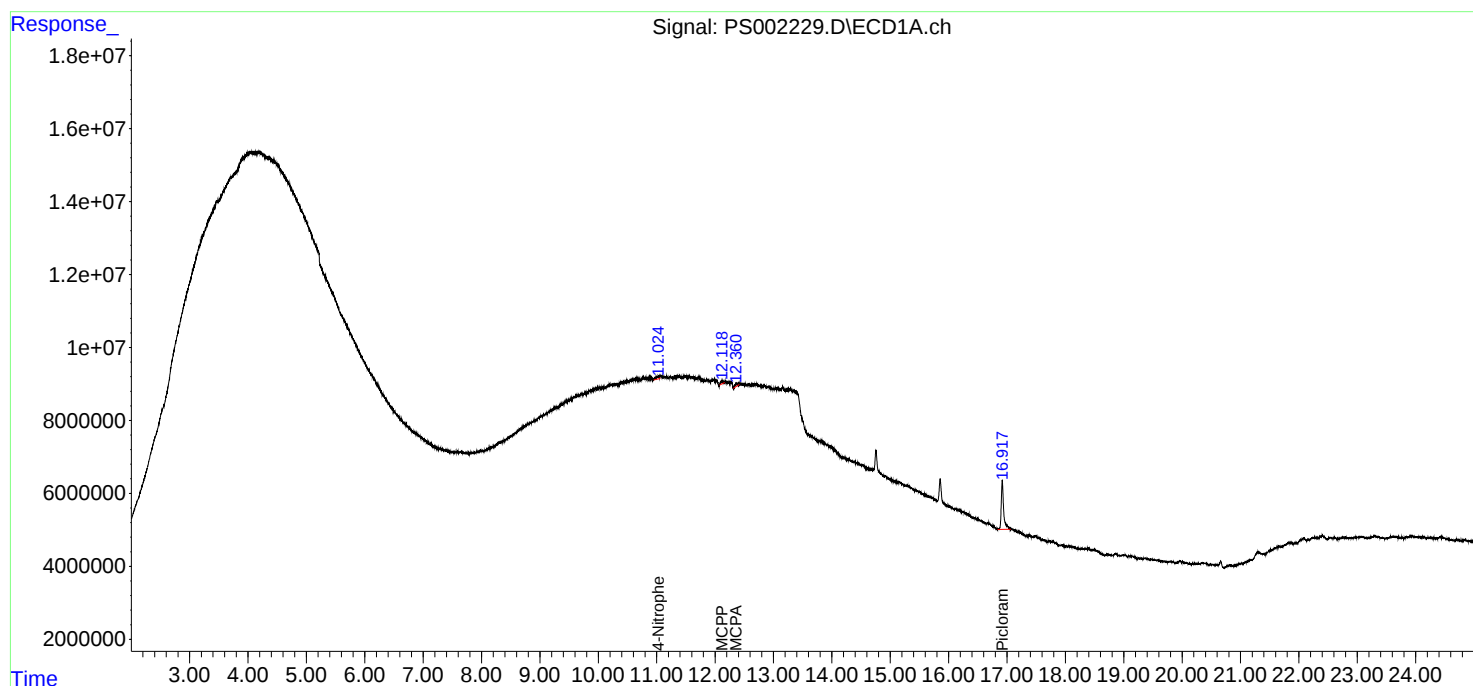


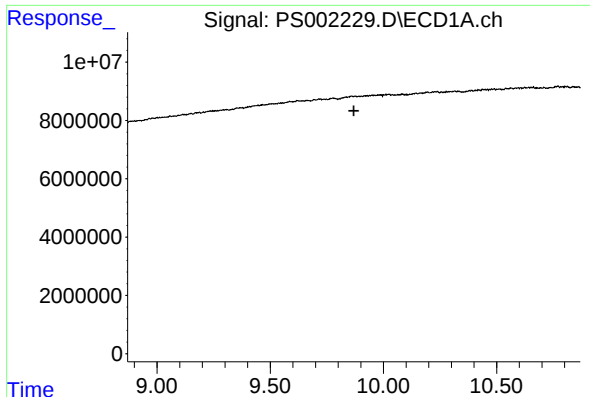

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 9.870 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

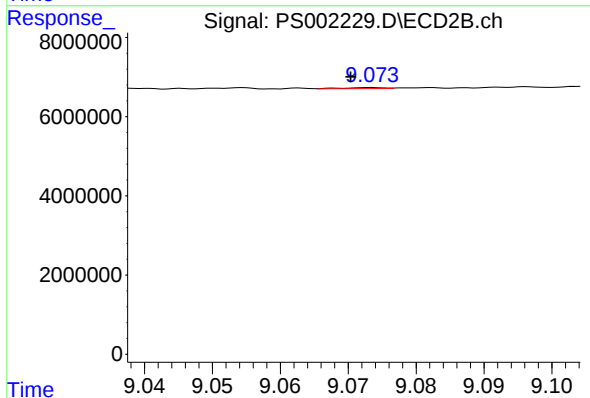


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 9.073 min
Delta R.T.: 0.003 min
Response: 114587
Conc: 0.26 ng/ml

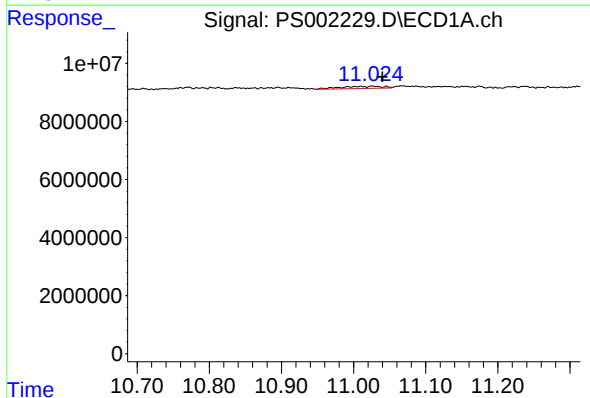


#3 4-Nitrophenol

R.T.: 11.026 min
Delta R.T.: -0.013 min
Response: 3190959
Conc: 19.13 ng/ml

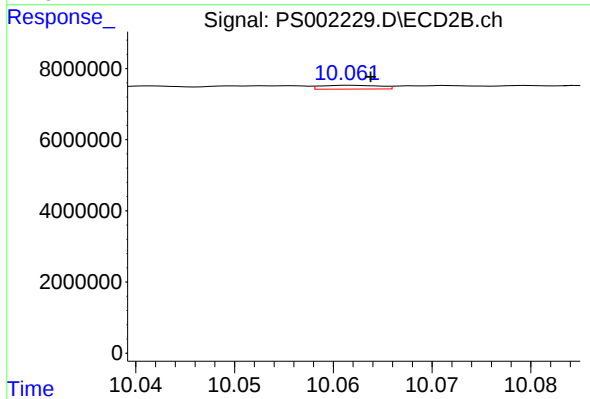

#3 4-Nitrophenol


R.T.: 10.062 min
Delta R.T.: -0.002 min
Response: 446169
Conc: 2.50 ng/ml

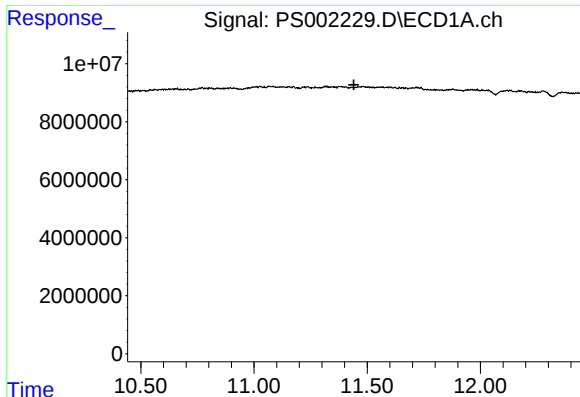

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 11.441 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

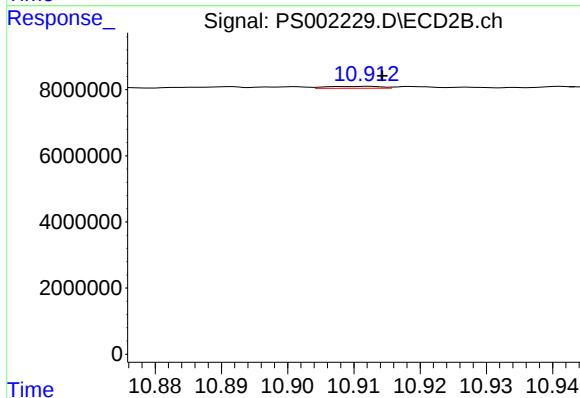


#4 2,4-DCAA

R.T.: 10.912 min
Delta R.T.: -0.002 min
Response: 333718
Conc: 0.93 ng/ml

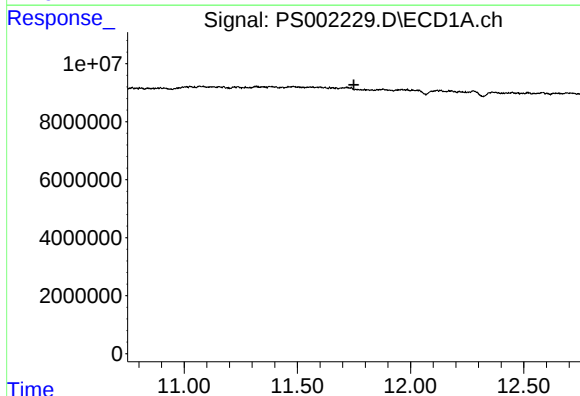


#5 DICAMBA

R.T.: 0.000 min
Exp R.T.: 11.750 min
Response: 0
Conc: N.D.

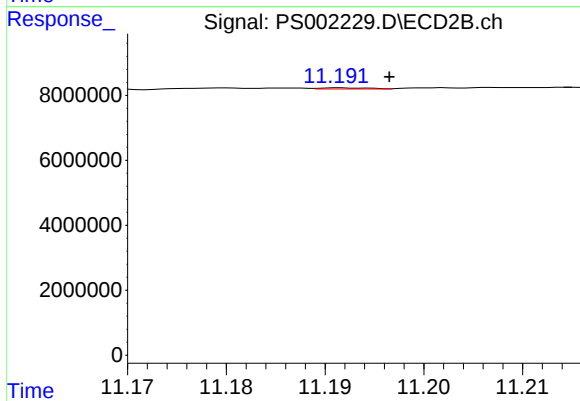

#5 DICAMBA


R.T.: 11.192 min
Delta R.T.: -0.005 min
Response: 121962
Conc: 0.10 ng/ml

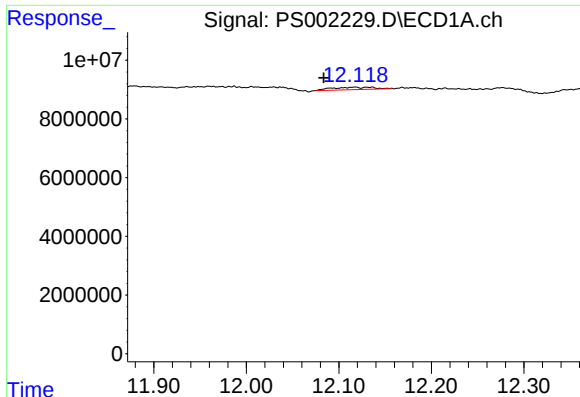

#6 MCPP


R.T.: 12.117 min
Delta R.T.: 0.033 min
Response: 2613728
Conc: 2.65 ug/ml

Instrument :
ECD_S
ClientSampleId :

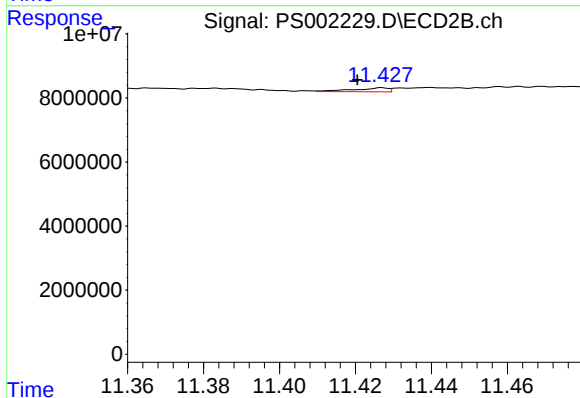


#6 MCPP

R.T.: 11.427 min
Delta R.T.: 0.007 min
Response: 798624
Conc: 0.93 ug/ml

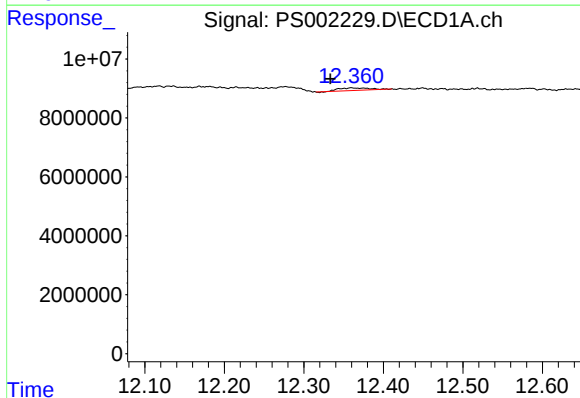


#7 MCPA

R.T.: 12.360 min
Delta R.T.: 0.027 min
Response: 2468475
Conc: 1.64 ug/ml

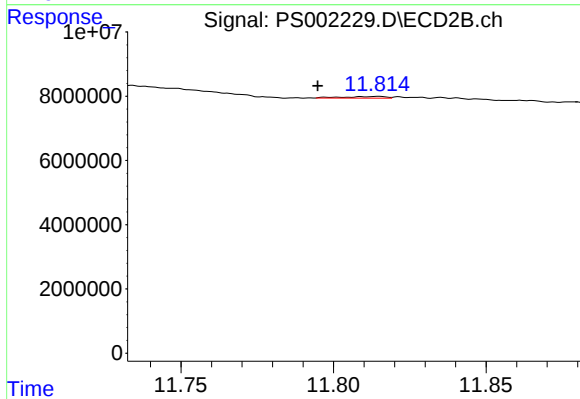

#7 MCPA


R.T.: 11.815 min
Delta R.T.: 0.020 min
Response: 496551
Conc: 0.37 ug/ml

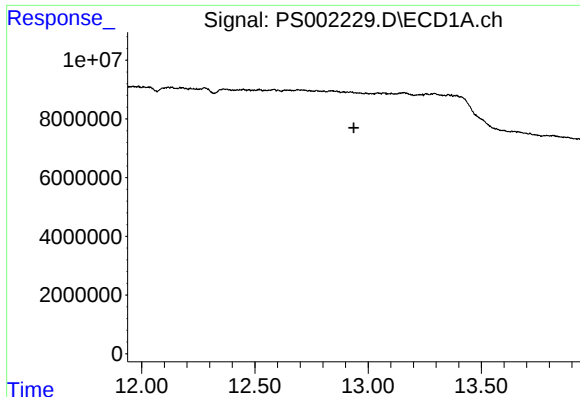

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T. : 12.937 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

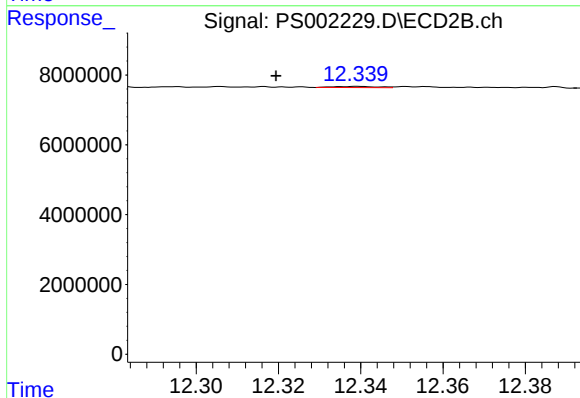


#8 DICHLORPROP

R.T.: 12.339 min
Delta R.T.: 0.020 min
Response: 240700
Conc: 0.75 ng/ml

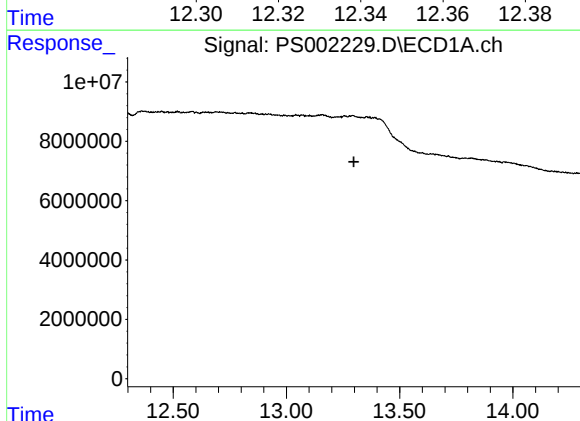


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 13.298 min
Response: 0
Conc: N.D.

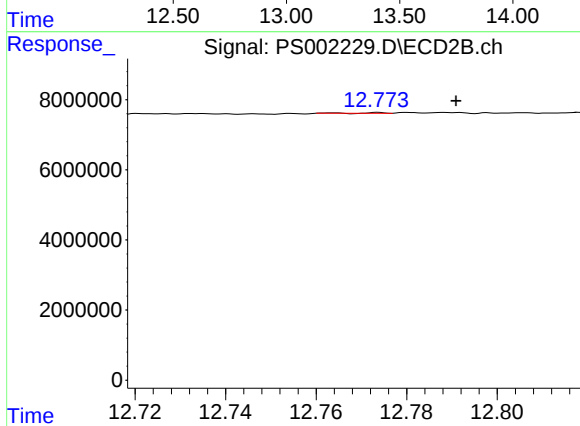

#9 2,4-D


R.T.: 12.774 min
Delta R.T.: -0.017 min
Response: 46509
Conc: 0.11 ng/ml

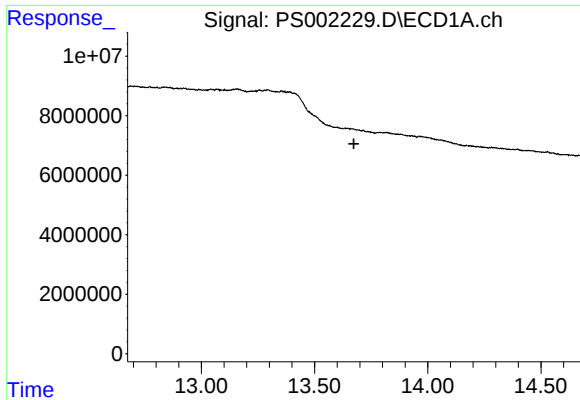

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 13.674 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

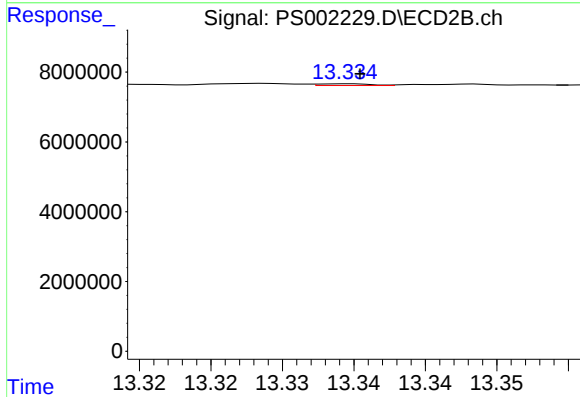


#10 Pentachlorophenol

R.T.: 13.335 min
Delta R.T.: 0.000 min
Response: 128989
Conc: 0.03 ng/ml

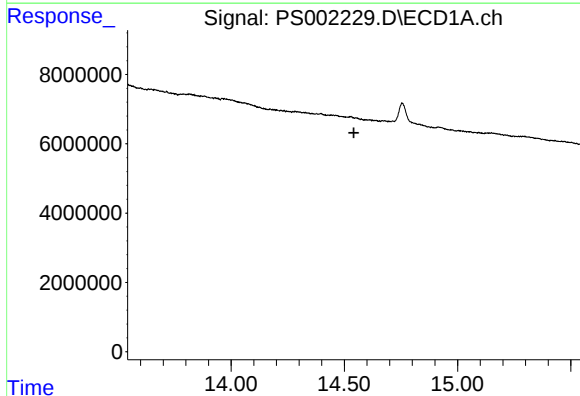


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 14.542 min
Response: 0
Conc: N.D.

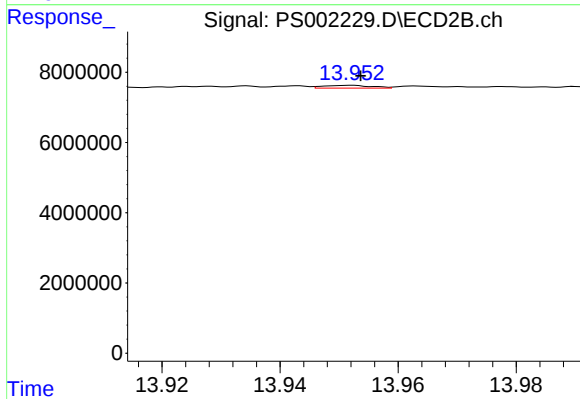

#11 2,4,5-TP (SILVEX)


R.T.: 13.952 min
Delta R.T.: -0.001 min
Response: 446713
Conc: 0.24 ng/ml

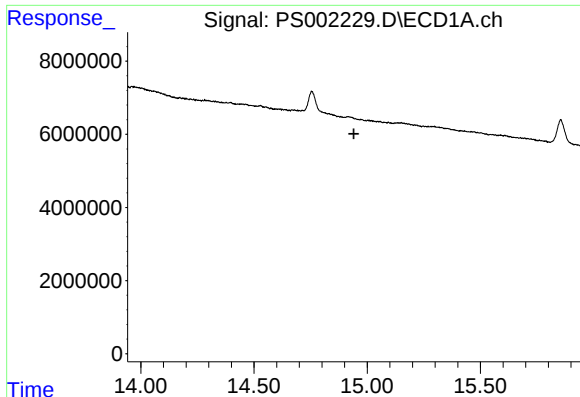

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 14.941 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

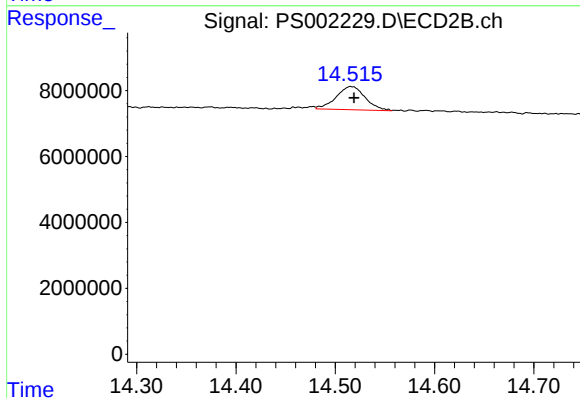


#12 2,4,5-T

R.T.: 14.515 min
Delta R.T.: -0.004 min
Response: 14394952
Conc: 9.61 ng/ml

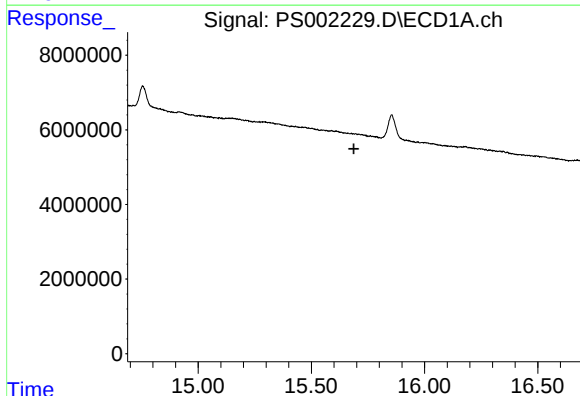


#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 15.688 min
Response: 0
Conc: N.D.

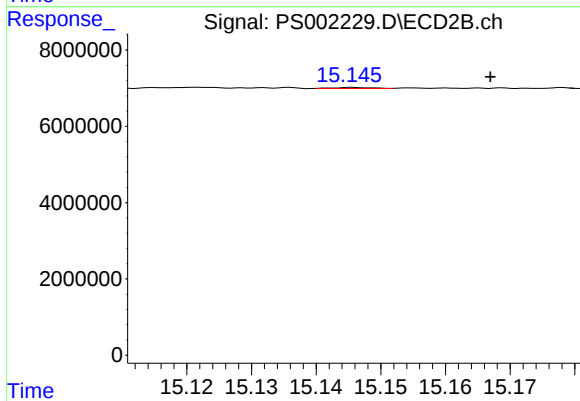

#13 2,4-DB


R.T.: 15.146 min
Delta R.T.: -0.021 min
Response: 117183
Conc: 0.53 ng/ml

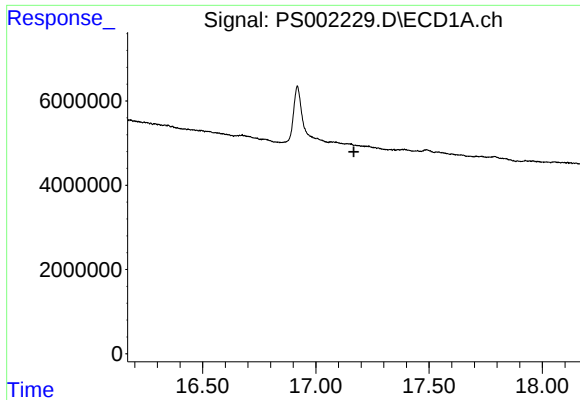

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 17.168 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

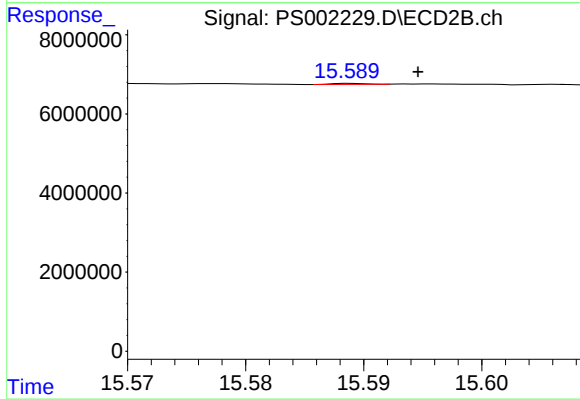


#14 DINOSEB

R.T.: 15.589 min
Delta R.T.: -0.005 min
Response: 43717
Conc: 0.03 ng/ml

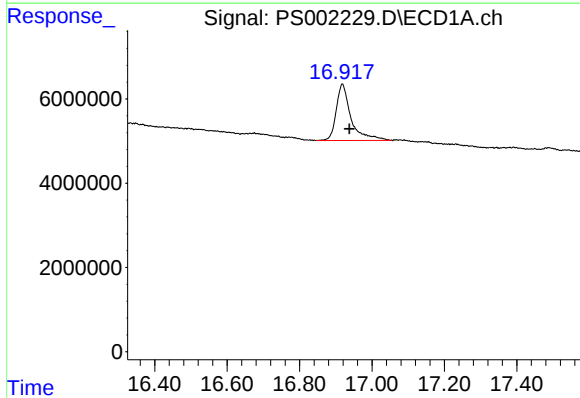


#15 Picloram

R.T.: 16.918 min
Delta R.T.: -0.019 min
Response: 37859081
Conc: 15.87 ng/ml

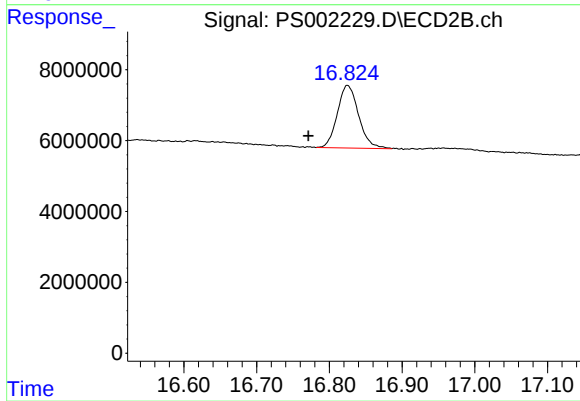

#15 Picloram


R.T.: 16.825 min
Delta R.T.: 0.053 min
Response: 35987396
Conc: 15.91 ng/ml

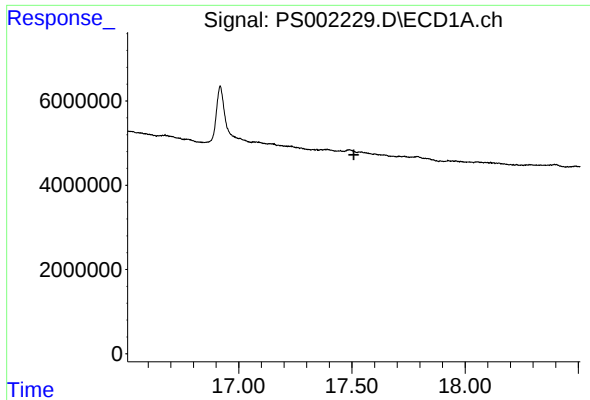

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.509 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

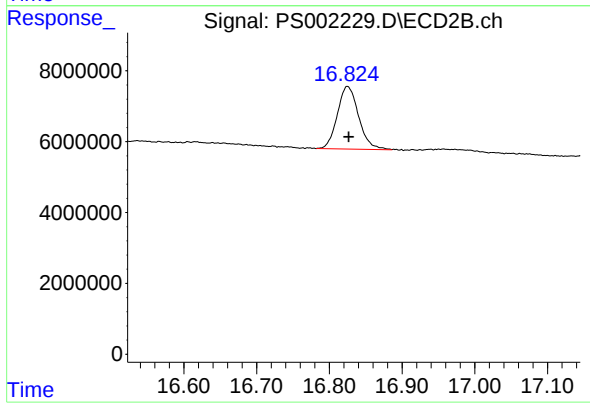

#16 DCPA

R.T.: 16.825 min
Delta R.T.: -0.002 min
Response: 35987396
Conc: 15.20 ng/ml