

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110118\
 Data File : PS002230.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Nov 2018 10:50
 Operator : EI\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 02 03:46:13 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102618.M
 Quant Title : 8080.M
 QLast Update : Sat Oct 27 01:34:10 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.439	10.930	146.8E6	139.4E6	466.644	388.159
Target Compounds							
1) T	Dalapon	0.000	2.369	0	20402	N.D.	0.045 #
7) T	MCPA	0.000	11.795	0	300280	N.D.	0.222 #
9) T	2,4-D	0.000	12.738	0	77406	N.D.	0.182 #
12) T	2,4,5-T	0.000	14.545	0	5299955	N.D.	3.539 #
15) T	Picloram	16.945	16.786	18947840	36581	7.944	0.016 #
16) T	DCPA	0.000	16.849	0	17402154	N.D.	7.349 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110118\
Data File : PS002230.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Nov 2018 10:50
Operator : EI\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 02 03:46:13 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102618.M
Quant Title : 8080.M
QLast Update : Sat Oct 27 01:34:10 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

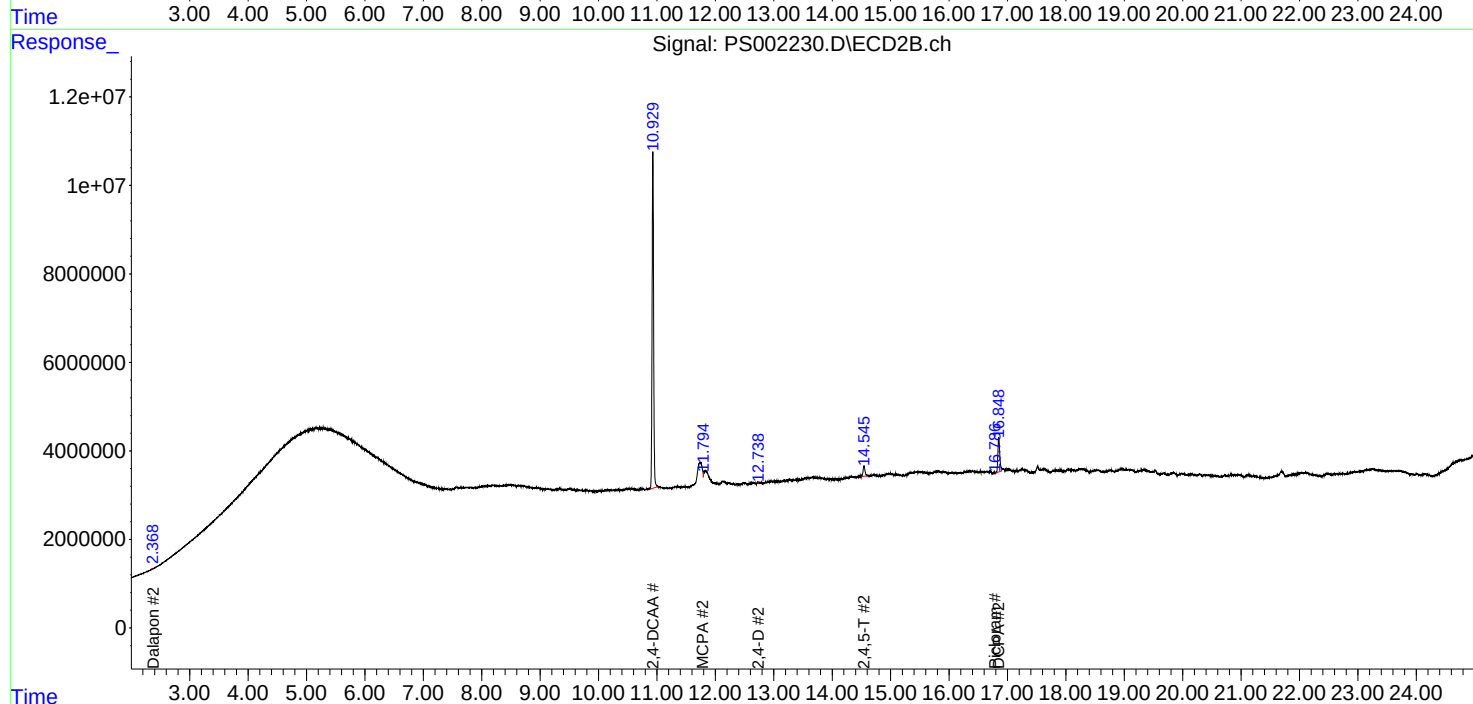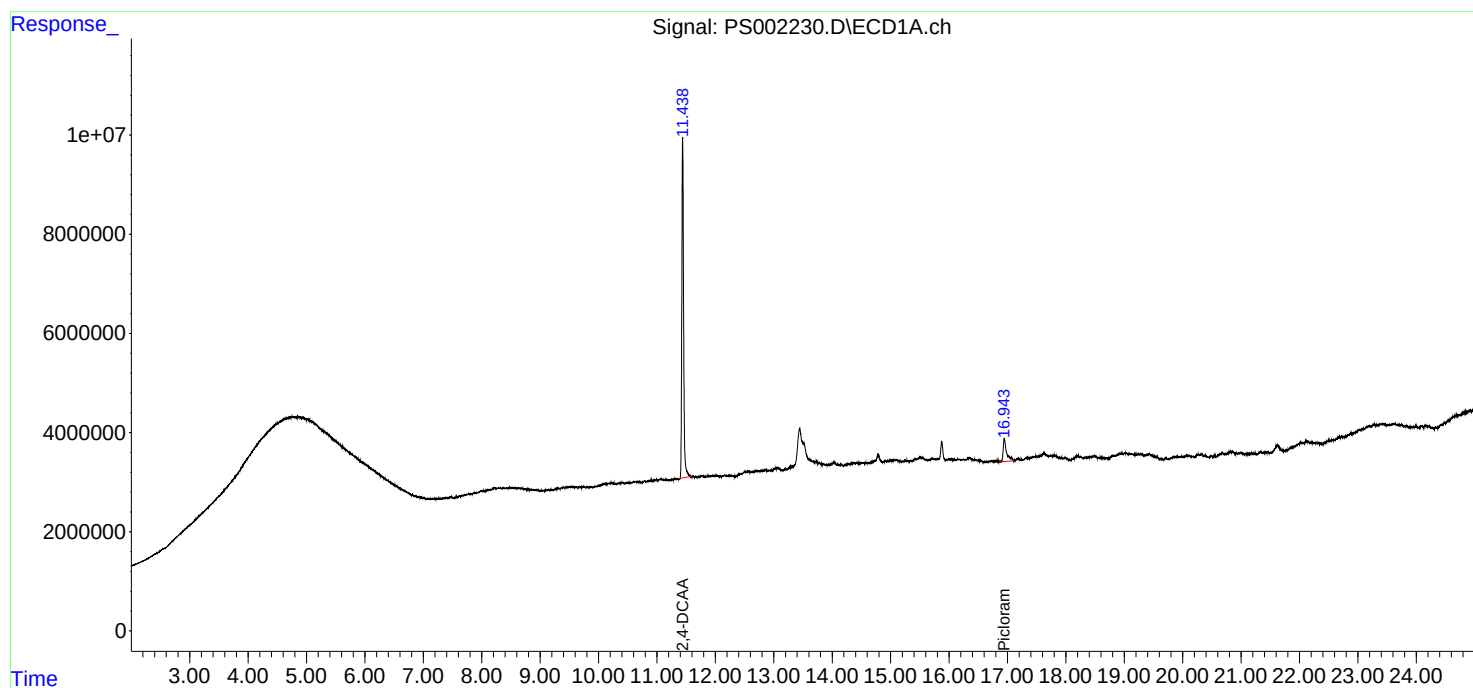


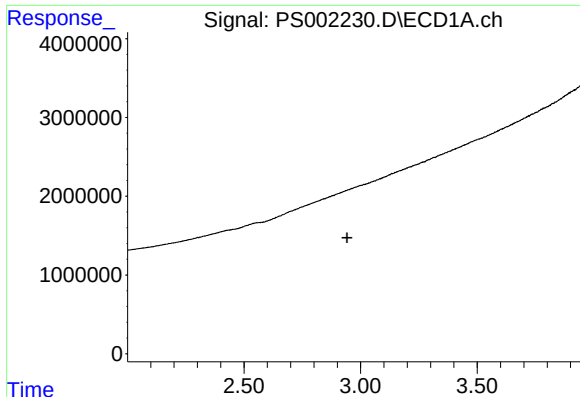

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.942 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

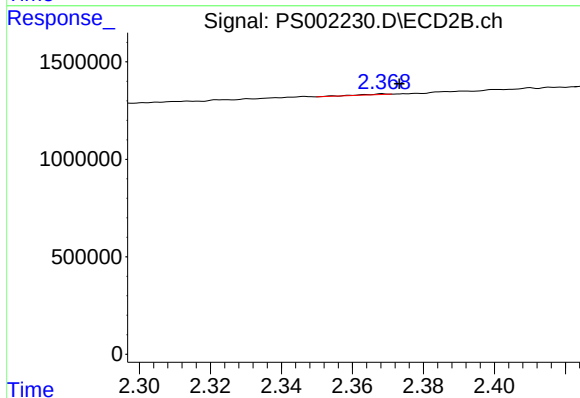


#1 Dalapon

R.T.: 2.369 min
Delta R.T.: -0.005 min
Response: 20402
Conc: 0.05 ng/ml

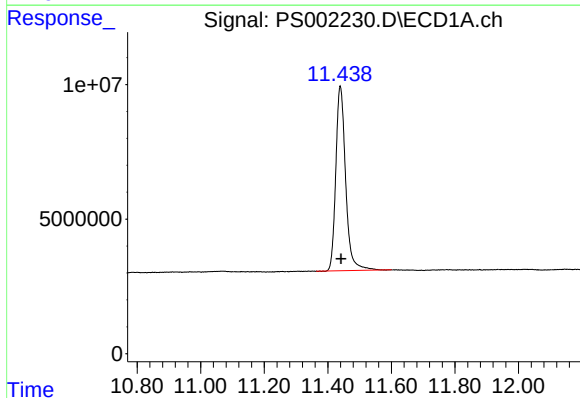


#4 2,4-DCAA

R.T.: 11.439 min
Delta R.T.: -0.002 min
Response: 146846163
Conc: 466.64 ng/ml

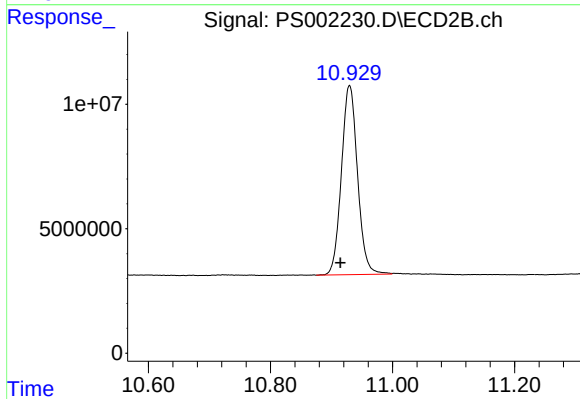

#4 2,4-DCAA


R.T.: 10.930 min
Delta R.T.: 0.015 min
Response: 139386962
Conc: 388.16 ng/ml

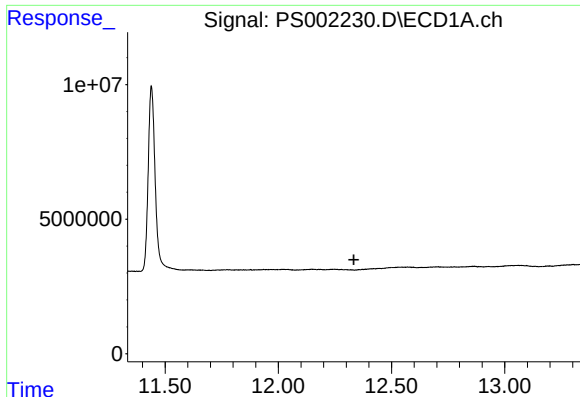

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 12.333 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

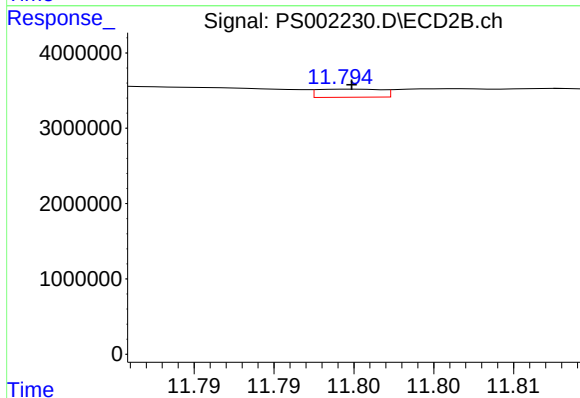


#7 MCPA

R.T.: 11.795 min
Delta R.T.: 0.000 min
Response: 300280
Conc: 0.22 ug/ml

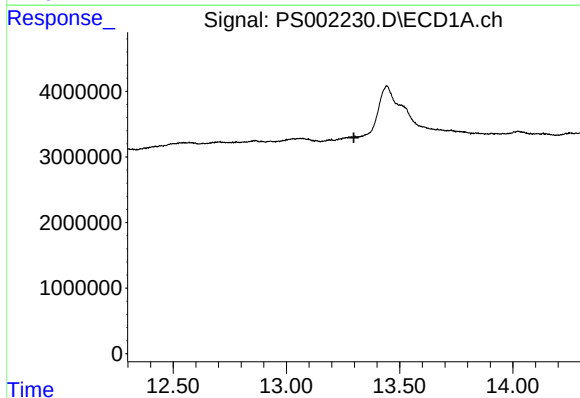


#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 13.298 min
Response: 0
Conc: N.D.

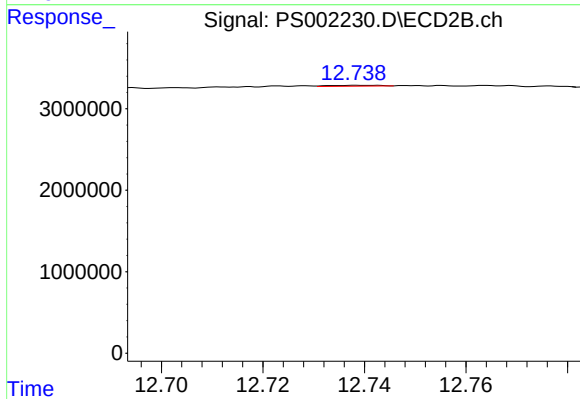

#9 2,4-D


R.T.: 12.738 min
Delta R.T.: -0.053 min
Response: 77406
Conc: 0.18 ng/ml

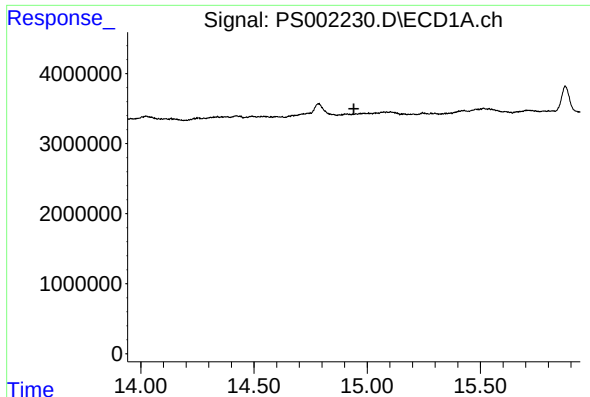

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 14.941 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

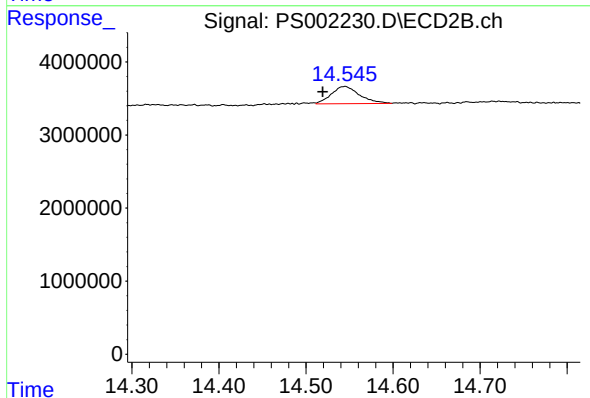


#12 2,4,5-T

R.T.: 14.545 min
Delta R.T.: 0.026 min
Response: 5299955
Conc: 3.54 ng/ml

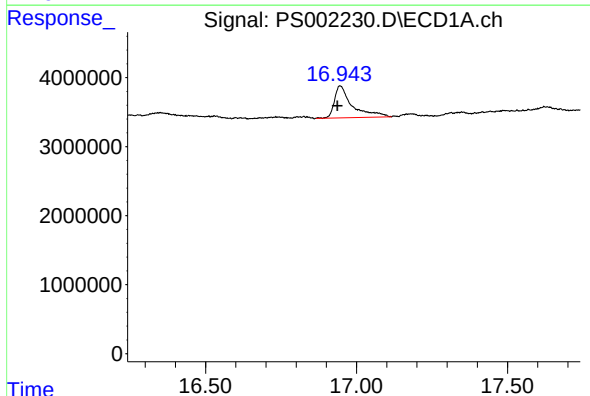


#15 Picloram

R.T.: 16.945 min
Delta R.T.: 0.008 min
Response: 18947840
Conc: 7.94 ng/ml

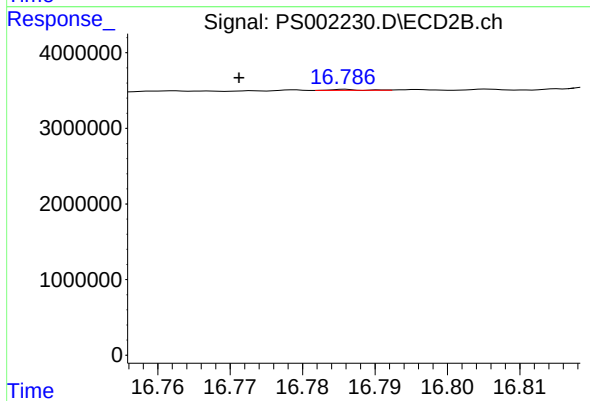

#15 Picloram


R.T.: 16.786 min
Delta R.T.: 0.015 min
Response: 36581
Conc: 0.02 ng/ml

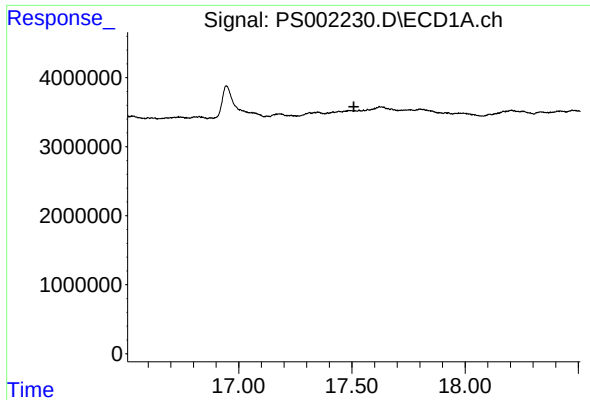

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.509 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

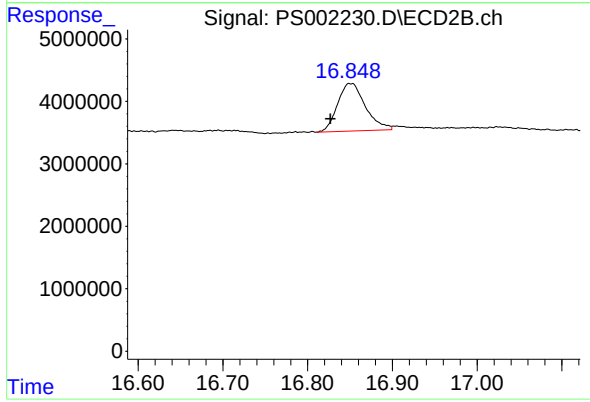

#16 DCPA

R.T.: 16.849 min
Delta R.T.: 0.022 min
Response: 17402154
Conc: 7.35 ng/ml