

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110118\
 Data File : PS002233.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Nov 2018 13:04
 Operator : EI\SJ
 Sample : PB114372BS
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 02 03:47:15 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102618.M
 Quant Title : 8080.M
 QLast Update : Sat Oct 27 01:34:10 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.420	10.910	131.1E6	138.2E6	416.522	384.943
Target Compounds							
1) T	Dalapon	2.935	2.371	148.2E6	192.5E6	323.020	426.407 #
2) T	3,5-DICHL...	0.000	9.065	0	163.0E6	N.D.	367.444 #
3) T	4-Nitroph...	11.012	10.056	66206166	79648642	396.850	446.685
5) T	DICAMBA	11.729	11.194	510.6E6	385.8E6	384.463	308.738
6) T	MCPD	12.069	11.420	6814601	32205835	6.898	37.434 #
7) T	MCPA	12.383	11.795	-39335188	58276846	N.D.	43.059
8) T	DICHLORPROP	12.915	12.317	136.8E6	24137886	392.812	75.165 #
9) T	2,4-D	0.000	12.787	0	144.3E6	N.D.	338.740 #
10) T	Pentachlo...	13.653	13.334	2003.2E6	1866.3E6	416.397	397.295
11) T	2,4,5-TP ...	0.000	13.952	0	804.3E6	N.D.	439.592 #
12) T	2,4,5-T	14.917	14.517	688.4E6	576.9E6	384.086	385.267
13) T	2,4-DB	0.000	15.167	0	74980449	N.D.	338.423 #
14) T	DINOSEB	17.144	15.594	514.6E6	502.4E6	375.638	396.861
15) T	Picloram	16.910	16.772	871.0E6	698.9E6	365.149	308.963
16) T	DCPA	0.000	16.826	0	928.3E6	N.D.	392.057 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110118\
Data File : PS002233.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Nov 2018 13:04
Operator : EI\SJ
Sample : PB114372BS
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 02 03:47:15 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102618.M
Quant Title : 8080.M
QLast Update : Sat Oct 27 01:34:10 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

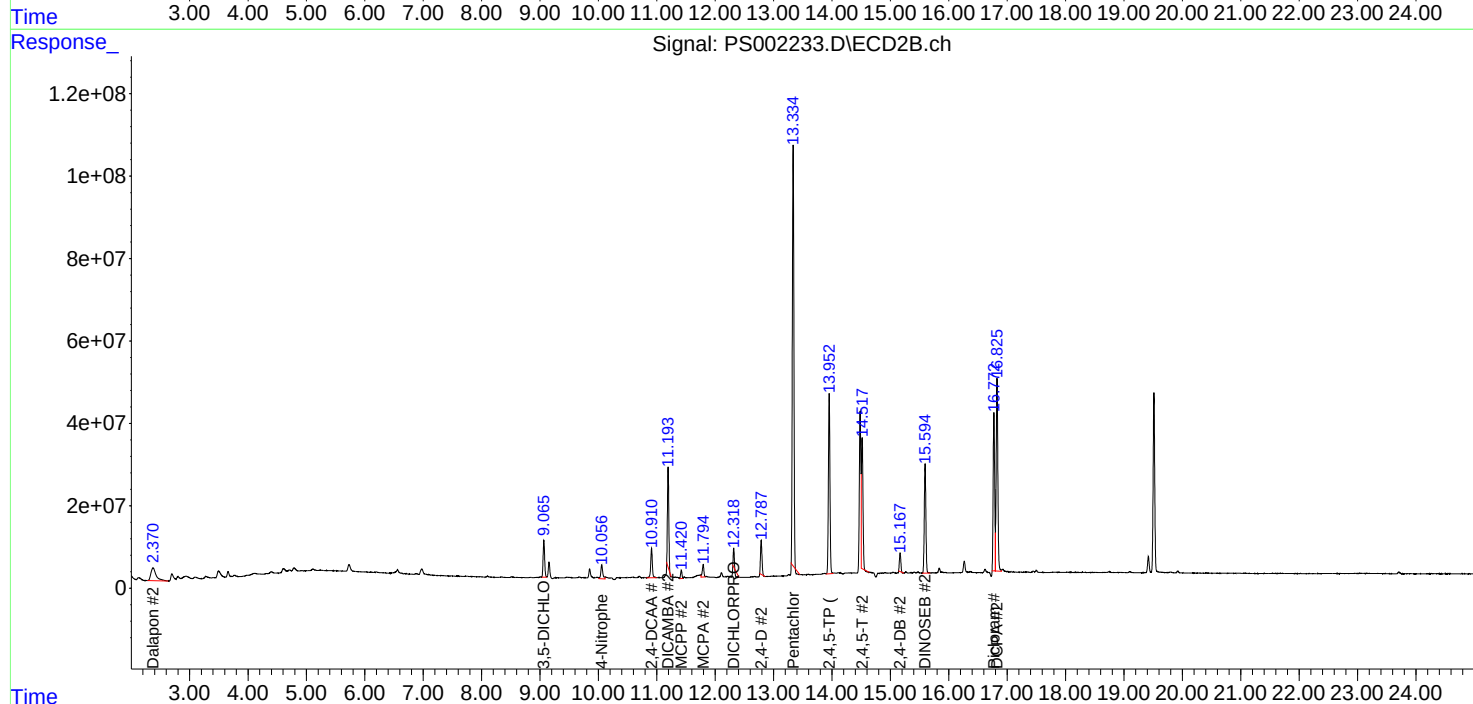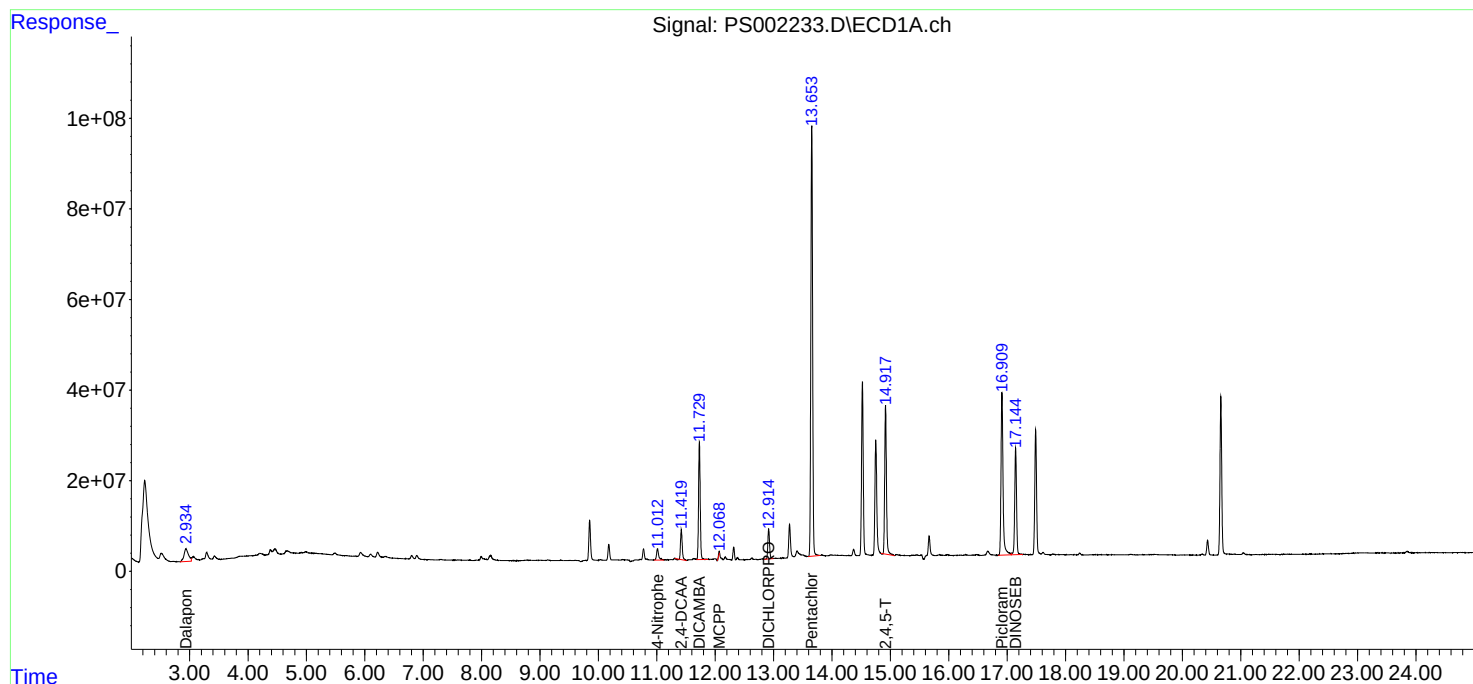


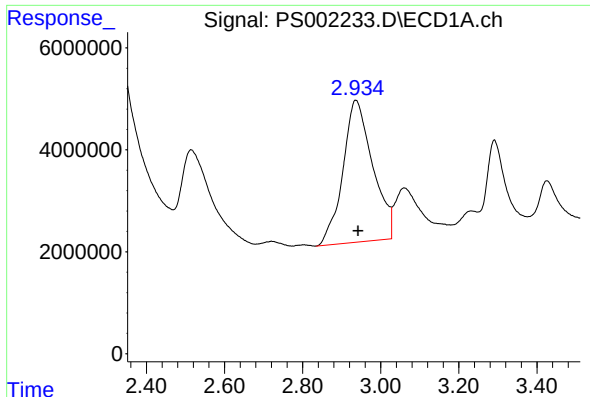

#1 Dalapon


R.T.: 2.935 min
Delta R.T.: -0.007 min
Response: 148158595
Conc: 323.02 ng/ml

Instrument :
ECD_S
ClientSampleId :

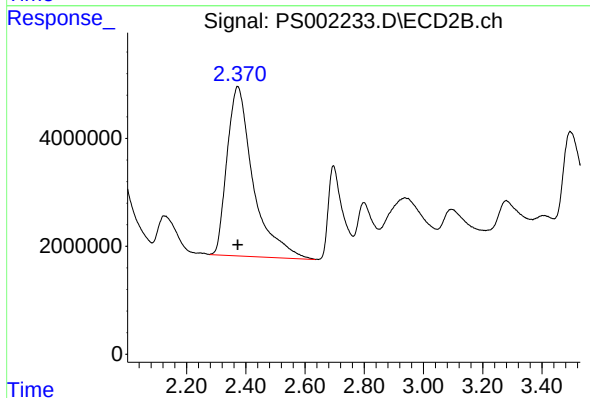


#1 Dalapon

R.T.: 2.371 min
Delta R.T.: -0.002 min
Response: 192525918
Conc: 426.41 ng/ml

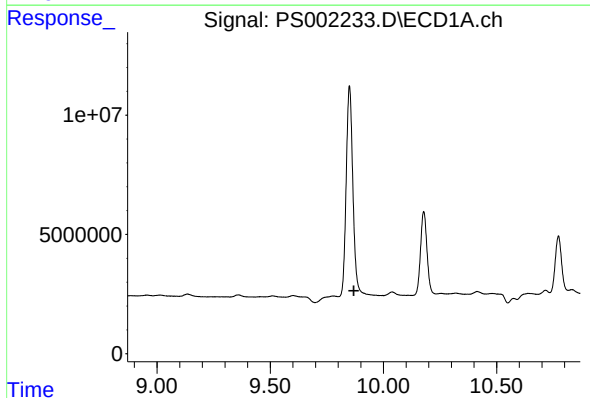


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.870 min
Response: 0
Conc: N.D.

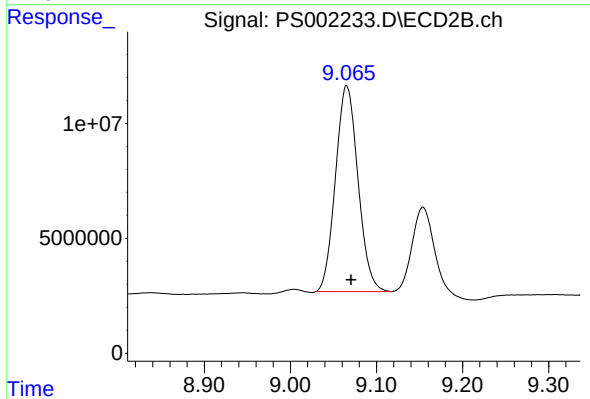

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.065 min
Delta R.T.: -0.005 min
Response: 162981400
Conc: 367.44 ng/ml

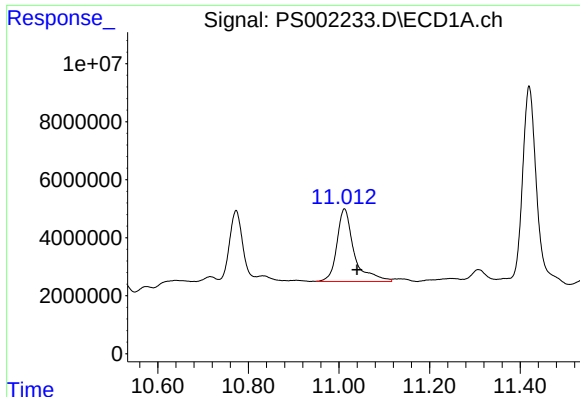

#3 4-Nitrophenol


R.T.: 11.012 min
Delta R.T.: -0.028 min
Response: 66206166
Conc: 396.85 ng/ml

Instrument :
ECD_S
ClientSampleId :

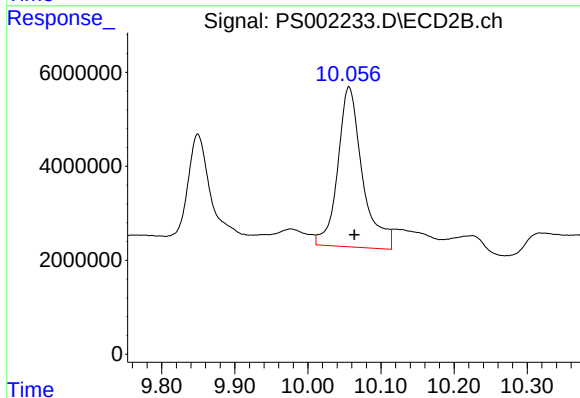


#3 4-Nitrophenol

R.T.: 10.056 min
Delta R.T.: -0.008 min
Response: 79648642
Conc: 446.68 ng/ml

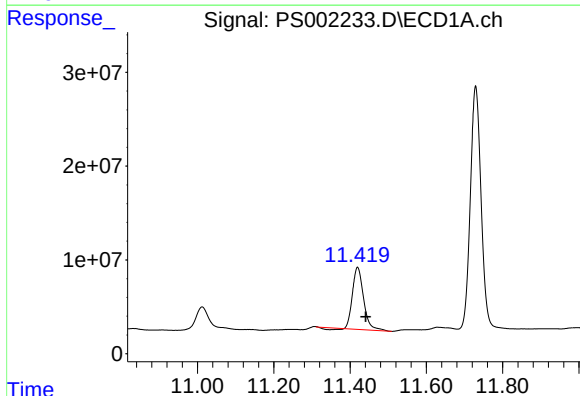


#4 2,4-DCAA

R.T.: 11.420 min
Delta R.T.: -0.021 min
Response: 131073479
Conc: 416.52 ng/ml

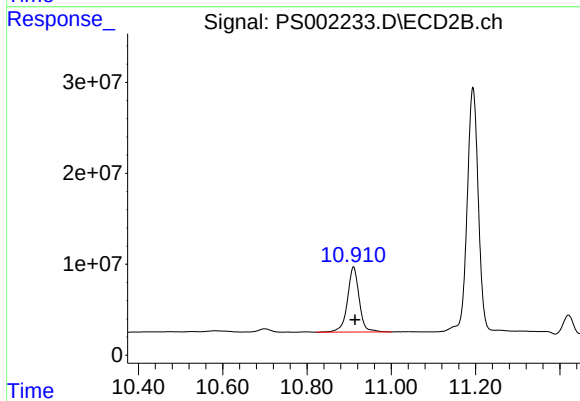

#4 2,4-DCAA


R.T.: 10.910 min
Delta R.T.: -0.004 min
Response: 138232273
Conc: 384.94 ng/ml

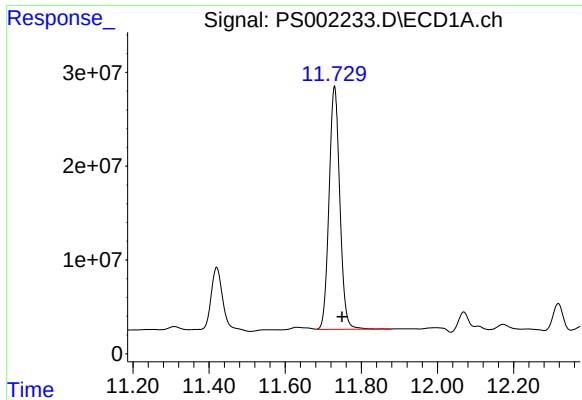

#5 DICAMBA


R.T.: 11.729 min
Delta R.T.: -0.020 min
Response: 510574172
Conc: 384.46 ng/ml

Instrument :
ECD_S
ClientSampleId :

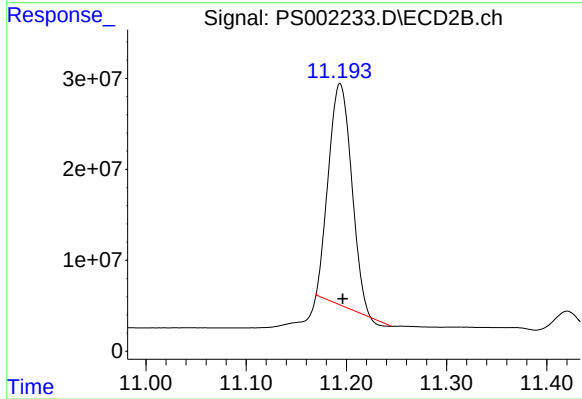


#5 DICAMBA

R.T.: 11.194 min
Delta R.T.: -0.003 min
Response: 385829531
Conc: 308.74 ng/ml

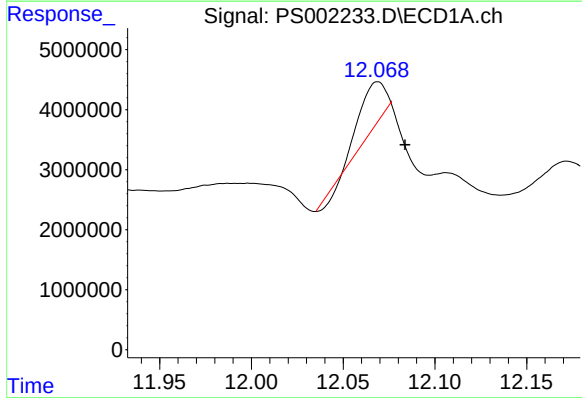


#6 MCP

R.T.: 12.069 min
Delta R.T.: -0.015 min
Response: 6814601
Conc: 6.90 ug/ml

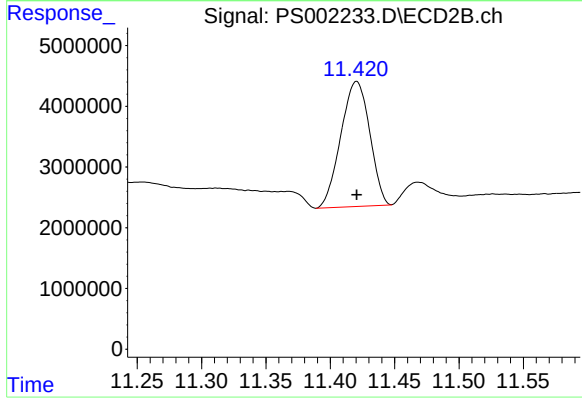

#6 MCP


R.T.: 11.420 min
Delta R.T.: 0.000 min
Response: 32205835
Conc: 37.43 ug/ml

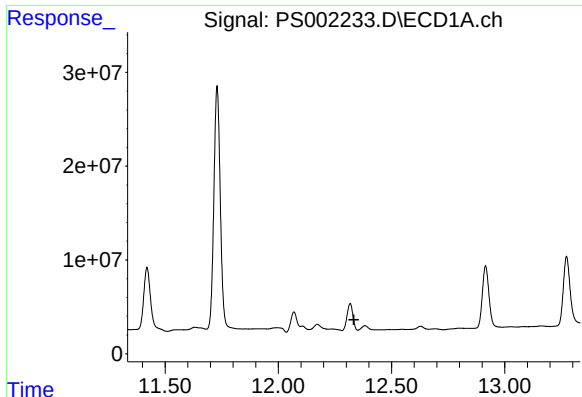

#7 MCPA


R.T.: 12.383 min
Delta R.T.: 0.049 min
Response: -39335188
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

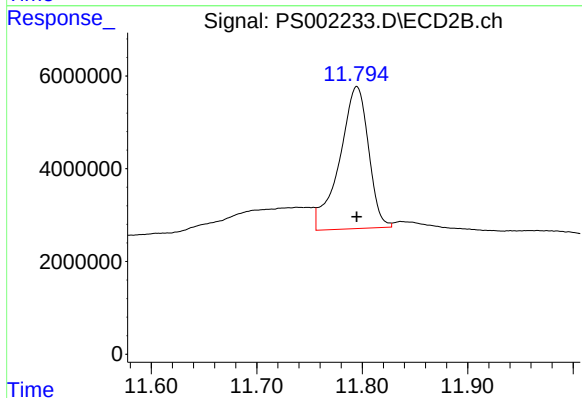


#7 MCPA

R.T.: 11.795 min
Delta R.T.: 0.000 min
Response: 58276846
Conc: 43.06 ug/ml

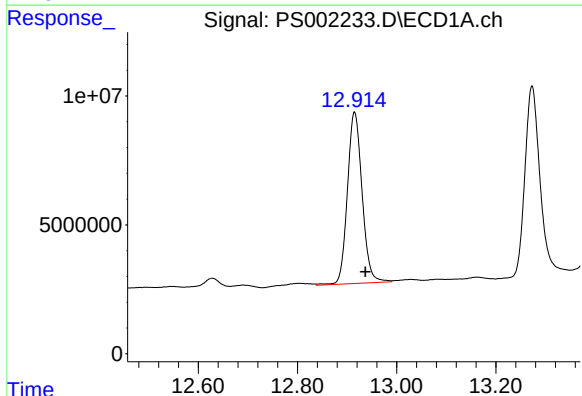


#8 DICHLORPROP

R.T.: 12.915 min
Delta R.T.: -0.022 min
Response: 136797898
Conc: 392.81 ng/ml

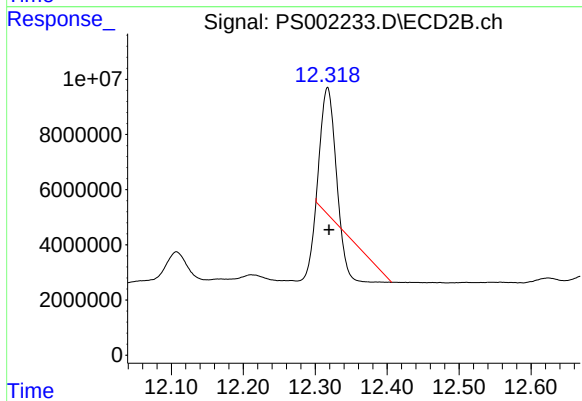

#8 DICHLORPROP


R.T.: 12.317 min
Delta R.T.: -0.002 min
Response: 24137886
Conc: 75.16 ng/ml

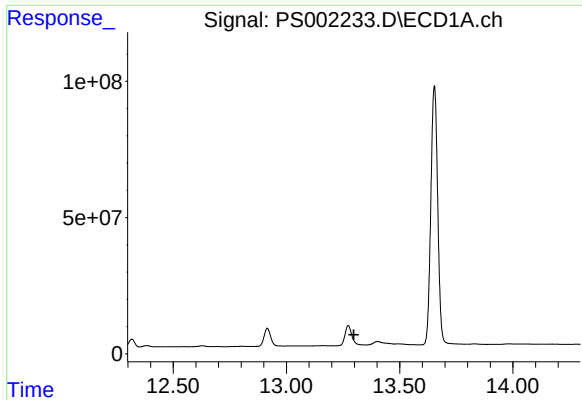

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 13.298 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

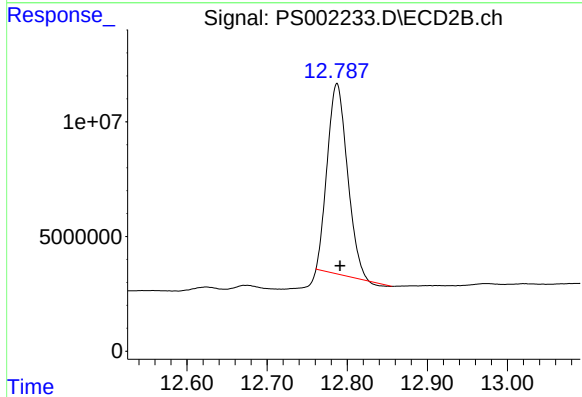


#9 2,4-D

R.T.: 12.787 min
Delta R.T.: -0.004 min
Response: 144267139
Conc: 338.74 ng/ml

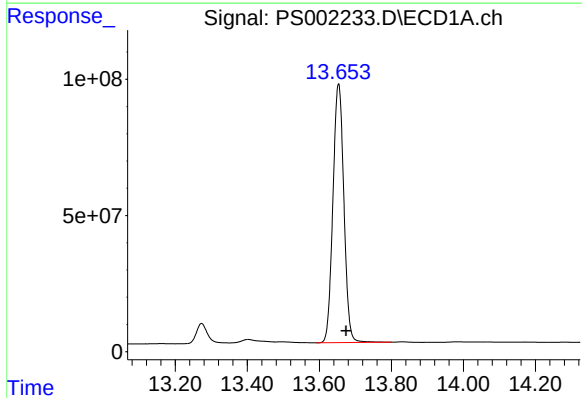


#10 Pentachlorophenol

R.T.: 13.653 min
Delta R.T.: -0.021 min
Response: 2003153119
Conc: 416.40 ng/ml

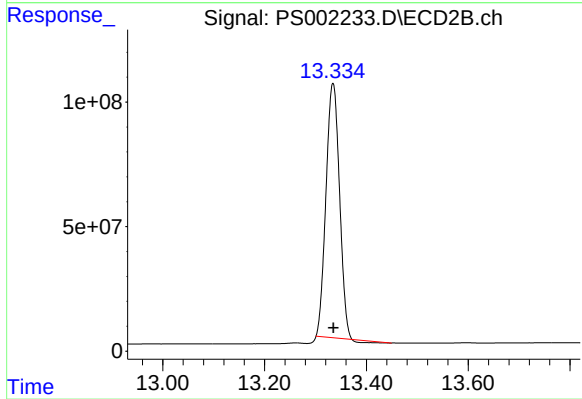

#10 Pentachlorophenol


R.T.: 13.334 min
Delta R.T.: -0.001 min
Response: 1866267738
Conc: 397.29 ng/ml

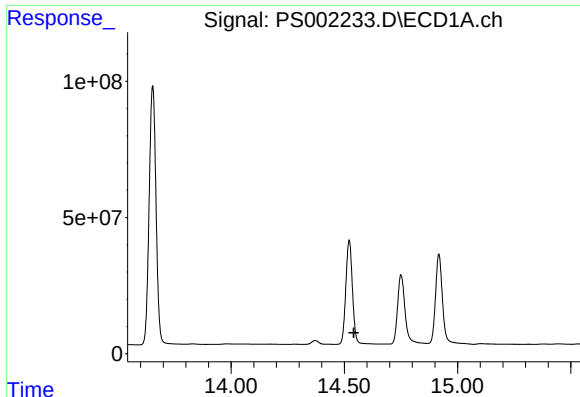

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 14.542 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

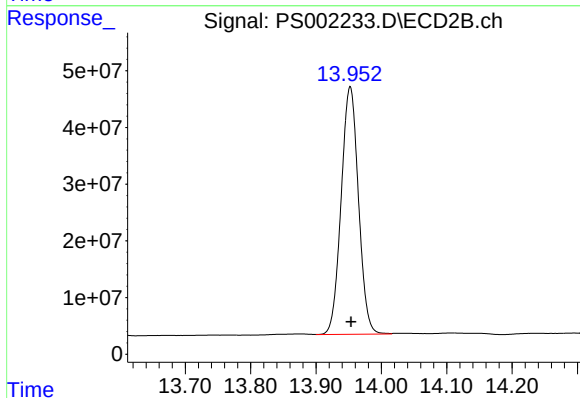


#11 2,4,5-TP (SILVEX)

R.T.: 13.952 min
Delta R.T.: -0.001 min
Response: 804262470
Conc: 439.59 ng/ml

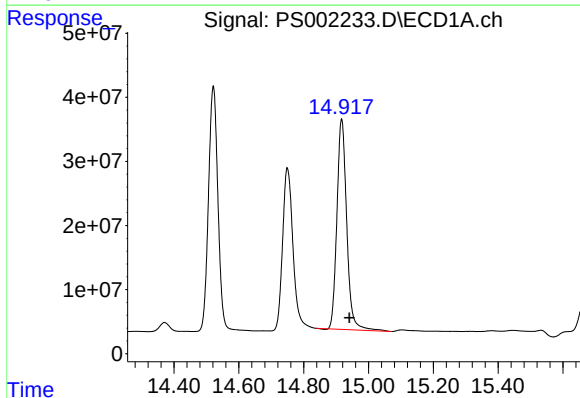


#12 2,4,5-T

R.T.: 14.917 min
Delta R.T.: -0.024 min
Response: 688380473
Conc: 384.09 ng/ml

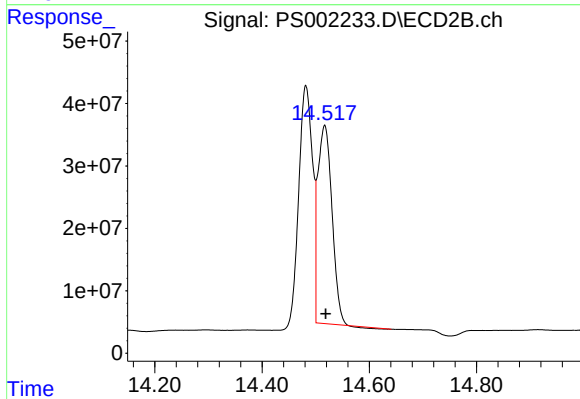

#12 2,4,5-T


R.T.: 14.517 min
Delta R.T.: -0.002 min
Response: 576929094
Conc: 385.27 ng/ml

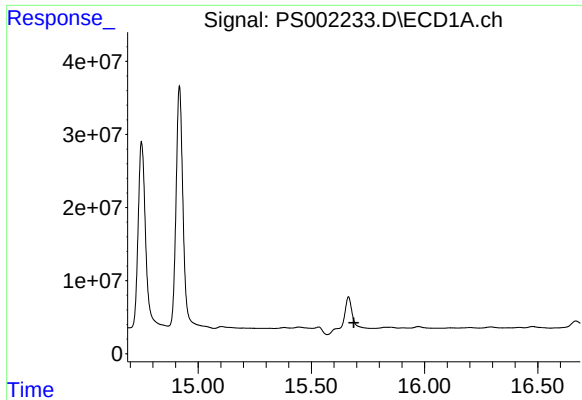

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 15.688 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

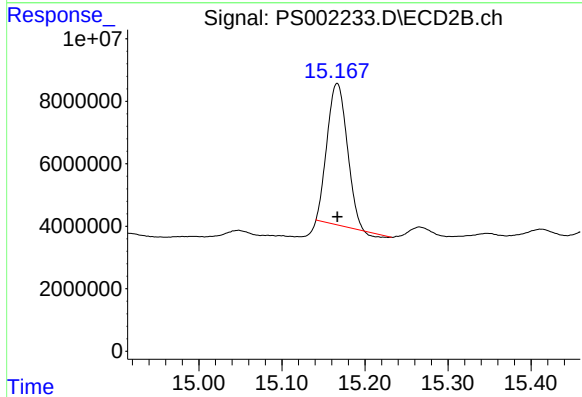


#13 2,4-DB

R.T.: 15.167 min
Delta R.T.: 0.000 min
Response: 74980449
Conc: 338.42 ng/ml

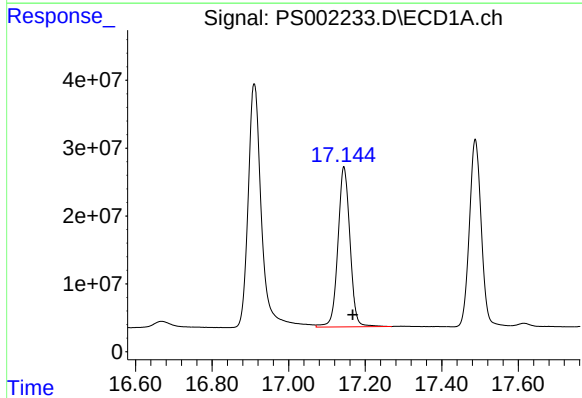


#14 DINOSEB

R.T.: 17.144 min
Delta R.T.: -0.023 min
Response: 514642928
Conc: 375.64 ng/ml

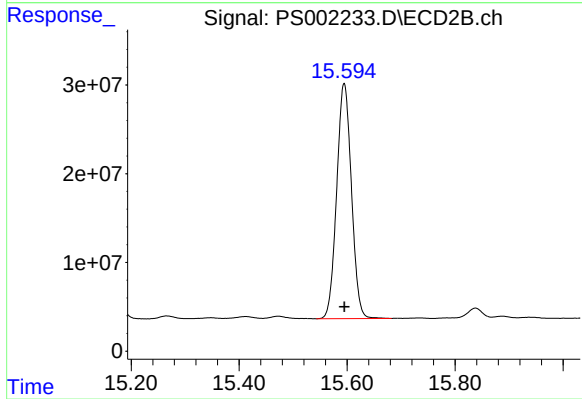

#14 DINOSEB


R.T.: 15.594 min
Delta R.T.: 0.000 min
Response: 502373749
Conc: 396.86 ng/ml

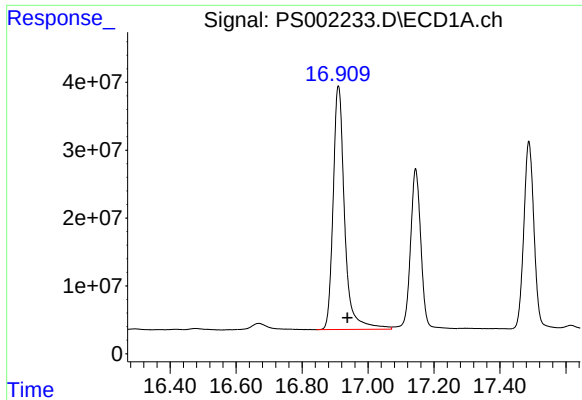

#15 Picloram


R.T.: 16.910 min
Delta R.T.: -0.027 min
Response: 870987260
Conc: 365.15 ng/ml

Instrument :
ECD_S
ClientSampleId :

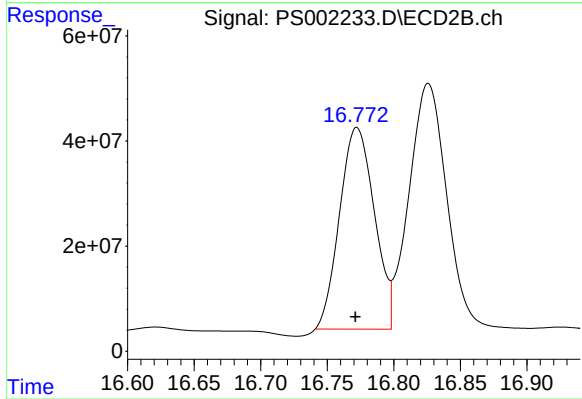


#15 Picloram

R.T.: 16.772 min
Delta R.T.: 0.000 min
Response: 698942274
Conc: 308.96 ng/ml

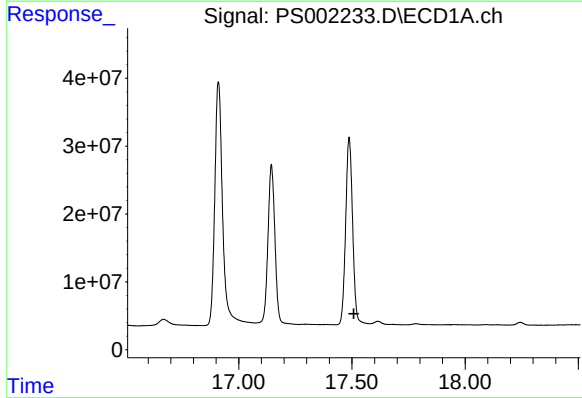

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.509 min
Response: 0
Conc: N.D.

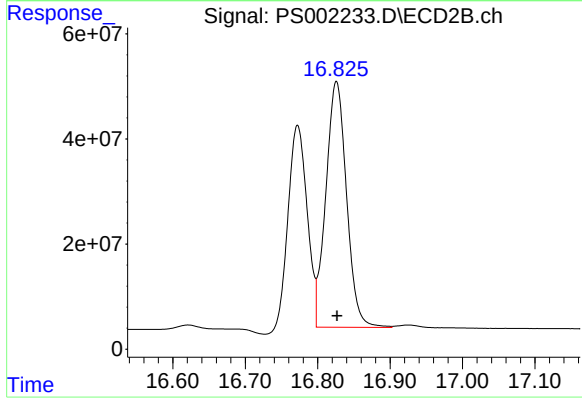

#16 DCPA

R.T.: 16.826 min
Delta R.T.: 0.000 min
Response: 928337951
Conc: 392.06 ng/ml