

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110118\
 Data File : PS002244.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Nov 2018 18:46
 Operator : EI\SJ
 Sample : J5205-10
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 02 03:51:02 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102618.M
 Quant Title : 8080.M
 QLast Update : Sat Oct 27 01:34:10 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.449	10.940	118.6E6	109.0E6	376.909	303.478
Target Compounds							
1) T	Dalapon	2.920	2.368	25389251	45428610	55.354	100.616 #
2) T	3,5-DICHL...	0.000	9.102	0	2595519	N.D.	5.852 #
3) T	4-Nitroph...	11.100	10.099	6046760	4752390	36.245	26.652 #
5) T	DICAMBA	0.000	11.181	0	1090353	N.D.	0.872 #
6) T	MCPD	12.129	0.000	12101342	0	12.250	N.D. #
7) T	MCPA	0.000	11.844	0	1230248	N.D.	0.909 #
8) T	DICHLORPROP	0.000	12.295	0	81697	N.D.	0.254 #
9) T	2,4-D	0.000	12.809	0	1922134	N.D.	4.513 #
11) T	2,4,5-TP ...	0.000	13.905	0	12594038	N.D.	6.884 #
12) T	2,4,5-T	0.000	14.550	0	9004248	N.D.	6.013 #
15) T	Picloram	16.945	16.715	39594500	2609796	16.599	1.154 #
16) T	DCPA	0.000	16.856	0	50177819	N.D.	21.191 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110118\
Data File : PS002244.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Nov 2018 18:46
Operator : EI\SJ
Sample : J5205-10
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 02 03:51:02 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102618.M
Quant Title : 8080.M
QLast Update : Sat Oct 27 01:34:10 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

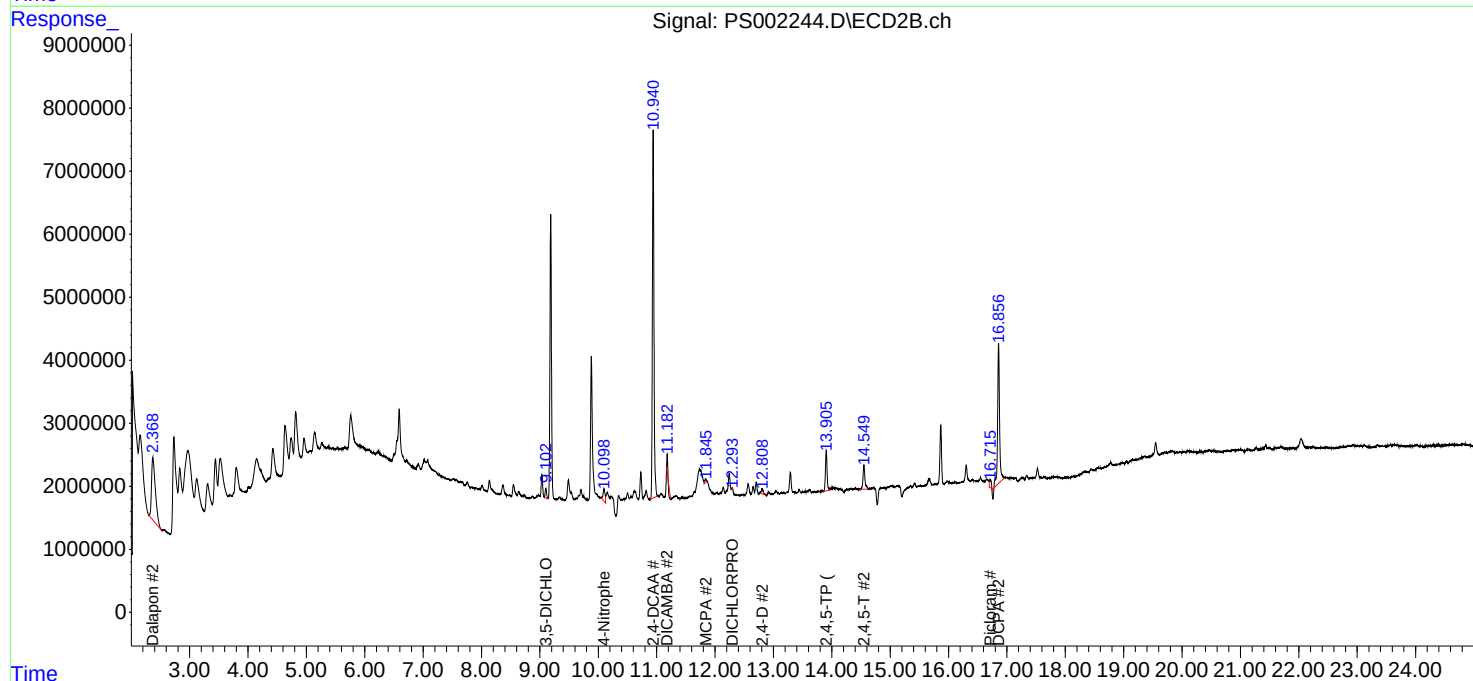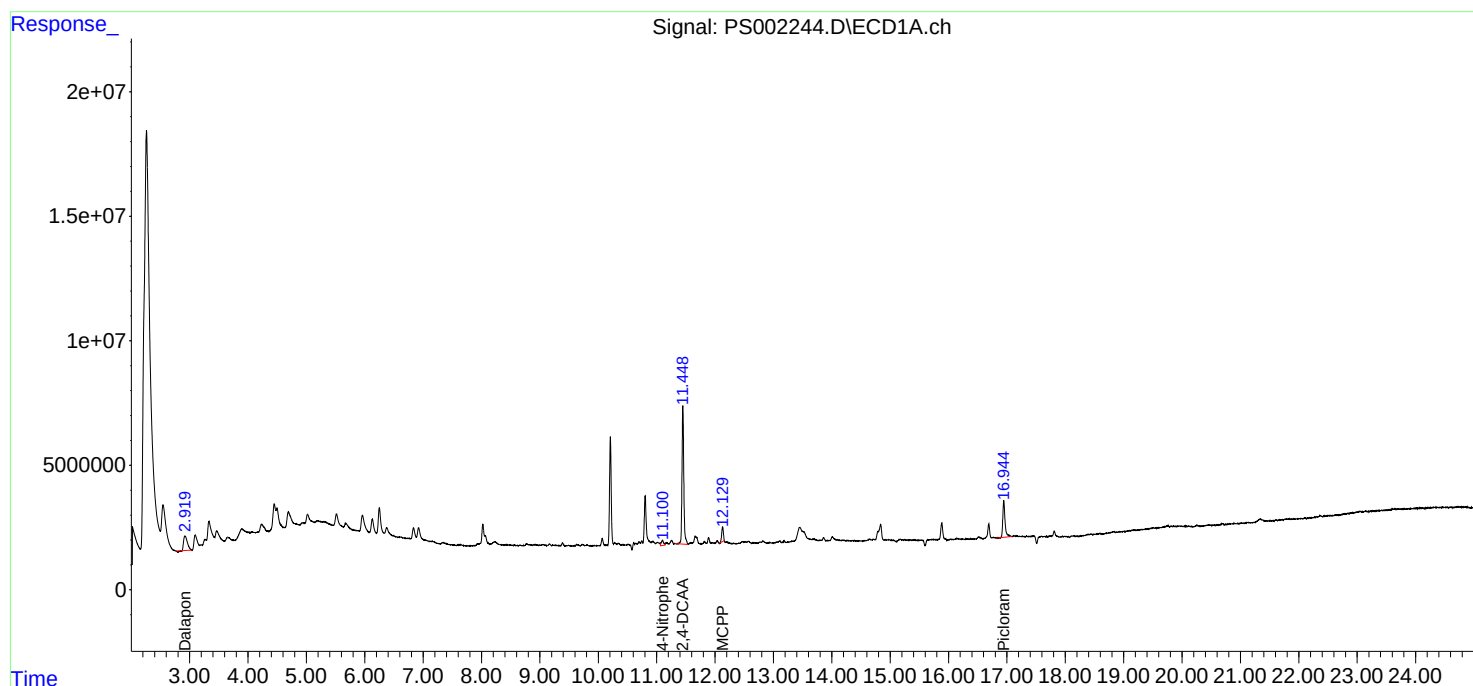


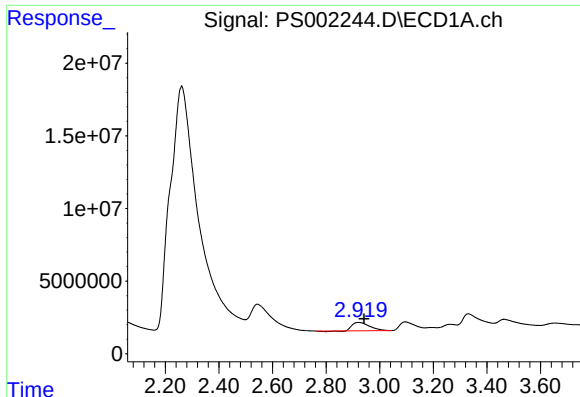

#1 Dalapon


R.T.: 2.920 min
Delta R.T.: -0.022 min
Response: 25389251
Conc: 55.35 ng/ml

Instrument :
ECD_S
ClientSampleId :

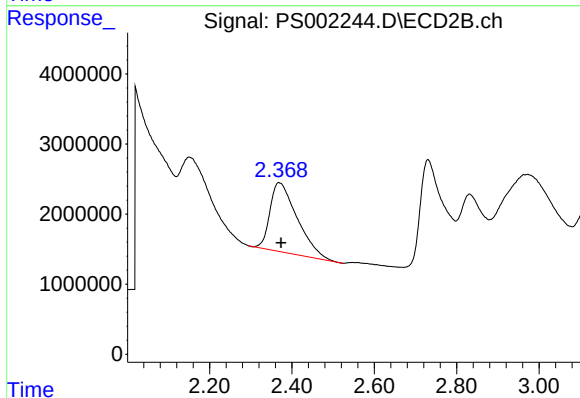


#1 Dalapon

R.T.: 2.368 min
Delta R.T.: -0.005 min
Response: 45428610
Conc: 100.62 ng/ml

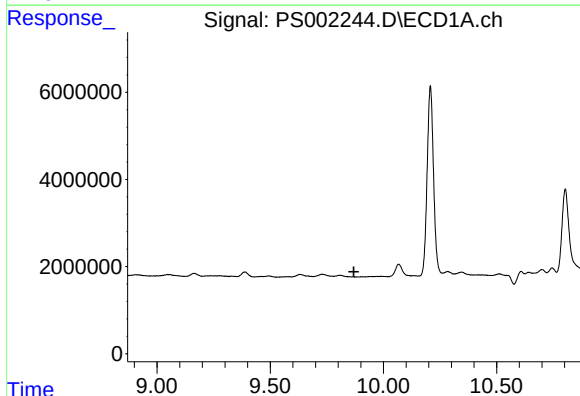


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.870 min
Response: 0
Conc: N.D.

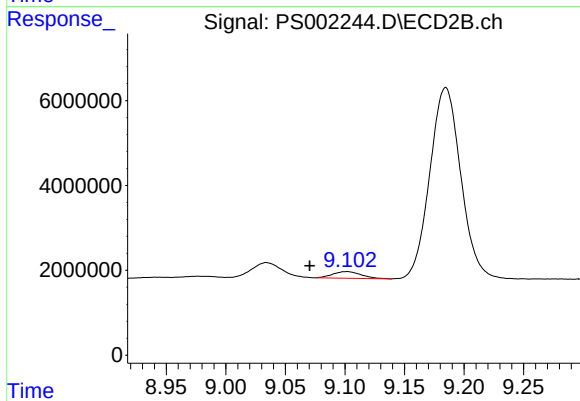

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.102 min
Delta R.T.: 0.032 min
Response: 2595519
Conc: 5.85 ng/ml

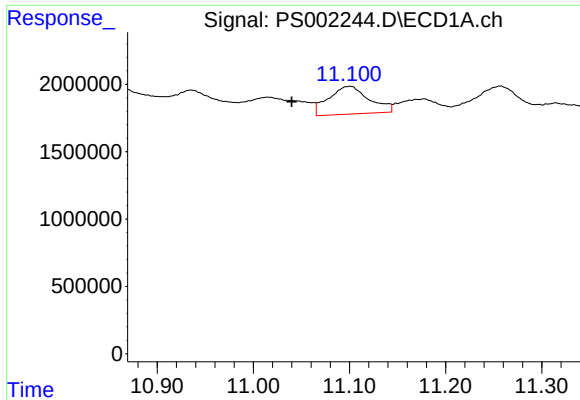

#3 4-Nitrophenol


R.T.: 11.100 min
Delta R.T.: 0.060 min
Response: 6046760
Conc: 36.25 ng/ml

Instrument :
ECD_S
ClientSampleId :

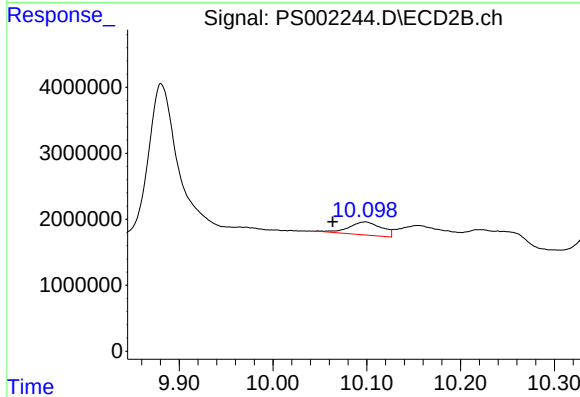


#3 4-Nitrophenol

R.T.: 10.099 min
Delta R.T.: 0.035 min
Response: 4752390
Conc: 26.65 ng/ml

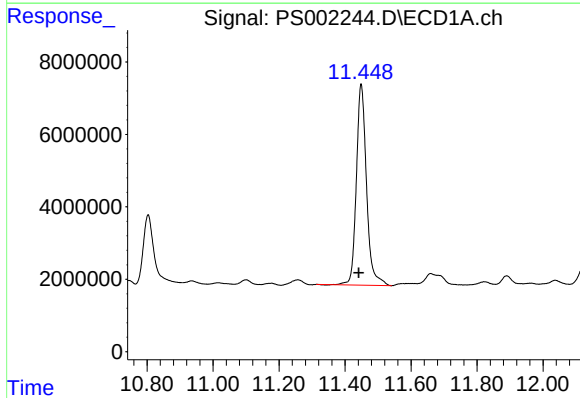


#4 2,4-DCAA

R.T.: 11.449 min
Delta R.T.: 0.008 min
Response: 118607939
Conc: 376.91 ng/ml

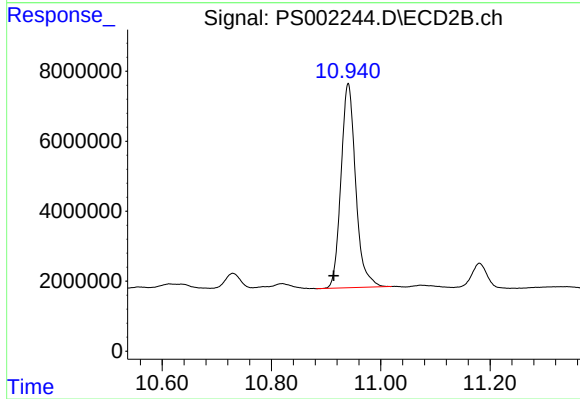

#4 2,4-DCAA


R.T.: 10.940 min
Delta R.T.: 0.026 min
Response: 108978423
Conc: 303.48 ng/ml

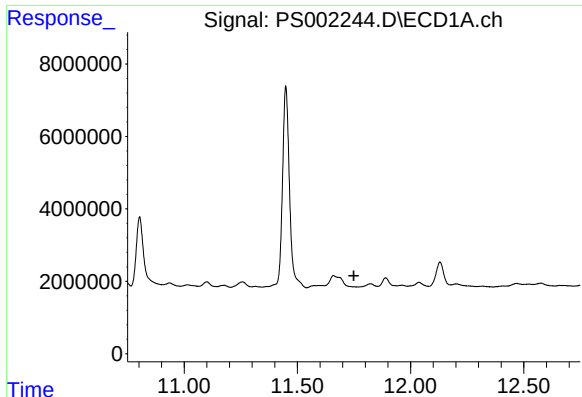

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.750 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

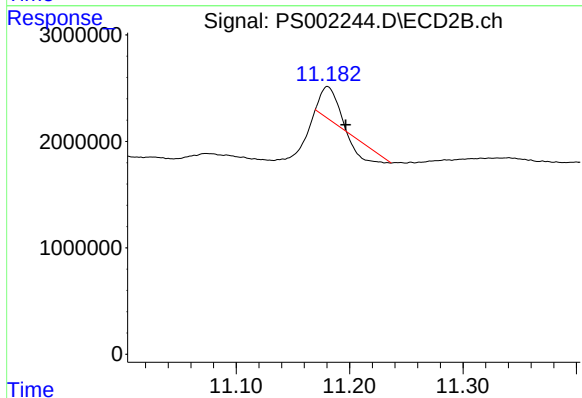


#5 DICAMBA

R.T.: 11.181 min
Delta R.T.: -0.016 min
Response: 1090353
Conc: 0.87 ng/ml

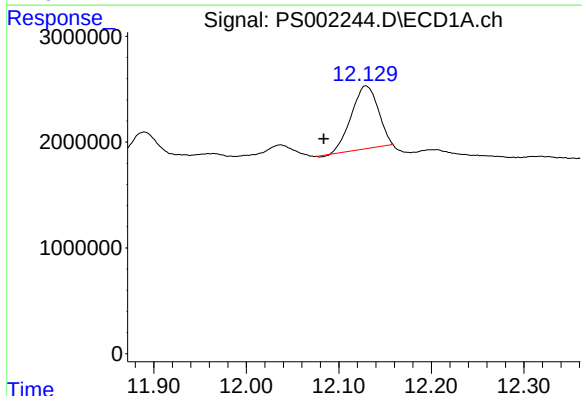


#6 MCP

R.T.: 12.129 min
Delta R.T.: 0.046 min
Response: 12101342
Conc: 12.25 ug/ml

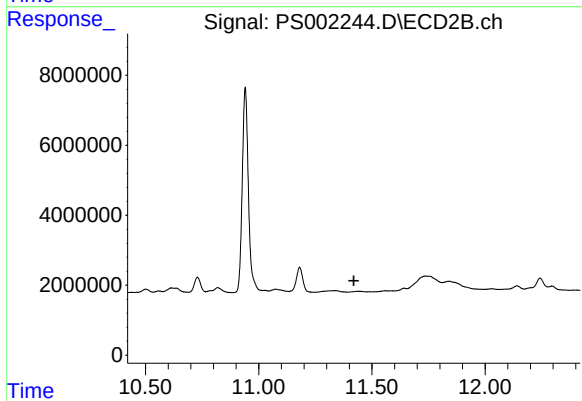

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.420 min
Response: 0
Conc: N.D.

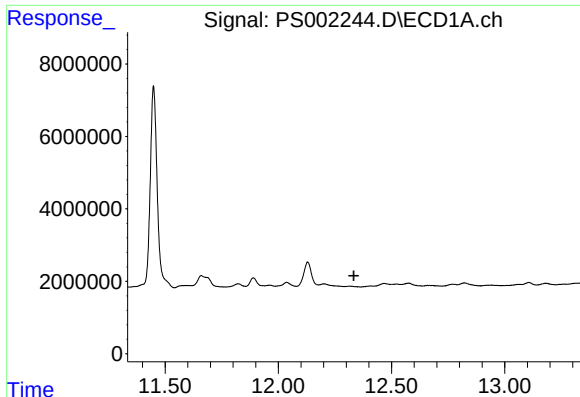

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 12.333 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

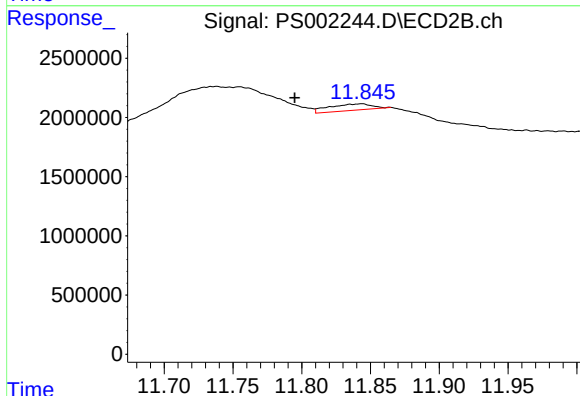


#7 MCPA

R.T.: 11.844 min
Delta R.T.: 0.049 min
Response: 1230248
Conc: 0.91 ug/ml

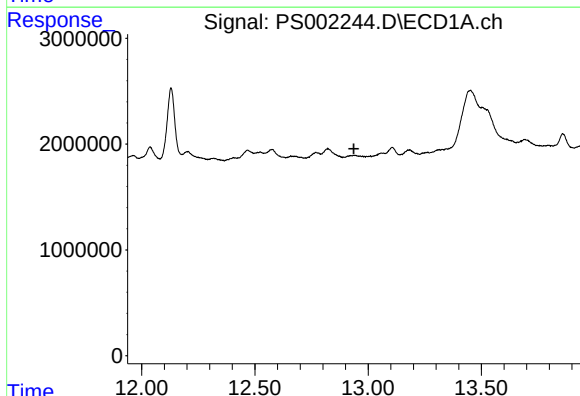


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 12.937 min
Response: 0
Conc: N.D.

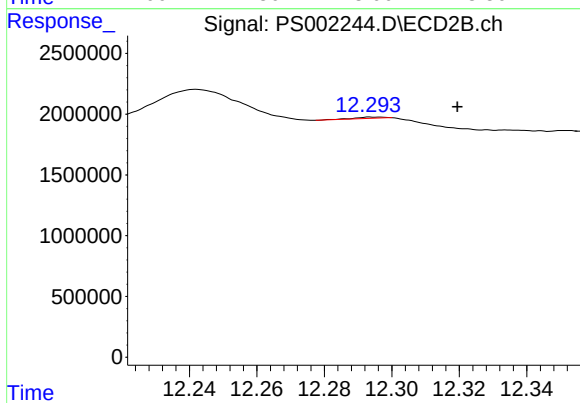

#8 DICHLORPROP


R.T.: 12.295 min
Delta R.T.: -0.025 min
Response: 81697
Conc: 0.25 ng/ml

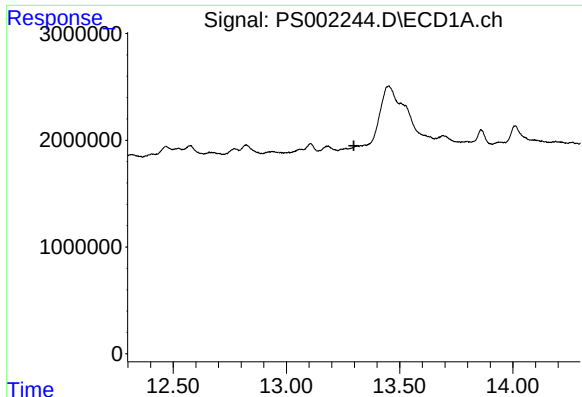

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 13.298 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

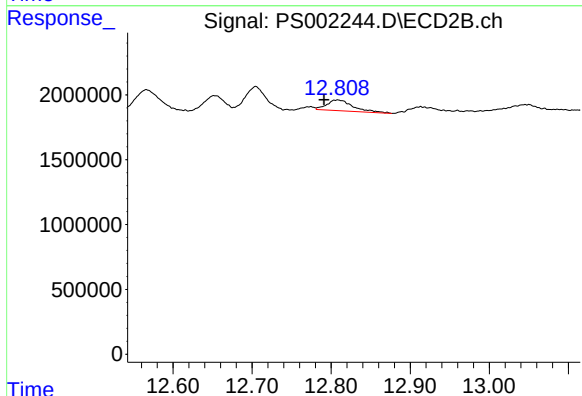


#9 2,4-D

R.T.: 12.809 min
Delta R.T.: 0.018 min
Response: 1922134
Conc: 4.51 ng/ml

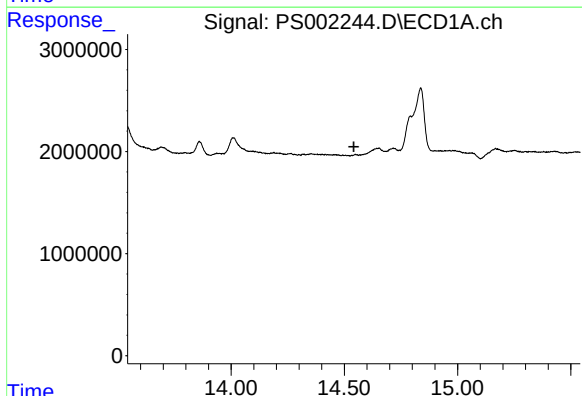


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 14.542 min
Response: 0
Conc: N.D.

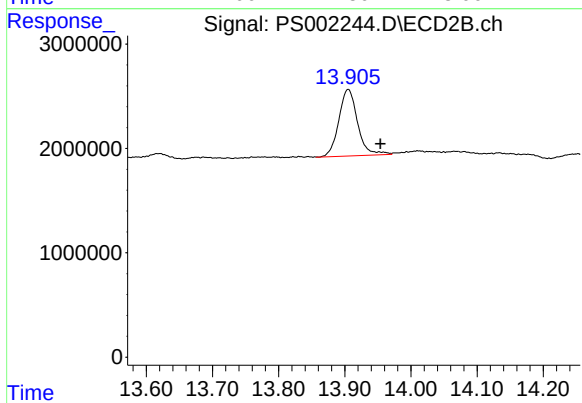

#11 2,4,5-TP (SILVEX)


R.T.: 13.905 min
Delta R.T.: -0.048 min
Response: 12594038
Conc: 6.88 ng/ml

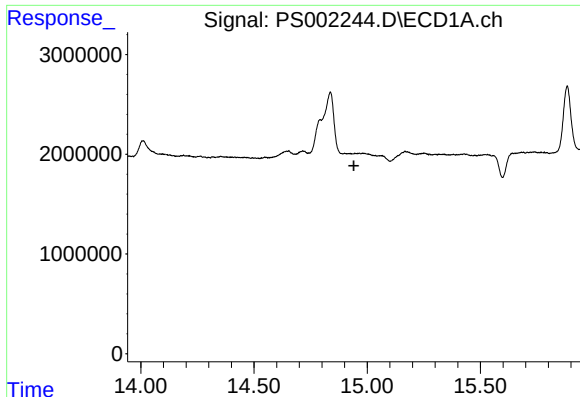

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 14.941 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

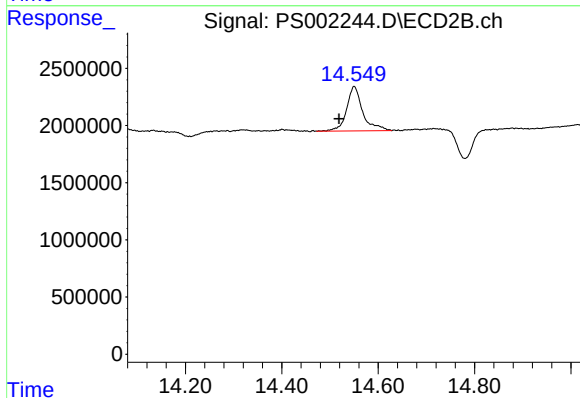


#12 2,4,5-T

R.T.: 14.550 min
Delta R.T.: 0.031 min
Response: 9004248
Conc: 6.01 ng/ml

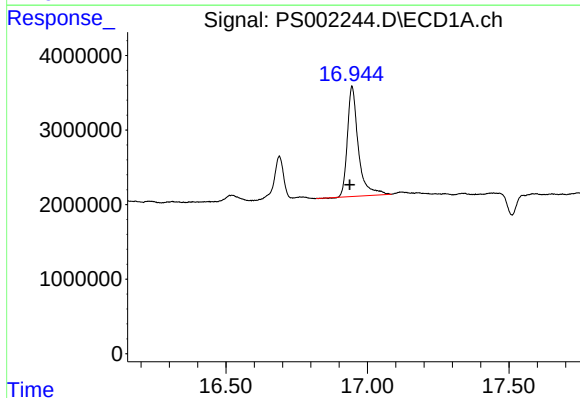


#15 Picloram

R.T.: 16.945 min
Delta R.T.: 0.008 min
Response: 39594500
Conc: 16.60 ng/ml

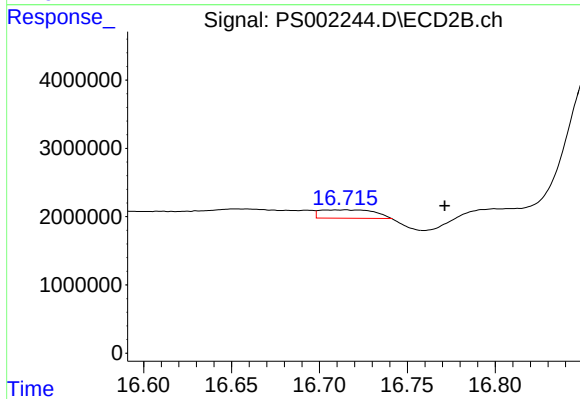

#15 Picloram


R.T.: 16.715 min
Delta R.T.: -0.056 min
Response: 2609796
Conc: 1.15 ng/ml

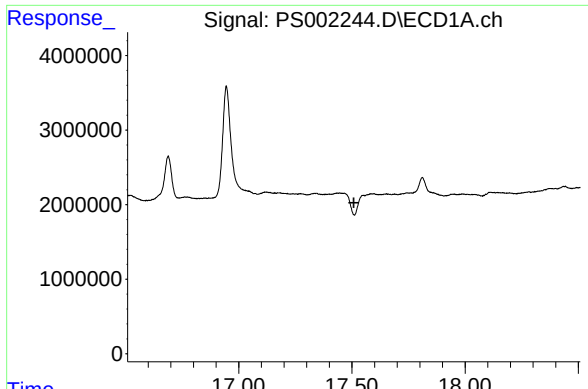

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.509 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

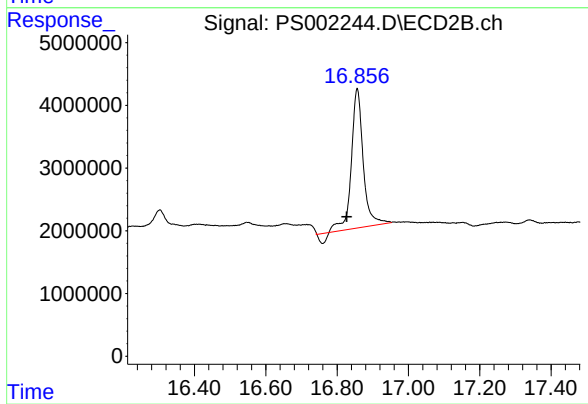

#16 DCPA

R.T.: 16.856 min
Delta R.T.: 0.030 min
Response: 50177819
Conc: 21.19 ng/ml