

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110118\
 Data File : PS002247.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Nov 2018 20:19
 Operator : EI\SJ
 Sample : J5737-02MS
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 02 03:52:08 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102618.M
 Quant Title : 8080.M
 QLast Update : Sat Oct 27 01:34:10 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.414	10.907	125.4E6	130.7E6	398.561	363.837
Target Compounds							
1) T	Dalapon	2.934	2.371	186.9E6	209.8E6	407.533	464.671
2) T	3,5-DICHL...	0.000	9.062	0	183.6E6	N.D.	413.961 #
3) T	4-Nitroph...	11.064	10.062	5969662	14910628	35.783	83.622 #
5) T	DICAMBA	11.724	11.190	620.2E6	263.3E6	467.025	210.693 #
6) T	MCPD	12.066	11.420	-20399259	47250508	N.D.	54.921
7) T	MCPA	0.000	11.795	0	78854879	N.D.	58.264 #
8) T	DICHLORPROP	12.910	12.314	181.4E6	-26713642	520.751	N.D. #
9) T	2,4-D	0.000	12.784	0	167.0E6	N.D.	392.058 #
10) T	Pentachlo...	13.648	13.330	2062.4E6	1744.7E6	428.721	371.409
11) T	2,4,5-TP ...	0.000	13.948	0	1083.0E6	N.D.	591.918 #
12) T	2,4,5-T	14.911	14.513	948.2E6	522.2E6	529.077	348.705 #
13) T	2,4-DB	0.000	15.162	0	81930515	N.D.	369.792 #
14) T	DINOSEB	17.139	15.591	494.1E6	481.0E6	360.623	379.961
15) T	Picloram	16.904	16.768	1124.5E6	794.2E6	471.427	351.063 #
16) T	DCPA	0.000	16.820	0	1107.0E6	N.D.	467.524 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110118\
Data File : PS002247.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Nov 2018 20:19
Operator : EI\SJ
Sample : J5737-02MS
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 02 03:52:08 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102618.M
Quant Title : 8080.M
QLast Update : Sat Oct 27 01:34:10 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

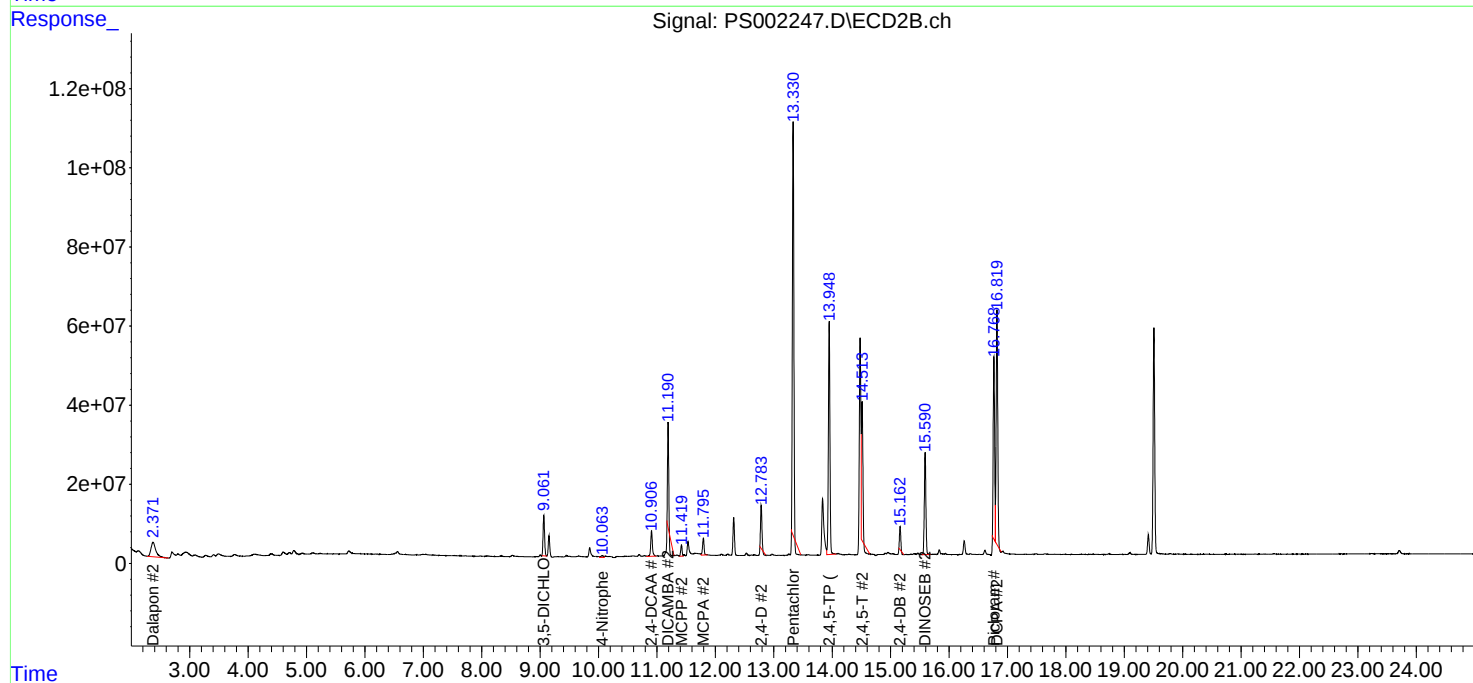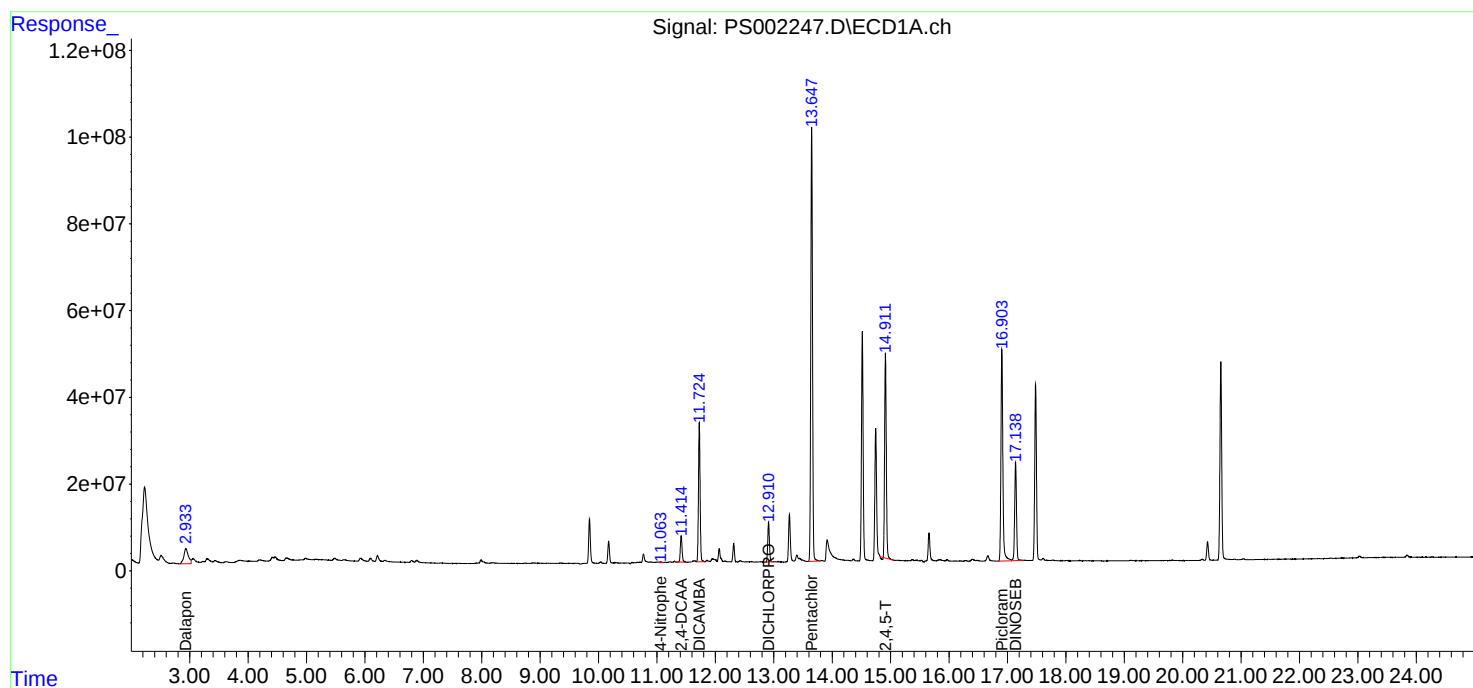


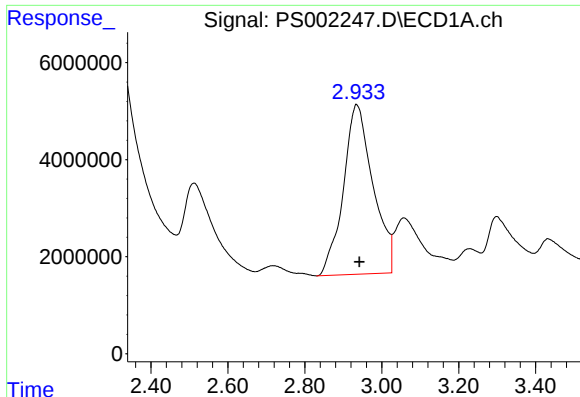

#1 Dalapon


R.T.: 2.934 min
Delta R.T.: -0.008 min
Response: 186921869
Conc: 407.53 ng/ml

Instrument :
ECD_S
ClientSampleId :

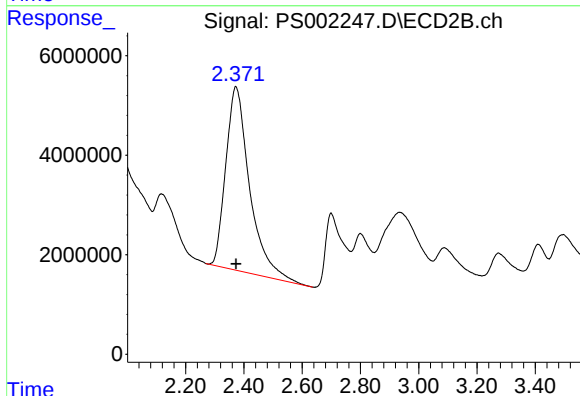


#1 Dalapon

R.T.: 2.371 min
Delta R.T.: -0.002 min
Response: 209802280
Conc: 464.67 ng/ml

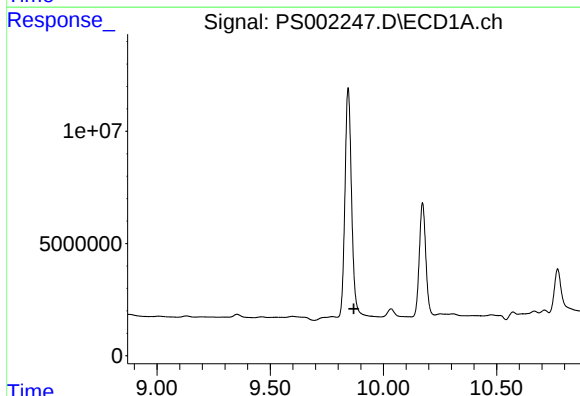


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.870 min
Response: 0
Conc: N.D.

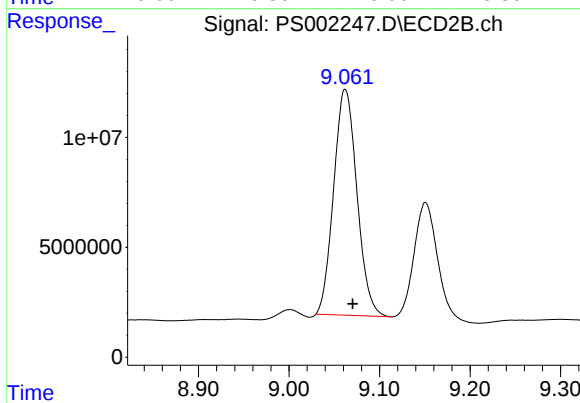

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.062 min
Delta R.T.: -0.008 min
Response: 183614228
Conc: 413.96 ng/ml

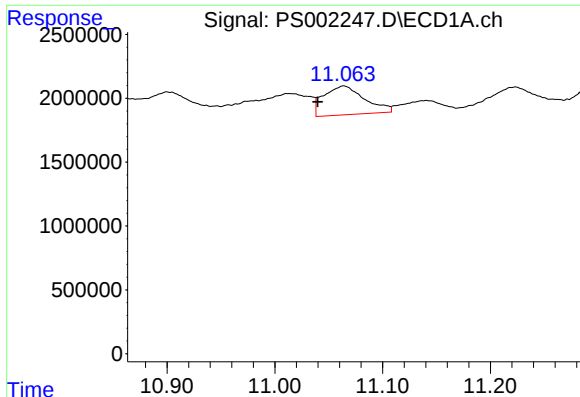

#3 4-Nitrophenol


R.T.: 11.064 min
Delta R.T.: 0.024 min
Response: 5969662
Conc: 35.78 ng/ml

Instrument :
ECD_S
ClientSampleId :

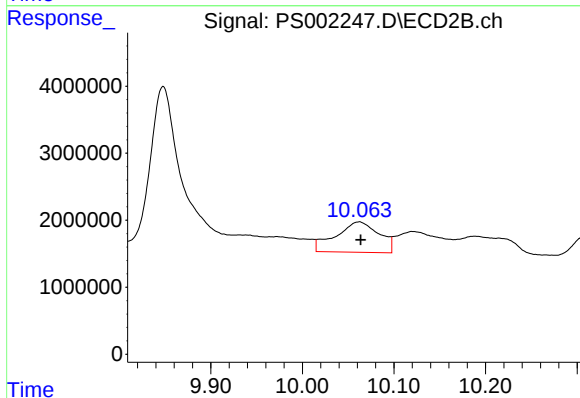


#3 4-Nitrophenol

R.T.: 10.062 min
Delta R.T.: -0.002 min
Response: 14910628
Conc: 83.62 ng/ml

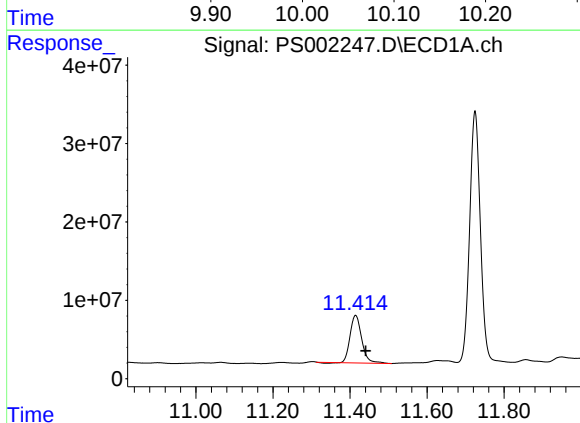


#4 2,4-DCAA

R.T.: 11.414 min
Delta R.T.: -0.027 min
Response: 125421331
Conc: 398.56 ng/ml

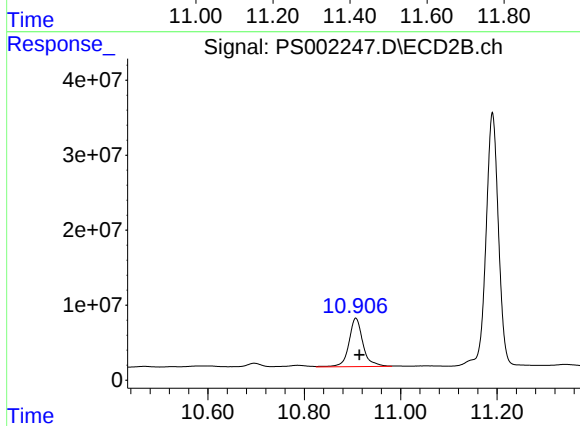

#4 2,4-DCAA


R.T.: 10.907 min
Delta R.T.: -0.008 min
Response: 130652971
Conc: 363.84 ng/ml

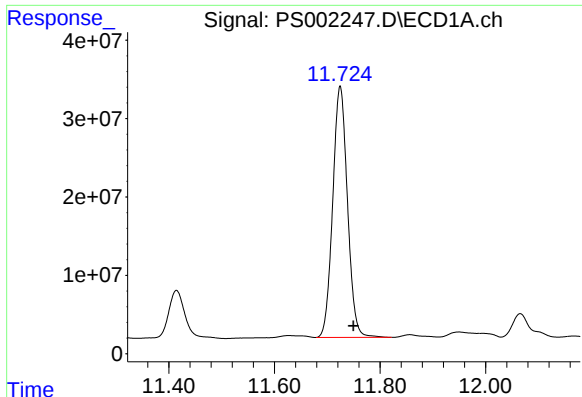

#5 DICAMBA


R.T.: 11.724 min
Delta R.T.: -0.025 min
Response: 620217222
Conc: 467.02 ng/ml

Instrument :
ECD_S
ClientSampleId :

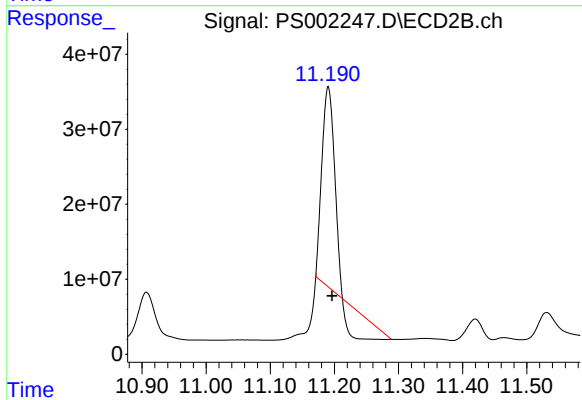


#5 DICAMBA

R.T.: 11.190 min
Delta R.T.: -0.006 min
Response: 263302399
Conc: 210.69 ng/ml

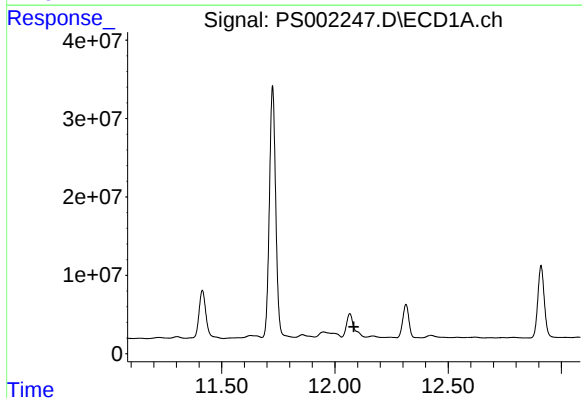


#6 MCP

R.T.: 12.066 min
Delta R.T.: -0.018 min
Response: -20399259
Conc: N.D.

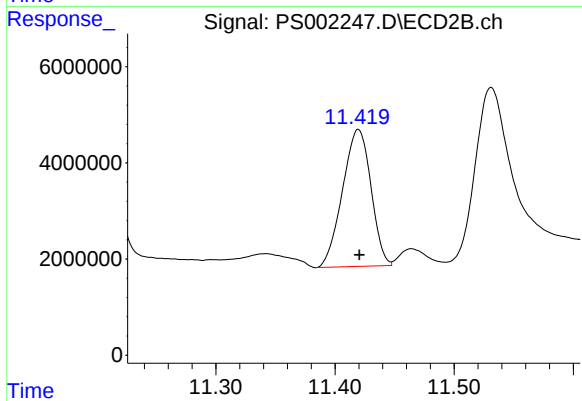

#6 MCP


R.T.: 11.420 min
Delta R.T.: 0.000 min
Response: 47250508
Conc: 54.92 ug/ml

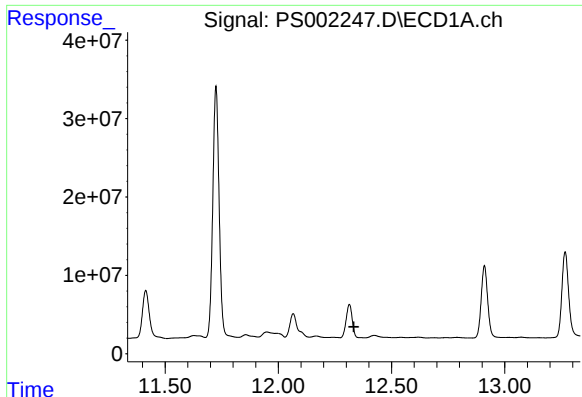

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 12.333 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

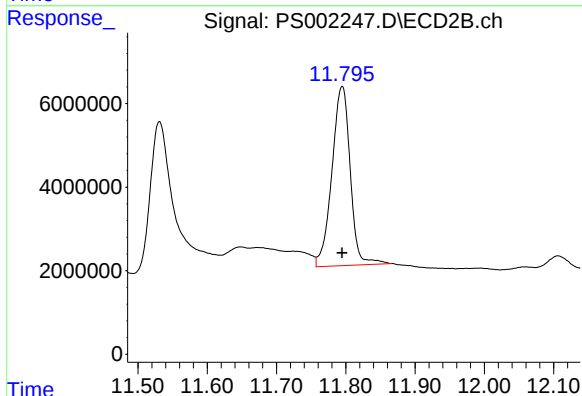


#7 MCPA

R.T.: 11.795 min
Delta R.T.: 0.000 min
Response: 78854879
Conc: 58.26 ug/ml

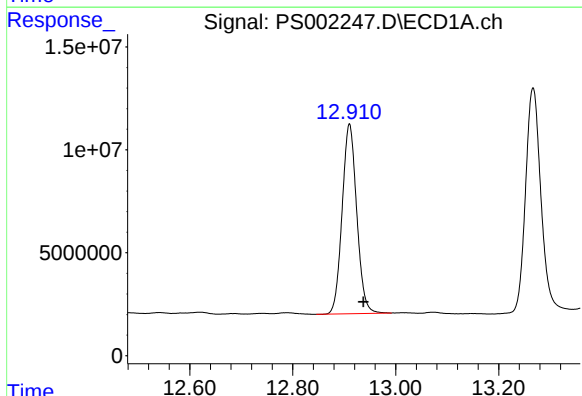


#8 DICHLORPROP

R.T.: 12.910 min
Delta R.T.: -0.027 min
Response: 181353098
Conc: 520.75 ng/ml

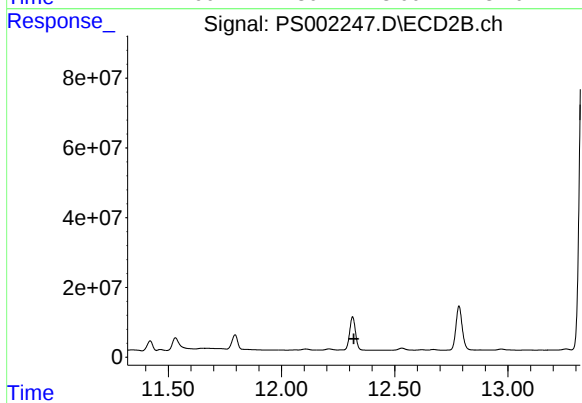

#8 DICHLORPROP


R.T.: 12.314 min
Delta R.T.: -0.006 min
Response: -26713642
Conc: N.D.

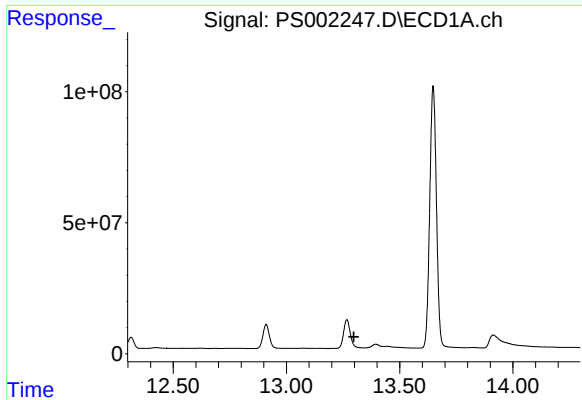

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 13.298 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

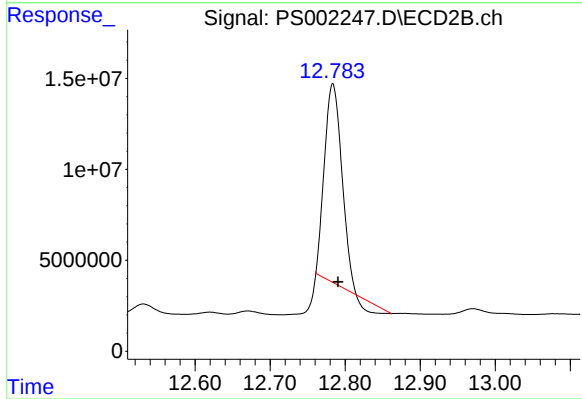


#9 2,4-D

R.T.: 12.784 min
Delta R.T.: -0.007 min
Response: 166974631
Conc: 392.06 ng/ml

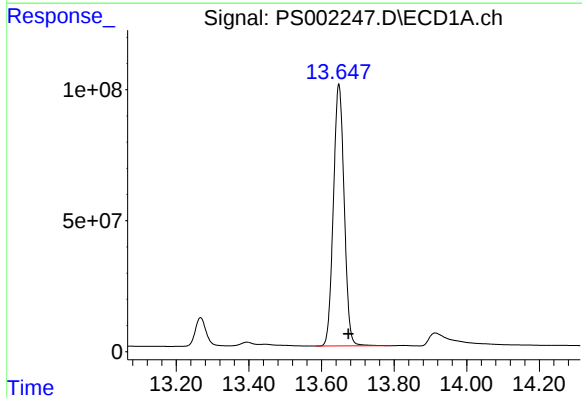


#10 Pentachlorophenol

R.T.: 13.648 min
Delta R.T.: -0.026 min
Response: 2062439323
Conc: 428.72 ng/ml

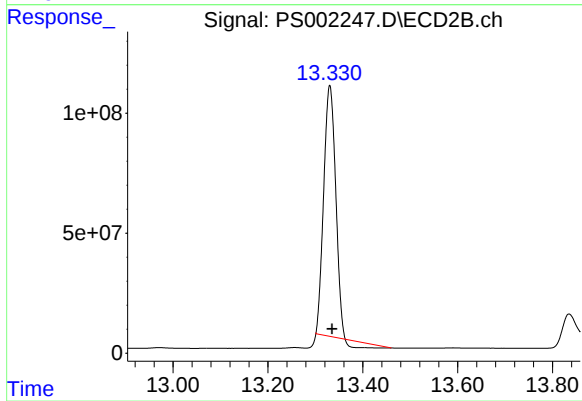

#10 Pentachlorophenol


R.T.: 13.330 min
Delta R.T.: -0.005 min
Response: 1744673233
Conc: 371.41 ng/ml

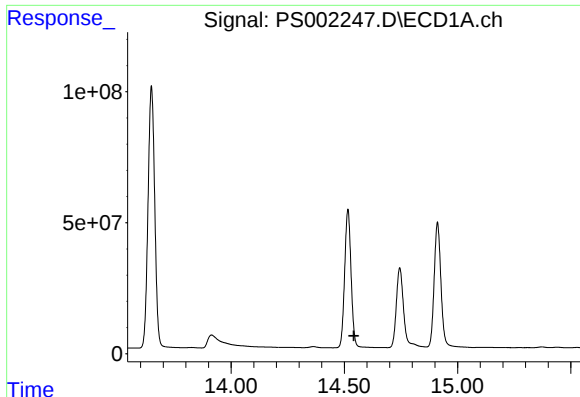

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 14.542 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

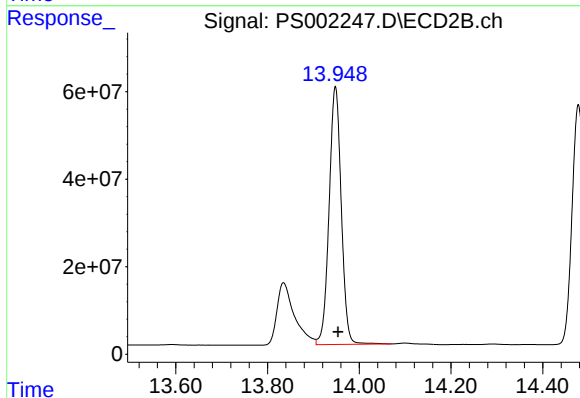


#11 2,4,5-TP (SILVEX)

R.T.: 13.948 min
Delta R.T.: -0.006 min
Response: 1082953049
Conc: 591.92 ng/ml

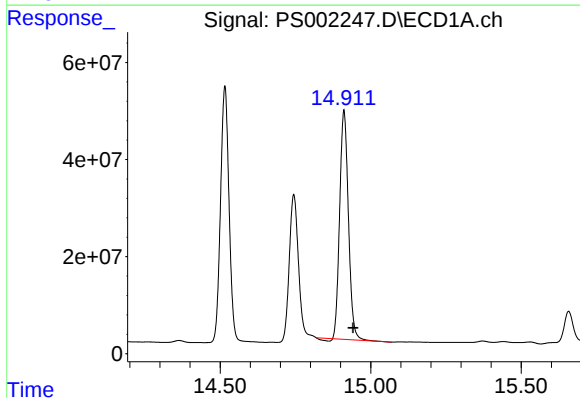


#12 2,4,5-T

R.T.: 14.911 min
Delta R.T.: -0.030 min
Response: 948241882
Conc: 529.08 ng/ml

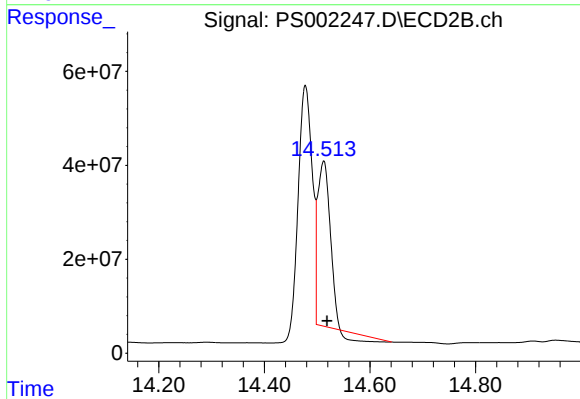

#12 2,4,5-T


R.T.: 14.513 min
Delta R.T.: -0.006 min
Response: 522179254
Conc: 348.71 ng/ml

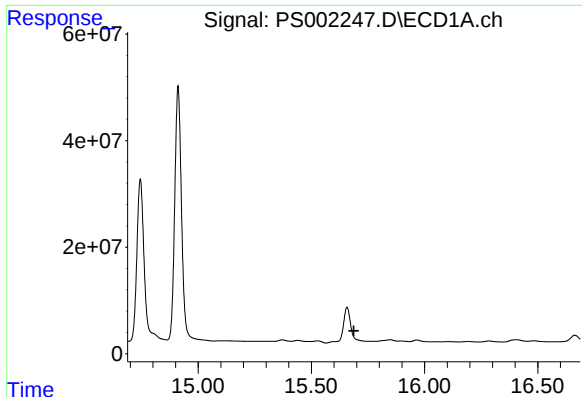

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 15.688 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

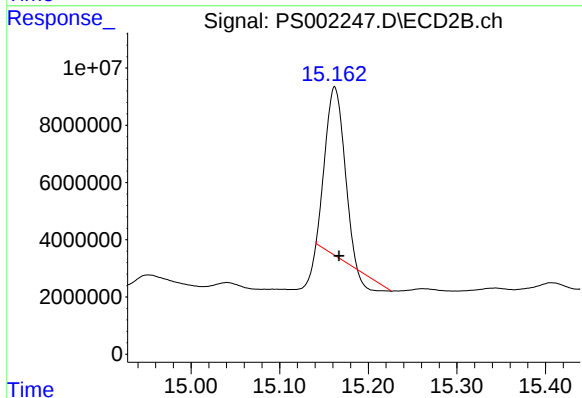


#13 2,4-DB

R.T.: 15.162 min
Delta R.T.: -0.005 min
Response: 81930515
Conc: 369.79 ng/ml

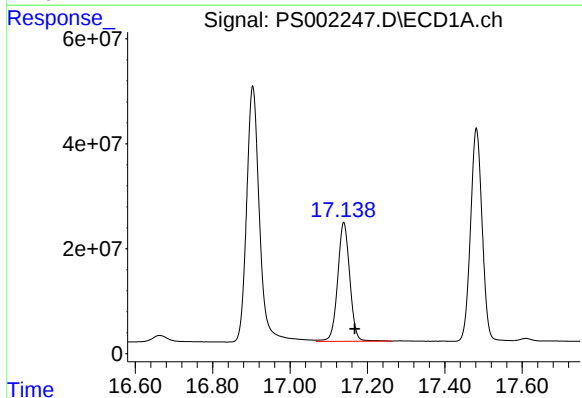


#14 DINOSEB

R.T.: 17.139 min
Delta R.T.: -0.029 min
Response: 494071307
Conc: 360.62 ng/ml

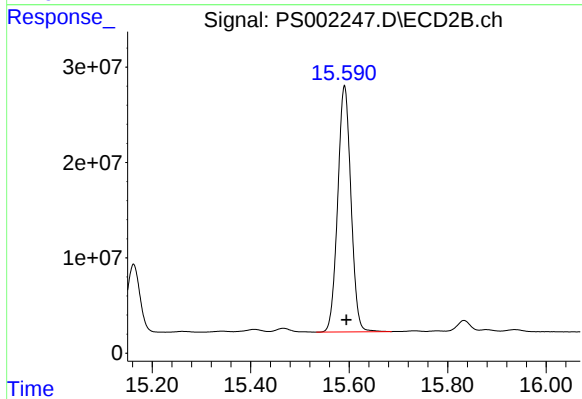

#14 DINOSEB


R.T.: 15.591 min
Delta R.T.: -0.004 min
Response: 480980449
Conc: 379.96 ng/ml

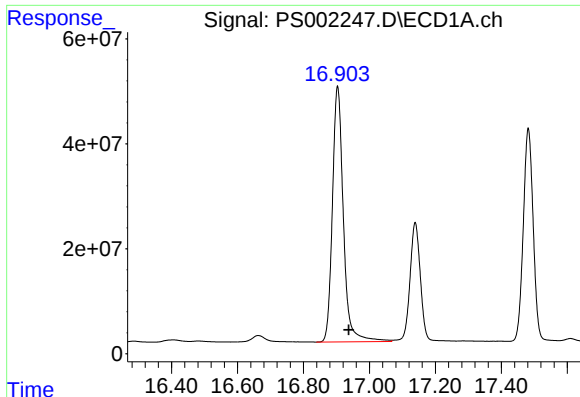

#15 Picloram


R.T.: 16.904 min
Delta R.T.: -0.034 min
Response: 1124493204
Conc: 471.43 ng/ml

Instrument :
ECD_S
ClientSampleId :

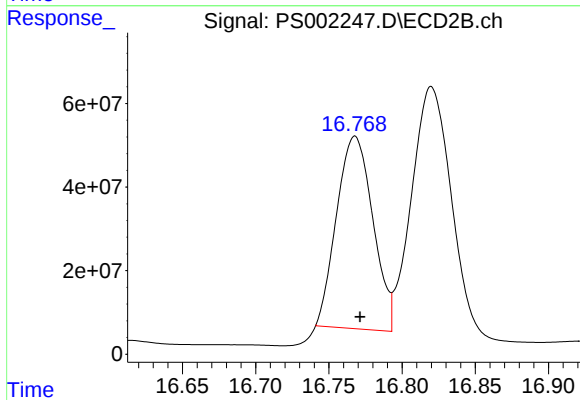


#15 Picloram

R.T.: 16.768 min
Delta R.T.: -0.003 min
Response: 794182628
Conc: 351.06 ng/ml

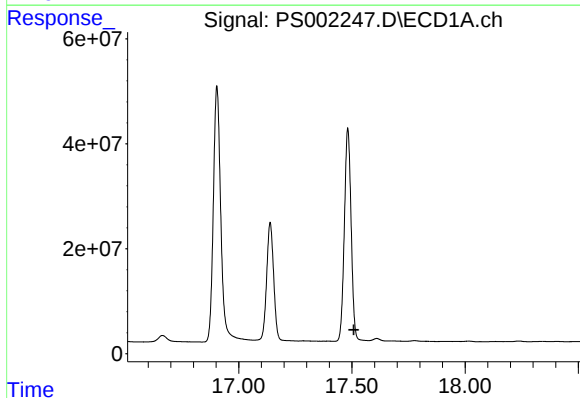

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.509 min
Response: 0
Conc: N.D.

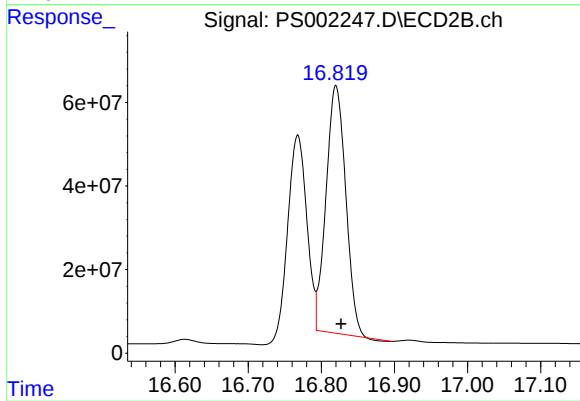

#16 DCPA

R.T.: 16.820 min
Delta R.T.: -0.007 min
Response: 1107033641
Conc: 467.52 ng/ml