

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110118\
 Data File : PS002253.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Nov 2018 23:25
 Operator : EI\SJ
 Sample : J5741-14
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 02 03:54:15 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102618.M
 Quant Title : 8080.M
 QLast Update : Sat Oct 27 01:34:10 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.434	10.910	120.1E6	119.2E6	381.512	331.891
Target Compounds							
1) T	Dalapon	2.908	2.338	20042841	26615886	43.698	58.949 #
2) T	3,5-DICHL...	0.000	9.071	0	2851135	N.D.	6.428 #
3) T	4-Nitroph...	0.000	10.067	0	10975971	N.D.	61.555 #
5) T	DICAMBA	0.000	11.151	0	7682075	N.D.	6.147 #
6) T	MCPD	12.116	0.000	8153741	0	8.254	N.D. #
7) T	MCPA	0.000	11.803	0	4818308	N.D.	3.560 #
8) T	DICHLORPROP	0.000	12.266	0	1499427	N.D.	4.669 #
9) T	2,4-D	0.000	12.778	0	582677	N.D.	1.368 #
11) T	2,4,5-TP ...	0.000	13.975	0	219427	N.D.	0.120 #
14) T	DINOSEB	0.000	15.640	0	4113940	N.D.	3.250 #
15) T	Picloram	0.000	16.771	0	4907100	N.D.	2.169 #
16) T	DCPA	0.000	16.836	0	4438461	N.D.	1.874 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110118\
Data File : PS002253.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Nov 2018 23:25
Operator : EI\SJ
Sample : J5741-14
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 02 03:54:15 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102618.M
Quant Title : 8080.M
QLast Update : Sat Oct 27 01:34:10 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

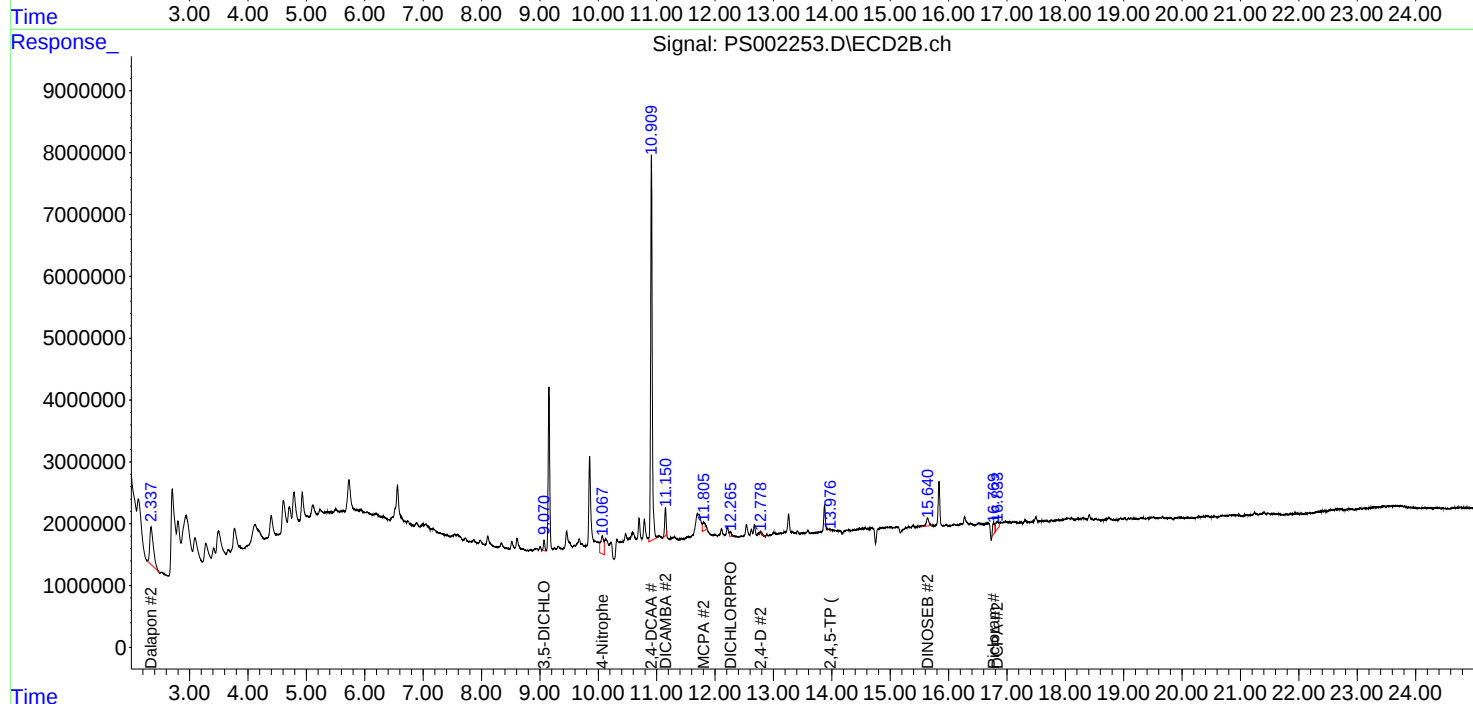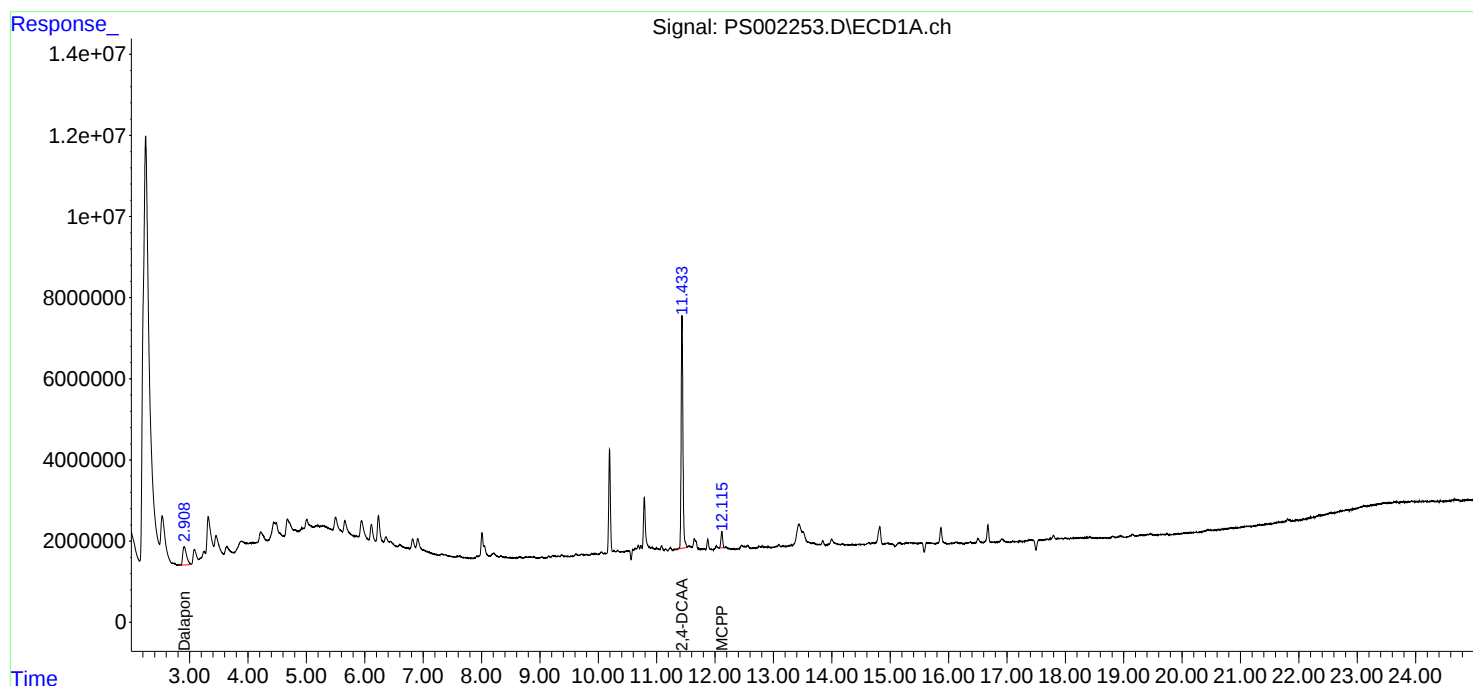


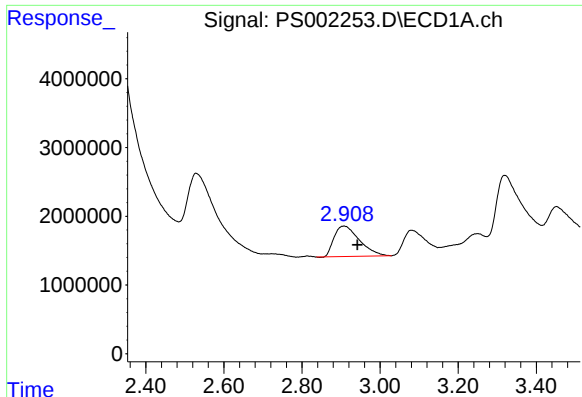

#1 Dalapon


R.T.: 2.908 min
Delta R.T.: -0.034 min
Response: 20042841
Conc: 43.70 ng/ml

Instrument :
ECD_S
ClientSampleId :

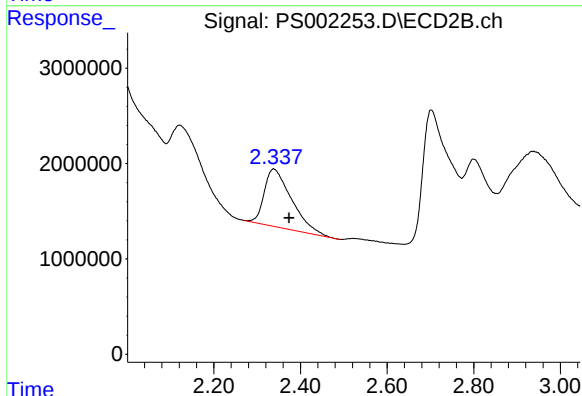


#1 Dalapon

R.T.: 2.338 min
Delta R.T.: -0.036 min
Response: 26615886
Conc: 58.95 ng/ml

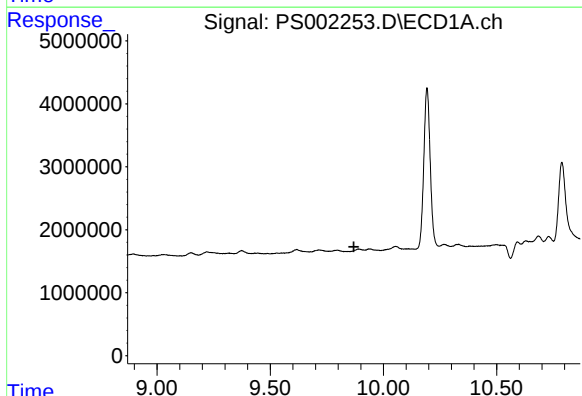


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.870 min
Response: 0
Conc: N.D.

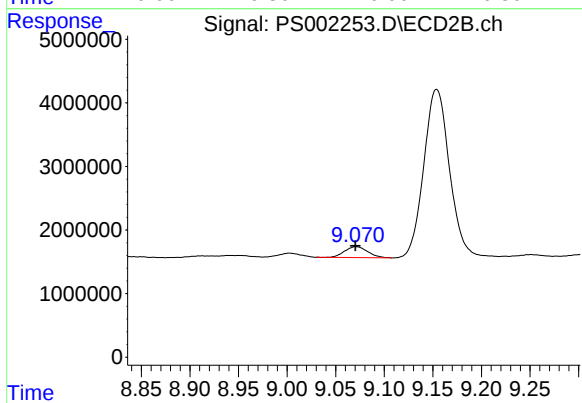

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.071 min
Delta R.T.: 0.000 min
Response: 2851135
Conc: 6.43 ng/ml

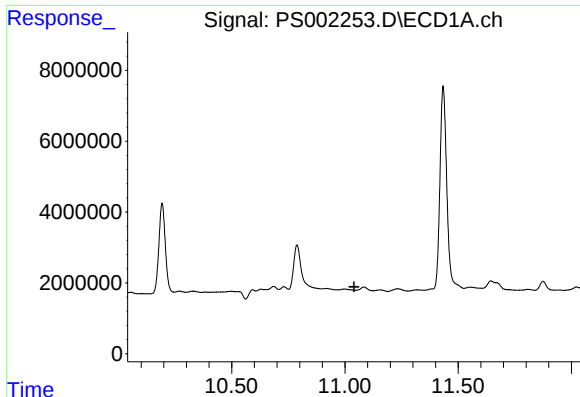

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 11.040 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

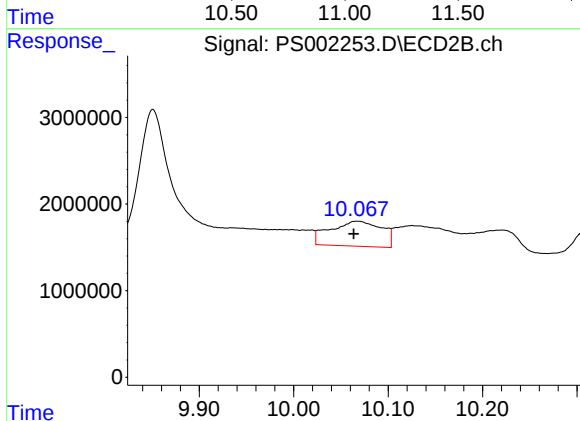


#3 4-Nitrophenol

R.T.: 10.067 min
Delta R.T.: 0.003 min
Response: 10975971
Conc: 61.56 ng/ml

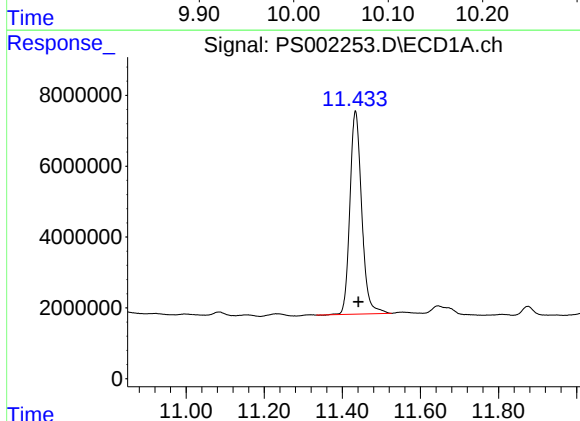


#4 2,4-DCAA

R.T.: 11.434 min
Delta R.T.: -0.007 min
Response: 120056262
Conc: 381.51 ng/ml

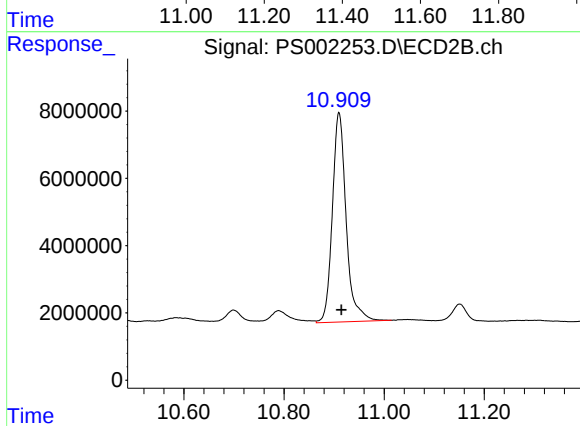

#4 2,4-DCAA


R.T.: 10.910 min
Delta R.T.: -0.005 min
Response: 119181461
Conc: 331.89 ng/ml

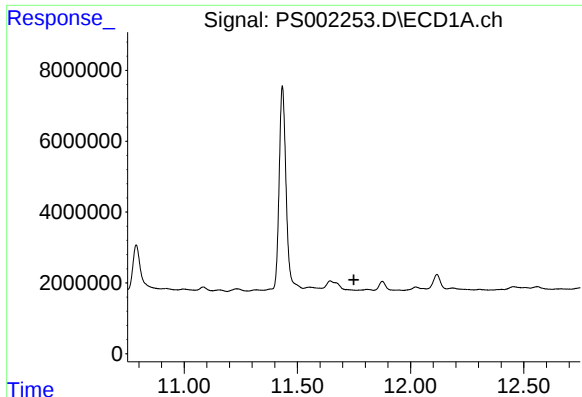

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.750 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

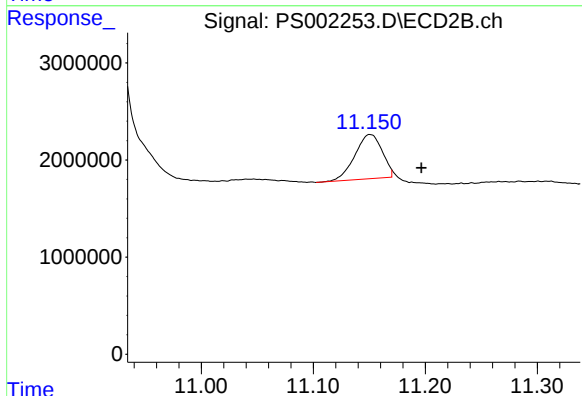


#5 DICAMBA

R.T.: 11.151 min
Delta R.T.: -0.046 min
Response: 7682075
Conc: 6.15 ng/ml

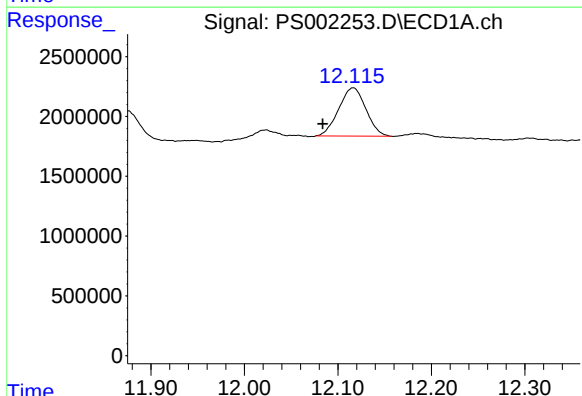


#6 MCP

R.T.: 12.116 min
Delta R.T.: 0.032 min
Response: 8153741
Conc: 8.25 ug/ml

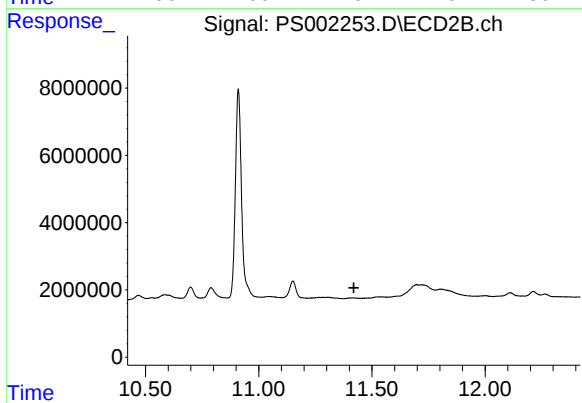

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.420 min
Response: 0
Conc: N.D.

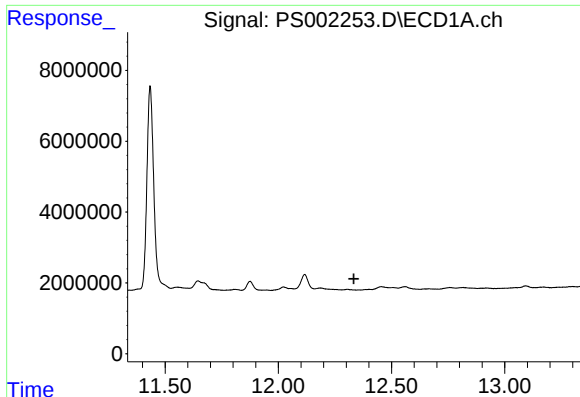

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 12.333 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

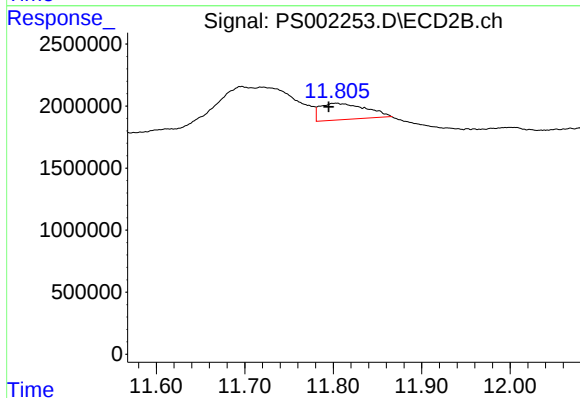


#7 MCPA

R.T.: 11.803 min
Delta R.T.: 0.009 min
Response: 4818308
Conc: 3.56 ug/ml

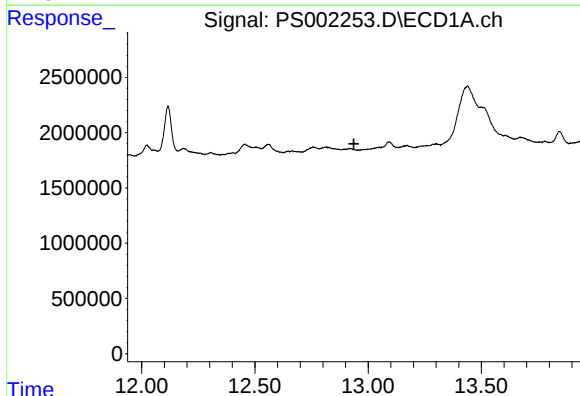


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 12.937 min
Response: 0
Conc: N.D.

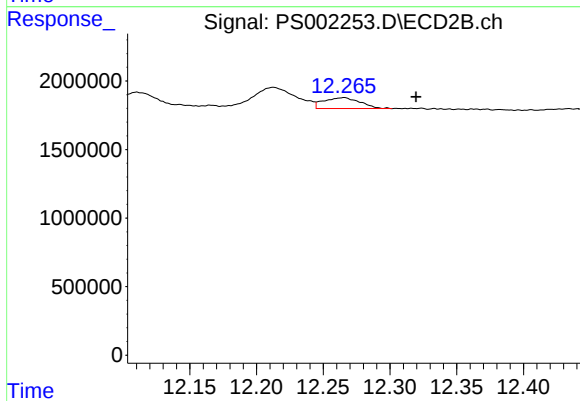

#8 DICHLORPROP


R.T.: 12.266 min
Delta R.T.: -0.054 min
Response: 1499427
Conc: 4.67 ng/ml

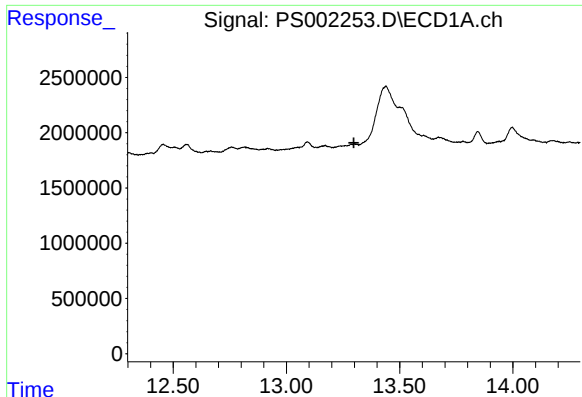

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 13.298 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

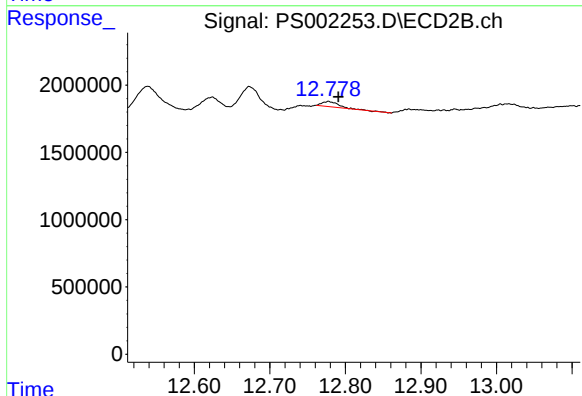


#9 2,4-D

R.T.: 12.778 min
Delta R.T.: -0.013 min
Response: 582677
Conc: 1.37 ng/ml

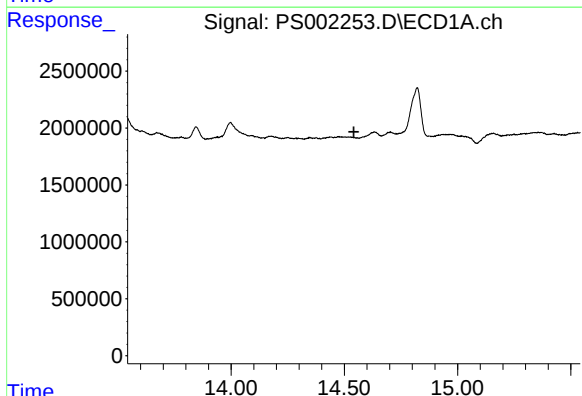


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 14.542 min
Response: 0
Conc: N.D.

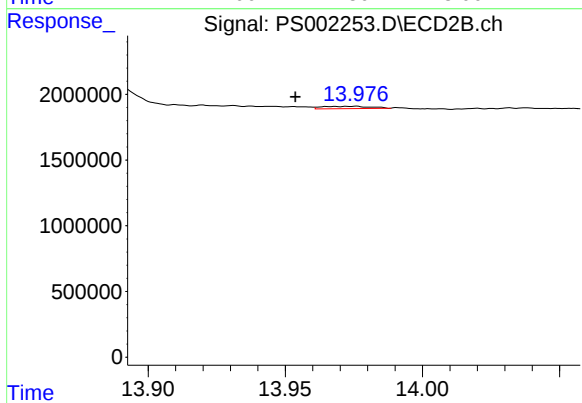

#11 2,4,5-TP (SILVEX)


R.T.: 13.975 min
Delta R.T.: 0.021 min
Response: 219427
Conc: 0.12 ng/ml

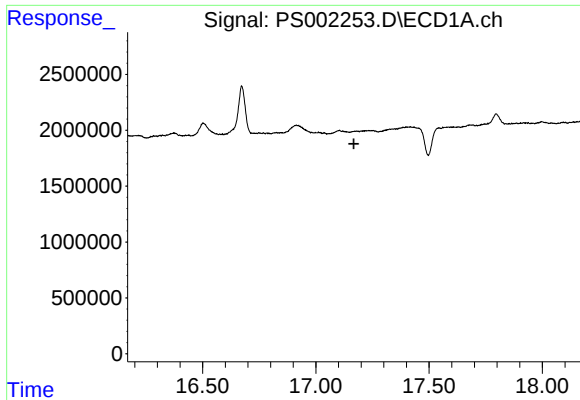

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 17.168 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

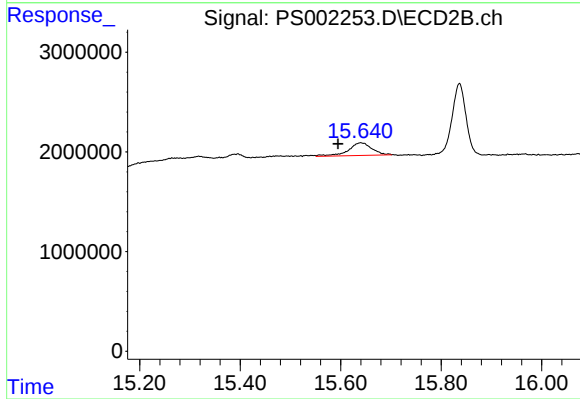


#14 DINOSEB

R.T.: 15.640 min
Delta R.T.: 0.045 min
Response: 4113940
Conc: 3.25 ng/ml

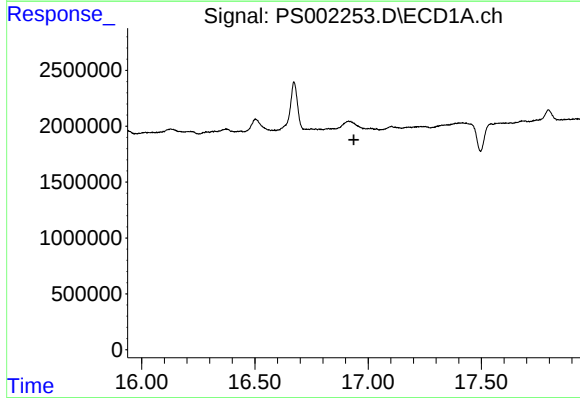


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 16.937 min
Response: 0
Conc: N.D.

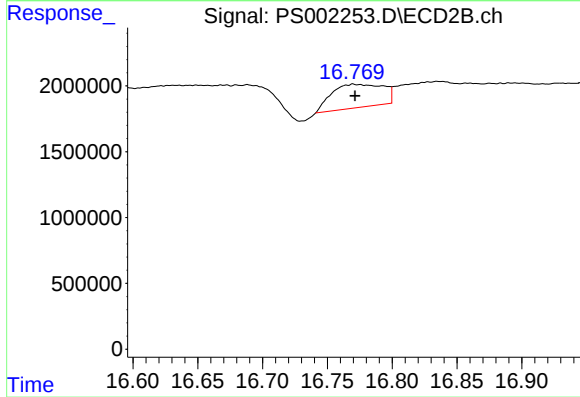

#15 Picloram


R.T.: 16.771 min
Delta R.T.: 0.000 min
Response: 4907100
Conc: 2.17 ng/ml

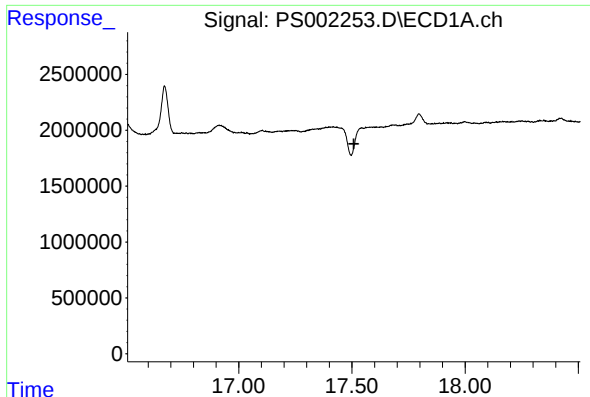

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.509 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

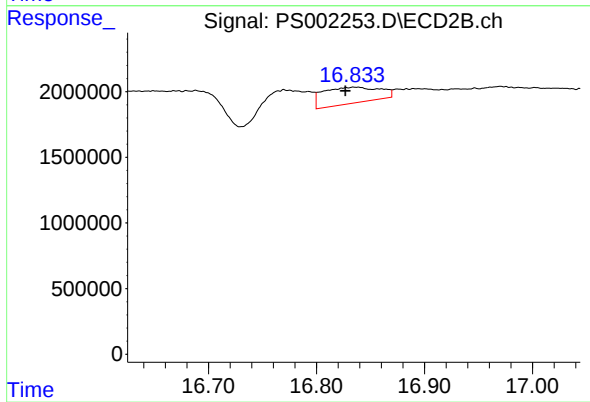

#16 DCPA

R.T.: 16.836 min
Delta R.T.: 0.010 min
Response: 4438461
Conc: 1.87 ng/ml