

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110118\
 Data File : PS002263.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Nov 2018 04:35
 Operator : EI\SJ
 Sample : J5741-46
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 02 07:14:27 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102618.M
 Quant Title : 8080.M
 QLast Update : Sat Oct 27 01:34:10 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.413	10.906	100.2E6	102.0E6	318.273	284.006
Target Compounds							
1) T	Dalapon	2.887	2.334	13641385	18408483	29.741	40.771 #
2) T	3,5-DICHL...	0.000	9.067	0	1813669	N.D.	4.089 #
3) T	4-Nitroph...	0.000	10.063	0	3567771	N.D.	20.009 #
5) T	DICAMBA	0.000	11.146	0	6458467	N.D.	5.168 #
6) T	MCPD	12.093	0.000	2488666	0	2.519	N.D. #
7) T	MCPA	0.000	11.793	0	1252651	N.D.	0.926 #
8) T	DICHLORPROP	0.000	12.259	0	1333631	N.D.	4.153 #
9) T	2,4-D	0.000	12.734	0	128314	N.D.	0.301 #
11) T	2,4,5-TP ...	0.000	13.912	0	105922	N.D.	0.058 #
14) T	DINOSEB	0.000	15.594	0	278195	N.D.	0.220 #
15) T	Picloram	0.000	16.775	0	690979	N.D.	0.305 #
16) T	DCPA	0.000	16.830	0	1124057	N.D.	0.475 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110118\
Data File : PS002263.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Nov 2018 04:35
Operator : EI\SJ
Sample : J5741-46
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 02 07:14:27 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102618.M
Quant Title : 8080.M
QLast Update : Sat Oct 27 01:34:10 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

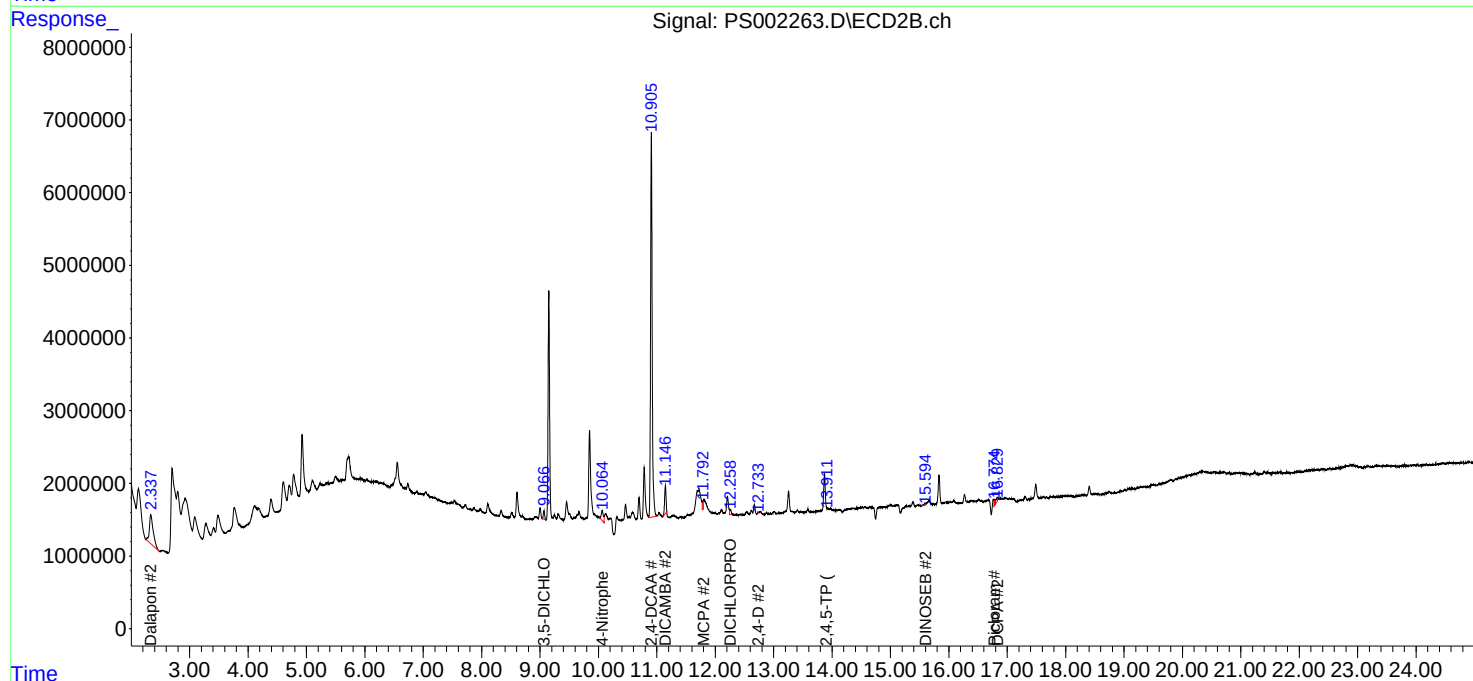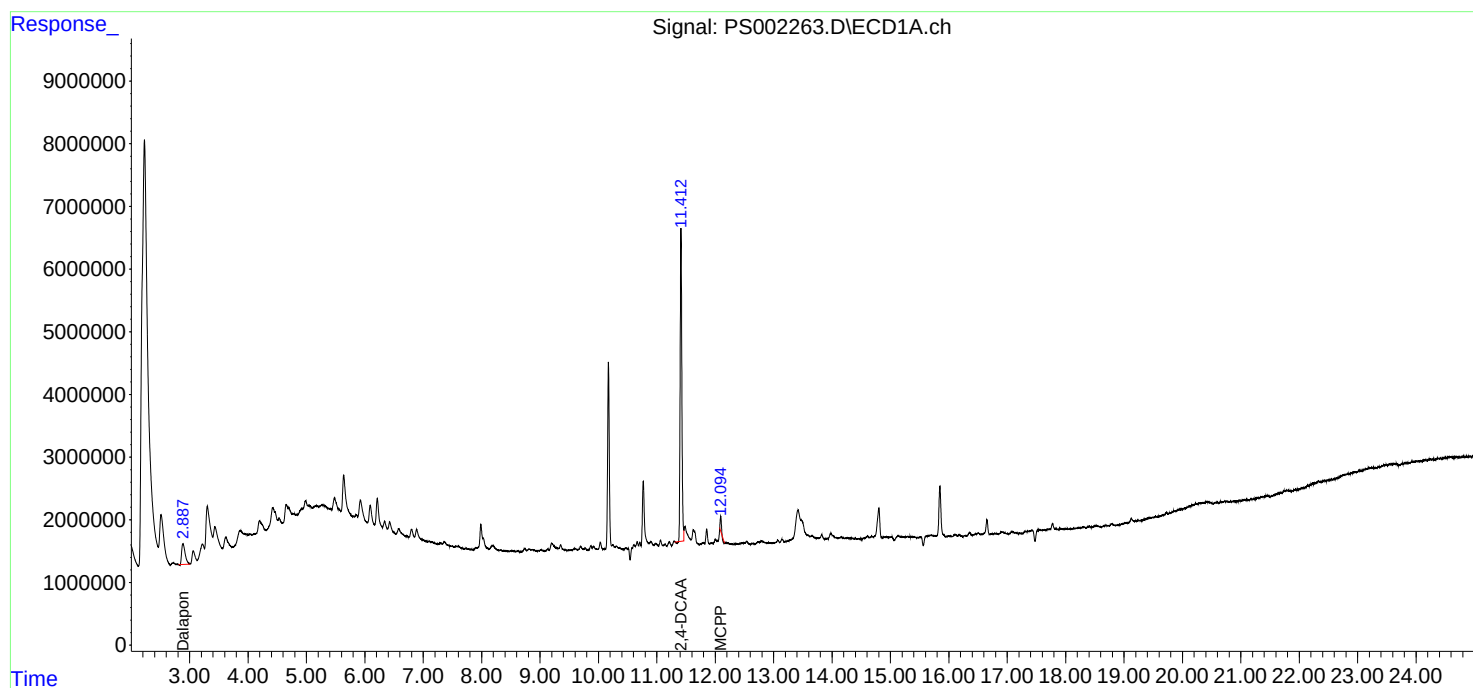


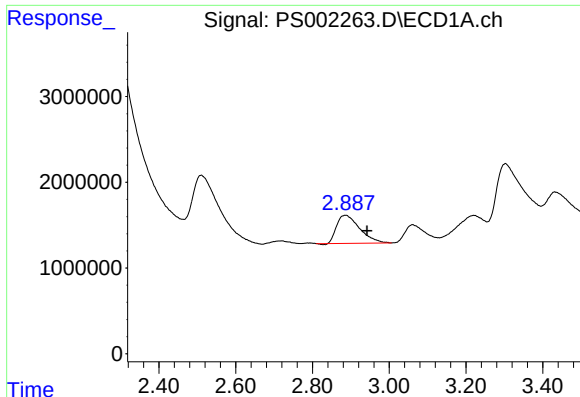

#1 Dalapon


R.T.: 2.887 min
Delta R.T.: -0.055 min
Response: 13641385
Conc: 29.74 ng/ml

Instrument :
ECD_S
ClientSampleId :

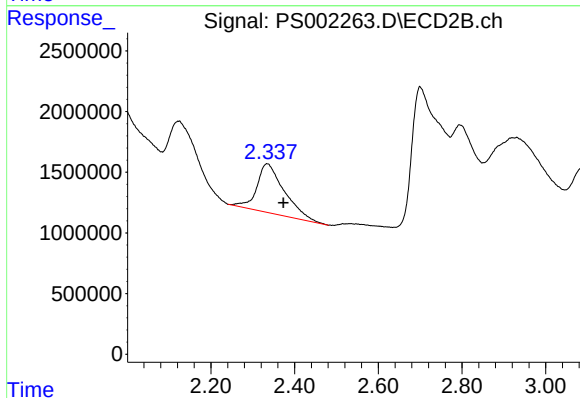


#1 Dalapon

R.T.: 2.334 min
Delta R.T.: -0.039 min
Response: 18408483
Conc: 40.77 ng/ml

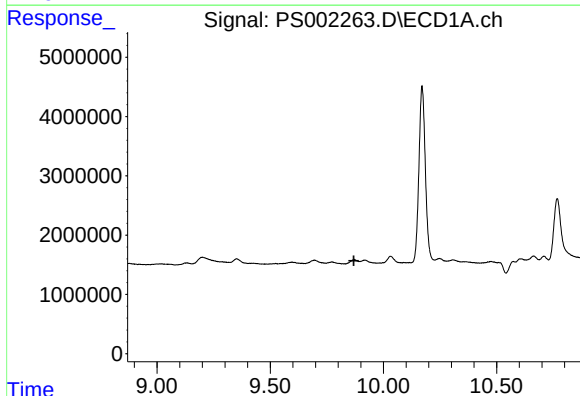


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.870 min
Response: 0
Conc: N.D.

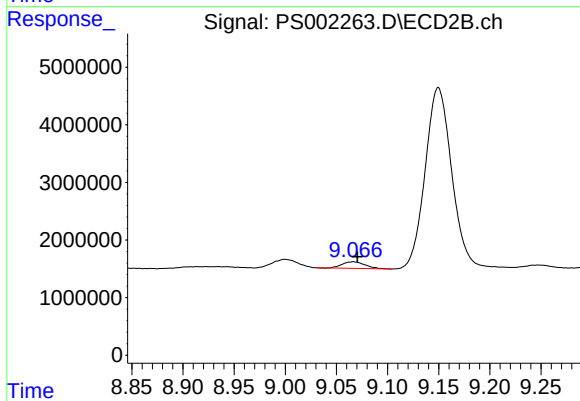

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.067 min
Delta R.T.: -0.004 min
Response: 1813669
Conc: 4.09 ng/ml

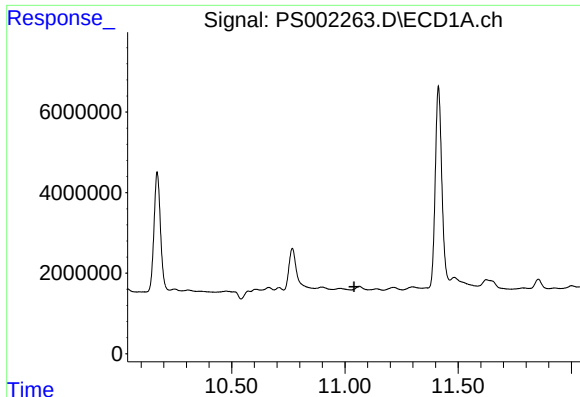

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 11.040 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

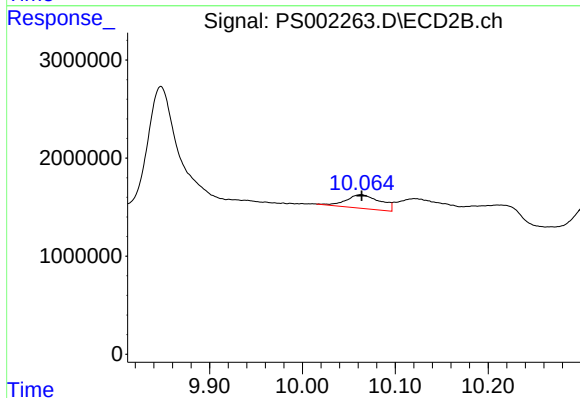


#3 4-Nitrophenol

R.T.: 10.063 min
Delta R.T.: 0.000 min
Response: 3567771
Conc: 20.01 ng/ml

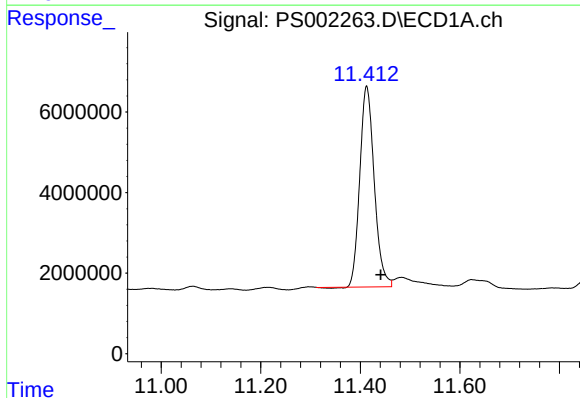


#4 2,4-DCAA

R.T.: 11.413 min
Delta R.T.: -0.028 min
Response: 100155951
Conc: 318.27 ng/ml

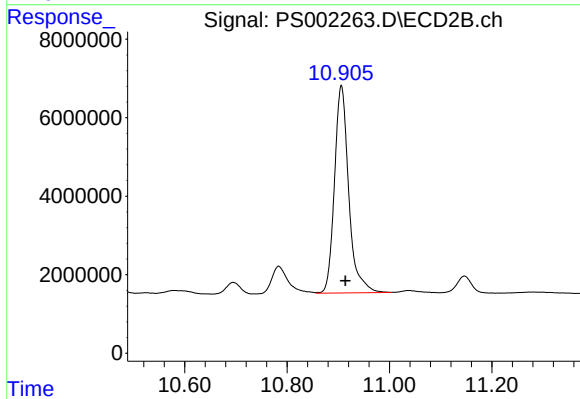

#4 2,4-DCAA


R.T.: 10.906 min
Delta R.T.: -0.008 min
Response: 101985825
Conc: 284.01 ng/ml

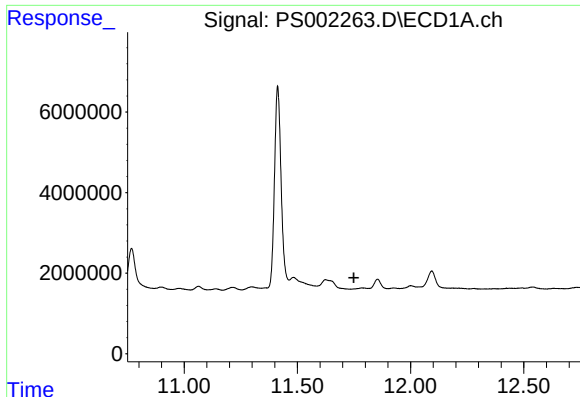

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.750 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

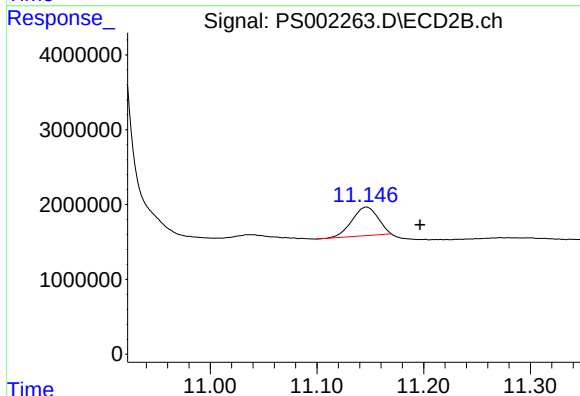


#5 DICAMBA

R.T.: 11.146 min
Delta R.T.: -0.050 min
Response: 6458467
Conc: 5.17 ng/ml

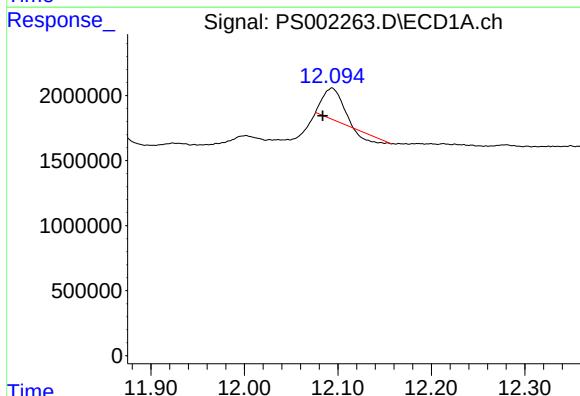


#6 MCP

R.T.: 12.093 min
Delta R.T.: 0.010 min
Response: 2488666
Conc: 2.52 ug/ml

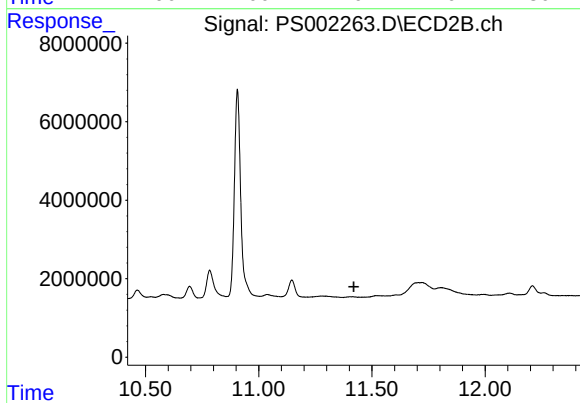

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.420 min
Response: 0
Conc: N.D.

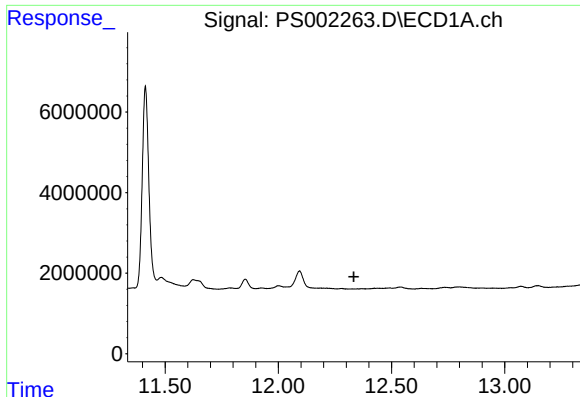

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 12.333 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

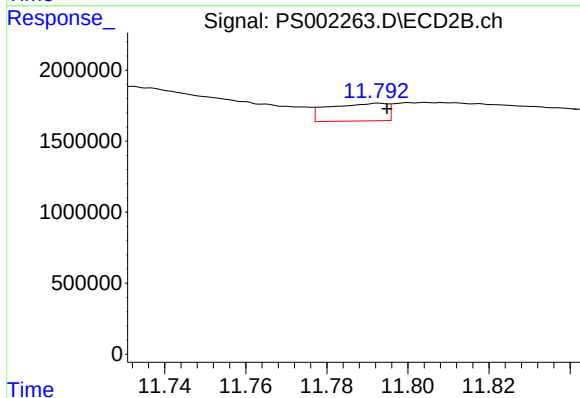


#7 MCPA

R.T.: 11.793 min
Delta R.T.: -0.002 min
Response: 1252651
Conc: 0.93 ug/ml

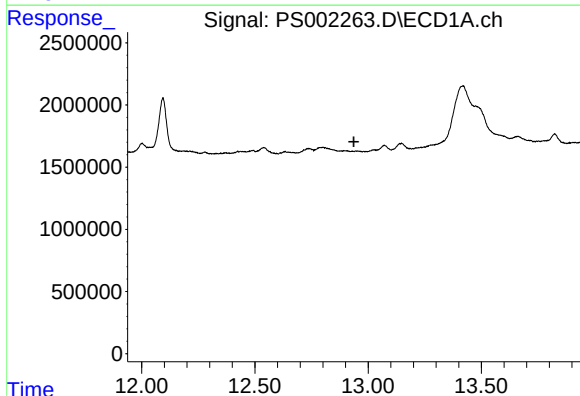


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 12.937 min
Response: 0
Conc: N.D.

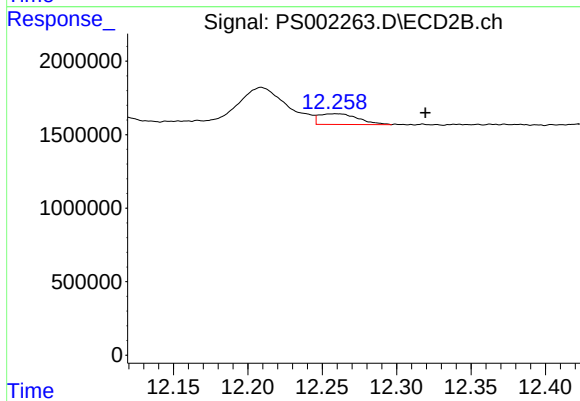

#8 DICHLORPROP


R.T.: 12.259 min
Delta R.T.: -0.060 min
Response: 1333631
Conc: 4.15 ng/ml

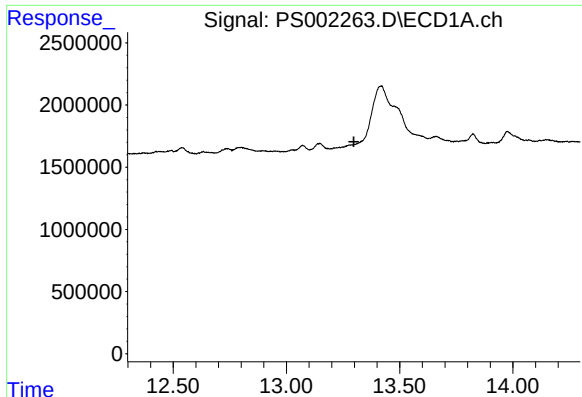

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 13.298 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

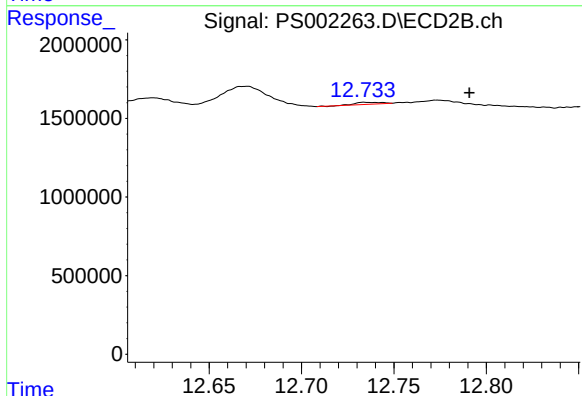


#9 2,4-D

R.T.: 12.734 min
Delta R.T.: -0.057 min
Response: 128314
Conc: 0.30 ng/ml

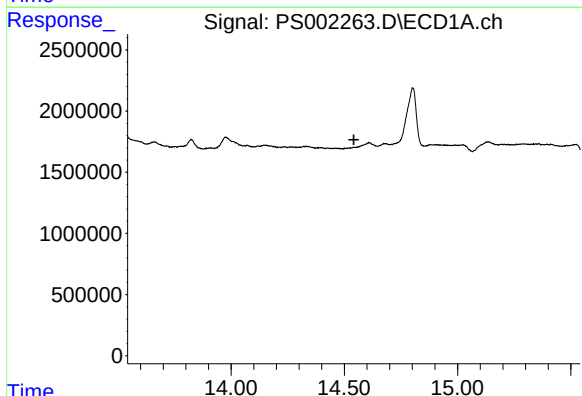


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 14.542 min
Response: 0
Conc: N.D.

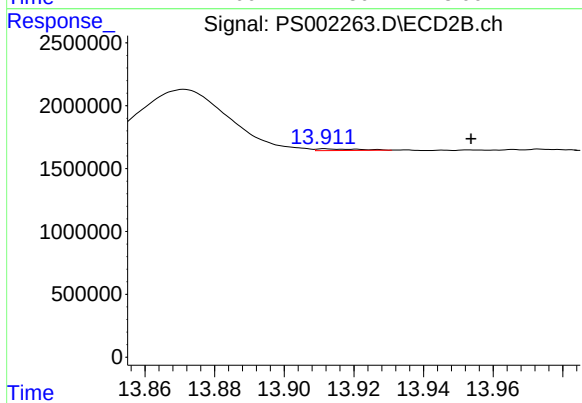

#11 2,4,5-TP (SILVEX)


R.T.: 13.912 min
Delta R.T.: -0.042 min
Response: 105922
Conc: 0.06 ng/ml

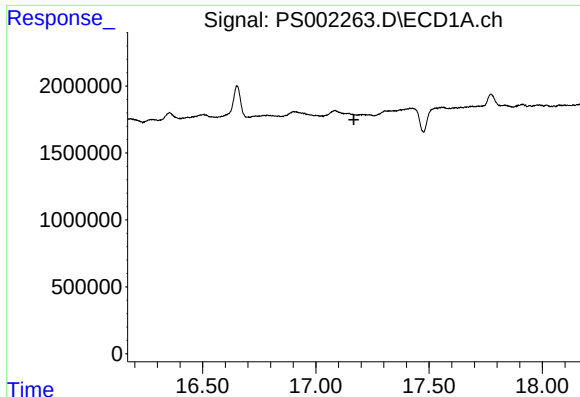

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 17.168 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

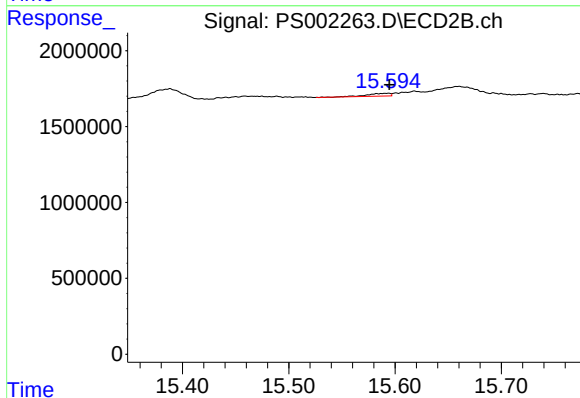


#14 DINOSEB

R.T.: 15.594 min
Delta R.T.: 0.000 min
Response: 278195
Conc: 0.22 ng/ml

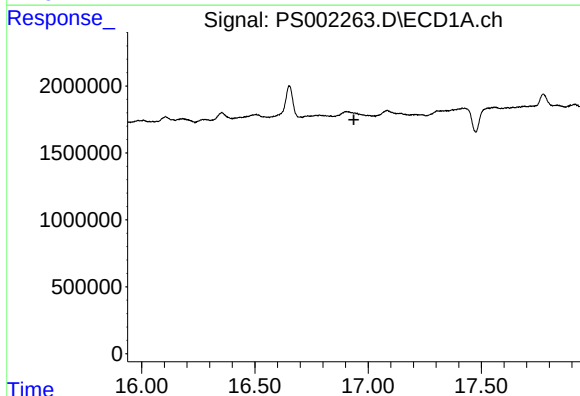


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 16.937 min
Response: 0
Conc: N.D.

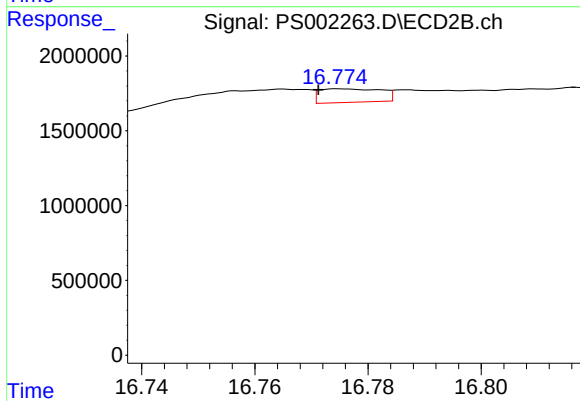

#15 Picloram


R.T.: 16.775 min
Delta R.T.: 0.004 min
Response: 690979
Conc: 0.31 ng/ml

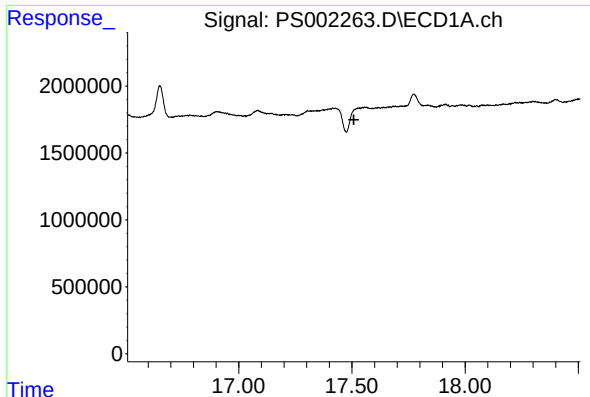

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.509 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

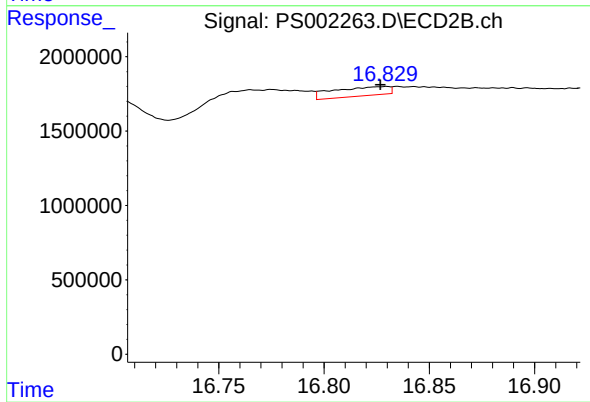

#16 DCPA

R.T.: 16.830 min
Delta R.T.: 0.003 min
Response: 1124057
Conc: 0.47 ng/ml