

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110119\
 Data File : PS007557.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Nov 2019 11:11
 Operator : SM\AJ
 Sample : PB124412BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB124412BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 01 12:44:55 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 14 13:54:23 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.427	5.153	765.2E6	403.8E6	559.060	574.097
Target Compounds							
1) T	Dalapon	1.989	1.699	48366718	37382960	28.905	41.080 #
2) T	3,5-DICHL...	0.000	4.488	0	56464834	N.D.	65.624
5) T	DICAMBA	5.522	5.282	33314689	13687306	6.780	5.260
7) T	MCPA	5.898	5.523	22826752	23936367	4.426	8.234 #
9) T	2,4-D	6.481	0.000	75146602	0	60.979	N.D. #
10) T	Pentachlo...	0.000	6.439	0	14684383	N.D.	1.527
12) T	2,4,5-T	0.000	7.202	0	16623130	N.D.	4.745
15) T	Picloram	8.932	8.892	72135130	57518846	6.536	9.368 #
16) T	DCPA	0.000	8.892	0	57518846	N.D.	11.470



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110119\
Data File : PS007557.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Nov 2019 11:11
Operator : SM\AJ
Sample : PB124412BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
PB124412BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 01 12:44:55 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
Quant Title : 8080.M
QLast Update : Mon Oct 14 13:54:23 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

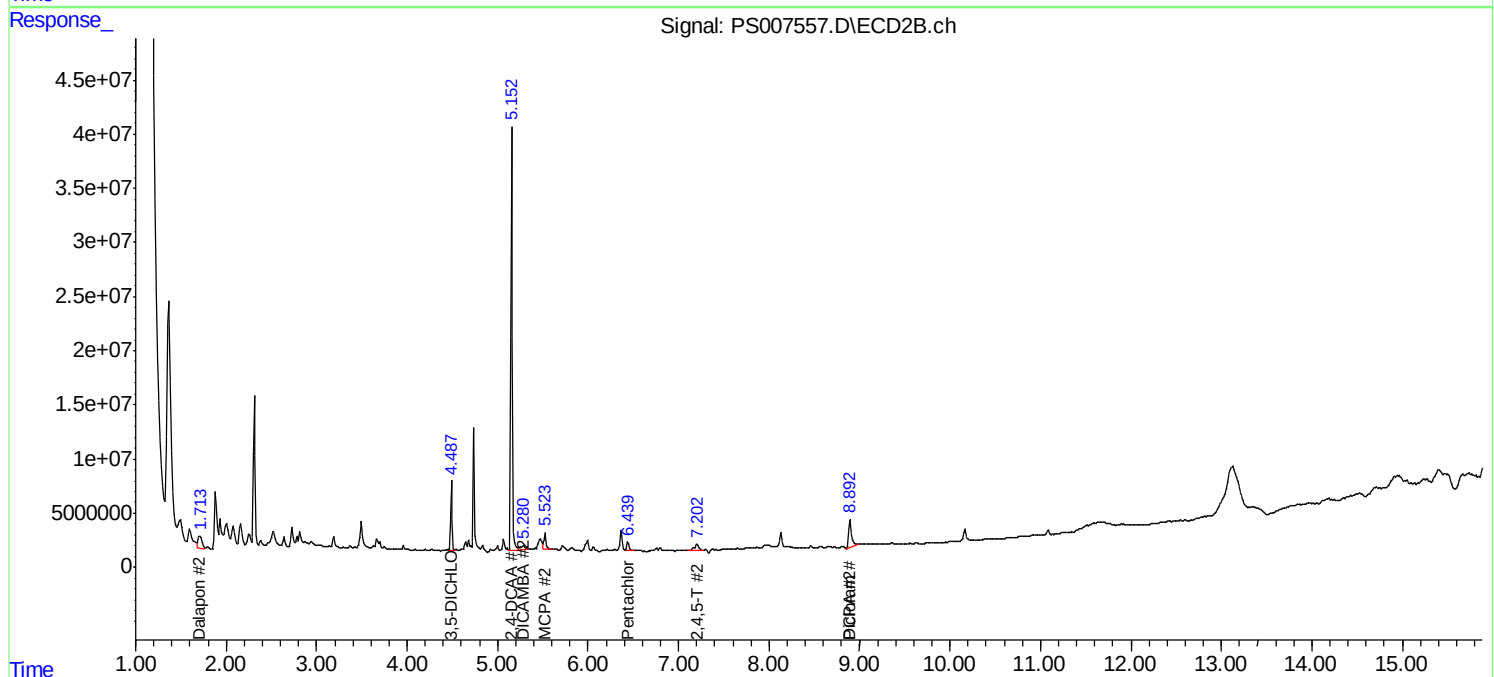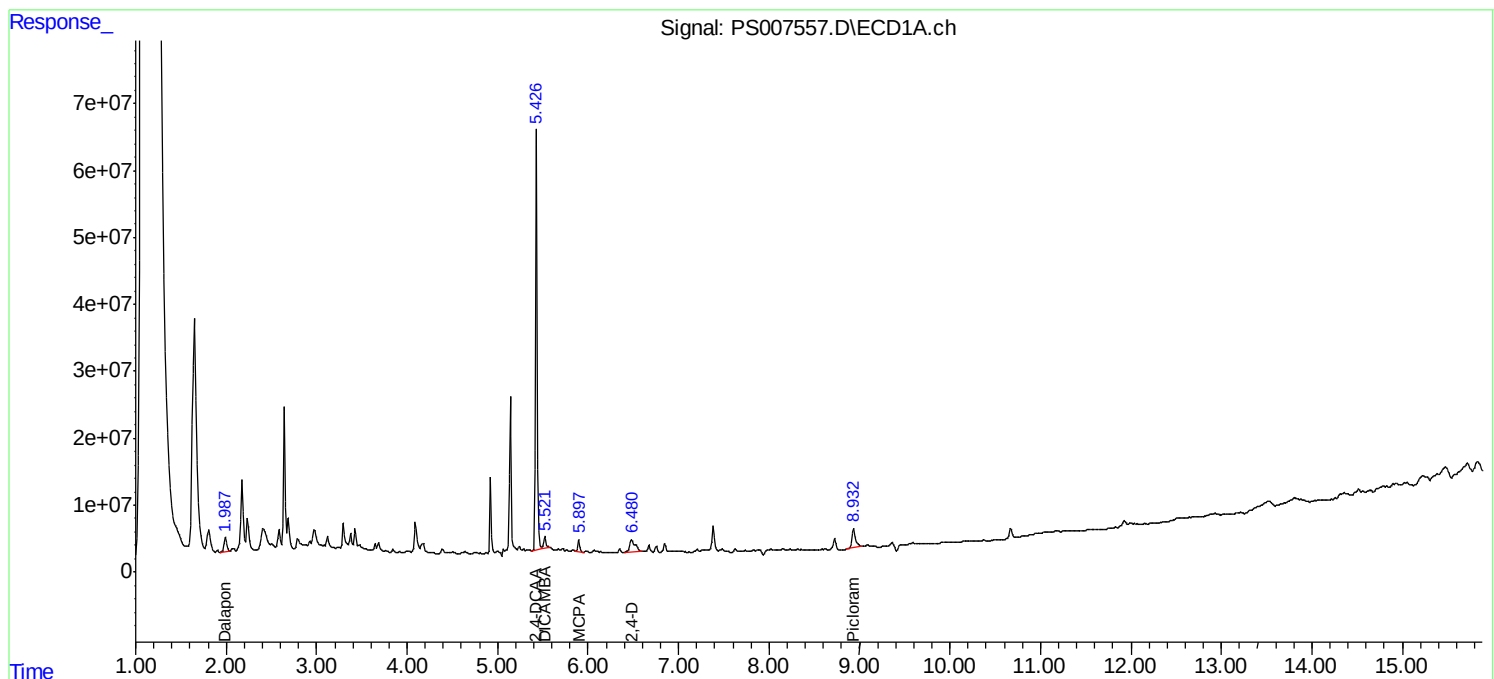


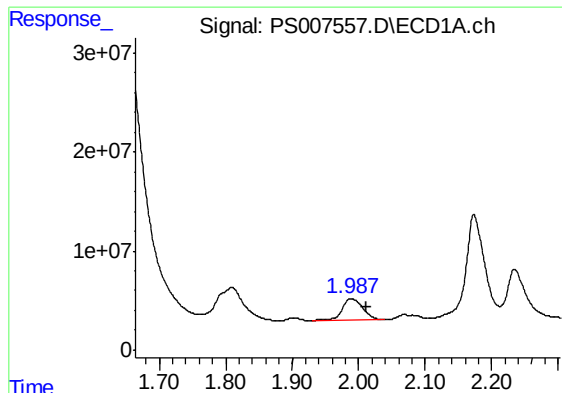

#1 Dalapon


R.T.: 1.989 min
Delta R.T.: -0.022 min
Response: 48366718
Conc: 28.91 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB124412BL

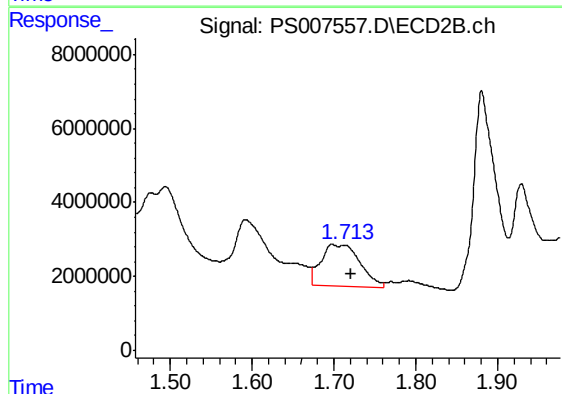


#1 Dalapon

R.T.: 1.699 min
Delta R.T.: -0.022 min
Response: 37382960
Conc: 41.08 ng/ml

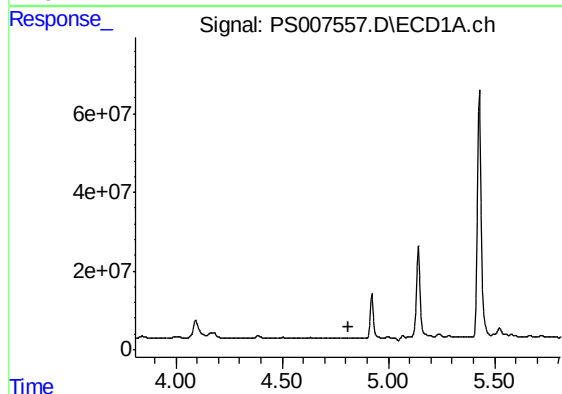


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.810 min
Response: 0
Conc: N.D.

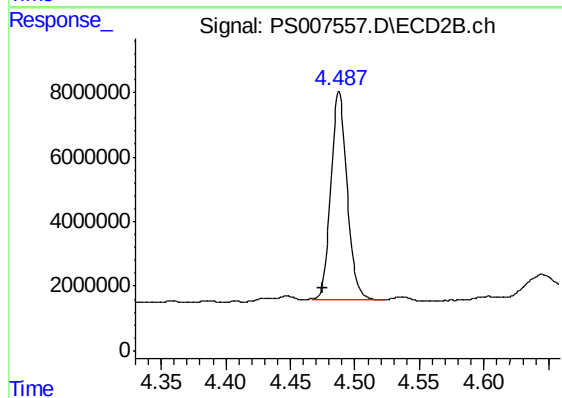

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.488 min
Delta R.T.: 0.013 min
Response: 56464834
Conc: 65.62 ng/ml

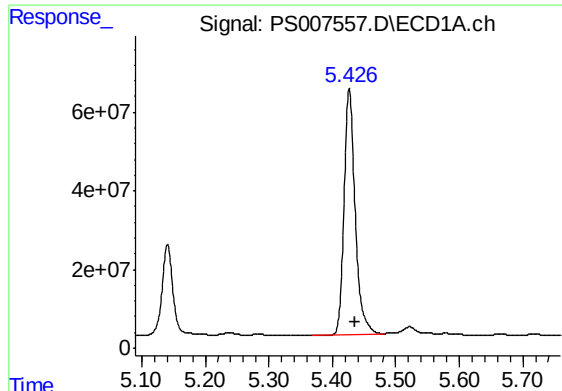

#4 2,4-DCAA


R.T.: 5.427 min
Delta R.T.: -0.009 min
Response: 765168159
Conc: 559.06 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB124412BL

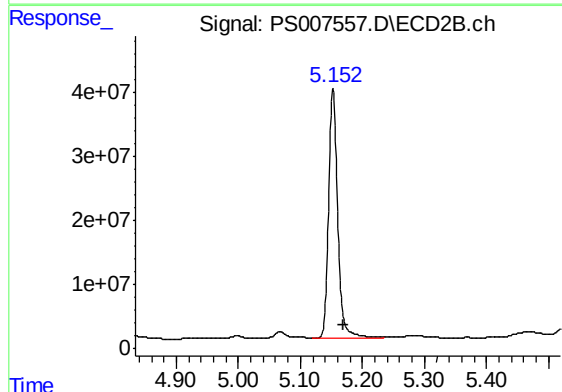


#4 2,4-DCAA

R.T.: 5.153 min
Delta R.T.: -0.016 min
Response: 403766249
Conc: 574.10 ng/ml

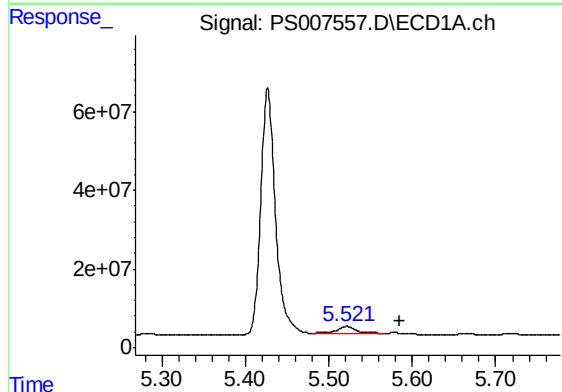


#5 DICAMBA

R.T.: 5.522 min
Delta R.T.: -0.064 min
Response: 33314689
Conc: 6.78 ng/ml

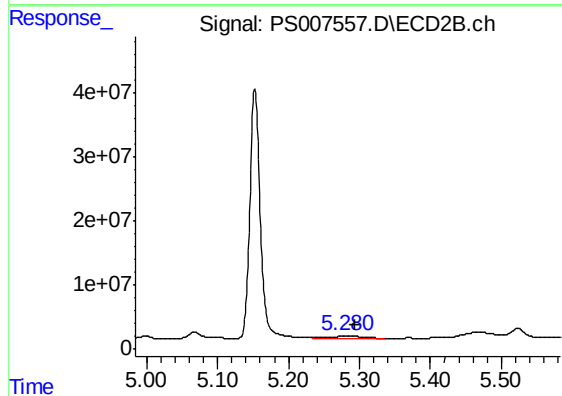

#5 DICAMBA


R.T.: 5.282 min
Delta R.T.: -0.012 min
Response: 13687306
Conc: 5.26 ng/ml

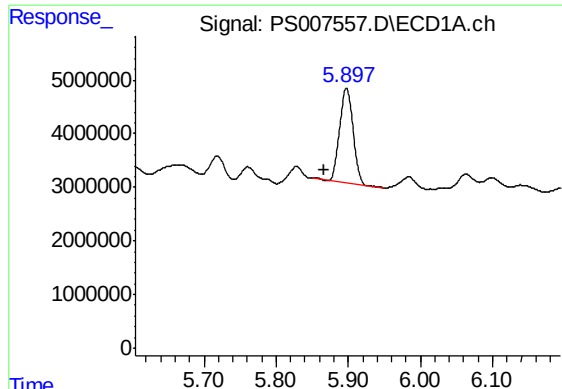

#7 MCPA


R.T.: 5.898 min
Delta R.T.: 0.030 min
Response: 22826752
Conc: 4.43 ug/ml

Instrument :
ECD_S
ClientSampleId :
PB124412BL

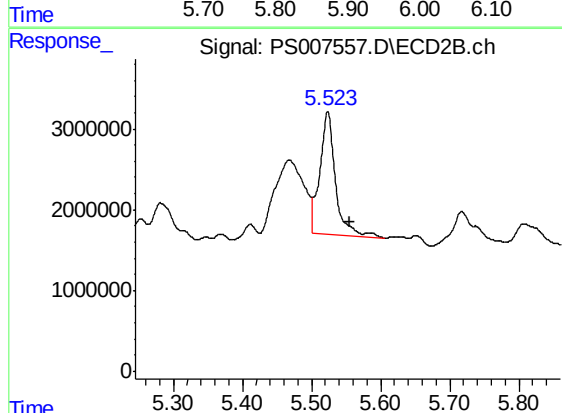


#7 MCPA

R.T.: 5.523 min
Delta R.T.: -0.032 min
Response: 23936367
Conc: 8.23 ug/ml

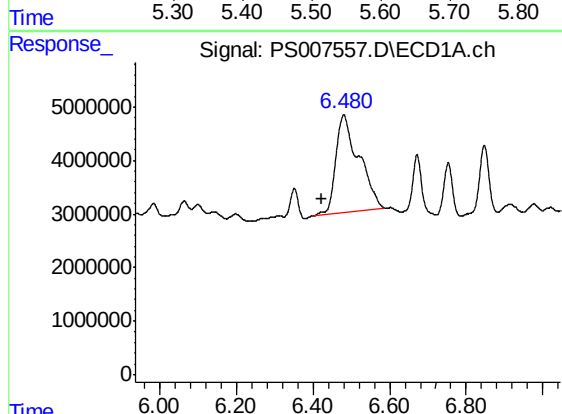


#9 2,4-D

R.T.: 6.481 min
Delta R.T.: 0.056 min
Response: 75146602
Conc: 60.98 ng/ml

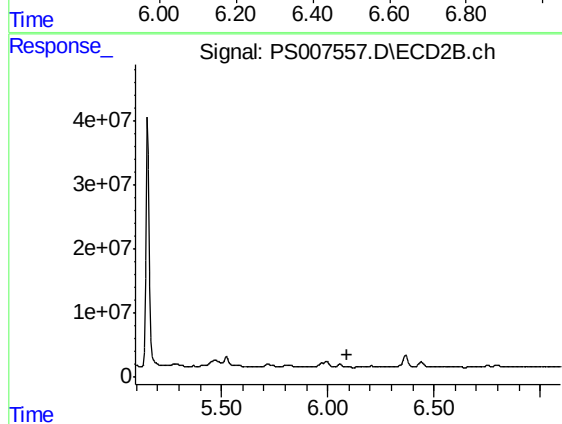

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 6.095 min
Response: 0
Conc: N.D.

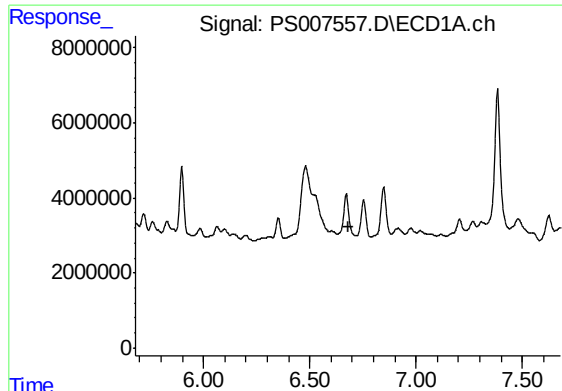

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T. : 6.680 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB124412BL

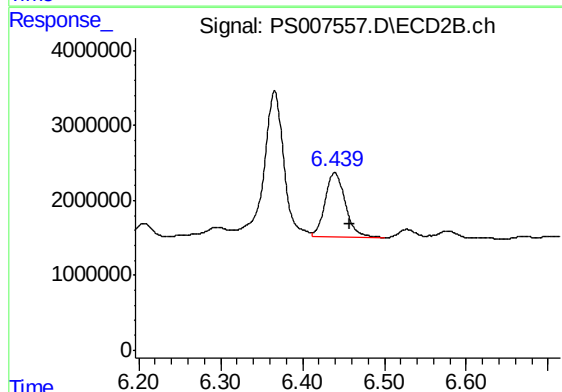


#10 Pentachlorophenol

R.T.: 6.439 min
Delta R.T.: -0.018 min
Response: 14684383
Conc: 1.53 ng/ml

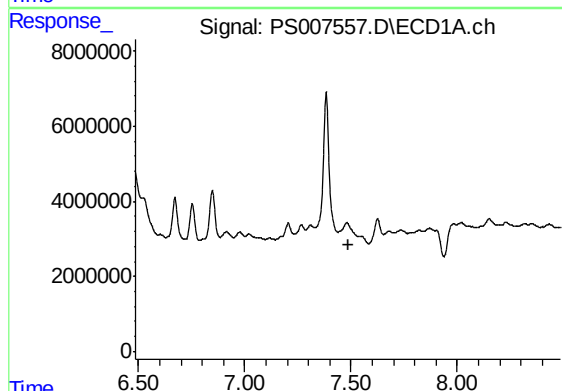


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 7.486 min
Response: 0
Conc: N.D.

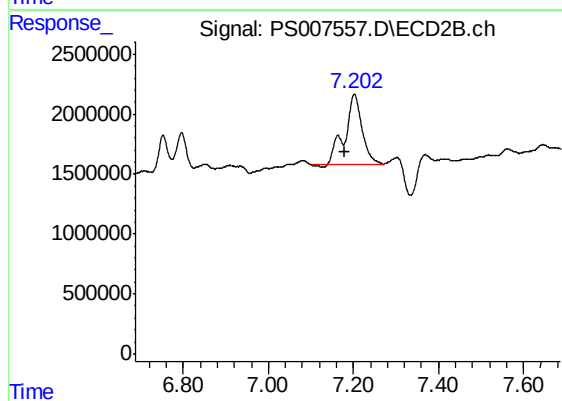

#12 2,4,5-T


R.T.: 7.202 min
Delta R.T.: 0.024 min
Response: 16623130
Conc: 4.74 ng/ml

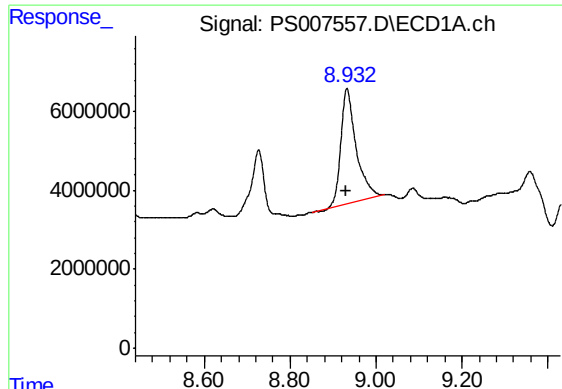

#15 Picloram


R.T.: 8.932 min
Delta R.T.: 0.003 min
Response: 72135130
Conc: 6.54 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB124412BL

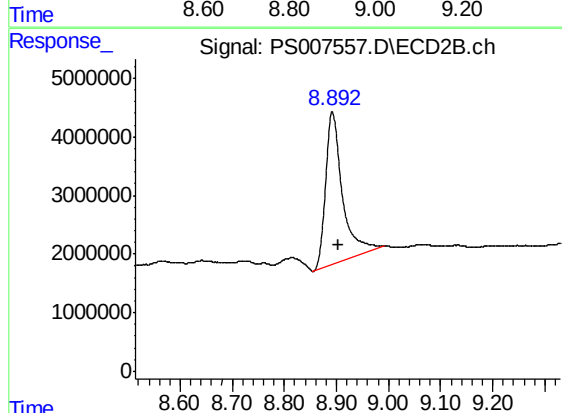


#15 Picloram

R.T.: 8.892 min
Delta R.T.: -0.012 min
Response: 57518846
Conc: 9.37 ng/ml

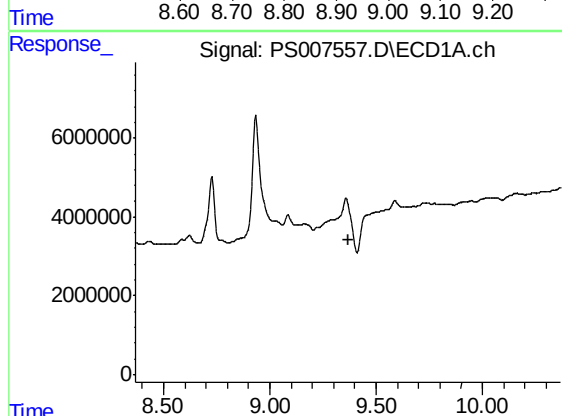

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 9.367 min
Response: 0
Conc: N.D.

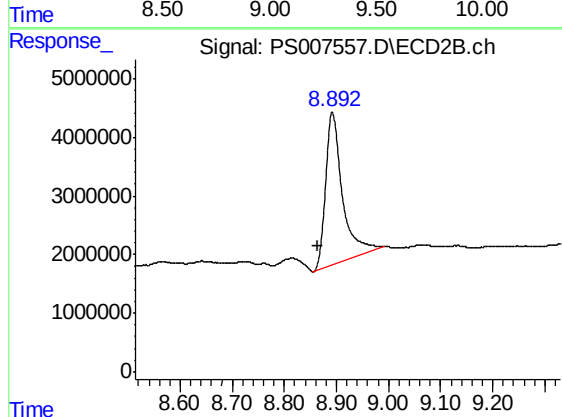

#16 DCPA

R.T.: 8.892 min
Delta R.T.: 0.029 min
Response: 57518846
Conc: 11.47 ng/ml