

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110119\
 Data File : PS007559.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Nov 2019 11:55
 Operator : SM\AJ
 Sample : PB124470BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB124470BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 01 12:45:33 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 14 13:54:23 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.443	5.158	714.9E6	369.8E6	522.350	525.773
Target Compounds							
1) T	Dalapon	2.004	1.702	40351630	38937026	24.115	42.788 #
2) T	3,5-DICHL...	0.000	4.492	0	51231035	N.D.	59.541
5) T	DICAMBA	5.538	0.000	45576059	0	9.276	N.D. #
7) T	MCPA	0.000	5.527	0	21353862	N.D.	7.345
10) T	Pentachlo...	0.000	6.444	0	13085522	N.D.	1.361
12) T	2,4,5-T	0.000	7.209	0	13818902	N.D.	3.944
15) T	Picloram	8.954	8.900	72024455	48291347	6.526	7.865
16) T	DCPA	0.000	8.900	0	48291347	N.D.	9.630



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110119\
Data File : PS007559.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Nov 2019 11:55
Operator : SM\AJ
Sample : PB124470BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
PB124470BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 01 12:45:33 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
Quant Title : 8080.M
QLast Update : Mon Oct 14 13:54:23 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

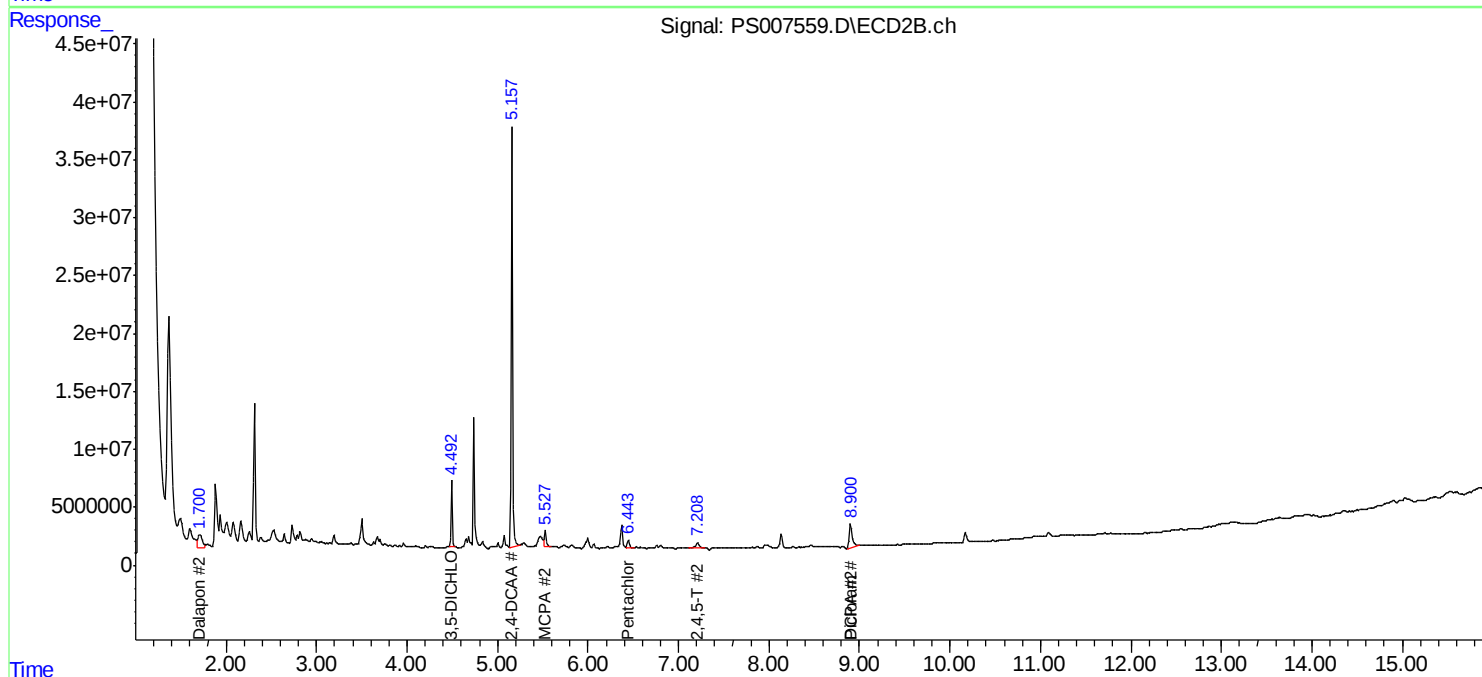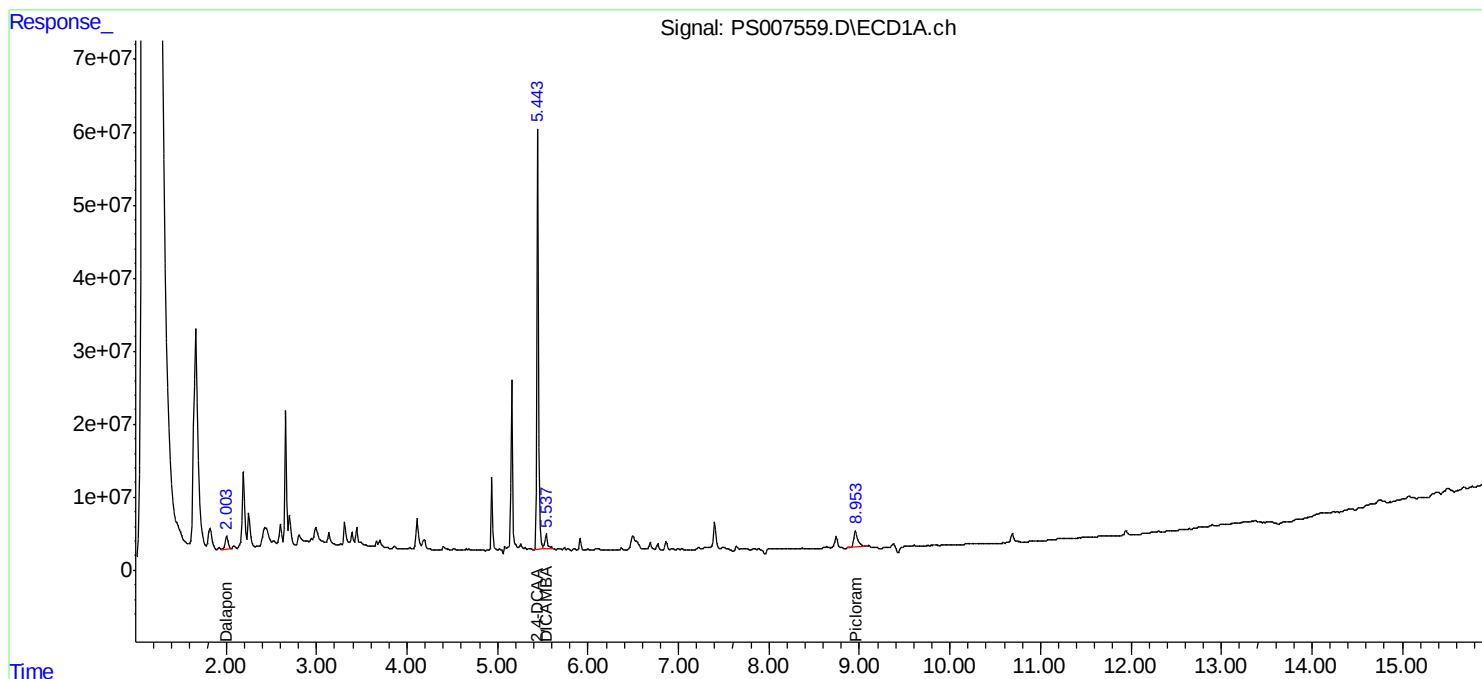


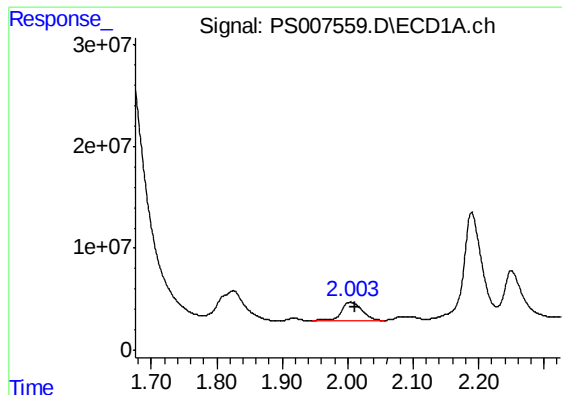

#1 Dalapon


R.T.: 2.004 min
Delta R.T.: -0.007 min
Response: 40351630
Conc: 24.12 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB124470BL

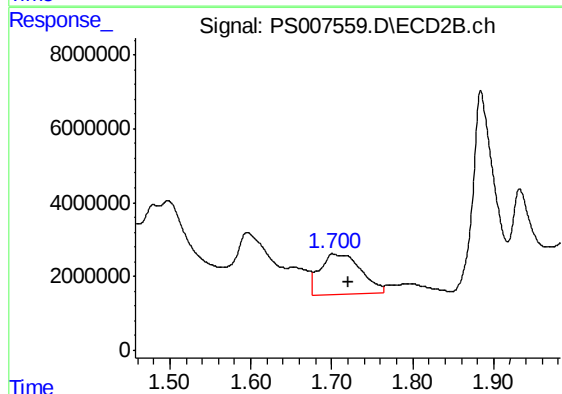


#1 Dalapon

R.T.: 1.702 min
Delta R.T.: -0.018 min
Response: 38937026
Conc: 42.79 ng/ml

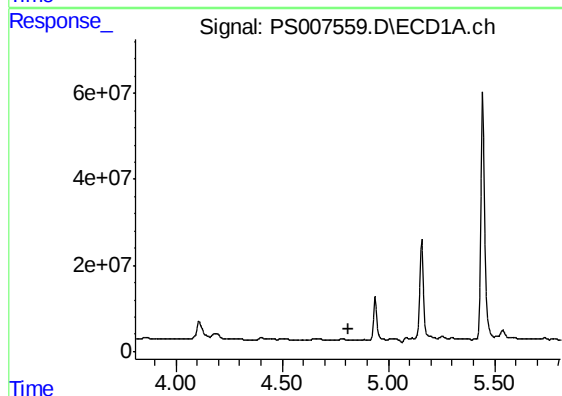


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.810 min
Response: 0
Conc: N.D.

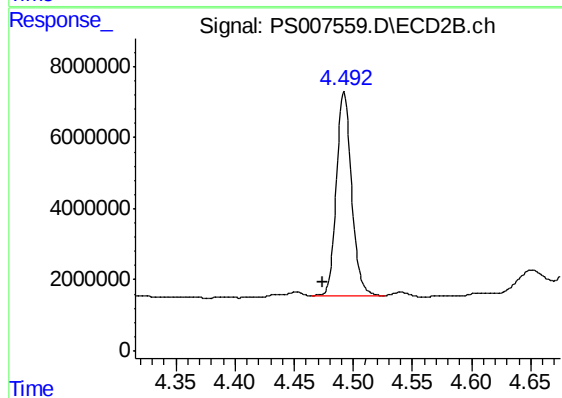

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.492 min
Delta R.T.: 0.017 min
Response: 51231035
Conc: 59.54 ng/ml

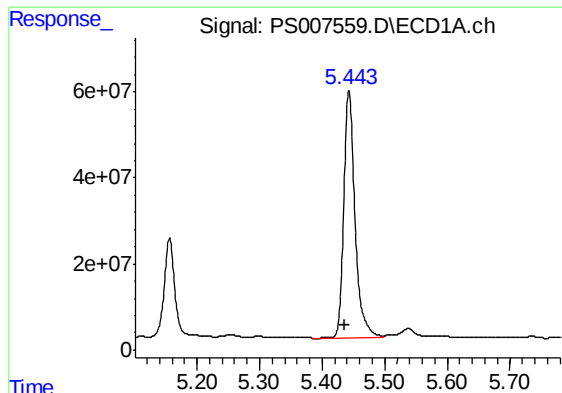

#4 2,4-DCAA


R.T.: 5.443 min
Delta R.T.: 0.007 min
Response: 714924170
Conc: 522.35 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB124470BL

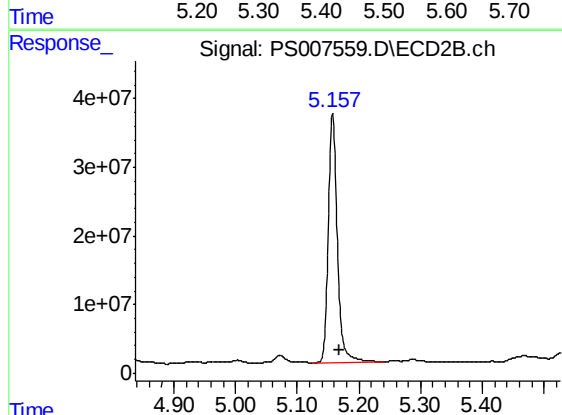


#4 2,4-DCAA

R.T.: 5.158 min
Delta R.T.: -0.011 min
Response: 369779459
Conc: 525.77 ng/ml

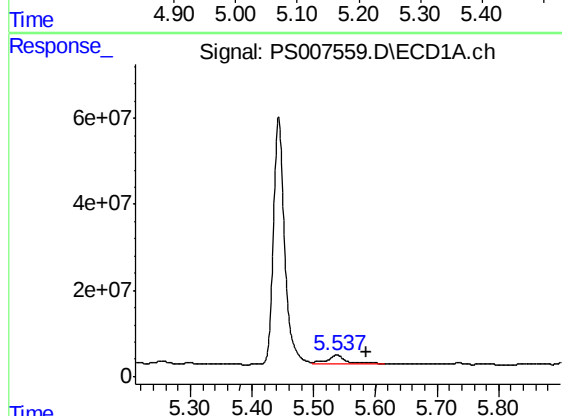


#5 DICAMBA

R.T.: 5.538 min
Delta R.T.: -0.048 min
Response: 45576059
Conc: 9.28 ng/ml

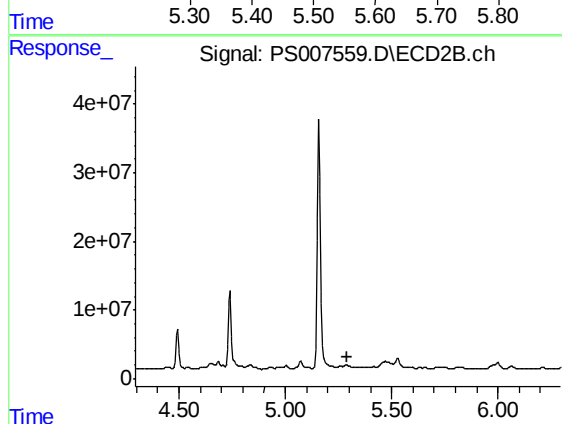

#5 DICAMBA


R.T.: 0.000 min
Exp R.T. : 5.294 min
Response: 0
Conc: N.D.

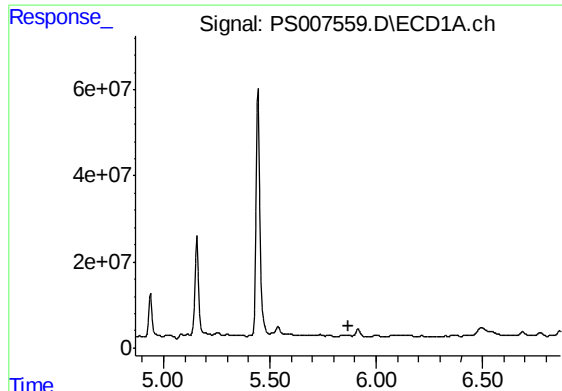

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 5.867 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB124470BL

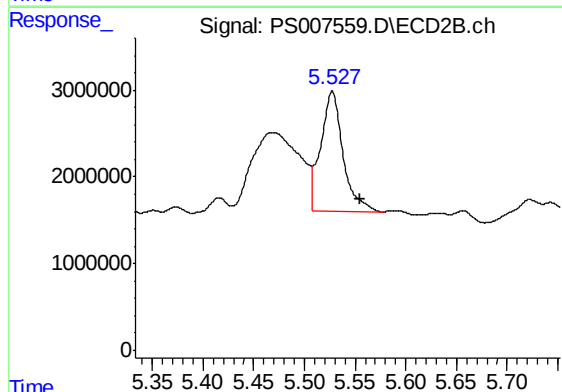


#7 MCPA

R.T.: 5.527 min
Delta R.T.: -0.027 min
Response: 21353862
Conc: 7.35 ug/ml

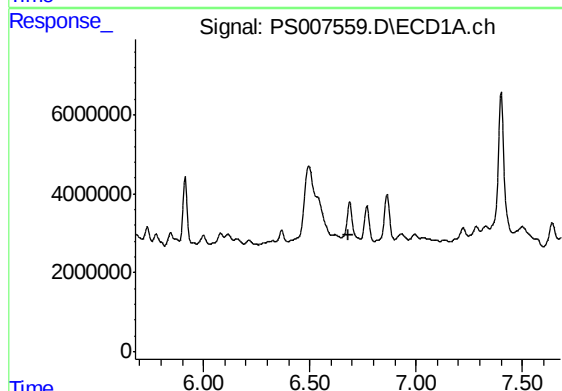


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T.: 6.680 min
Response: 0
Conc: N.D.

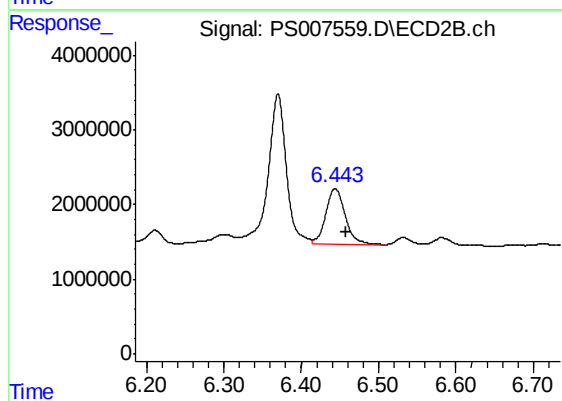

#10 Pentachlorophenol


R.T.: 6.444 min
Delta R.T.: -0.013 min
Response: 13085522
Conc: 1.36 ng/ml

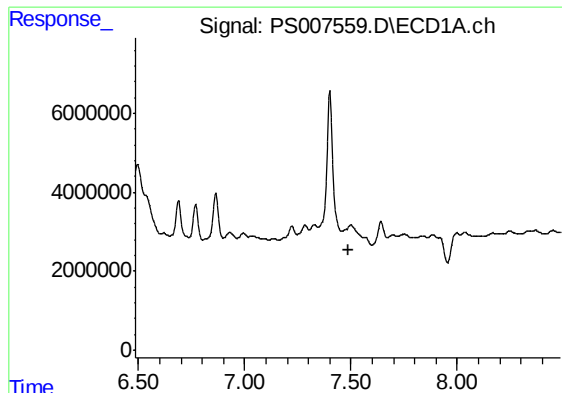

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 7.486 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB124470BL

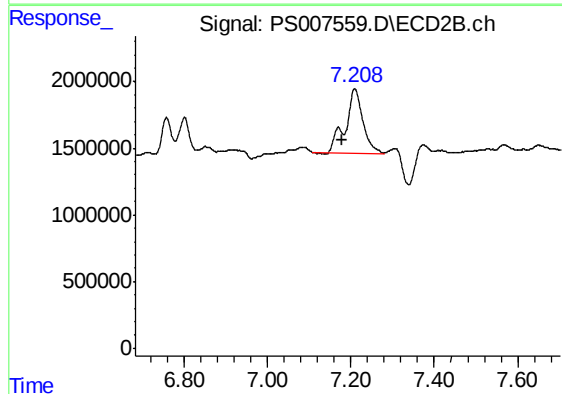


#12 2,4,5-T

R.T.: 7.209 min
Delta R.T.: 0.031 min
Response: 13818902
Conc: 3.94 ng/ml

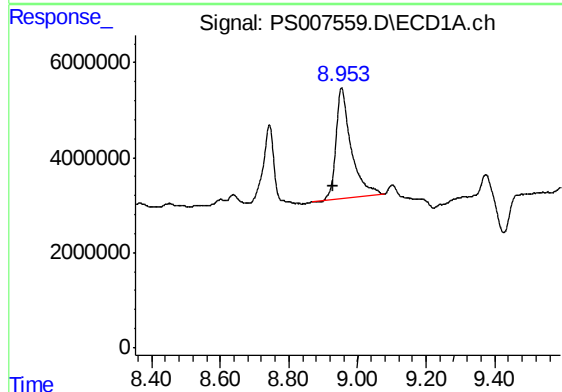


#15 Picloram

R.T.: 8.954 min
Delta R.T.: 0.024 min
Response: 72024455
Conc: 6.53 ng/ml

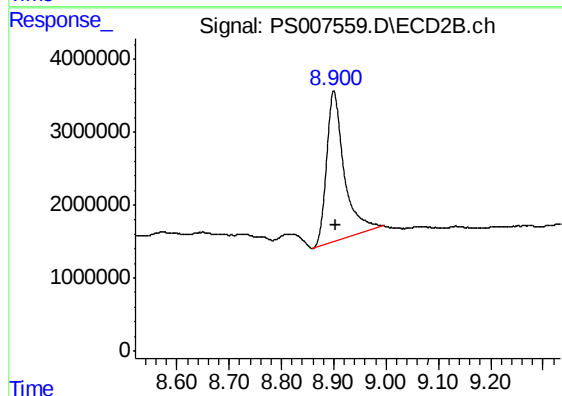

#15 Picloram


R.T.: 8.900 min
Delta R.T.: -0.004 min
Response: 48291347
Conc: 7.86 ng/ml

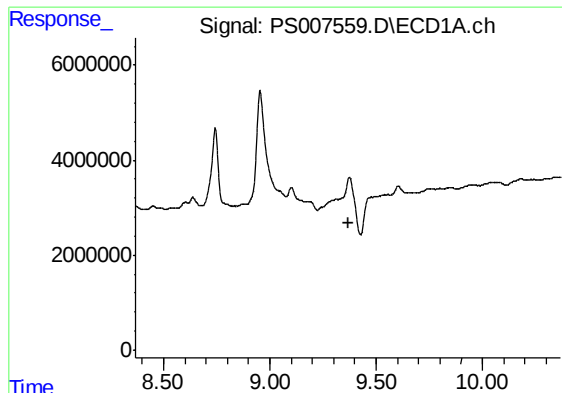

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 9.367 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB124470BL

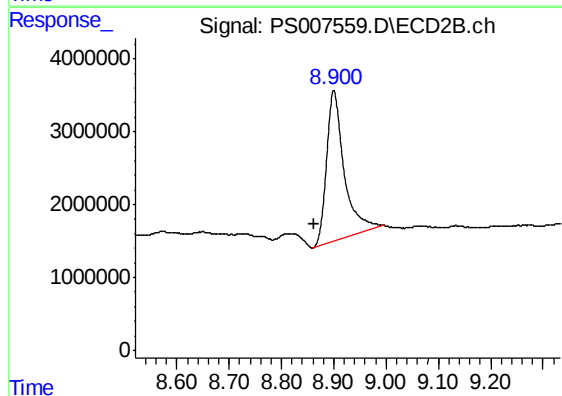

#16 DCPA

R.T.: 8.900 min
Delta R.T.: 0.037 min
Response: 48291347
Conc: 9.63 ng/ml