

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110119\
 Data File : PS007561.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Nov 2019 12:39
 Operator : SM\AJ
 Sample : PB124470TB
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB124470TB

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 01 14:55:03 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 14 13:54:23 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.435	5.160	691.1E6	366.9E6	504.944	521.684
Target Compounds							
1) T	Dalapon	1.996	1.705	37480706	23623247	22.400	25.960
2) T	3,5-DICHL...	0.000	4.495	0	49199048	N.D.	57.180
5) T	DICAMBA	5.529	5.289	37322271	12249124	7.596	4.707 #
7) T	MCPA	0.000	5.530	0	25638129	N.D.	8.819
9) T	2,4-D	6.489	0.000	90201333	0	73.195	N.D. #
10) T	Pentachlo...	0.000	6.447	0	13648157	N.D.	1.419
12) T	2,4,5-T	0.000	7.213	0	13515294	N.D.	3.858
15) T	Picloram	8.949	8.903	67668987	48264851	6.131	7.861 #
16) T	DCPA	0.000	8.903	0	48264851	N.D.	9.625



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110119\
Data File : PS007561.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Nov 2019 12:39
Operator : SM\AJ
Sample : PB124470TB
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
PB124470TB

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 01 14:55:03 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
Quant Title : 8080.M
QLast Update : Mon Oct 14 13:54:23 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

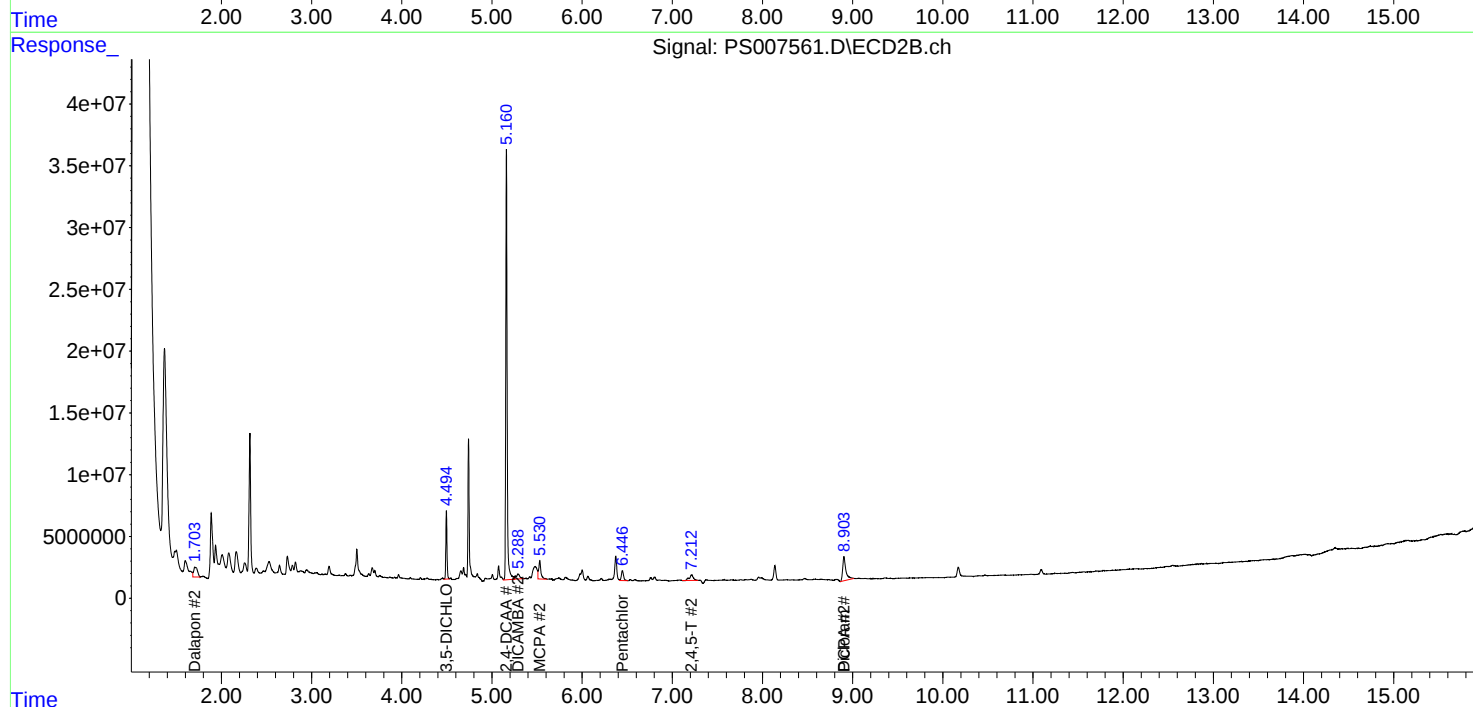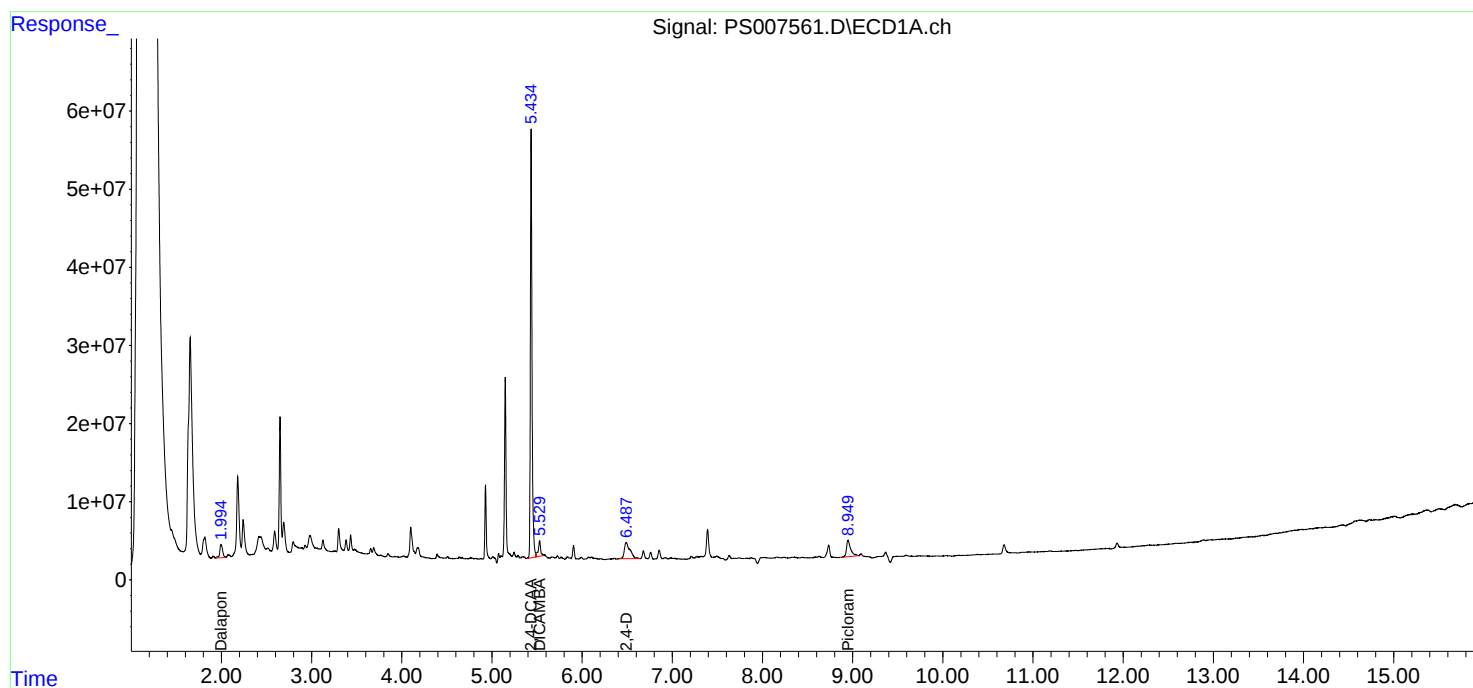


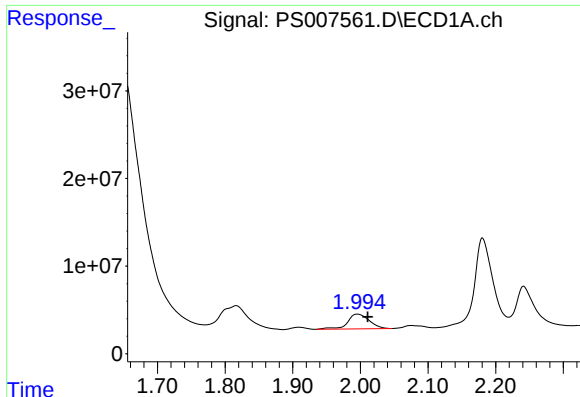

#1 Dalapon


R.T.: 1.996 min
Delta R.T.: -0.015 min
Response: 37480706
Conc: 22.40 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB124470TB

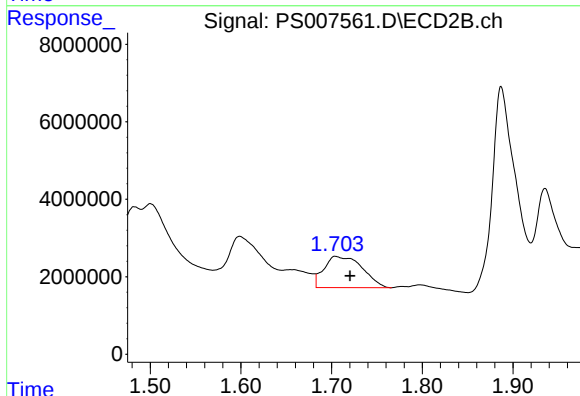


#1 Dalapon

R.T.: 1.705 min
Delta R.T.: -0.015 min
Response: 23623247
Conc: 25.96 ng/ml

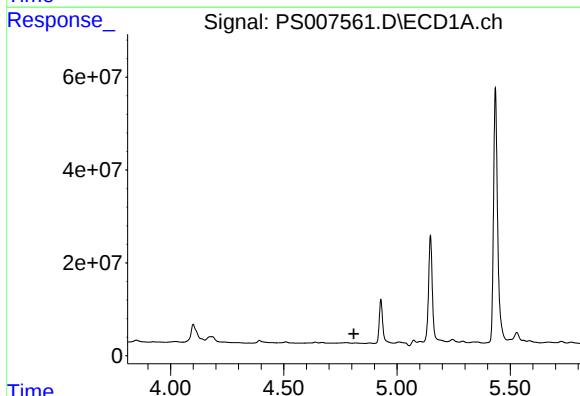


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.810 min
Response: 0
Conc: N.D.

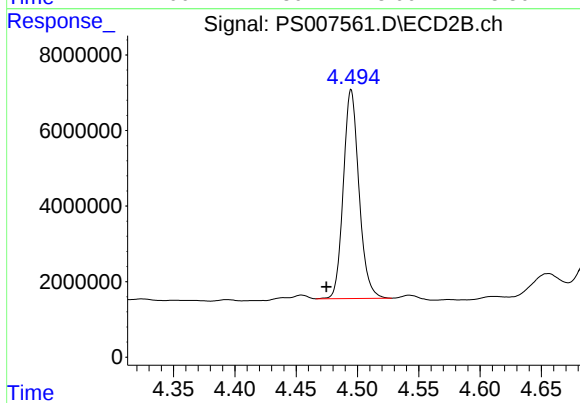

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.495 min
Delta R.T.: 0.020 min
Response: 49199048
Conc: 57.18 ng/ml

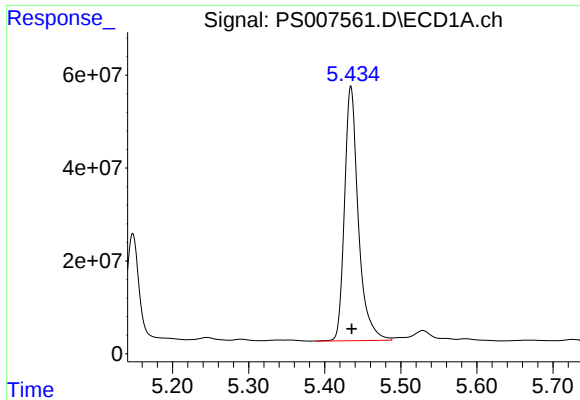

#4 2,4-DCAA


R.T.: 5.435 min
Delta R.T.: -0.001 min
Response: 691100549
Conc: 504.94 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB124470TB

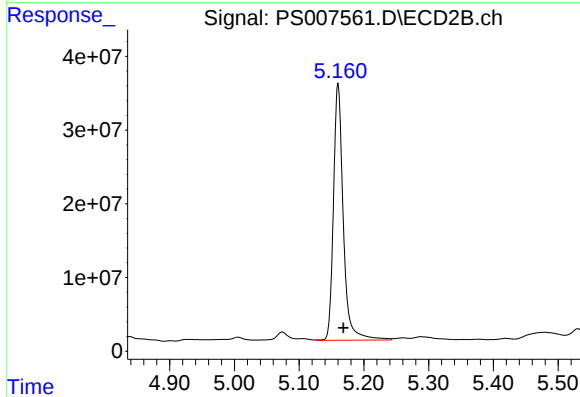


#4 2,4-DCAA

R.T.: 5.160 min
Delta R.T.: -0.008 min
Response: 366903530
Conc: 521.68 ng/ml

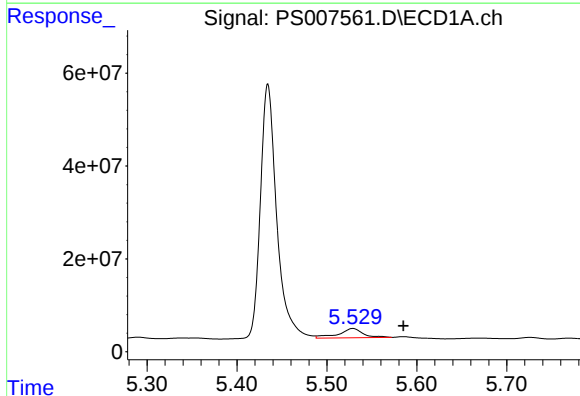


#5 DICAMBA

R.T.: 5.529 min
Delta R.T.: -0.056 min
Response: 37322271
Conc: 7.60 ng/ml

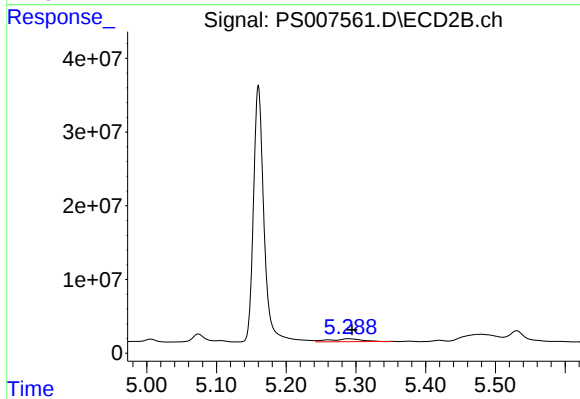

#5 DICAMBA


R.T.: 5.289 min
Delta R.T.: -0.005 min
Response: 12249124
Conc: 4.71 ng/ml

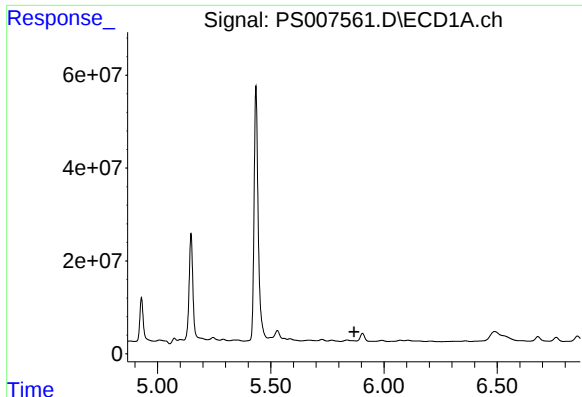

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 5.867 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB124470TB

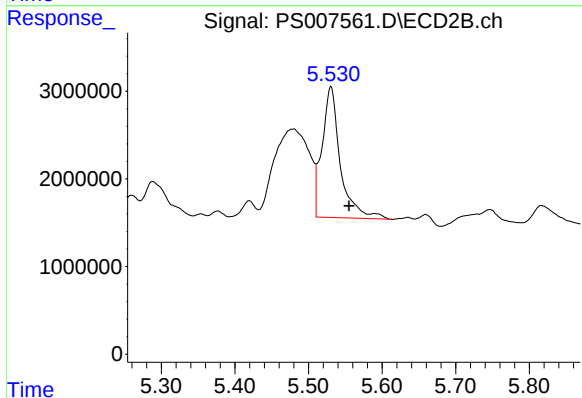


#7 MCPA

R.T.: 5.530 min
Delta R.T.: -0.024 min
Response: 25638129
Conc: 8.82 ug/ml

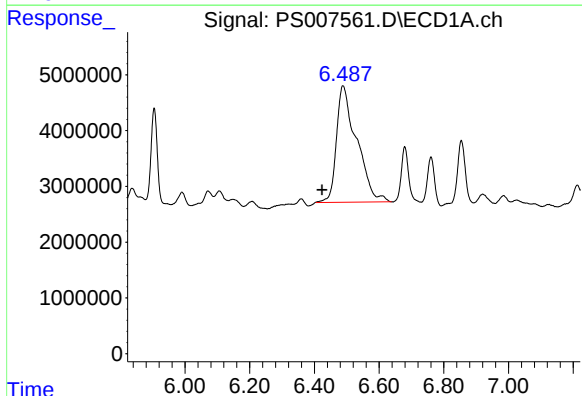


#9 2,4-D

R.T.: 6.489 min
Delta R.T.: 0.064 min
Response: 90201333
Conc: 73.20 ng/ml

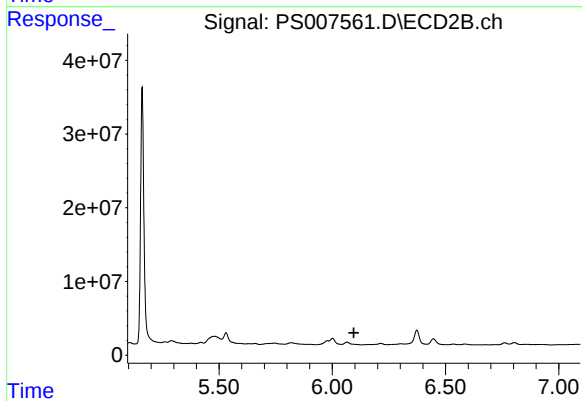

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.095 min
Response: 0
Conc: N.D.

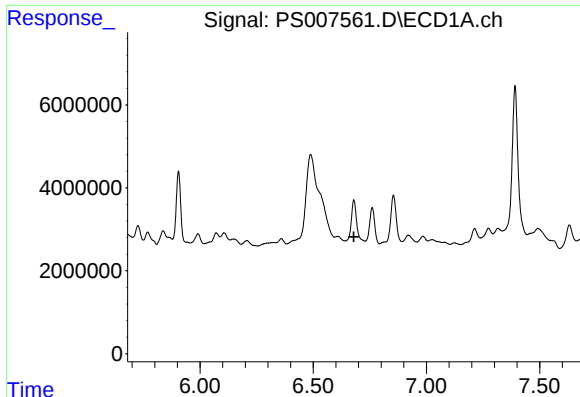

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 6.680 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB124470TB

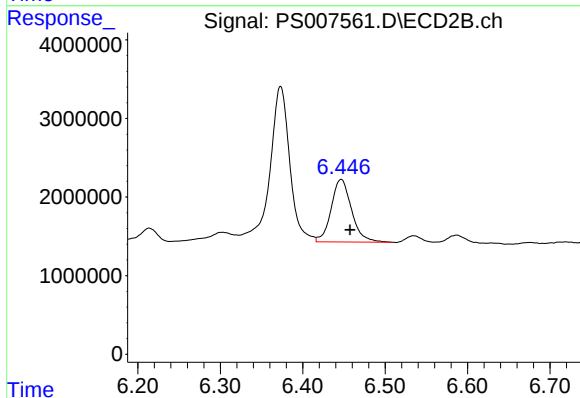


#10 Pentachlorophenol

R.T.: 6.447 min
Delta R.T.: -0.011 min
Response: 13648157
Conc: 1.42 ng/ml

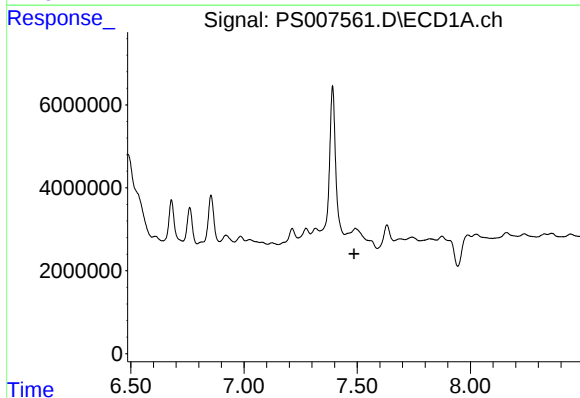


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 7.486 min
Response: 0
Conc: N.D.

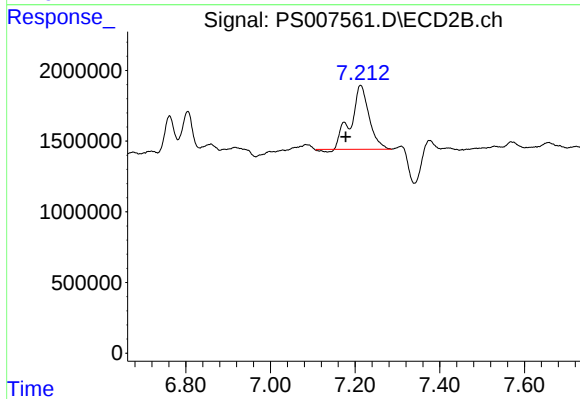

#12 2,4,5-T


R.T.: 7.213 min
Delta R.T.: 0.035 min
Response: 13515294
Conc: 3.86 ng/ml

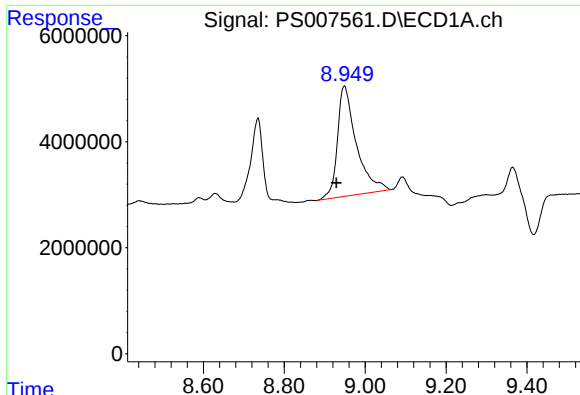

#15 Picloram


R.T.: 8.949 min
Delta R.T.: 0.019 min
Response: 67668987
Conc: 6.13 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB124470TB

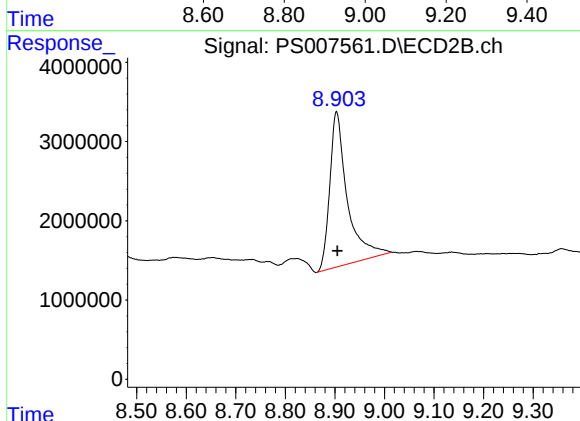


#15 Picloram

R.T.: 8.903 min
Delta R.T.: -0.001 min
Response: 48264851
Conc: 7.86 ng/ml

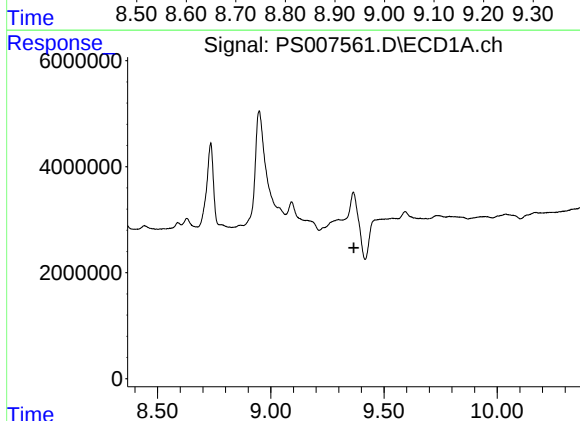

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 9.367 min
Response: 0
Conc: N.D.

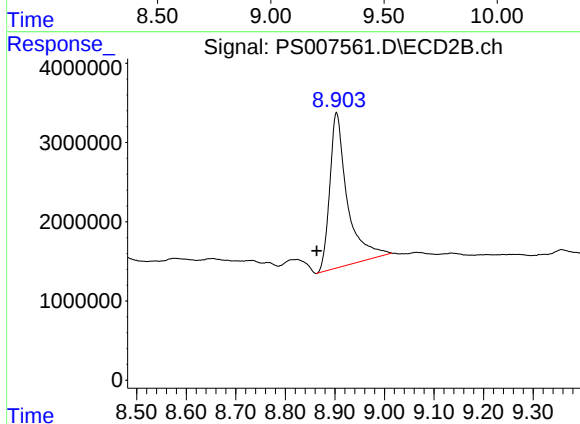

#16 DCPA

R.T.: 8.903 min
Delta R.T.: 0.040 min
Response: 48264851
Conc: 9.62 ng/ml