

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS110119\  
 Data File : PS007575.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 01 Nov 2019 17:46  
 Operator : SM\AJ  
 Sample : I.BLK  
 Misc :  
 ALS Vial : 2 Sample Multiplier: 1

Instrument :  
 ECD\_S  
 ClientSampleId :  
 I.BLK

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Nov 01 23:27:15 2019  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS101419.M  
 Quant Title : 8080.M  
 QLast Update : Mon Oct 14 13:54:23 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

|                             | Compound | RT#1  | RT#2  | Resp#1     | Resp#2  | ng/ml   | ng/ml   |
|-----------------------------|----------|-------|-------|------------|---------|---------|---------|
| -----                       |          |       |       |            |         |         |         |
| System Monitoring Compounds |          |       |       |            |         |         |         |
| 4) S                        | 2,4-DCAA | 5.454 | 5.178 | 598.8E6    | 305.1E6 | 437.521 | 433.777 |
| Target Compounds            |          |       |       |            |         |         |         |
| 7) T                        | MCPA     | 0.000 | 5.499 | 0 43404311 | N.D.    | 14.930  |         |
| -----                       |          |       |       |            |         |         |         |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS110119\  
Data File : PS007575.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 01 Nov 2019 17:46  
Operator : SM\AJ  
Sample : I.BLK  
Misc :  
ALS Vial : 2 Sample Multiplier: 1

Instrument :  
ECD\_S  
ClientSampleId :  
I.BLK

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Nov 01 23:27:15 2019  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS101419.M  
Quant Title : 8080.M  
QLast Update : Mon Oct 14 13:54:23 2019  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2 µl  
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

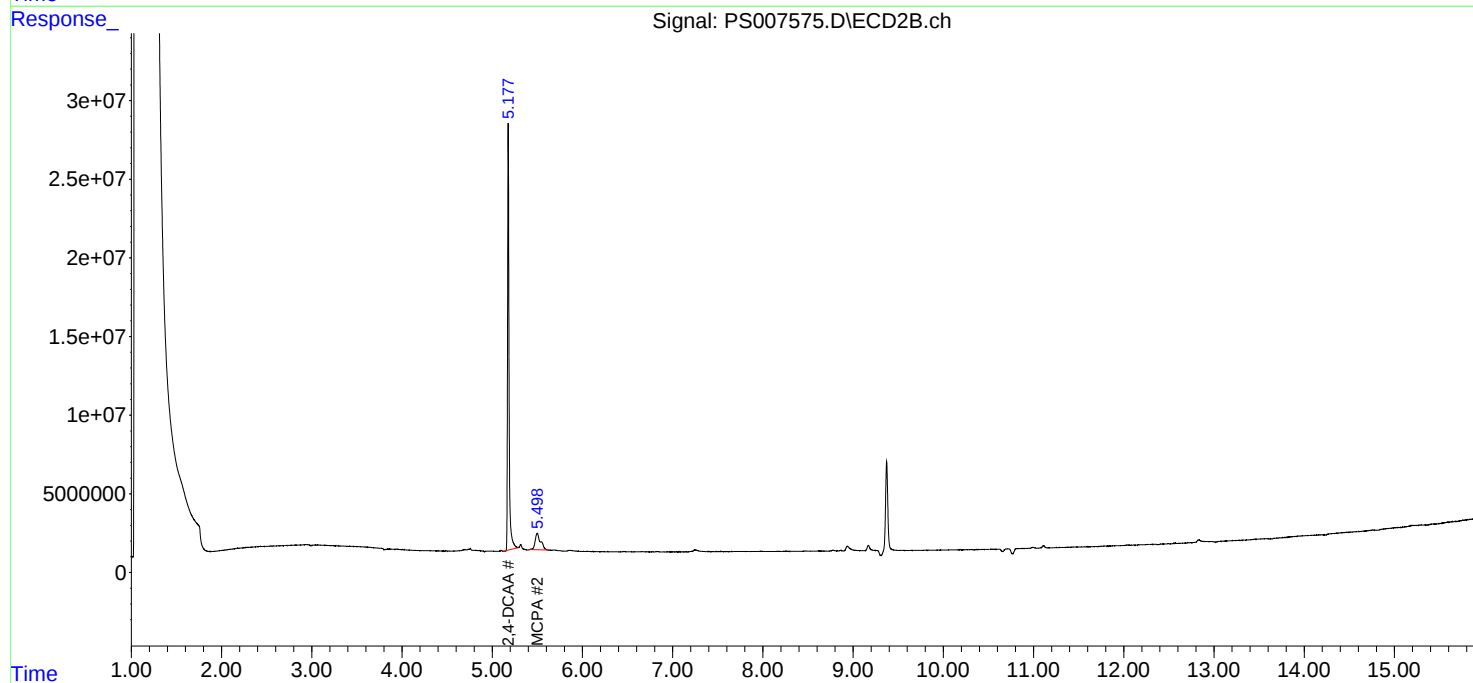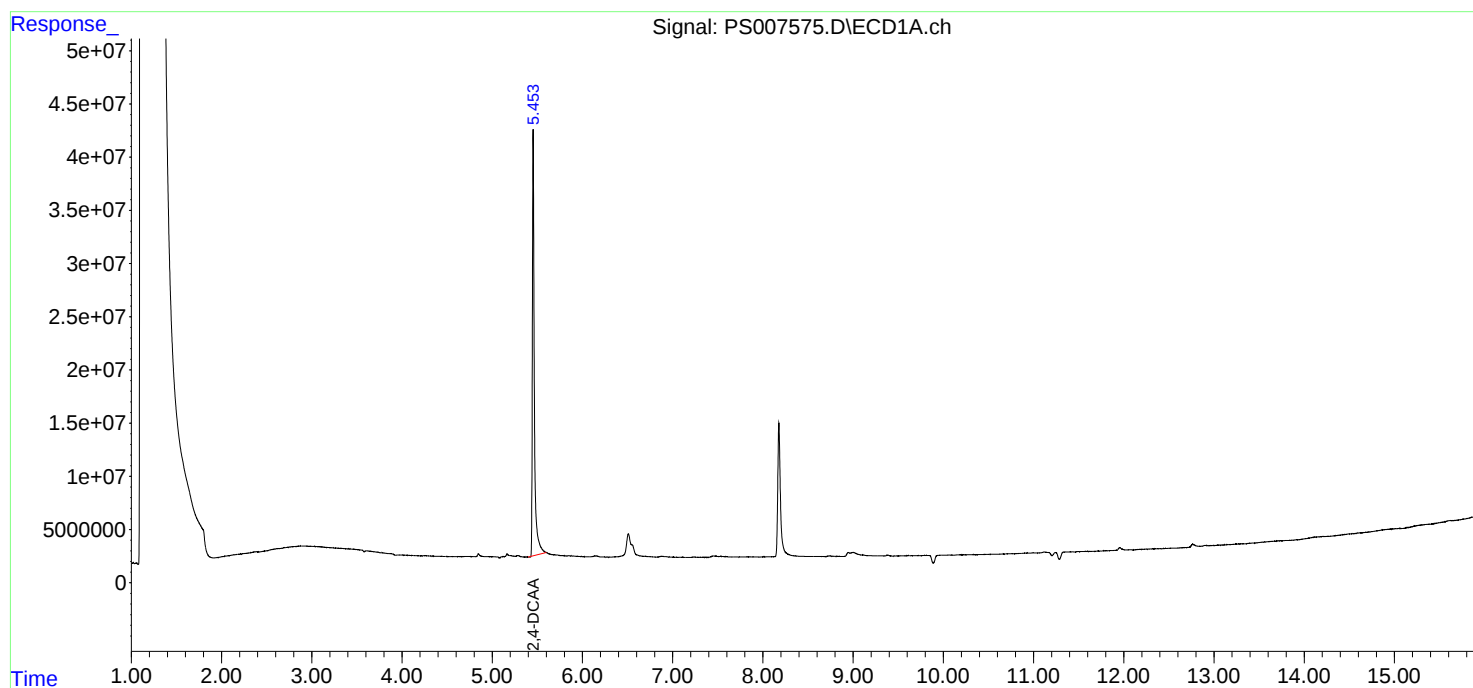


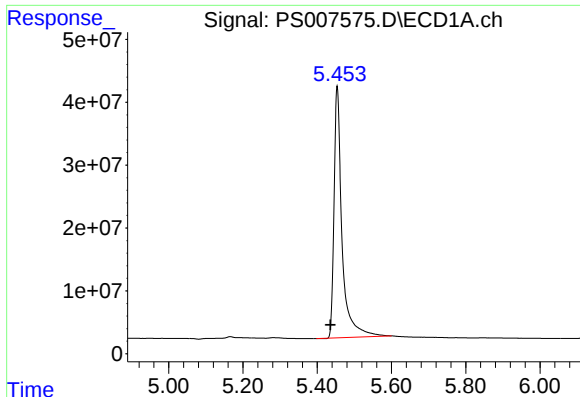

#4 2,4-DCAA


R.T.: 5.454 min  
Delta R.T.: 0.018 min  
Response: 598821728  
Conc: 437.52 ng/ml

Instrument :  
ECD\_S  
ClientSampleId :  
I.BLK

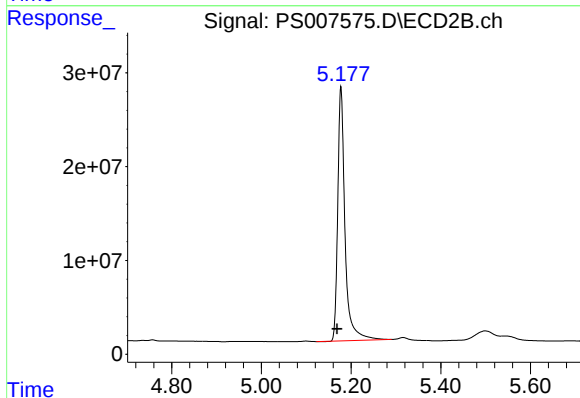


#4 2,4-DCAA

R.T.: 5.178 min  
Delta R.T.: 0.009 min  
Response: 305078165  
Conc: 433.78 ng/ml

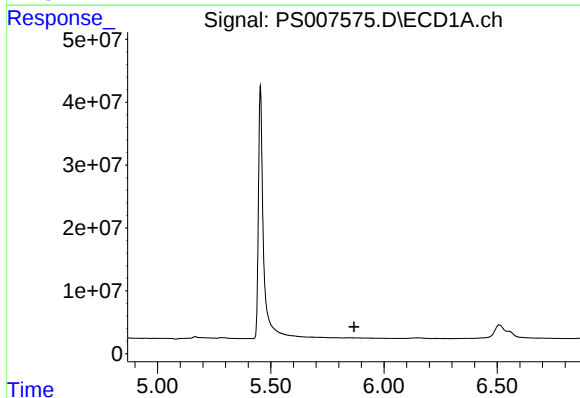

#7 MCPA

R.T.: 0.000 min  
Exp R.T. : 5.867 min  
Response: 0  
Conc: N.D.

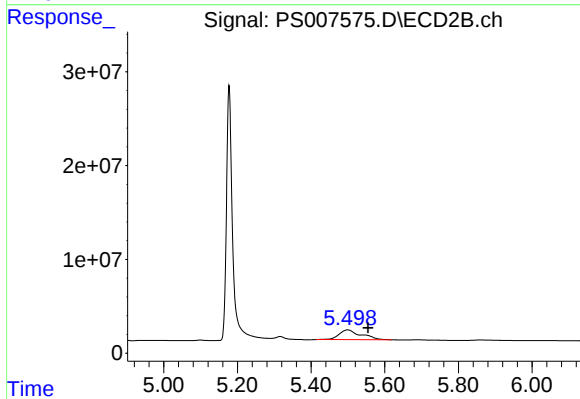

#7 MCPA

R.T.: 5.499 min  
Delta R.T.: -0.056 min  
Response: 43404311  
Conc: 14.93 ug/ml