

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110119\
 Data File : PS007580.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Nov 2019 19:36
 Operator : SM\AJ
 Sample : K5599-03
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 Z3-20B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 01 23:29:13 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 14 13:54:23 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.445	5.171	809.4E6	340.5E6	591.402	484.124
Target Compounds							
1) T	Dalapon	0.000	1.673	0	561.4E6	N.D.	616.927
2) T	3,5-DICHL...	0.000	4.506	0	46213127	N.D.	53.709
5) T	DICAMBA	5.541	5.287	46130000	8955270	9.389	3.442 #
7) T	MCPA	0.000	5.542	0	26112302	N.D.	8.982
9) T	2,4-D	0.000	6.045	0	9120033	N.D.	11.432
10) T	Pentachlo...	6.678	0.000	28254920	0	1.583	N.D. #
11) T	2,4,5-TP ...	0.000	6.855	0	14047670	N.D.	3.693
14) T	DINOSEB	0.000	7.998	0	16778536	N.D.	5.977
15) T	Picloram	0.000	8.913	0	27665598	N.D.	4.506
16) T	DCPA	0.000	8.913	0	27665598	N.D.	5.517



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110119\
Data File : PS007580.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Nov 2019 19:36
Operator : SM\AJ
Sample : K5599-03
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
Z3-20B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 01 23:29:13 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
Quant Title : 8080.M
QLast Update : Mon Oct 14 13:54:23 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

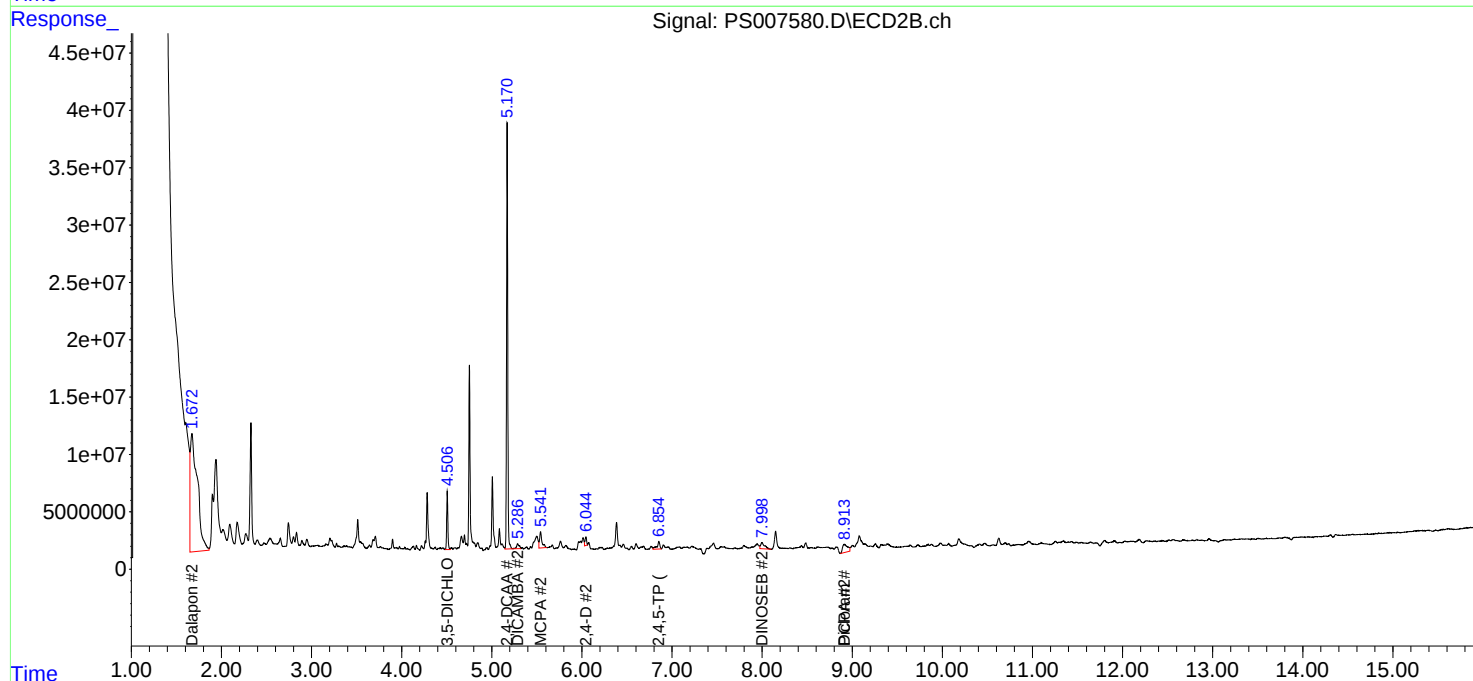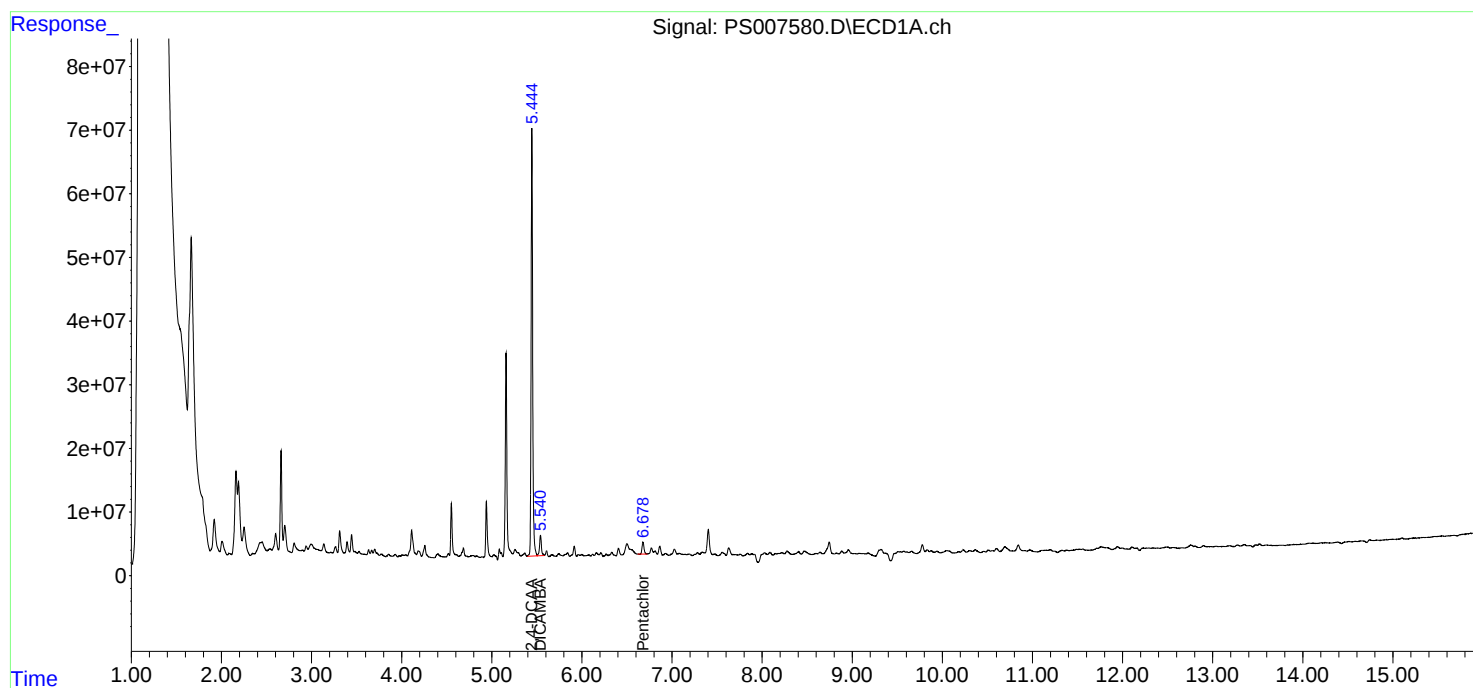


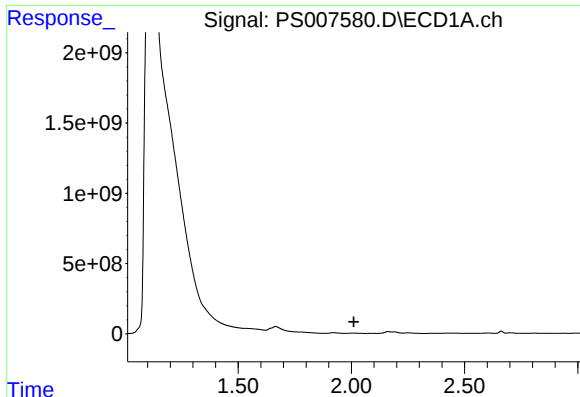

#1 Dalapon


R.T.: 0.000 min
Exp R.T. : 2.011 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
Z3-20B

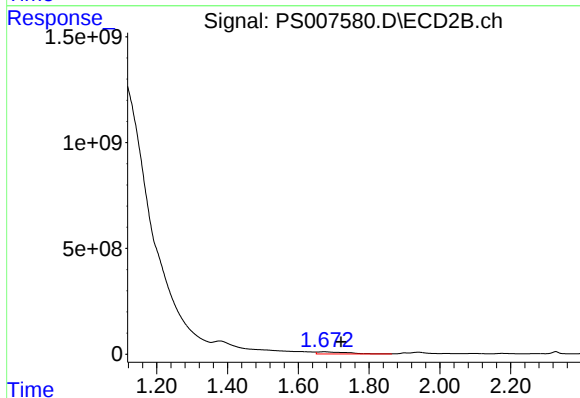


#1 Dalapon

R.T.: 1.673 min
Delta R.T.: -0.048 min
Response: 561405749
Conc: 616.93 ng/ml

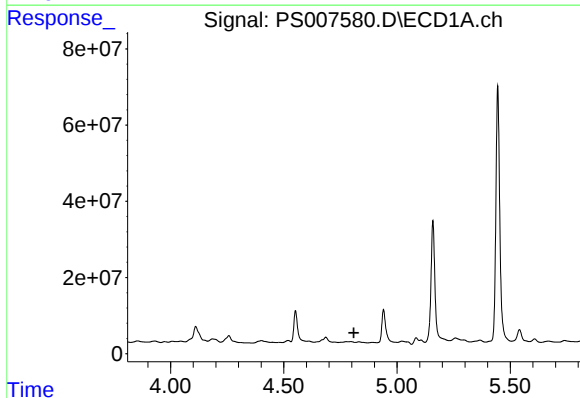


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.810 min
Response: 0
Conc: N.D.

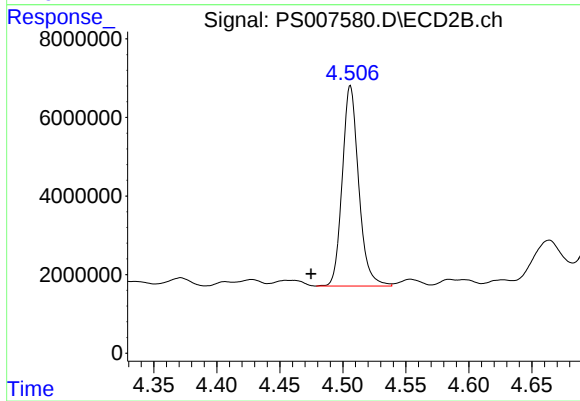

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.506 min
Delta R.T.: 0.031 min
Response: 46213127
Conc: 53.71 ng/ml

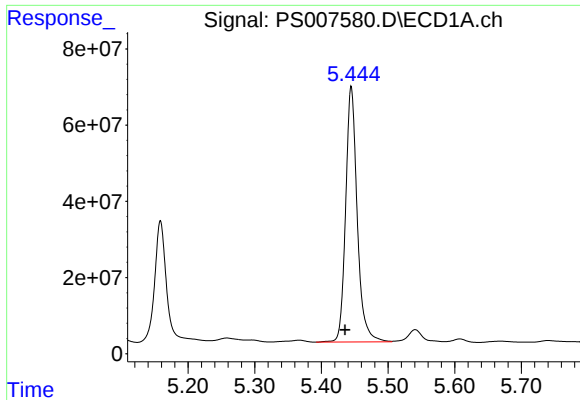

#4 2,4-DCAA


R.T.: 5.445 min
Delta R.T.: 0.009 min
Response: 809433238
Conc: 591.40 ng/ml

Instrument :
ECD_S
ClientSampleId :
Z3-20B

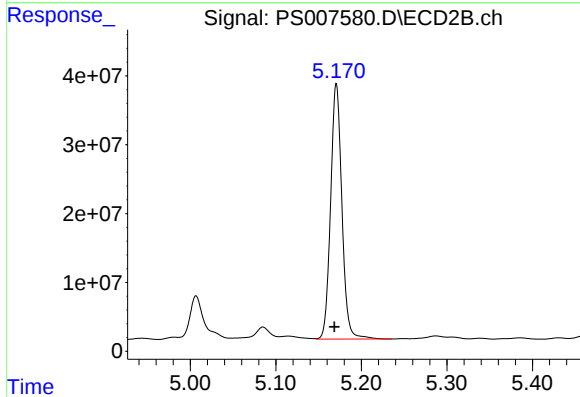


#4 2,4-DCAA

R.T.: 5.171 min
Delta R.T.: 0.002 min
Response: 340487882
Conc: 484.12 ng/ml

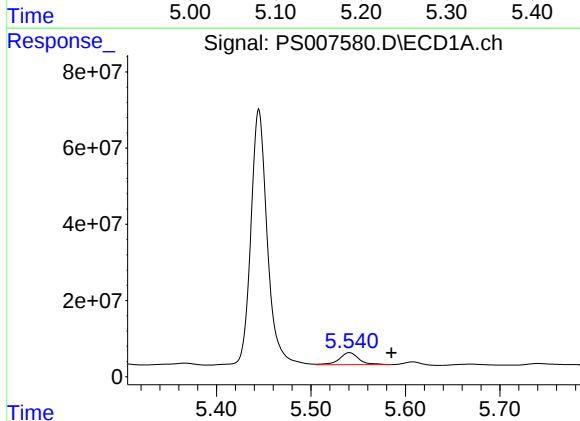


#5 DICAMBA

R.T.: 5.541 min
Delta R.T.: -0.044 min
Response: 46130000
Conc: 9.39 ng/ml

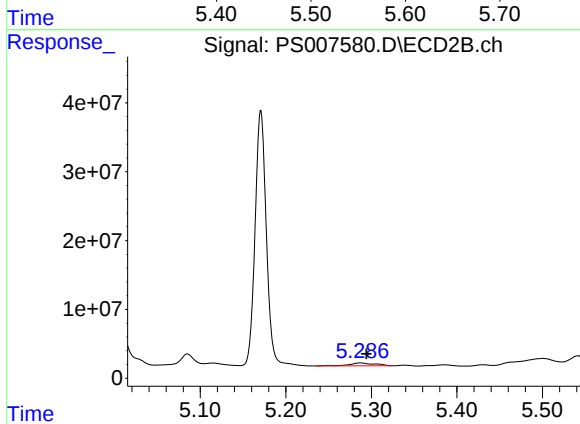

#5 DICAMBA


R.T.: 5.287 min
Delta R.T.: -0.007 min
Response: 8955270
Conc: 3.44 ng/ml

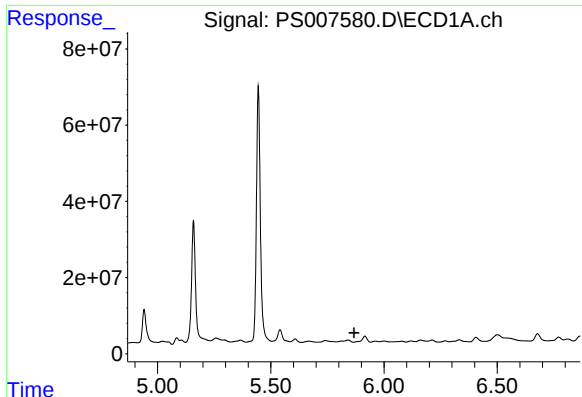

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 5.867 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
Z3-20B

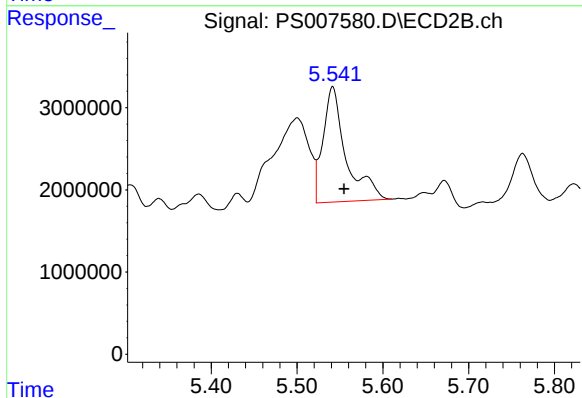


#7 MCPA

R.T.: 5.542 min
Delta R.T.: -0.013 min
Response: 26112302
Conc: 8.98 ug/ml

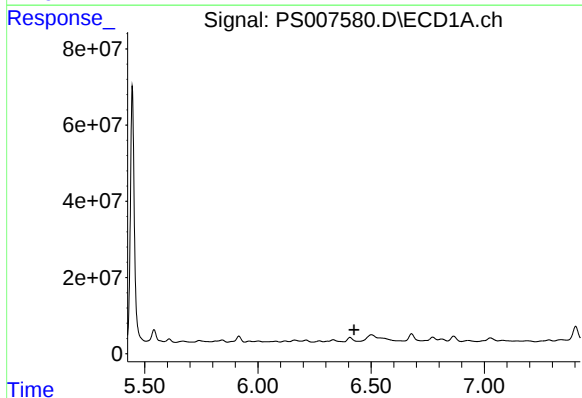


#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 6.424 min
Response: 0
Conc: N.D.

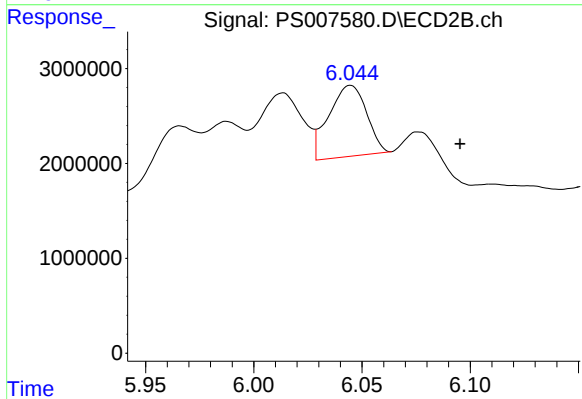

#9 2,4-D


R.T.: 6.045 min
Delta R.T.: -0.051 min
Response: 9120033
Conc: 11.43 ng/ml

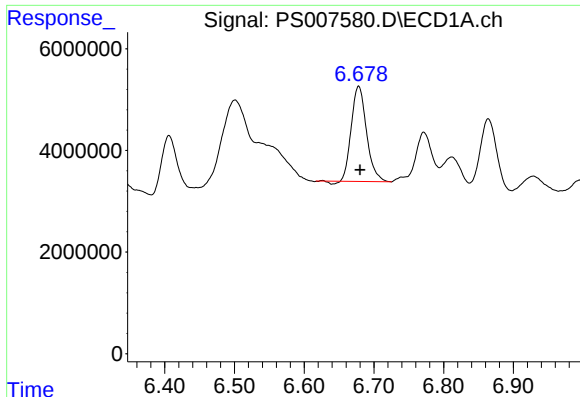

#10 Pentachlorophenol


R.T.: 6.678 min
Delta R.T.: -0.002 min
Response: 28254920
Conc: 1.58 ng/ml

Instrument :
ECD_S
ClientSampleId :
Z3-20B

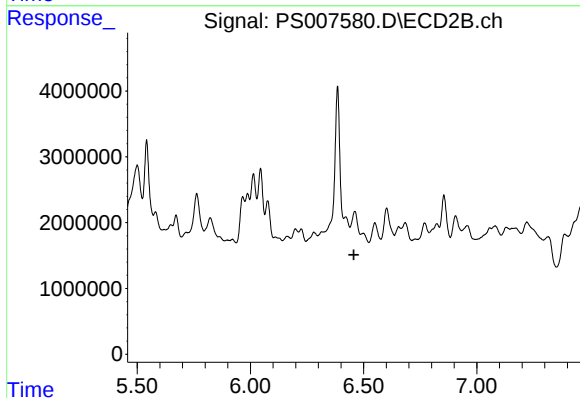


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 6.457 min
Response: 0
Conc: N.D.

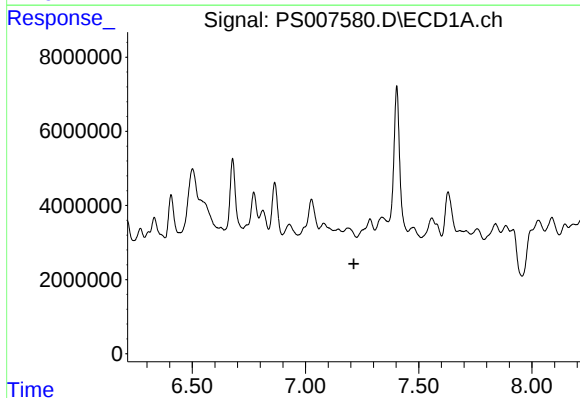


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 7.214 min
Response: 0
Conc: N.D.

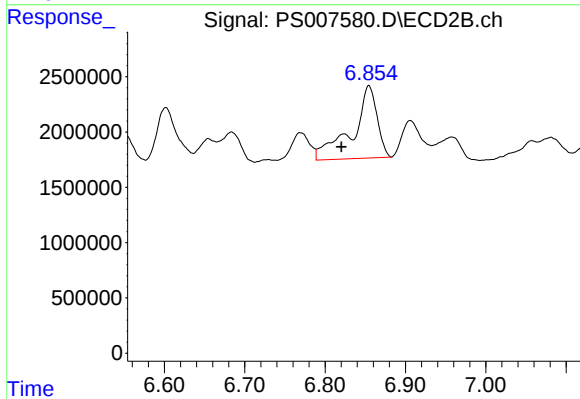

#11 2,4,5-TP (SILVEX)


R.T.: 6.855 min
Delta R.T.: 0.034 min
Response: 14047670
Conc: 3.69 ng/ml

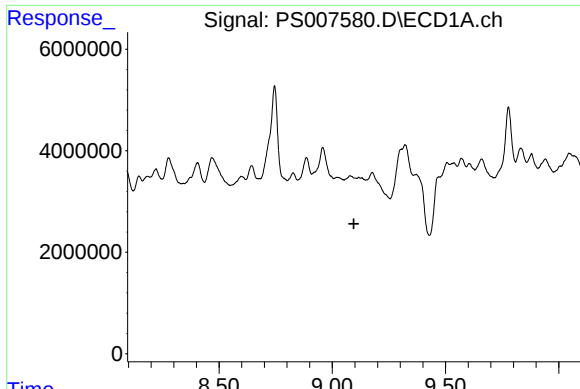

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 9.095 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
Z3-20B

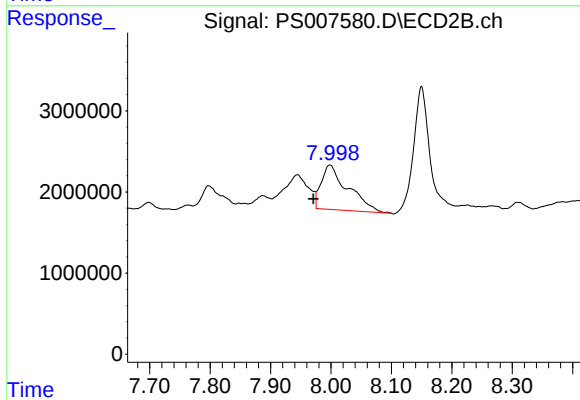


#14 DINOSEB

R.T.: 7.998 min
Delta R.T.: 0.028 min
Response: 16778536
Conc: 5.98 ng/ml

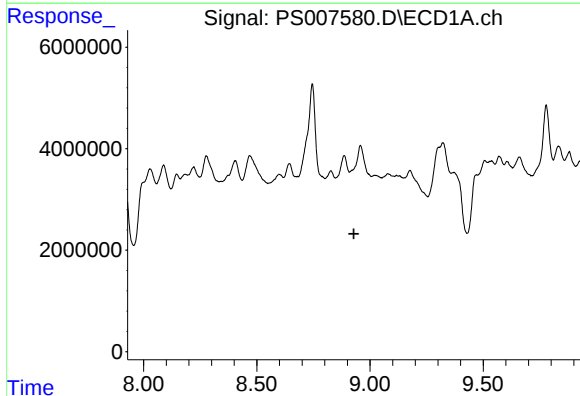


#15 Picloram

R.T.: 0.000 min
Exp R.T.: 8.929 min
Response: 0
Conc: N.D.

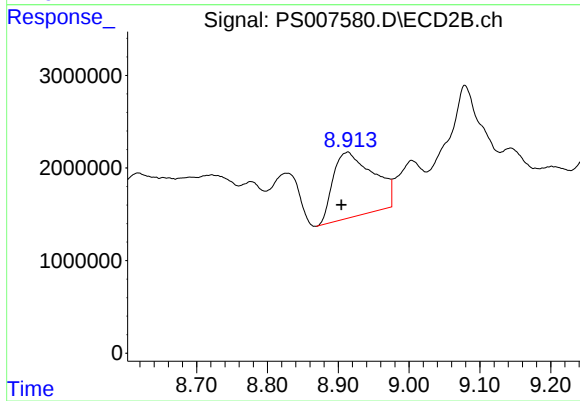

#15 Picloram


R.T.: 8.913 min
Delta R.T.: 0.008 min
Response: 27665598
Conc: 4.51 ng/ml

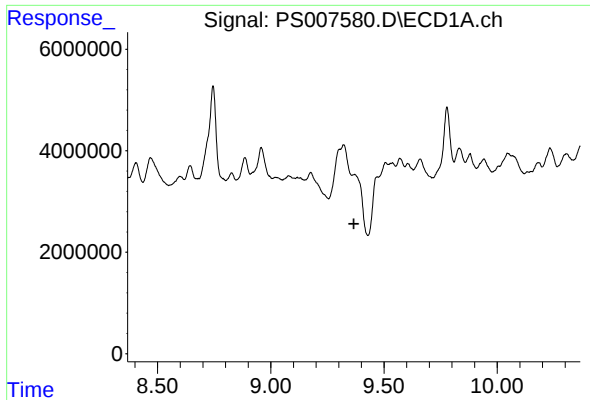

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 9.367 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
Z3-20B

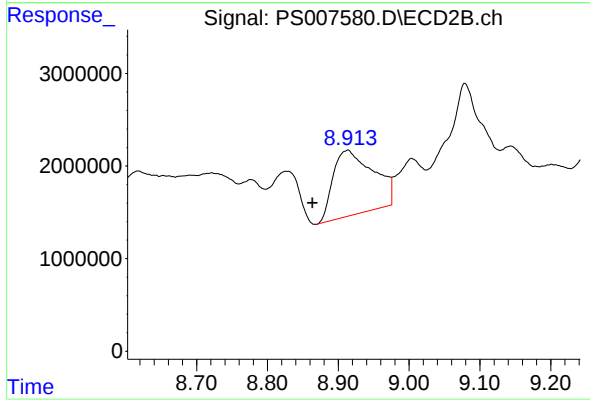

#16 DCPA

R.T.: 8.913 min
Delta R.T.: 0.050 min
Response: 27665598
Conc: 5.52 ng/ml