

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110119\
 Data File : PS007581.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Nov 2019 19:58
 Operator : SM\AJ
 Sample : K5599-05
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 Z3-21A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 01 23:29:34 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 14 13:54:23 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.433	5.158	628.4E6	296.0E6	459.112	420.804
Target Compounds							
1) T	Dalapon	0.000	1.659	0	671.5E6	N.D.	737.881
2) T	3,5-DICHL...	0.000	4.493	0	54001593	N.D.	62.761
5) T	DICAMBA	5.527	0.000	56826120	0	11.566	N.D. #
7) T	MCPA	5.902	5.528	26407612	31424207	5.120	10.809 #
9) T	2,4-D	6.489	6.063	110.4E6	10965313	89.584	13.745 #
10) T	Pentachlo...	6.666	6.413	53095919	20305751	2.974	2.112 #
12) T	2,4,5-T	0.000	7.204	0	17202520	N.D.	4.910
14) T	DINOSEB	0.000	7.952	0	20217163	N.D.	7.201
15) T	Picloram	0.000	8.913	0	21539339	N.D.	3.508
16) T	DCPA	0.000	8.828	0	16415203	N.D.	3.273



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110119\
Data File : PS007581.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Nov 2019 19:58
Operator : SM\AJ
Sample : K5599-05
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
Z3-21A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 01 23:29:34 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
Quant Title : 8080.M
QLast Update : Mon Oct 14 13:54:23 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

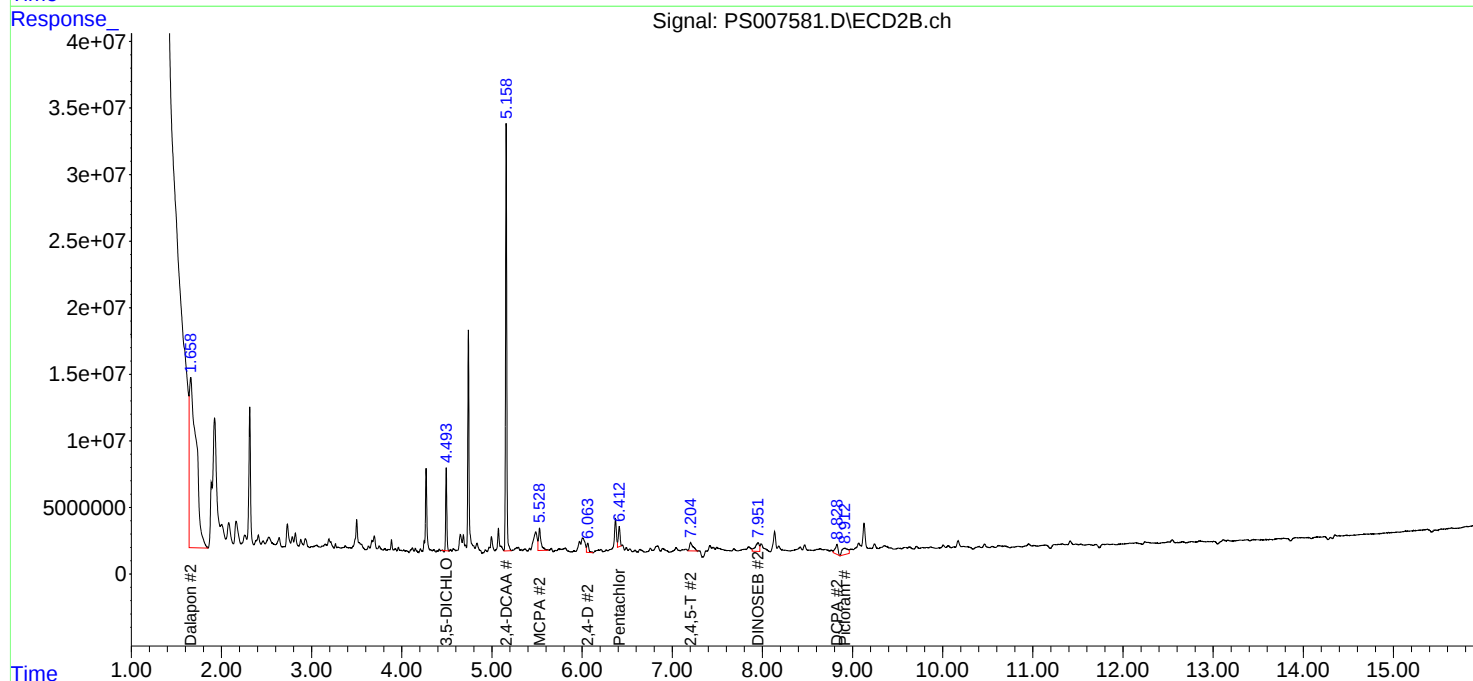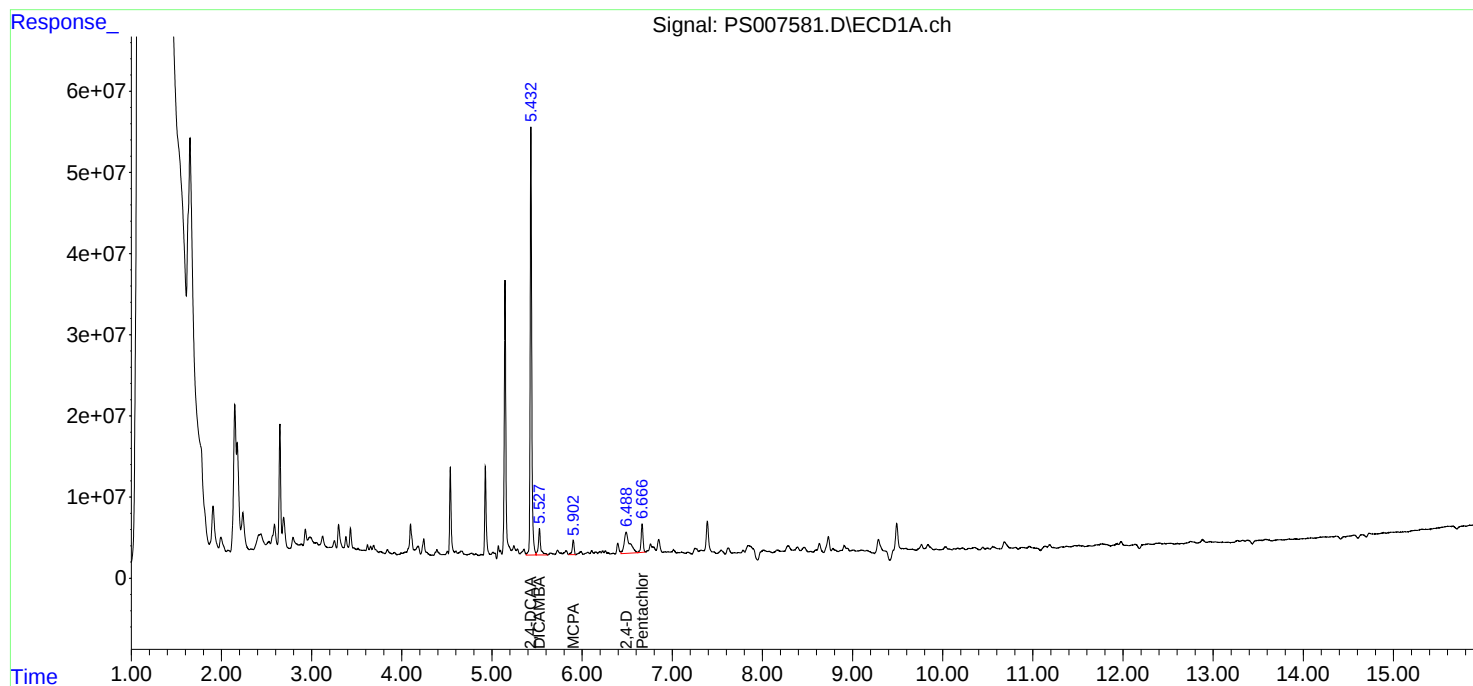


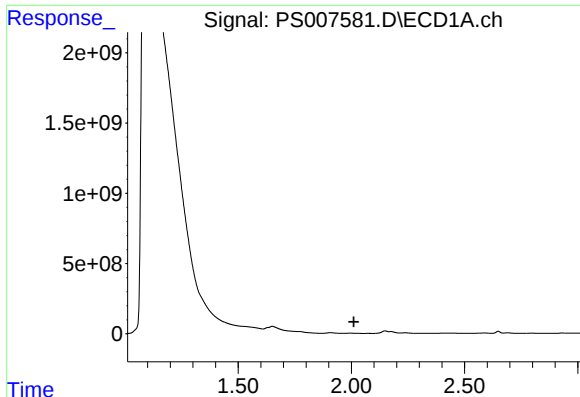

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.011 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
Z3-21A

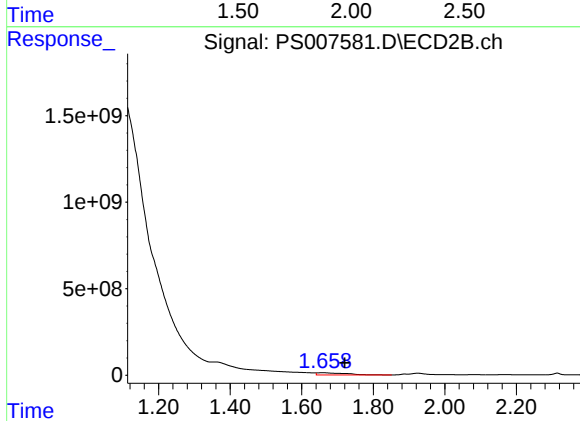


#1 Dalapon

R.T.: 1.659 min
Delta R.T.: -0.061 min
Response: 671474680
Conc: 737.88 ng/ml

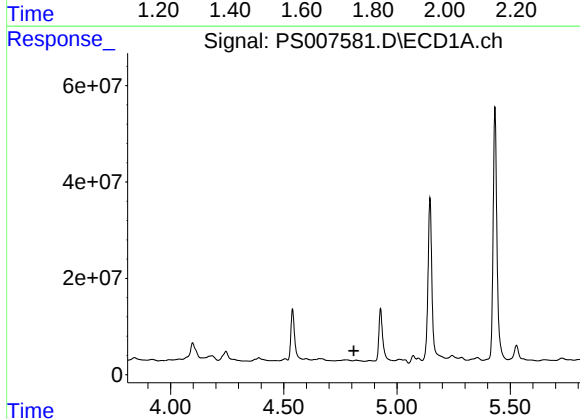


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T.: 4.810 min
Response: 0
Conc: N.D.

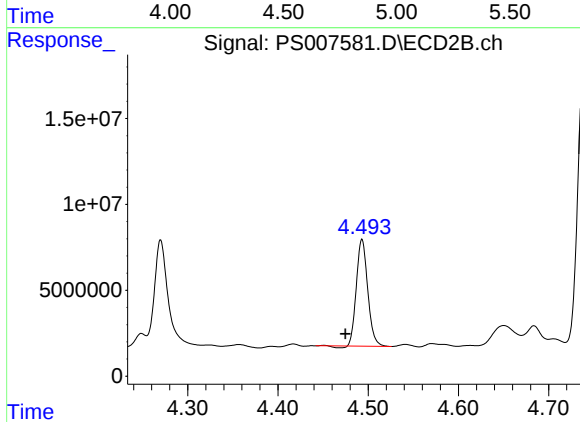

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.493 min
Delta R.T.: 0.018 min
Response: 54001593
Conc: 62.76 ng/ml

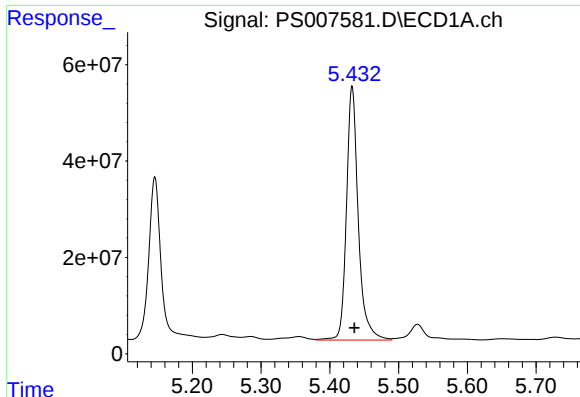

#4 2,4-DCAA


R.T.: 5.433 min
Delta R.T.: -0.003 min
Response: 628372898
Conc: 459.11 ng/ml

Instrument :
ECD_S
ClientSampleId :
Z3-21A

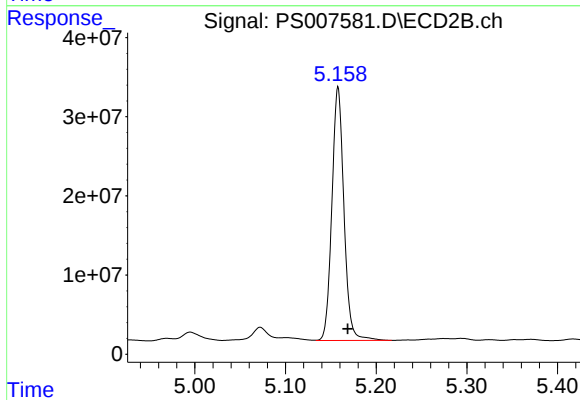


#4 2,4-DCAA

R.T.: 5.158 min
Delta R.T.: -0.011 min
Response: 295954415
Conc: 420.80 ng/ml

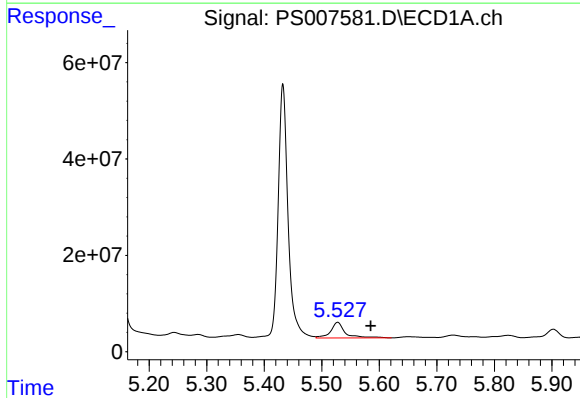


#5 DICAMBA

R.T.: 5.527 min
Delta R.T.: -0.058 min
Response: 56826120
Conc: 11.57 ng/ml

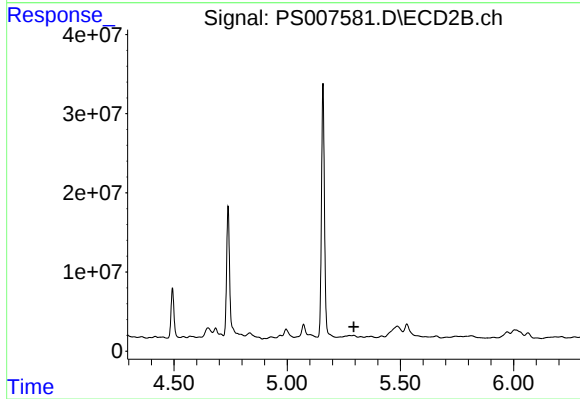

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 5.294 min
Response: 0
Conc: N.D.

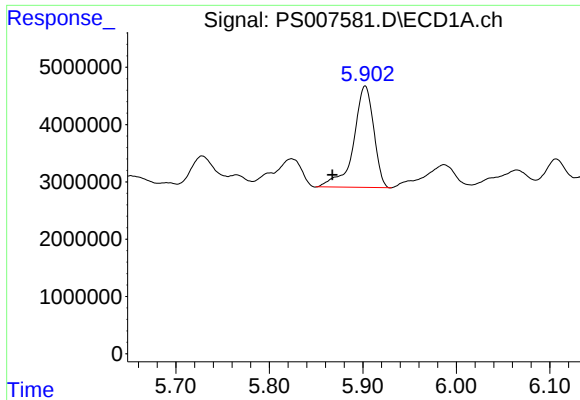

#7 MCPA


R.T.: 5.902 min
Delta R.T.: 0.035 min
Response: 26407612
Conc: 5.12 ug/ml

Instrument :
ECD_S
ClientSampleId :
Z3-21A

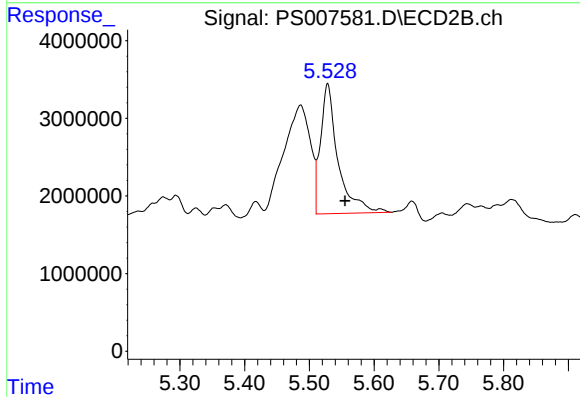


#7 MCPA

R.T.: 5.528 min
Delta R.T.: -0.026 min
Response: 31424207
Conc: 10.81 ug/ml

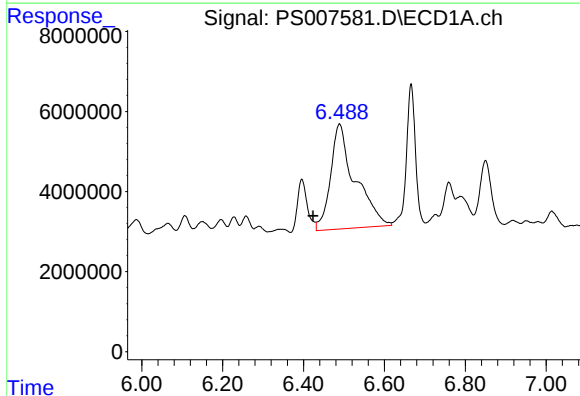


#9 2,4-D

R.T.: 6.489 min
Delta R.T.: 0.065 min
Response: 110397561
Conc: 89.58 ng/ml

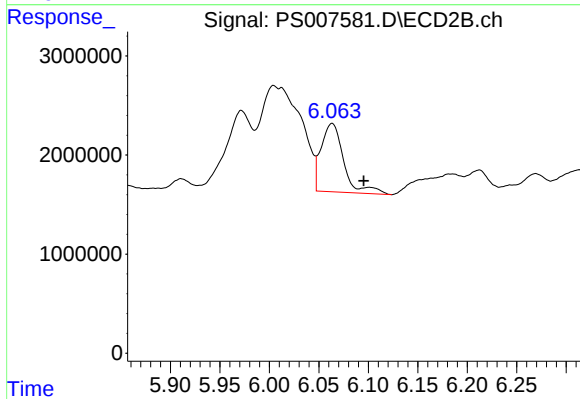

#9 2,4-D


R.T.: 6.063 min
Delta R.T.: -0.032 min
Response: 10965313
Conc: 13.74 ng/ml

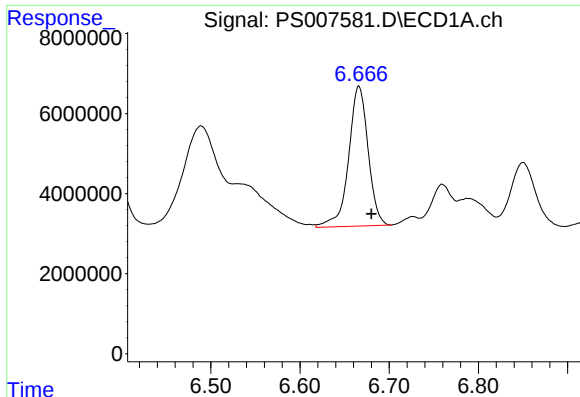

#10 Pentachlorophenol


R.T.: 6.666 min
Delta R.T.: -0.014 min
Response: 53095919
Conc: 2.97 ng/ml

Instrument :
ECD_S
ClientSampleId :
Z3-21A

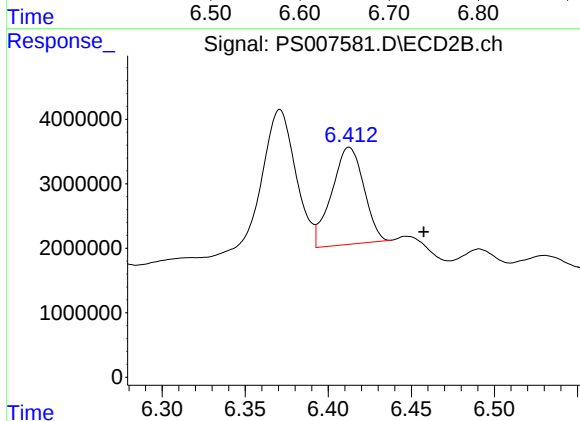


#10 Pentachlorophenol

R.T.: 6.413 min
Delta R.T.: -0.045 min
Response: 20305751
Conc: 2.11 ng/ml

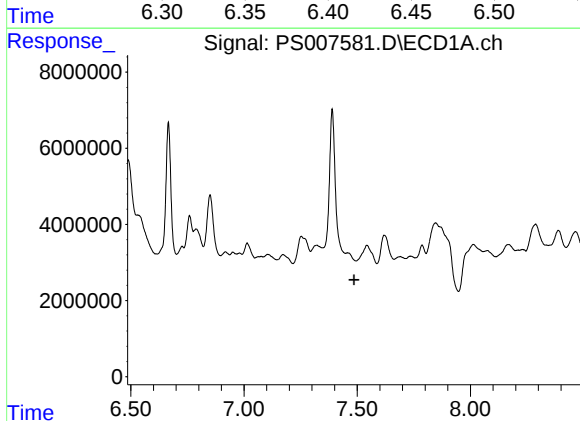


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 7.486 min
Response: 0
Conc: N.D.

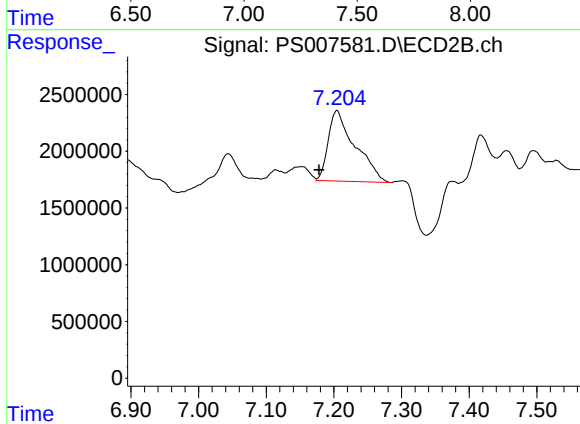

#12 2,4,5-T


R.T.: 7.204 min
Delta R.T.: 0.026 min
Response: 17202520
Conc: 4.91 ng/ml

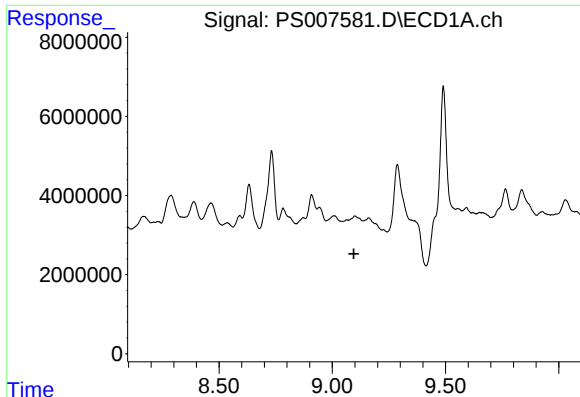

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 9.095 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
Z3-21A

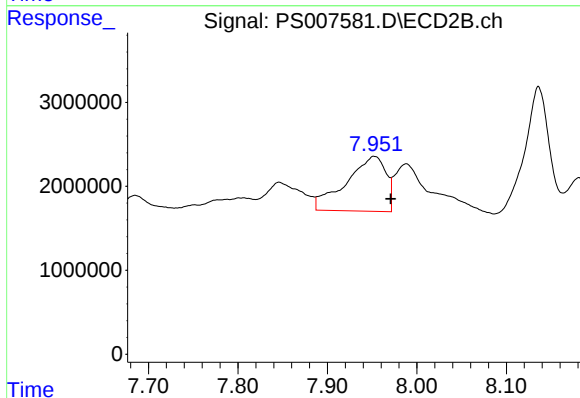


#14 DINOSEB

R.T.: 7.952 min
Delta R.T.: -0.018 min
Response: 20217163
Conc: 7.20 ng/ml

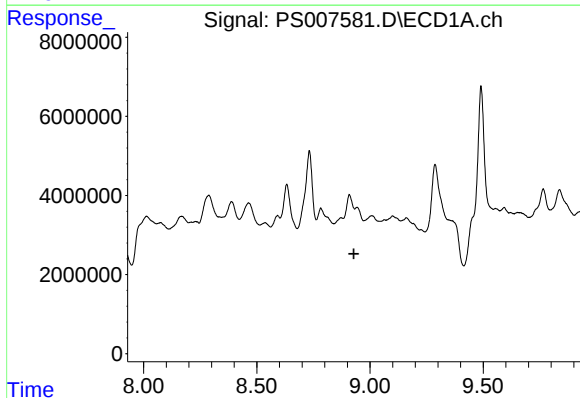


#15 Picloram

R.T.: 0.000 min
Exp R.T.: 8.929 min
Response: 0
Conc: N.D.

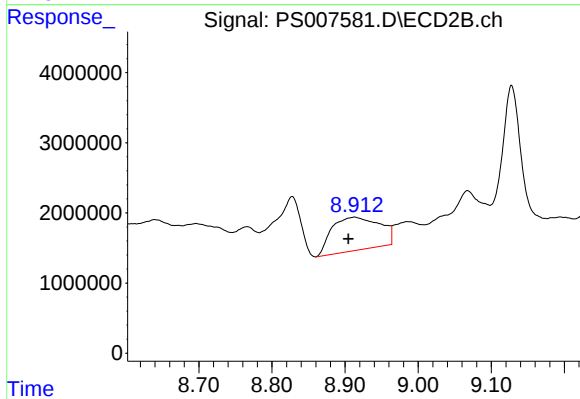

#15 Picloram


R.T.: 8.913 min
Delta R.T.: 0.008 min
Response: 21539339
Conc: 3.51 ng/ml

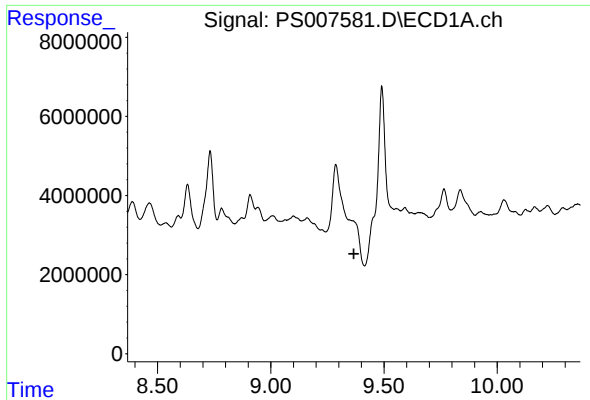

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 9.367 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
Z3-21A

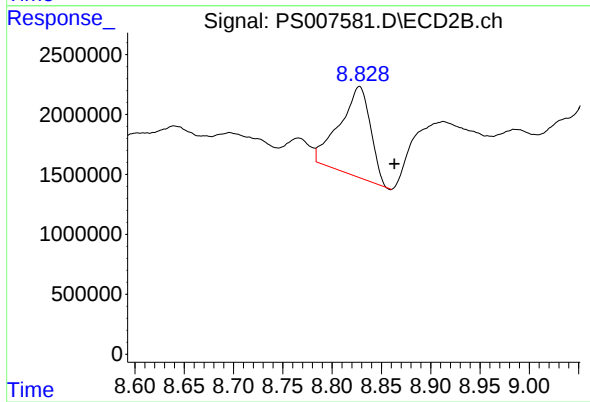

#16 DCPA

R.T.: 8.828 min
Delta R.T.: -0.036 min
Response: 16415203
Conc: 3.27 ng/ml