

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110119\
 Data File : PS007586.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Nov 2019 21:48
 Operator : SM\AJ
 Sample : K5599-15
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 Z3-23B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 01 23:31:24 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 14 13:54:23 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.431	5.157	846.9E6	417.1E6	618.798	593.083
Target Compounds							
1) T	Dalapon	0.000	1.659	0	512.1E6	N.D.	562.715
2) T	3,5-DICHL...	0.000	4.492	0	61620492	N.D.	71.616
5) T	DICAMBA	5.527	5.270	44486144	12645322	9.054	4.860 #
7) T	MCPA	0.000	5.528	0	25406699	N.D.	8.739
9) T	2,4-D	6.485	6.030	33761737	6050949	27.396	7.585 #
10) T	Pentachlo...	6.664	6.410	33563828	9702085	1.880	1.009 #
14) T	DINOSEB	0.000	7.902	0	14952682	N.D.	5.326
15) T	Picloram	0.000	8.897	0	20803395	N.D.	3.388
16) T	DCPA	0.000	8.897	0	20803395	N.D.	4.149



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110119\
Data File : PS007586.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Nov 2019 21:48
Operator : SM\AJ
Sample : K5599-15
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
Z3-23B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 01 23:31:24 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
Quant Title : 8080.M
QLast Update : Mon Oct 14 13:54:23 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

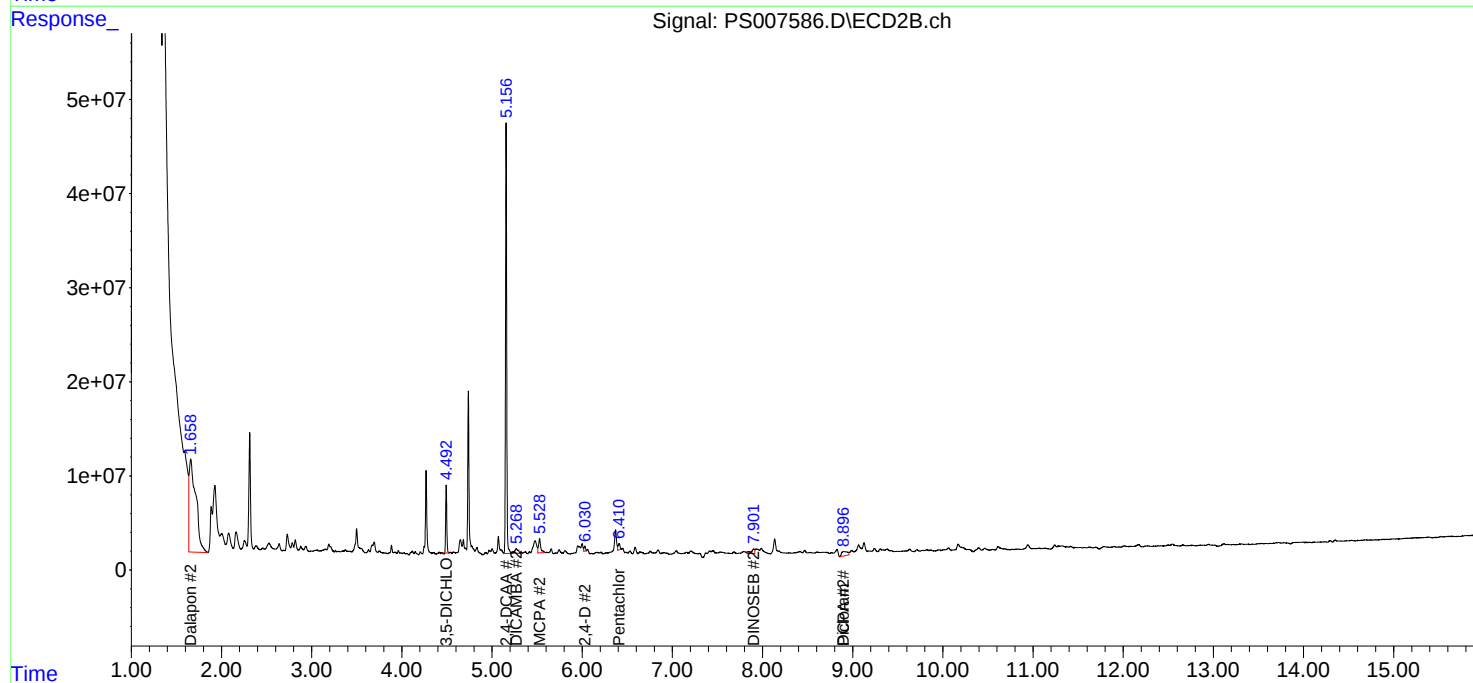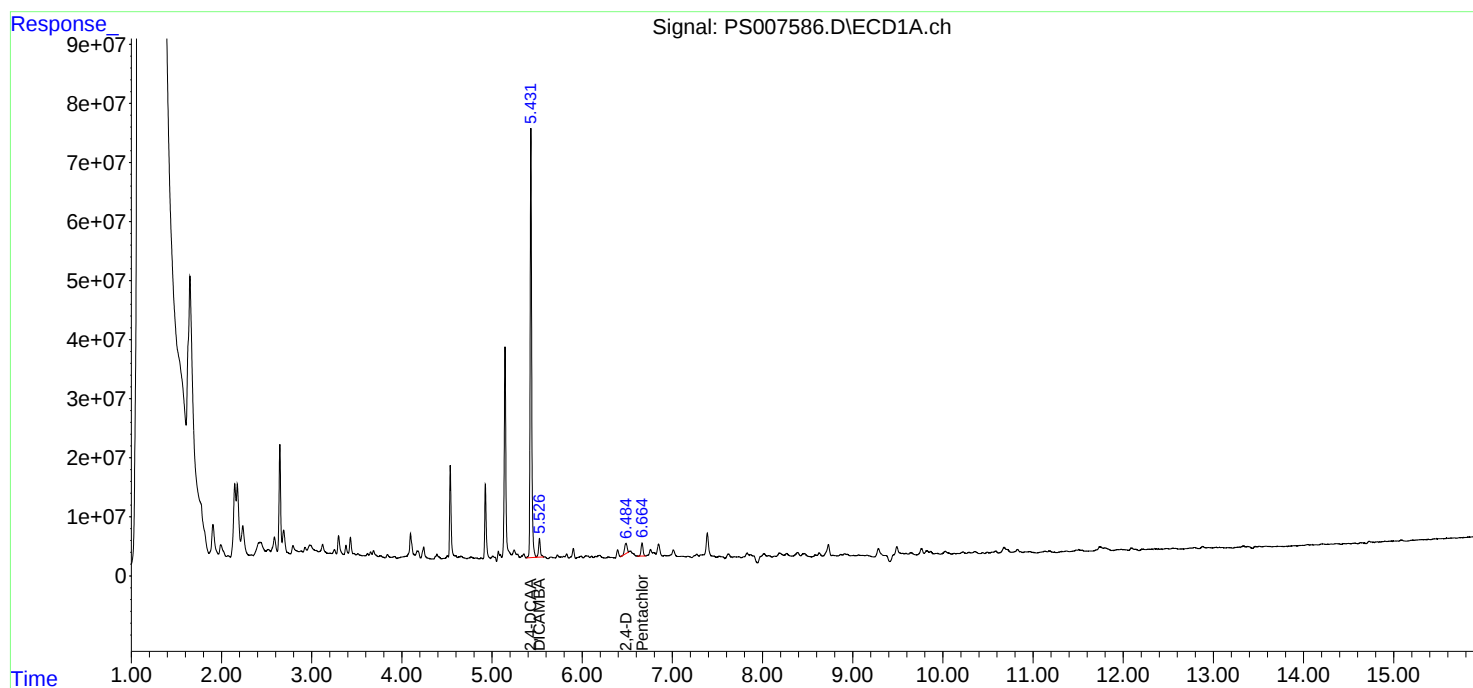


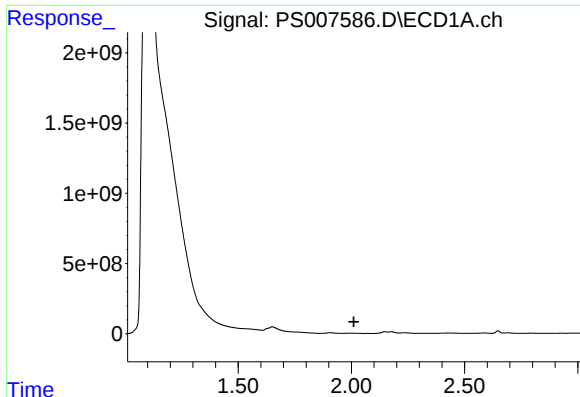

#1 Dalapon


R.T.: 0.000 min
Exp R.T. : 2.011 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
Z3-23B

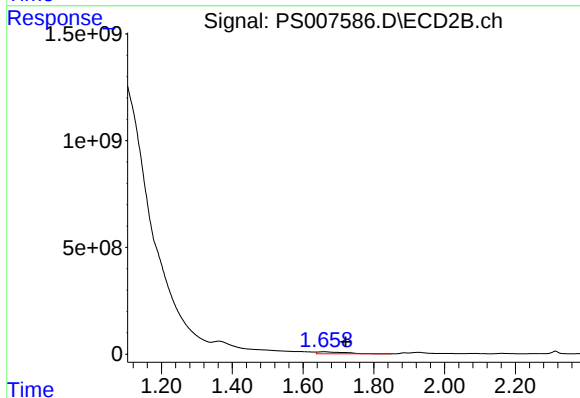


#1 Dalapon

R.T.: 1.659 min
Delta R.T.: -0.062 min
Response: 512072320
Conc: 562.71 ng/ml

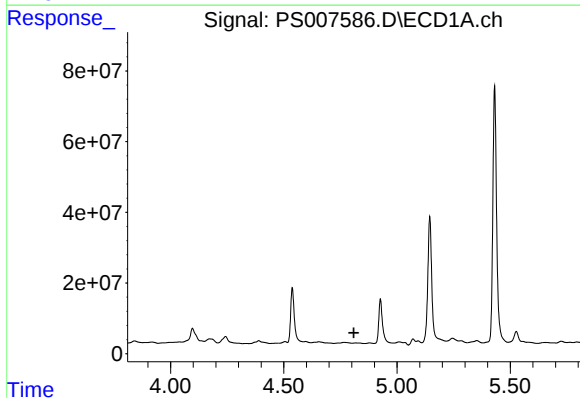


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.810 min
Response: 0
Conc: N.D.

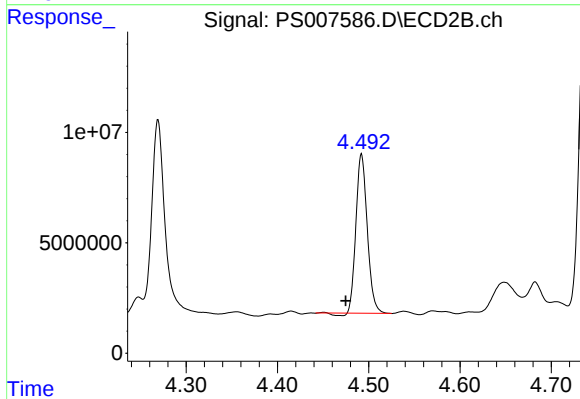

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.492 min
Delta R.T.: 0.017 min
Response: 61620492
Conc: 71.62 ng/ml

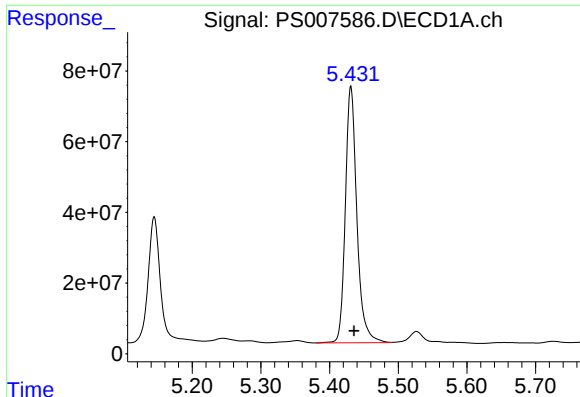

#4 2,4-DCAA


R.T.: 5.431 min
Delta R.T.: -0.005 min
Response: 846929976
Conc: 618.80 ng/ml

Instrument :
ECD_S
ClientSampleId :
Z3-23B

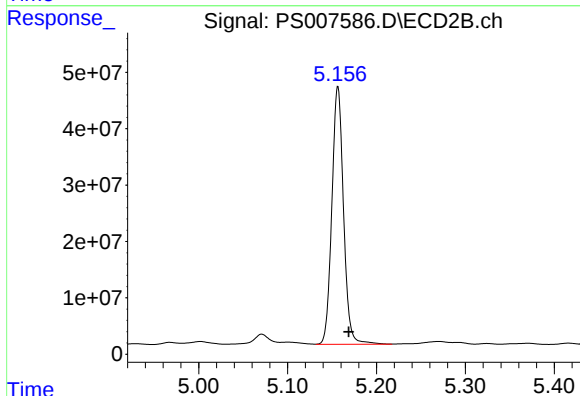


#4 2,4-DCAA

R.T.: 5.157 min
Delta R.T.: -0.012 min
Response: 417118977
Conc: 593.08 ng/ml

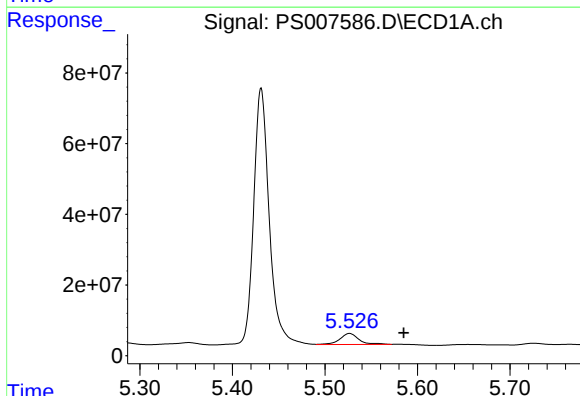


#5 DICAMBA

R.T.: 5.527 min
Delta R.T.: -0.059 min
Response: 44486144
Conc: 9.05 ng/ml

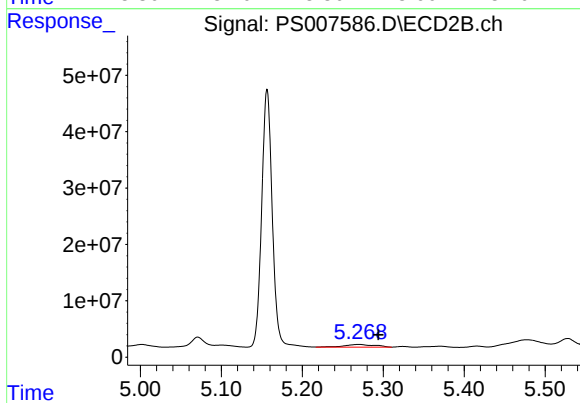

#5 DICAMBA


R.T.: 5.270 min
Delta R.T.: -0.025 min
Response: 12645322
Conc: 4.86 ng/ml

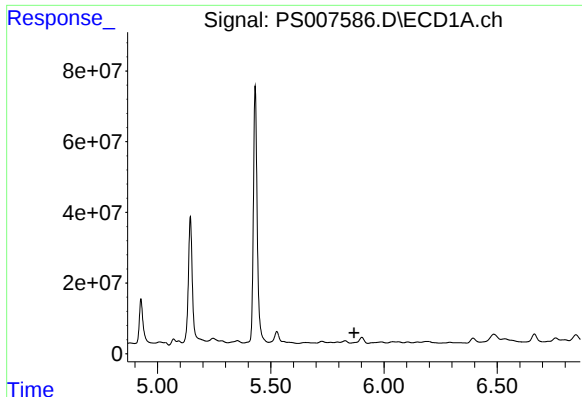

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 5.867 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
Z3-23B

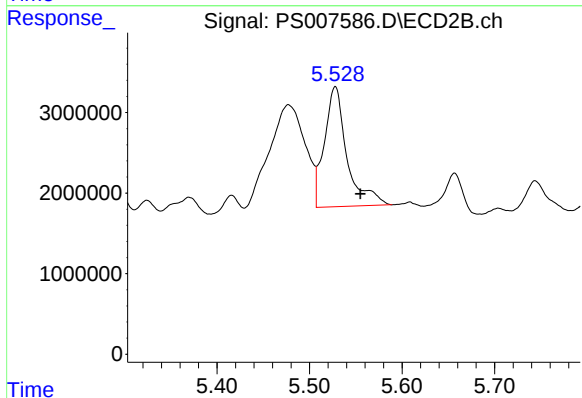


#7 MCPA

R.T.: 5.528 min
Delta R.T.: -0.027 min
Response: 25406699
Conc: 8.74 ug/ml

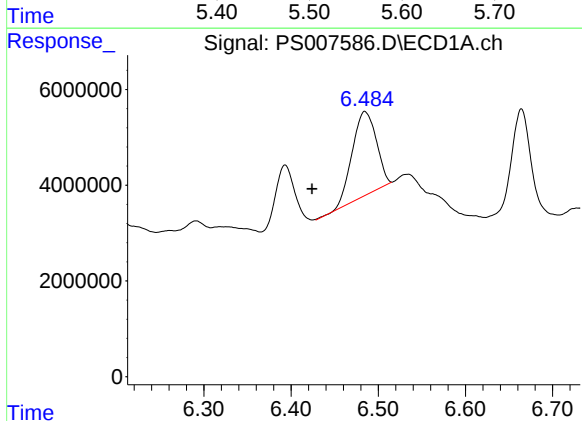


#9 2,4-D

R.T.: 6.485 min
Delta R.T.: 0.061 min
Response: 33761737
Conc: 27.40 ng/ml

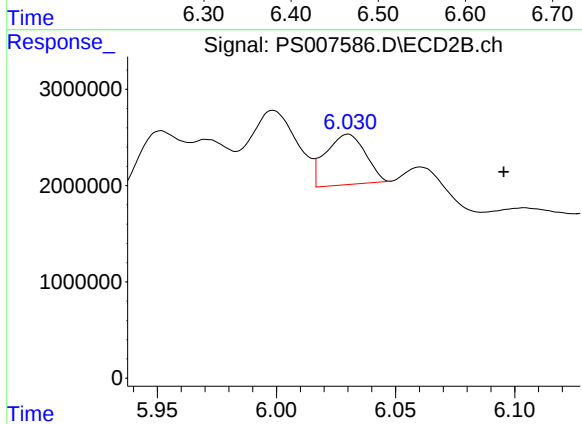

#9 2,4-D


R.T.: 6.030 min
Delta R.T.: -0.065 min
Response: 6050949
Conc: 7.58 ng/ml

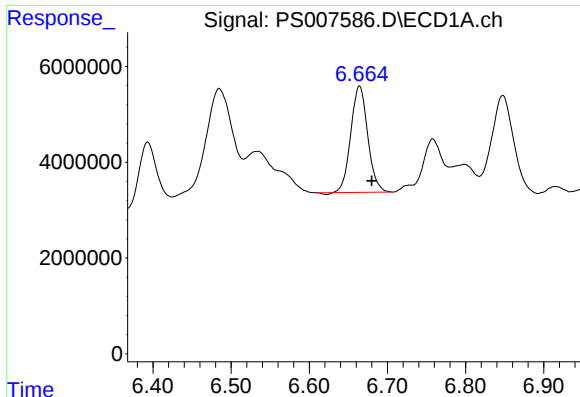

#10 Pentachlorophenol


R.T.: 6.664 min
Delta R.T.: -0.016 min
Response: 33563828
Conc: 1.88 ng/ml

Instrument :
ECD_S
ClientSampleId :
Z3-23B

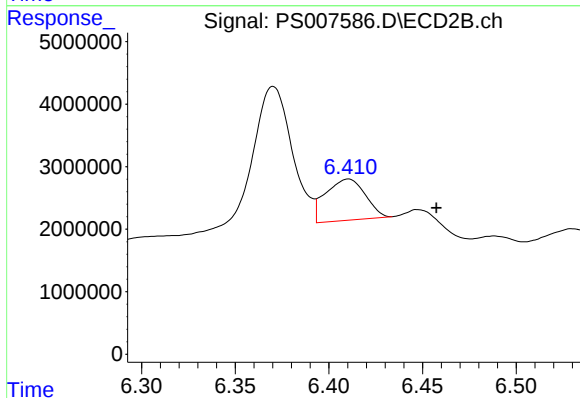


#10 Pentachlorophenol

R.T.: 6.410 min
Delta R.T.: -0.047 min
Response: 9702085
Conc: 1.01 ng/ml

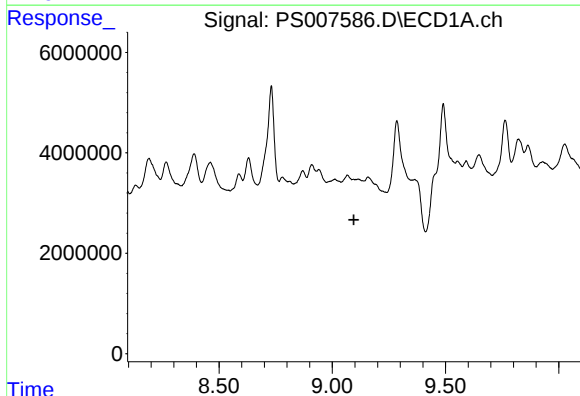


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 9.095 min
Response: 0
Conc: N.D.

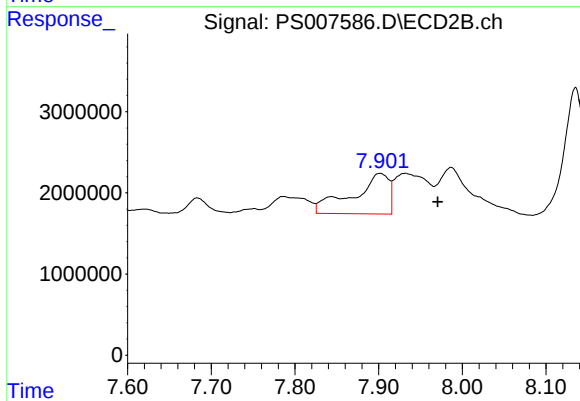

#14 DINOSEB


R.T.: 7.902 min
Delta R.T.: -0.069 min
Response: 14952682
Conc: 5.33 ng/ml

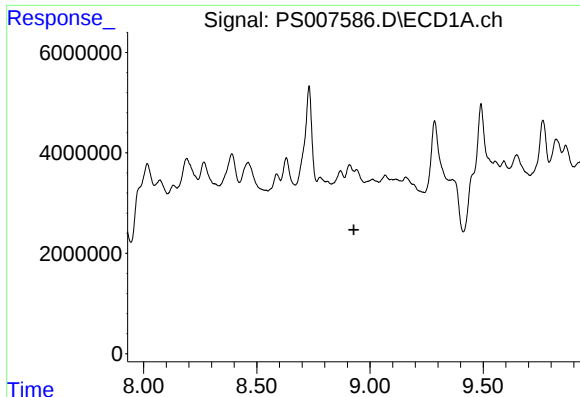

#15 Picloram


R.T.: 0.000 min
Exp R.T.: 8.929 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
Z3-23B

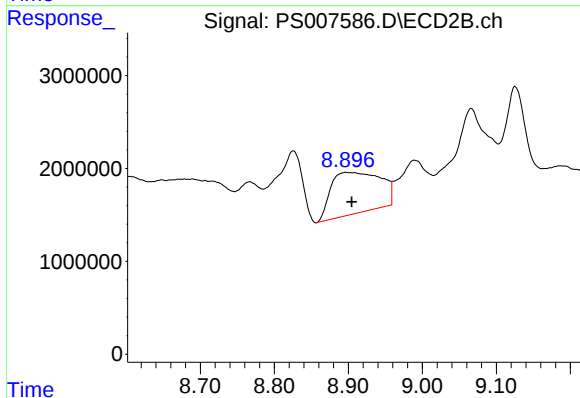


#15 Picloram

R.T.: 8.897 min
Delta R.T.: -0.007 min
Response: 20803395
Conc: 3.39 ng/ml

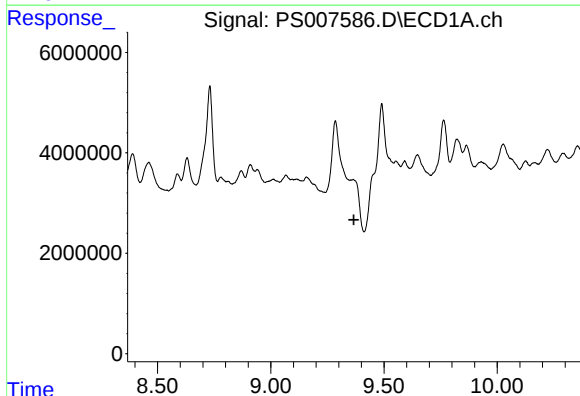

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 9.367 min
Response: 0
Conc: N.D.

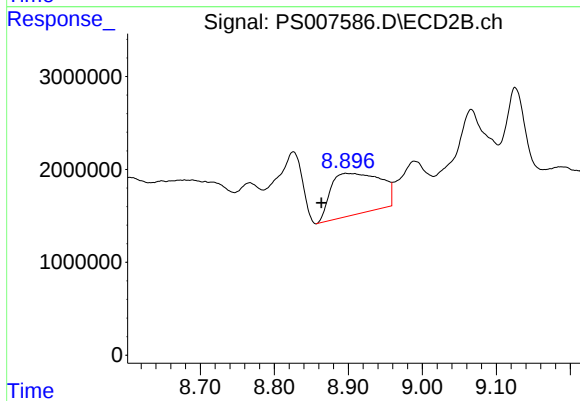

#16 DCPA

R.T.: 8.897 min
Delta R.T.: 0.034 min
Response: 20803395
Conc: 4.15 ng/ml