

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110119\
 Data File : PS007594.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Nov 2019 00:43
 Operator : SM\AJ
 Sample : K5599-01
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 Z3-20A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 02 03:01:11 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 14 13:54:23 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.427	5.152	729.0E6	355.7E6	532.601	505.821
Target Compounds							
1) T	Dalapon	0.000	1.654	0	522.9E6	N.D.	574.584
2) T	3,5-DICHL...	0.000	4.488	0	57509344	N.D.	66.838
3) T	4-Nitroph...	0.000	4.827	0	19357133	N.D.	49.018
5) T	DICAMBA	5.523	0.000	47280921	0	9.623	N.D. #
7) T	MCPA	0.000	5.523	0	23373359	N.D.	8.040
9) T	2,4-D	6.479	0.000	43819676	0	35.558	N.D. #
10) T	Pentachlo...	6.661	6.407	56230006	44930374	3.150	4.672 #
11) T	2,4,5-TP ...	0.000	6.835	0	12773001	N.D.	3.358
12) T	2,4,5-T	0.000	7.196	0	24506229	N.D.	6.995
14) T	DINOSEB	0.000	7.983	0	21978518	N.D.	7.829
15) T	Picloram	0.000	8.904	0	14047699	N.D.	2.288
16) T	DCPA	0.000	8.904	0	14047699	N.D.	2.801



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110119\
Data File : PS007594.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Nov 2019 00:43
Operator : SM\AJ
Sample : K5599-01
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
Z3-20A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 02 03:01:11 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
Quant Title : 8080.M
QLast Update : Mon Oct 14 13:54:23 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

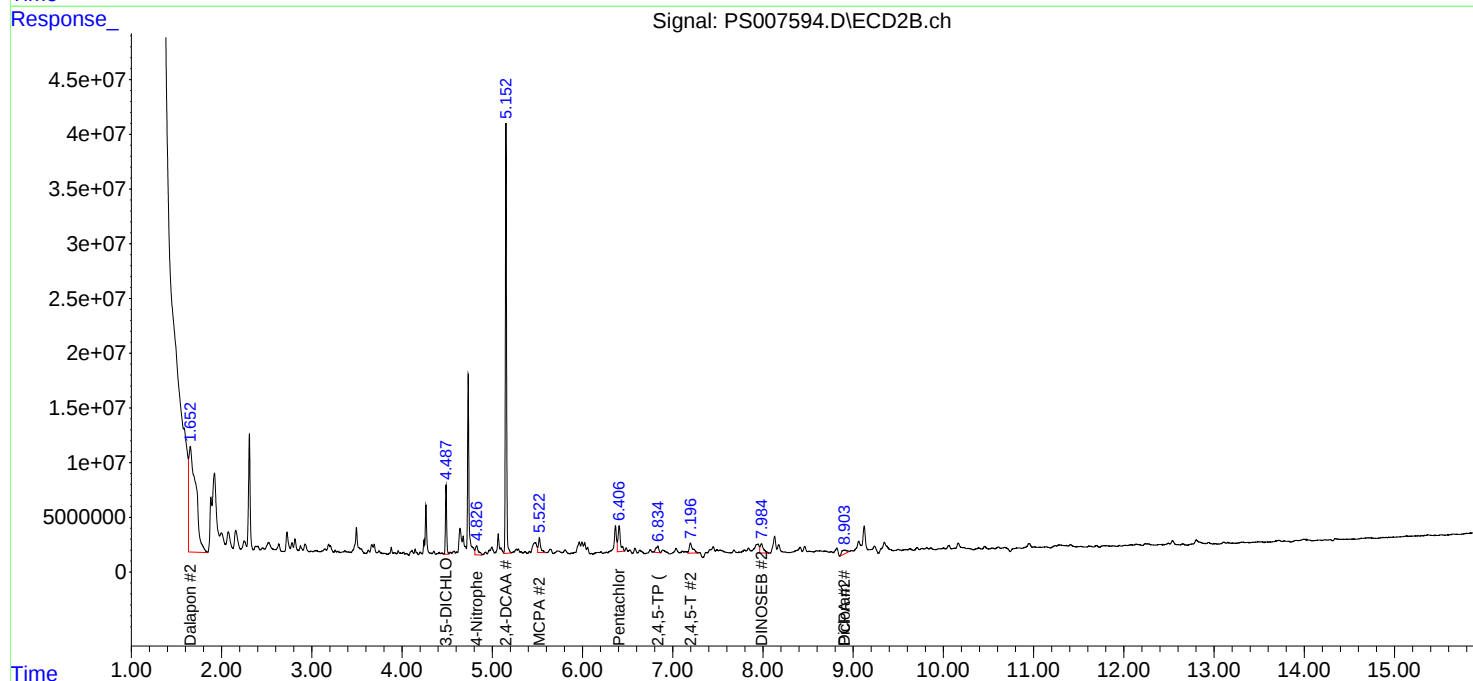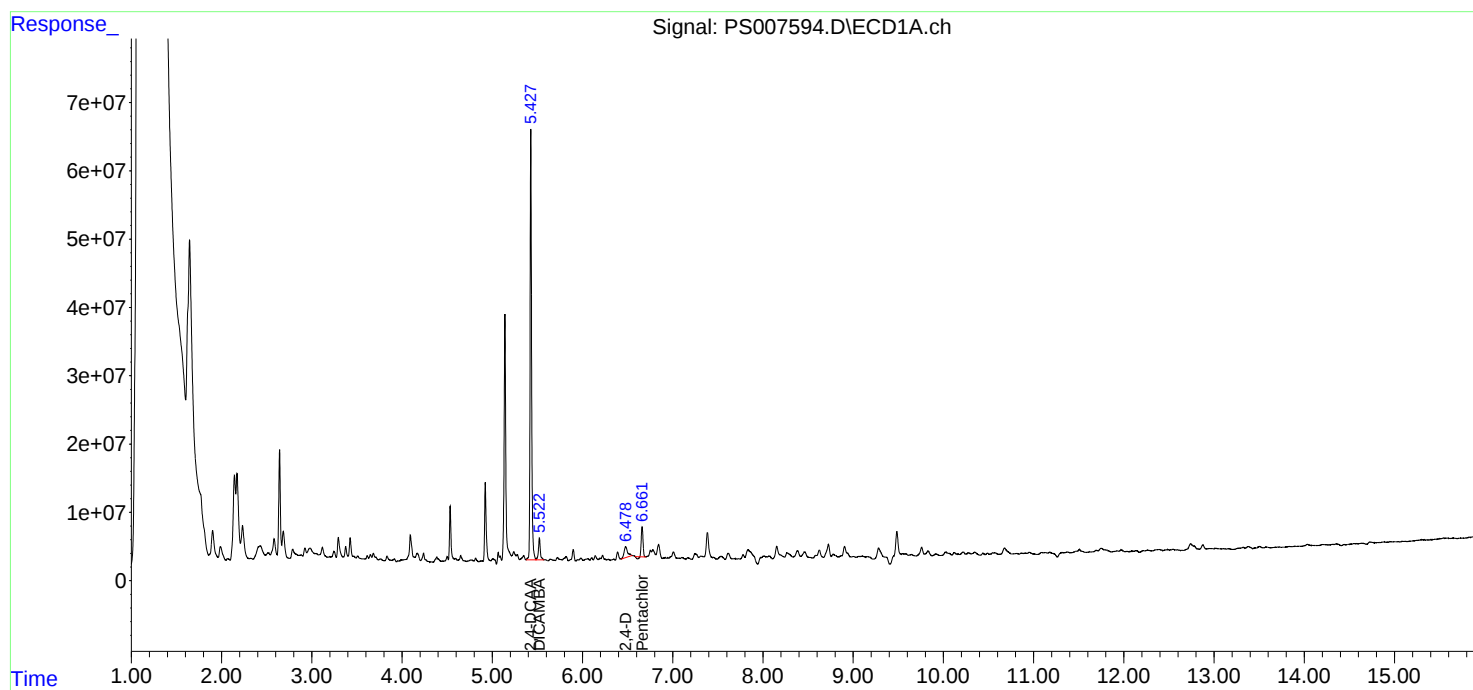


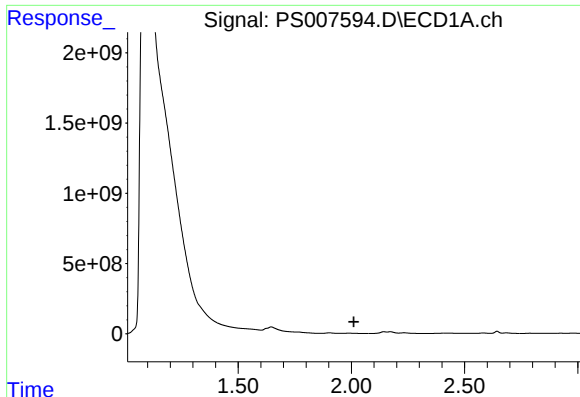

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.011 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
Z3-20A

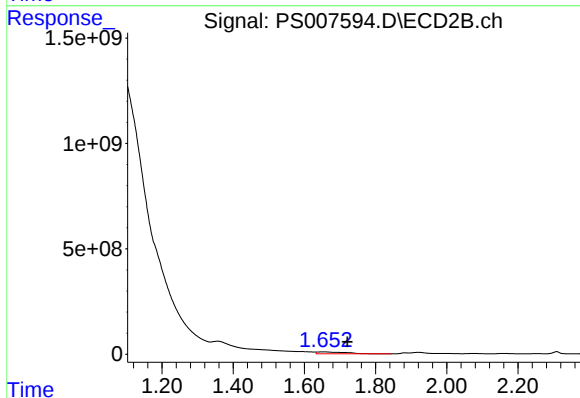


#1 Dalapon

R.T.: 1.654 min
Delta R.T.: -0.067 min
Response: 522873486
Conc: 574.58 ng/ml

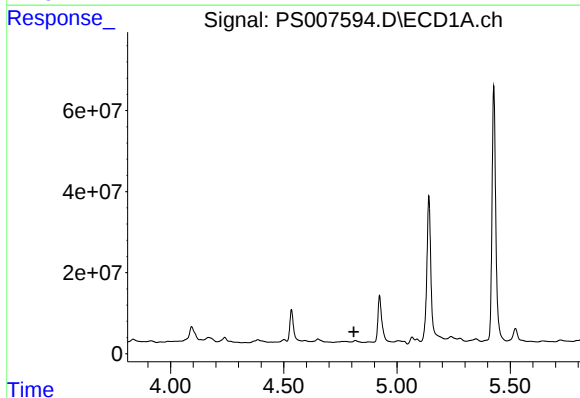


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T.: 4.810 min
Response: 0
Conc: N.D.

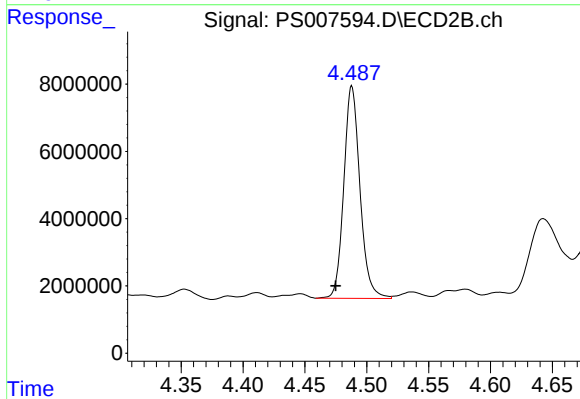

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.488 min
Delta R.T.: 0.013 min
Response: 57509344
Conc: 66.84 ng/ml

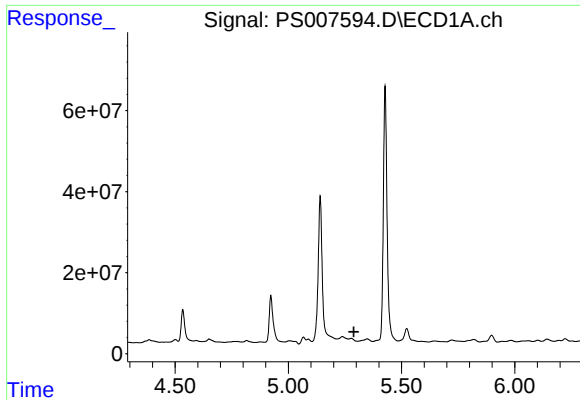

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 5.290 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
Z3-20A

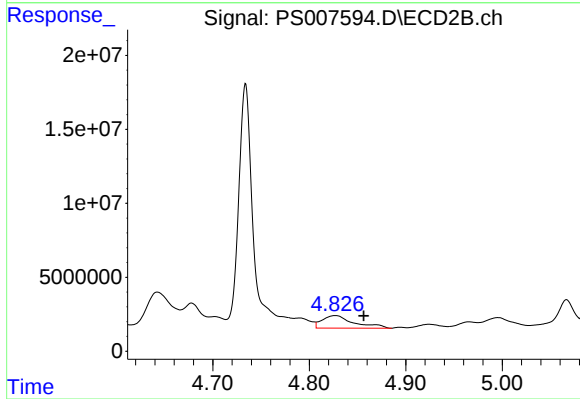


#3 4-Nitrophenol

R.T.: 4.827 min
Delta R.T.: -0.030 min
Response: 19357133
Conc: 49.02 ng/ml

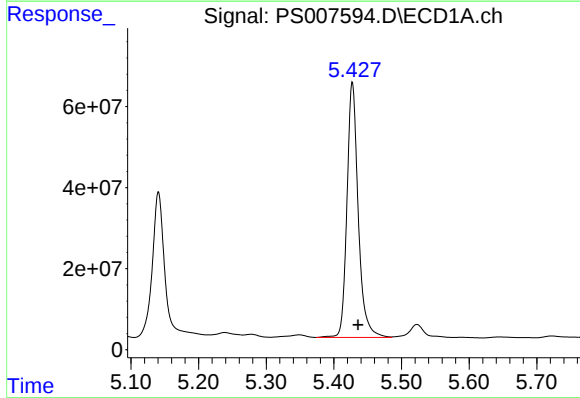


#4 2,4-DCAA

R.T.: 5.427 min
Delta R.T.: -0.008 min
Response: 728953856
Conc: 532.60 ng/ml

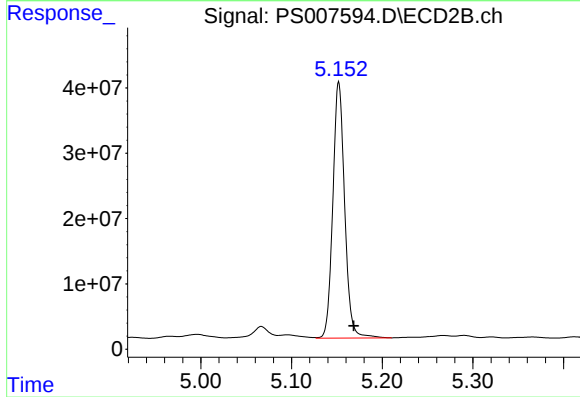

#4 2,4-DCAA


R.T.: 5.152 min
Delta R.T.: -0.016 min
Response: 355747196
Conc: 505.82 ng/ml

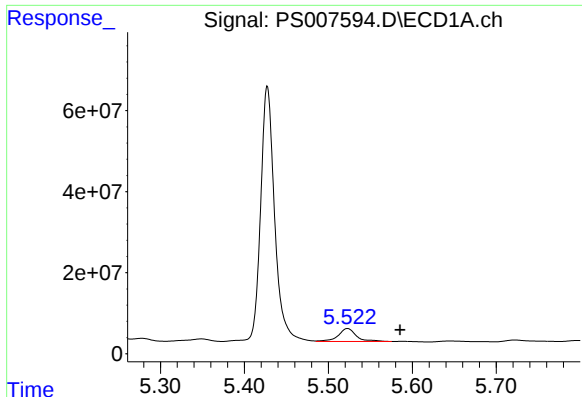

#5 DICAMBA


R.T.: 5.523 min
Delta R.T.: -0.062 min
Response: 47280921
Conc: 9.62 ng/ml

Instrument :
ECD_S
ClientSampleId :
Z3-20A

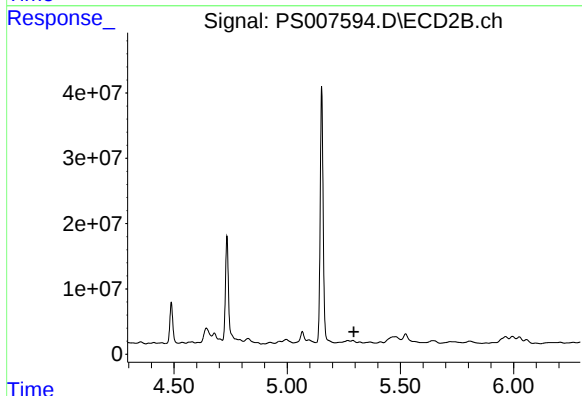


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 5.294 min
Response: 0
Conc: N.D.

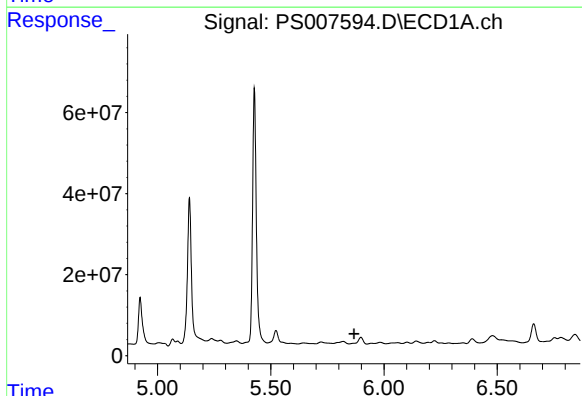


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 5.867 min
Response: 0
Conc: N.D.

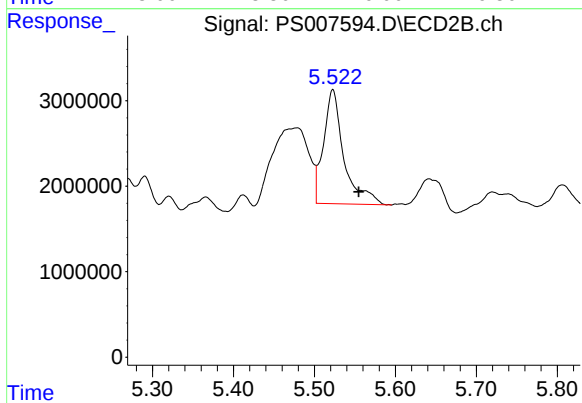

#7 MCPA


R.T.: 5.523 min
Delta R.T.: -0.032 min
Response: 23373359
Conc: 8.04 ug/ml

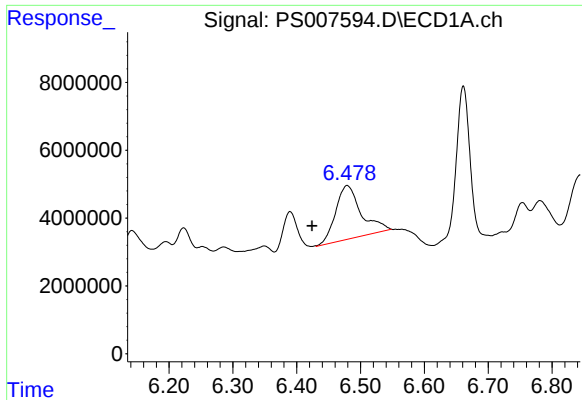

#9 2,4-D


R.T.: 6.479 min
Delta R.T.: 0.055 min
Response: 43819676
Conc: 35.56 ng/ml

Instrument :
ECD_S
ClientSampleId :
Z3-20A

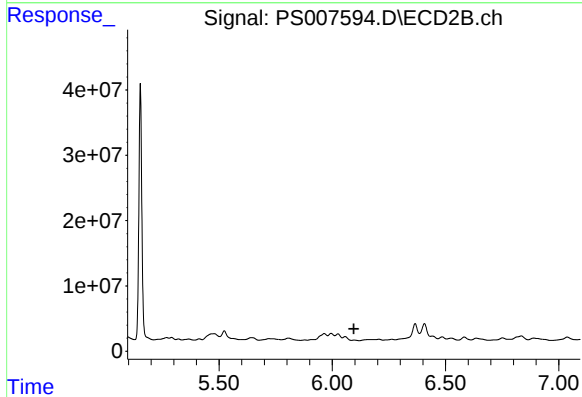


#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 6.095 min
Response: 0
Conc: N.D.

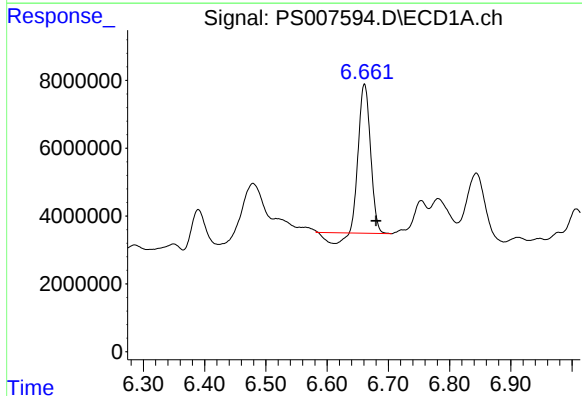


#10 Pentachlorophenol

R.T.: 6.661 min
Delta R.T.: -0.019 min
Response: 56230006
Conc: 3.15 ng/ml

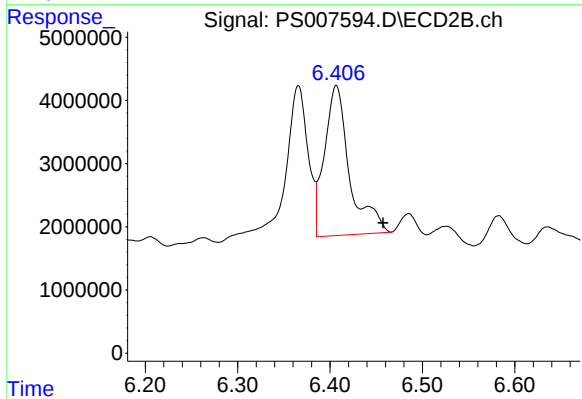

#10 Pentachlorophenol


R.T.: 6.407 min
Delta R.T.: -0.051 min
Response: 44930374
Conc: 4.67 ng/ml

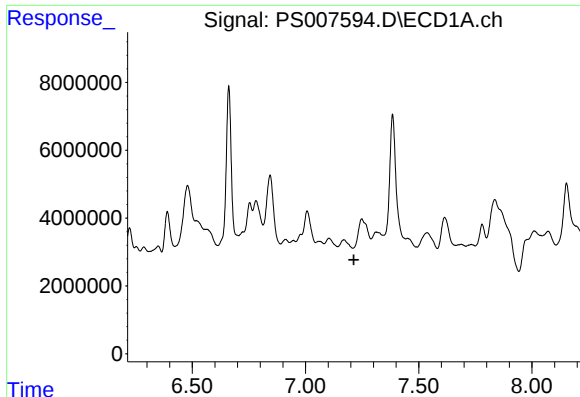

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.214 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
Z3-20A

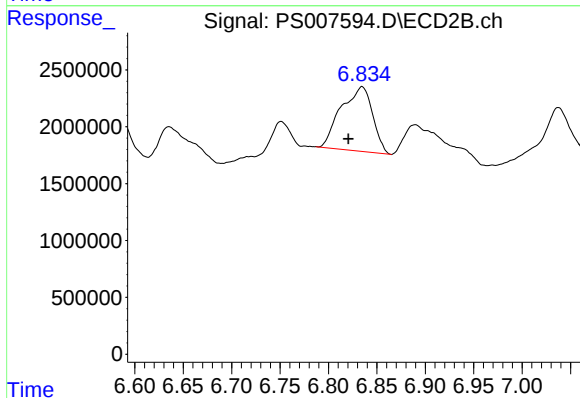


#11 2,4,5-TP (SILVEX)

R.T.: 6.835 min
Delta R.T.: 0.014 min
Response: 12773001
Conc: 3.36 ng/ml

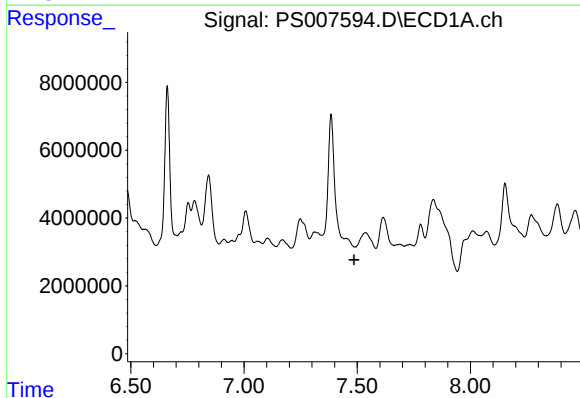


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 7.486 min
Response: 0
Conc: N.D.

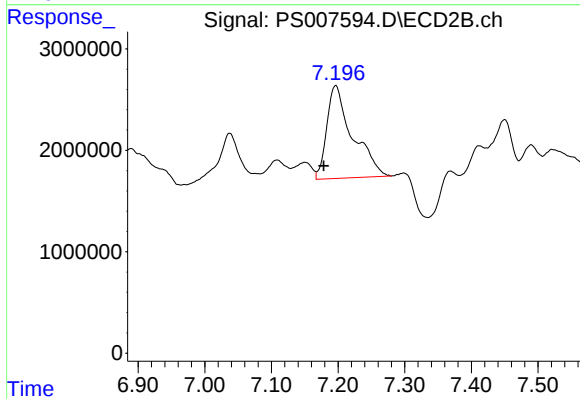

#12 2,4,5-T


R.T.: 7.196 min
Delta R.T.: 0.018 min
Response: 24506229
Conc: 6.99 ng/ml

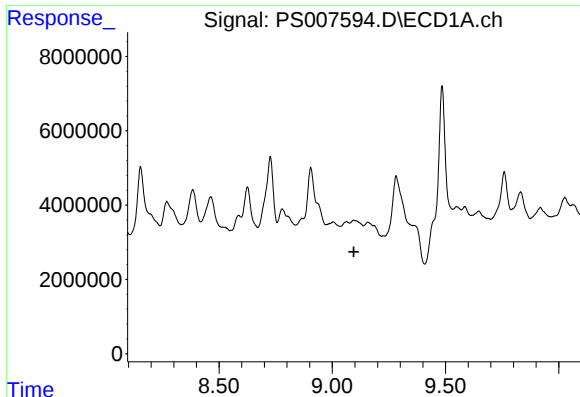

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 9.095 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
Z3-20A

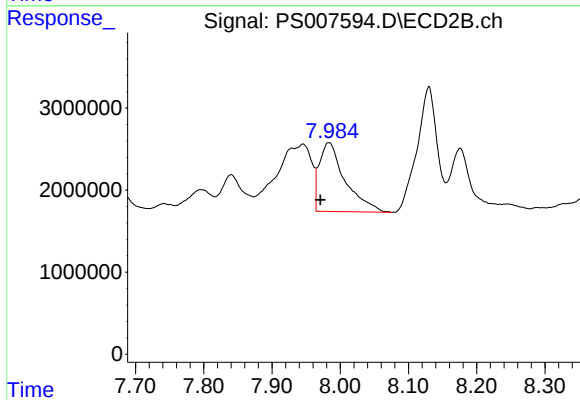


#14 DINOSEB

R.T.: 7.983 min
Delta R.T.: 0.013 min
Response: 21978518
Conc: 7.83 ng/ml

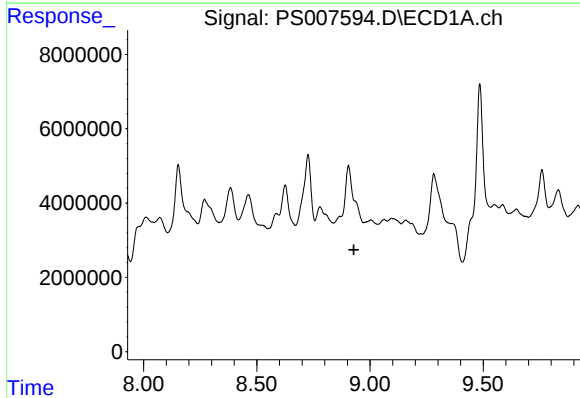


#15 Picloram

R.T.: 0.000 min
Exp R.T.: 8.929 min
Response: 0
Conc: N.D.

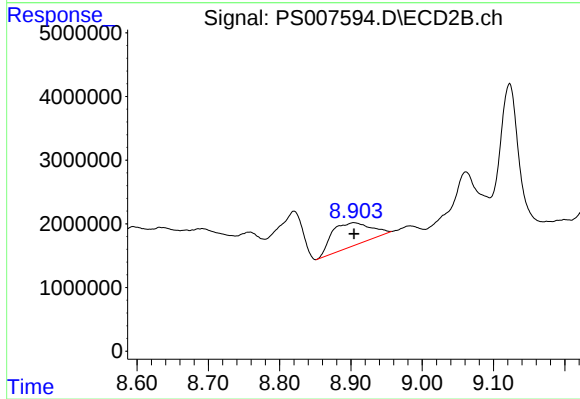

#15 Picloram


R.T.: 8.904 min
Delta R.T.: 0.000 min
Response: 14047699
Conc: 2.29 ng/ml

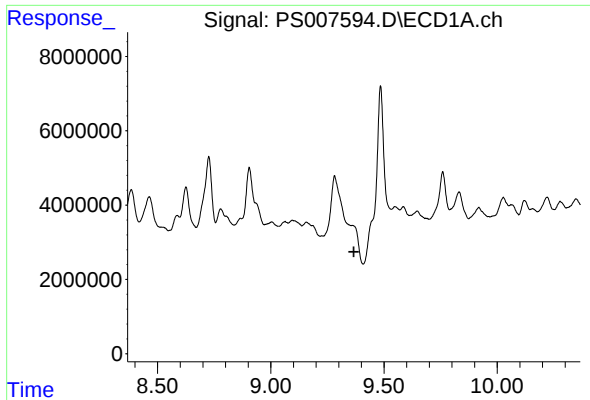

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 9.367 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
Z3-20A

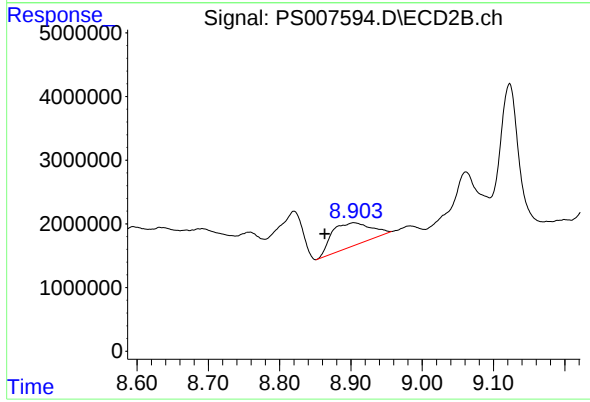

#16 DCPA

R.T.: 8.904 min
Delta R.T.: 0.041 min
Response: 14047699
Conc: 2.80 ng/ml