

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110119\
 Data File : PS007568.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Nov 2019 15:13
 Operator : SM\AJ
 Sample : K5138-06
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 AU-08-103019

Manual Integrations
 APPROVED

Ankita
 11/4/2019 8:25:30 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 01 16:29:22 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 14 13:54:23 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.436	5.161	787.0E6	415.0E6	575.019	590.040m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110119\
Data File : PS007568.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Nov 2019 15:13
Operator : SM\AJ
Sample : K5138-06
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
AU-08-103019


Manual Integrations
APPROVED

Ankita
11/4/2019 8:25:30 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 01 16:29:22 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
Quant Title : 8080.M
QLast Update : Mon Oct 14 13:54:23 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

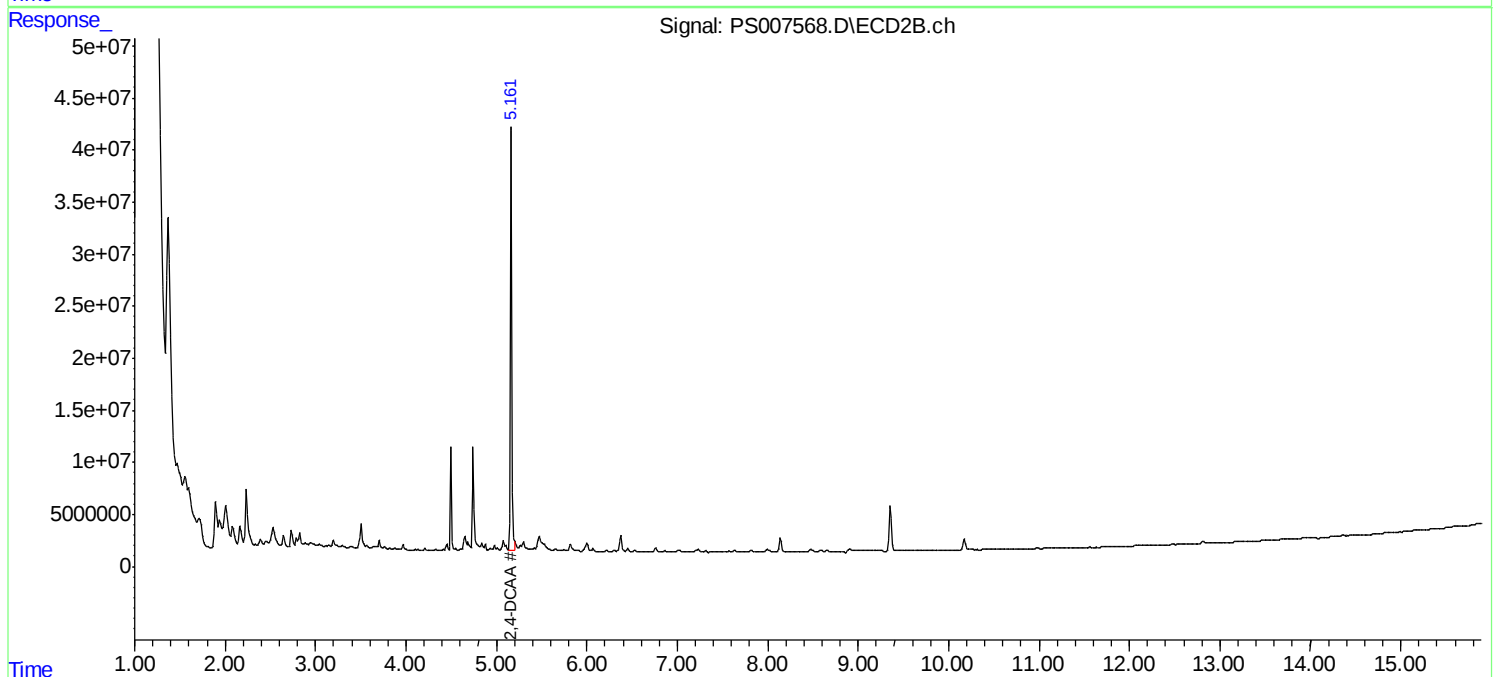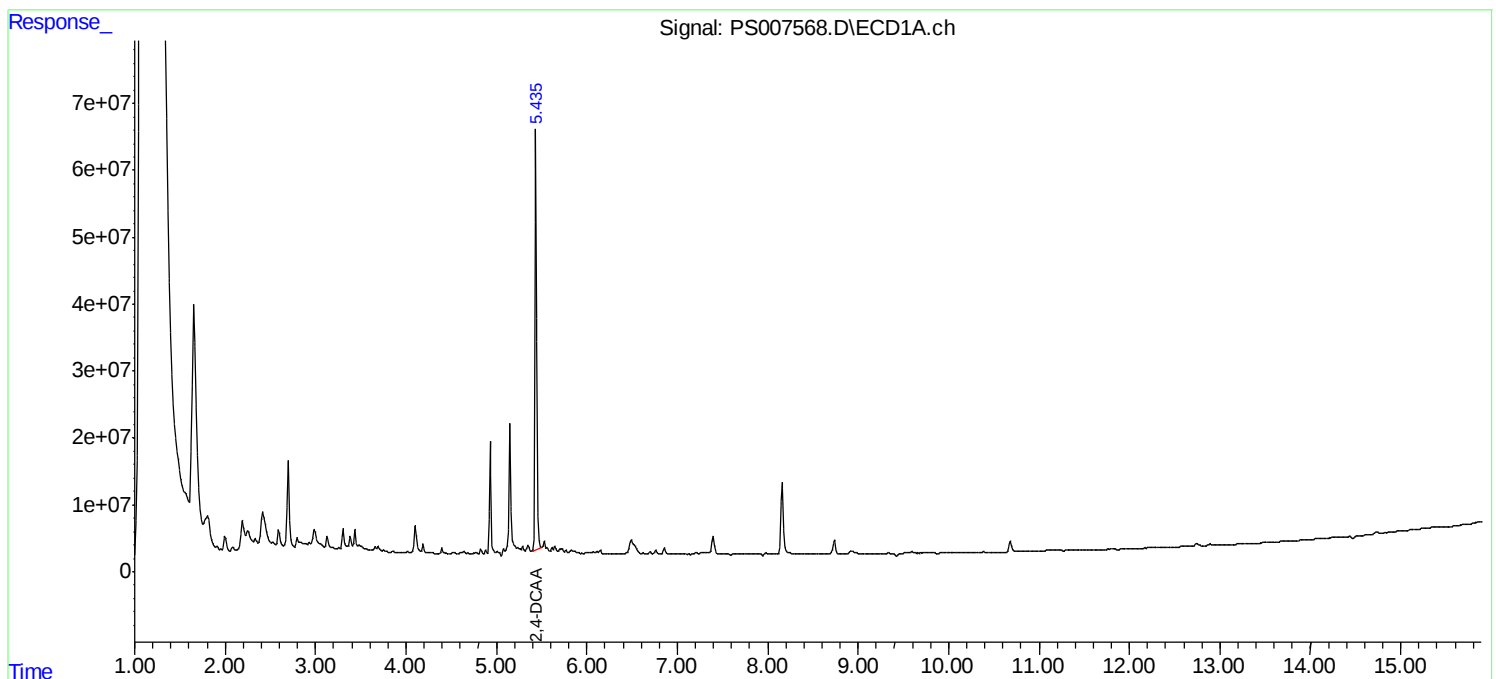

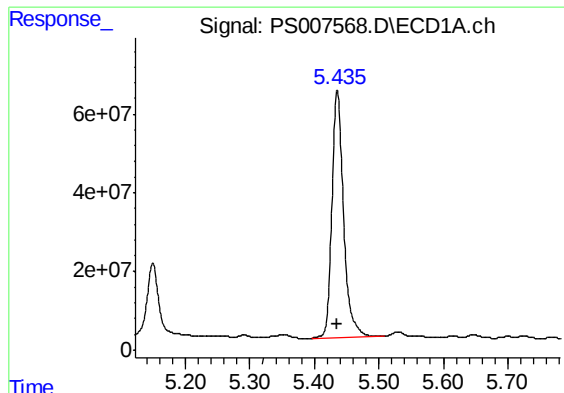


#4 2,4-DCAA

R.T.: 5.436 min
Delta R.T.: 0.000 min
Response: 787010247
Conc: 575.02 ng/ml

Instrument :
ECD_S
ClientSampleId :
AU-08-103019

Manual Integrations
APPROVED

Ankita
11/4/2019 8:25:30 AM

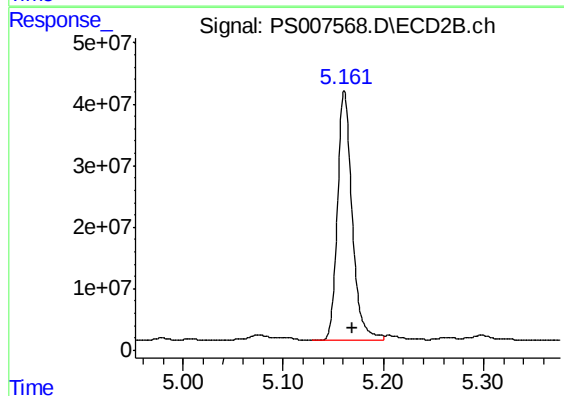

#4 2,4-DCAA

R.T.: 5.161 min
Delta R.T.: -0.008 min
Response: 414979034
Conc: 590.04 ng/ml m