

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110122\
 Data File : PS020986.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Nov 2022 14:25
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 01 15:20:17 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102822.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 31 10:07:57 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.410	6.847	1137.6E6	771.5E6	545.072	557.790
Target Compounds							
3) T	4-Nitroph...	6.249	0.000	5895867	0	3.920	N.D. #
5) T	DICAMBA	0.000	7.001	0	4294941	N.D.	<MDL
6) T	MCP	6.741	7.070f	5844681	2269223	<MDL	<MDL #
7) T	MCPA	6.776f	0.000	7522313	0	<MDL	N.D. #
8) T	DICHLORPROP	7.202f	7.659	-199844	11510605	N.D.	7.475
9) T	2,4-D	0.000	7.981f	0	118846	N.D.	<MDL
10) T	Pentachlo...	7.577	8.371	2722936	2747748	<MDL	<MDL #
11) T	2,4,5-TP ...	8.135	8.752	45868717	9857515	3.453	1.098 #
12) T	2,4,5-T	8.394	9.113	55202623	14166090	4.149	1.643 #
13) T	2,4-DB	8.821f	9.615	-1017204	7761408	N.D.	6.973
14) T	DINOSEB	9.889f	9.969	38689789	10366639	3.563	1.619 #
15) T	Picloram	9.747	10.926	8638200	50038366	<MDL	3.944 #
16) T	DCPA	10.242	10.926f	6721751	50038366	<MDL	4.686 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110122\
Data File : PS020986.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Nov 2022 14:25
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 01 15:20:17 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102822.M
Quant Title : 8080.M
QLast Update : Mon Oct 31 10:07:57 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

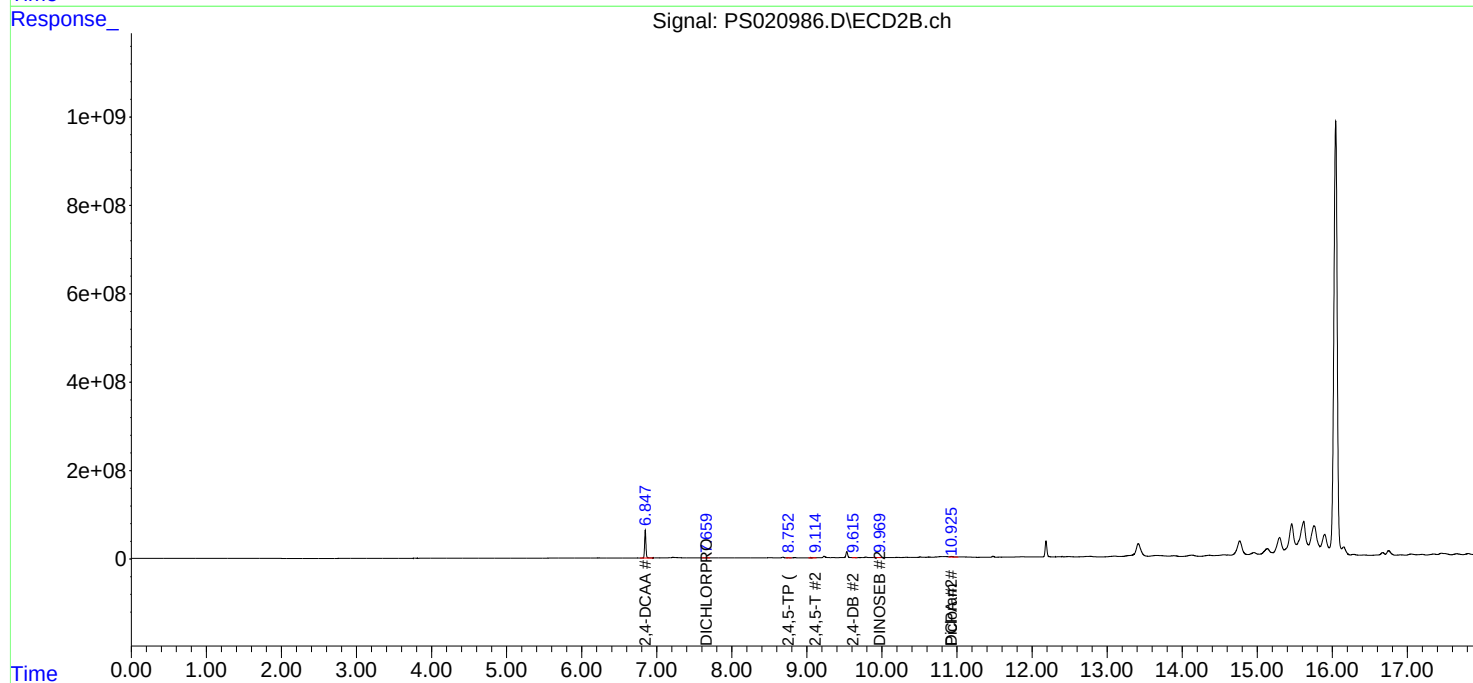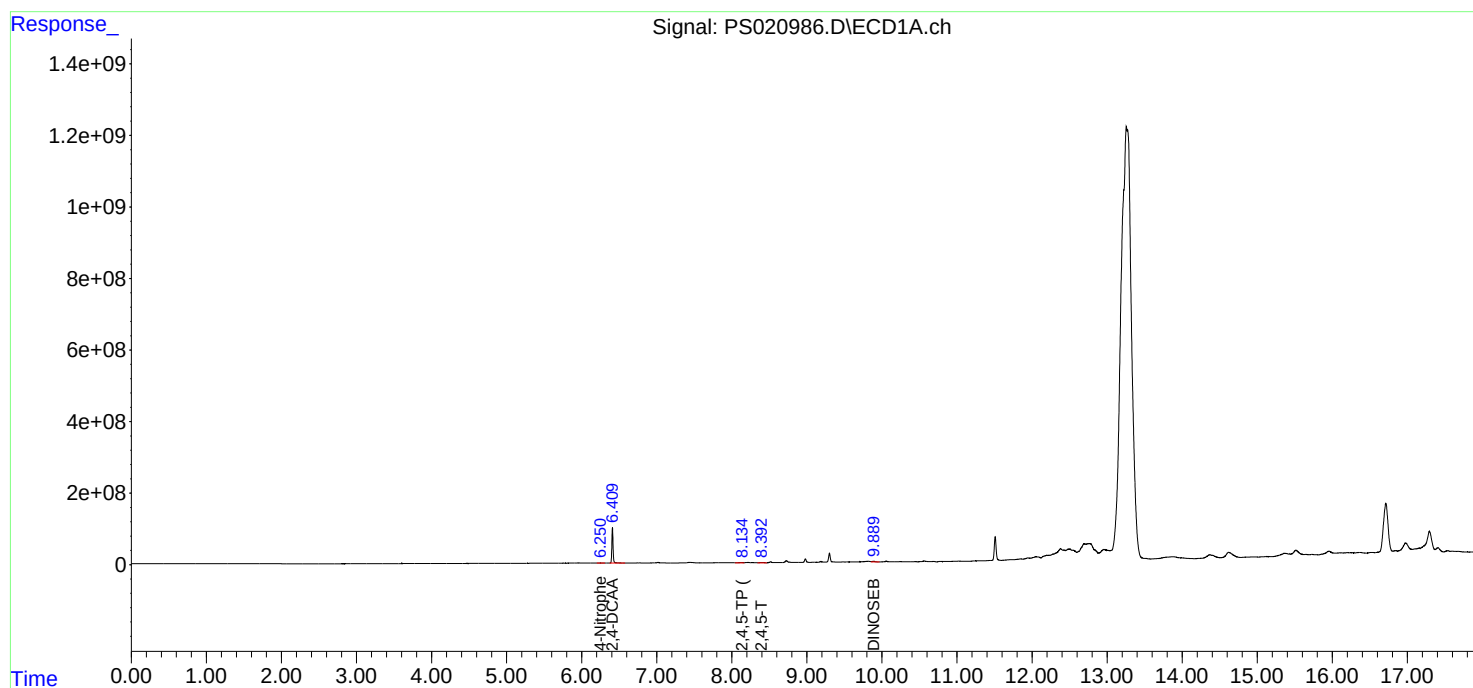


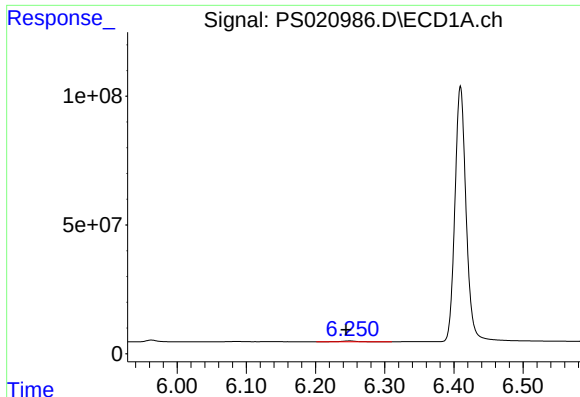

#3 4-Nitrophenol


R.T.: 6.249 min
Delta R.T.: 0.005 min
Response: 5895867
Conc: 3.92 ng/ml

Instrument :
ECD_S
ClientSampleId :

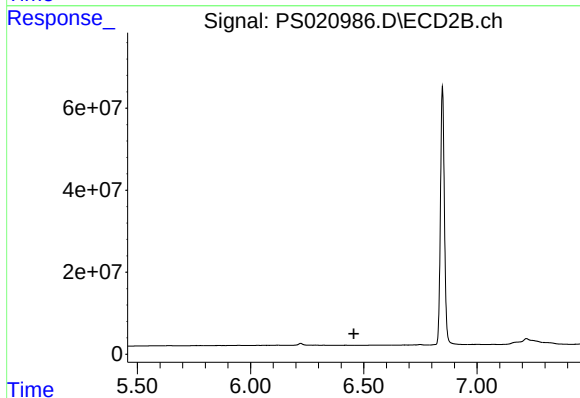


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.456 min
Response: 0
Conc: N.D.

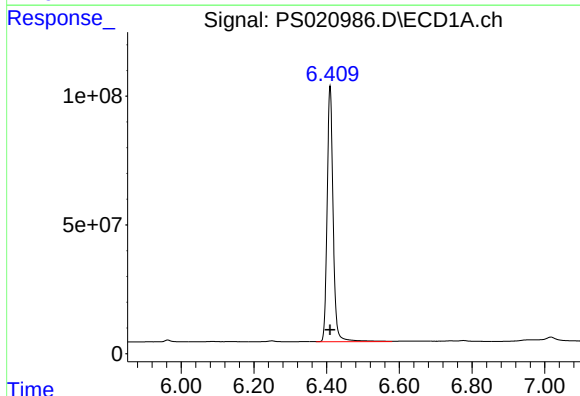


#4 2,4-DCAA

R.T.: 6.410 min
Delta R.T.: 0.000 min
Response: 1137608094
Conc: 545.07 ng/ml

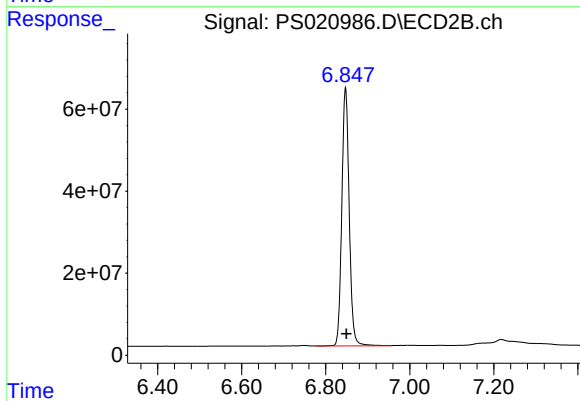

#4 2,4-DCAA


R.T.: 6.847 min
Delta R.T.: -0.002 min
Response: 771504293
Conc: 557.79 ng/ml

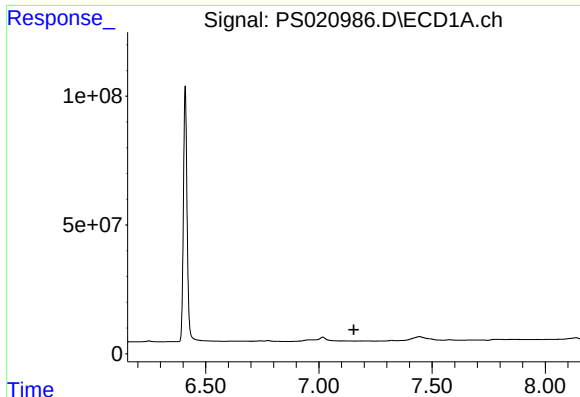

#8 DICHLORPROP


R.T.: 7.202 min
Delta R.T.: 0.047 min
Response: -199844
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

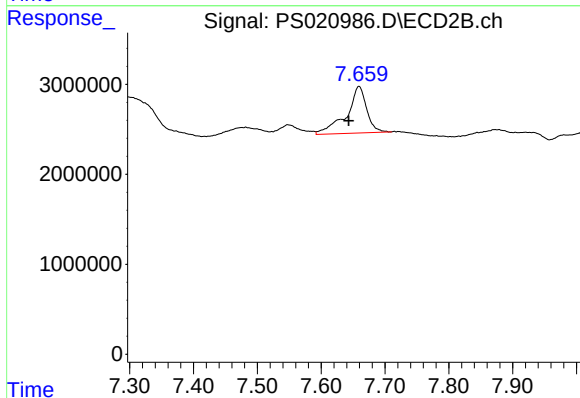


#8 DICHLORPROP

R.T.: 7.659 min
Delta R.T.: 0.016 min
Response: 11510605
Conc: 7.48 ng/ml

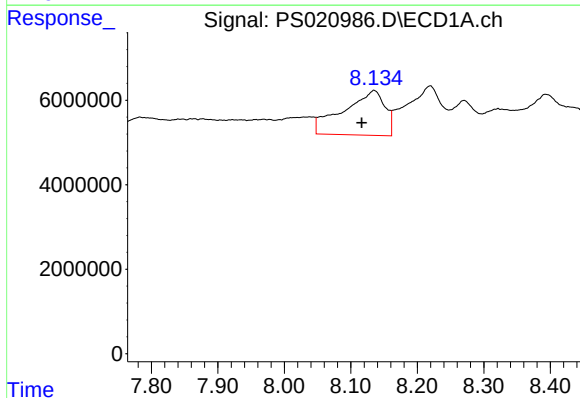


#11 2,4,5-TP (SILVEX)

R.T.: 8.135 min
Delta R.T.: 0.019 min
Response: 45868717
Conc: 3.45 ng/ml

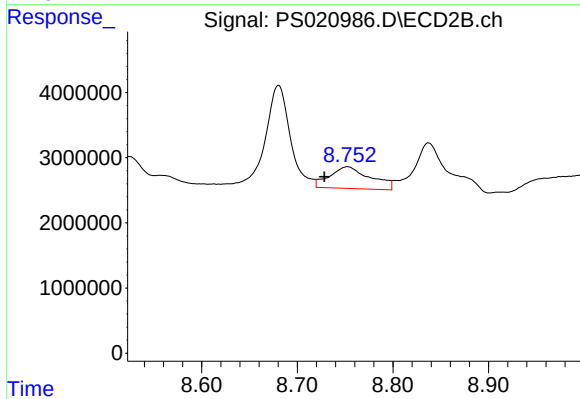

#11 2,4,5-TP (SILVEX)


R.T.: 8.752 min
Delta R.T.: 0.024 min
Response: 9857515
Conc: 1.10 ng/ml

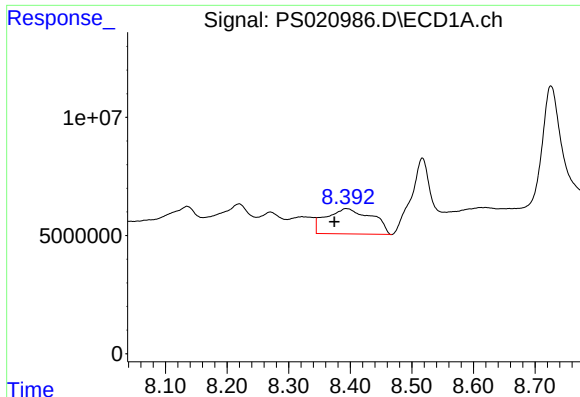

#12 2,4,5-T


R.T.: 8.394 min
Delta R.T.: 0.020 min
Response: 55202623
Conc: 4.15 ng/ml

Instrument :
ECD_S
ClientSampleId :

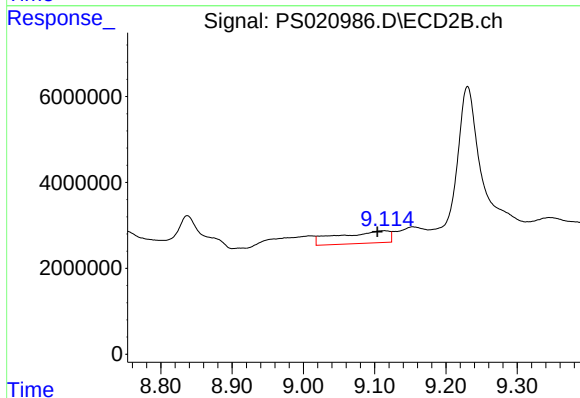


#12 2,4,5-T

R.T.: 9.113 min
Delta R.T.: 0.009 min
Response: 14166090
Conc: 1.64 ng/ml

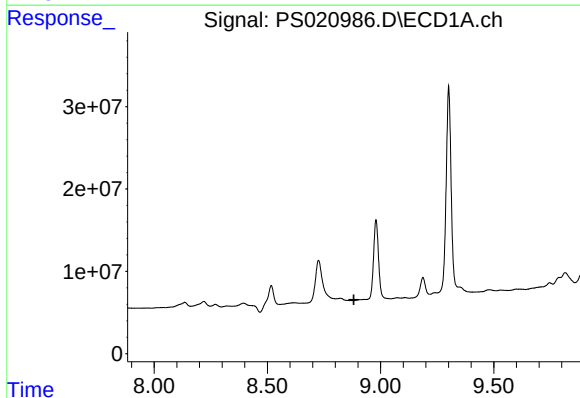


#13 2,4-DB

R.T.: 8.821 min
Delta R.T.: -0.061 min
Response: -1017204
Conc: N.D.

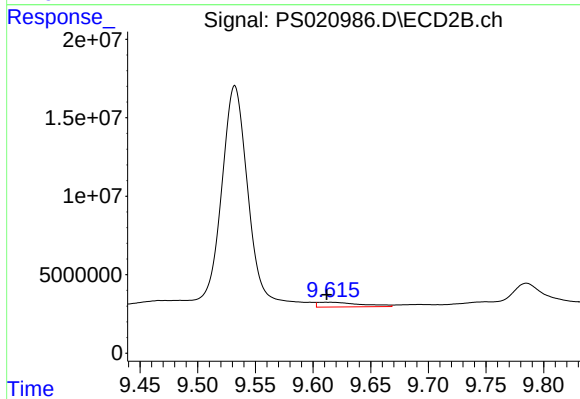

#13 2,4-DB


R.T.: 9.615 min
Delta R.T.: 0.003 min
Response: 7761408
Conc: 6.97 ng/ml

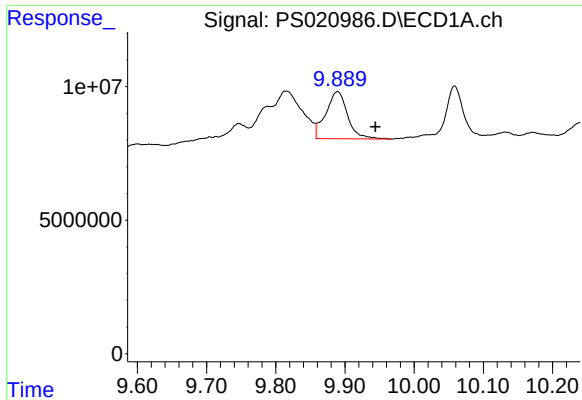

#14 DINOSEB


R.T.: 9.889 min
Delta R.T.: -0.055 min
Response: 38689789
Conc: 3.56 ng/ml

Instrument :
ECD_S
ClientSampleId :

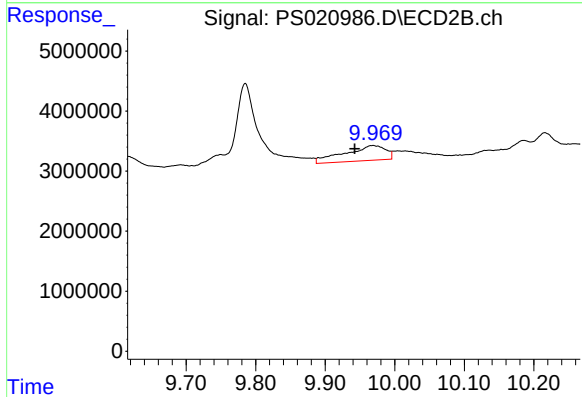


#14 DINOSEB

R.T.: 9.969 min
Delta R.T.: 0.026 min
Response: 10366639
Conc: 1.62 ng/ml

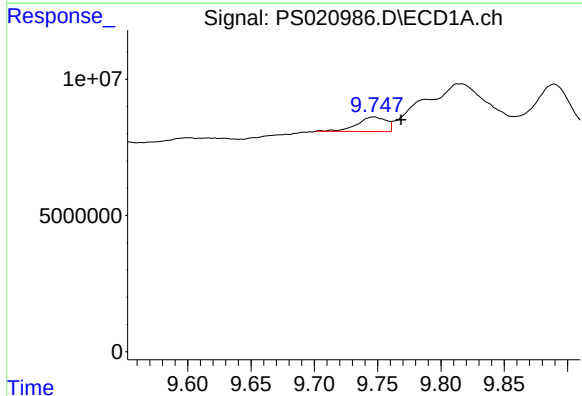


#15 Picloram

R.T.: 9.747 min
Delta R.T.: -0.022 min
Response: 8638200
Conc: N.D.

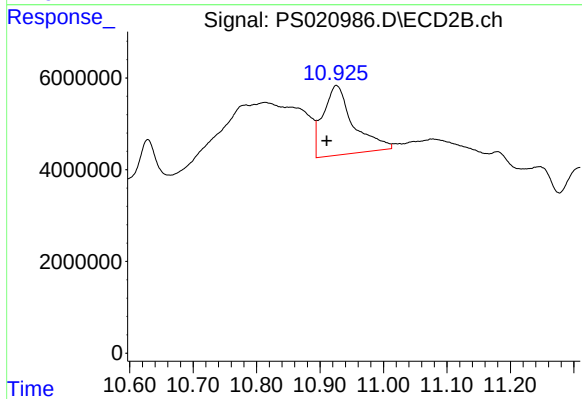

#15 Picloram


R.T.: 10.926 min
Delta R.T.: 0.015 min
Response: 50038366
Conc: 3.94 ng/ml

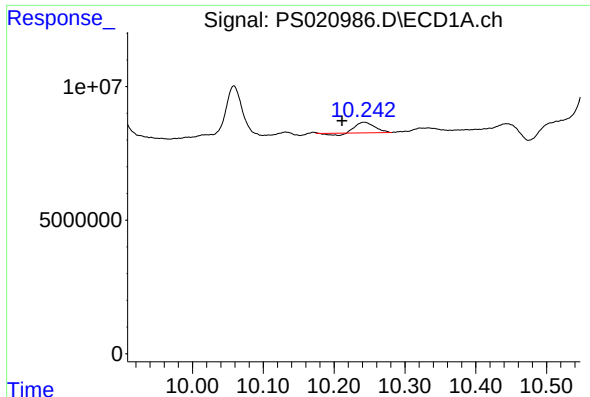

#16 DCPA

R.T.: 10.242 min
Delta R.T.: 0.031 min
Response: 6721751
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

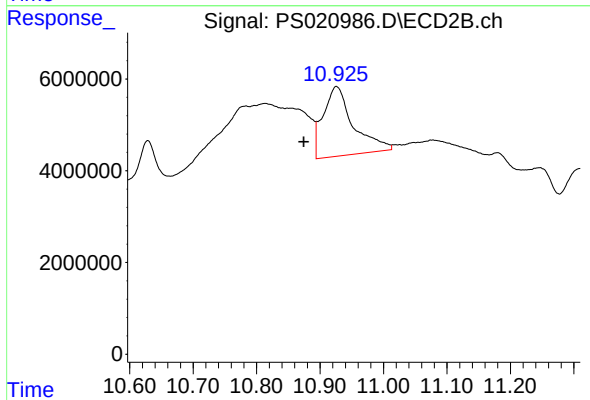

#16 DCPA

R.T.: 10.926 min
Delta R.T.: 0.052 min
Response: 50038366
Conc: 4.69 ng/ml