

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110122\
 Data File : PS020993.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Nov 2022 17:40
 Operator : AR\AJ
 Sample : HSTDCCC750
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HSTDCCC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 02 05:09:08 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102822.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 31 10:07:57 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.409	6.847	1505.0E6	1021.0E6	721.106	738.208
Target Compounds							
1) T	Dalapon	2.507	2.579	1716.0E6	1193.0E6	648.406	655.934
2) T	3,5-DICHL...	5.777	6.019	2035.2E6	1426.0E6	664.609	698.685
3) T	4-Nitroph...	6.246	6.456	982.4E6	597.0E6	653.138	694.366
5) T	DICAMBA	6.554	7.015	5992.6E6	4320.2E6	678.305	695.679
6) T	MCPD	6.713	7.115	442.8E6	324.0E6	67.840	68.208
7) T	MCPA	6.840	7.328	622.6E6	464.2E6	66.353	68.414
8) T	DICHLORPROP	7.154	7.640	1533.6E6	1070.4E6	671.868	695.134
9) T	2,4-D	7.354	7.931	1881.0E6	1310.6E6	673.040	699.784
10) T	Pentachlo...	7.588	8.364	21556.4E6	14866.6E6	684.131	700.863
11) T	2,4,5-TP ...	8.115	8.725	9088.9E6	6288.4E6	684.166	700.744
12) T	2,4,5-T	8.373	9.101	9248.2E6	6105.1E6	695.013	708.079
13) T	2,4-DB	8.882	9.609	1830.2E6	860.6E6	663.358	773.221
14) T	DINOSEB	9.943	9.939	7363.5E6	4477.3E6	678.201	699.425
15) T	Picloram	9.773	10.911	14406.1E6	8676.7E6	682.016	683.883
16) T	DCPA	10.210	10.869	12326.7E6	7571.2E6	681.135	709.057



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110122\
Data File : PS020993.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Nov 2022 17:40
Operator : AR\AJ
Sample : HSTDCCC750
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 02 05:09:08 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102822.M
Quant Title : 8080.M
QLast Update : Mon Oct 31 10:07:57 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

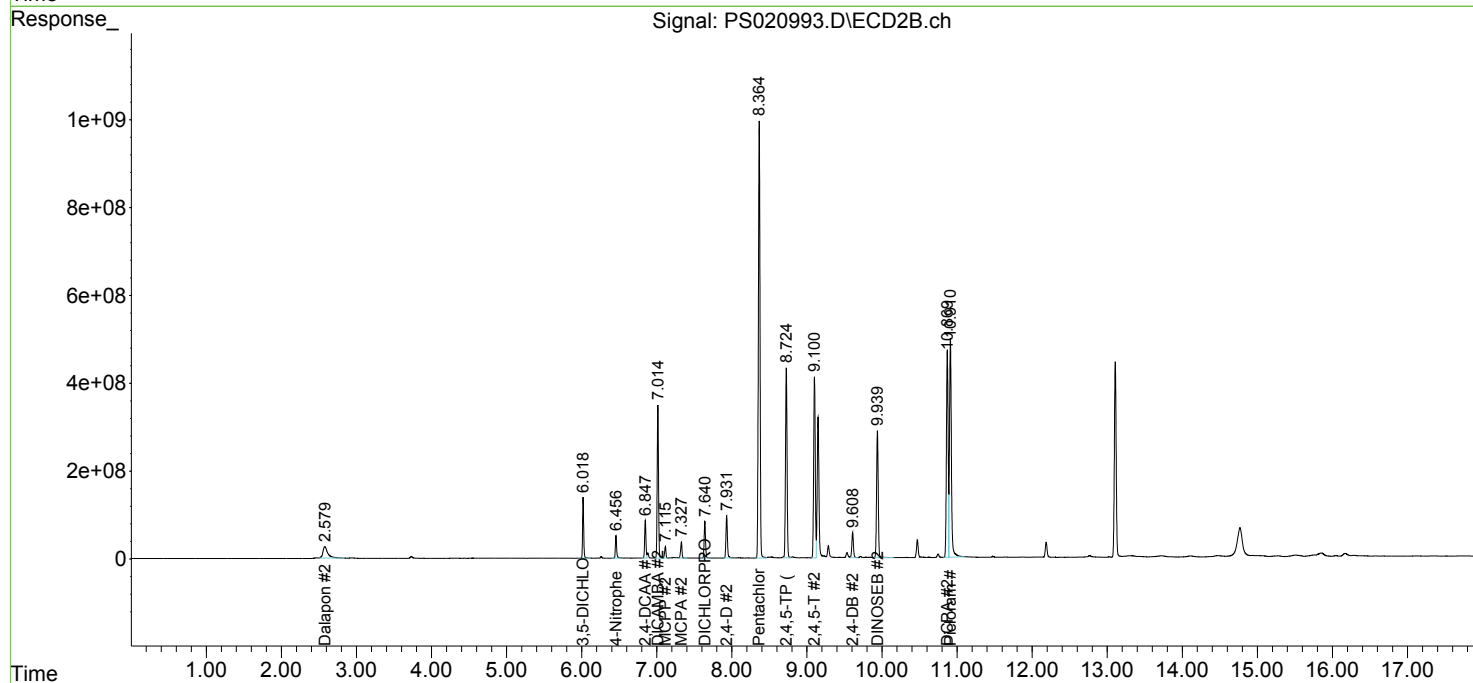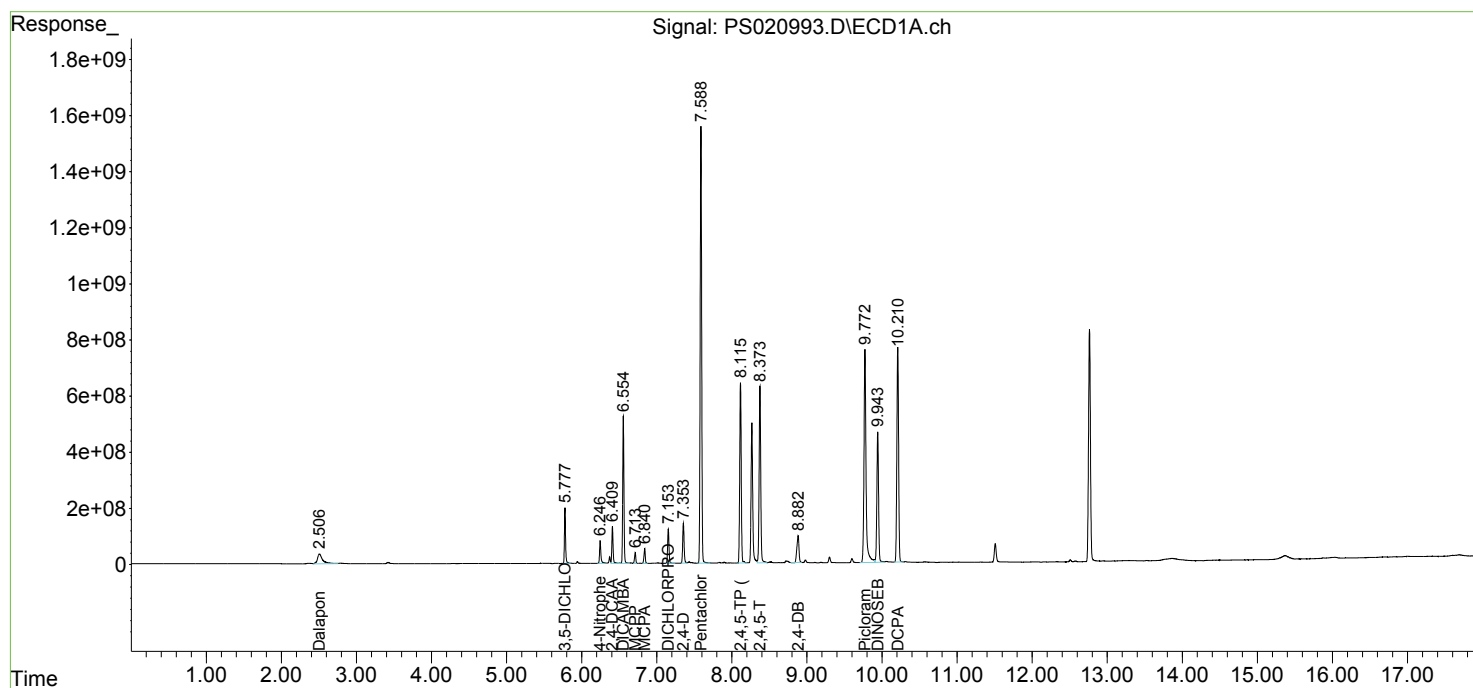


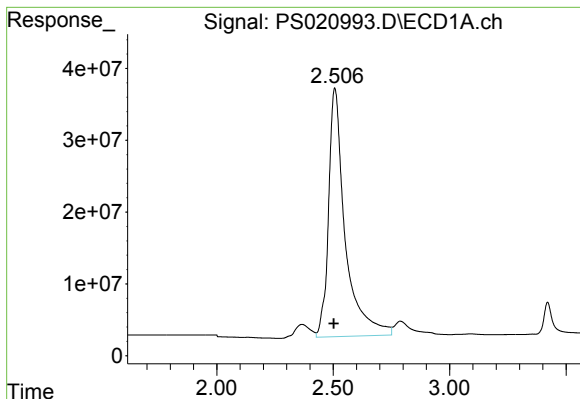

#1 Dalapon


R.T.: 2.507 min
Delta R.T.: 0.003 min
Response: 1716022601
Conc: 648.41 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

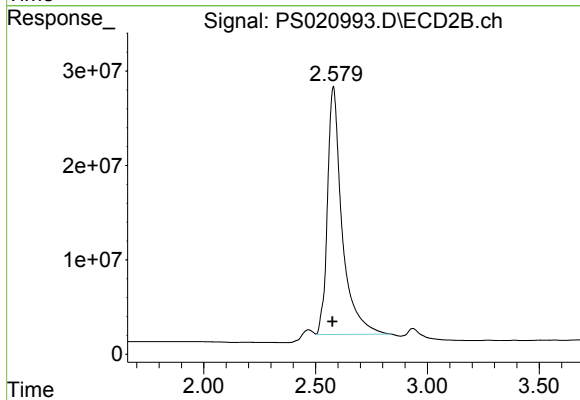


#1 Dalapon

R.T.: 2.579 min
Delta R.T.: 0.004 min
Response: 1192984185
Conc: 655.93 ng/ml

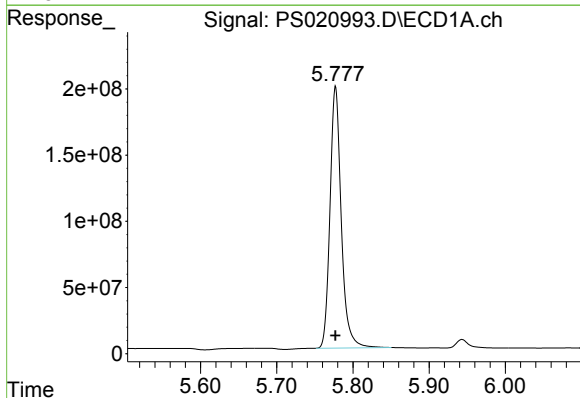


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 5.777 min
Delta R.T.: 0.000 min
Response: 2035216978
Conc: 664.61 ng/ml

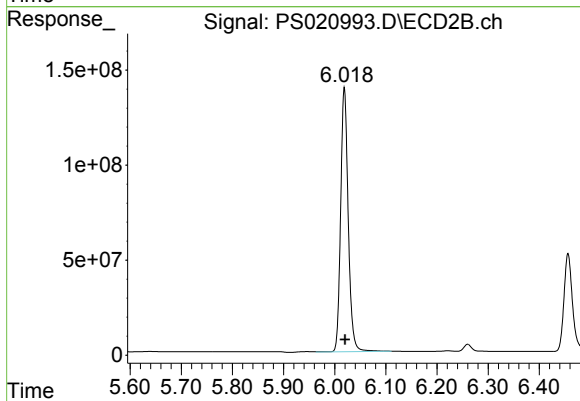

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.019 min
Delta R.T.: -0.001 min
Response: 1425955346
Conc: 698.69 ng/ml

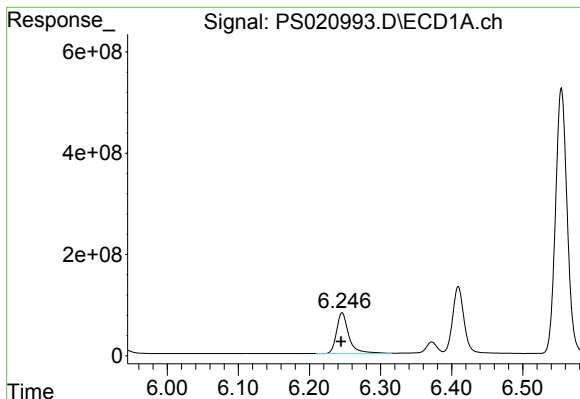

#3 4-Nitrophenol


R.T.: 6.246 min
Delta R.T.: 0.002 min
Response: 982360162
Conc: 653.14 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

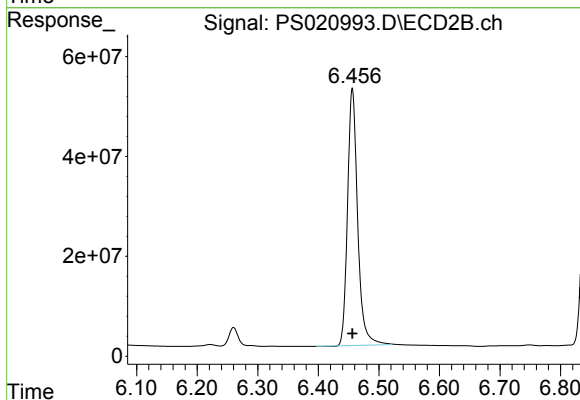


#3 4-Nitrophenol

R.T.: 6.456 min
Delta R.T.: 0.000 min
Response: 597003531
Conc: 694.37 ng/ml

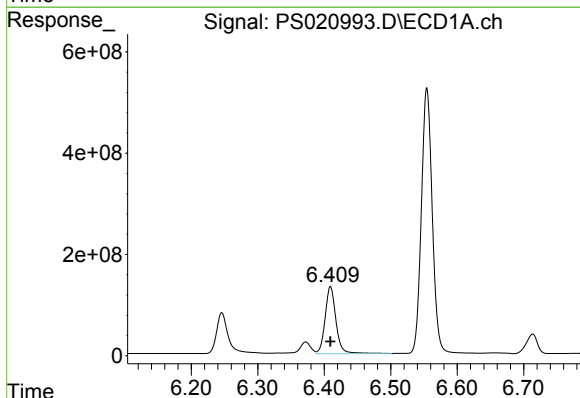


#4 2,4-DCAA

R.T.: 6.409 min
Delta R.T.: 0.000 min
Response: 1505004175
Conc: 721.11 ng/ml

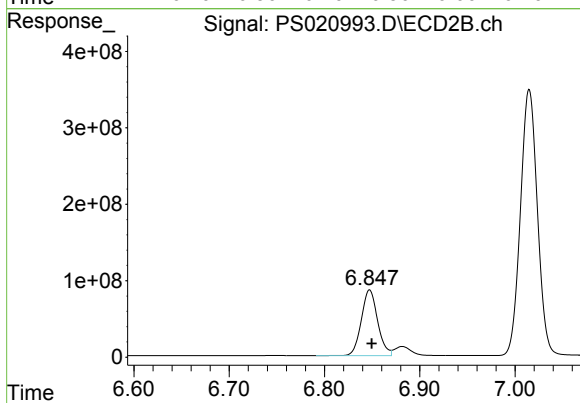

#4 2,4-DCAA


R.T.: 6.847 min
Delta R.T.: -0.002 min
Response: 1021049638
Conc: 738.21 ng/ml

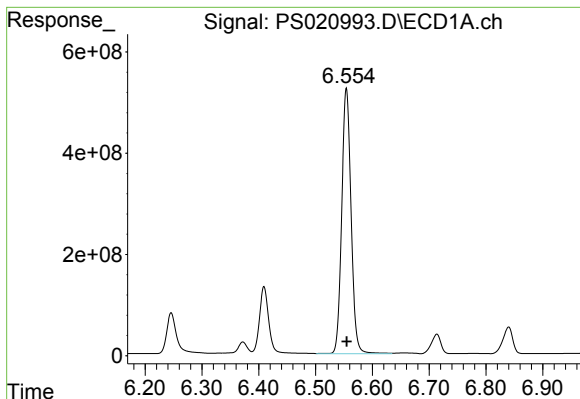

#5 DICAMBA


R.T.: 6.554 min
Delta R.T.: 0.000 min
Response: 5992624918
Conc: 678.31 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

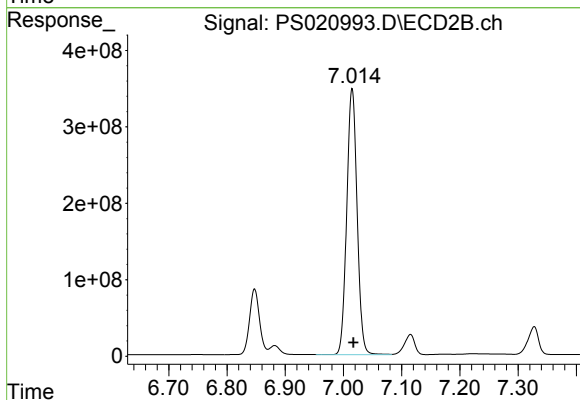


#5 DICAMBA

R.T.: 7.015 min
Delta R.T.: -0.002 min
Response: 4320240053
Conc: 695.68 ng/ml

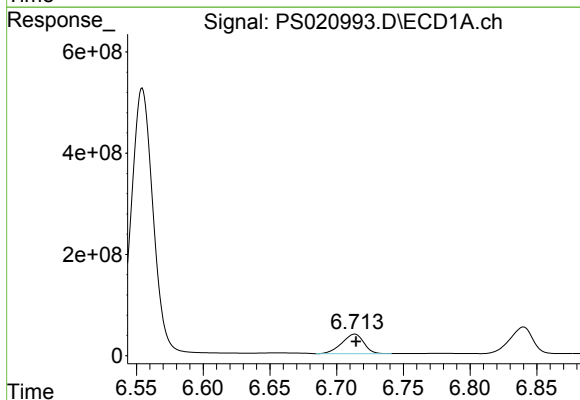


#6 MCP

R.T.: 6.713 min
Delta R.T.: -0.001 min
Response: 442759530
Conc: 67.84 ug/ml

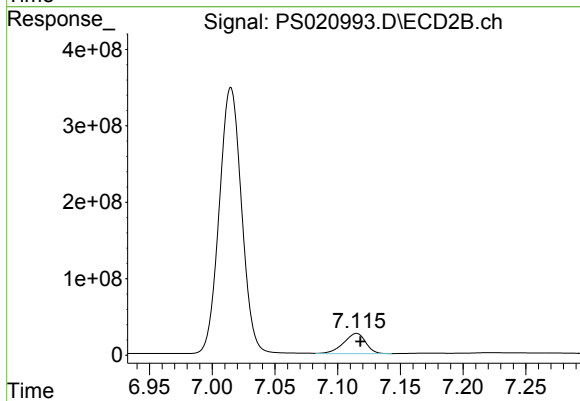

#6 MCP


R.T.: 7.115 min
Delta R.T.: -0.003 min
Response: 324043280
Conc: 68.21 ug/ml

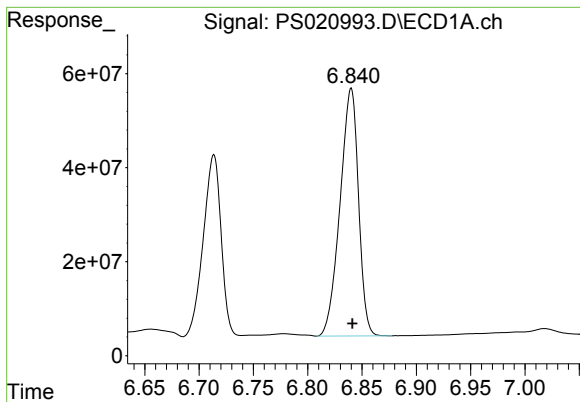

#7 MCPA


R.T.: 6.840 min
Delta R.T.: -0.001 min
Response: 622588425
Conc: 66.35 ug/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

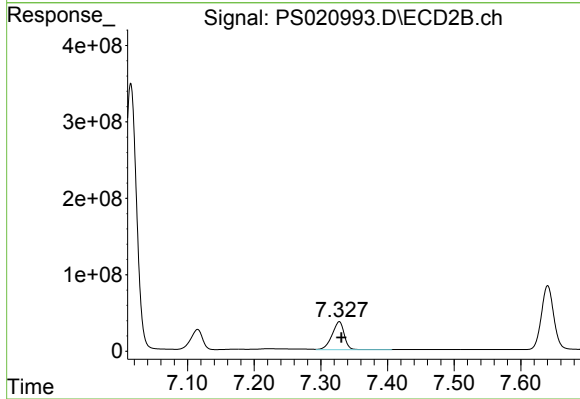


#7 MCPA

R.T.: 7.328 min
Delta R.T.: -0.003 min
Response: 464202686
Conc: 68.41 ug/ml

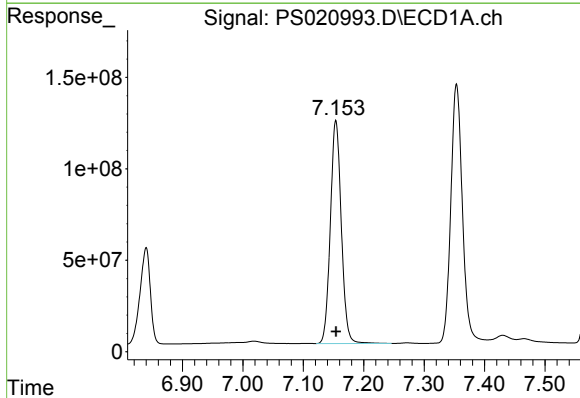


#8 DICHLORPROP

R.T.: 7.154 min
Delta R.T.: 0.000 min
Response: 1533626636
Conc: 671.87 ng/ml

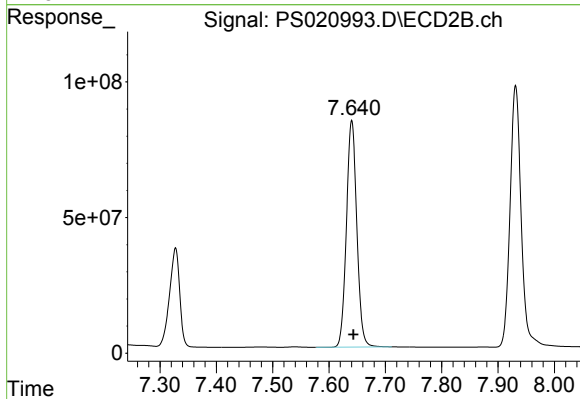

#8 DICHLORPROP


R.T.: 7.640 min
Delta R.T.: -0.003 min
Response: 1070378187
Conc: 695.13 ng/ml

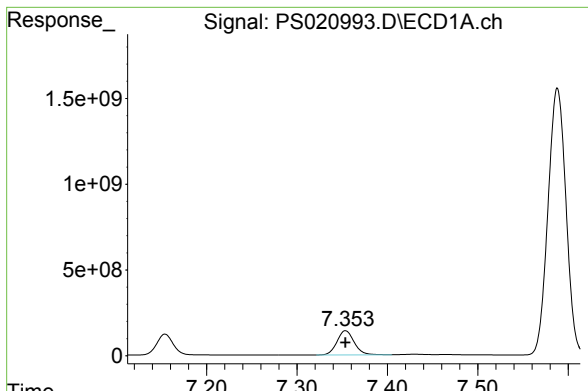

#9 2,4-D


R.T.: 7.354 min
Delta R.T.: 0.000 min
Response: 1880979297
Conc: 673.04 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

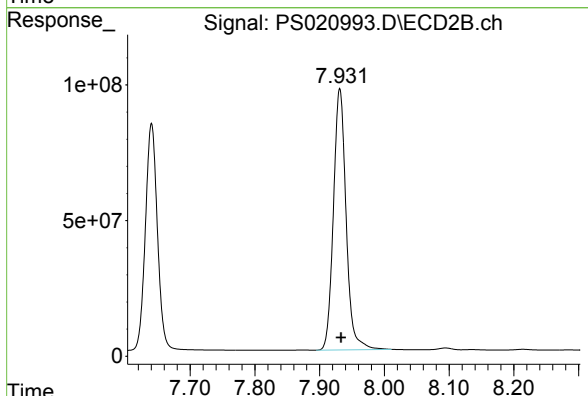


#9 2,4-D

R.T.: 7.931 min
Delta R.T.: -0.002 min
Response: 1310593632
Conc: 699.78 ng/ml

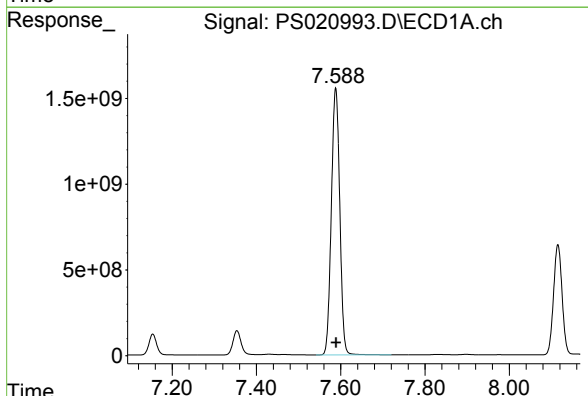


#10 Pentachlorophenol

R.T.: 7.588 min
Delta R.T.: -0.001 min
Response: 21556360186
Conc: 684.13 ng/ml

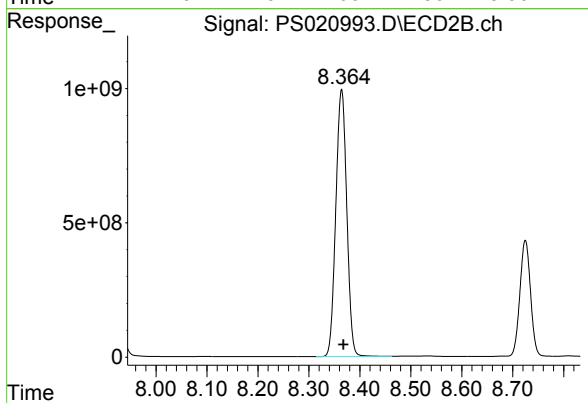

#10 Pentachlorophenol


R.T.: 8.364 min
Delta R.T.: -0.004 min
Response: 14866613599
Conc: 700.86 ng/ml

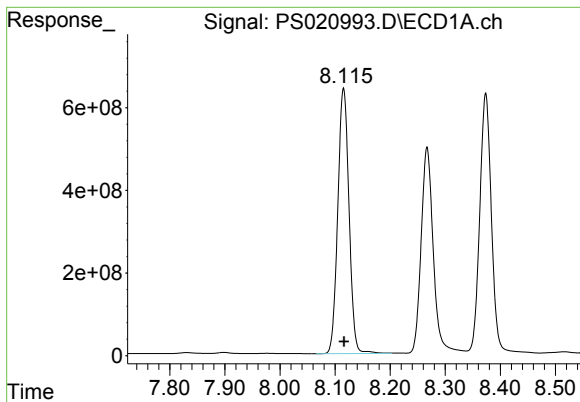

#11 2,4,5-TP (SILVEX)


R.T.: 8.115 min
Delta R.T.: 0.000 min
Response: 9088944015
Conc: 684.17 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

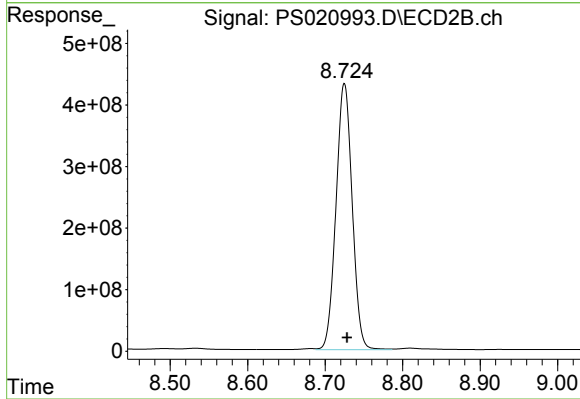


#11 2,4,5-TP (SILVEX)

R.T.: 8.725 min
Delta R.T.: -0.004 min
Response: 6288370545
Conc: 700.74 ng/ml

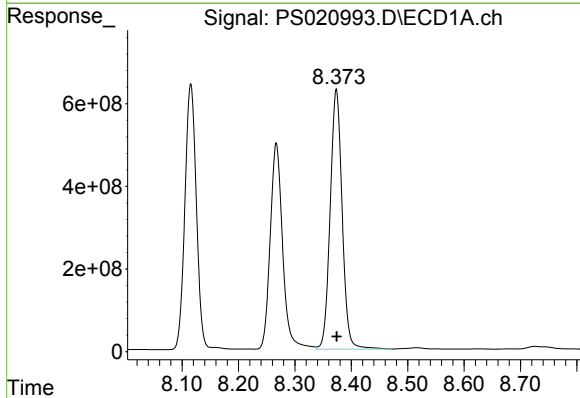


#12 2,4,5-T

R.T.: 8.373 min
Delta R.T.: 0.000 min
Response: 9248232306
Conc: 695.01 ng/ml

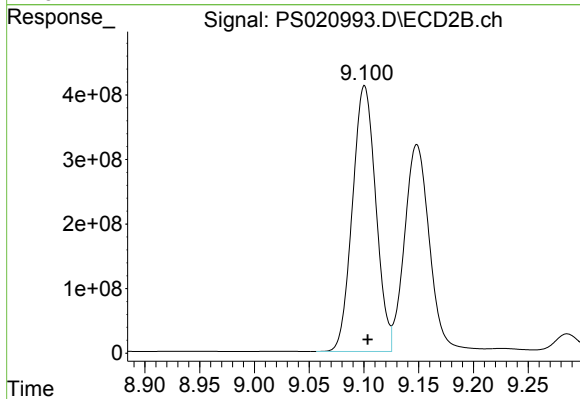

#12 2,4,5-T


R.T.: 9.101 min
Delta R.T.: -0.003 min
Response: 6105102388
Conc: 708.08 ng/ml

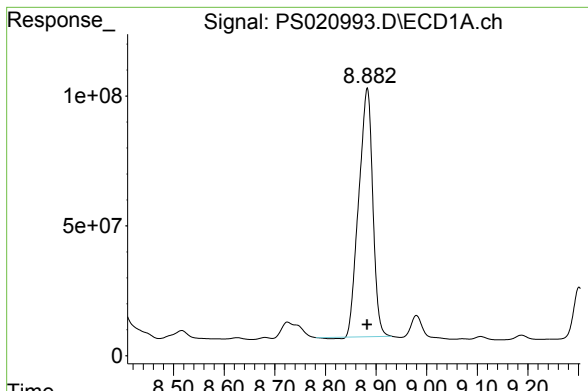

#13 2,4-DB


R.T.: 8.882 min
Delta R.T.: 0.000 min
Response: 1830187265
Conc: 663.36 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

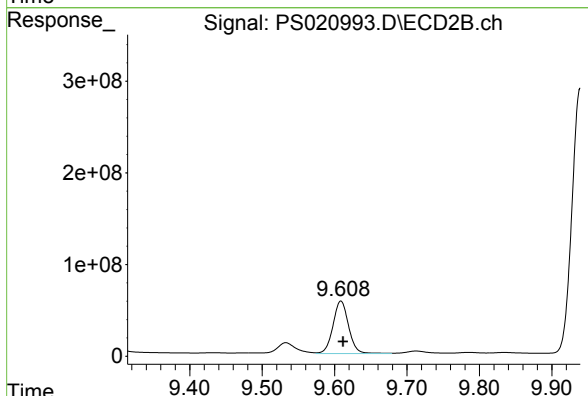


#13 2,4-DB

R.T.: 9.609 min
Delta R.T.: -0.003 min
Response: 860615223
Conc: 773.22 ng/ml

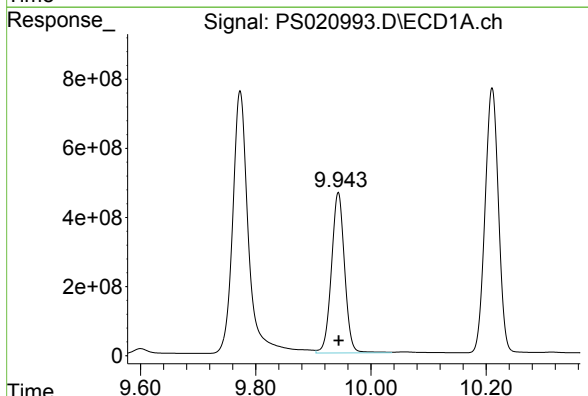


#14 DINOSEB

R.T.: 9.943 min
Delta R.T.: 0.000 min
Response: 7363511749
Conc: 678.20 ng/ml

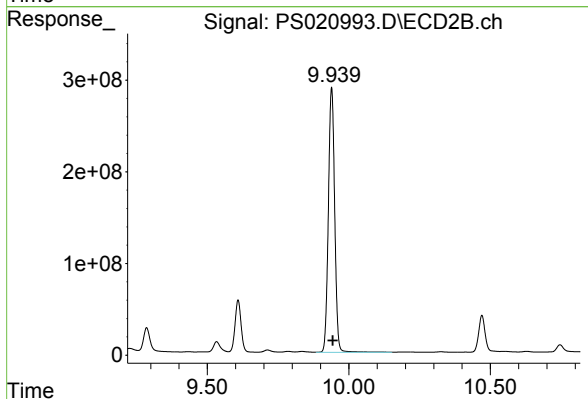

#14 DINOSEB


R.T.: 9.939 min
Delta R.T.: -0.003 min
Response: 4477260862
Conc: 699.43 ng/ml

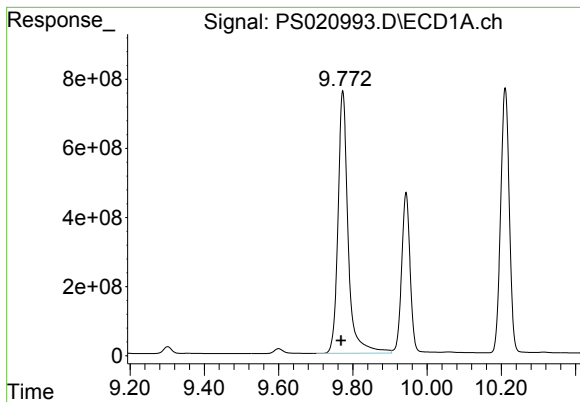

#15 Picloram


R.T.: 9.773 min
Delta R.T.: 0.004 min
Response: 14406072518
Conc: 682.02 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

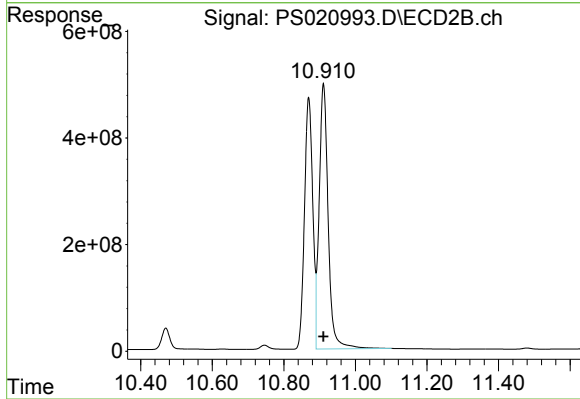


#15 Picloram

R.T.: 10.911 min
Delta R.T.: 0.000 min
Response: 8676749999
Conc: 683.88 ng/ml

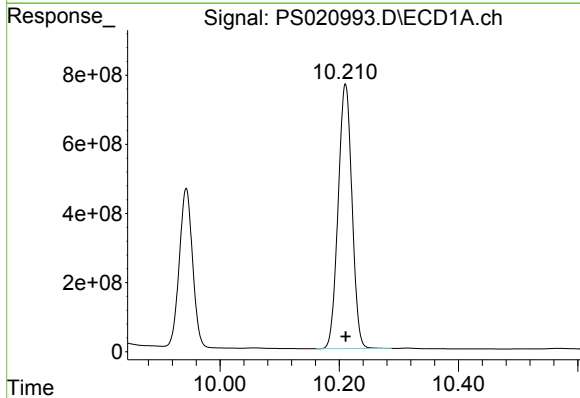

#16 DCPA

R.T.: 10.210 min
Delta R.T.: 0.000 min
Response: 12326727743
Conc: 681.14 ng/ml

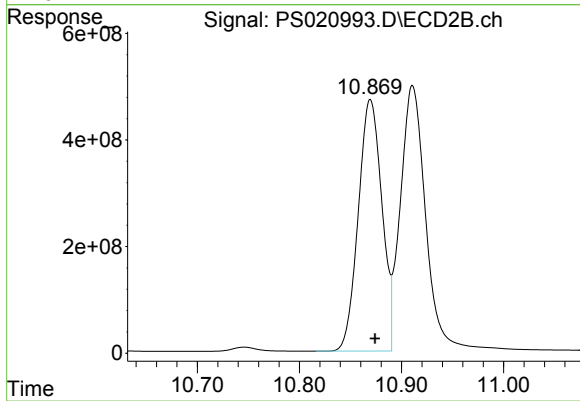

#16 DCPA

R.T.: 10.869 min
Delta R.T.: -0.005 min
Response: 7571221673
Conc: 709.06 ng/ml