

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110218\
 Data File : PS002271.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Nov 2018 11:36
 Operator : EI\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 02 23:22:15 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102618.M
 Quant Title : 8080.M
 QLast Update : Sat Oct 27 01:34:10 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.435	10.927	149.4E6	141.4E6	474.735	393.713
Target Compounds							
7) T	MCPA	0.000	11.820	0	1996827	N.D.	1.475 #
12) T	2,4,5-T	0.000	14.553	0	779713	N.D.	0.521 #
16) T	DCPA	0.000	16.856	0	5177901	N.D.	2.187 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110218\
Data File : PS002271.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Nov 2018 11:36
Operator : EI\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 02 23:22:15 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102618.M
Quant Title : 8080.M
QLast Update : Sat Oct 27 01:34:10 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

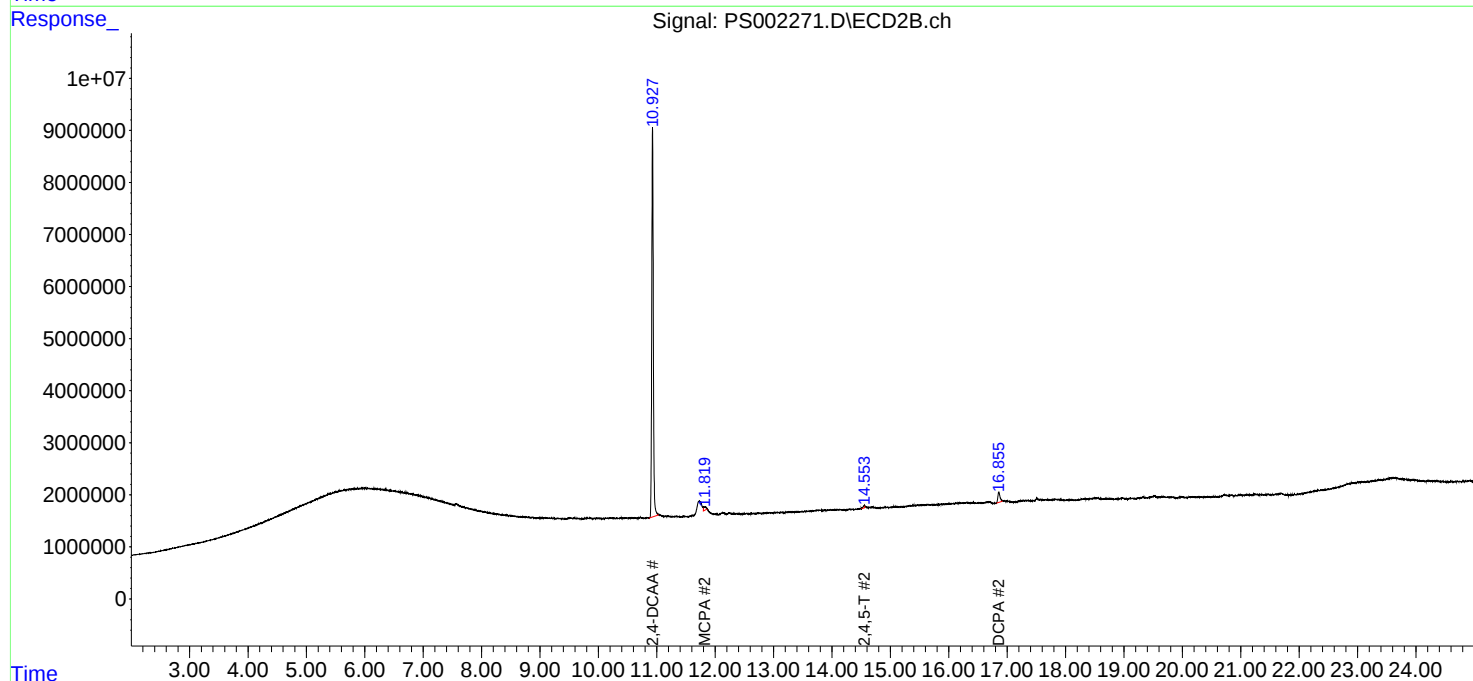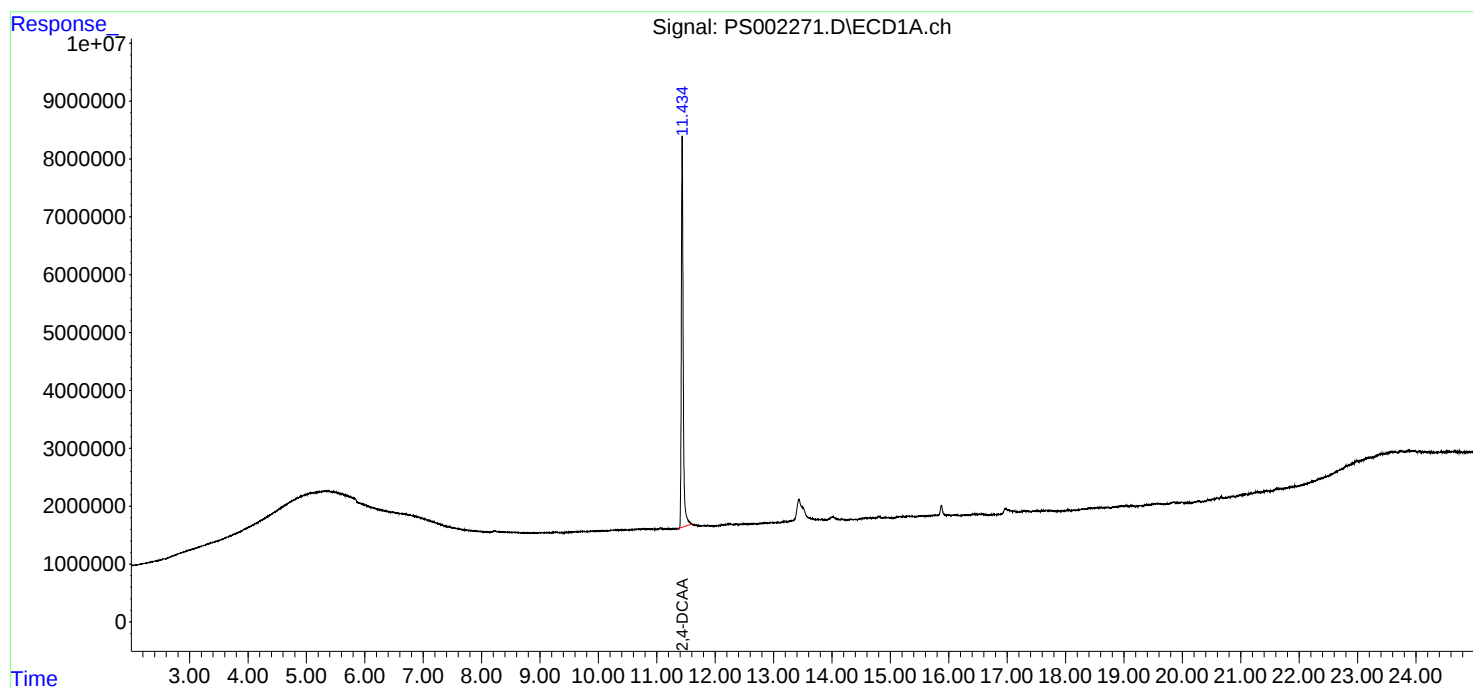


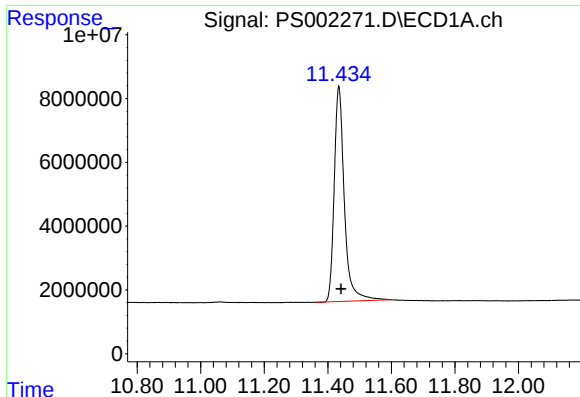

#4 2,4-DCAA


R.T.: 11.435 min
Delta R.T.: -0.006 min
Response: 149392451
Conc: 474.74 ng/ml

Instrument :
ECD_S
ClientSampleId :

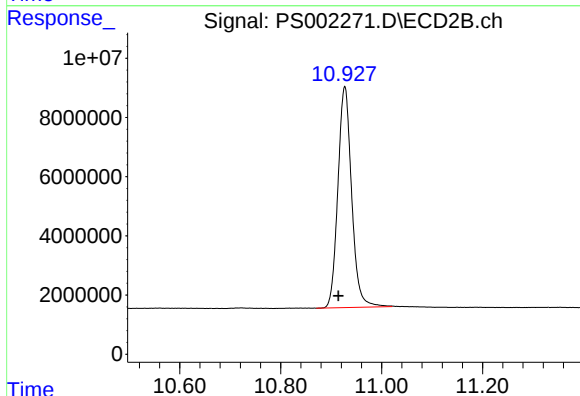


#4 2,4-DCAA

R.T.: 10.927 min
Delta R.T.: 0.013 min
Response: 141381540
Conc: 393.71 ng/ml

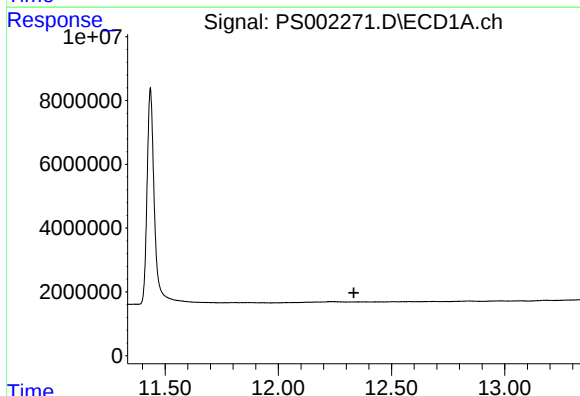


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 12.333 min
Response: 0
Conc: N.D.

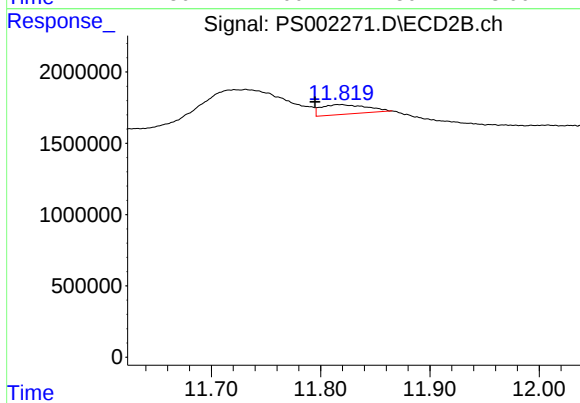

#7 MCPA


R.T.: 11.820 min
Delta R.T.: 0.025 min
Response: 1996827
Conc: 1.48 ug/ml

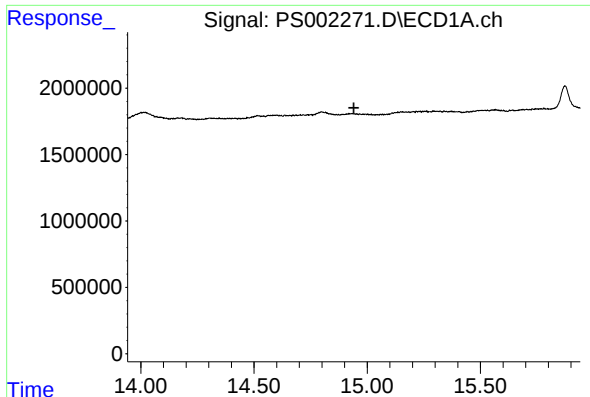

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T. : 14.941 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

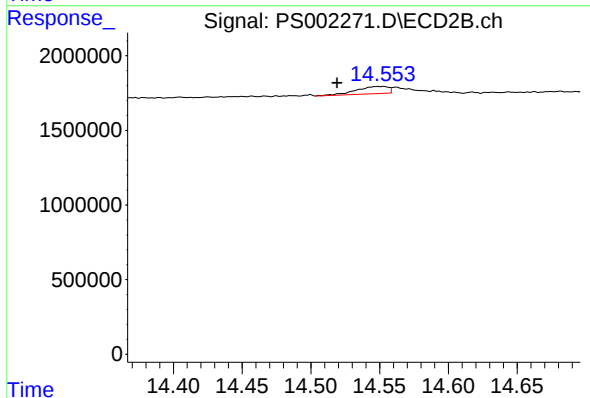


#12 2,4,5-T

R.T.: 14.553 min
Delta R.T.: 0.034 min
Response: 779713
Conc: 0.52 ng/ml

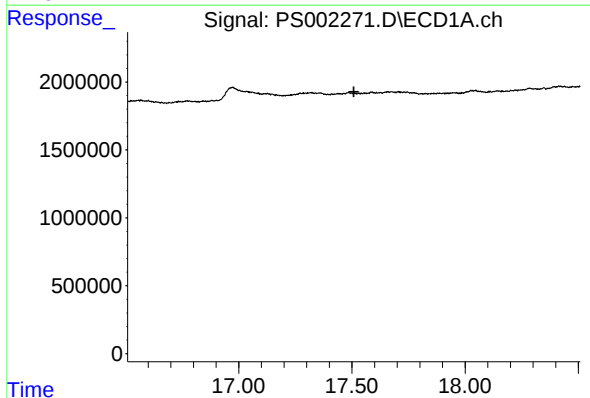

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.509 min
Response: 0
Conc: N.D.

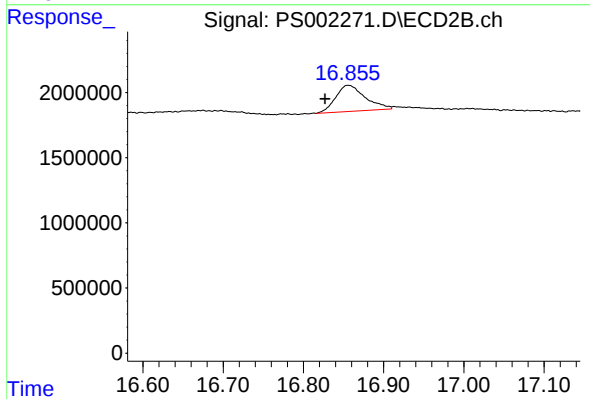

#16 DCPA

R.T.: 16.856 min
Delta R.T.: 0.029 min
Response: 5177901
Conc: 2.19 ng/ml