

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110218\
 Data File : PS002282.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Nov 2018 23:54
 Operator : EI\SJ
 Sample : J5755-08
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 03 06:39:51 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102618.M
 Quant Title : 8080.M
 QLast Update : Sat Oct 27 01:34:10 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.455	10.947	101.8E6	91257136	323.403	254.129
Target Compounds							
1) T	Dalapon	2.928	2.379	30545588	70305863	66.596	155.714 #
2) T	3,5-DICHL...	0.000	9.041	0	2653072	N.D.	5.981 #
3) T	4-Nitroph...	0.000	10.106	0	2627409	N.D.	14.735 #
5) T	DICAMBA	0.000	11.187	0	15538532	N.D.	12.434 #
6) T	MCPD	12.042	0.000	2957584	0	2.994	N.D. #
7) T	MCPA	0.000	11.837	0	994939	N.D.	0.735 #
9) T	2,4-D	0.000	12.780	0	769415	N.D.	1.807 #
11) T	2,4,5-TP ...	0.000	13.896	0	36640783	N.D.	20.027 #
12) T	2,4,5-T	0.000	14.493	0	537191	N.D.	0.359 #
15) T	Picloram	0.000	16.808	0	347919	N.D.	0.154 #
16) T	DCPA	0.000	16.822	0	411693	N.D.	0.174 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110218\
Data File : PS002282.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Nov 2018 23:54
Operator : EI\SJ
Sample : J5755-08
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 03 06:39:51 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102618.M
Quant Title : 8080.M
QLast Update : Sat Oct 27 01:34:10 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

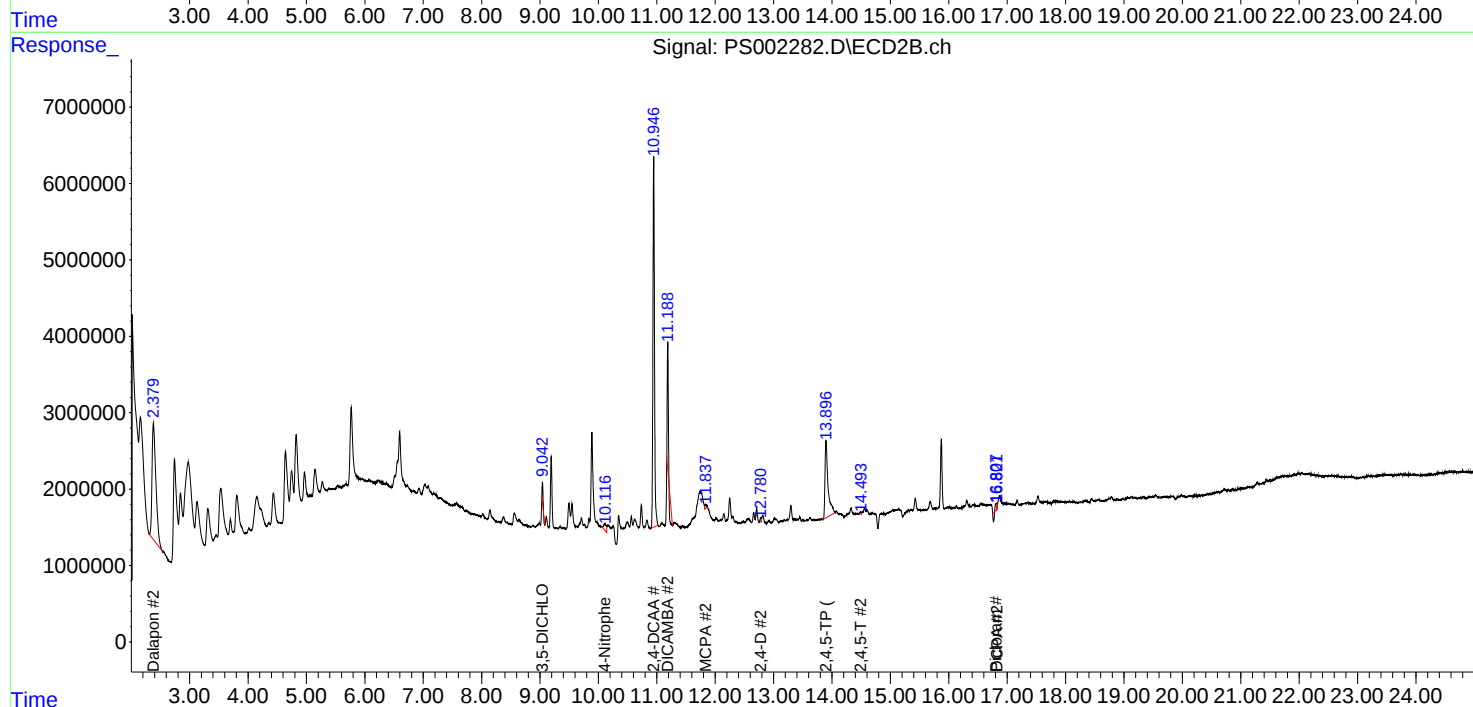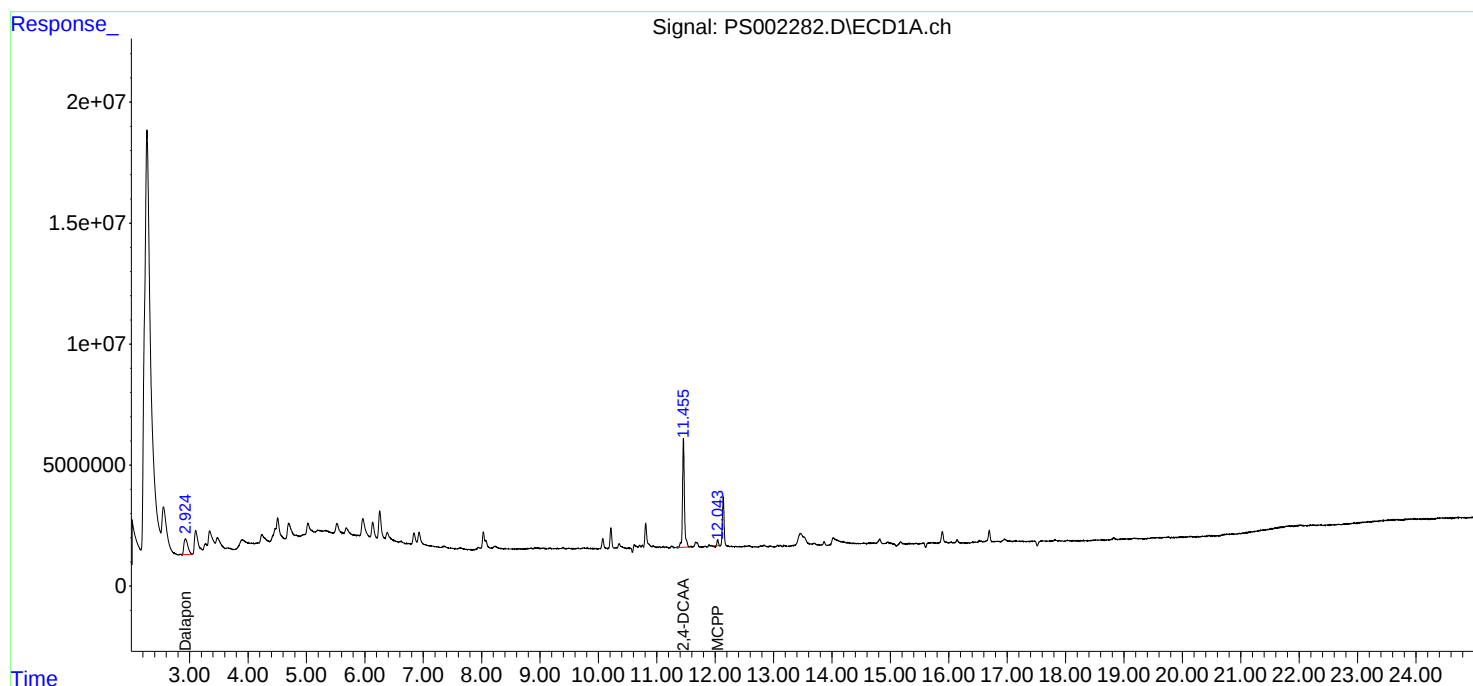


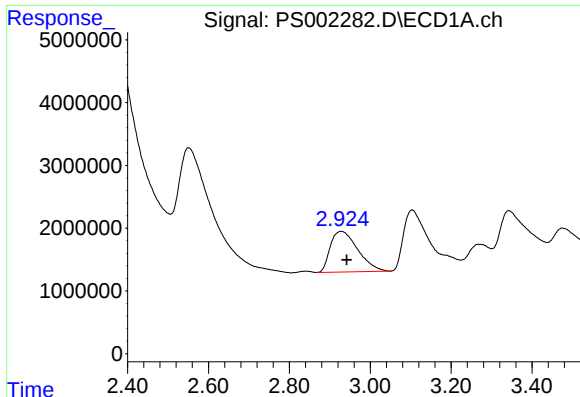

#1 Dalapon


R.T.: 2.928 min
Delta R.T.: -0.014 min
Response: 30545588
Conc: 66.60 ng/ml

Instrument :
ECD_S
ClientSampleId :

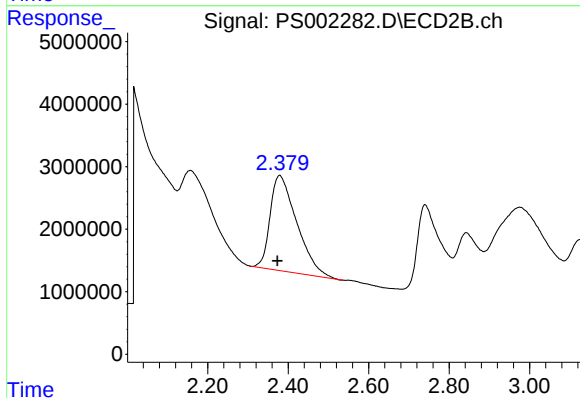


#1 Dalapon

R.T.: 2.379 min
Delta R.T.: 0.006 min
Response: 70305863
Conc: 155.71 ng/ml

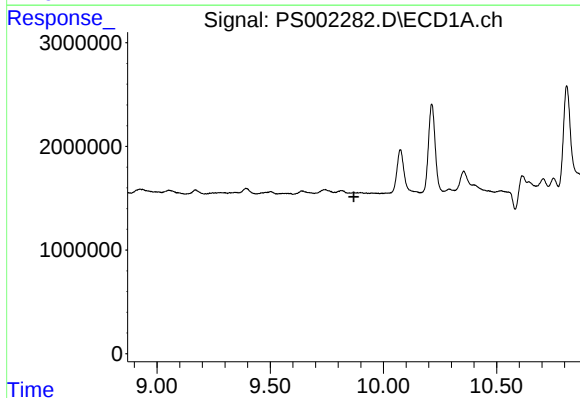


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.870 min
Response: 0
Conc: N.D.

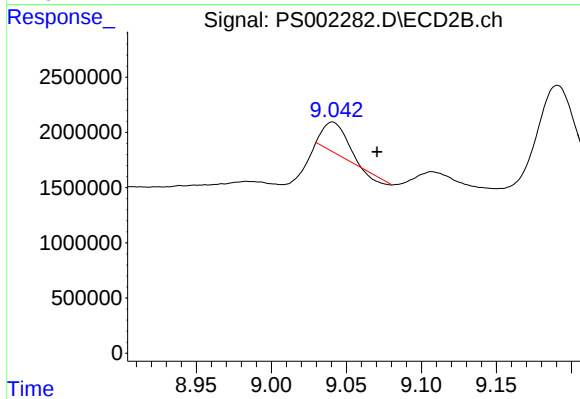

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.041 min
Delta R.T.: -0.030 min
Response: 2653072
Conc: 5.98 ng/ml

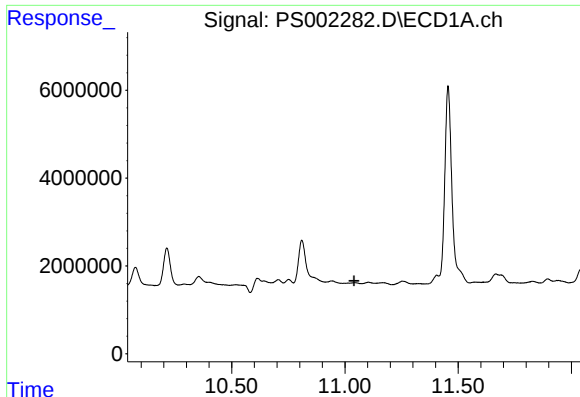

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 11.040 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

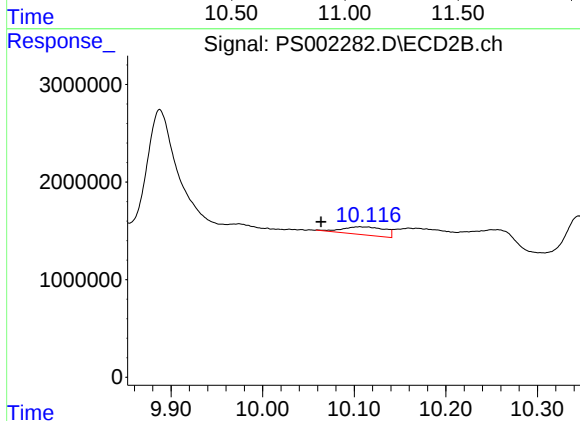


#3 4-Nitrophenol

R.T.: 10.106 min
Delta R.T.: 0.042 min
Response: 2627409
Conc: 14.74 ng/ml

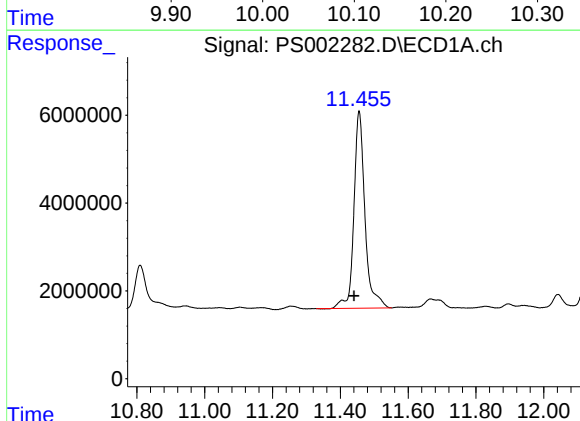


#4 2,4-DCAA

R.T.: 11.455 min
Delta R.T.: 0.014 min
Response: 101770293
Conc: 323.40 ng/ml

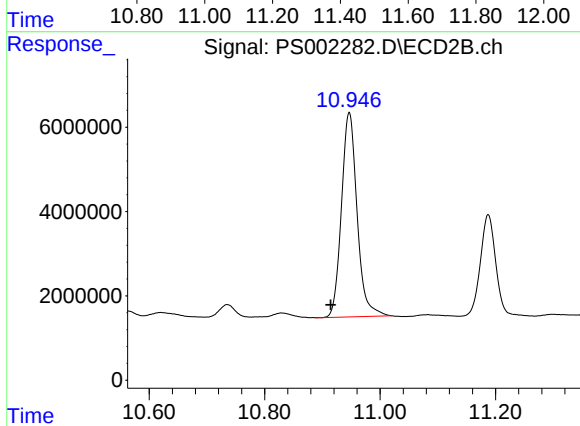

#4 2,4-DCAA


R.T.: 10.947 min
Delta R.T.: 0.032 min
Response: 91257136
Conc: 254.13 ng/ml

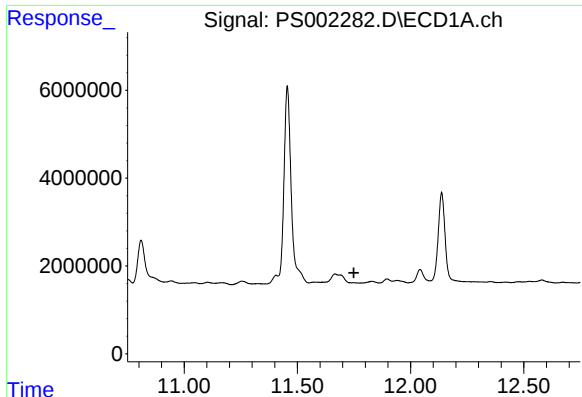

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.750 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

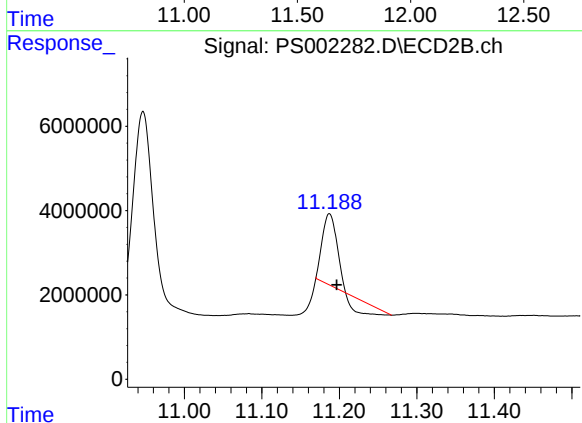


#5 DICAMBA

R.T.: 11.187 min
Delta R.T.: -0.009 min
Response: 15538532
Conc: 12.43 ng/ml

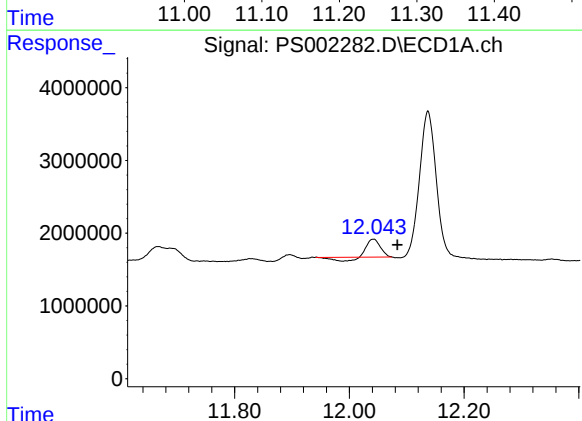


#6 MCP

R.T.: 12.042 min
Delta R.T.: -0.042 min
Response: 2957584
Conc: 2.99 ug/ml

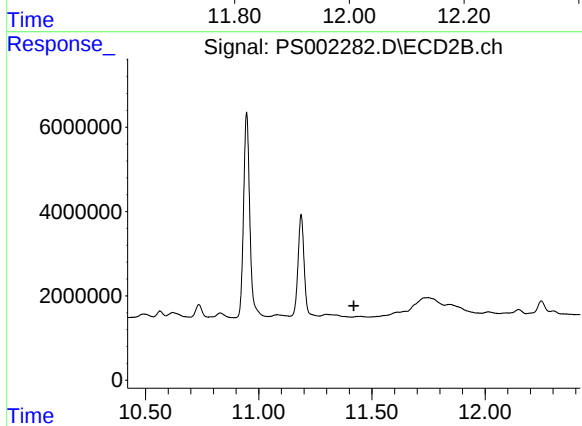

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.420 min
Response: 0
Conc: N.D.

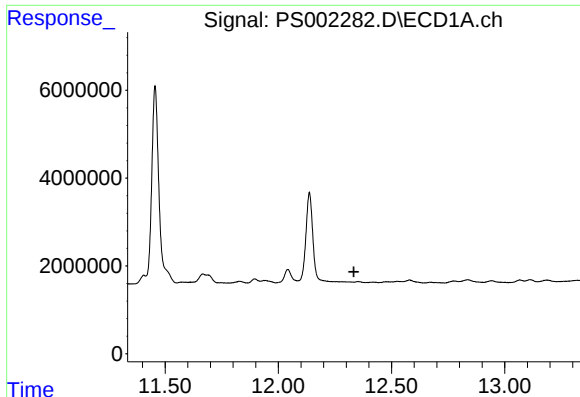

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 12.333 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

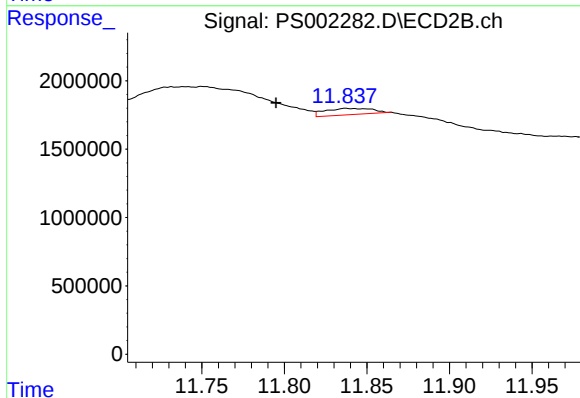


#7 MCPA

R.T.: 11.837 min
Delta R.T.: 0.042 min
Response: 994939
Conc: 0.74 ug/ml

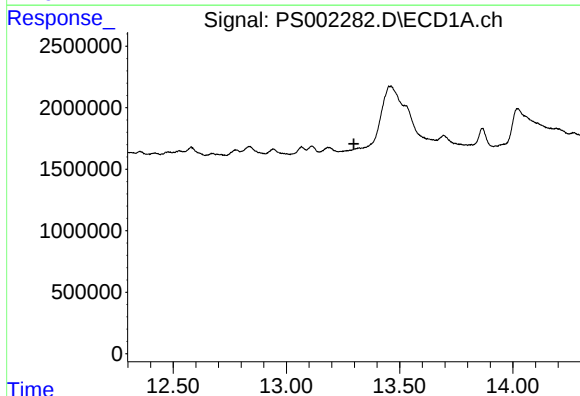


#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 13.298 min
Response: 0
Conc: N.D.

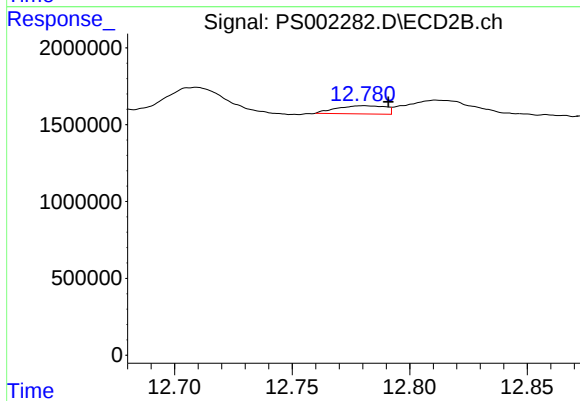

#9 2,4-D


R.T.: 12.780 min
Delta R.T.: -0.010 min
Response: 769415
Conc: 1.81 ng/ml

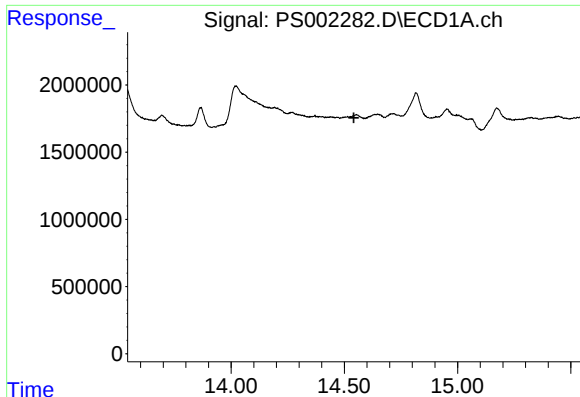

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 14.542 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

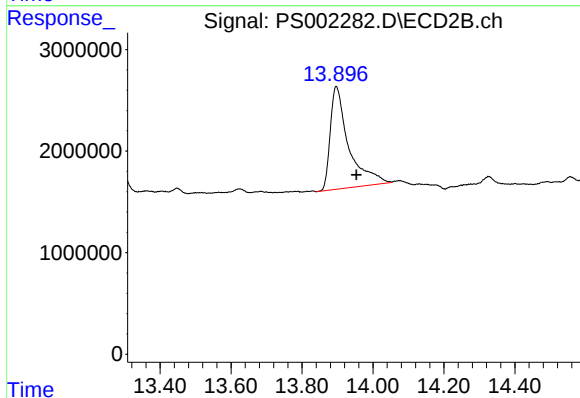


#11 2,4,5-TP (SILVEX)

R.T.: 13.896 min
Delta R.T.: -0.057 min
Response: 36640783
Conc: 20.03 ng/ml

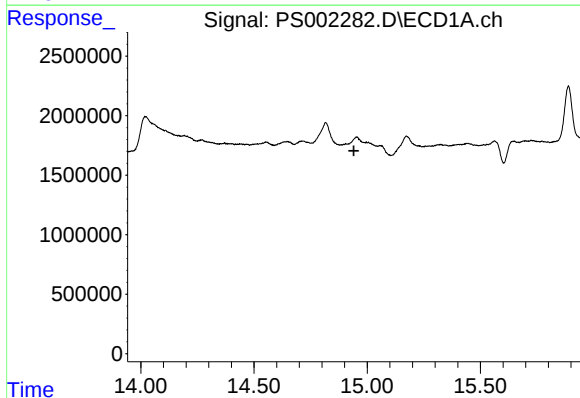


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 14.941 min
Response: 0
Conc: N.D.

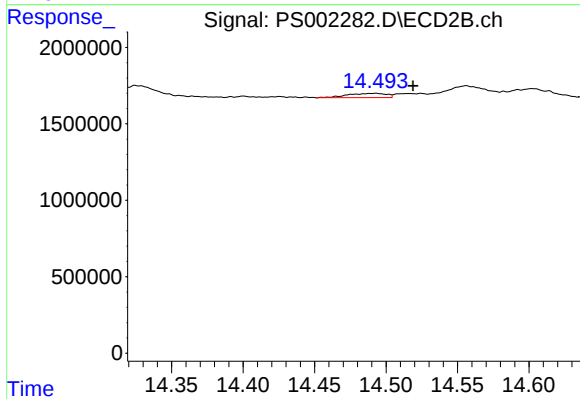

#12 2,4,5-T


R.T.: 14.493 min
Delta R.T.: -0.026 min
Response: 537191
Conc: 0.36 ng/ml

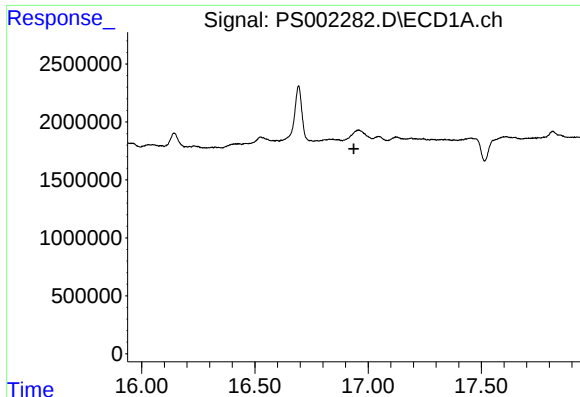

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 16.937 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

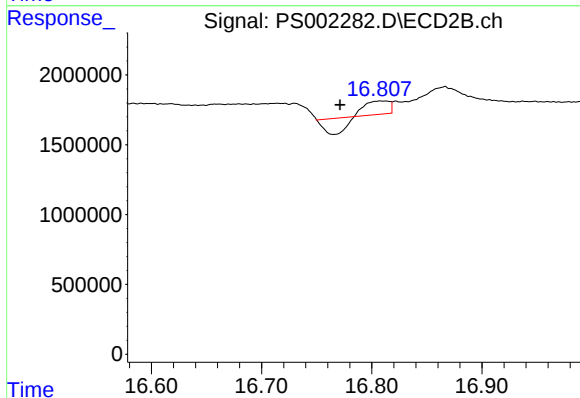


#15 Picloram

R.T.: 16.808 min
Delta R.T.: 0.037 min
Response: 347919
Conc: 0.15 ng/ml

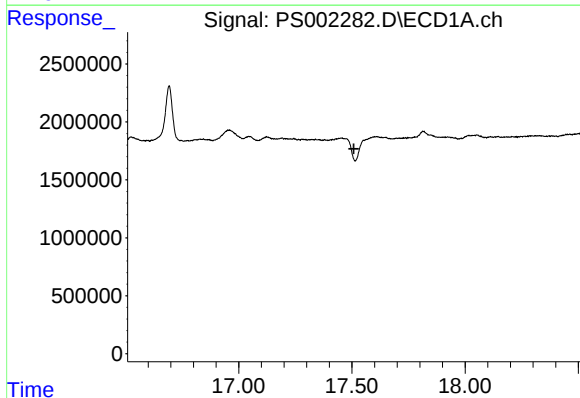

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.509 min
Response: 0
Conc: N.D.

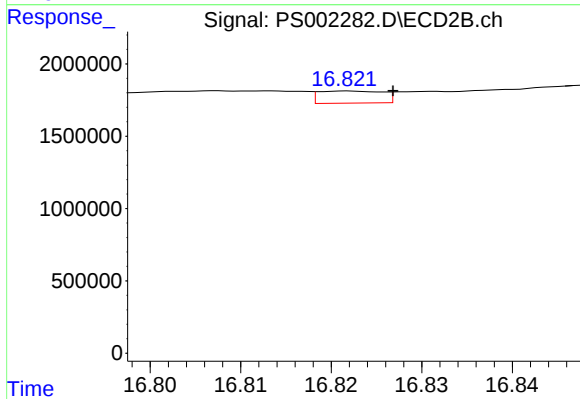

#16 DCPA

R.T.: 16.822 min
Delta R.T.: -0.005 min
Response: 411693
Conc: 0.17 ng/ml