

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110218\
 Data File : PS002299.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Nov 2018 08:42
 Operator : EI\SJ
 Sample : HSTDCCC750
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 05 03:54:53 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102618.M
 Quant Title : 8080.M
 QLast Update : Sat Oct 27 01:34:10 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.417	10.907	129.5E6	282.2E6	411.446	785.809 #
Target Compounds							
1) T	Dalapon	2.936	2.374	305.3E6	298.8E6	665.694	661.790
2) T	3,5-DICHL...	0.000	9.062	0	307.7E6	N.D.	693.720 #
3) T	4-Nitroph...	11.010	10.053	123.4E6	122.9E6	739.473	689.449
5) T	DICAMBA	11.727	11.190	976.2E6	464.2E6	735.118	371.415 #
6) T	MCPD	0.000	11.422	0	66755117	N.D.	77.592 #
7) T	MCPA	0.000	11.797	0	108.2E6	N.D.	79.944 #
8) T	DICHLORPROP	12.913	12.313	252.5E6	-58258923	725.127	N.D. #
9) T	2,4-D	0.000	12.784	0	209.4E6	N.D.	491.732 #
10) T	Pentachlo...	13.650	13.330	3539.6E6	3217.8E6	735.775	685.013
11) T	2,4,5-TP ...	0.000	13.948	0	1503.0E6	N.D.	821.515 #
12) T	2,4,5-T	14.915	14.511	1195.1E6	982.3E6	666.794	655.942
13) T	2,4-DB	0.000	15.162	0	108.3E6	N.D.	488.674 #
14) T	DINOSEB	17.140	15.589	1002.5E6	1030.7E6	731.759	814.228
15) T	Picloram	16.907	16.767	1560.4E6	1620.3E6	654.182	716.264
16) T	DCPA	0.000	16.820	0	1382.4E6	N.D.	583.802 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110218\
Data File : PS002299.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Nov 2018 08:42
Operator : EI\SJ
Sample : HSTDCCC750
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 05 03:54:53 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102618.M
Quant Title : 8080.M
QLast Update : Sat Oct 27 01:34:10 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

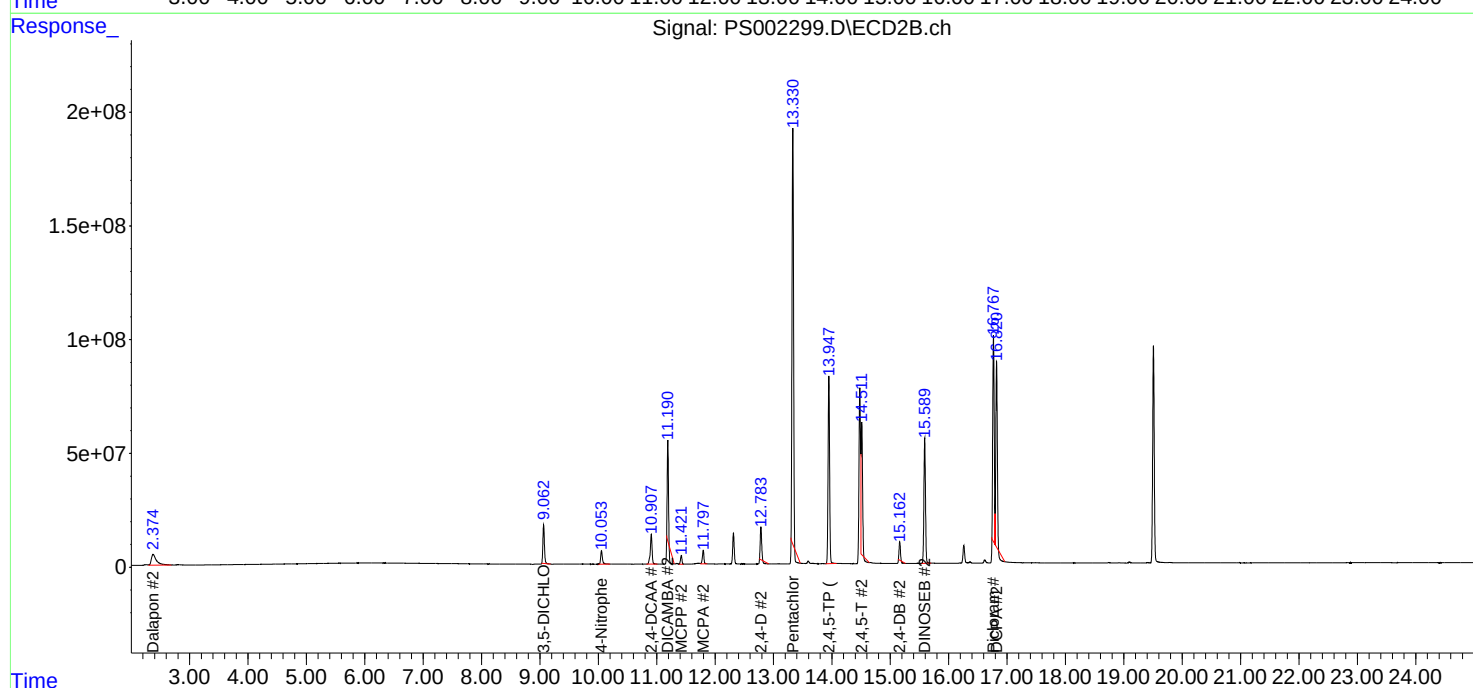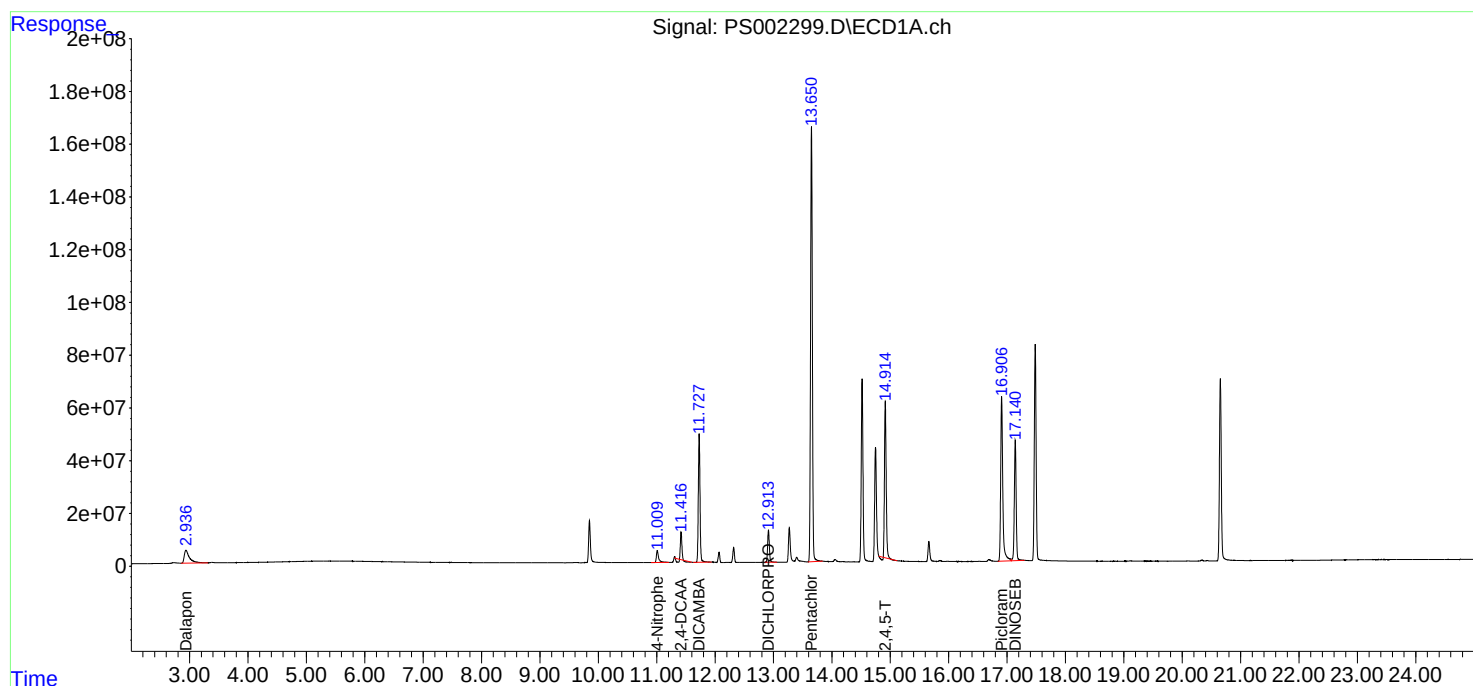


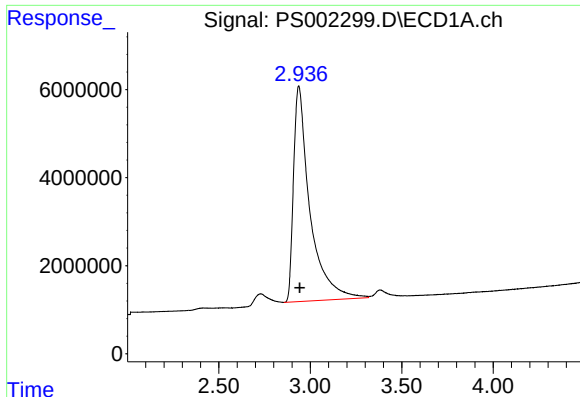

#1 Dalapon


R.T.: 2.936 min
Delta R.T.: -0.006 min
Response: 305332051
Conc: 665.69 ng/ml

Instrument :
ECD_S
ClientSampleId :

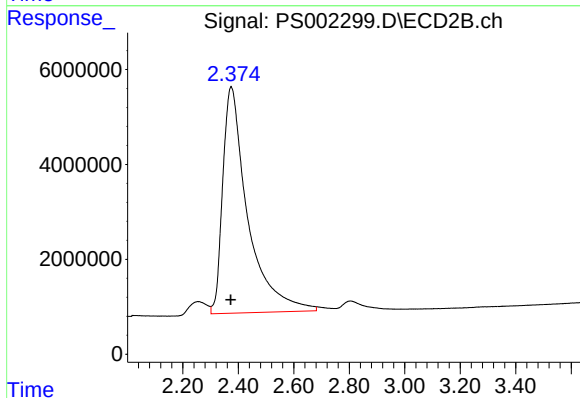


#1 Dalapon

R.T.: 2.374 min
Delta R.T.: 0.000 min
Response: 298802737
Conc: 661.79 ng/ml

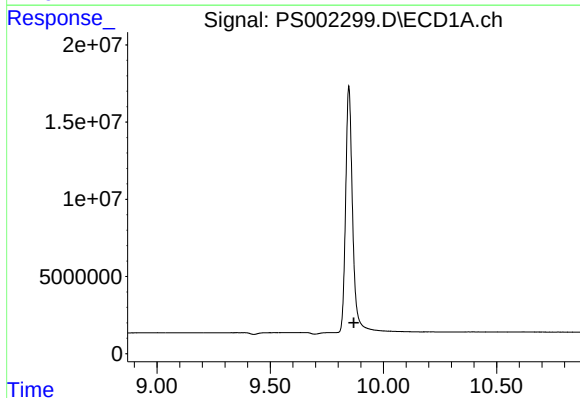


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.870 min
Response: 0
Conc: N.D.

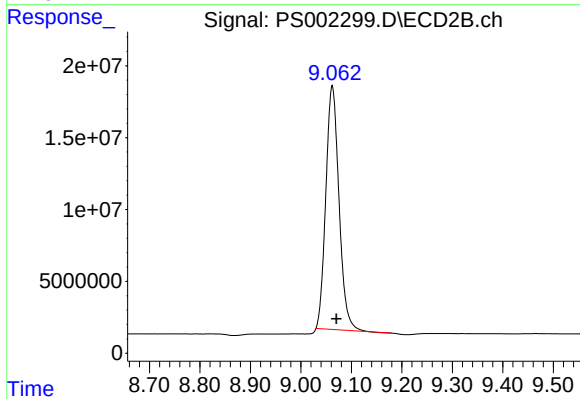

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.062 min
Delta R.T.: -0.008 min
Response: 307702679
Conc: 693.72 ng/ml

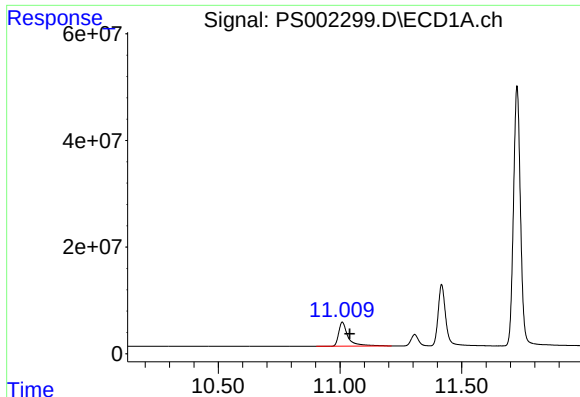

#3 4-Nitrophenol


R.T.: 11.010 min
Delta R.T.: -0.030 min
Response: 123365610
Conc: 739.47 ng/ml

Instrument :
ECD_S
ClientSampleId :

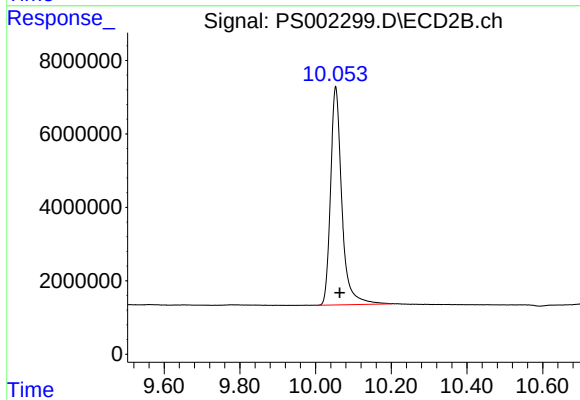


#3 4-Nitrophenol

R.T.: 10.053 min
Delta R.T.: -0.011 min
Response: 122936140
Conc: 689.45 ng/ml

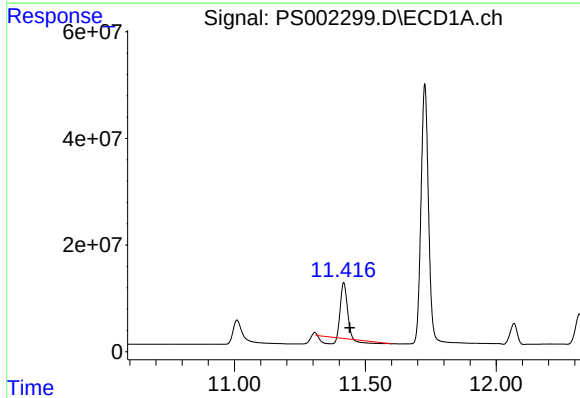


#4 2,4-DCAA

R.T.: 11.417 min
Delta R.T.: -0.024 min
Response: 129476097
Conc: 411.45 ng/ml

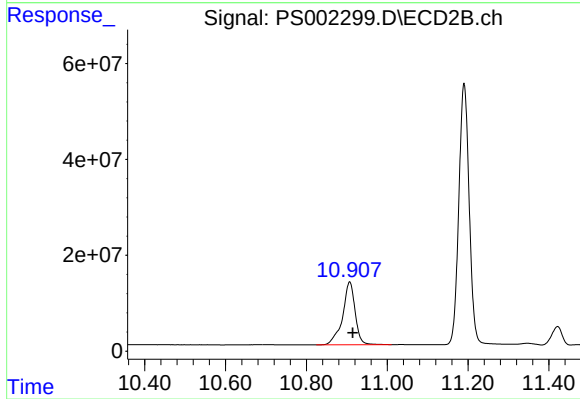

#4 2,4-DCAA


R.T.: 10.907 min
Delta R.T.: -0.007 min
Response: 282182546
Conc: 785.81 ng/ml

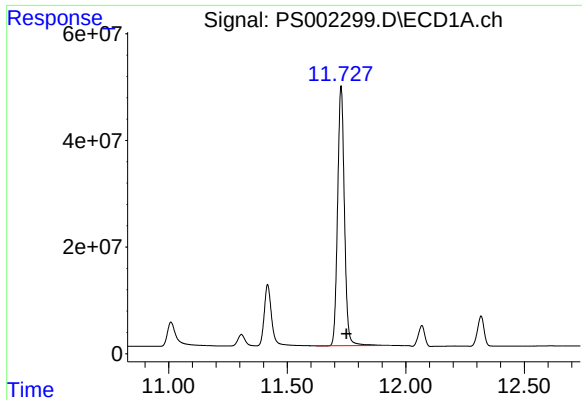

#5 DICAMBA


R.T.: 11.727 min
Delta R.T.: -0.023 min
Response: 976249895
Conc: 735.12 ng/ml

Instrument :
ECD_S
ClientSampleId :

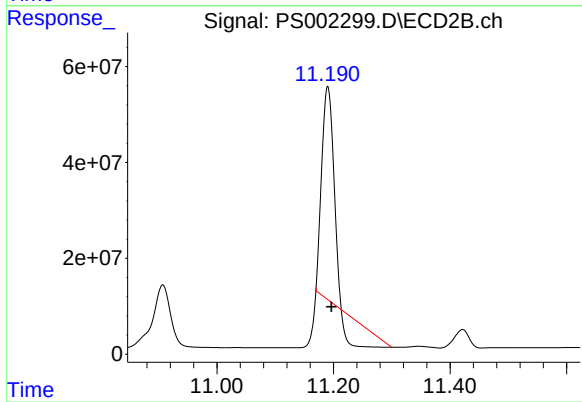


#5 DICAMBA

R.T.: 11.190 min
Delta R.T.: -0.007 min
Response: 464157258
Conc: 371.42 ng/ml

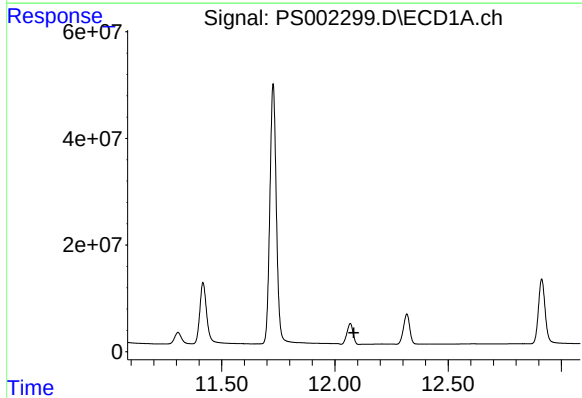


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 12.084 min
Response: 0
Conc: N.D.

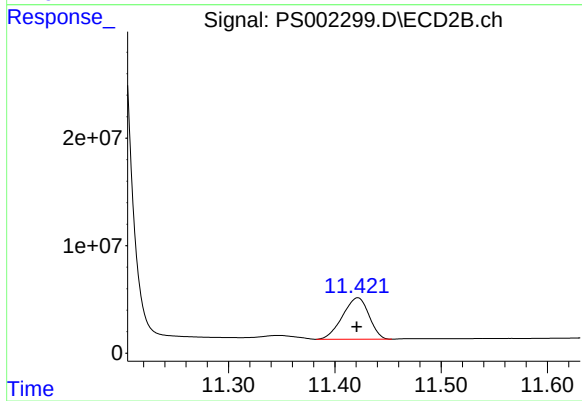

#6 MCPP


R.T.: 11.422 min
Delta R.T.: 0.001 min
Response: 66755117
Conc: 77.59 ug/ml

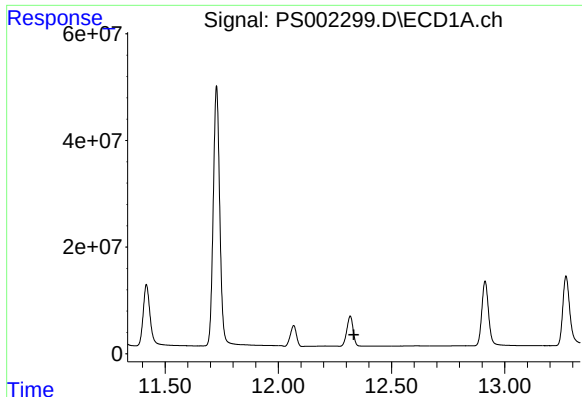

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 12.333 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

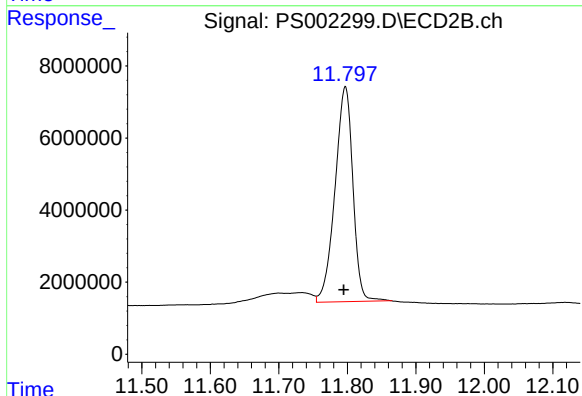


#7 MCPA

R.T.: 11.797 min
Delta R.T.: 0.002 min
Response: 108197002
Conc: 79.94 ug/ml

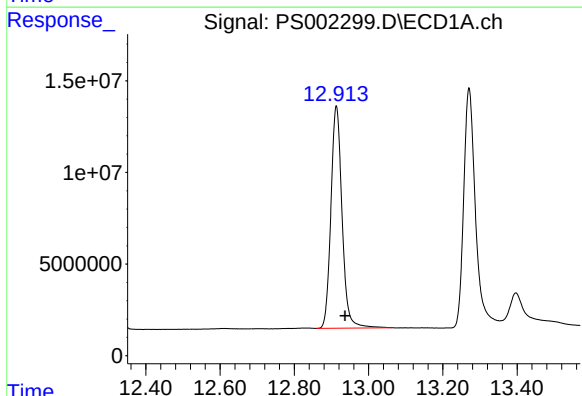


#8 DICHLORPROP

R.T.: 12.913 min
Delta R.T.: -0.024 min
Response: 252527456
Conc: 725.13 ng/ml

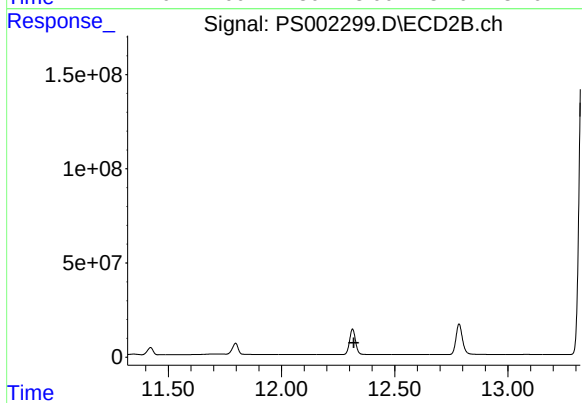

#8 DICHLORPROP


R.T.: 12.313 min
Delta R.T.: -0.006 min
Response: -58258923
Conc: N.D.

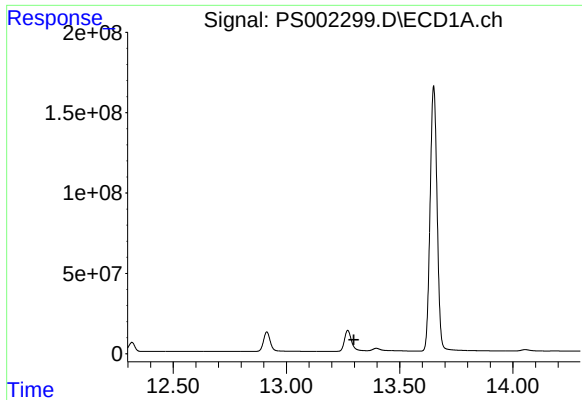

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 13.298 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

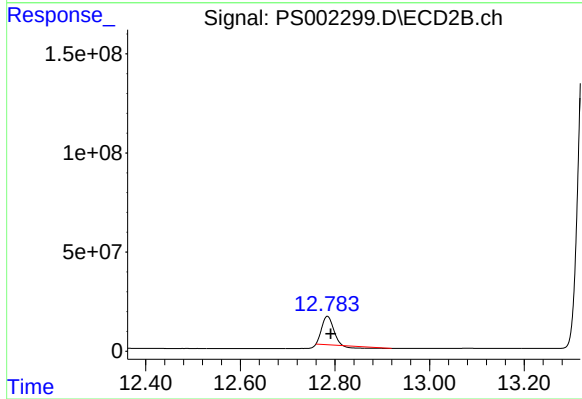


#9 2,4-D

R.T.: 12.784 min
Delta R.T.: -0.007 min
Response: 209424944
Conc: 491.73 ng/ml

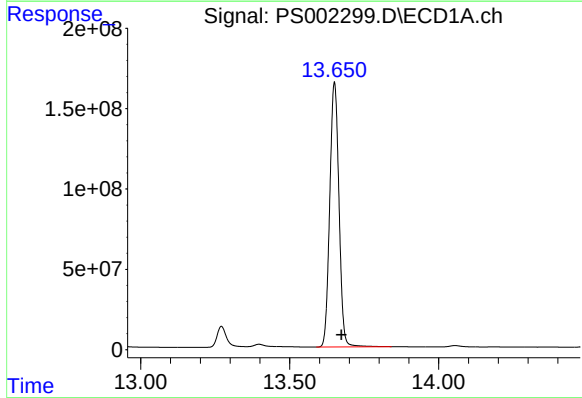


#10 Pentachlorophenol

R.T.: 13.650 min
Delta R.T.: -0.024 min
Response: 3539574918
Conc: 735.77 ng/ml

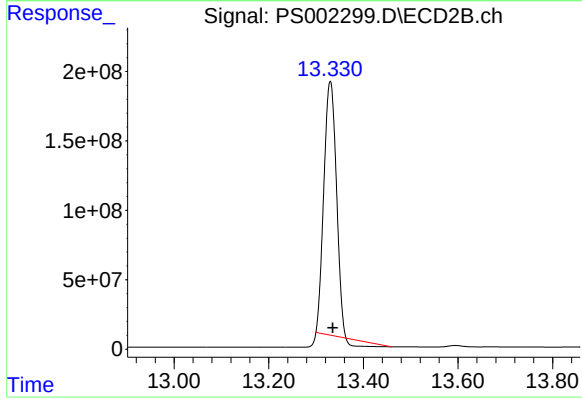

#10 Pentachlorophenol


R.T.: 13.330 min
Delta R.T.: -0.005 min
Response: 3217806727
Conc: 685.01 ng/ml

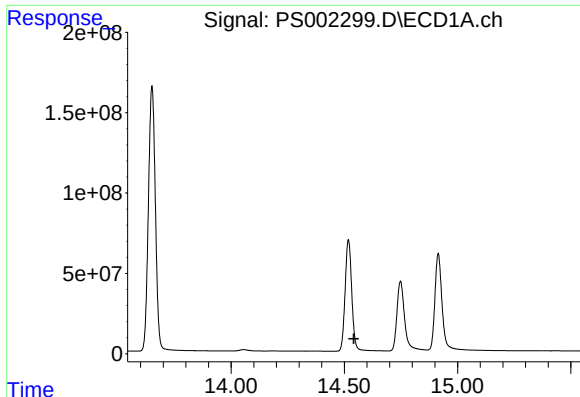

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 14.542 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

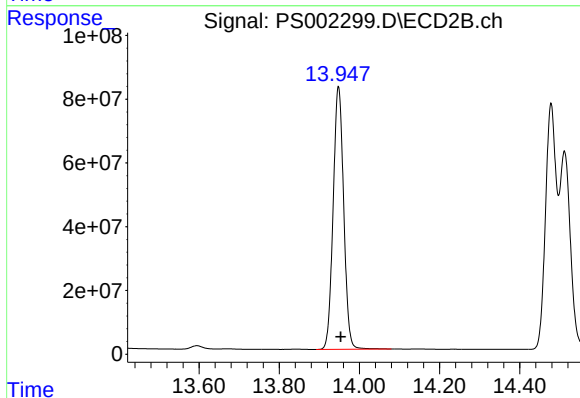


#11 2,4,5-TP (SILVEX)

R.T.: 13.948 min
Delta R.T.: -0.006 min
Response: 1503014582
Conc: 821.51 ng/ml

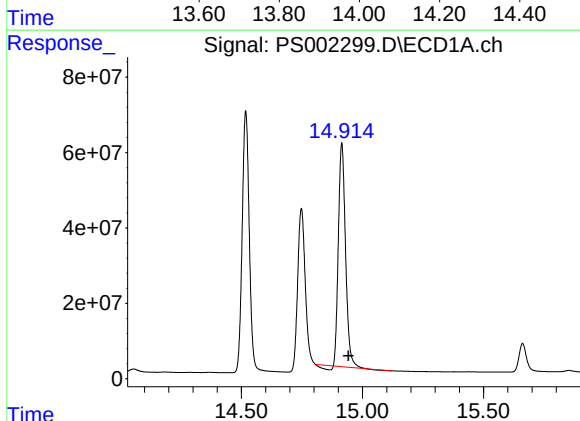


#12 2,4,5-T

R.T.: 14.915 min
Delta R.T.: -0.027 min
Response: 1195067648
Conc: 666.79 ng/ml

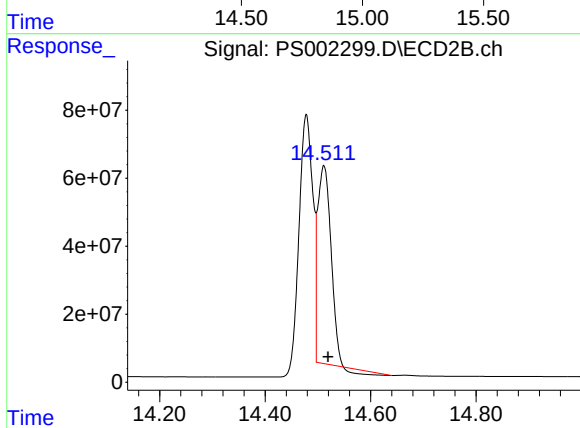

#12 2,4,5-T


R.T.: 14.511 min
Delta R.T.: -0.008 min
Response: 982260106
Conc: 655.94 ng/ml

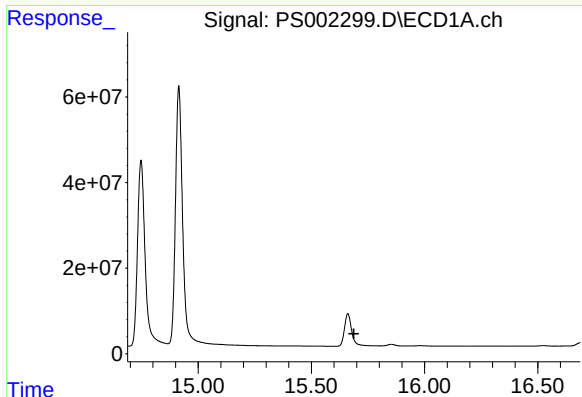

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 15.688 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

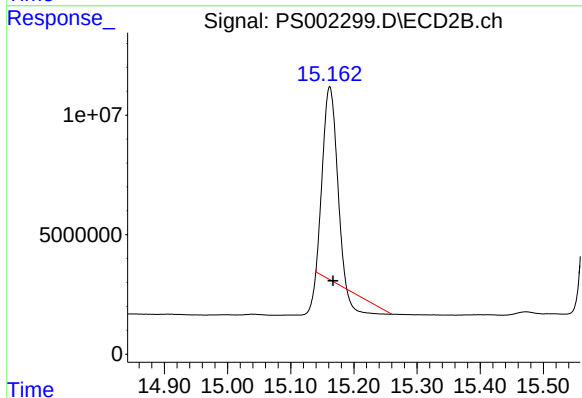


#13 2,4-DB

R.T.: 15.162 min
Delta R.T.: -0.005 min
Response: 108269815
Conc: 488.67 ng/ml

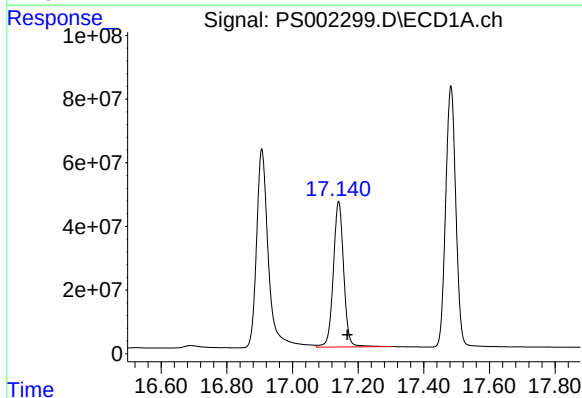


#14 DINOSEB

R.T.: 17.140 min
Delta R.T.: -0.027 min
Response: 1002545798
Conc: 731.76 ng/ml

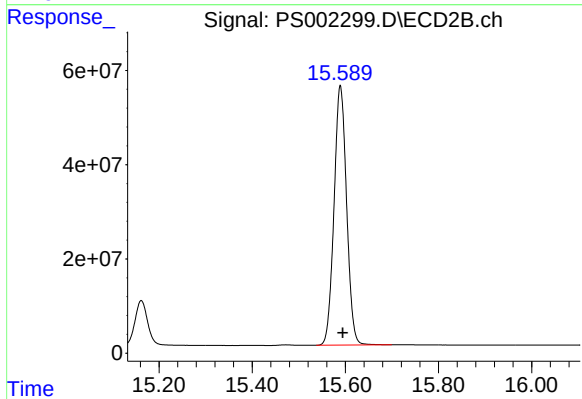

#14 DINOSEB


R.T.: 15.589 min
Delta R.T.: -0.005 min
Response: 1030705620
Conc: 814.23 ng/ml

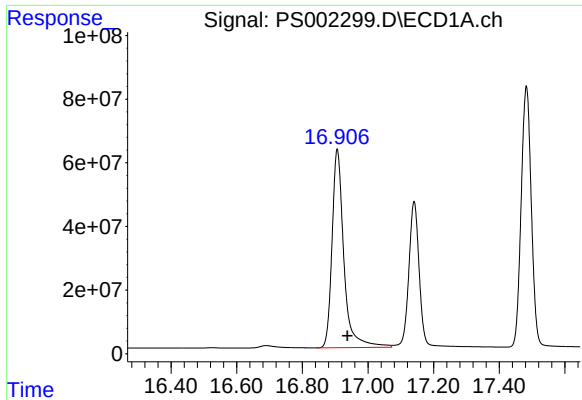

#15 Picloram


R.T.: 16.907 min
Delta R.T.: -0.031 min
Response: 1560416226
Conc: 654.18 ng/ml

Instrument :
ECD_S
ClientSampleId :

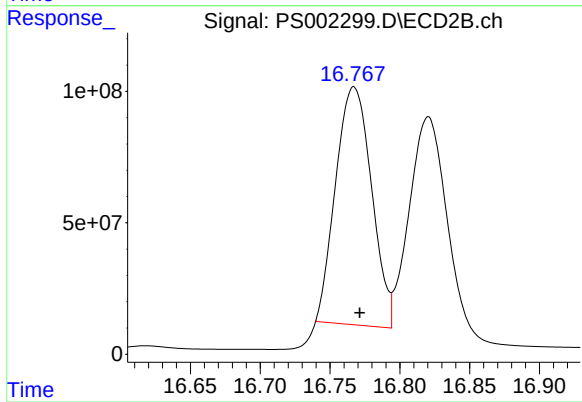


#15 Picloram

R.T.: 16.767 min
Delta R.T.: -0.004 min
Response: 1620346686
Conc: 716.26 ng/ml

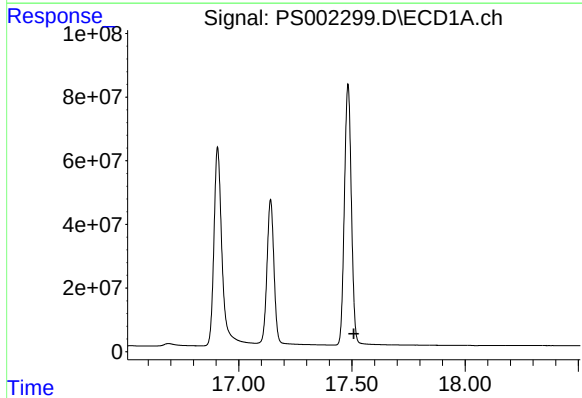

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.509 min
Response: 0
Conc: N.D.

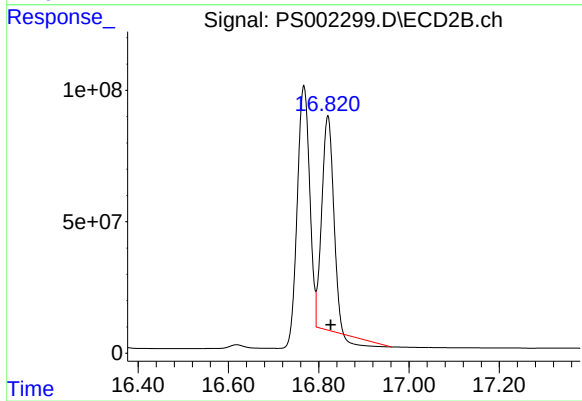

#16 DCPA

R.T.: 16.820 min
Delta R.T.: -0.006 min
Response: 1382362615
Conc: 583.80 ng/ml