

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110222\
 Data File : PS021006.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Nov 2022 17:32
 Operator : AR\AJ
 Sample : PB148745BS
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB148745BS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 02 22:24:24 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102822.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 31 10:07:57 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.409	6.847	1149.6E6	749.6E6	550.827	541.932
Target Compounds							
1) T	Dalapon	2.509	2.580	1281.0E6	879.7E6	484.037	483.665
2) T	3,5-DICHL...	5.777	6.018	1525.1E6	1064.2E6	498.024	521.431
3) T	4-Nitroph...	6.246	6.456	727.3E6	428.7E6	483.554	498.557
5) T	DICAMBA	6.554	7.014	4504.8E6	3172.4E6	509.896	510.852
6) T	MCPD	6.711	7.112	315.8E6	228.7E6	48.394	48.148
7) T	MCPA	6.837	7.324	444.8E6	336.0E6	47.406	49.527
8) T	DICHLORPROP	7.154	7.640	1134.5E6	783.6E6	497.002	508.899
9) T	2,4-D	7.354	7.930	1397.8E6	960.6E6	500.151	512.915
10) T	Pentachlo...	7.588	8.363	16595.1E6	11338.2E6	526.676	534.521
11) T	2,4,5-TP ...	8.115	8.724	7104.4E6	4697.0E6	534.782	523.405
12) T	2,4,5-T	8.373	9.100	7009.0E6	4523.3E6	526.730	524.618
13) T	2,4-DB	8.882	9.609	1295.0E6	630.5E6	469.395	566.512
14) T	DINOSEB	9.943	9.939	5458.9E6	3264.4E6	502.780	509.962
15) T	Picloram	9.774	10.911	10418.0E6	6534.5E6	493.210	515.035
16) T	DCPA	10.209	10.870	9260.7E6	5994.4E6	511.716	561.385



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110222\
Data File : PS021006.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Nov 2022 17:32
Operator : AR\AJ
Sample : PB148745BS
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
PB148745BS

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 02 22:24:24 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102822.M
Quant Title : 8080.M
QLast Update : Mon Oct 31 10:07:57 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

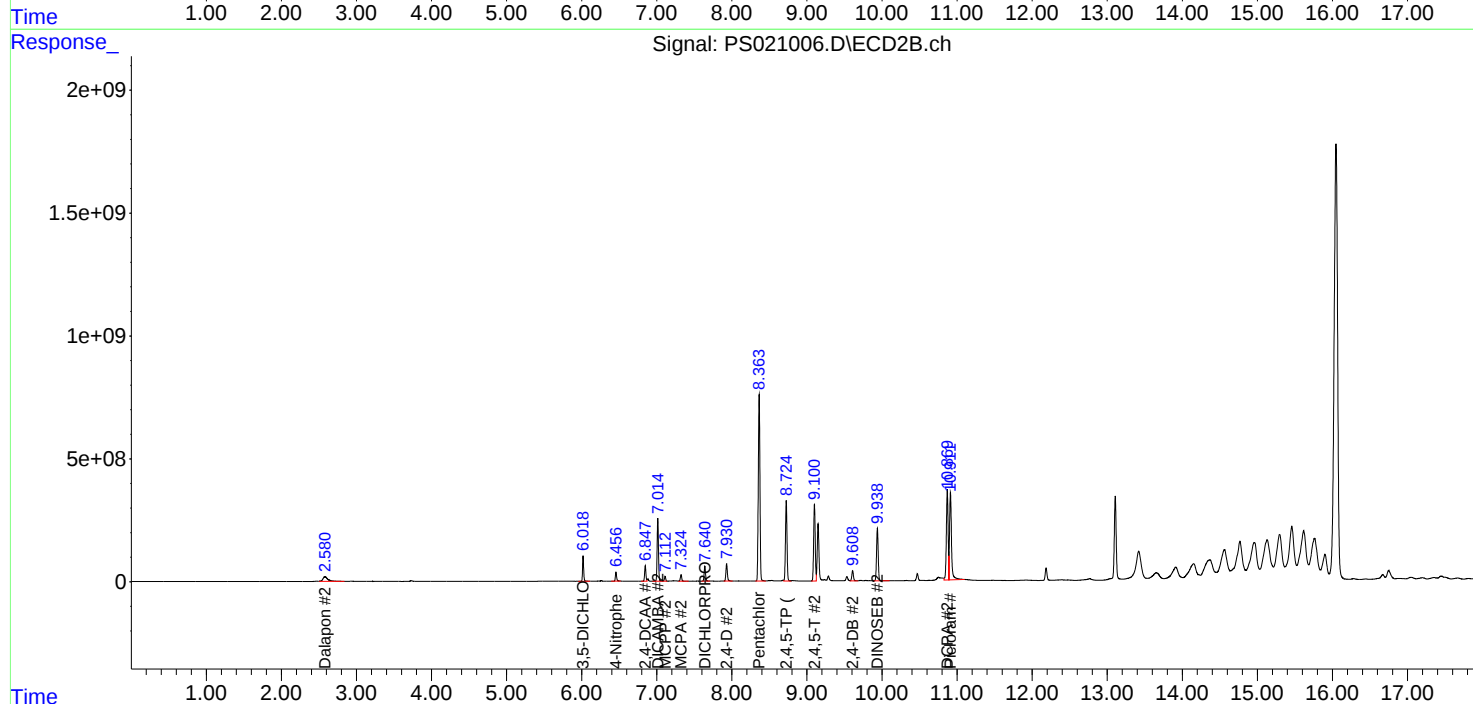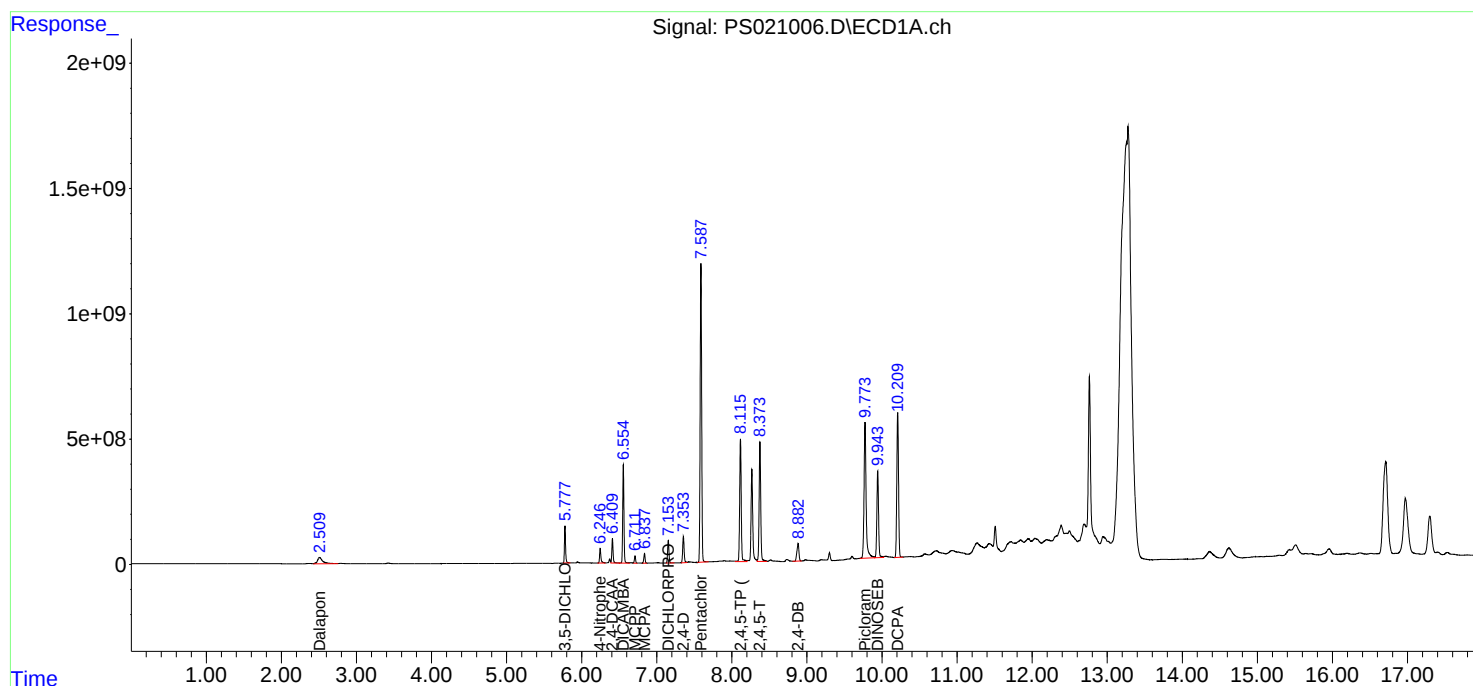


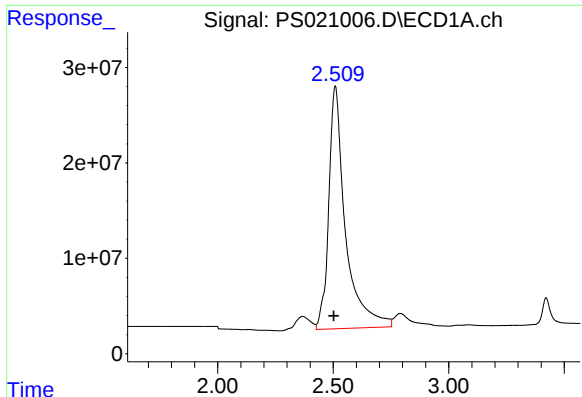

#1 Dalapon


R.T.: 2.509 min
Delta R.T.: 0.006 min
Response: 1281016474
Conc: 484.04 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB148745BS

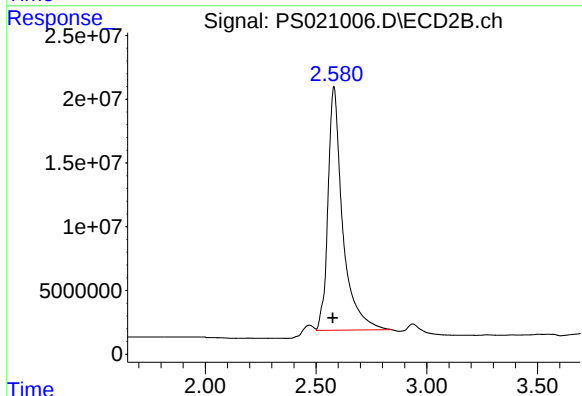


#1 Dalapon

R.T.: 2.580 min
Delta R.T.: 0.005 min
Response: 879667464
Conc: 483.66 ng/ml

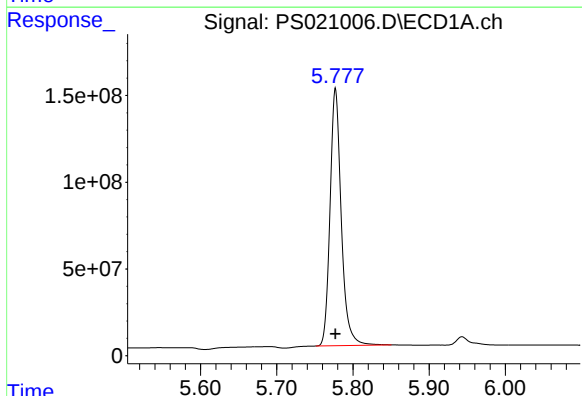


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 5.777 min
Delta R.T.: 0.000 min
Response: 1525089058
Conc: 498.02 ng/ml

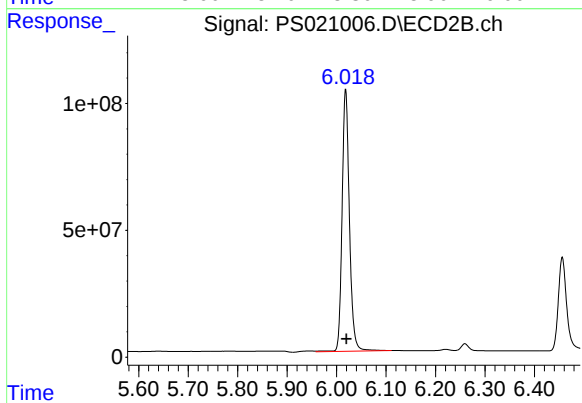

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.018 min
Delta R.T.: -0.002 min
Response: 1064193772
Conc: 521.43 ng/ml

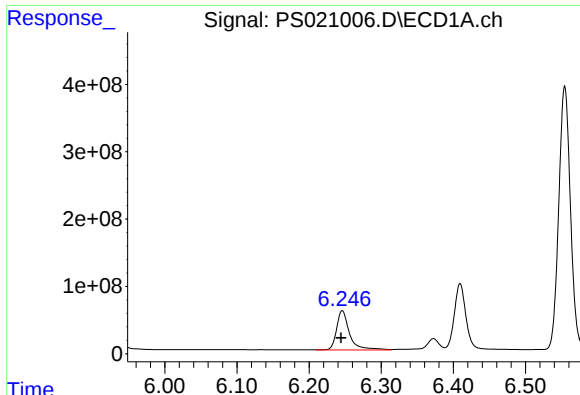

#3 4-Nitrophenol


R.T.: 6.246 min
Delta R.T.: 0.002 min
Response: 727296135
Conc: 483.55 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB148745BS

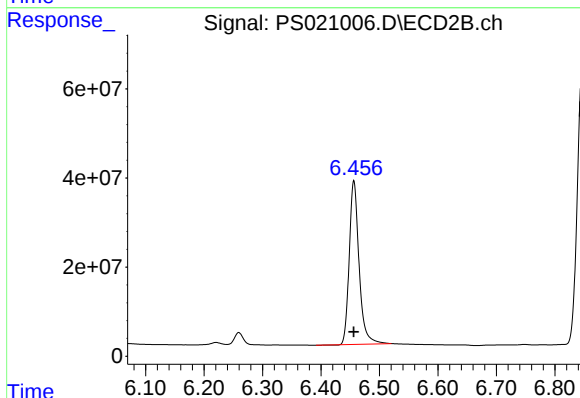


#3 4-Nitrophenol

R.T.: 6.456 min
Delta R.T.: 0.000 min
Response: 428650030
Conc: 498.56 ng/ml

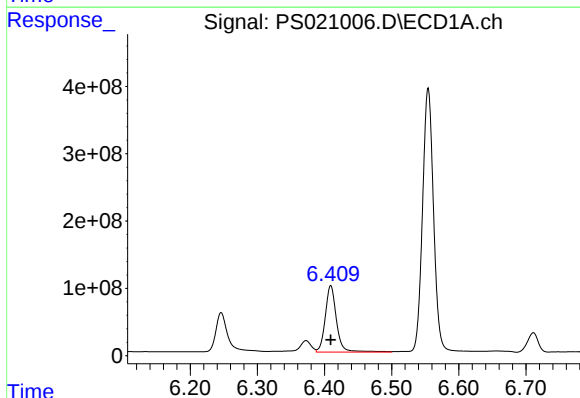


#4 2,4-DCAA

R.T.: 6.409 min
Delta R.T.: 0.000 min
Response: 1149618440
Conc: 550.83 ng/ml

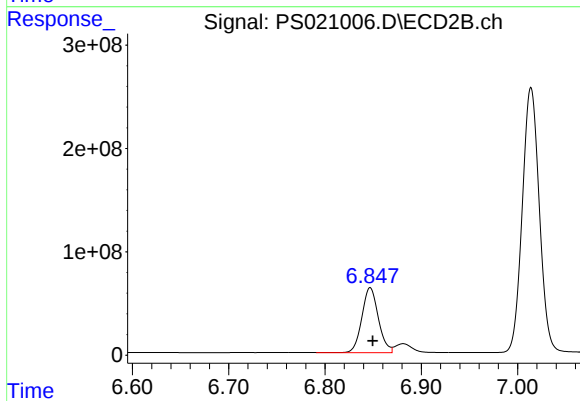

#4 2,4-DCAA


R.T.: 6.847 min
Delta R.T.: -0.003 min
Response: 749571101
Conc: 541.93 ng/ml

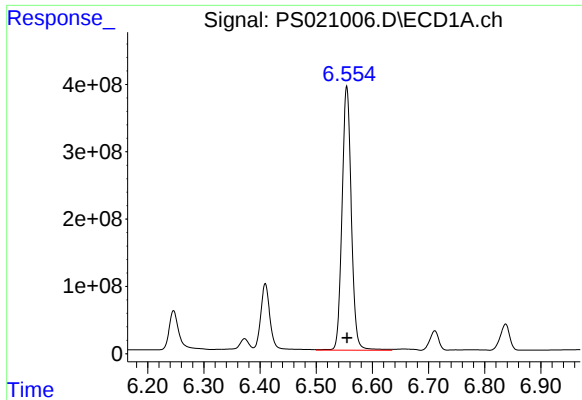

#5 DICAMBA


R.T.: 6.554 min
Delta R.T.: 0.000 min
Response: 4504775970
Conc: 509.90 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB148745BS

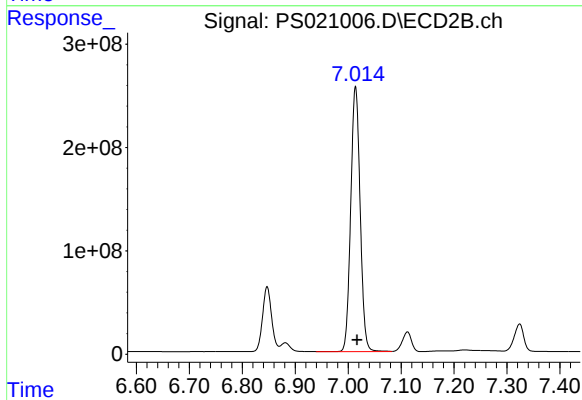


#5 DICAMBA

R.T.: 7.014 min
Delta R.T.: -0.003 min
Response: 3172443664
Conc: 510.85 ng/ml

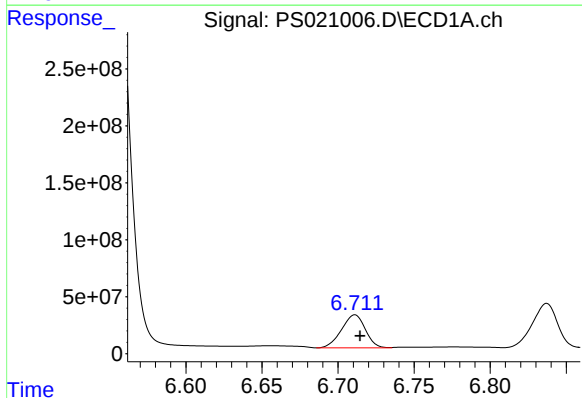


#6 MCP

R.T.: 6.711 min
Delta R.T.: -0.003 min
Response: 315845725
Conc: 48.39 ug/ml

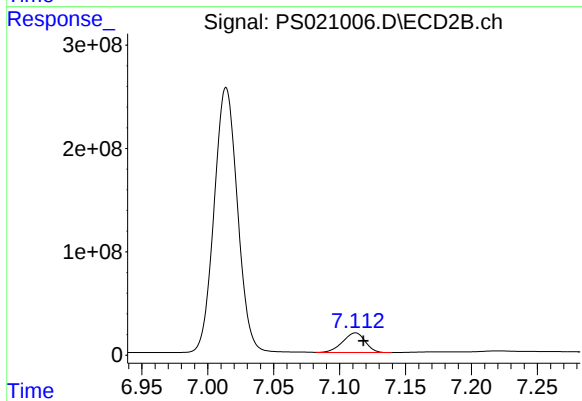

#6 MCP


R.T.: 7.112 min
Delta R.T.: -0.006 min
Response: 228744188
Conc: 48.15 ug/ml

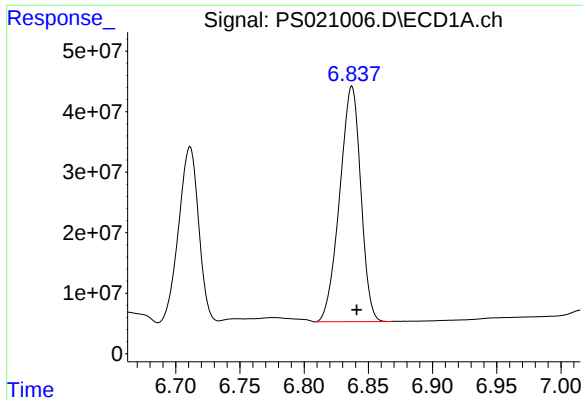

#7 MCPA


R.T.: 6.837 min
Delta R.T.: -0.004 min
Response: 444806441
Conc: 47.41 ug/ml

Instrument :
ECD_S
ClientSampleId :
PB148745BS

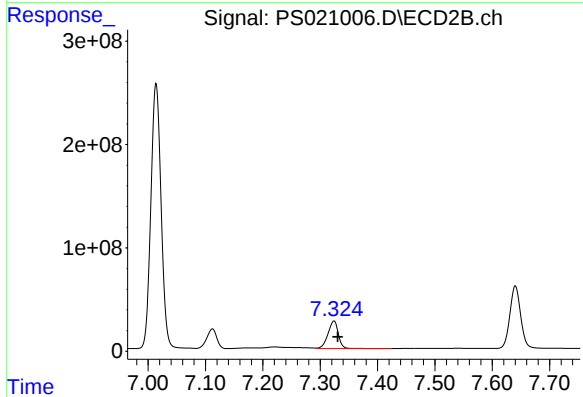


#7 MCPA

R.T.: 7.324 min
Delta R.T.: -0.007 min
Response: 336049961
Conc: 49.53 ug/ml

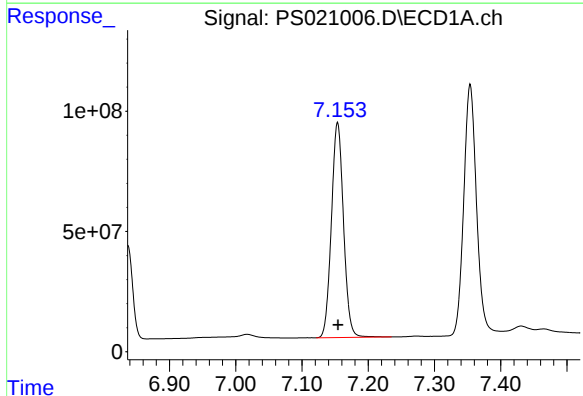


#8 DICHLORPROP

R.T.: 7.154 min
Delta R.T.: 0.000 min
Response: 1134472398
Conc: 497.00 ng/ml

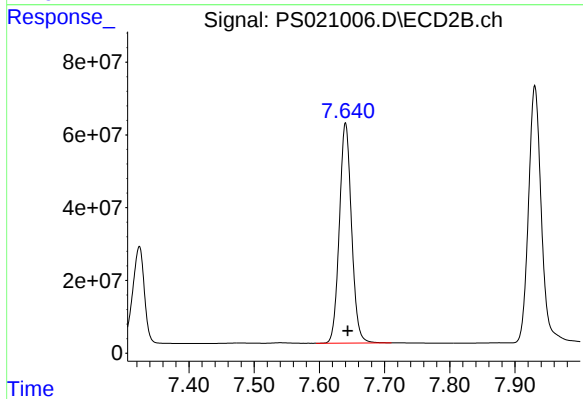

#8 DICHLORPROP


R.T.: 7.640 min
Delta R.T.: -0.003 min
Response: 783610593
Conc: 508.90 ng/ml

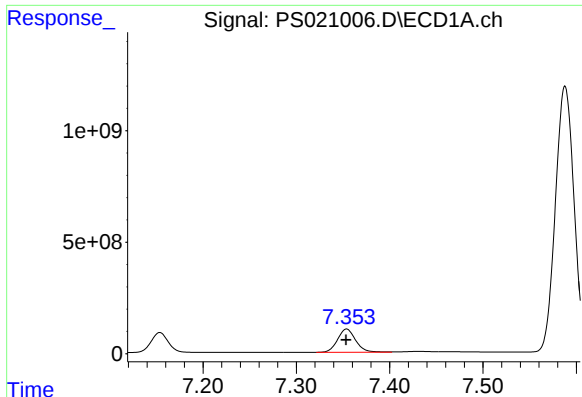

#9 2,4-D


R.T.: 7.354 min
Delta R.T.: 0.000 min
Response: 1397796792
Conc: 500.15 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB148745BS

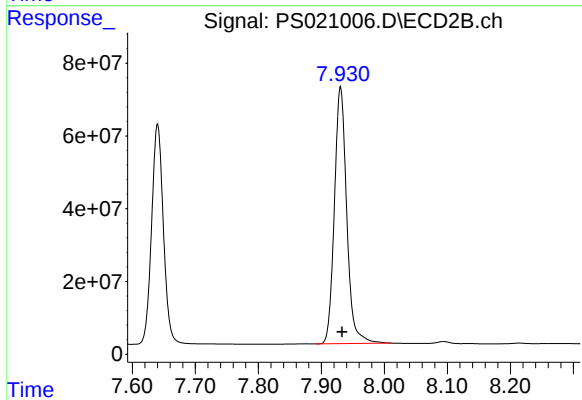


#9 2,4-D

R.T.: 7.930 min
Delta R.T.: -0.003 min
Response: 960615720
Conc: 512.92 ng/ml

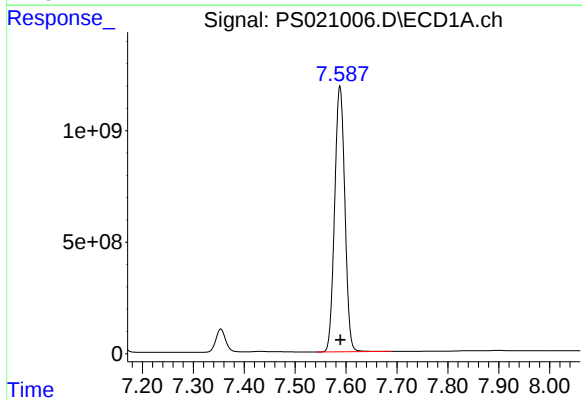


#10 Pentachlorophenol

R.T.: 7.588 min
Delta R.T.: -0.001 min
Response: 16595086592
Conc: 526.68 ng/ml

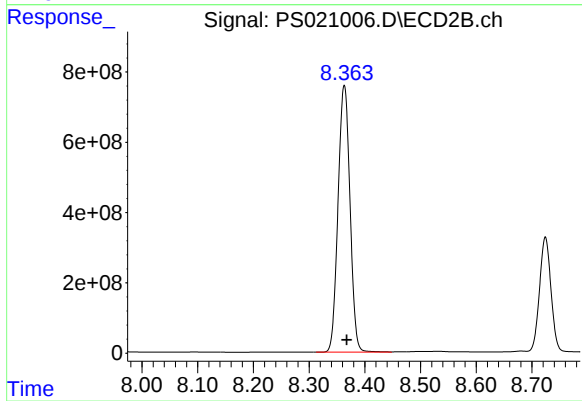

#10 Pentachlorophenol


R.T.: 8.363 min
Delta R.T.: -0.005 min
Response: 11338194737
Conc: 534.52 ng/ml

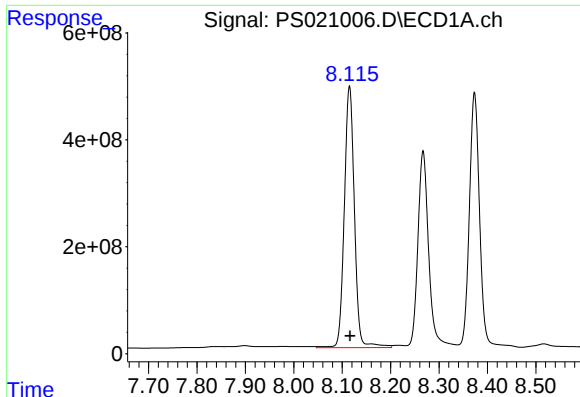

#11 2,4,5-TP (SILVEX)


R.T.: 8.115 min
Delta R.T.: -0.001 min
Response: 7104423407
Conc: 534.78 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB148745BS

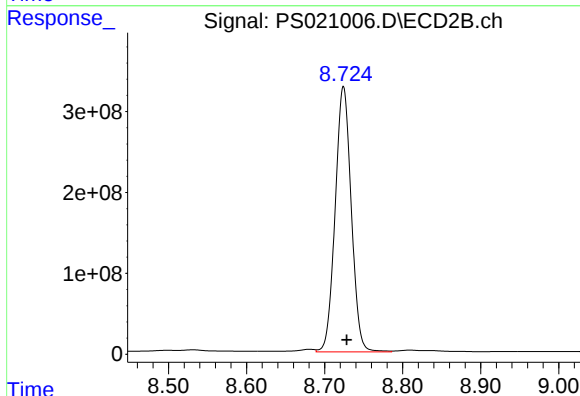


#11 2,4,5-TP (SILVEX)

R.T.: 8.724 min
Delta R.T.: -0.004 min
Response: 4696960655
Conc: 523.41 ng/ml

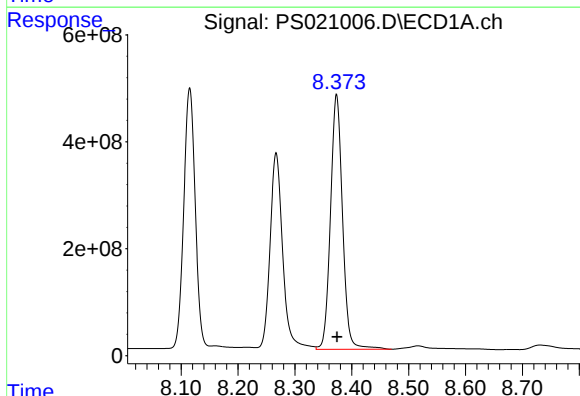


#12 2,4,5-T

R.T.: 8.373 min
Delta R.T.: 0.000 min
Response: 7008967323
Conc: 526.73 ng/ml

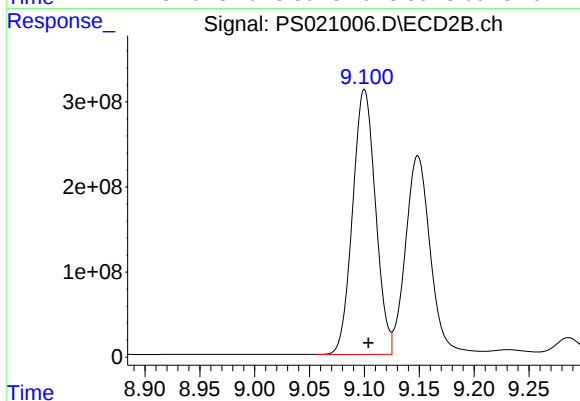

#12 2,4,5-T


R.T.: 9.100 min
Delta R.T.: -0.004 min
Response: 4523290655
Conc: 524.62 ng/ml

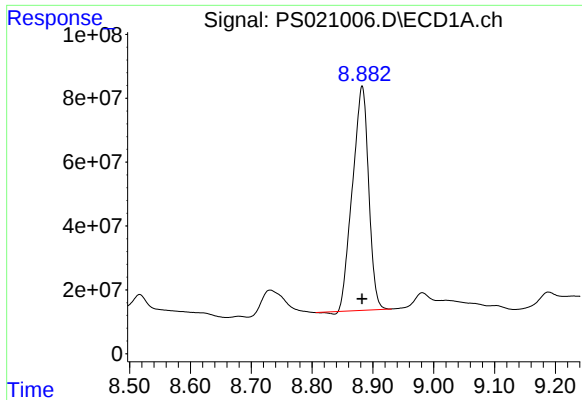

#13 2,4-DB


R.T.: 8.882 min
Delta R.T.: 0.000 min
Response: 1295049266
Conc: 469.40 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB148745BS

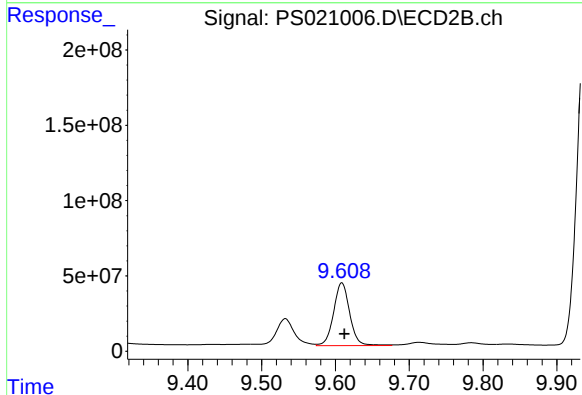


#13 2,4-DB

R.T.: 9.609 min
Delta R.T.: -0.003 min
Response: 630542756
Conc: 566.51 ng/ml

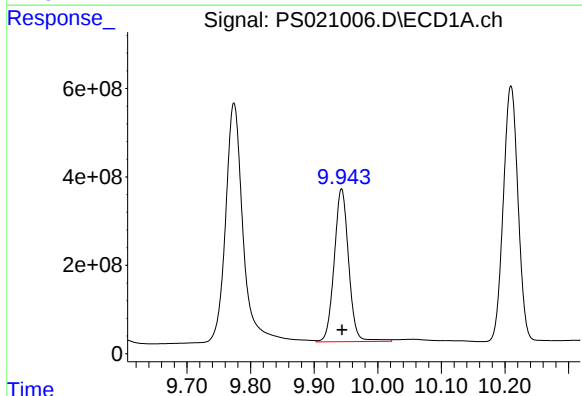


#14 DINOSEB

R.T.: 9.943 min
Delta R.T.: 0.000 min
Response: 5458890263
Conc: 502.78 ng/ml

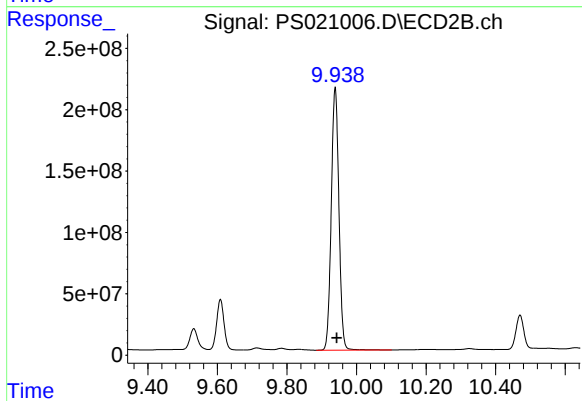

#14 DINOSEB


R.T.: 9.939 min
Delta R.T.: -0.004 min
Response: 3264439246
Conc: 509.96 ng/ml

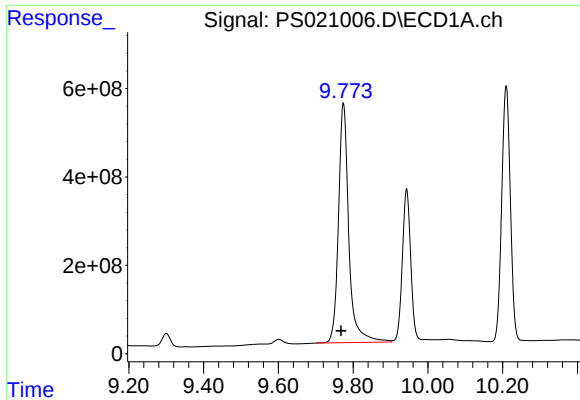

#15 Picloram


R.T.: 9.774 min
Delta R.T.: 0.005 min
Response: 10417978218
Conc: 493.21 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB148745BS

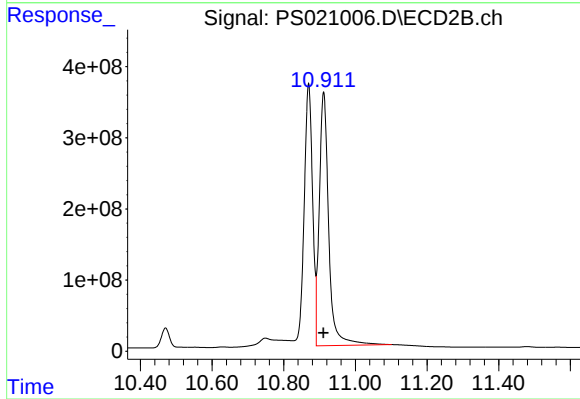


#15 Picloram

R.T.: 10.911 min
Delta R.T.: 0.000 min
Response: 6534491356
Conc: 515.03 ng/ml

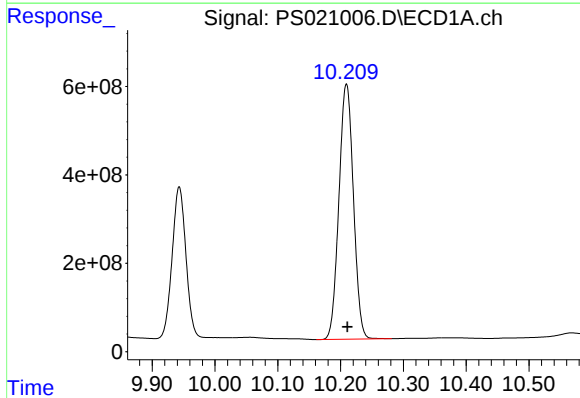

#16 DCPA

R.T.: 10.209 min
Delta R.T.: -0.002 min
Response: 9260687294
Conc: 511.72 ng/ml

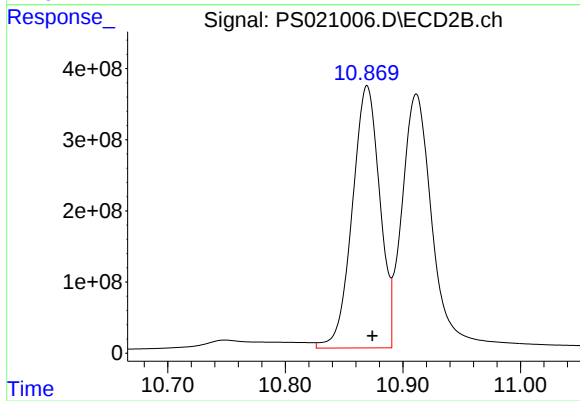

#16 DCPA

R.T.: 10.870 min
Delta R.T.: -0.005 min
Response: 5994404947
Conc: 561.39 ng/ml