

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110223\
 Data File : PS024734.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Nov 2023 12:19
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 02 23:10:24 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100323.M
 Quant Title : 8080.M
 QLast Update : Tue Oct 03 14:54:54 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
1) T	Dalapon	0.000	2.565	0	2095689	1.873
5) T	DICAMBA	0.000	6.977	0	5862851	1.980
6) T	MCP	6.678	6.977f	7064347	5862851	2.975 #
8) T	DICHLORPROP	0.000	7.559	0	3421387	4.549
9) T	2,4-D	7.249	7.778f	77809612	898231	<MDL #
10) T	Pentachlo...	0.000	8.256	0	590964	<MDL
11) T	2,4,5-TP ...	0.000	8.613	0	791759	<MDL
12) T	2,4,5-T	0.000	8.986	0	818600	<MDL
14) T	DINOSEB	0.000	9.866	0	143676	<MDL
15) T	Picloram	9.657	10.770	169.6E6	31060165	4.998 #
16) T	DCPA	0.000	10.770	0	31060165	5.953



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110223\
Data File : PS024734.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Nov 2023 12:19
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 02 23:10:24 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100323.M
Quant Title : 8080.M
QLast Update : Tue Oct 03 14:54:54 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

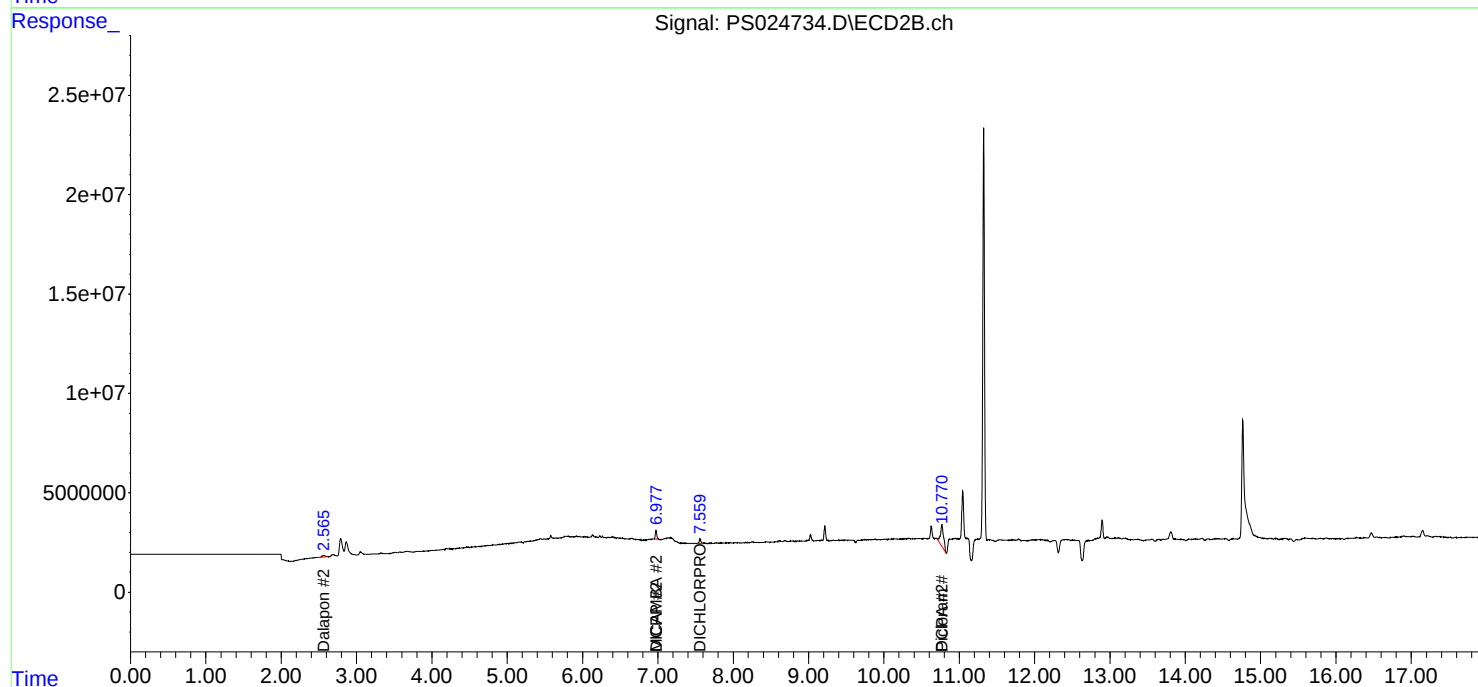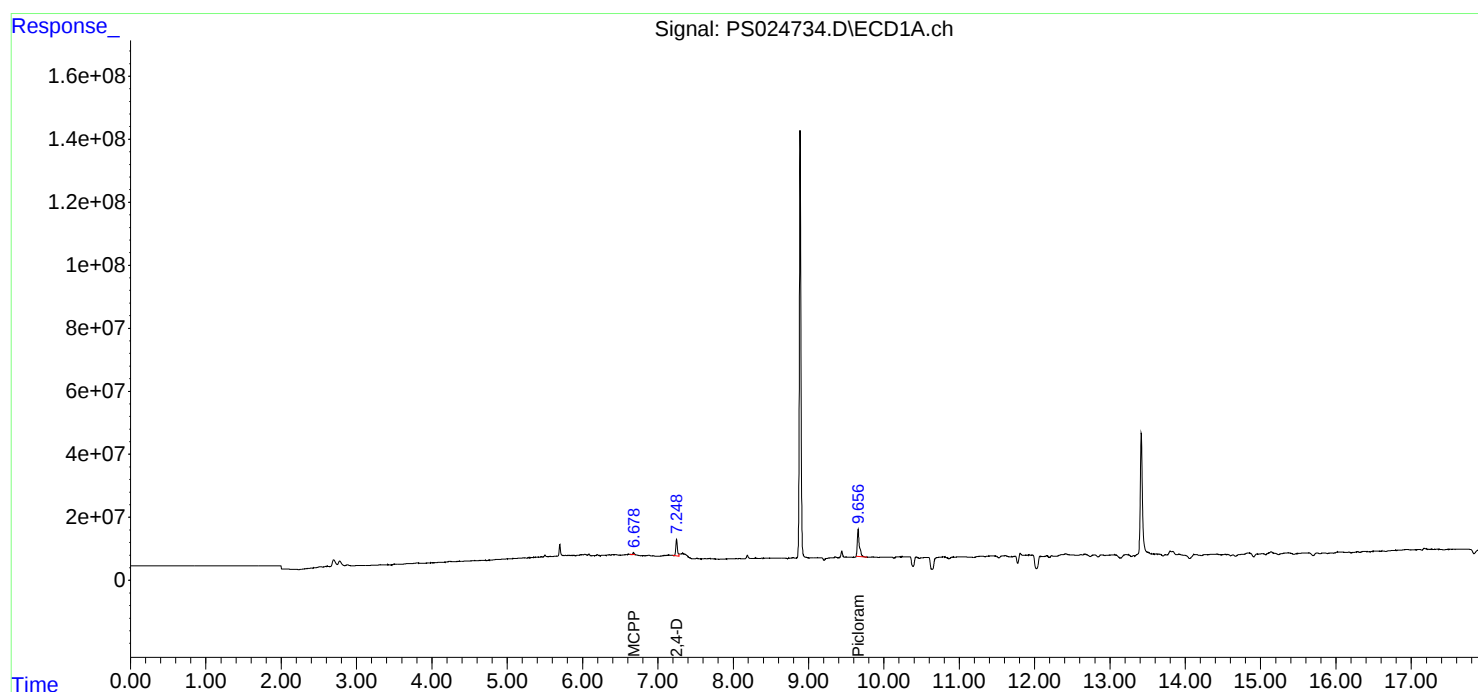


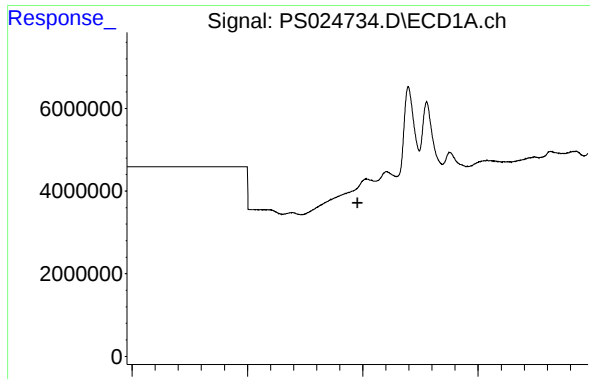

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.477 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

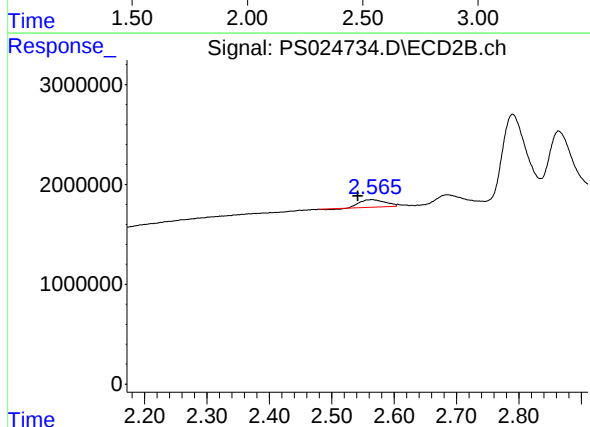


#1 Dalapon

R.T.: 2.565 min
Delta R.T.: 0.023 min
Response: 2095689
Conc: 1.87 ng/ml

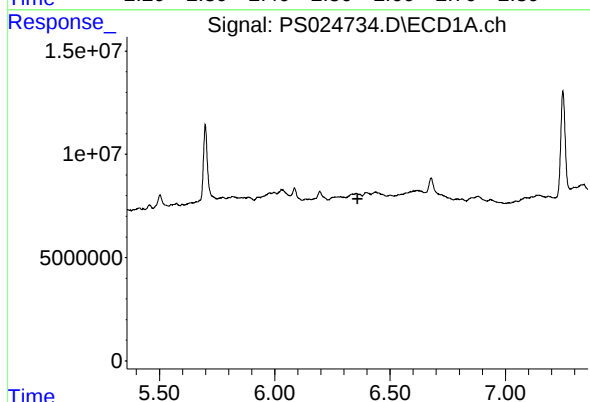


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 6.359 min
Response: 0
Conc: N.D.

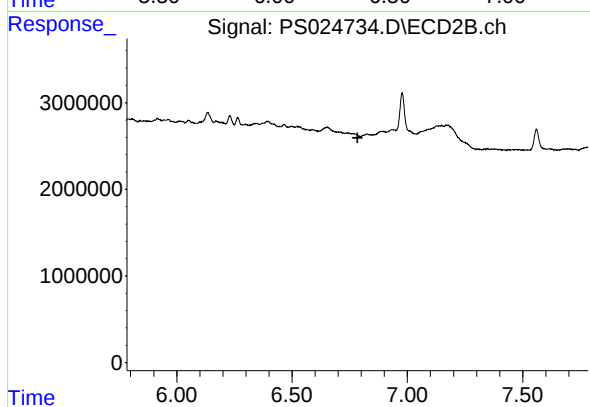

#4 2,4-DCAA


R.T.: 6.826 min
Delta R.T.: 0.043 min
Response: -52622
Conc: N.D.

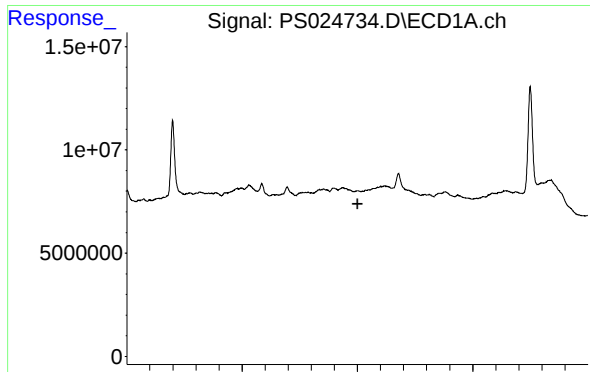

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 6.501 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

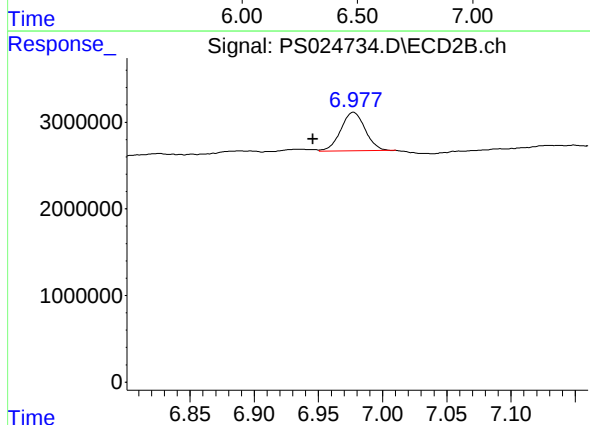


#5 DICAMBA

R.T.: 6.977 min
Delta R.T.: 0.032 min
Response: 5862851
Conc: 1.98 ng/ml

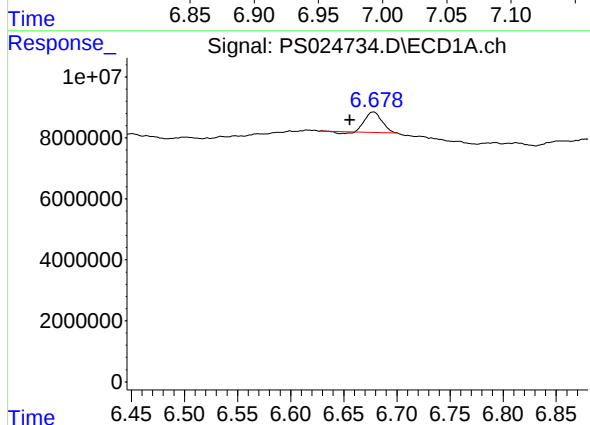


#6 MCPP

R.T.: 6.678 min
Delta R.T.: 0.022 min
Response: 7064347
Conc: 1.12 ug/ml

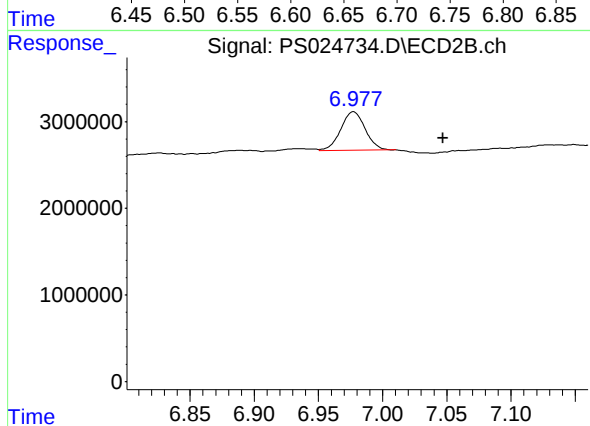

#6 MCPP


R.T.: 6.977 min
Delta R.T.: -0.070 min
Response: 5862851
Conc: 2.98 ug/ml

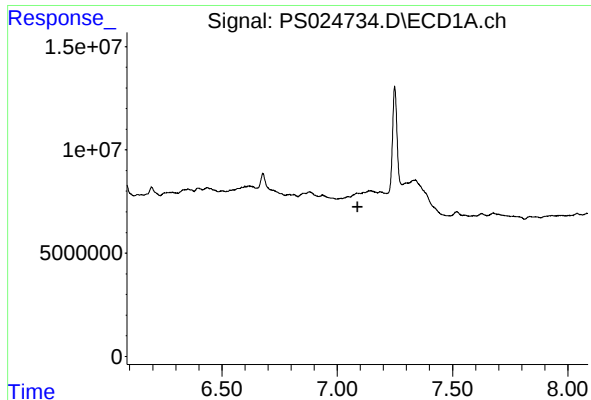

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 7.088 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

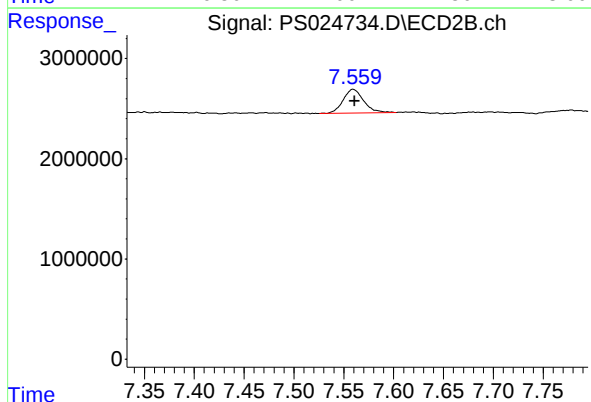


#8 DICHLORPROP

R.T.: 7.559 min
Delta R.T.: -0.002 min
Response: 3421387
Conc: 4.55 ng/ml

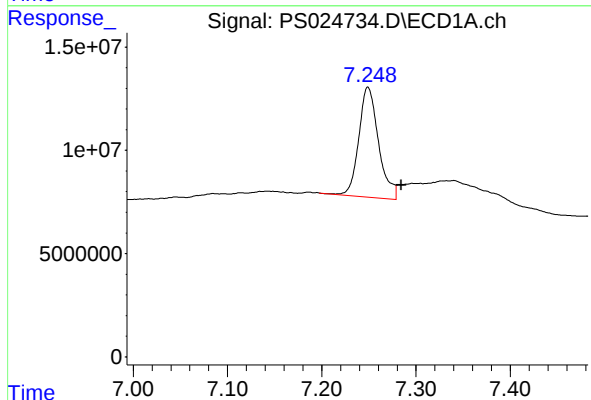


#9 2,4-D

R.T.: 7.249 min
Delta R.T.: -0.035 min
Response: 77809612
Conc: 28.16 ng/ml

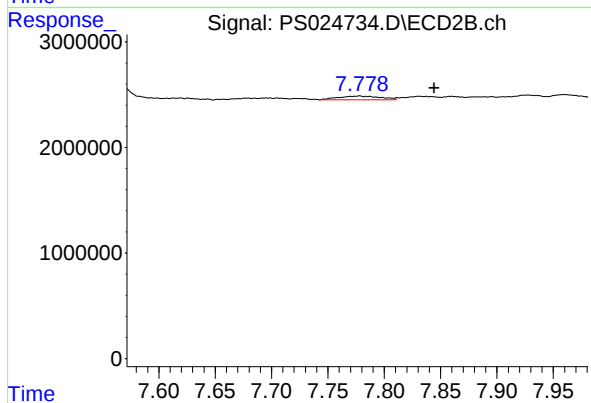

#9 2,4-D


R.T.: 7.778 min
Delta R.T.: -0.066 min
Response: 898231
Conc: N.D.

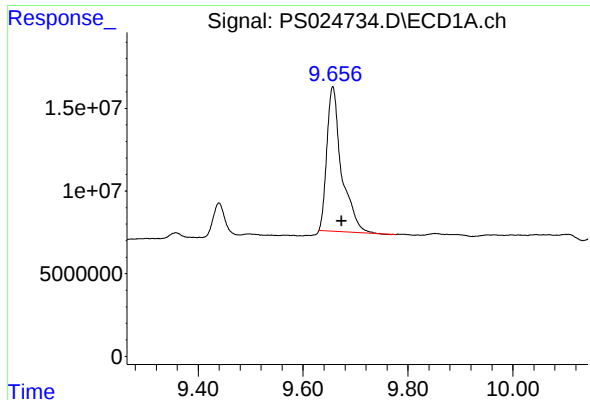

#15 Picloram


R.T.: 9.657 min
Delta R.T.: -0.016 min
Response: 169628195
Conc: 9.73 ng/ml

Instrument :
ECD_S
ClientSampleId :

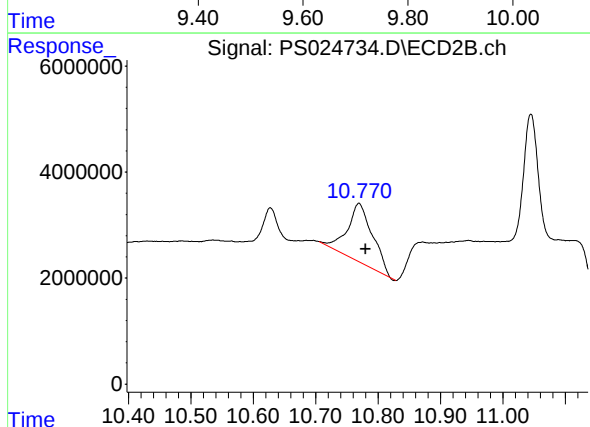


#15 Picloram

R.T.: 10.770 min
Delta R.T.: -0.011 min
Response: 31060165
Conc: 5.00 ng/ml

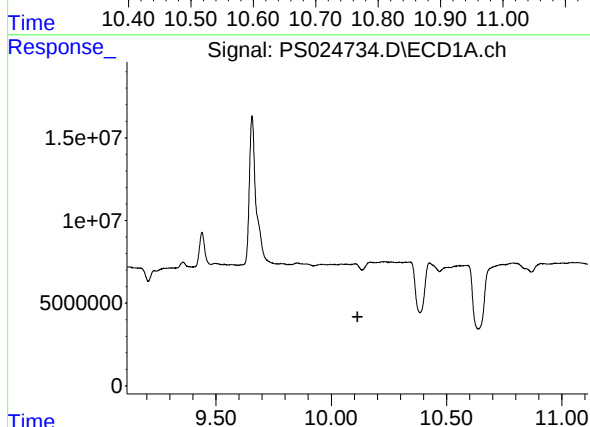

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 10.114 min
Response: 0
Conc: N.D.

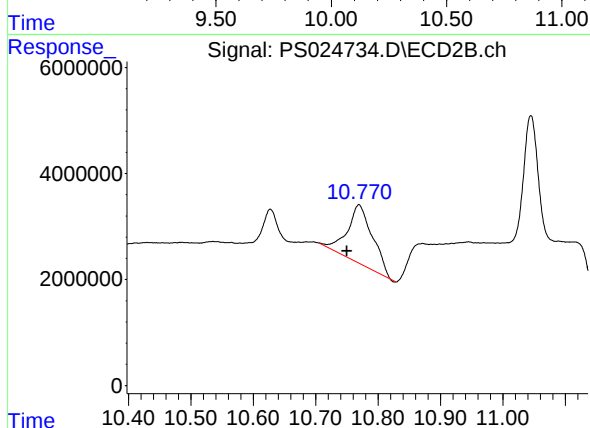

#16 DCPA

R.T.: 10.770 min
Delta R.T.: 0.019 min
Response: 31060165
Conc: 5.95 ng/ml