

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110223\
 Data File : PS024735.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Nov 2023 12:43
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 02 23:10:34 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100323.M
 Quant Title : 8080.M
 QLast Update : Tue Oct 03 14:54:54 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	6.358	6.777	993.6E6	322.7E6	482.980	466.765
Target Compounds						
1) T Dalapon	0.000	2.570	0	2965949	N.D.	2.650
5) T DICAMBA	0.000	6.978	0	684469	N.D.	<MDL
6) T MCPP	0.000	6.978f	0	684469	N.D.	<MDL
7) T MCPA	0.000	7.243	0	3364852	N.D.	1.050
8) T DICHLORPROP	0.000	7.569	0	876228	N.D.	1.165
9) T 2,4-D	0.000	7.779f	0	572019	N.D.	<MDL
11) T 2,4,5-TP ...	0.000	8.614	0	511321	N.D.	<MDL
12) T 2,4,5-T	0.000	9.032	0	3753024	N.D.	<MDL
15) T Picloram	9.687	10.773	35939231	11726714	2.061	1.887
16) T DCPA	0.000	10.773	0	11726714	N.D.	2.248



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110223\
Data File : PS024735.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Nov 2023 12:43
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 02 23:10:34 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100323.M
Quant Title : 8080.M
QLast Update : Tue Oct 03 14:54:54 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

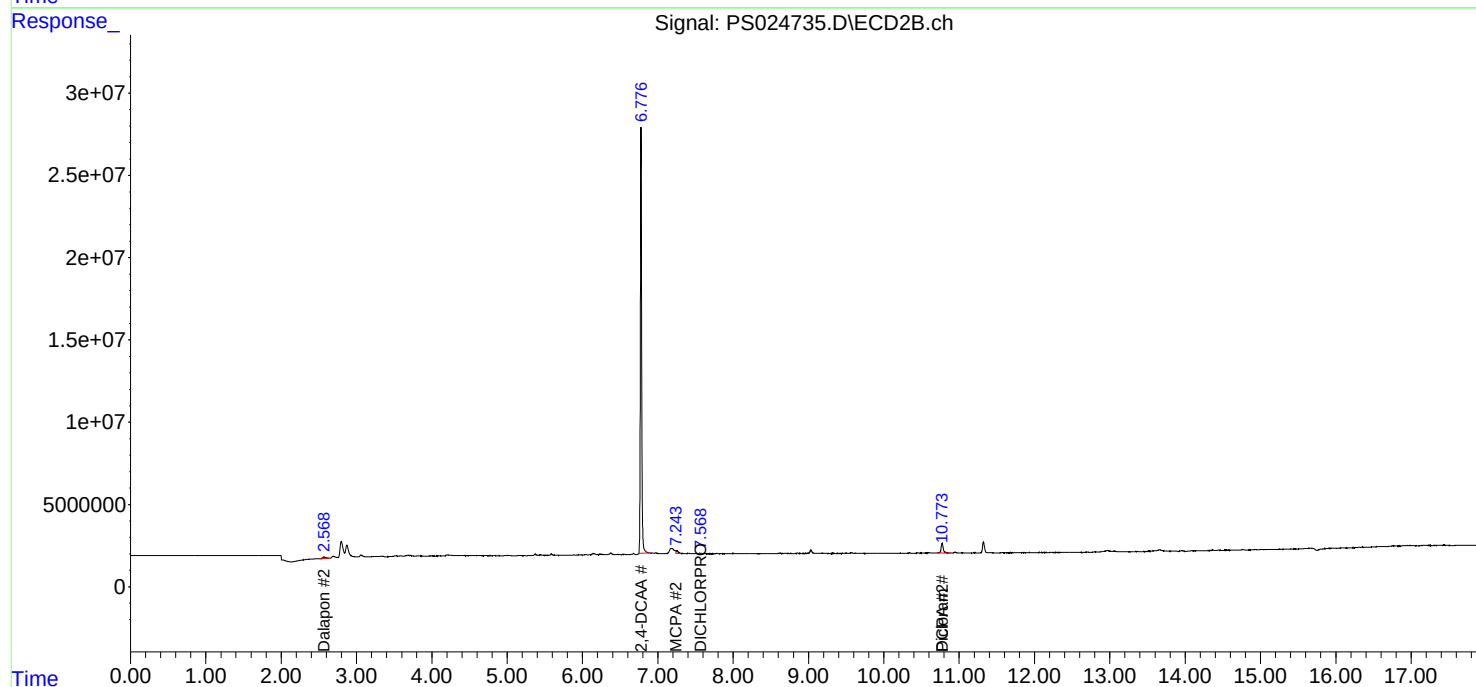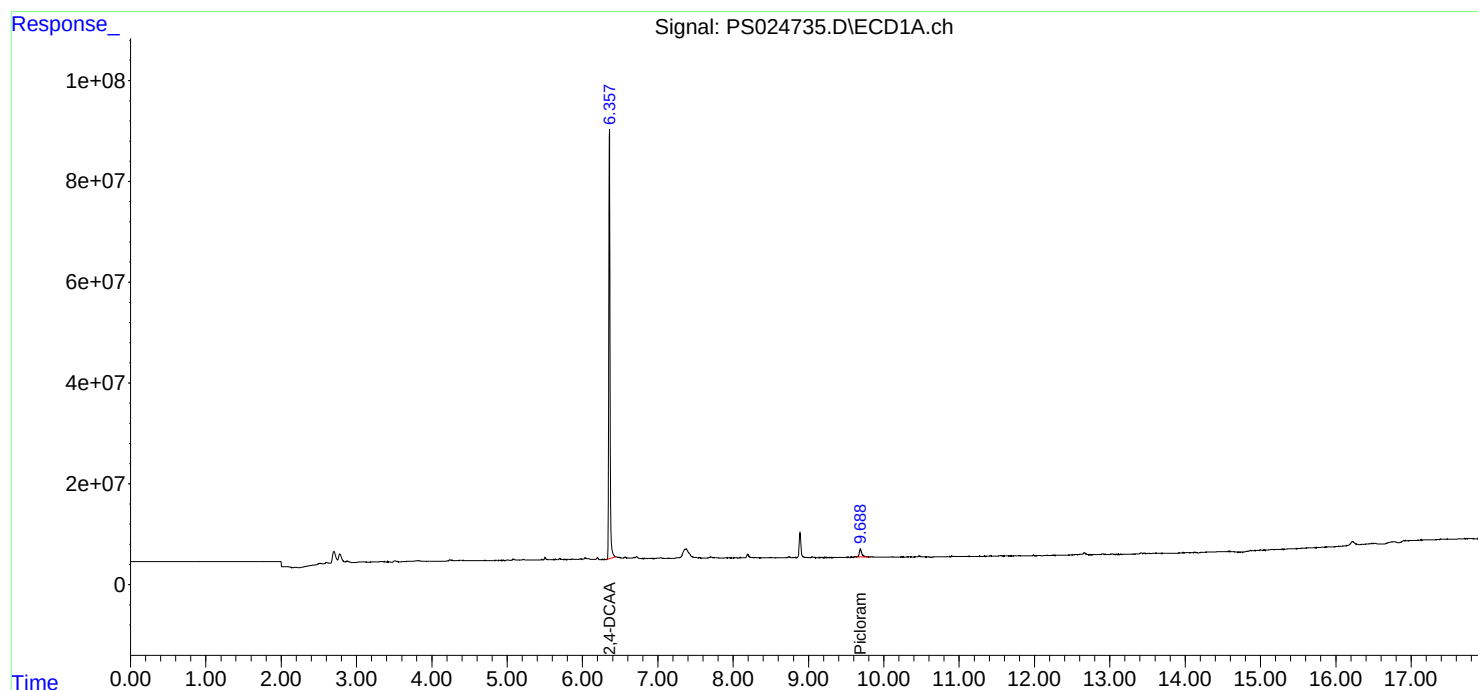


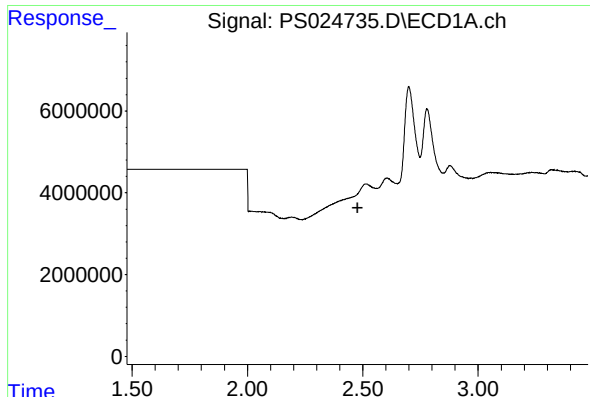

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.477 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

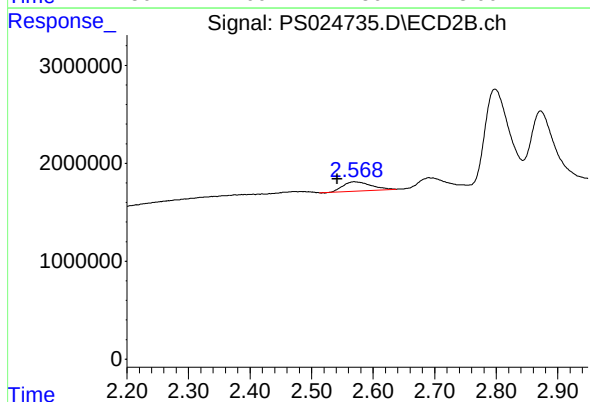


#1 Dalapon

R.T.: 2.570 min
Delta R.T.: 0.028 min
Response: 2965949
Conc: 2.65 ng/ml

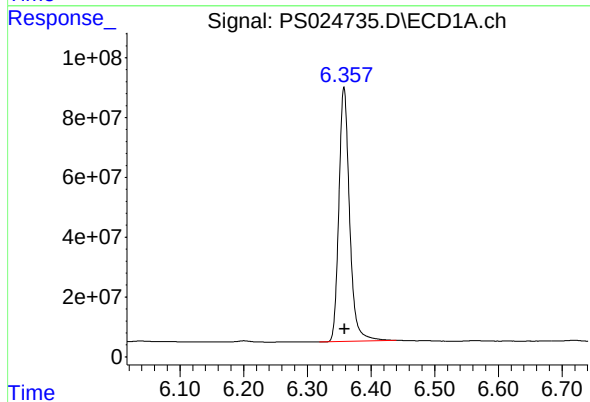


#4 2,4-DCAA

R.T.: 6.358 min
Delta R.T.: -0.001 min
Response: 993647862
Conc: 482.98 ng/ml

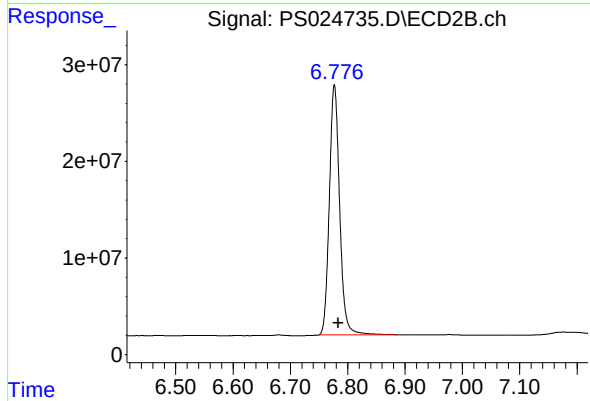

#4 2,4-DCAA


R.T.: 6.777 min
Delta R.T.: -0.007 min
Response: 322670393
Conc: 466.77 ng/ml

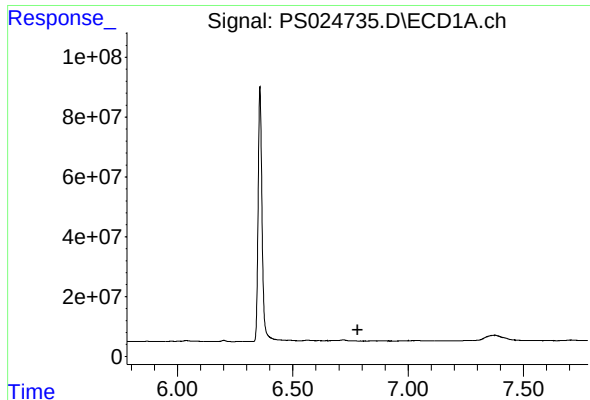

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 6.780 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

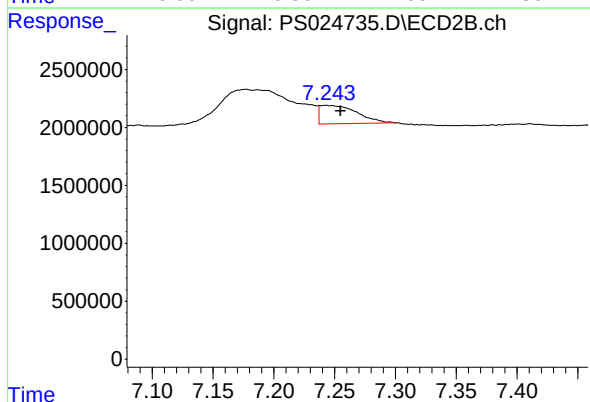


#7 MCPA

R.T.: 7.243 min
Delta R.T.: -0.012 min
Response: 3364852
Conc: 1.05 ug/ml

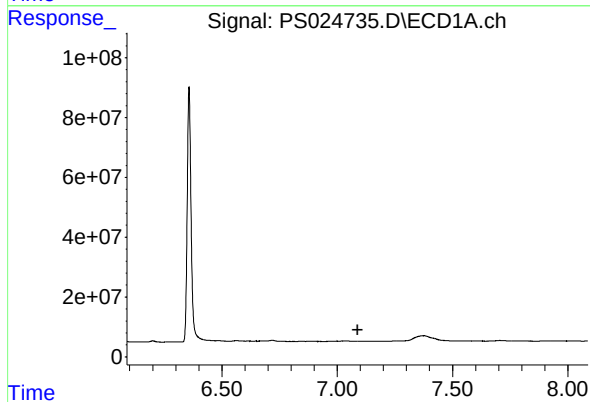


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 7.088 min
Response: 0
Conc: N.D.

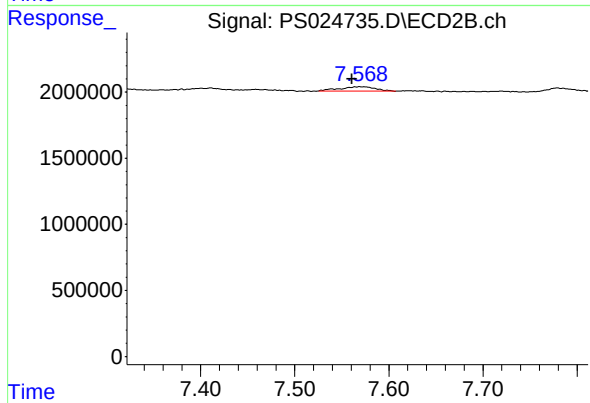

#8 DICHLORPROP


R.T.: 7.569 min
Delta R.T.: 0.008 min
Response: 876228
Conc: 1.17 ng/ml

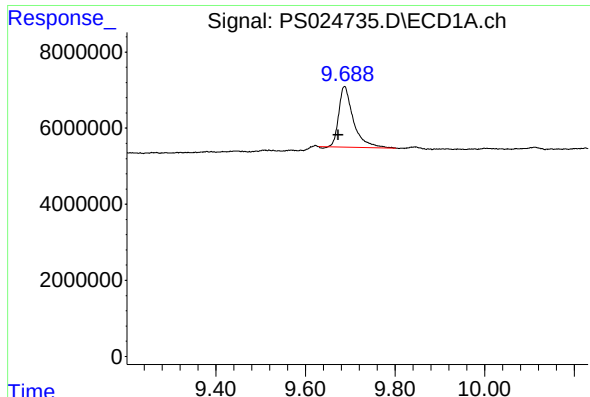

#15 Picloram


R.T.: 9.687 min
Delta R.T.: 0.014 min
Response: 35939231
Conc: 2.06 ng/ml

Instrument :
ECD_S
ClientSampleId :

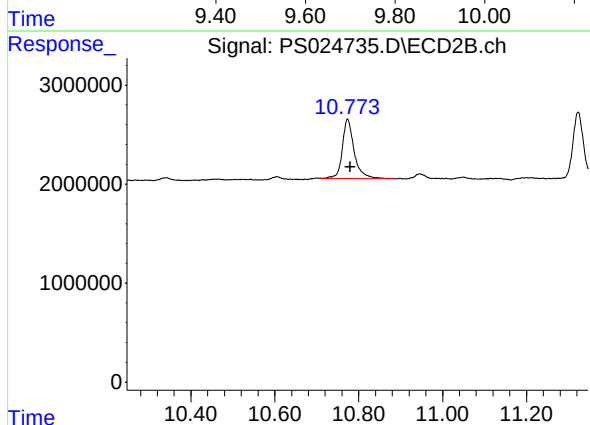


#15 Picloram

R.T.: 10.773 min
Delta R.T.: -0.007 min
Response: 11726714
Conc: 1.89 ng/ml

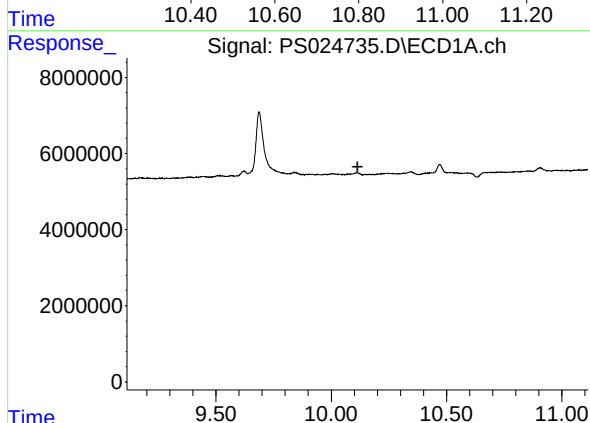

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 10.114 min
Response: 0
Conc: N.D.

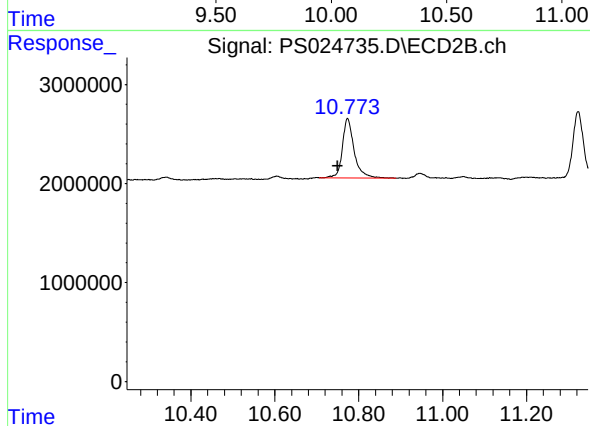

#16 DCPA

R.T.: 10.773 min
Delta R.T.: 0.023 min
Response: 11726714
Conc: 2.25 ng/ml