

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110223\
 Data File : PS024742.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Nov 2023 15:56
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 02 23:11:35 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100323.M
 Quant Title : 8080.M
 QLast Update : Tue Oct 03 14:54:54 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.357	6.777	984.9E6	324.6E6	478.715	469.499
Target Compounds							
1) T	Dalapon	0.000	2.569	0	2984563	N.D.	2.667
3) T	4-Nitroph...	6.199	0.000	7076923	0	5.228	N.D. #
6) T	MCPP	6.685	0.000	1608400	0	<MDL	N.D. #
7) T	MCPA	0.000	7.247	0	7456628	N.D.	2.327
8) T	DICHLORPROP	0.000	7.567	0	3624892	N.D.	4.820
9) T	2,4-D	0.000	7.781f	0	694785	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	8.615	0	610228	N.D.	<MDL
12) T	2,4,5-T	0.000	8.990	0	457246	N.D.	<MDL
13) T	2,4-DB	0.000	9.492	0	685949	N.D.	1.346
15) T	Picloram	9.688	10.775	11872253	4501345	<MDL	<MDL #
16) T	DCPA	0.000	10.775	0	4501345	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110223\
Data File : PS024742.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Nov 2023 15:56
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 02 23:11:35 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100323.M
Quant Title : 8080.M
QLast Update : Tue Oct 03 14:54:54 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

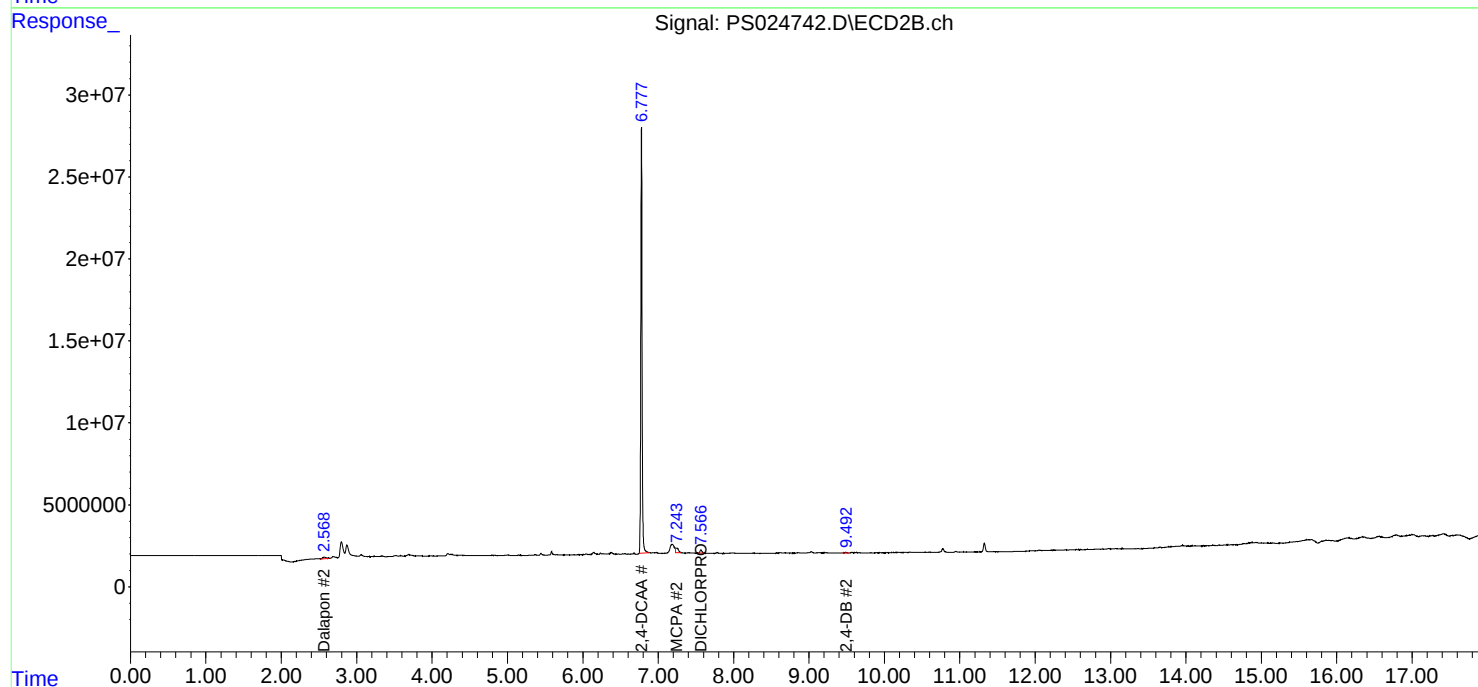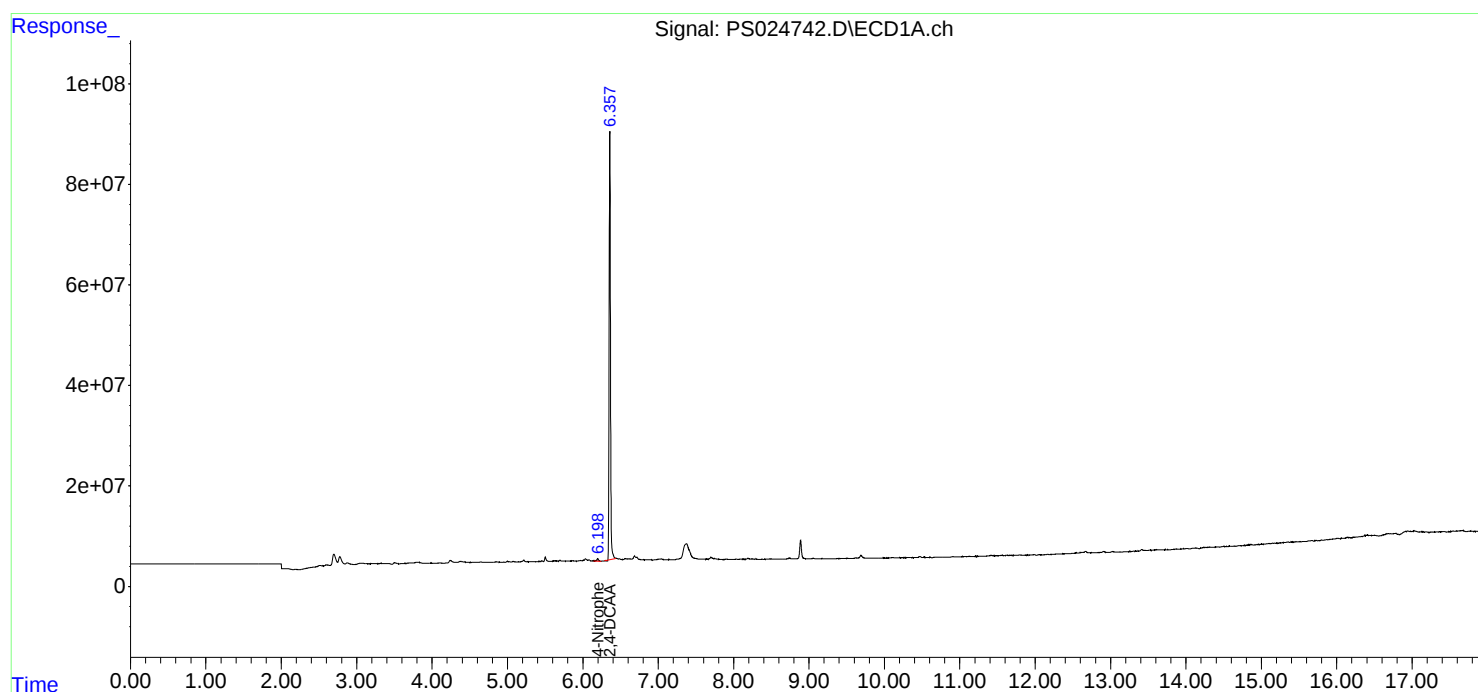


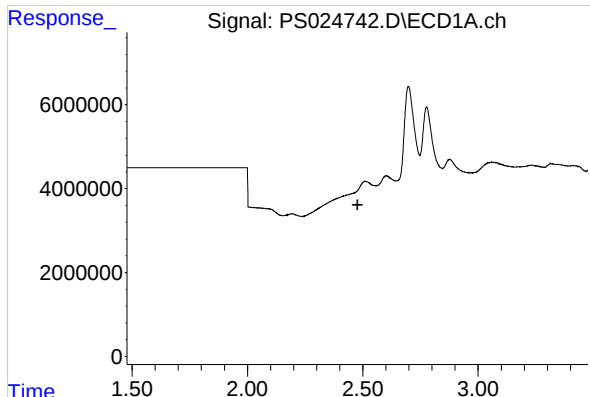

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.477 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

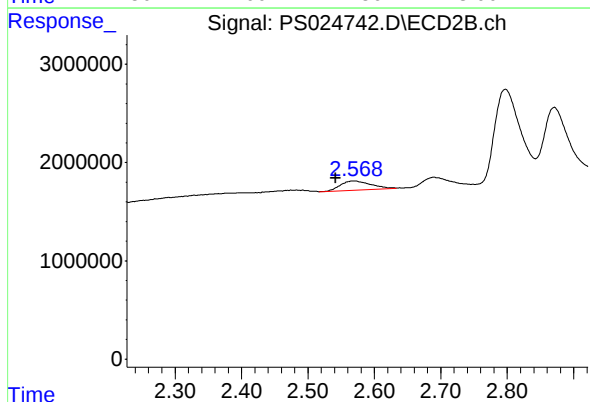


#1 Dalapon

R.T.: 2.569 min
Delta R.T.: 0.027 min
Response: 2984563
Conc: 2.67 ng/ml

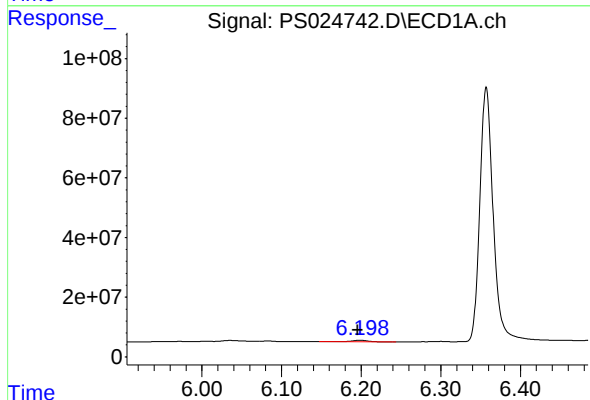


#3 4-Nitrophenol

R.T.: 6.199 min
Delta R.T.: 0.003 min
Response: 7076923
Conc: 5.23 ng/ml

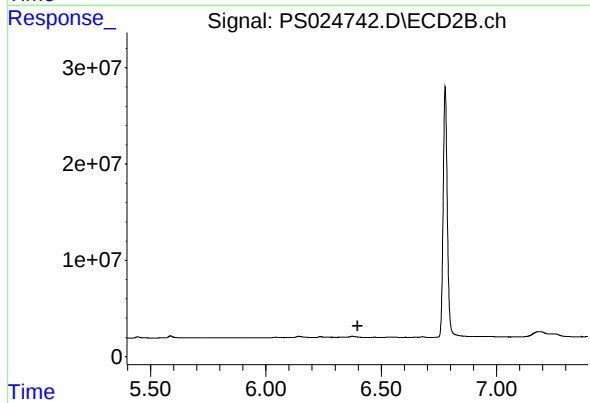

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 6.397 min
Response: 0
Conc: N.D.

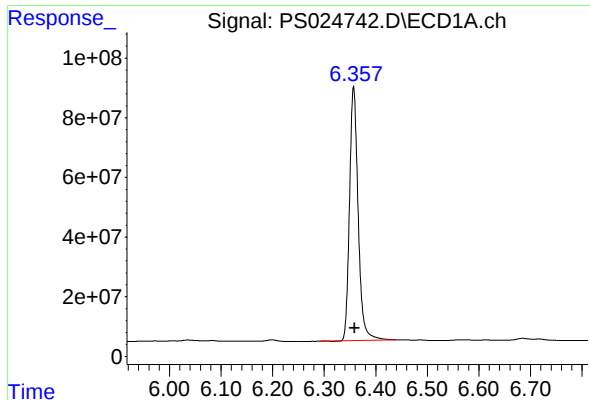

#4 2,4-DCAA


R.T.: 6.357 min
Delta R.T.: -0.002 min
Response: 984873742
Conc: 478.71 ng/ml

Instrument :
ECD_S
ClientSampleId :

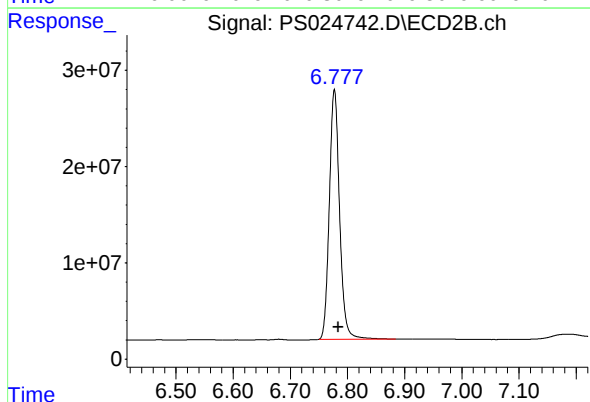


#4 2,4-DCAA

R.T.: 6.777 min
Delta R.T.: -0.007 min
Response: 324560172
Conc: 469.50 ng/ml

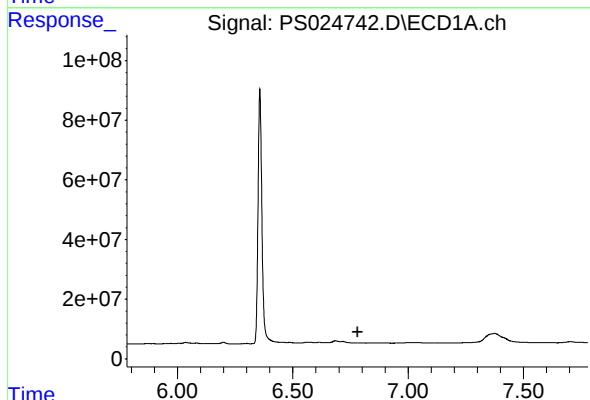


#7 MCPA

R.T.: 0.000 min
Exp R.T.: 6.780 min
Response: 0
Conc: N.D.

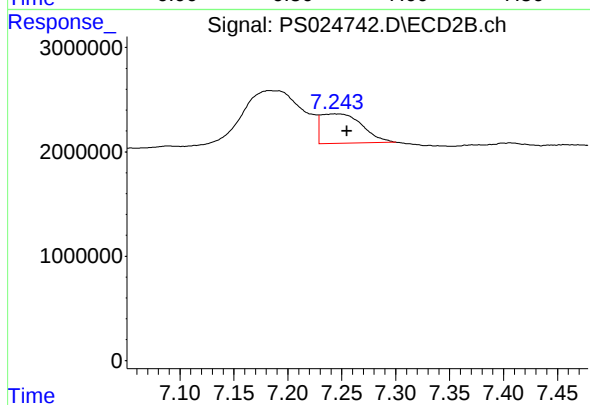

#7 MCPA


R.T.: 7.247 min
Delta R.T.: -0.008 min
Response: 7456628
Conc: 2.33 ug/ml

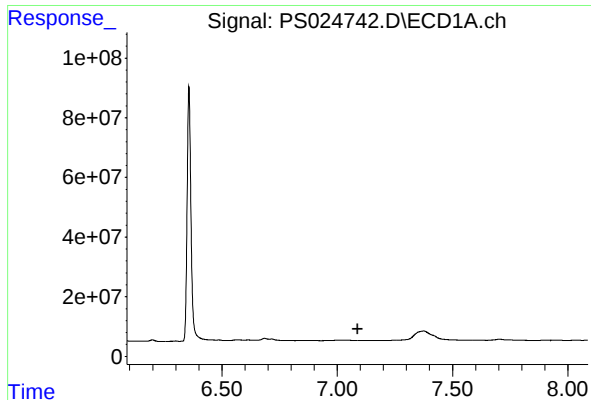

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 7.088 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

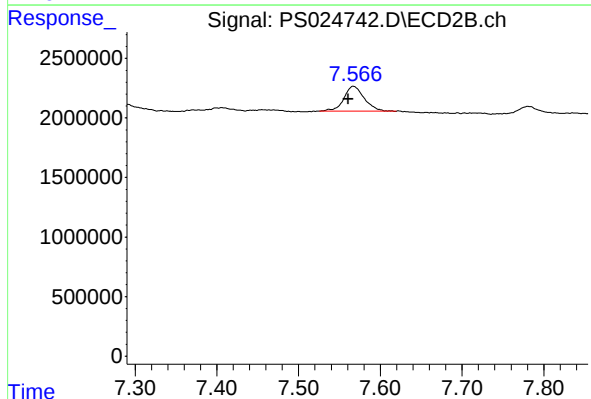


#8 DICHLORPROP

R.T.: 7.567 min
Delta R.T.: 0.006 min
Response: 3624892
Conc: 4.82 ng/ml

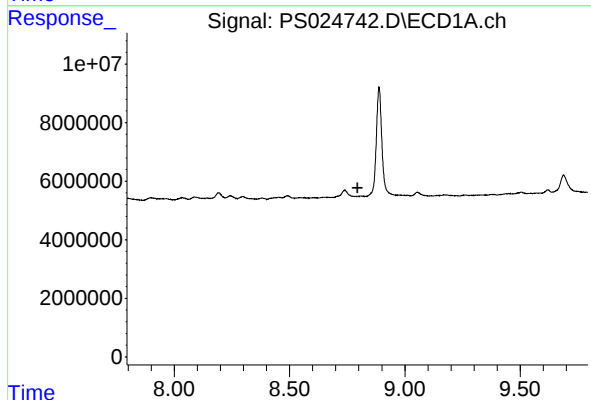

#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 8.795 min
Response: 0
Conc: N.D.

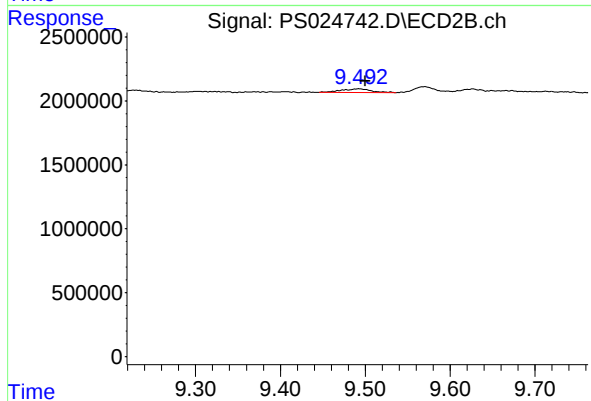

#13 2,4-DB

R.T.: 9.492 min
Delta R.T.: -0.008 min
Response: 685949
Conc: 1.35 ng/ml