

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110223\
 Data File : PS024749.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Nov 2023 19:13
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 02 23:12:49 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100323.M
 Quant Title : 8080.M
 QLast Update : Tue Oct 03 14:54:54 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	6.357	6.777	977.4E6	323.0E6	475.060	467.230
Target Compounds						
1) T Dalapon	0.000	2.571	0	3473374	N.D.	3.104
3) T 4-Nitroph...	6.197	0.000	9572179	0	7.071	N.D. #
6) T MCPP	6.684	0.000	2509403	0	<MDL	N.D. #
8) T DICHLORPROP	0.000	7.566	0	5217999	N.D.	6.938
9) T 2,4-D	0.000	7.781f	0	1200356	N.D.	1.304
10) T Pentachlo...	0.000	8.260	0	432470	N.D.	<MDL
11) T 2,4,5-TP ...	0.000	8.617	0	705685	N.D.	<MDL
12) T 2,4,5-T	0.000	8.988	0	608917	N.D.	<MDL
13) T 2,4-DB	0.000	9.482	0	906608	N.D.	1.779
15) T Picloram	9.685	10.773	37690846	12340176	2.162	1.986
16) T DCPA	0.000	10.773	0	12340176	N.D.	2.365



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110223\
Data File : PS024749.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Nov 2023 19:13
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 02 23:12:49 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100323.M
Quant Title : 8080.M
QLast Update : Tue Oct 03 14:54:54 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

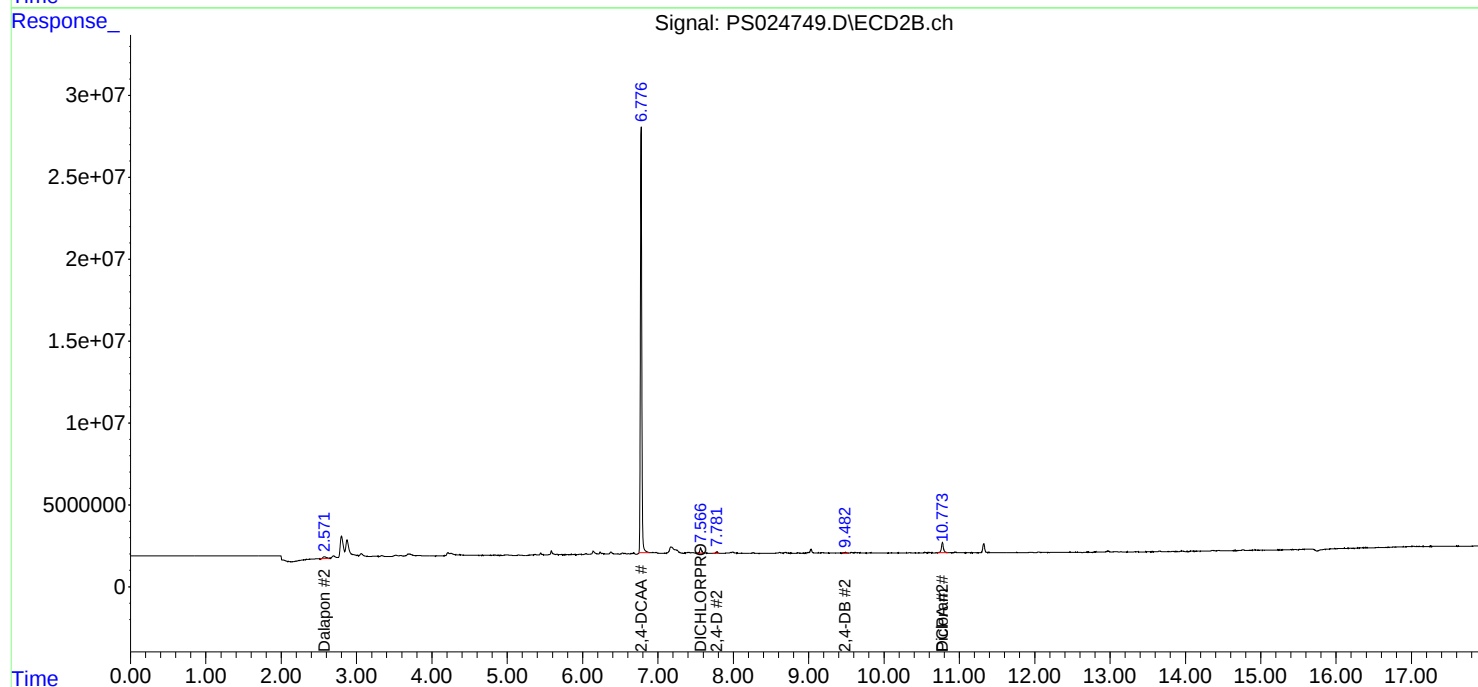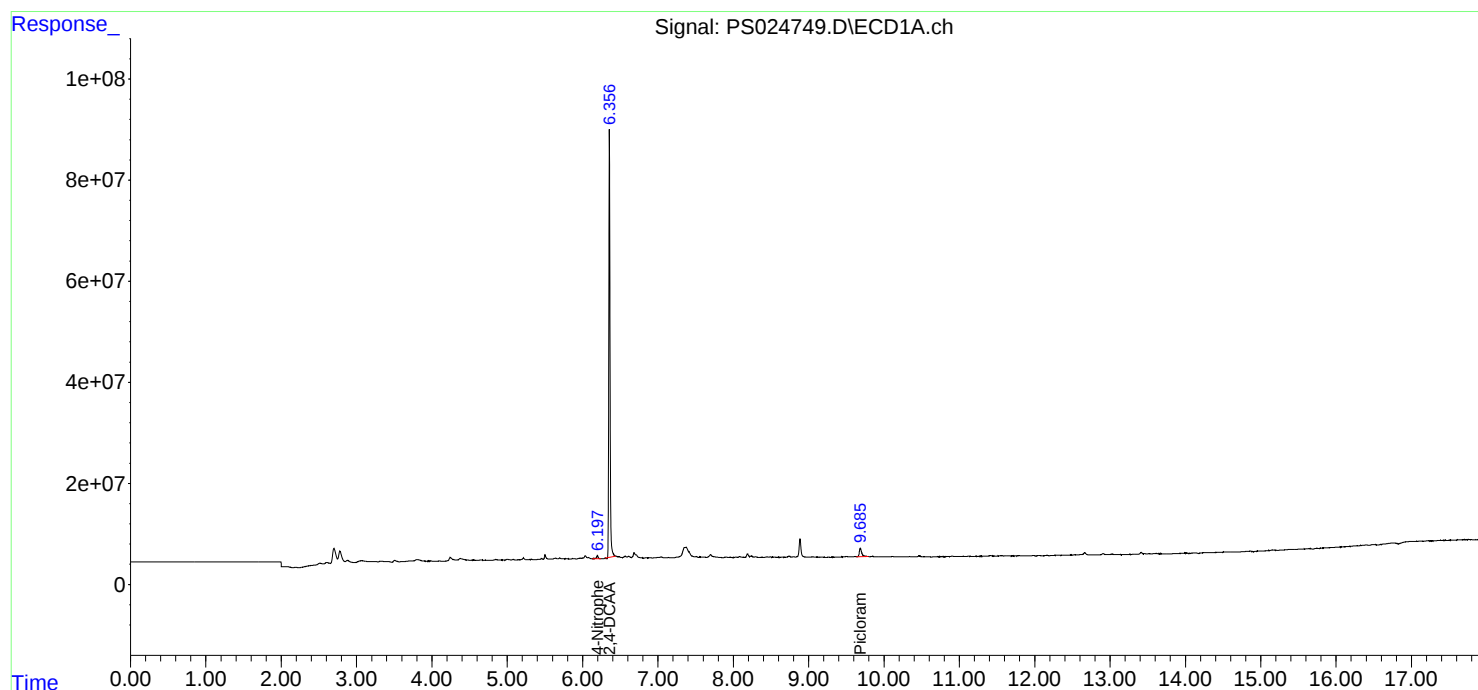


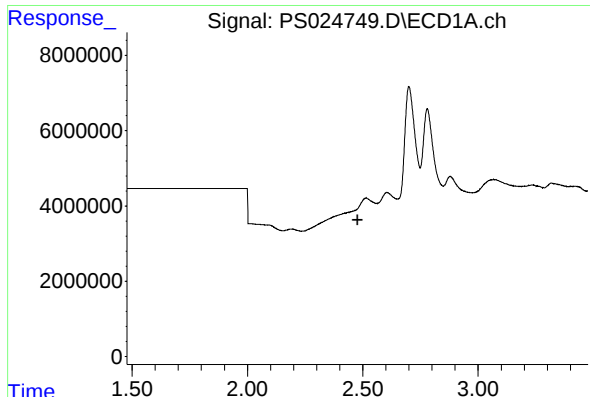

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.477 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

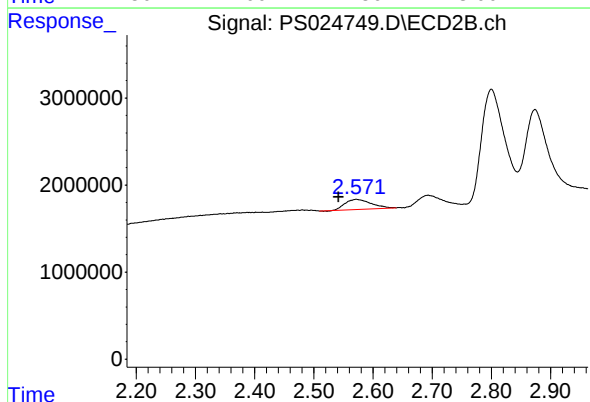


#1 Dalapon

R.T.: 2.571 min
Delta R.T.: 0.029 min
Response: 3473374
Conc: 3.10 ng/ml

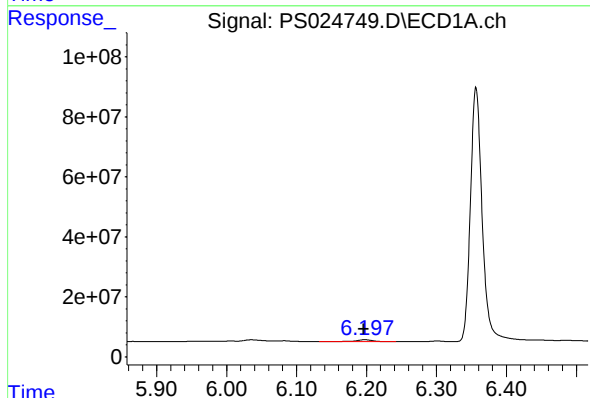


#3 4-Nitrophenol

R.T.: 6.197 min
Delta R.T.: 0.001 min
Response: 9572179
Conc: 7.07 ng/ml

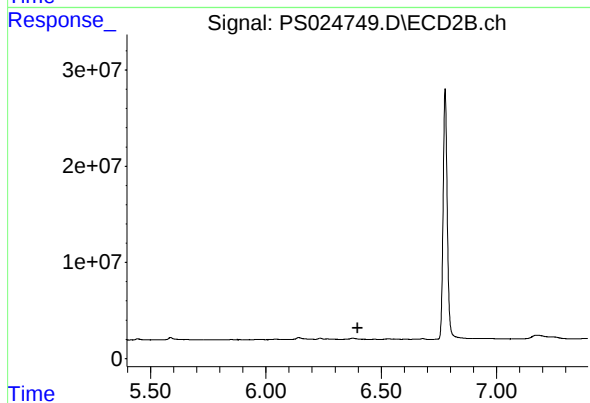

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 6.397 min
Response: 0
Conc: N.D.

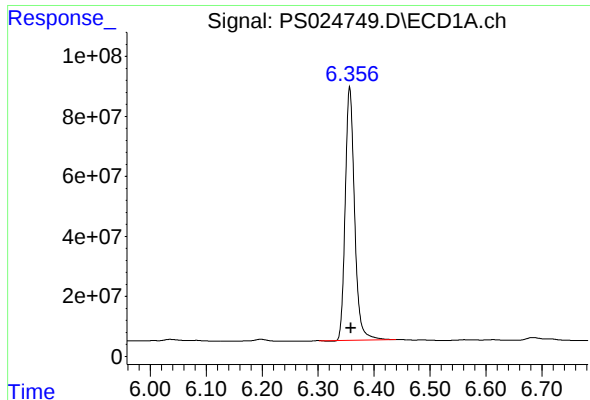

#4 2,4-DCAA


R.T.: 6.357 min
Delta R.T.: -0.002 min
Response: 977354423
Conc: 475.06 ng/ml

Instrument :
ECD_S
ClientSampleId :

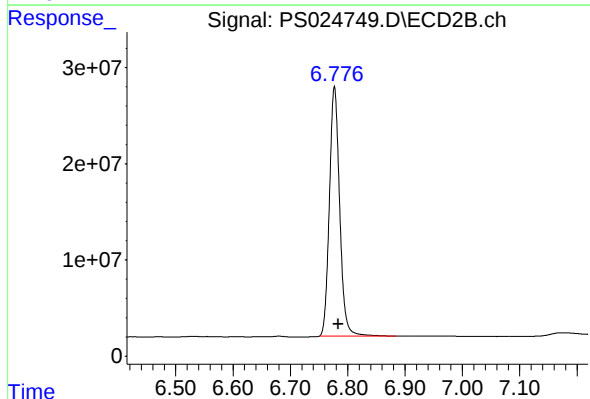


#4 2,4-DCAA

R.T.: 6.777 min
Delta R.T.: -0.007 min
Response: 322992026
Conc: 467.23 ng/ml

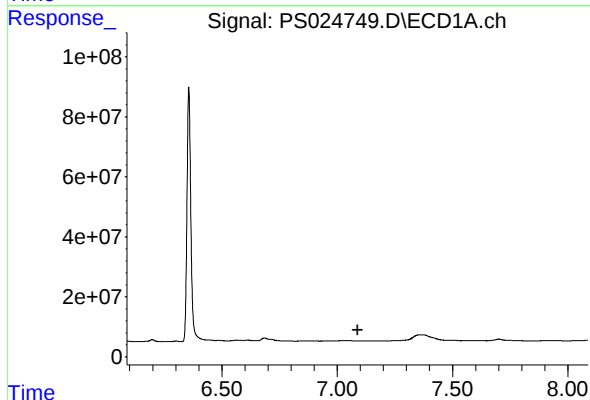


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 7.088 min
Response: 0
Conc: N.D.

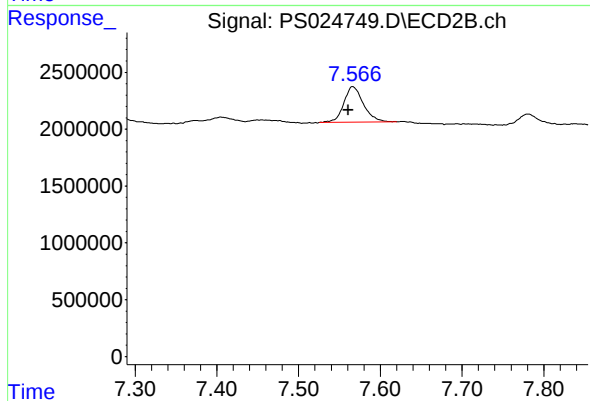

#8 DICHLORPROP


R.T.: 7.566 min
Delta R.T.: 0.005 min
Response: 5217999
Conc: 6.94 ng/ml

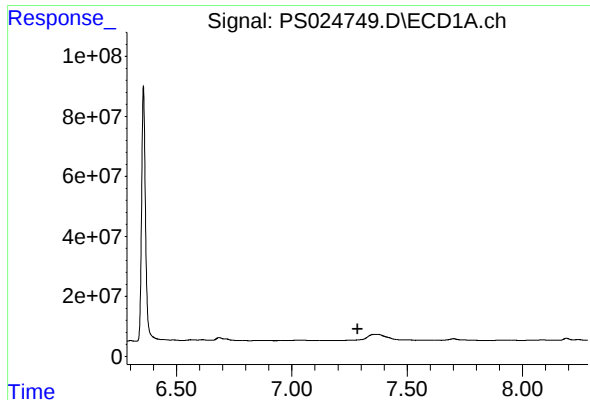

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 7.284 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

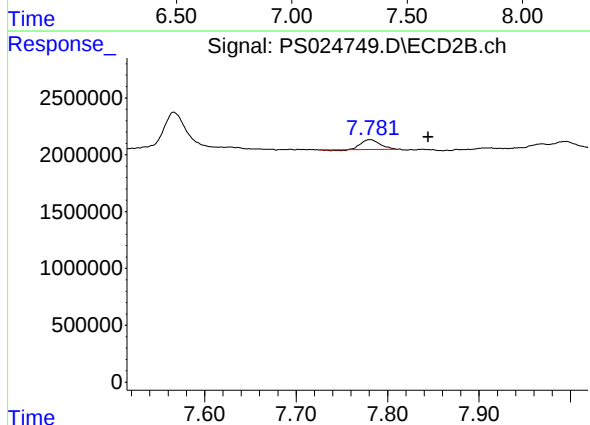


#9 2,4-D

R.T.: 7.781 min
Delta R.T.: -0.063 min
Response: 1200356
Conc: 1.30 ng/ml

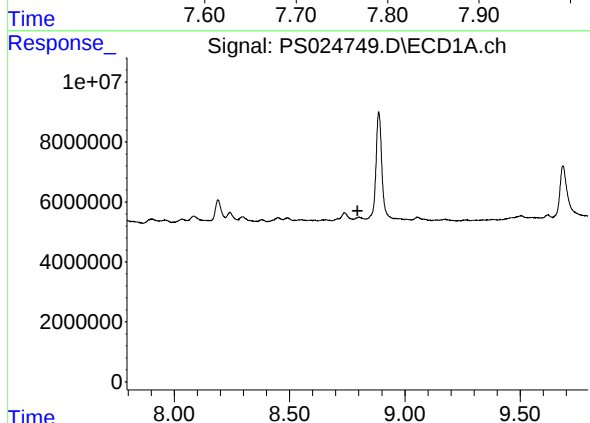


#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 8.795 min
Response: 0
Conc: N.D.

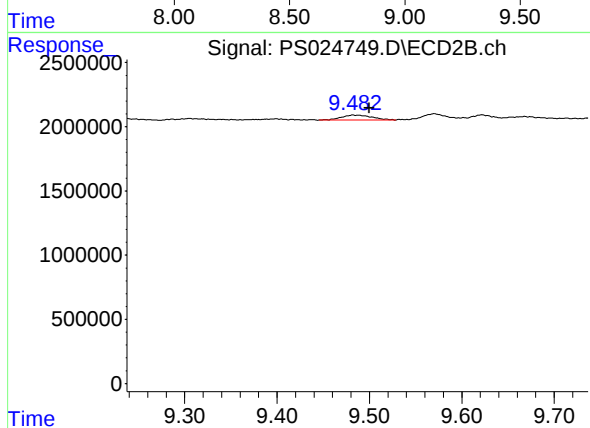

#13 2,4-DB


R.T.: 9.482 min
Delta R.T.: -0.018 min
Response: 906608
Conc: 1.78 ng/ml

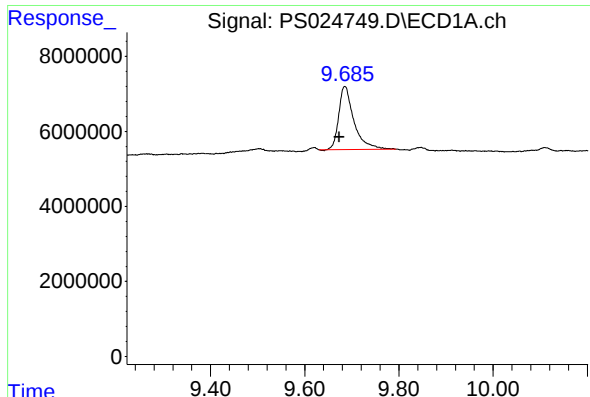

#15 Picloram


R.T.: 9.685 min
Delta R.T.: 0.012 min
Response: 37690846
Conc: 2.16 ng/ml

Instrument :
ECD_S
ClientSampleId :

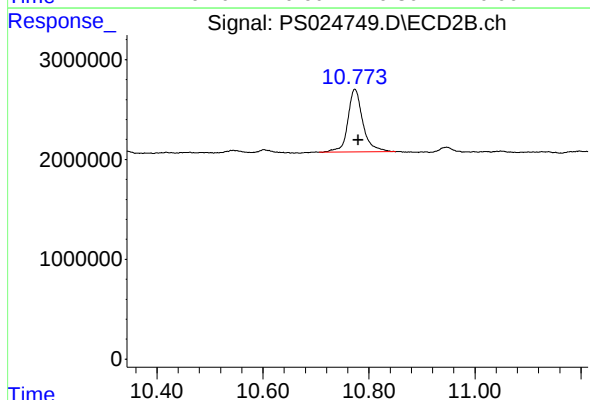


#15 Picloram

R.T.: 10.773 min
Delta R.T.: -0.007 min
Response: 12340176
Conc: 1.99 ng/ml

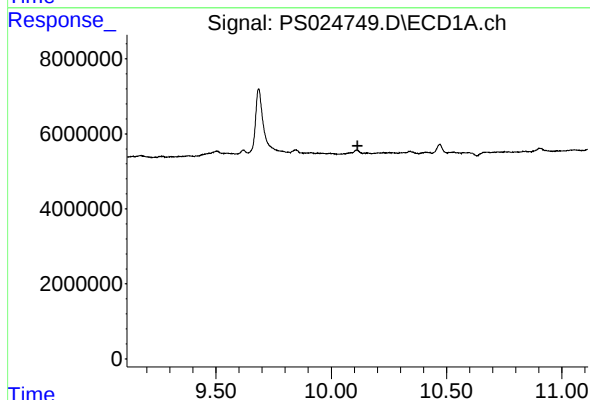

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 10.114 min
Response: 0
Conc: N.D.

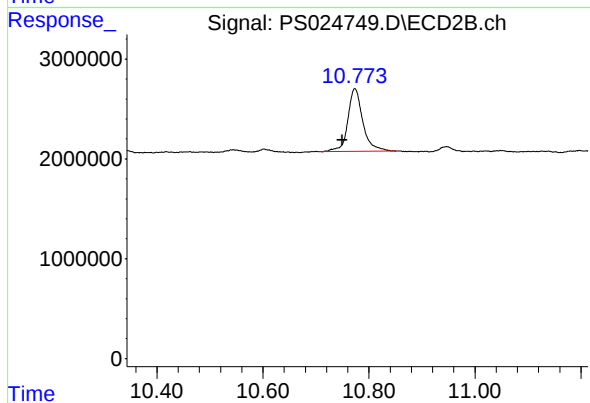

#16 DCPA

R.T.: 10.773 min
Delta R.T.: 0.023 min
Response: 12340176
Conc: 2.37 ng/ml