

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110321\
 Data File : PS017327.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Nov 2021 11:40
 Operator : DD\AJ
 Sample : M4433-03
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PSC-124035

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 11/04/2021
 Supervised By :mohammad ahmed 11/05/2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 03 14:58:00 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101821.M
 Quant Title : 8080.M
 QLast Update : Tue Oct 19 01:21:46 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	7.148	6.736	764.1E6	306.8E6	499.930m	524.994m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110321\
Data File : PS017327.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Nov 2021 11:40
Operator : DD\AJ
Sample : M4433-03
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
PSC-124035


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 11/04/2021
Supervised By :mohammad ahmed 11/05/2021

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 03 14:58:00 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101821.M
Quant Title : 8080.M
QLast Update : Tue Oct 19 01:21:46 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

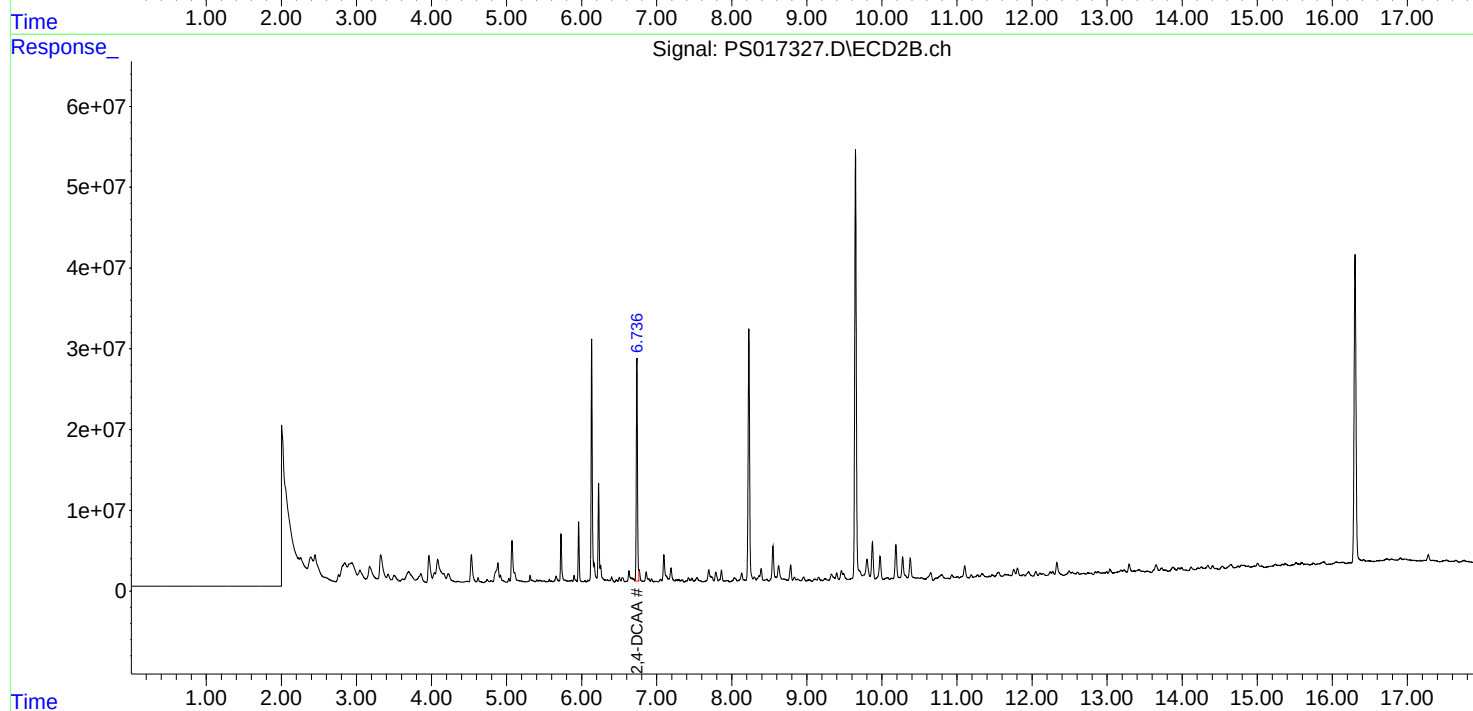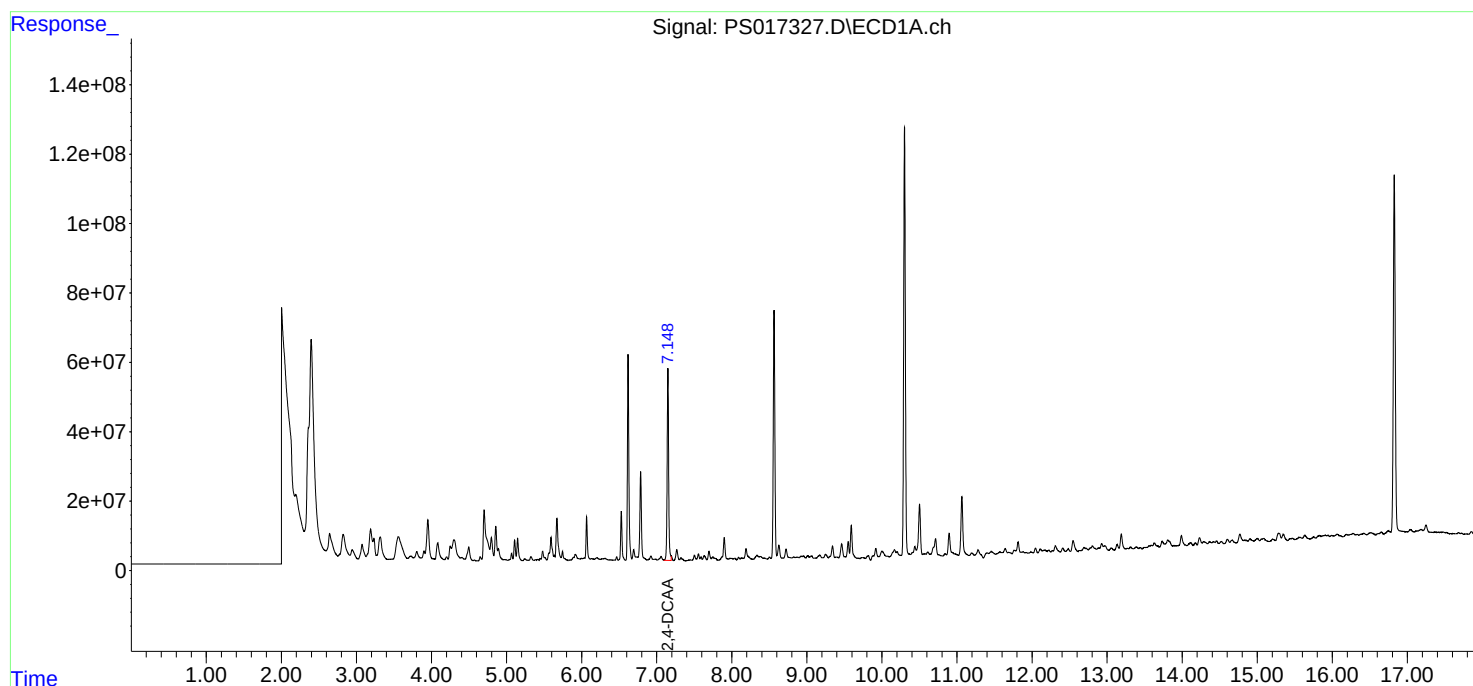

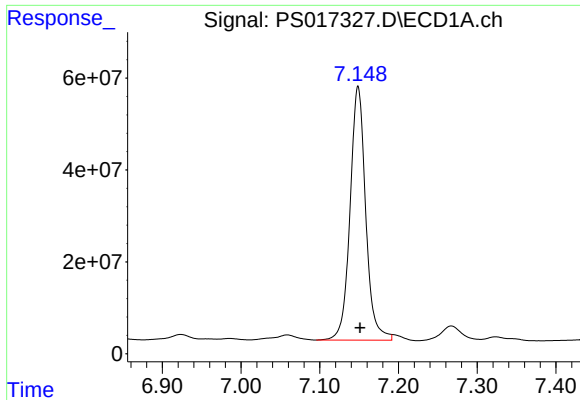


#4 2,4-DCAA

R.T.: 7.148 min
Delta R.T.: -0.003 min
Response: 764123382
Conc: 499.93 ng/ml

Instrument :
ECD_S
ClientSampleId :
PSC-124035

Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 11/04/2021
Supervised By :mohammad ahmed 11/05/2021

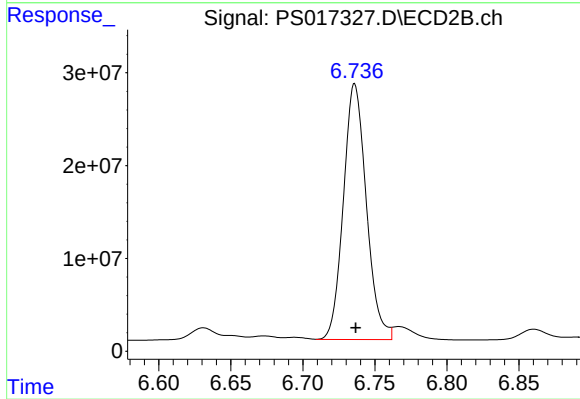

#4 2,4-DCAA

R.T.: 6.736 min
Delta R.T.: -0.001 min
Response: 306828341
Conc: 524.99 ng/ml m