

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110322\
 Data File : PS021022.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Nov 2022 10:56
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 03 17:25:07 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102822.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 31 10:07:57 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.411	6.848	1100.5E6	754.0E6	527.290	545.117
Target Compounds							
1) T	Dalapon	2.506	0.000	500895	0	<MDL	N.D. #
3) T	4-Nitroph...	6.246	6.444	10752932	2554862	7.149	2.972 #
5) T	DICAMBA	6.624f	7.017	7241195	5009949	<MDL	<MDL #
6) T	MCP	6.676	7.067f	12639690	4017084	1.937	<MDL #
7) T	MCPA	6.780f	0.000	15985253	0	1.704	N.D. #
8) T	DICHLORPROP	7.216f	7.668	881496	5748730	<MDL	3.733 #
9) T	2,4-D	7.285f	7.895	120726	4208316	<MDL	2.247 #
10) T	Pentachlo...	7.577	0.000	3995157	0	<MDL	N.D. #
11) T	2,4,5-TP ...	8.136	8.688f	4572399	6638133	<MDL	<MDL #
12) T	2,4,5-T	8.337	9.108	18271621	1174774	1.373	<MDL #
13) T	2,4-DB	8.848	0.000	3033530	0	1.100	N.D. #
14) T	DINOSEB	9.899f	0.000	9610104	0	<MDL	N.D. #
15) T	Picloram	9.756	10.958f	2703187	18267023	<MDL	1.440 #
16) T	DCPA	10.200	0.000	991211	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110322\
Data File : PS021022.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Nov 2022 10:56
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 03 17:25:07 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102822.M
Quant Title : 8080.M
QLast Update : Mon Oct 31 10:07:57 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

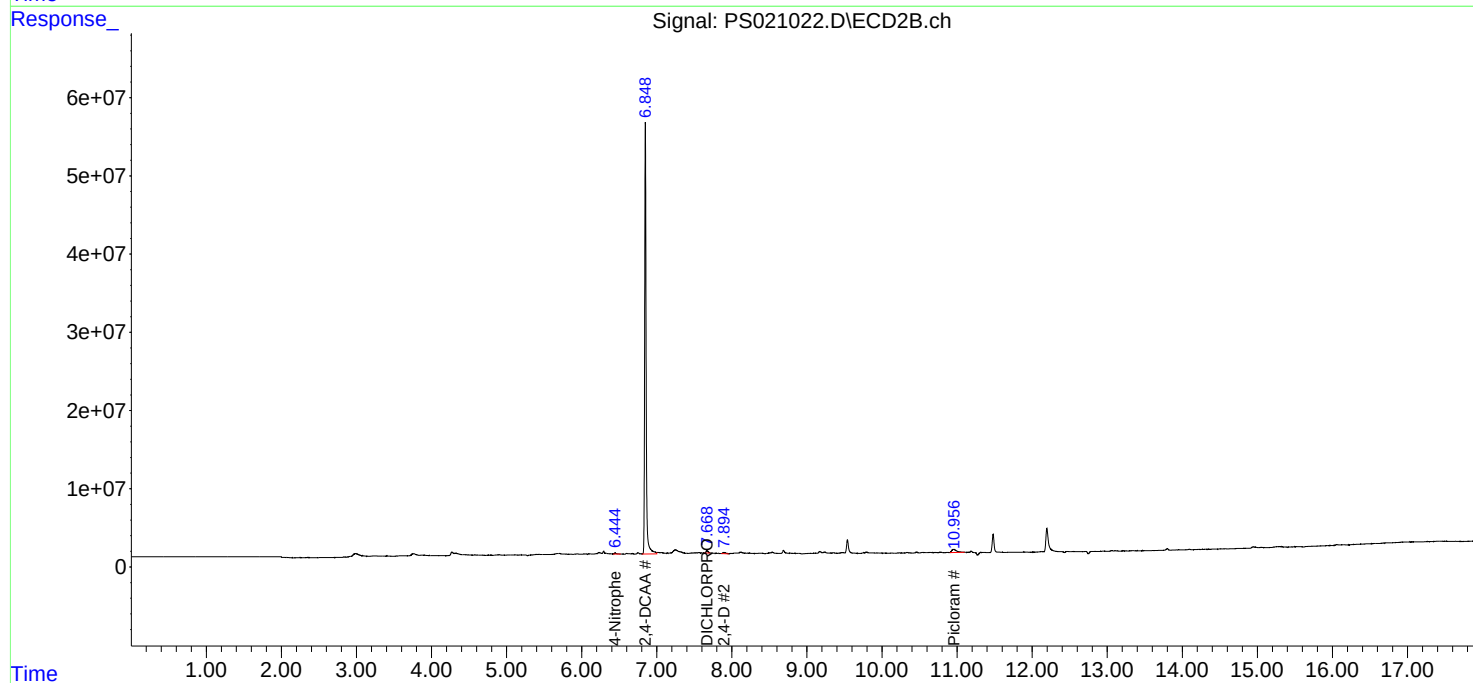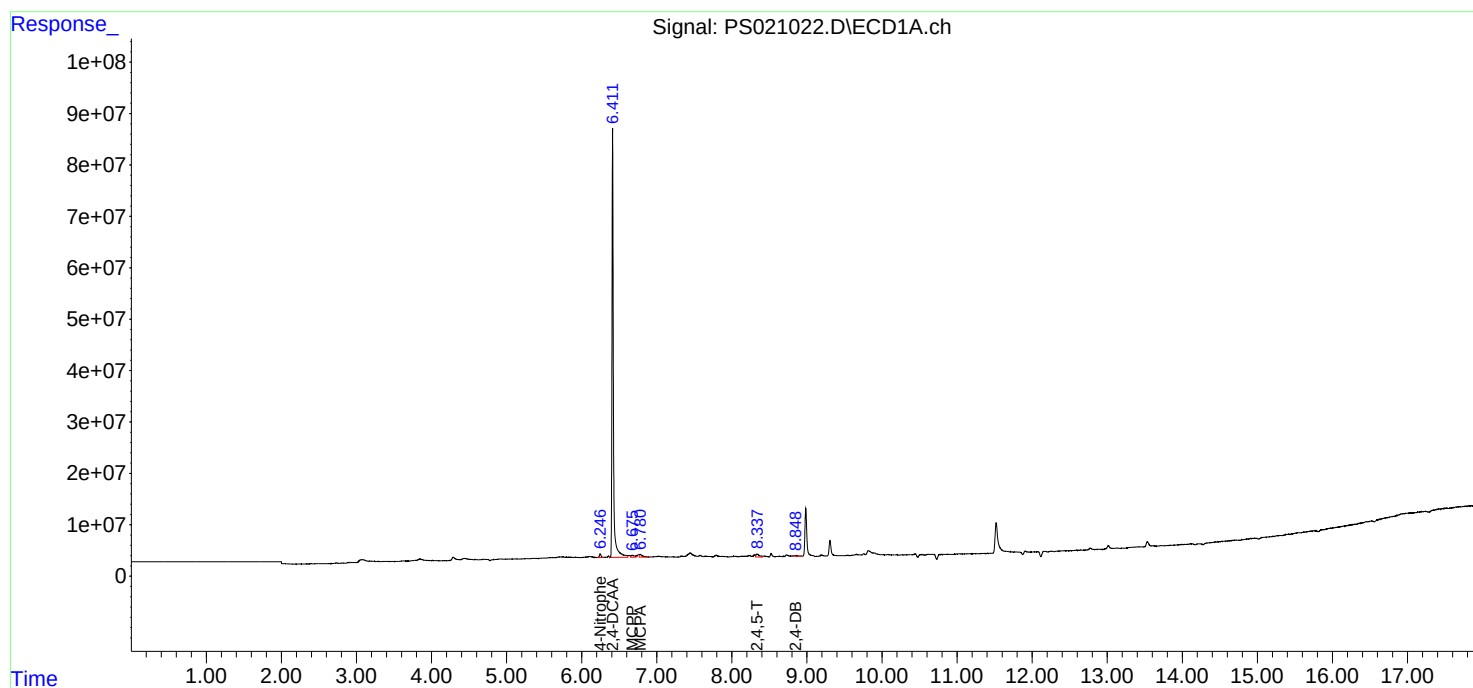


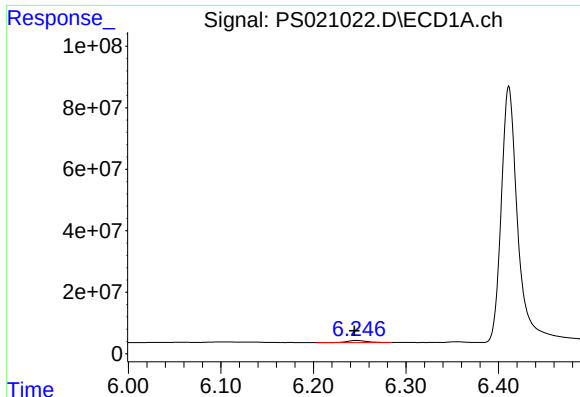

#3 4-Nitrophenol


R.T.: 6.246 min
Delta R.T.: 0.002 min
Response: 10752932
Conc: 7.15 ng/ml

Instrument :
ECD_S
ClientSampleId :

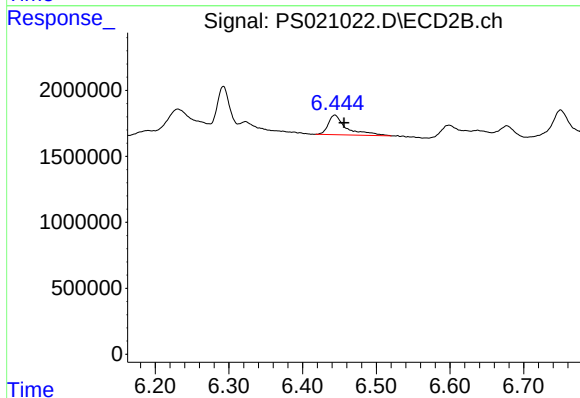


#3 4-Nitrophenol

R.T.: 6.444 min
Delta R.T.: -0.012 min
Response: 2554862
Conc: 2.97 ng/ml

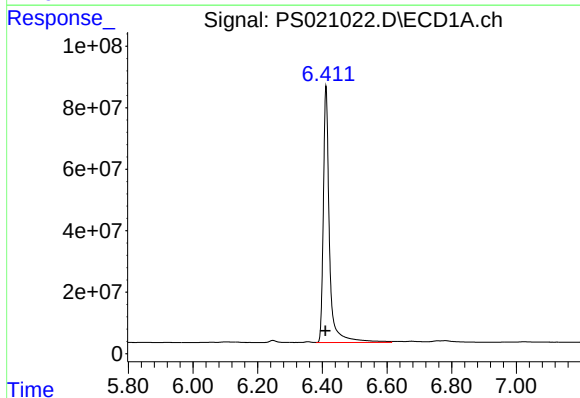


#4 2,4-DCAA

R.T.: 6.411 min
Delta R.T.: 0.002 min
Response: 1100495207
Conc: 527.29 ng/ml

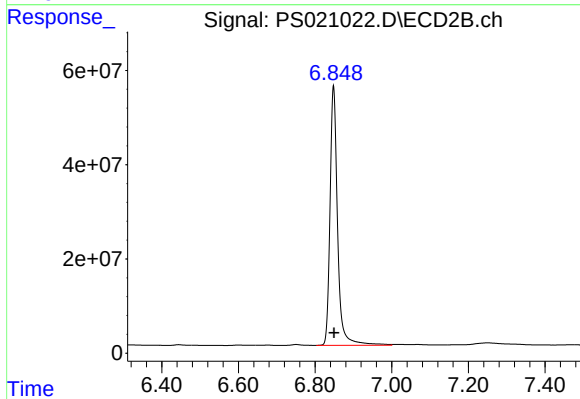

#4 2,4-DCAA


R.T.: 6.848 min
Delta R.T.: -0.002 min
Response: 753976667
Conc: 545.12 ng/ml

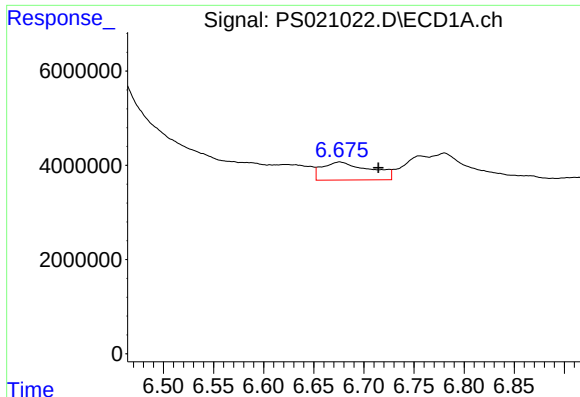

#6 MCPP


R.T.: 6.676 min
Delta R.T.: -0.039 min
Response: 12639690
Conc: 1.94 ug/ml

Instrument :
ECD_S
ClientSampleId :

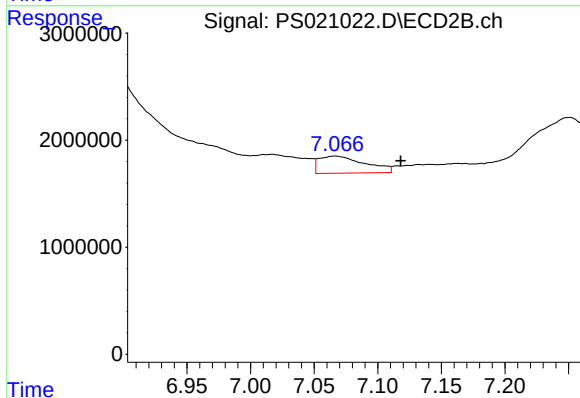


#6 MCPP

R.T.: 7.067 min
Delta R.T.: -0.051 min
Response: 4017084
Conc: N.D.

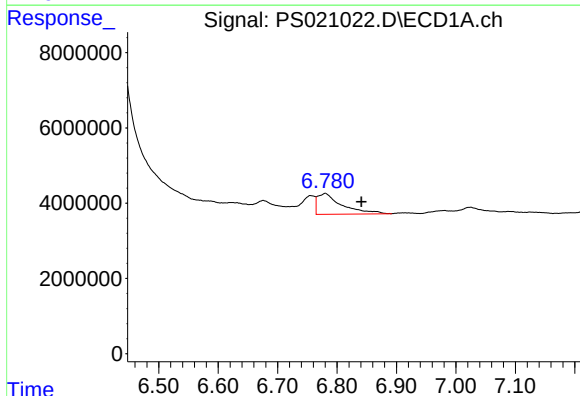


#7 MCPA

R.T.: 6.780 min
Delta R.T.: -0.061 min
Response: 15985253
Conc: 1.70 ug/ml

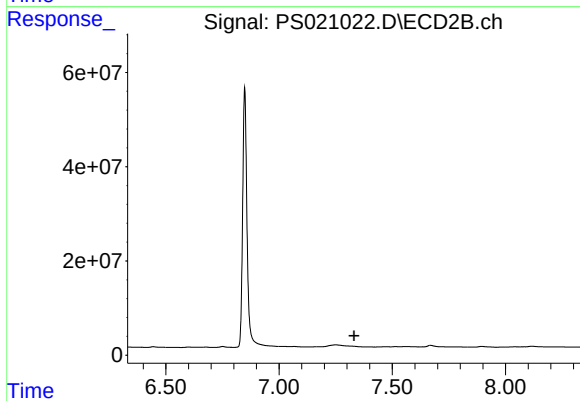

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 7.331 min
Response: 0
Conc: N.D.

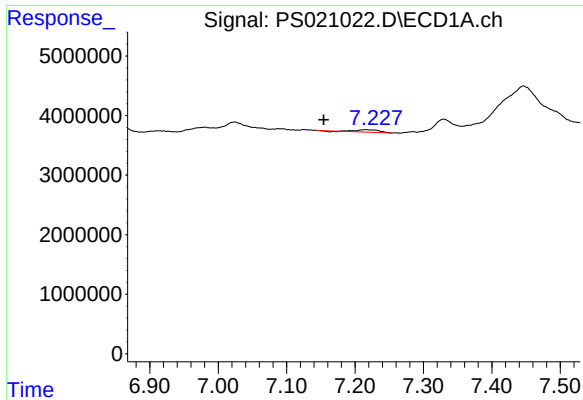

#8 DICHLORPROP


R.T.: 7.216 min
Delta R.T.: 0.061 min
Response: 881496
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

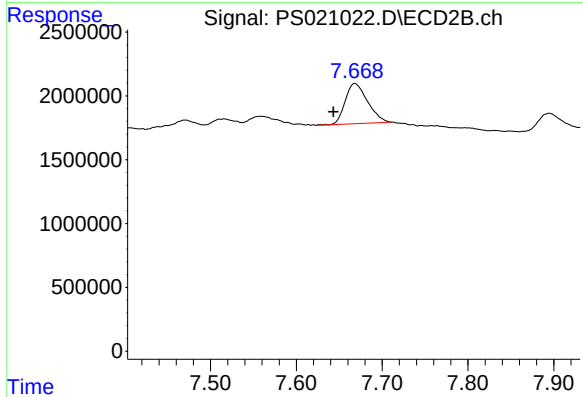


#8 DICHLORPROP

R.T.: 7.668 min
Delta R.T.: 0.025 min
Response: 5748730
Conc: 3.73 ng/ml

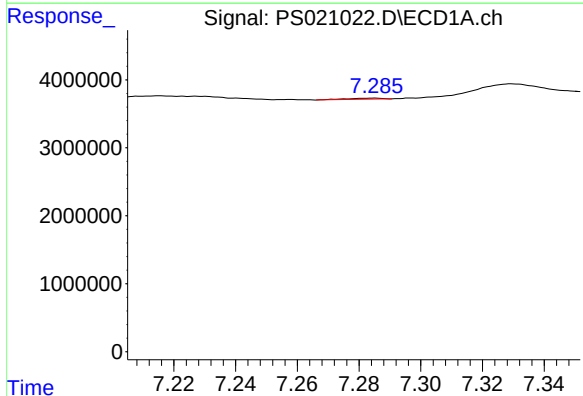


#9 2,4-D

R.T.: 7.285 min
Delta R.T.: -0.069 min
Response: 120726
Conc: N.D.

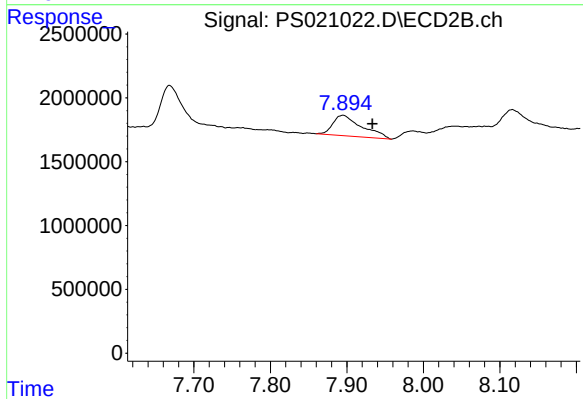

#9 2,4-D


R.T.: 7.895 min
Delta R.T.: -0.038 min
Response: 4208316
Conc: 2.25 ng/ml

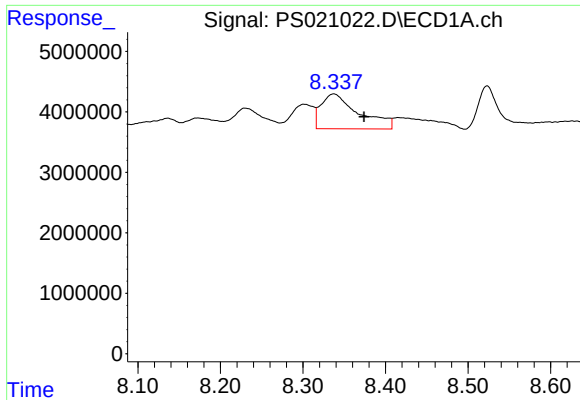

#12 2,4,5-T


R.T.: 8.337 min
Delta R.T.: -0.037 min
Response: 18271621
Conc: 1.37 ng/ml

Instrument :
ECD_S
ClientSampleId :

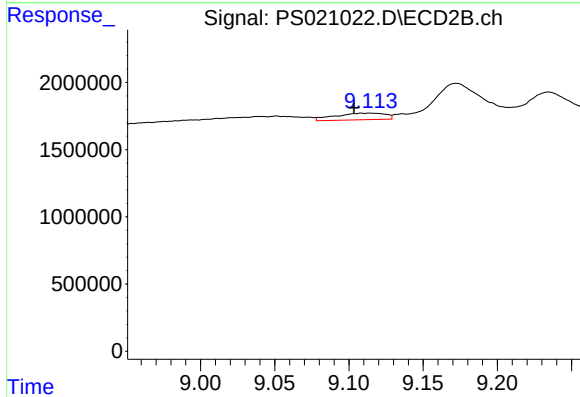


#12 2,4,5-T

R.T.: 9.108 min
Delta R.T.: 0.005 min
Response: 1174774
Conc: N.D.

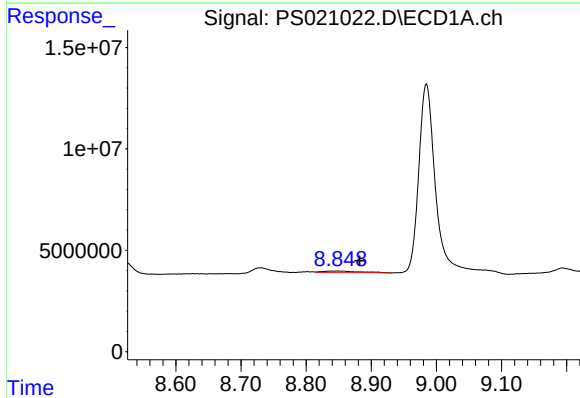


#13 2,4-DB

R.T.: 8.848 min
Delta R.T.: -0.034 min
Response: 3033530
Conc: 1.10 ng/ml

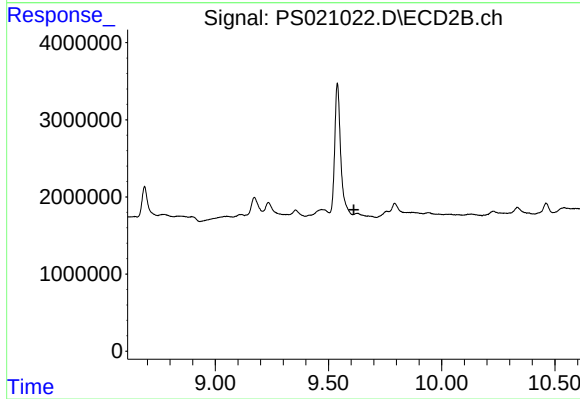

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 9.612 min
Response: 0
Conc: N.D.

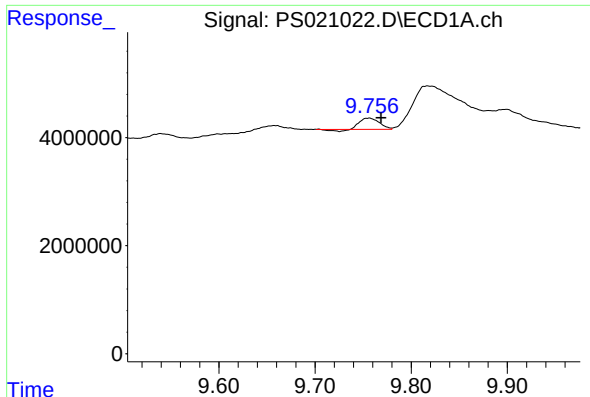

#15 Picloram

R.T.: 9.756 min
Delta R.T.: -0.012 min
Response: 2703187
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

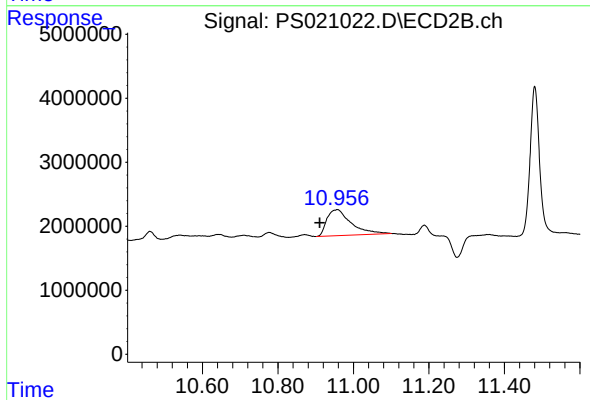

#15 Picloram

R.T.: 10.958 min
Delta R.T.: 0.047 min
Response: 18267023
Conc: 1.44 ng/ml