

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110322\
 Data File : PS021025.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Nov 2022 14:51
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 03 17:26:02 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102822.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 31 10:07:57 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.411	6.848	1114.9E6	770.1E6	534.211	556.788
Target Compounds							
1) T	Dalapon	2.521	0.000	512039	0	<MDL	N.D. #
3) T	4-Nitroph...	6.249	0.000	6672993	0	4.437	N.D. #
5) T	DICAMBA	6.625f	7.070f	19559601	5756731	2.214	<MDL #
6) T	MCP	6.783f	7.124	15640912	1211218	2.397	<MDL #
7) T	MCPA	6.783f	0.000	15640912	0	1.667	N.D. #
8) T	DICHLORPROP	0.000	7.668	0	4569378	N.D.	2.967
10) T	Pentachlo...	7.579	0.000	2735440	0	<MDL	N.D. #
11) T	2,4,5-TP ...	8.130	8.691	2249372	7862618	<MDL	<MDL #
12) T	2,4,5-T	8.395	9.119	2046397	1102473	<MDL	<MDL #
13) T	2,4-DB	8.904	9.627	364694	1017469	<MDL	<MDL #
14) T	DINOSEB	9.906	0.000	7947386	0	<MDL	N.D. #
15) T	Picloram	9.760	10.968f	4355657	7018168	<MDL	<MDL #
16) T	DCPA	10.202	0.000	750512	0	<MDL	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110322\
Data File : PS021025.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Nov 2022 14:51
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 03 17:26:02 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102822.M
Quant Title : 8080.M
QLast Update : Mon Oct 31 10:07:57 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

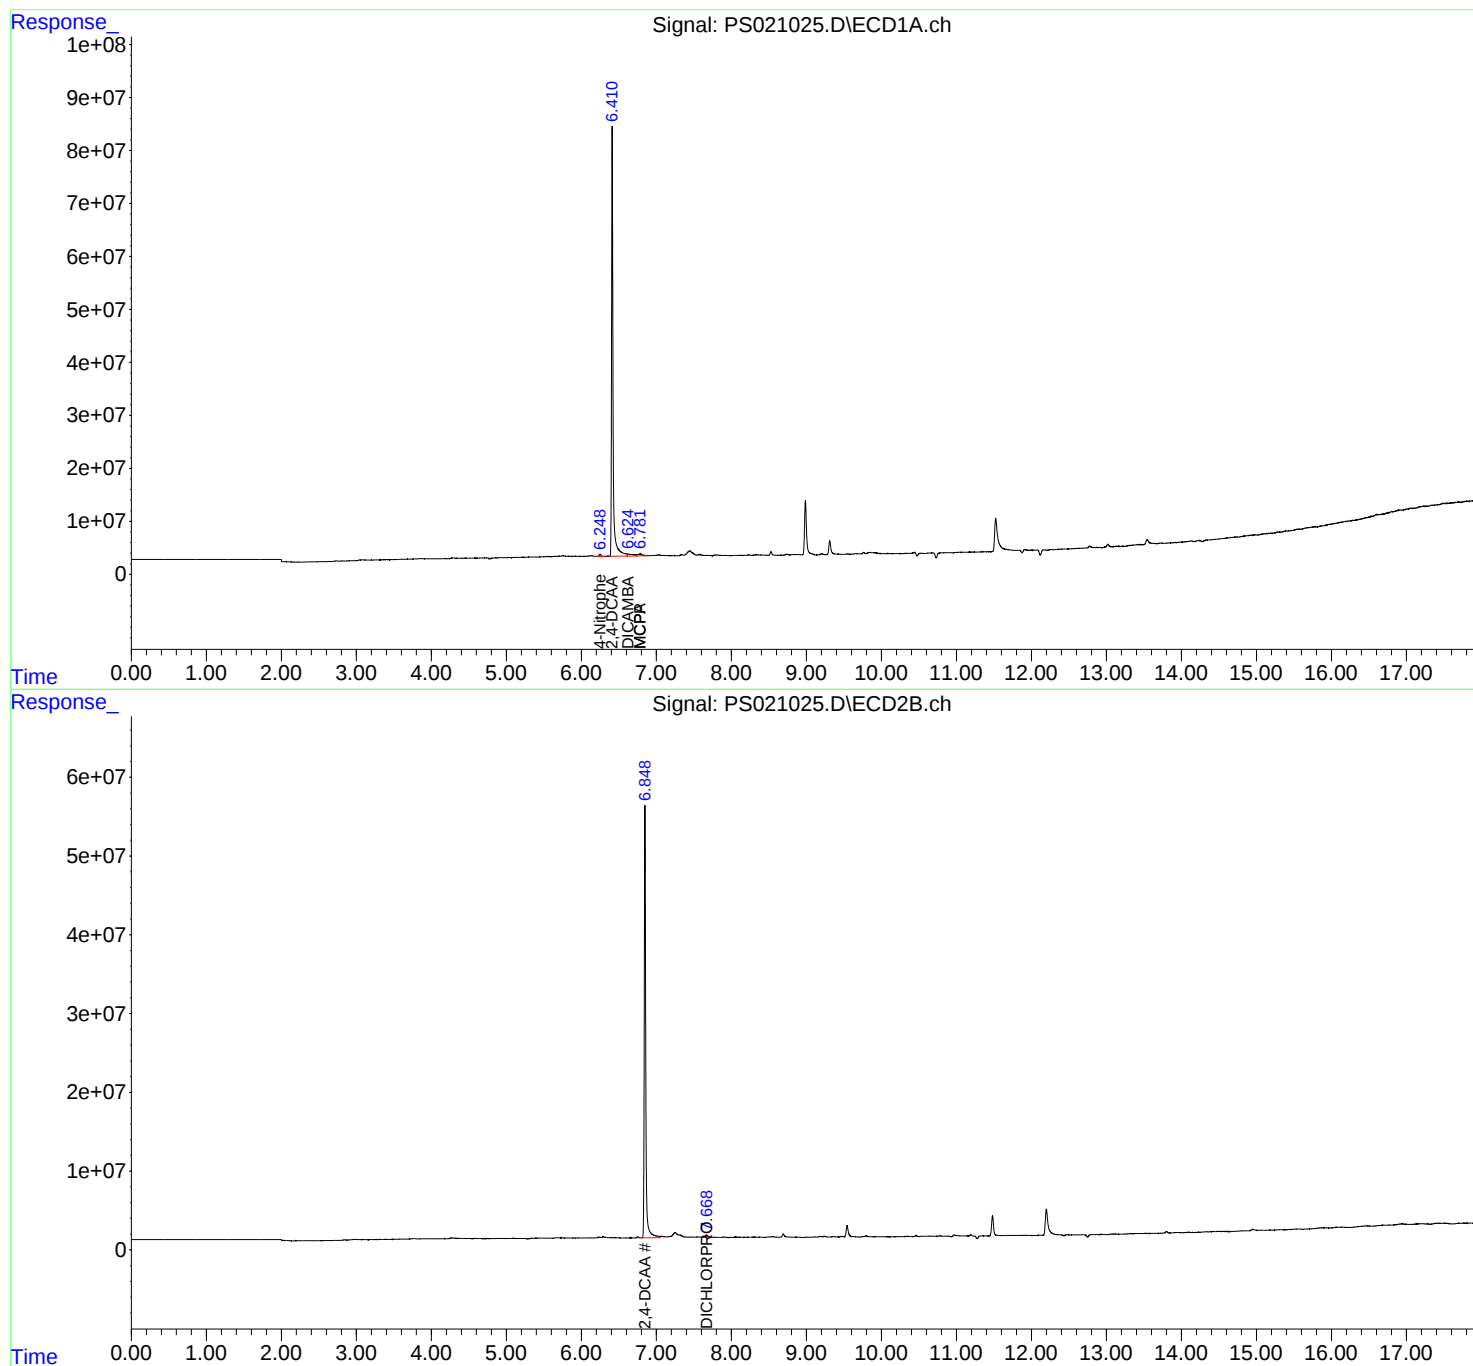


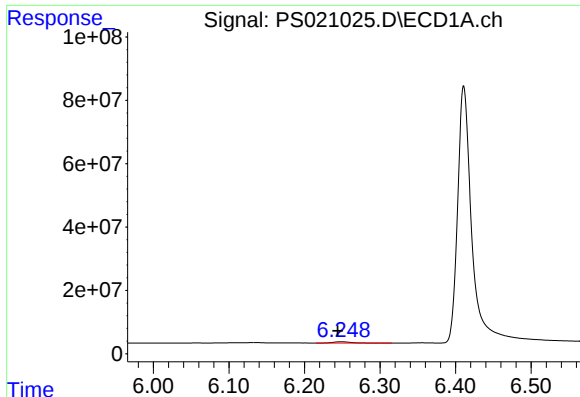

#3 4-Nitrophenol


R.T.: 6.249 min
Delta R.T.: 0.004 min
Response: 6672993
Conc: 4.44 ng/ml

Instrument :
ECD_S
ClientSampleId :

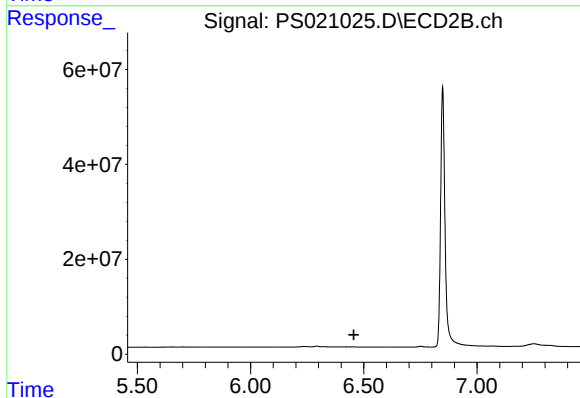


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.456 min
Response: 0
Conc: N.D.

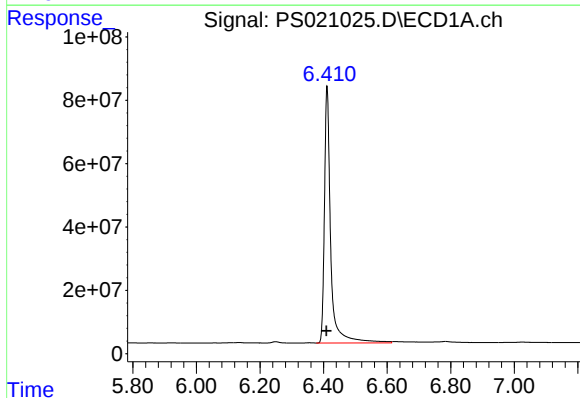


#4 2,4-DCAA

R.T.: 6.411 min
Delta R.T.: 0.002 min
Response: 1114939633
Conc: 534.21 ng/ml

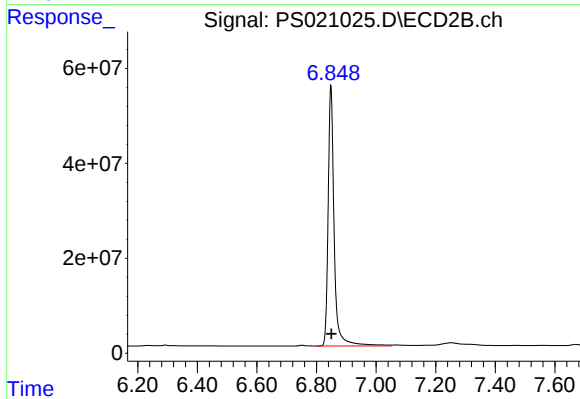

#4 2,4-DCAA


R.T.: 6.848 min
Delta R.T.: -0.002 min
Response: 770119241
Conc: 556.79 ng/ml

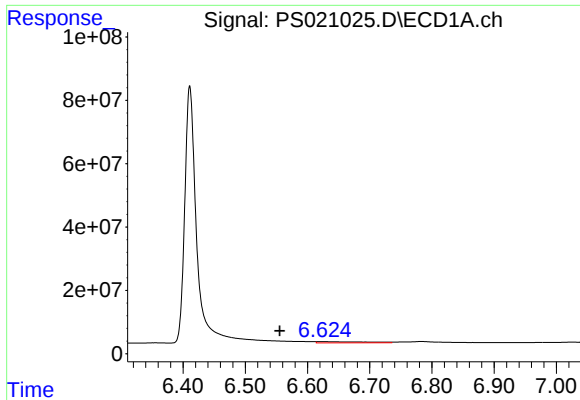

#5 DICAMBA


R.T.: 6.625 min
Delta R.T.: 0.069 min
Response: 19559601
Conc: 2.21 ng/ml

Instrument :
ECD_S
ClientSampleId :

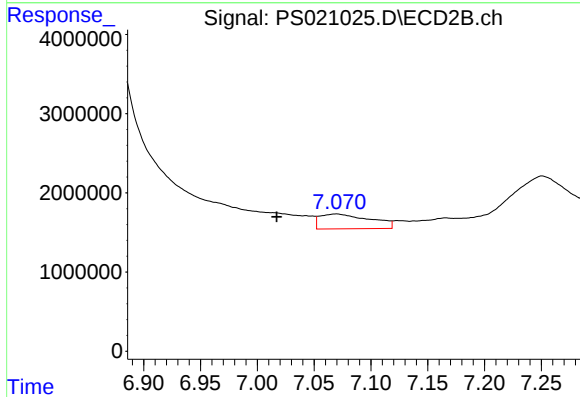


#5 DICAMBA

R.T.: 7.070 min
Delta R.T.: 0.053 min
Response: 5756731
Conc: N.D.

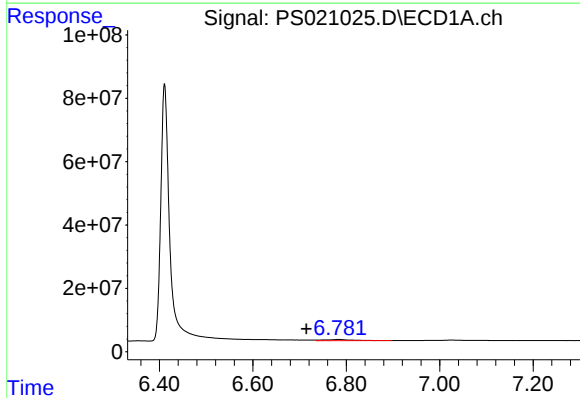


#6 MCP

R.T.: 6.783 min
Delta R.T.: 0.068 min
Response: 15640912
Conc: 2.40 ug/ml

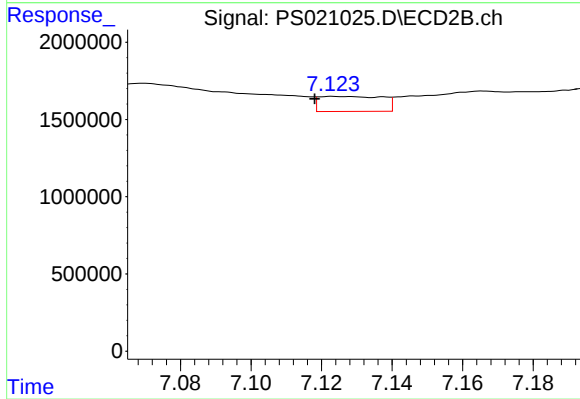

#6 MCP


R.T.: 7.124 min
Delta R.T.: 0.005 min
Response: 1211218
Conc: N.D.

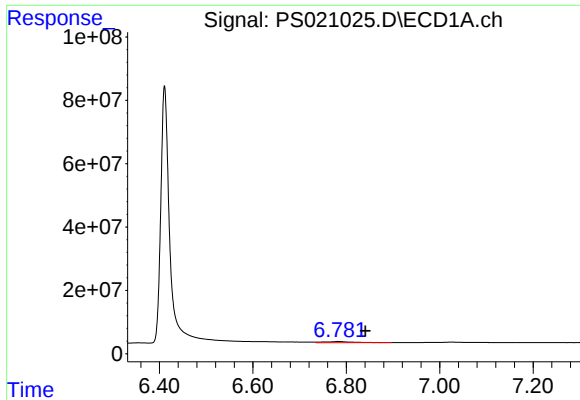

#7 MCPA


R.T.: 6.783 min
Delta R.T.: -0.058 min
Response: 15640912
Conc: 1.67 ug/ml

Instrument :
ECD_S
ClientSampleId :

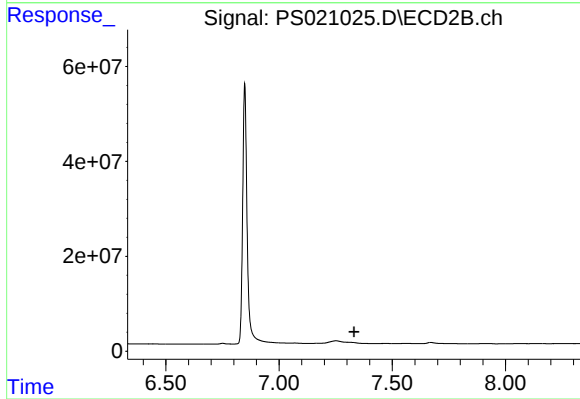


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.331 min
Response: 0
Conc: N.D.

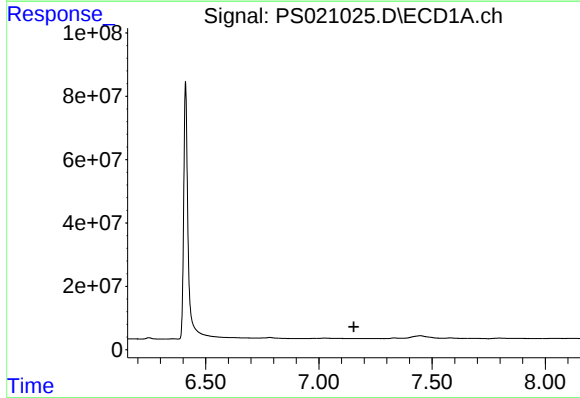

#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 7.154 min
Response: 0
Conc: N.D.

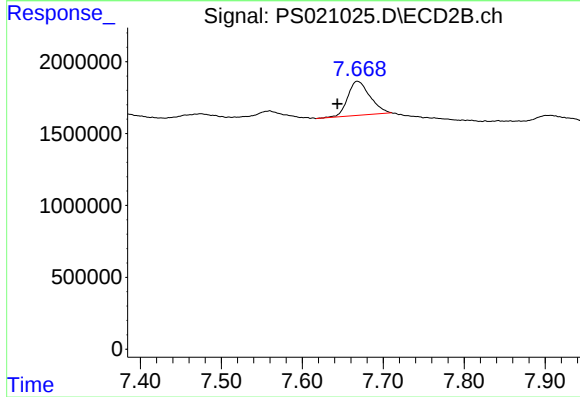

#8 DICHLORPROP

R.T.: 7.668 min
Delta R.T.: 0.025 min
Response: 4569378
Conc: 2.97 ng/ml