

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110323\
 Data File : PS024751.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Nov 2023 11:47
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 03 15:11:54 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110323.M
 Quant Title : 8080.M
 QLast Update : Fri Nov 03 15:07:01 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
1) T	Dalapon	2.515	2.571	10003933	7097706	4.153 6.737 #
2) T	3,5-DICHL...	0.000	6.034f	0	77400	N.D. <MDL
3) T	4-Nitroph...	0.000	6.371	0	1169293	N.D. 2.663
5) T	DICAMBA	0.000	6.931	0	503799	N.D. <MDL
6) T	MCP	0.000	6.966f	0	950658	N.D. <MDL
7) T	MCPA	0.000	7.245	0	8386824	N.D. 2.720
8) T	DICHLORPROP	0.000	7.565	0	806606	N.D. 1.104
9) T	2,4-D	0.000	7.779f	0	535638	N.D. <MDL
11) T	2,4,5-TP ...	0.000	8.613	0	515150	N.D. <MDL
12) T	2,4,5-T	0.000	9.030f	0	4820825	N.D. 1.208
15) T	Picloram	9.681	10.772	37484806	14569786	2.107 2.398
16) T	DCPA	10.154f	10.772	11279376	14569786	<MDL 2.899 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110323\
Data File : PS024751.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Nov 2023 11:47
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 03 15:11:54 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110323.M
Quant Title : 8080.M
QLast Update : Fri Nov 03 15:07:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

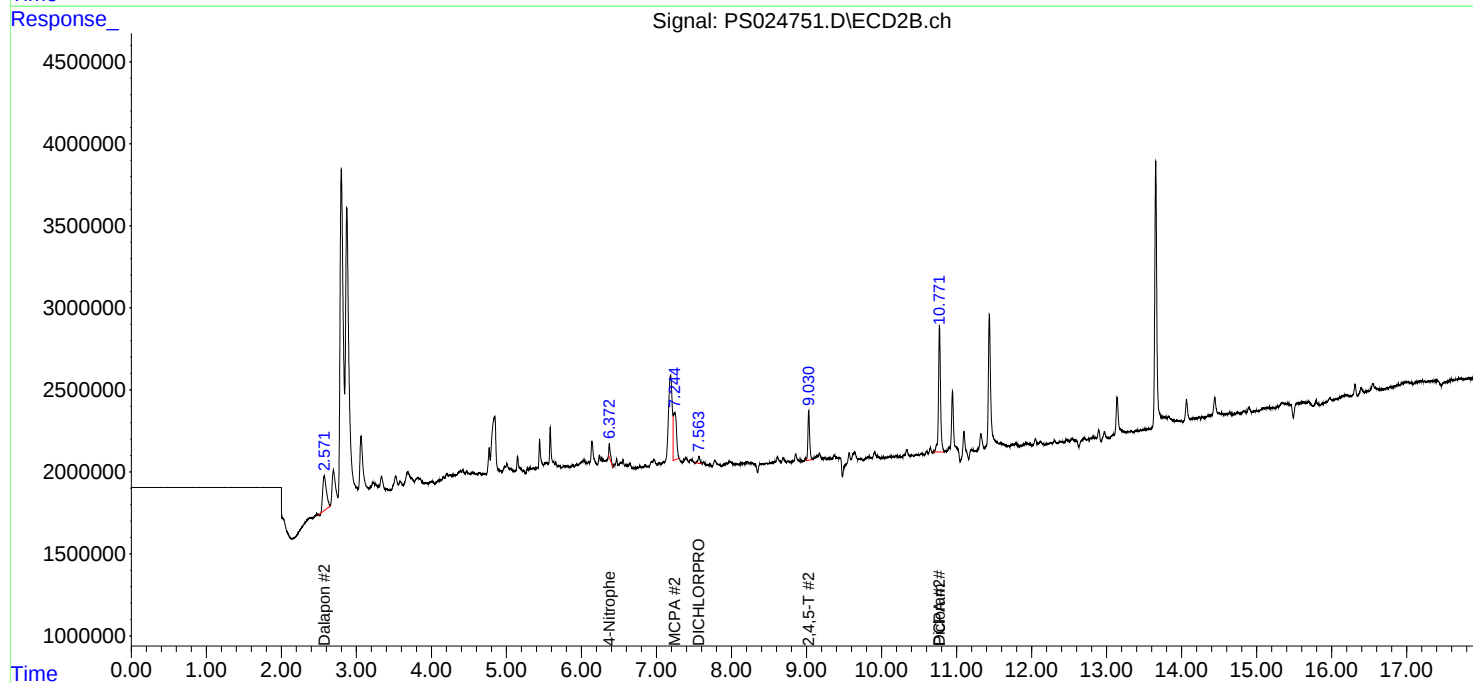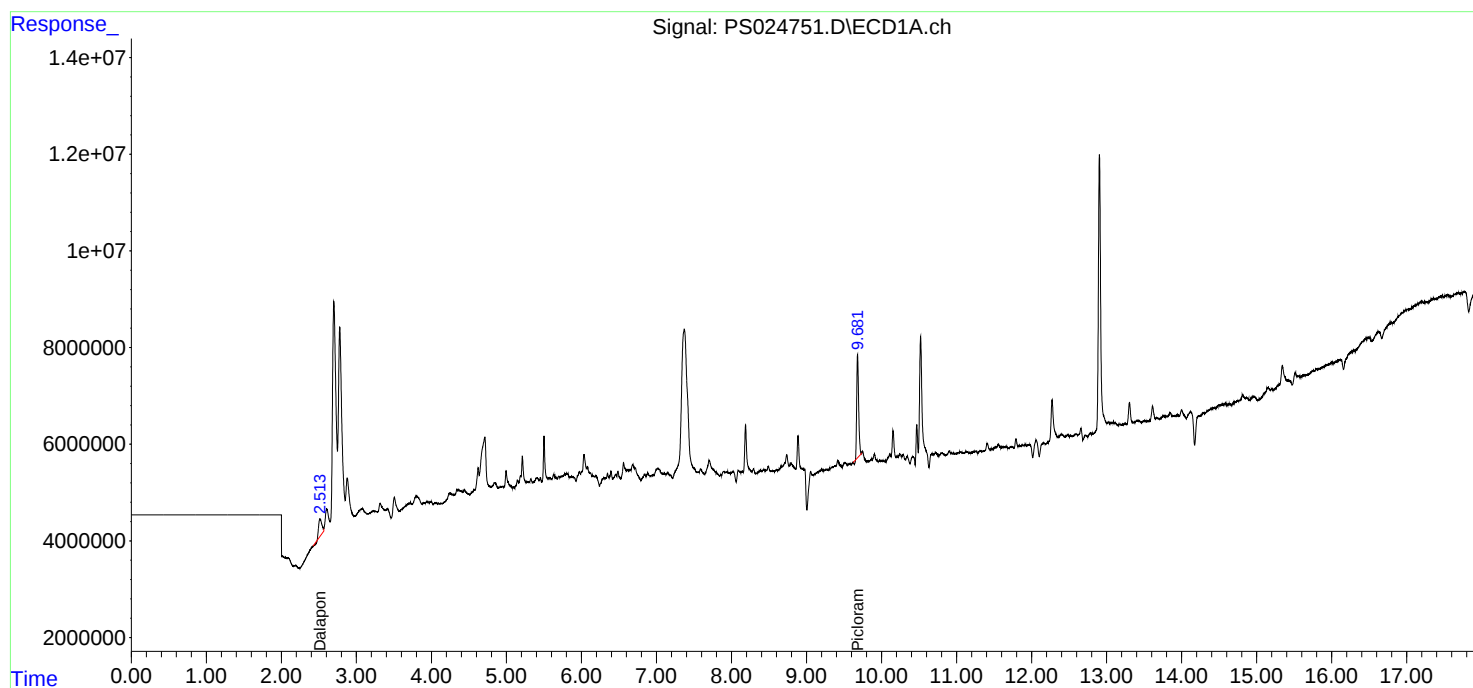


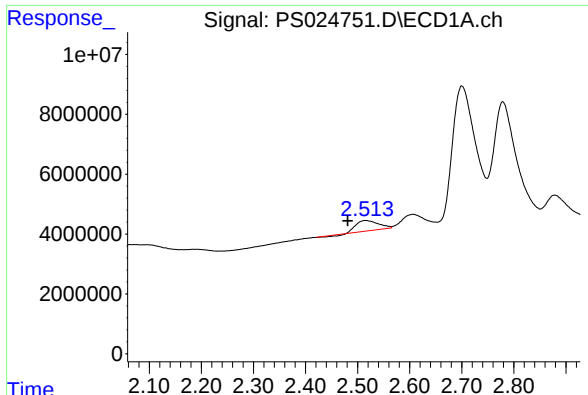

#1 Dalapon


R.T.: 2.515 min
Delta R.T.: 0.034 min
Response: 10003933
Conc: 4.15 ng/ml

Instrument :
ECD_S
ClientSampleId :

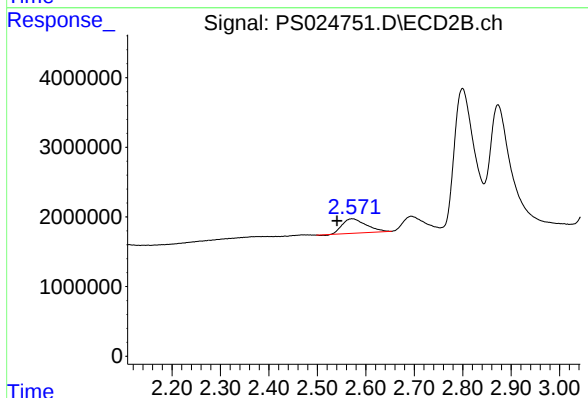


#1 Dalapon

R.T.: 2.571 min
Delta R.T.: 0.031 min
Response: 7097706
Conc: 6.74 ng/ml

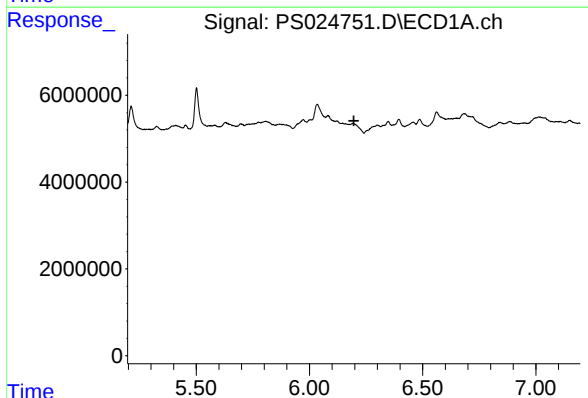


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.196 min
Response: 0
Conc: N.D.

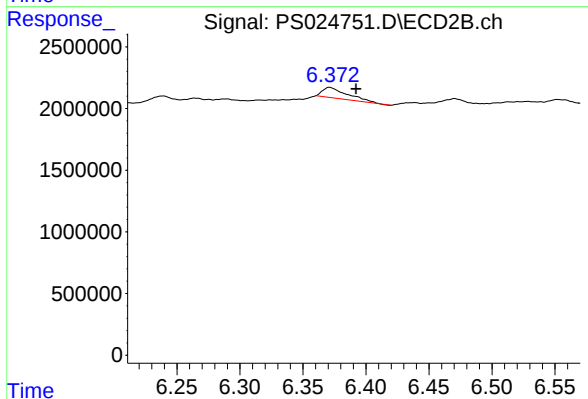

#3 4-Nitrophenol


R.T.: 6.371 min
Delta R.T.: -0.021 min
Response: 1169293
Conc: 2.66 ng/ml

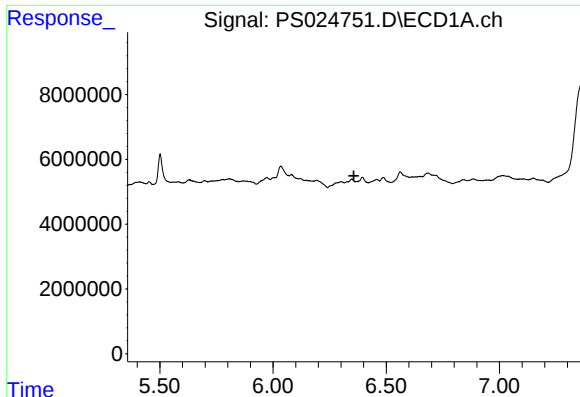

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 6.357 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

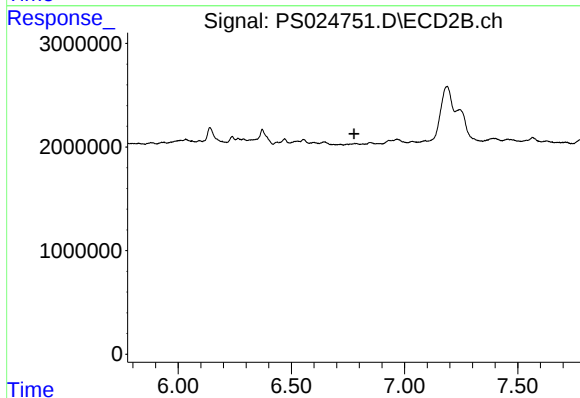


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 6.777 min
Response: 0
Conc: N.D.

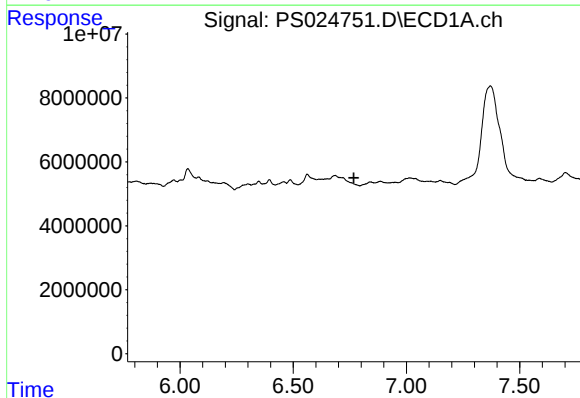


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 6.768 min
Response: 0
Conc: N.D.

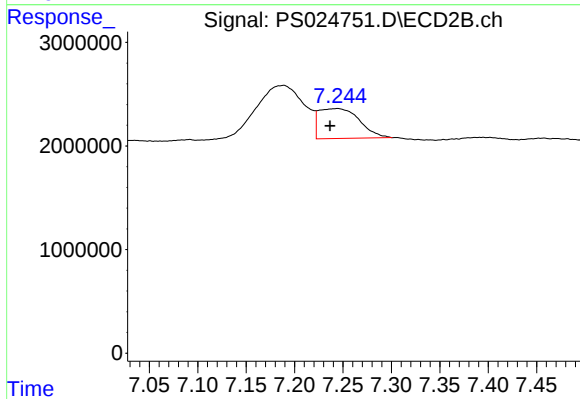

#7 MCPA


R.T.: 7.245 min
Delta R.T.: 0.008 min
Response: 8386824
Conc: 2.72 ug/ml

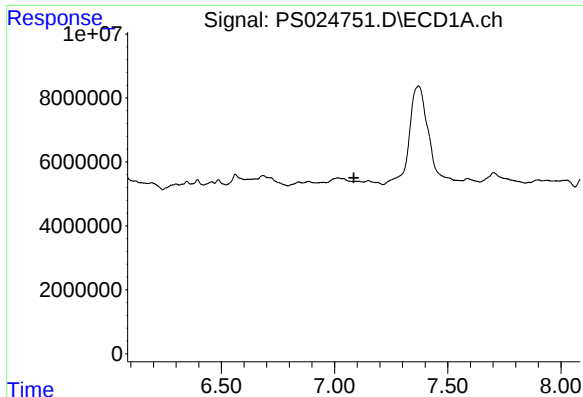

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 7.085 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

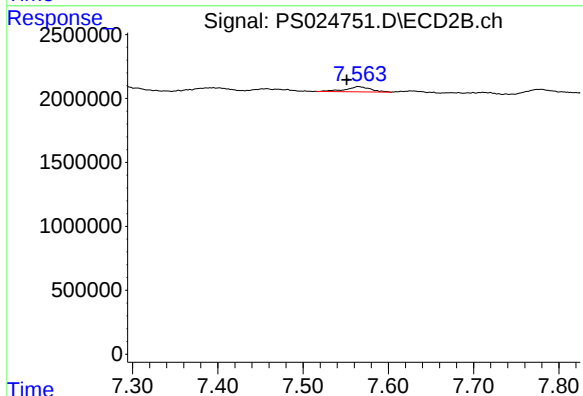


#8 DICHLORPROP

R.T.: 7.565 min
Delta R.T.: 0.013 min
Response: 806606
Conc: 1.10 ng/ml

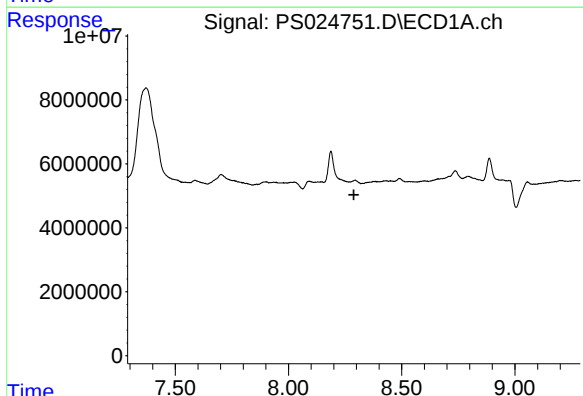


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 8.289 min
Response: 0
Conc: N.D.

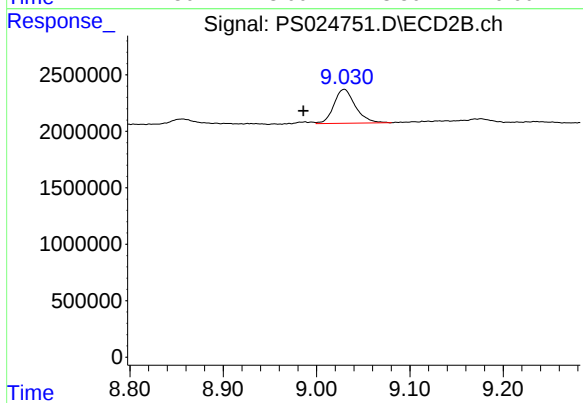

#12 2,4,5-T


R.T.: 9.030 min
Delta R.T.: 0.044 min
Response: 4820825
Conc: 1.21 ng/ml

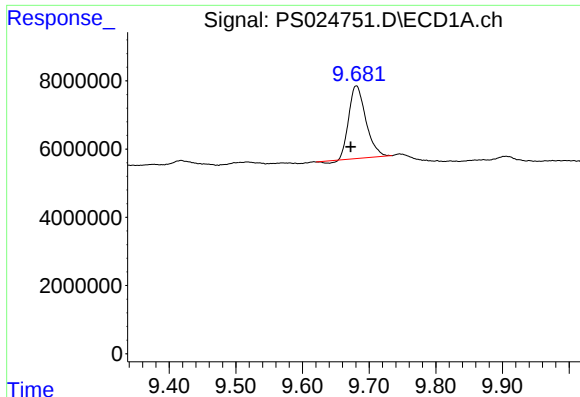

#15 Picloram


R.T.: 9.681 min
Delta R.T.: 0.008 min
Response: 37484806
Conc: 2.11 ng/ml

Instrument :
ECD_S
ClientSampleId :

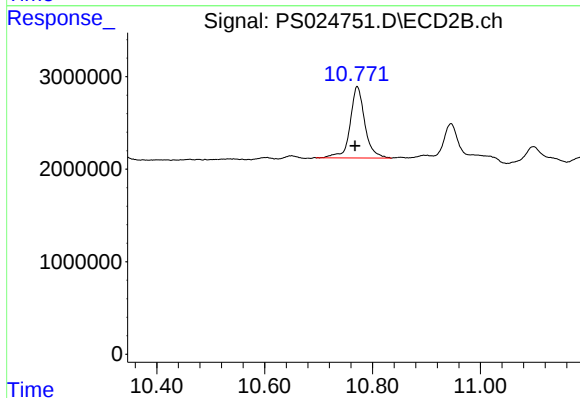


#15 Picloram

R.T.: 10.772 min
Delta R.T.: 0.004 min
Response: 14569786
Conc: 2.40 ng/ml

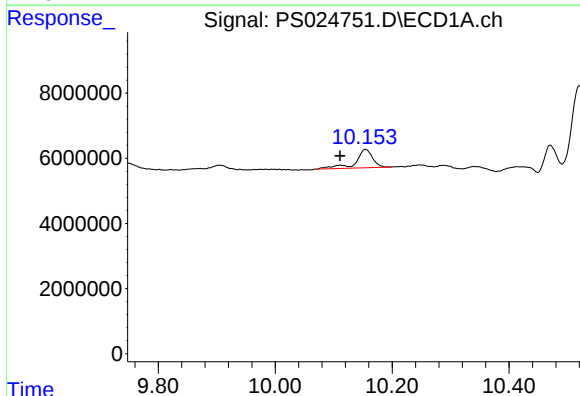

#16 DCPA

R.T.: 10.154 min
Delta R.T.: 0.044 min
Response: 11279376
Conc: N.D.

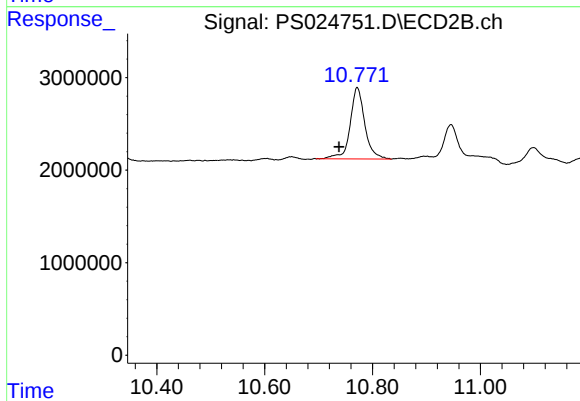

#16 DCPA

R.T.: 10.772 min
Delta R.T.: 0.034 min
Response: 14569786
Conc: 2.90 ng/ml