

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110325\
 Data File : PS032232.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Nov 2025 12:11
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 04 05:39:07 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110325.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 04 04:59:50 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml	

System Monitoring Compounds								
4) S	2,4-DCAA	7.290	7.628	1621.7E6	1871.5E6	357.891	513.367	#
Target Compounds								
2) T	3,5-DICHL...	6.448	0.000	2970640	0	<MDL	N.D.	#
3) T	4-Nitroph...	7.127f	0.000	38545	0	<MDL	N.D.	#
7) T	MCPA	7.798	8.112f	547296	1729276	<MDL	<MDL	#
8) T	DICHLORPROP	8.180	0.000	1687711	0	<MDL	N.D.	#
10) T	Pentachlo...	8.714	9.372	29107186	23615172	<MDL	<MDL	#
11) T	2,4,5-TP ...	9.250f	9.781f	887377	12631627	<MDL	<MDL	#
12) T	2,4,5-T	9.549f	10.143f	319480	2908153	<MDL	<MDL	#
13) T	2,4-DB	10.168	0.000	187847	0	<MDL	N.D.	#
14) T	DINOSEB	11.357	11.124	57639008	11105703	2.770	<MDL	#
15) T	Picloram	11.160	0.000	4549274	0	<MDL	N.D.	#
16) T	DCPA	11.654	12.151	25408779	27755971	<MDL	<MDL	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110325\
Data File : PS032232.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Nov 2025 12:11
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 04 05:39:07 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110325.M
Quant Title : 8080.M
QLast Update : Tue Nov 04 04:59:50 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

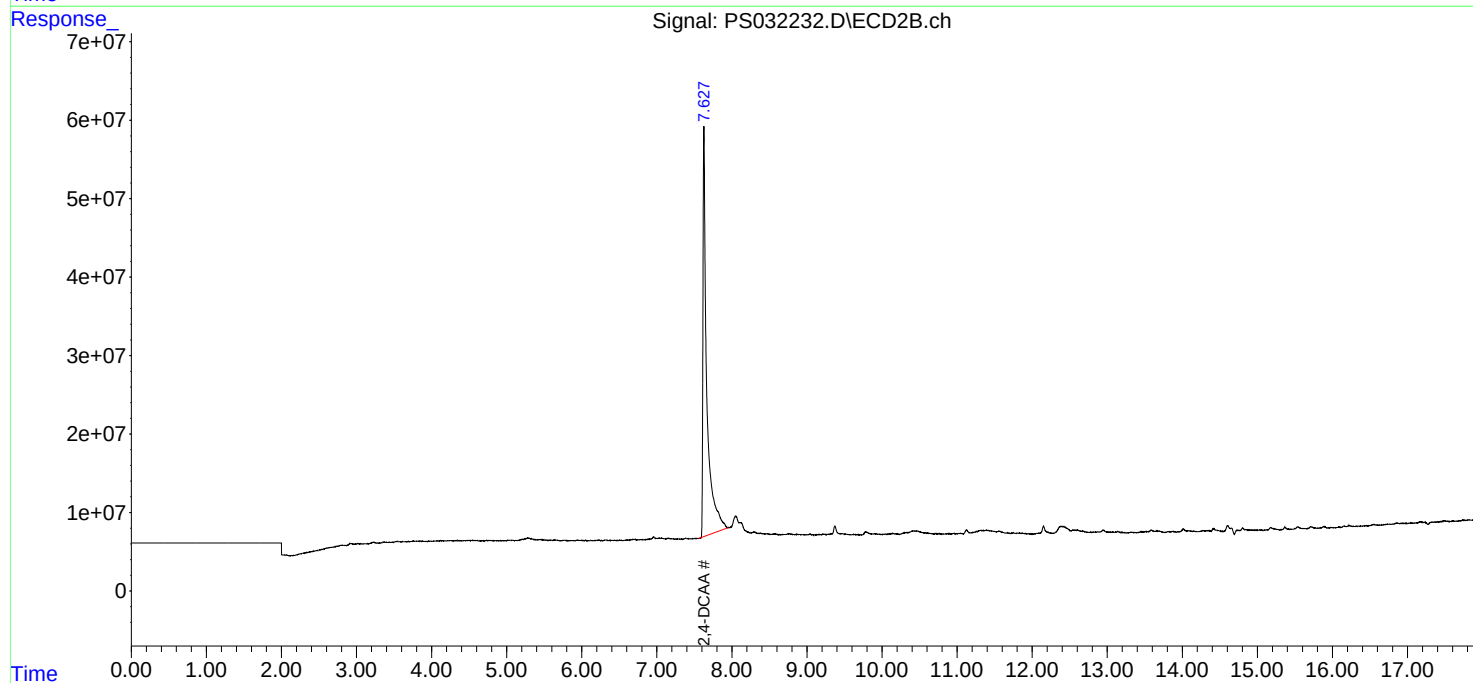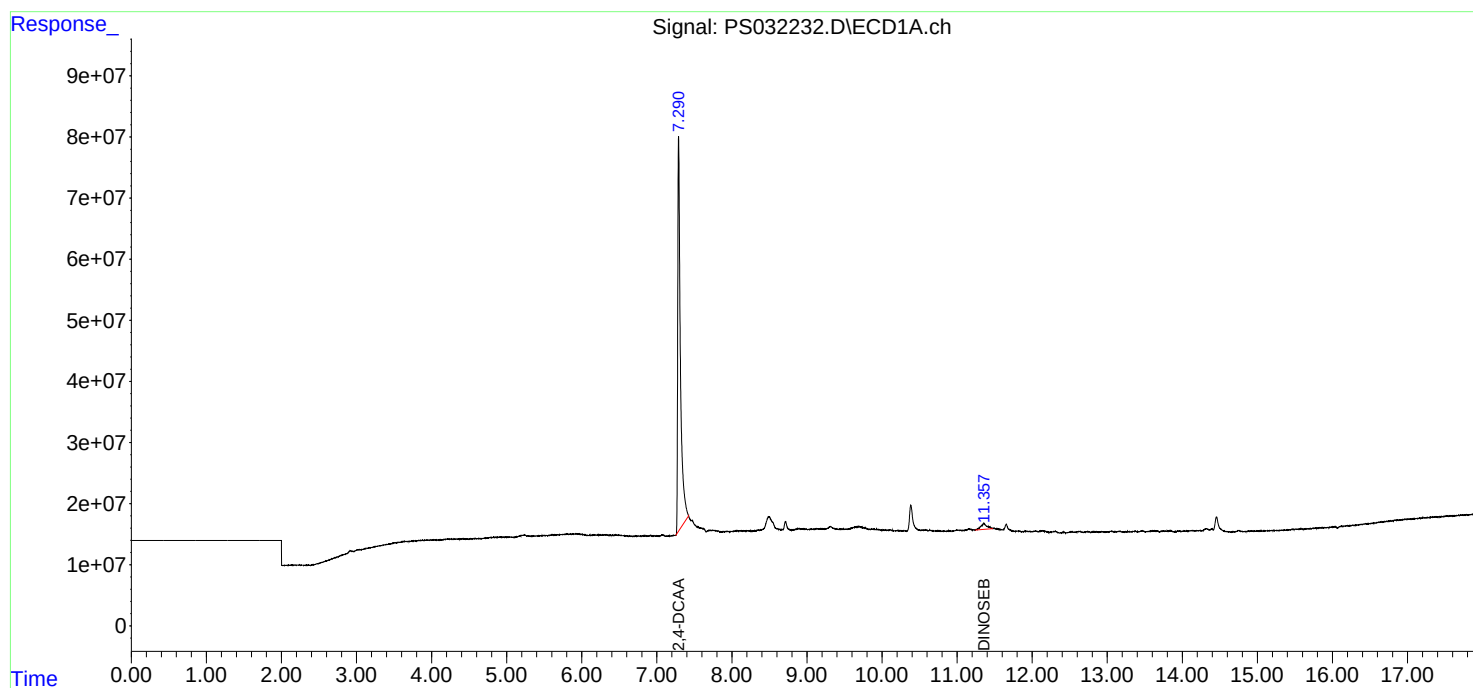


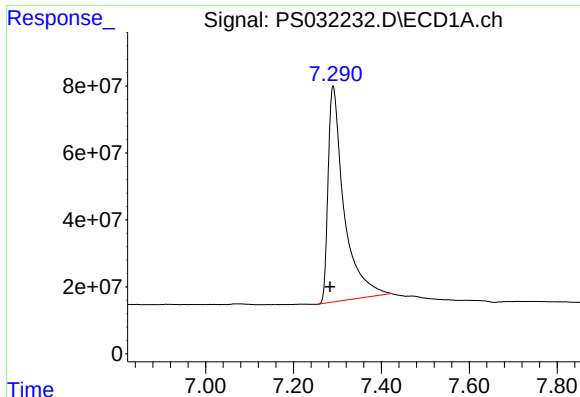

#4 2,4-DCAA


R.T.: 7.290 min
Delta R.T.: 0.007 min
Response: 1621704278
Conc: 357.89 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

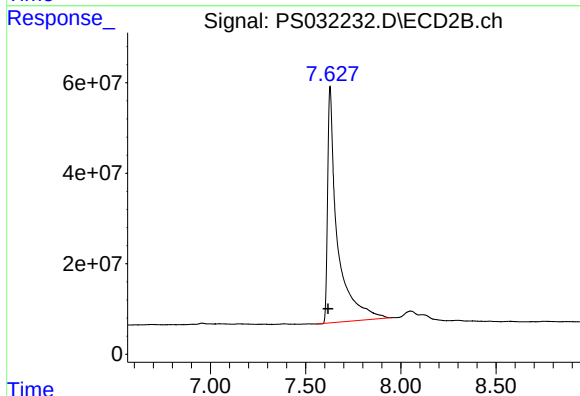


#4 2,4-DCAA

R.T.: 7.628 min
Delta R.T.: 0.011 min
Response: 1871478621
Conc: 513.37 ng/ml

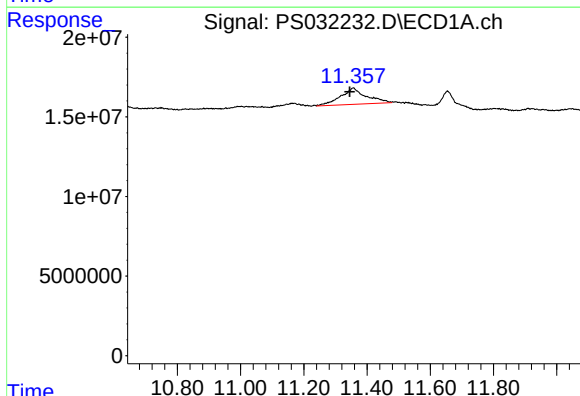

#14 DINOSEB

R.T.: 11.357 min
Delta R.T.: 0.012 min
Response: 57639008
Conc: 2.77 ng/ml

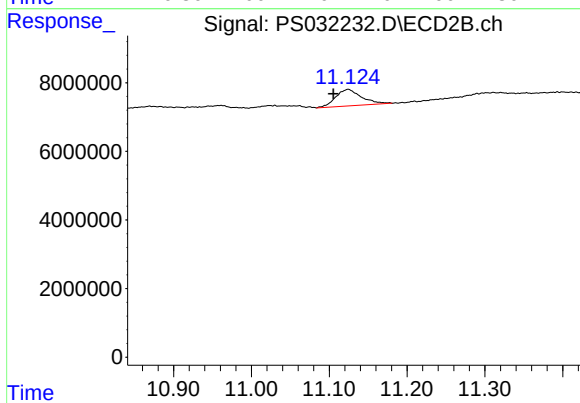

#14 DINOSEB

R.T.: 11.124 min
Delta R.T.: 0.019 min
Response: 11105703
Conc: N.D.