

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110325\
 Data File : PS032239.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Nov 2025 15:00
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 04 05:40:04 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110325.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 04 04:59:50 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml	

System Monitoring Compounds								
4) S	2,4-DCAA	7.288	7.626	1684.5E6	1847.3E6	371.746	506.744	#
Target Compounds								
2) T	3,5-DICHL...	6.449	0.000	195307	0	<MDL	N.D.	#
3) T	4-Nitroph...	7.069f	0.000	2330480	0	1.736	N.D.	#
7) T	MCPA	7.772	8.107f	281776	2345087	<MDL	<MDL	#
8) T	DICHLORPROP	8.205f	0.000	2321386	0	<MDL	N.D.	#
10) T	Pentachlo...	8.714	9.372	10550993	11839729	<MDL	<MDL	#
11) T	2,4,5-TP ...	9.299	9.788f	10052515	3569983	<MDL	<MDL	#
12) T	2,4,5-T	9.593	10.196	2330741	4277683	<MDL	<MDL	#
13) T	2,4-DB	10.112f	10.758	3055007	5230998	1.159	1.387	
14) T	DINOSEB	11.346	0.000	11828839	0	<MDL	N.D.	#
15) T	Picloram	11.163	0.000	1078998	0	<MDL	N.D.	#
16) T	DCPA	11.651	12.150	7187999	5425431	<MDL	<MDL	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110325\
Data File : PS032239.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Nov 2025 15:00
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 04 05:40:04 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110325.M
Quant Title : 8080.M
QLast Update : Tue Nov 04 04:59:50 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

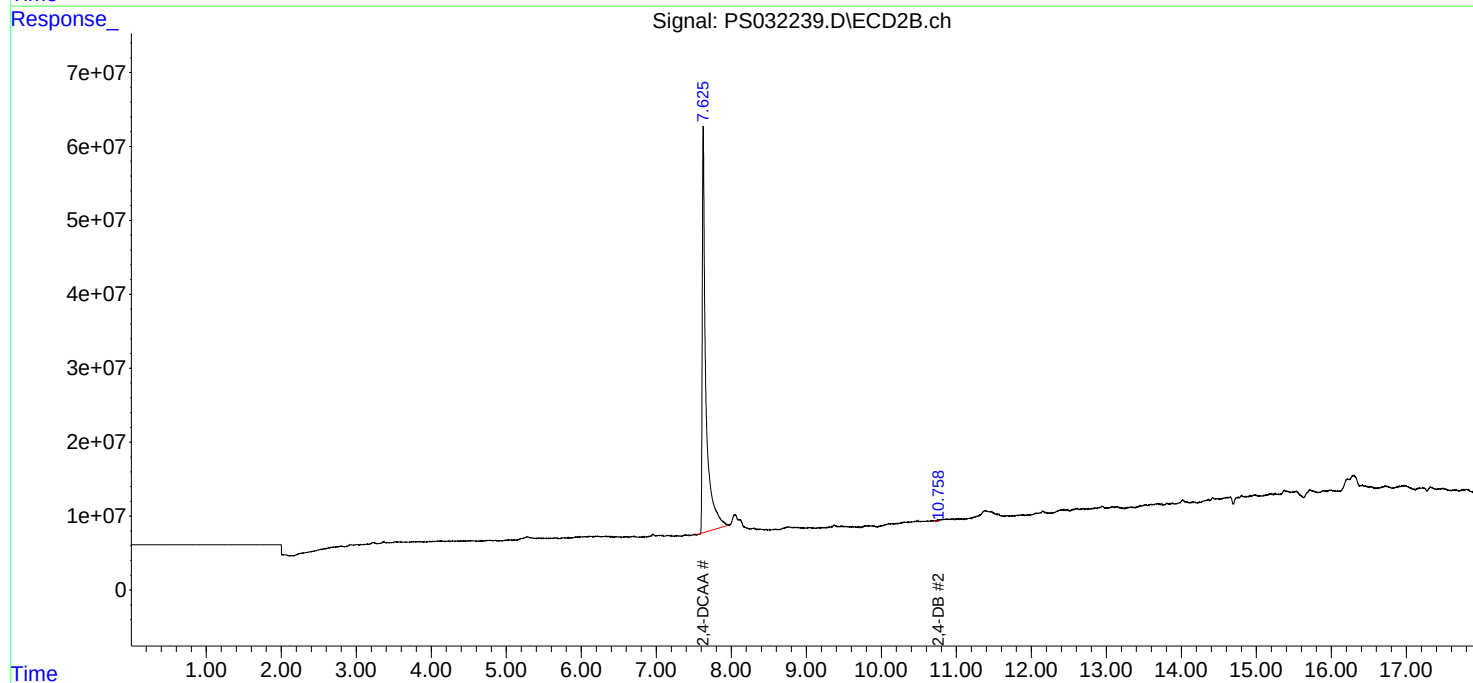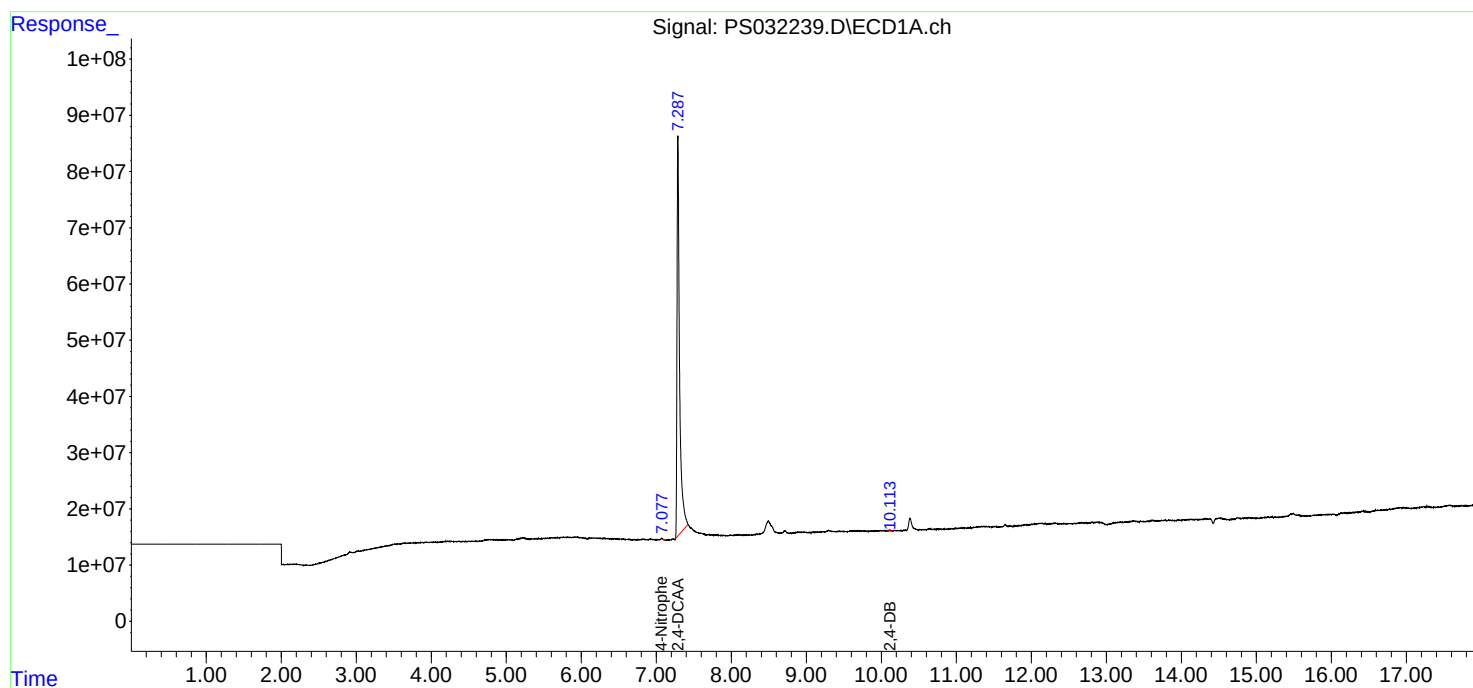


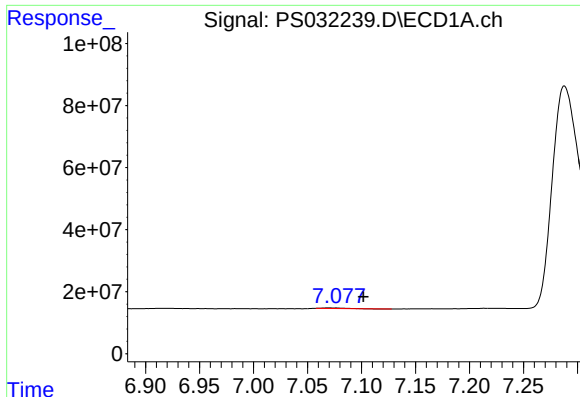

#3 4-Nitrophenol


R.T.: 7.069 min
Delta R.T.: -0.033 min
Response: 2330480
Conc: 1.74 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

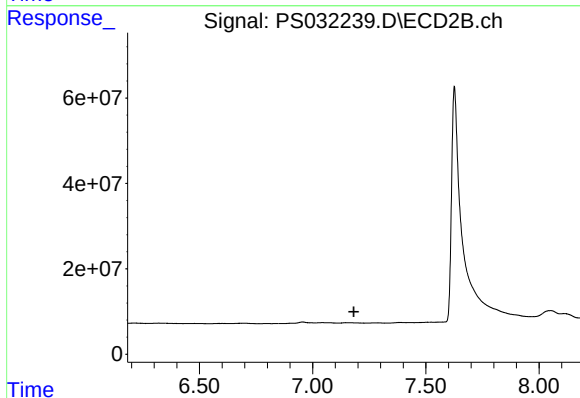


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 7.182 min
Response: 0
Conc: N.D.

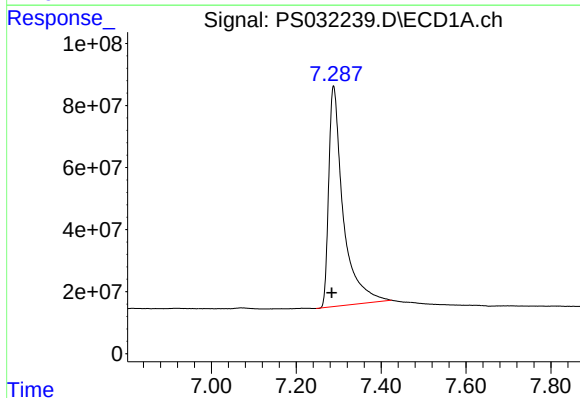


#4 2,4-DCAA

R.T.: 7.288 min
Delta R.T.: 0.005 min
Response: 1684481986
Conc: 371.75 ng/ml

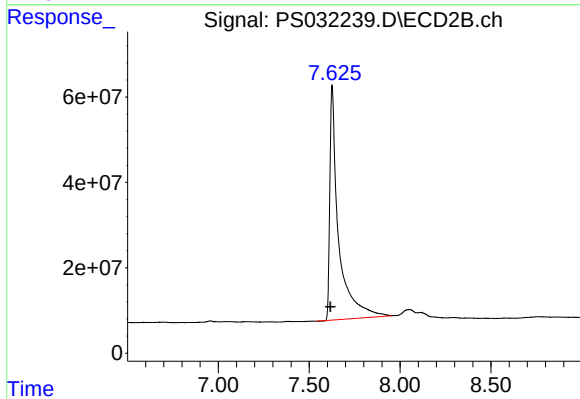

#4 2,4-DCAA


R.T.: 7.626 min
Delta R.T.: 0.009 min
Response: 1847333048
Conc: 506.74 ng/ml

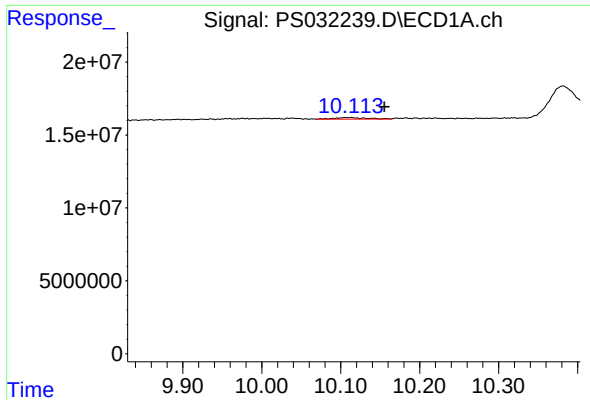

#13 2,4-DB

R.T.: 10.112 min
Delta R.T.: -0.043 min
Response: 3055007
Conc: 1.16 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

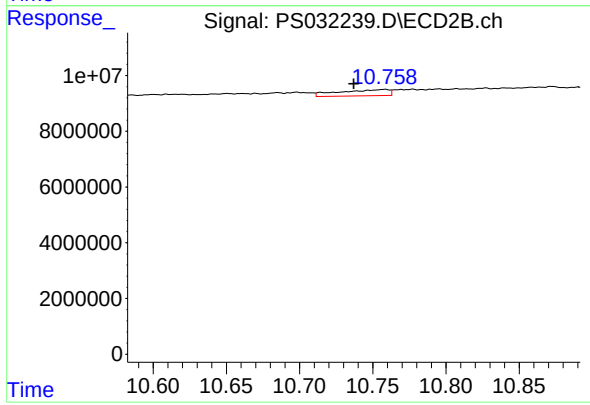

#13 2,4-DB

R.T.: 10.758 min
Delta R.T.: 0.021 min
Response: 5230998
Conc: 1.39 ng/ml