

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110325\
 Data File : PS032251.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Nov 2025 19:49
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 04 05:41:56 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110325.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 04 04:59:50 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml	

System Monitoring Compounds								
4) S	2,4-DCAA	7.287	7.625	1699.8E6	1872.7E6	375.124	513.701	#
Target Compounds								
1) T	Dalapon	2.699f	0.000	47519742	0	6.619	N.D.	#
2) T	3,5-DICHL...	6.449	0.000	1299937	0	<MDL	N.D.	#
3) T	4-Nitroph...	7.075f	0.000	2437388	0	1.816	N.D.	#
7) T	MCPA	7.795	0.000	246176	0	<MDL	N.D.	#
8) T	DICHLORPROP	8.183	0.000	491471	0	<MDL	N.D.	#
9) T	2,4-D	8.383f	0.000	201482	0	<MDL	N.D.	#
10) T	Pentachlo...	8.725	9.373	3168395	6952048	<MDL	<MDL	#
11) T	2,4,5-TP ...	9.286	0.000	4277701	0	<MDL	N.D.	#
12) T	2,4,5-T	9.582	10.190	470425	1311518	<MDL	<MDL	#
13) T	2,4-DB	10.154	0.000	2299343	0	<MDL	N.D.	#
14) T	DINOSEB	11.358	0.000	1617739	0	<MDL	N.D.	#
15) T	Picloram	11.157f	12.242	320402	1529231	<MDL	<MDL	#
16) T	DCPA	11.650	12.187f	2433442	5533437	<MDL	<MDL	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110325\
Data File : PS032251.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Nov 2025 19:49
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 04 05:41:56 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110325.M
Quant Title : 8080.M
QLast Update : Tue Nov 04 04:59:50 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

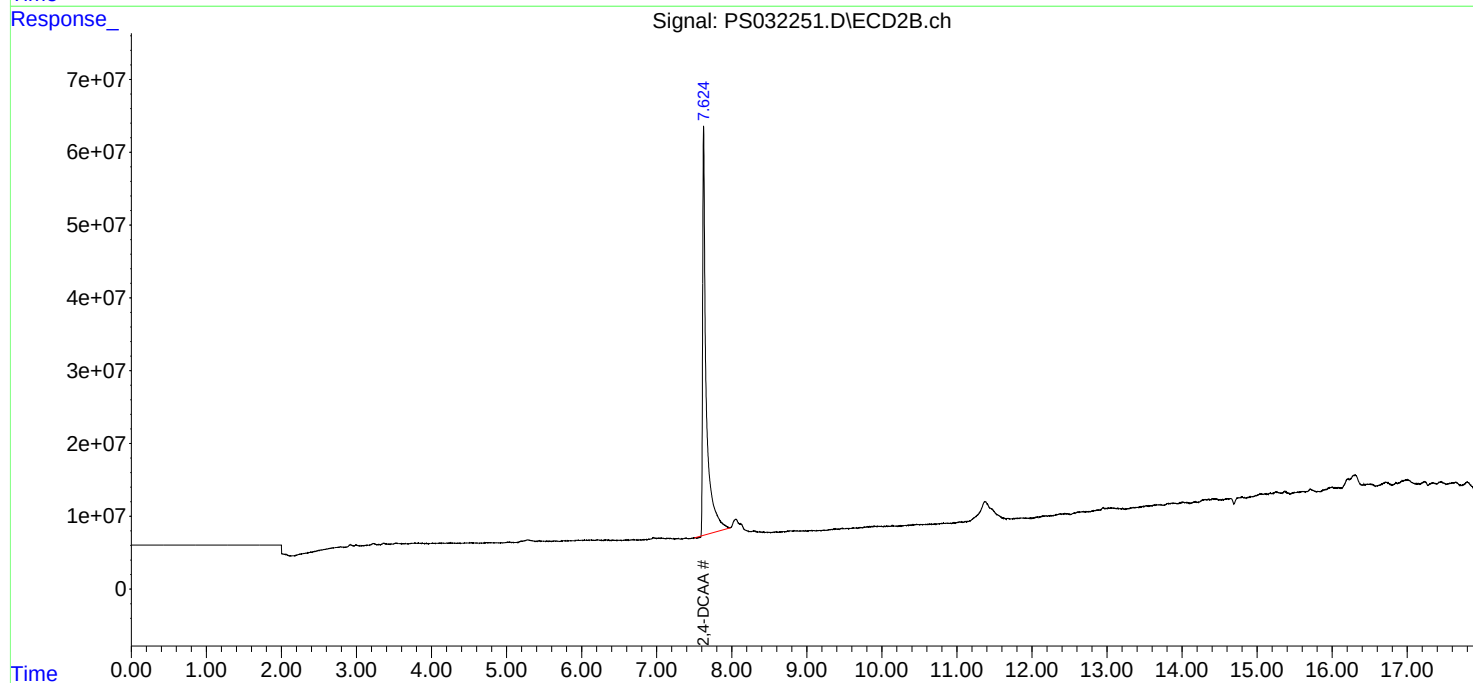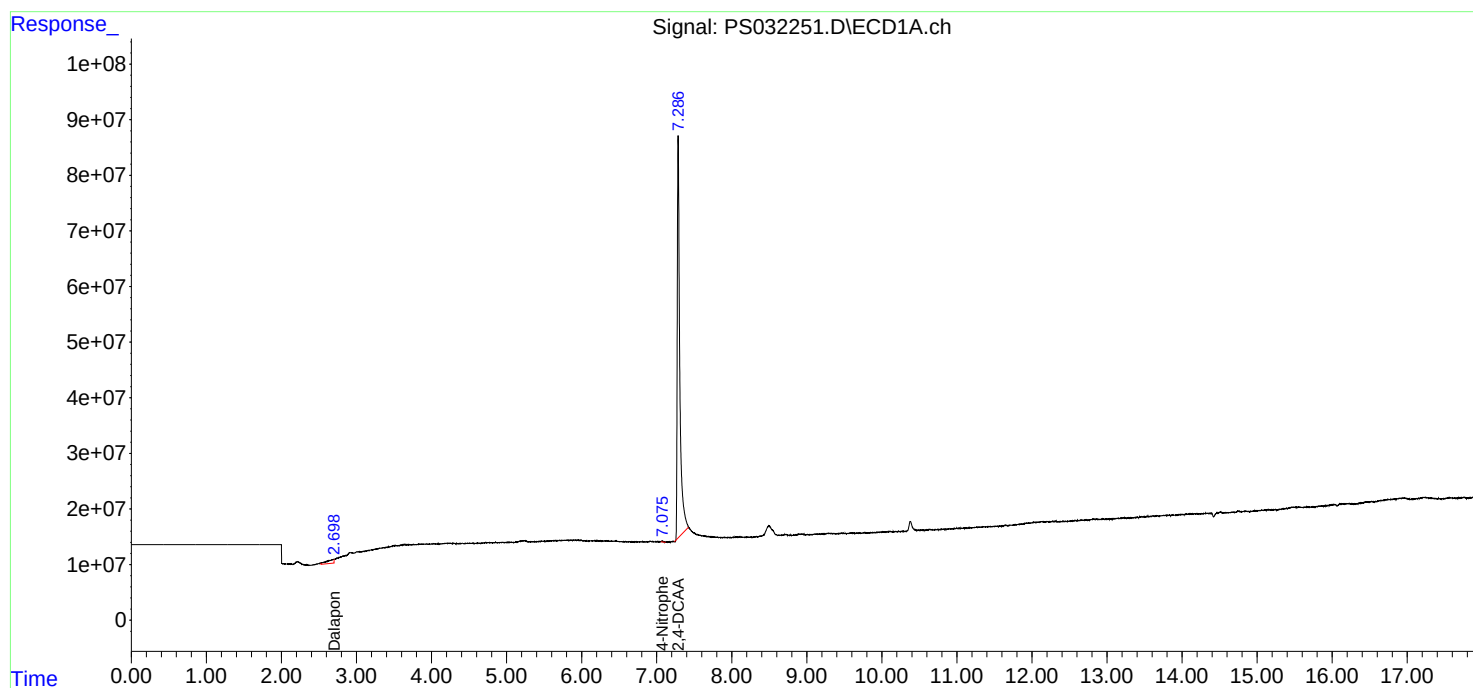


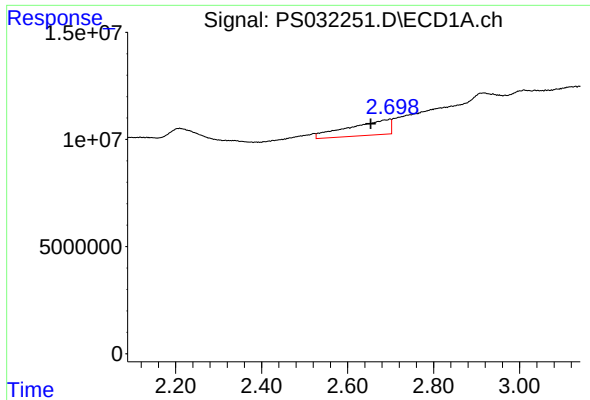

#1 Dalapon


R.T.: 2.699 min
Delta R.T.: 0.045 min
Response: 47519742
Conc: 6.62 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

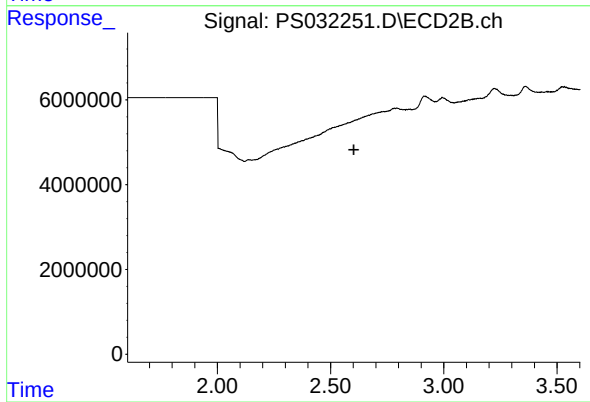


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.603 min
Response: 0
Conc: N.D.

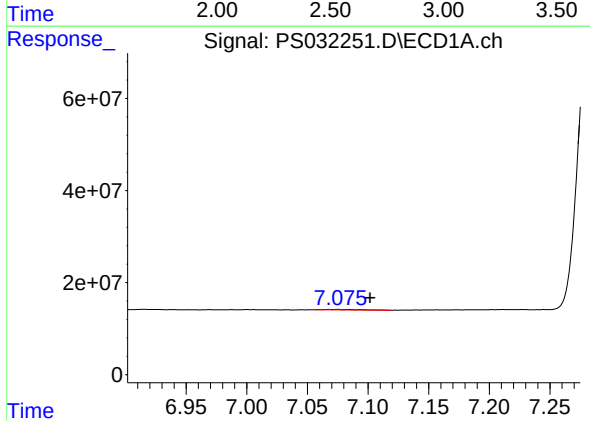


#3 4-Nitrophenol

R.T.: 7.075 min
Delta R.T.: -0.027 min
Response: 2437388
Conc: 1.82 ng/ml

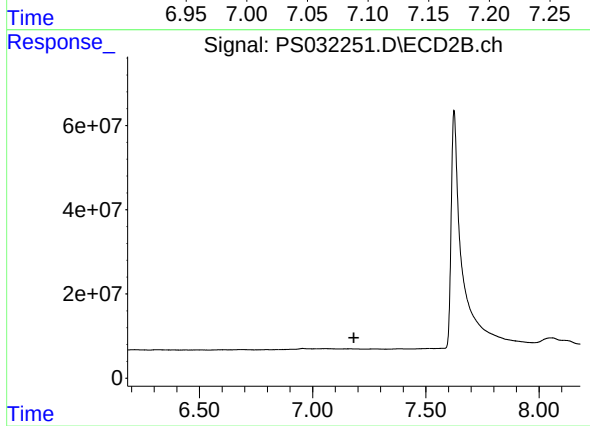

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 7.182 min
Response: 0
Conc: N.D.

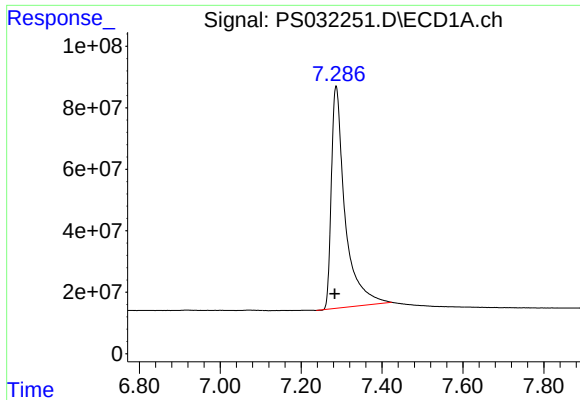

#4 2,4-DCAA

R.T.: 7.287 min
Delta R.T.: 0.003 min
Response: 1699791472
Conc: 375.12 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

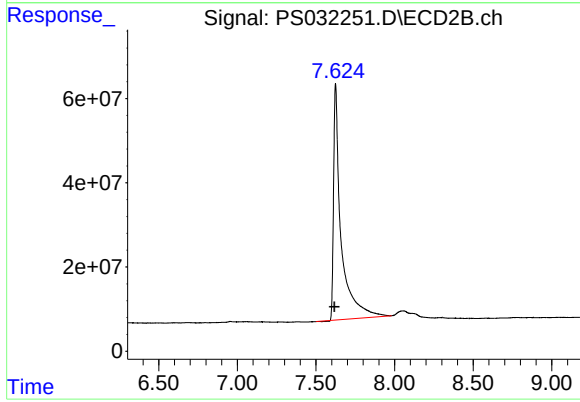

#4 2,4-DCAA

R.T.: 7.625 min
Delta R.T.: 0.007 min
Response: 1872695090
Conc: 513.70 ng/ml