

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110325\
 Data File : PS032263.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Nov 2025 01:51
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 04 05:44:32 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110325.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 04 04:59:50 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.282	7.619	1715.2E6	1791.8E6	378.515	491.514 #
Target Compounds							
2) T	3,5-DICHL...	6.451	0.000	2334620	0	<MDL	N.D. #
3) T	4-Nitroph...	7.075f	0.000	1266001	0	<MDL	N.D. #
6) T	MCP	7.680f	0.000	99434	0	<MDL	N.D. #
7) T	MCPA	7.798	0.000	504917	0	<MDL	N.D. #
8) T	DICHLORPROP	8.190	8.494f	7242430	42947918	1.628	9.005 #
10) T	Pentachlo...	8.715	9.404f	2534229	14683819	<MDL	<MDL #
11) T	2,4,5-TP ...	9.286	9.714f	18668400	39151471	<MDL	1.458 #
12) T	2,4,5-T	9.598	10.167	1817277	28905320	<MDL	1.219 #
13) T	2,4-DB	10.122f	0.000	15169104	0	5.757	N.D. #
14) T	DINOSEB	11.351	11.117	135.2E6	1541734	6.497	<MDL #
15) T	Picloram	11.187	0.000	399.0E6	0	18.798	N.D. #
16) T	DCPA	11.652	12.114f	-1117752	13468353	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110325\
Data File : PS032263.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Nov 2025 01:51
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 04 05:44:32 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110325.M
Quant Title : 8080.M
QLast Update : Tue Nov 04 04:59:50 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

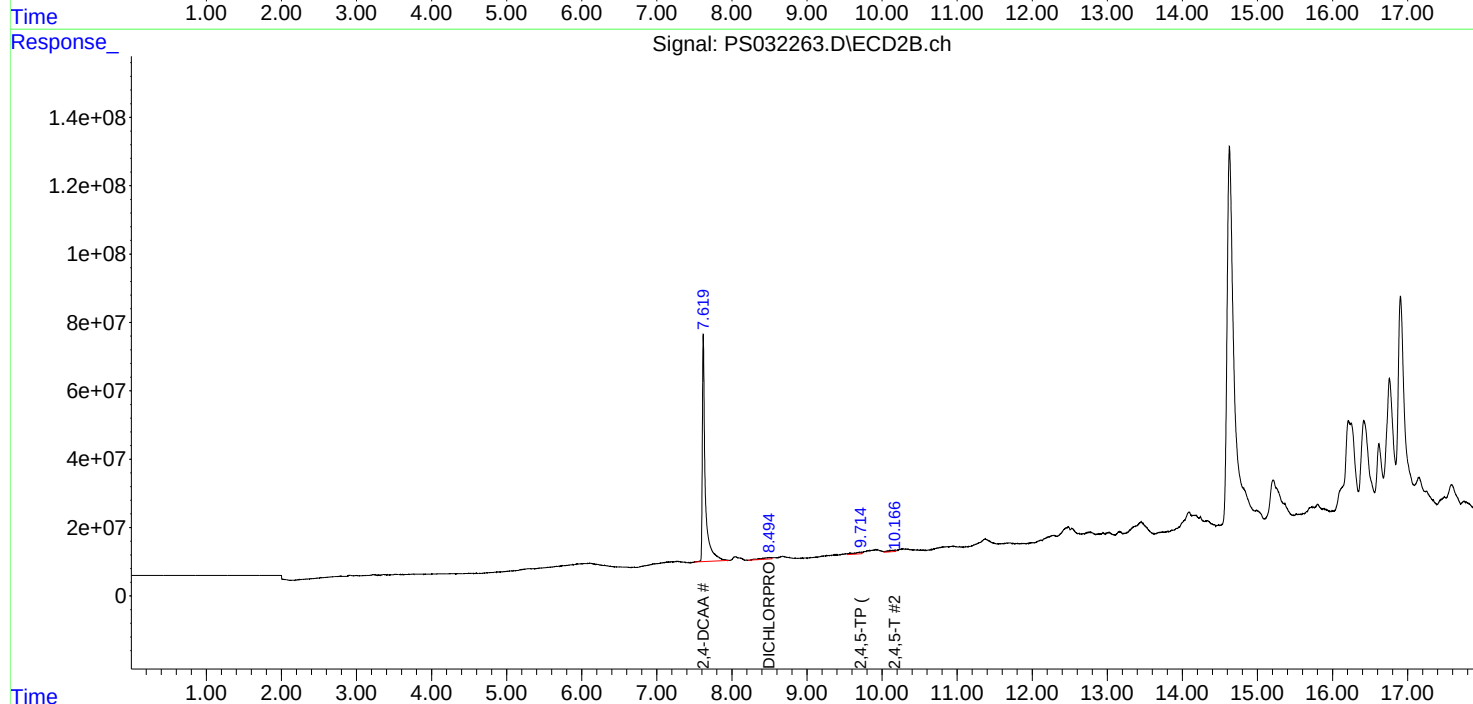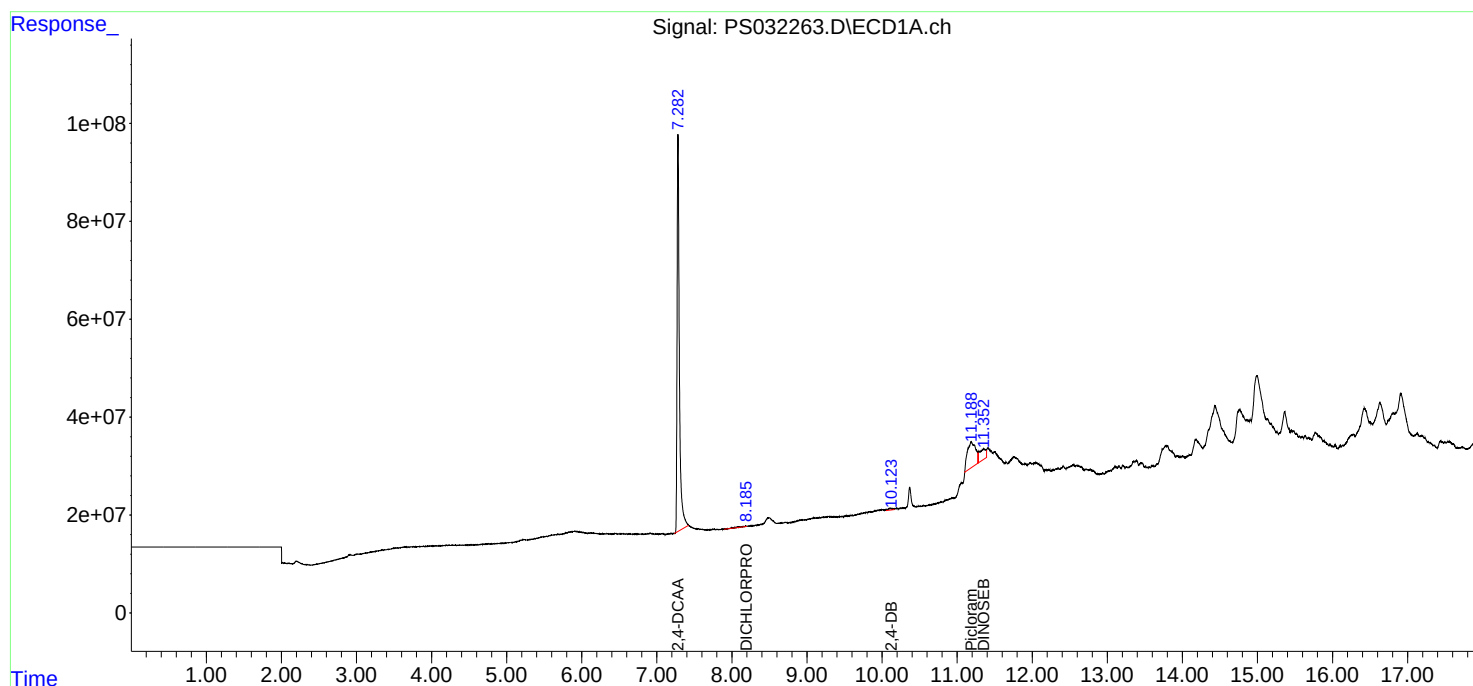


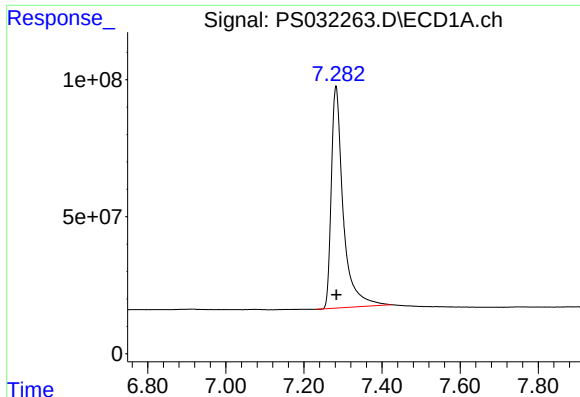

#4 2,4-DCAA


R.T.: 7.282 min
Delta R.T.: -0.001 min
Response: 1715157312
Conc: 378.52 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

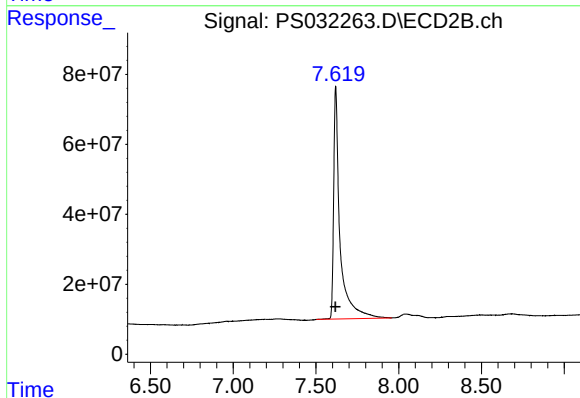


#4 2,4-DCAA

R.T.: 7.619 min
Delta R.T.: 0.002 min
Response: 1791812410
Conc: 491.51 ng/ml

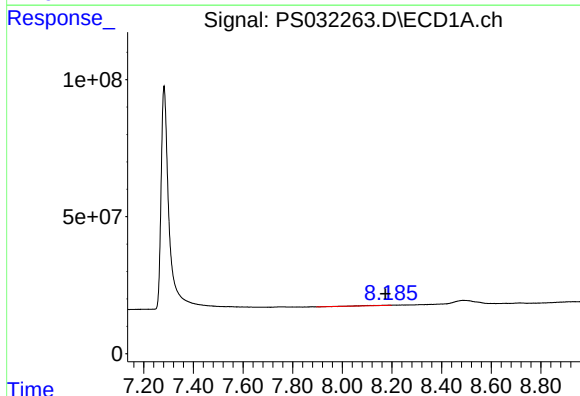


#8 DICHLORPROP

R.T.: 8.190 min
Delta R.T.: 0.016 min
Response: 7242430
Conc: 1.63 ng/ml

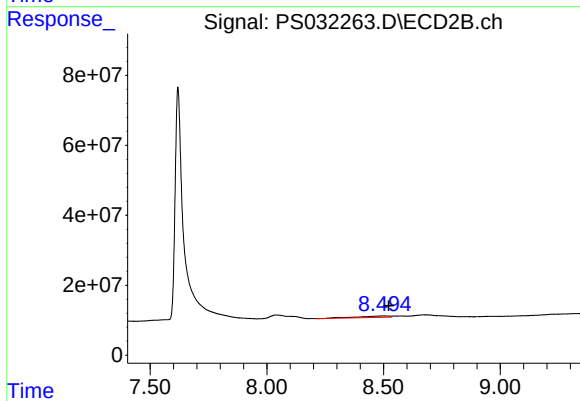

#8 DICHLORPROP


R.T.: 8.494 min
Delta R.T.: -0.027 min
Response: 42947918
Conc: 9.01 ng/ml

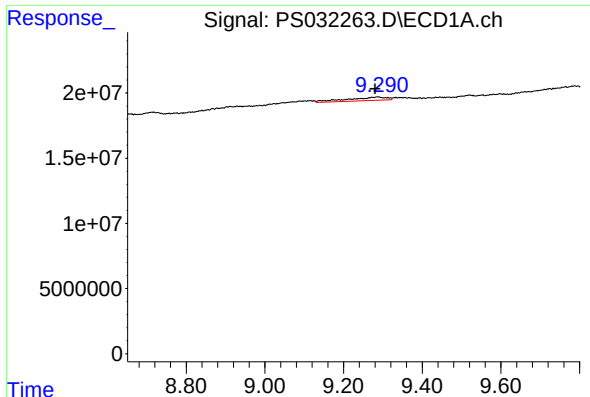

#11 2,4,5-TP (SILVEX)


R.T.: 9.286 min
Delta R.T.: 0.006 min
Response: 18668400
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

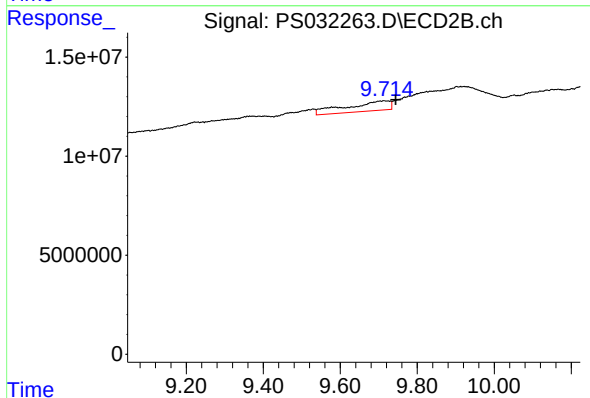


#11 2,4,5-TP (SILVEX)

R.T.: 9.714 min
Delta R.T.: -0.030 min
Response: 39151471
Conc: 1.46 ng/ml

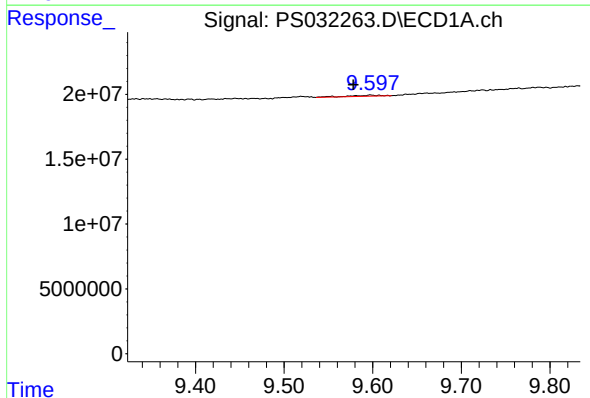


#12 2,4,5-T

R.T.: 9.598 min
Delta R.T.: 0.019 min
Response: 1817277
Conc: N.D.

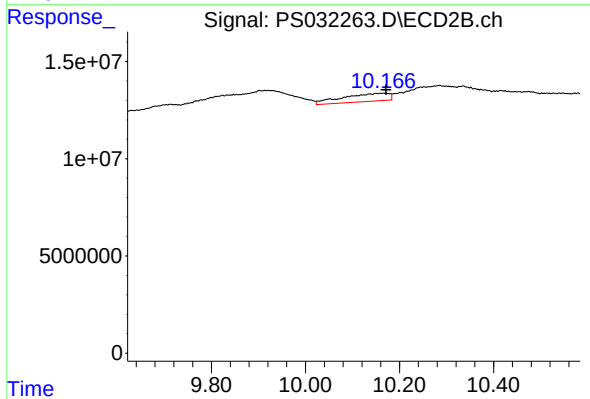

#12 2,4,5-T


R.T.: 10.167 min
Delta R.T.: -0.005 min
Response: 28905320
Conc: 1.22 ng/ml

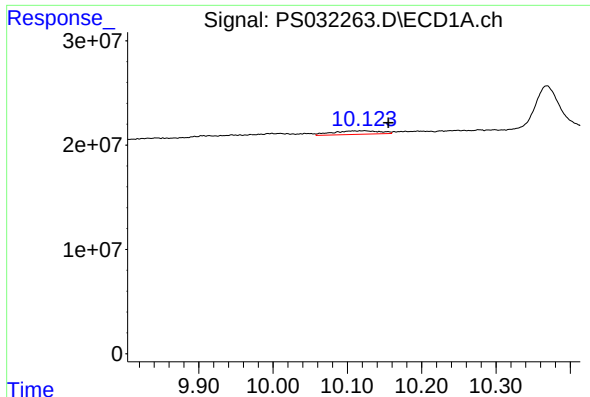

#13 2,4-DB


R.T.: 10.122 min
Delta R.T.: -0.033 min
Response: 15169104
Conc: 5.76 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

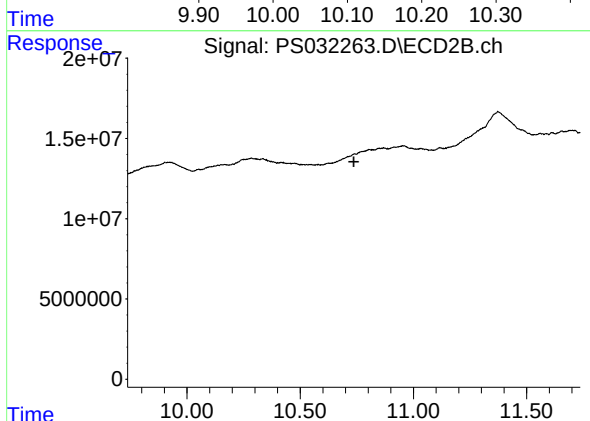


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 10.737 min
Response: 0
Conc: N.D.

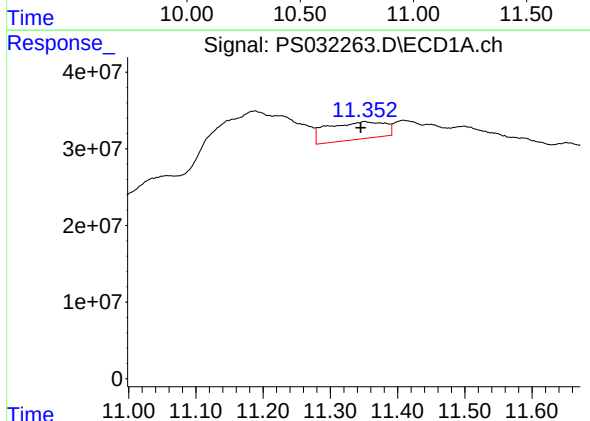


#14 DINOSEB

R.T.: 11.351 min
Delta R.T.: 0.006 min
Response: 135178240
Conc: 6.50 ng/ml

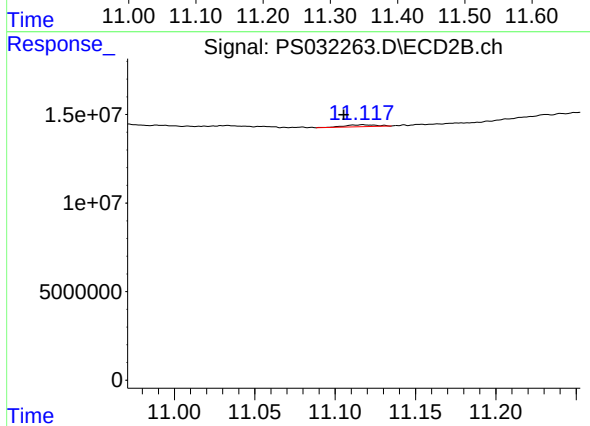

#14 DINOSEB


R.T.: 11.117 min
Delta R.T.: 0.012 min
Response: 1541734
Conc: N.D.

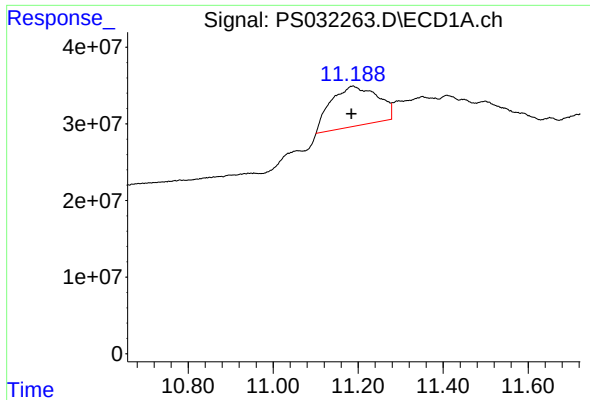

#15 Picloram

R.T.: 11.187 min
Delta R.T.: 0.003 min
Response: 398990060
Conc: 18.80 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

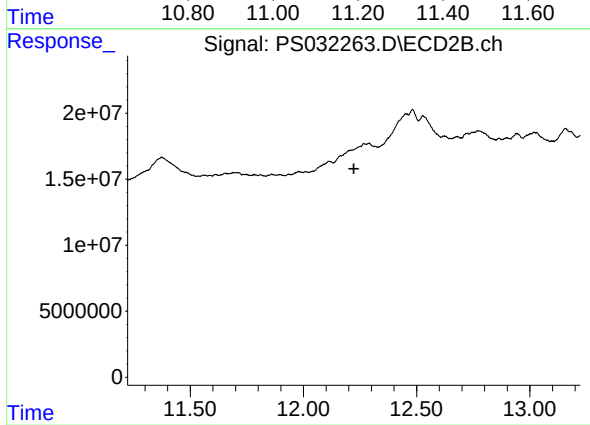

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 12.223 min
Response: 0
Conc: N.D.