

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110419\
 Data File : PS007601.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Nov 2019 17:17
 Operator : SM\AJ
 Sample : PB124507BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB124507BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 05 00:46:35 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 14 13:54:23 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.431	5.155	763.4E6	407.7E6	557.756	579.667
Target Compounds							
1) T	Dalapon	1.991	1.698	42746441	90329561	25.547	99.263 #
2) T	3,5-DICHL...	0.000	4.490	0	59938860	N.D.	69.661
5) T	DICAMBA	5.524	0.000	69303808	0	14.105	N.D. #
7) T	MCPA	5.900	5.525	25634720	24834914	4.970	8.543 #
9) T	2,4-D	6.487	6.058	71482926	8267668	58.006	10.363 #
11) T	2,4,5-TP ...	0.000	6.758	0	13388361	N.D.	3.520
15) T	Picloram	0.000	8.912	0	23096151	N.D.	3.761
16) T	DCPA	0.000	8.912	0	23096151	N.D.	4.606



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110419\
Data File : PS007601.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Nov 2019 17:17
Operator : SM\AJ
Sample : PB124507BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
PB124507BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 05 00:46:35 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
Quant Title : 8080.M
QLast Update : Mon Oct 14 13:54:23 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

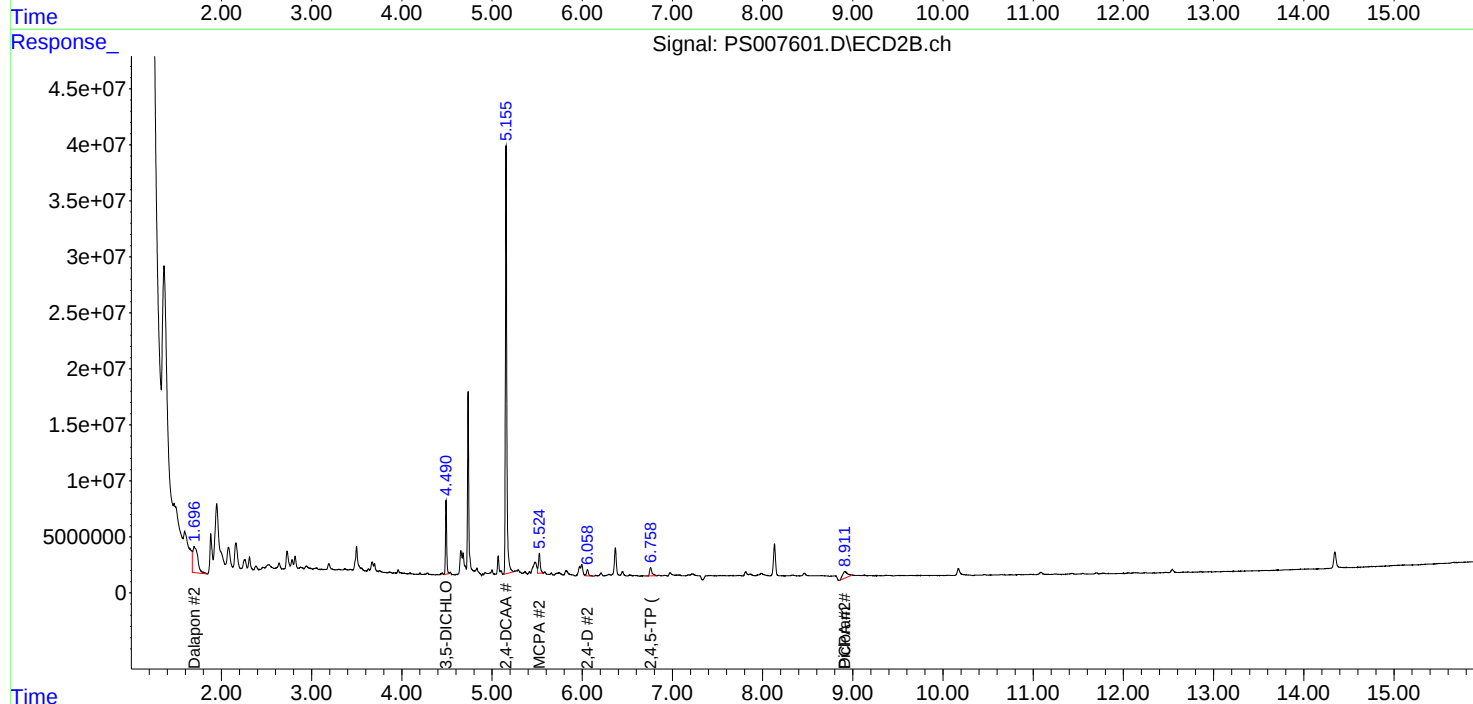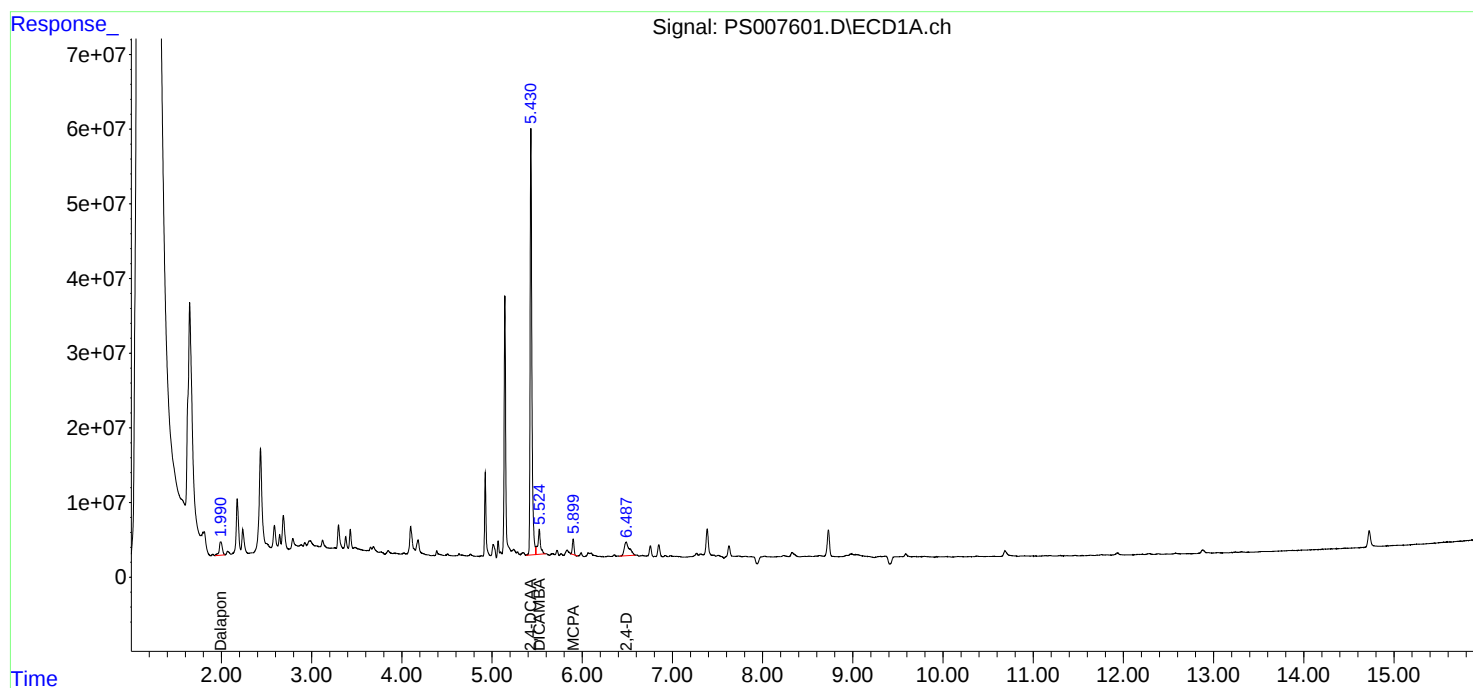


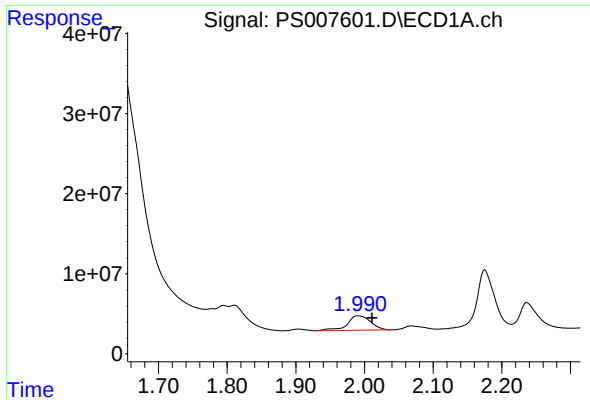

#1 Dalapon


R.T.: 1.991 min
Delta R.T.: -0.020 min
Response: 42746441
Conc: 25.55 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB124507BL

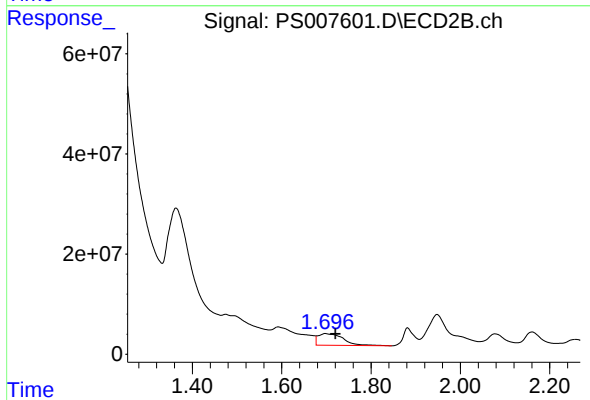


#1 Dalapon

R.T.: 1.698 min
Delta R.T.: -0.023 min
Response: 90329561
Conc: 99.26 ng/ml

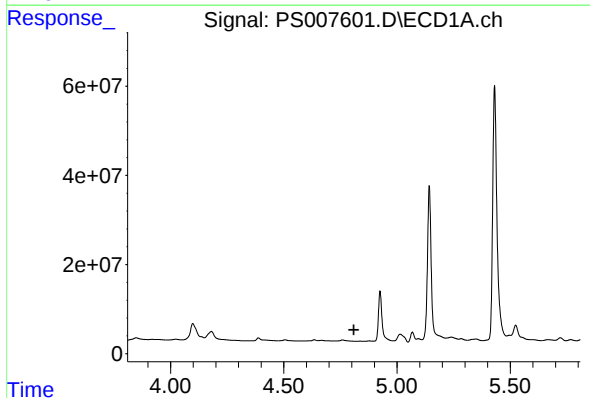


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.810 min
Response: 0
Conc: N.D.

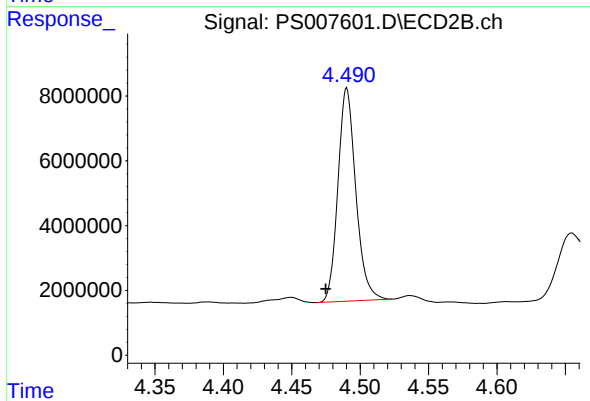

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.490 min
Delta R.T.: 0.016 min
Response: 59938860
Conc: 69.66 ng/ml

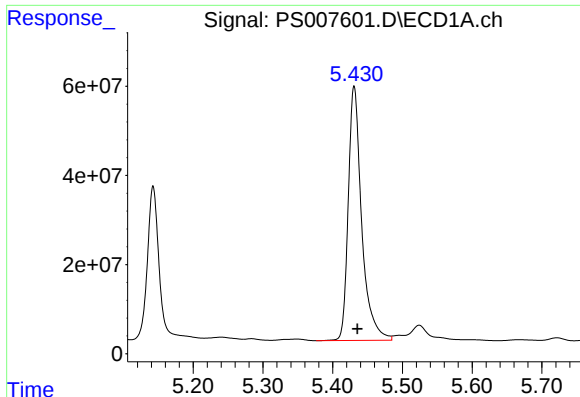

#4 2,4-DCAA


R.T.: 5.431 min
Delta R.T.: -0.005 min
Response: 763383707
Conc: 557.76 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB124507BL

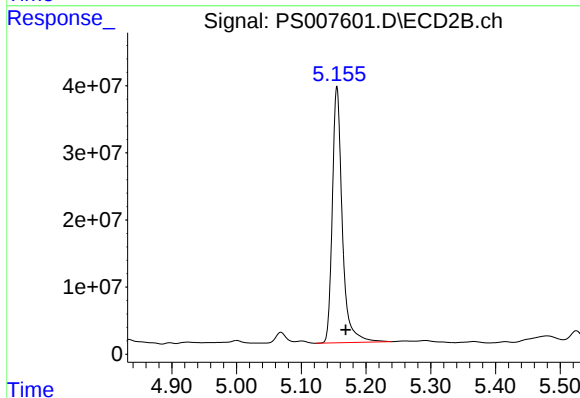


#4 2,4-DCAA

R.T.: 5.155 min
Delta R.T.: -0.013 min
Response: 407683420
Conc: 579.67 ng/ml

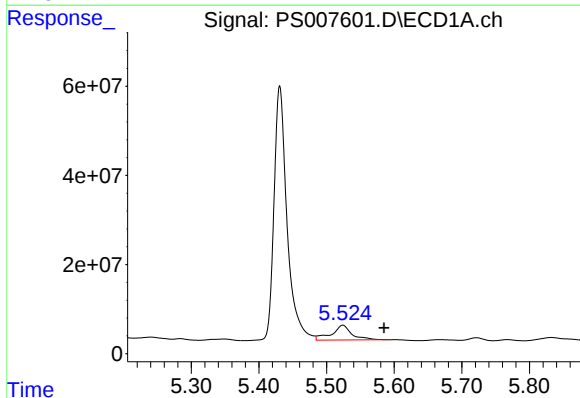


#5 DICAMBA

R.T.: 5.524 min
Delta R.T.: -0.061 min
Response: 69303808
Conc: 14.11 ng/ml

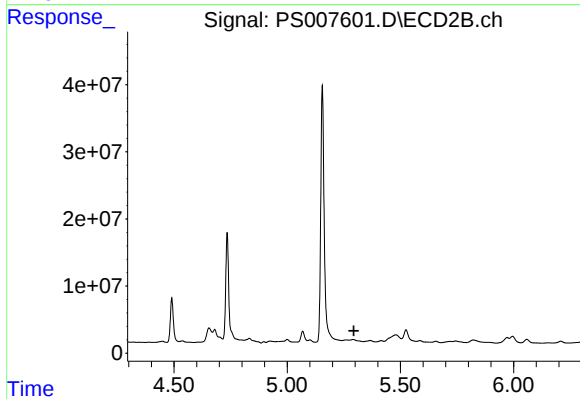

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 5.294 min
Response: 0
Conc: N.D.

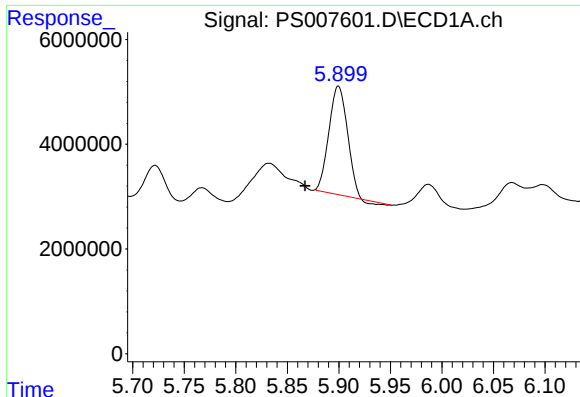

#7 MCPA


R.T.: 5.900 min
Delta R.T.: 0.032 min
Response: 25634720
Conc: 4.97 ug/ml

Instrument :
ECD_S
ClientSampleId :
PB124507BL

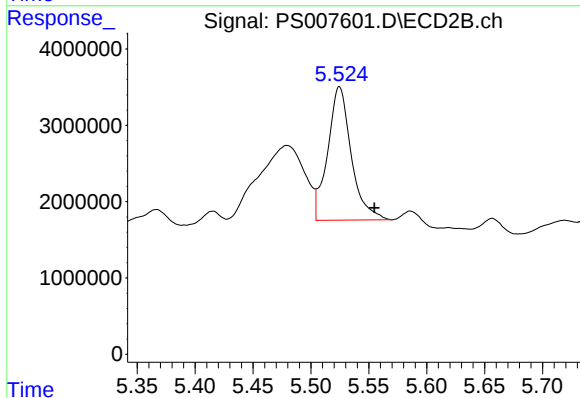


#7 MCPA

R.T.: 5.525 min
Delta R.T.: -0.030 min
Response: 24834914
Conc: 8.54 ug/ml

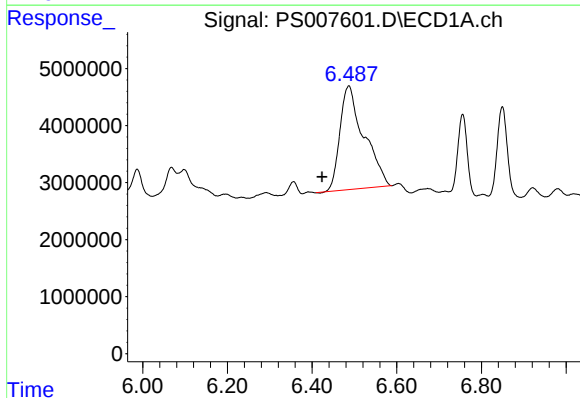


#9 2,4-D

R.T.: 6.487 min
Delta R.T.: 0.062 min
Response: 71482926
Conc: 58.01 ng/ml

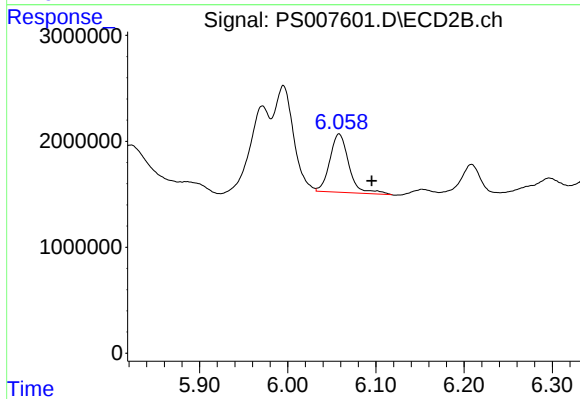

#9 2,4-D


R.T.: 6.058 min
Delta R.T.: -0.037 min
Response: 8267668
Conc: 10.36 ng/ml

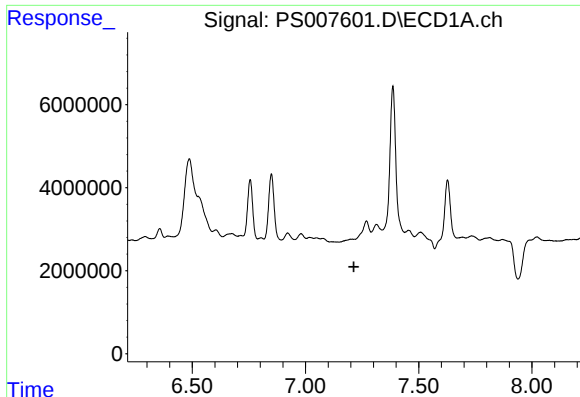

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.214 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB124507BL

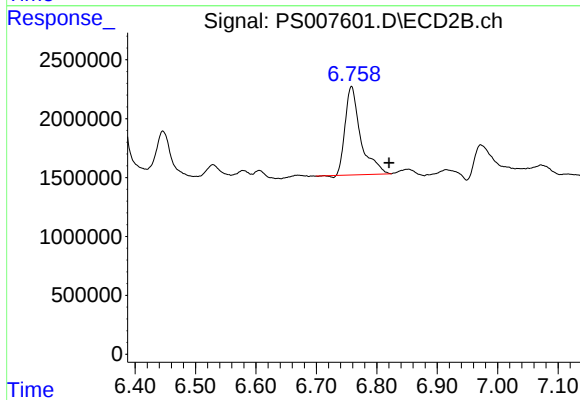


#11 2,4,5-TP (SILVEX)

R.T.: 6.758 min
Delta R.T.: -0.062 min
Response: 13388361
Conc: 3.52 ng/ml

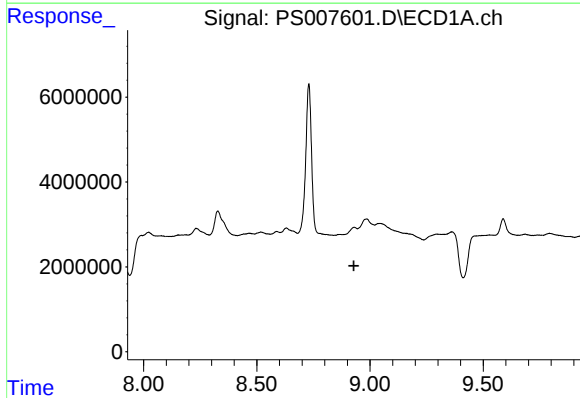


#15 Picloram

R.T.: 0.000 min
Exp R.T.: 8.929 min
Response: 0
Conc: N.D.

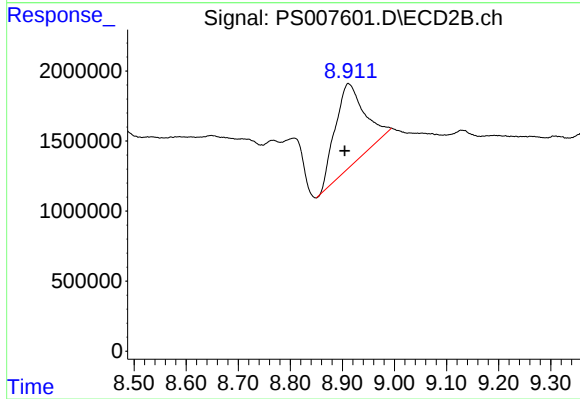

#15 Picloram


R.T.: 8.912 min
Delta R.T.: 0.007 min
Response: 23096151
Conc: 3.76 ng/ml

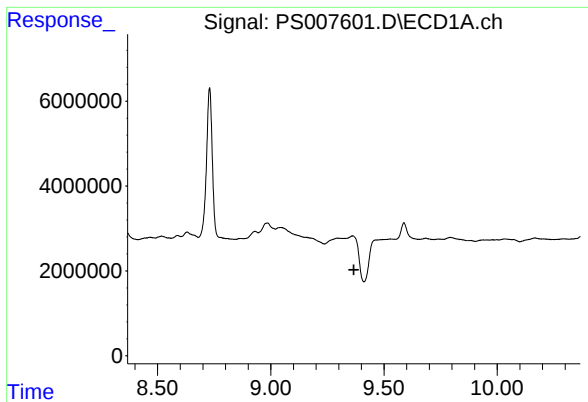

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 9.367 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB124507BL

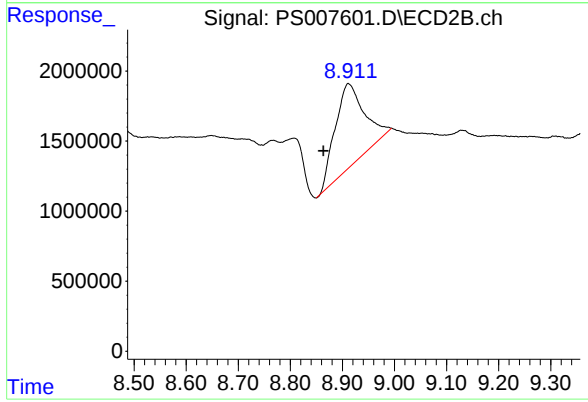

#16 DCPA

R.T.: 8.912 min
Delta R.T.: 0.049 min
Response: 23096151
Conc: 4.61 ng/ml