

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110419\
 Data File : PS007606.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Nov 2019 19:07
 Operator : SM\AJ
 Sample : K5615-09
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 RBR-52

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 05 00:47:38 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 14 13:54:23 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.450	5.176	753.3E6	379.4E6	550.422	539.480
Target Compounds							
2) T	3,5-DICHL...	0.000	4.511	0	52293458	N.D.	60.776
3) T	4-Nitroph...	0.000	4.853	0	9407757	N.D.	23.823
5) T	DICAMBA	5.545	5.310	50135211	20048527	10.204	7.705
6) T	MCP	0.000	5.310	0	20048527	N.D.	10.570
7) T	MCPA	5.920	5.545	30671351	27781506	5.947	9.556 #
9) T	2,4-D	0.000	6.078	0	12881302	N.D.	16.146
10) T	Pentachlo...	0.000	6.462	0	9228893	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	6.775	0	15868989	N.D.	4.172
13) T	2,4-DB	8.036	0.000	23047037	0	24.172	N.D. #
14) T	DINOSEB	0.000	8.000	0	27844382	N.D.	9.918
15) T	Picloram	0.000	8.919	0	24801320	N.D.	4.039
16) T	DCPA	0.000	8.824	0	23972044	N.D.	4.780



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110419\
Data File : PS007606.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Nov 2019 19:07
Operator : SM\AJ
Sample : K5615-09
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
RBR-52

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 05 00:47:38 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
Quant Title : 8080.M
QLast Update : Mon Oct 14 13:54:23 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

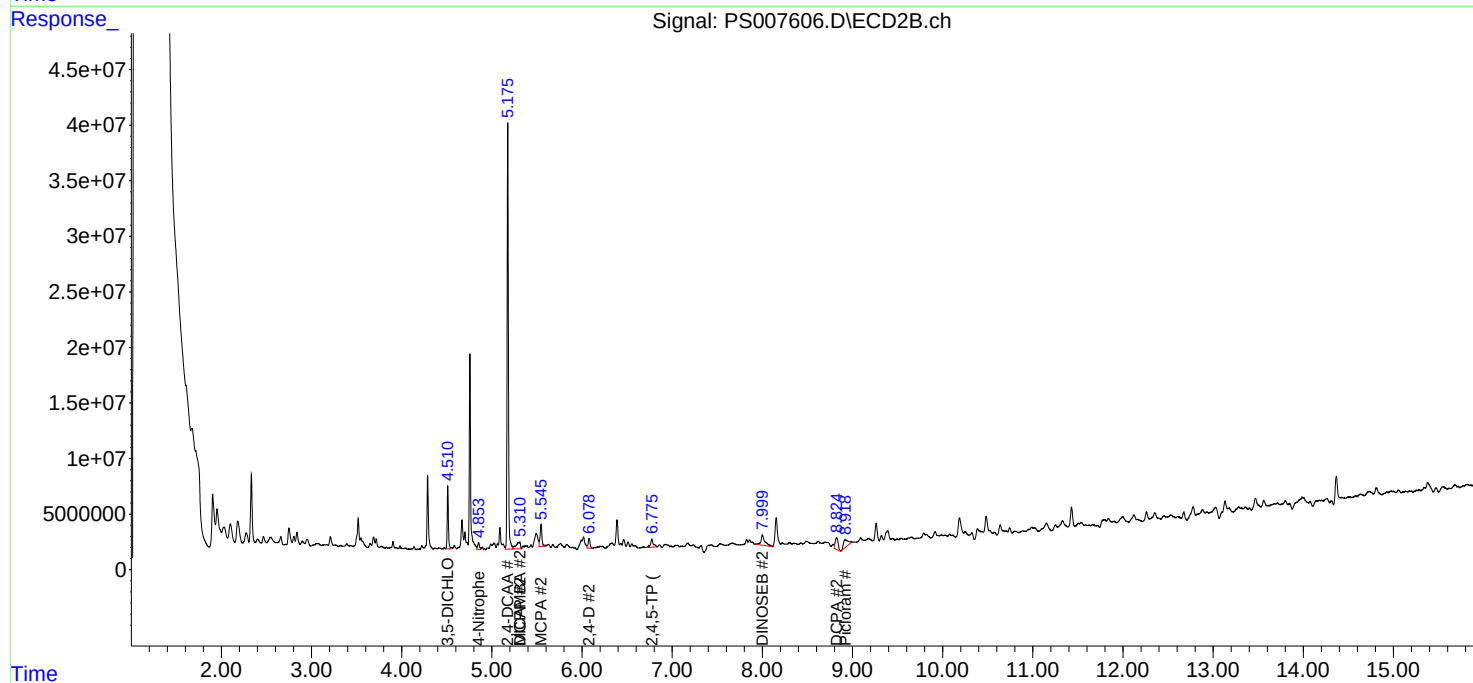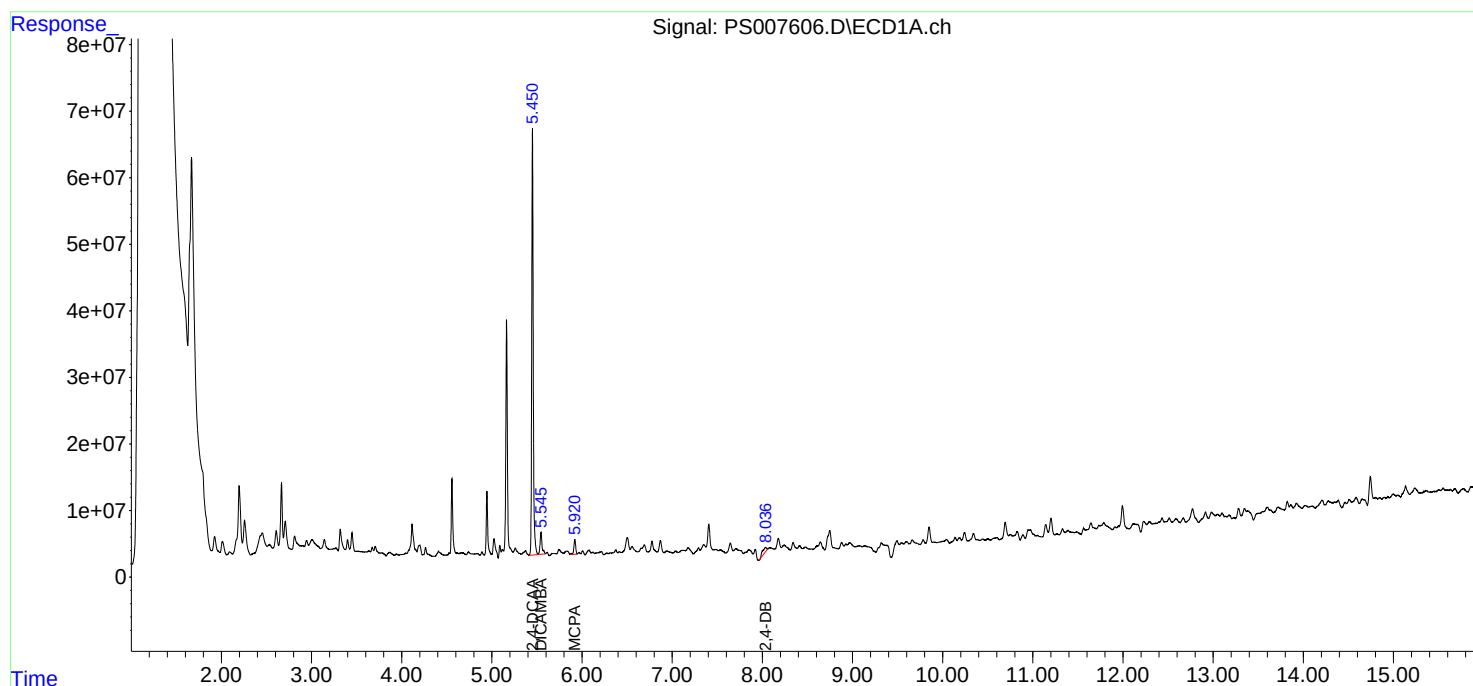


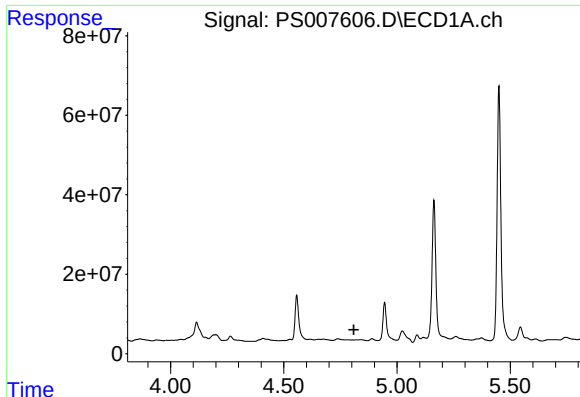

#2 3,5-DICHLORO BENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 4.810 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
RBR-52

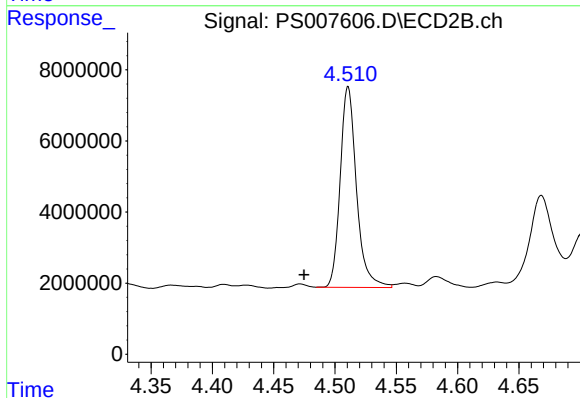


#2 3,5-DICHLORO BENZOIC ACID

R.T.: 4.511 min
Delta R.T.: 0.036 min
Response: 52293458
Conc: 60.78 ng/ml

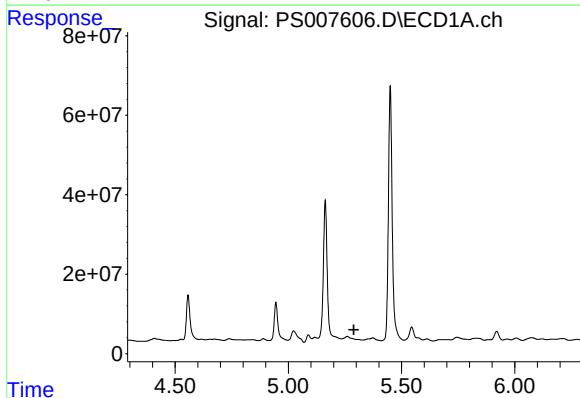


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 5.290 min
Response: 0
Conc: N.D.

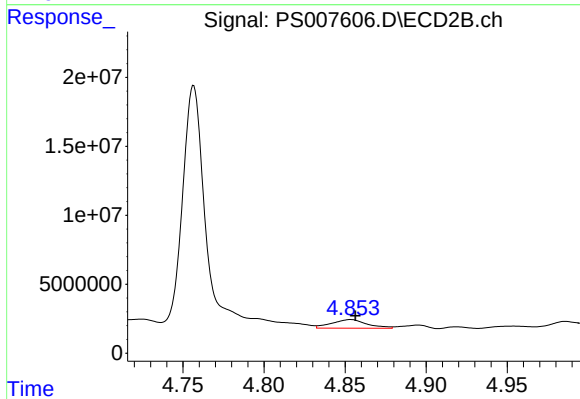

#3 4-Nitrophenol


R.T.: 4.853 min
Delta R.T.: -0.003 min
Response: 9407757
Conc: 23.82 ng/ml

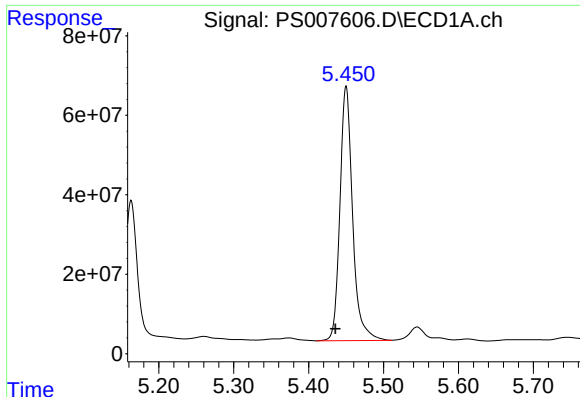

#4 2,4-DCAA


R.T.: 5.450 min
Delta R.T.: 0.014 min
Response: 753345513
Conc: 550.42 ng/ml

Instrument :
ECD_S
ClientSampleId :
RBR-52

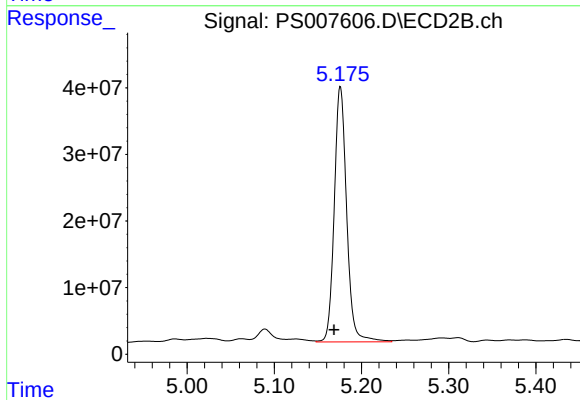


#4 2,4-DCAA

R.T.: 5.176 min
Delta R.T.: 0.007 min
Response: 379419642
Conc: 539.48 ng/ml

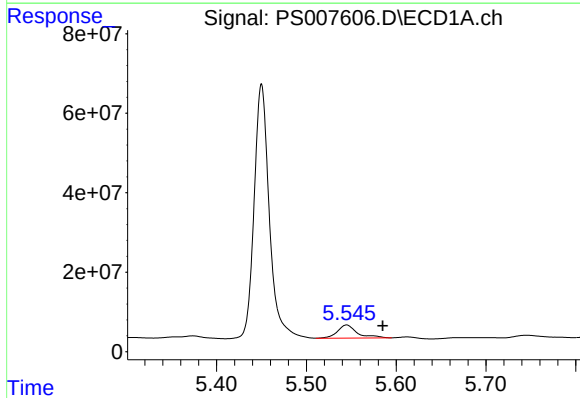


#5 DICAMBA

R.T.: 5.545 min
Delta R.T.: -0.040 min
Response: 50135211
Conc: 10.20 ng/ml

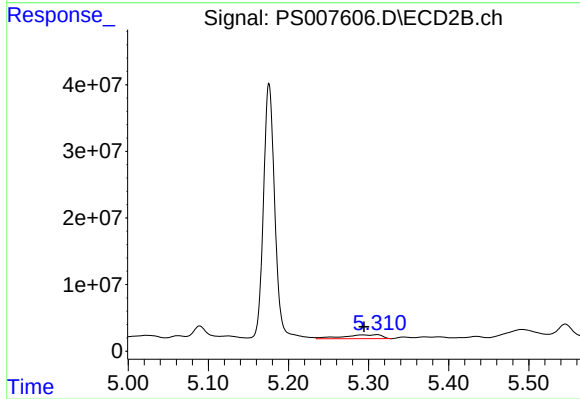

#5 DICAMBA


R.T.: 5.310 min
Delta R.T.: 0.016 min
Response: 20048527
Conc: 7.70 ng/ml

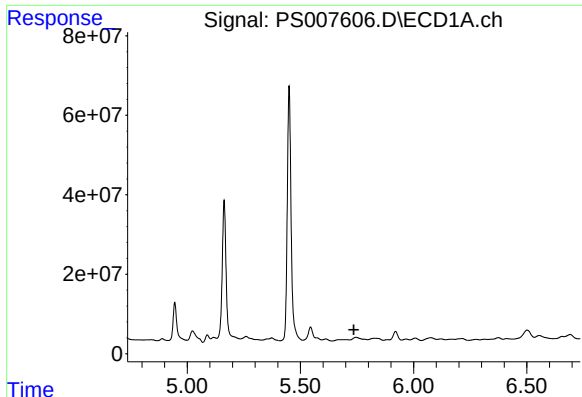

#6 MCP


R.T.: 0.000 min
Exp R.T.: 5.736 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
RBR-52

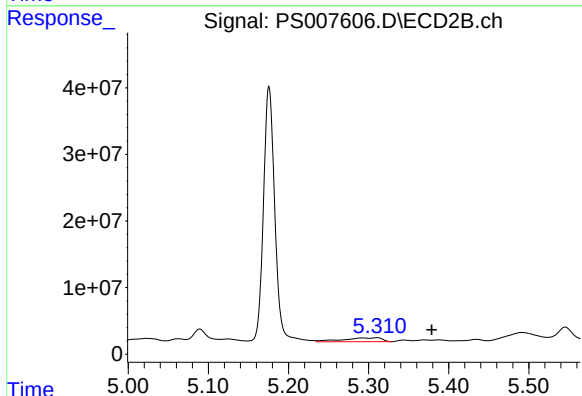


#6 MCP

R.T.: 5.310 min
Delta R.T.: -0.069 min
Response: 20048527
Conc: 10.57 ug/ml

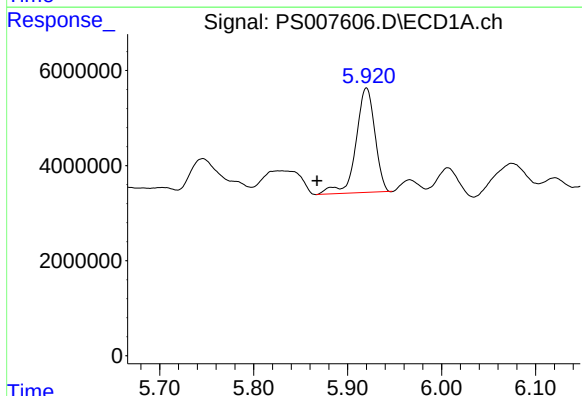


#7 MCP

R.T.: 5.920 min
Delta R.T.: 0.053 min
Response: 30671351
Conc: 5.95 ug/ml

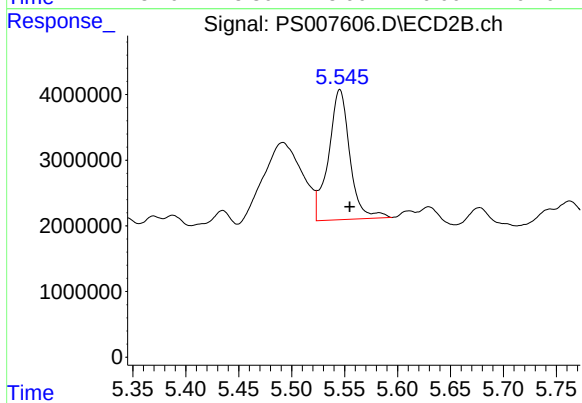

#7 MCP


R.T.: 5.545 min
Delta R.T.: -0.009 min
Response: 27781506
Conc: 9.56 ug/ml

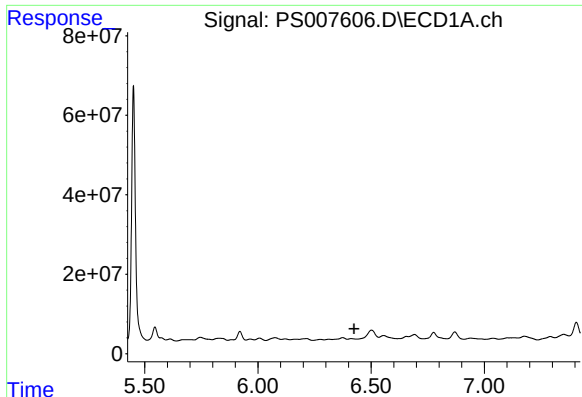

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.424 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
RBR-52

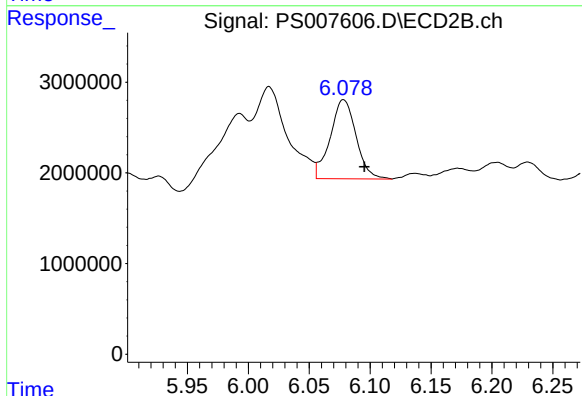


#9 2,4-D

R.T.: 6.078 min
Delta R.T.: -0.017 min
Response: 12881302
Conc: 16.15 ng/ml

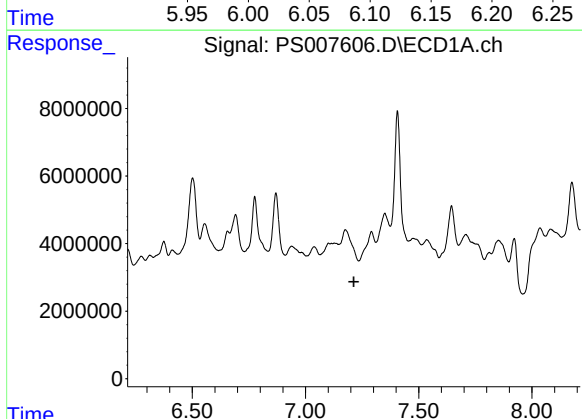


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 7.214 min
Response: 0
Conc: N.D.

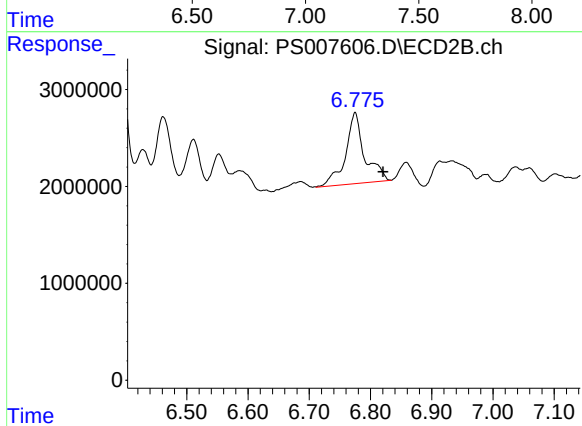

#11 2,4,5-TP (SILVEX)


R.T.: 6.775 min
Delta R.T.: -0.046 min
Response: 15868989
Conc: 4.17 ng/ml

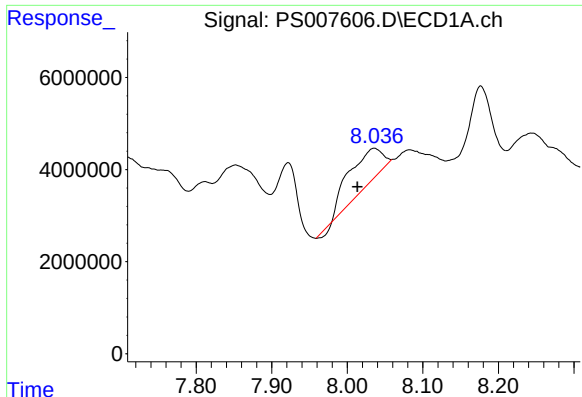

#13 2,4-DB


R.T.: 8.036 min
Delta R.T.: 0.022 min
Response: 23047037
Conc: 24.17 ng/ml

Instrument :
ECD_S
ClientSampleId :
RBR-52

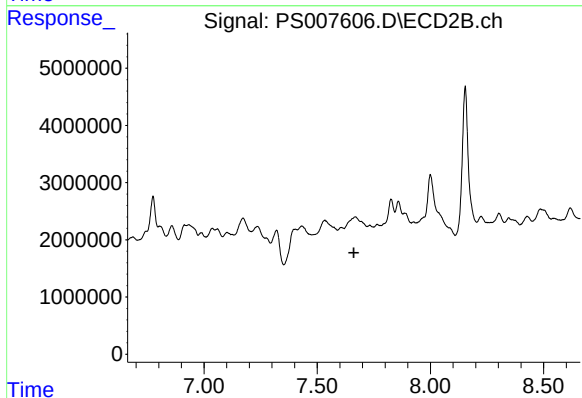


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 7.662 min
Response: 0
Conc: N.D.

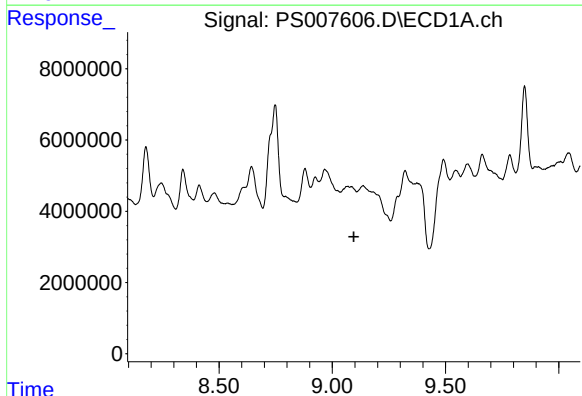


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 9.095 min
Response: 0
Conc: N.D.

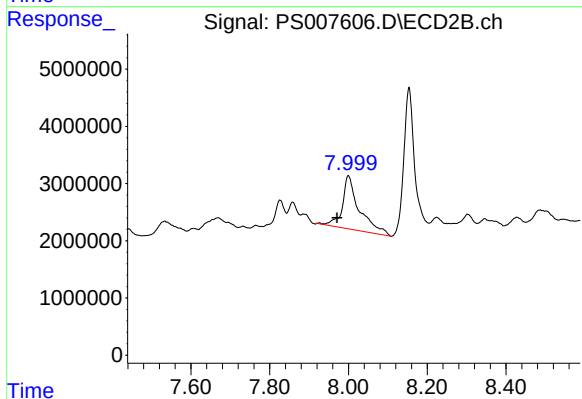

#14 DINOSEB


R.T.: 8.000 min
Delta R.T.: 0.029 min
Response: 27844382
Conc: 9.92 ng/ml

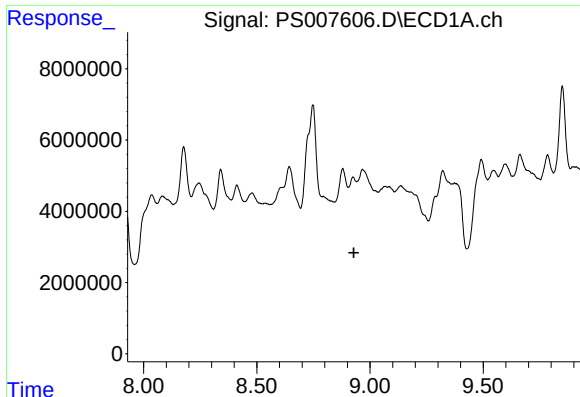

#15 Picloram


R.T.: 0.000 min
Exp R.T.: 8.929 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
RBR-52

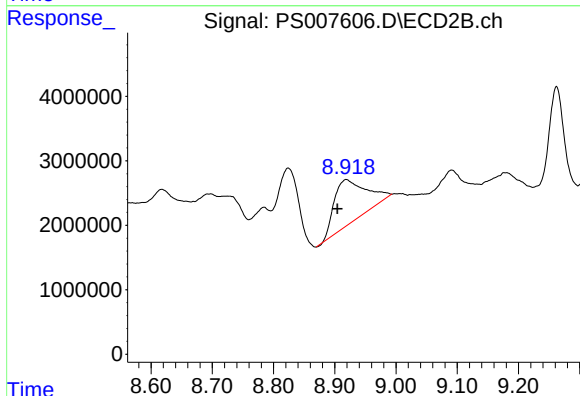


#15 Picloram

R.T.: 8.919 min
Delta R.T.: 0.014 min
Response: 24801320
Conc: 4.04 ng/ml

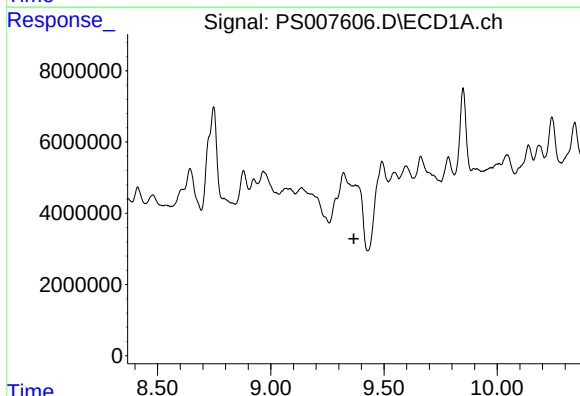

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 9.367 min
Response: 0
Conc: N.D.

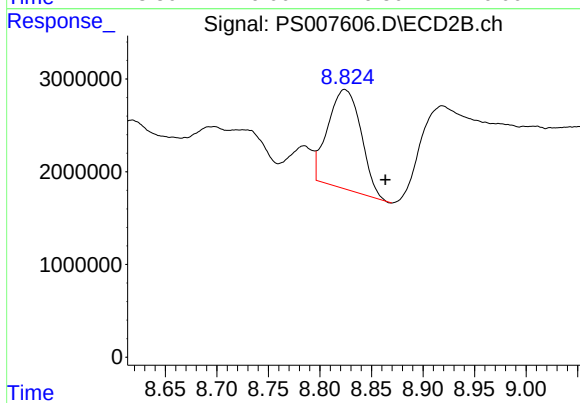

#16 DCPA

R.T.: 8.824 min
Delta R.T.: -0.039 min
Response: 23972044
Conc: 4.78 ng/ml